


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012619\
 Data File : VX007229.D
 Acq On : 25 Jan 2019 15:00
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Title : SW846 8260
 Last Update : Tue Jan 08 14:06:59 2019

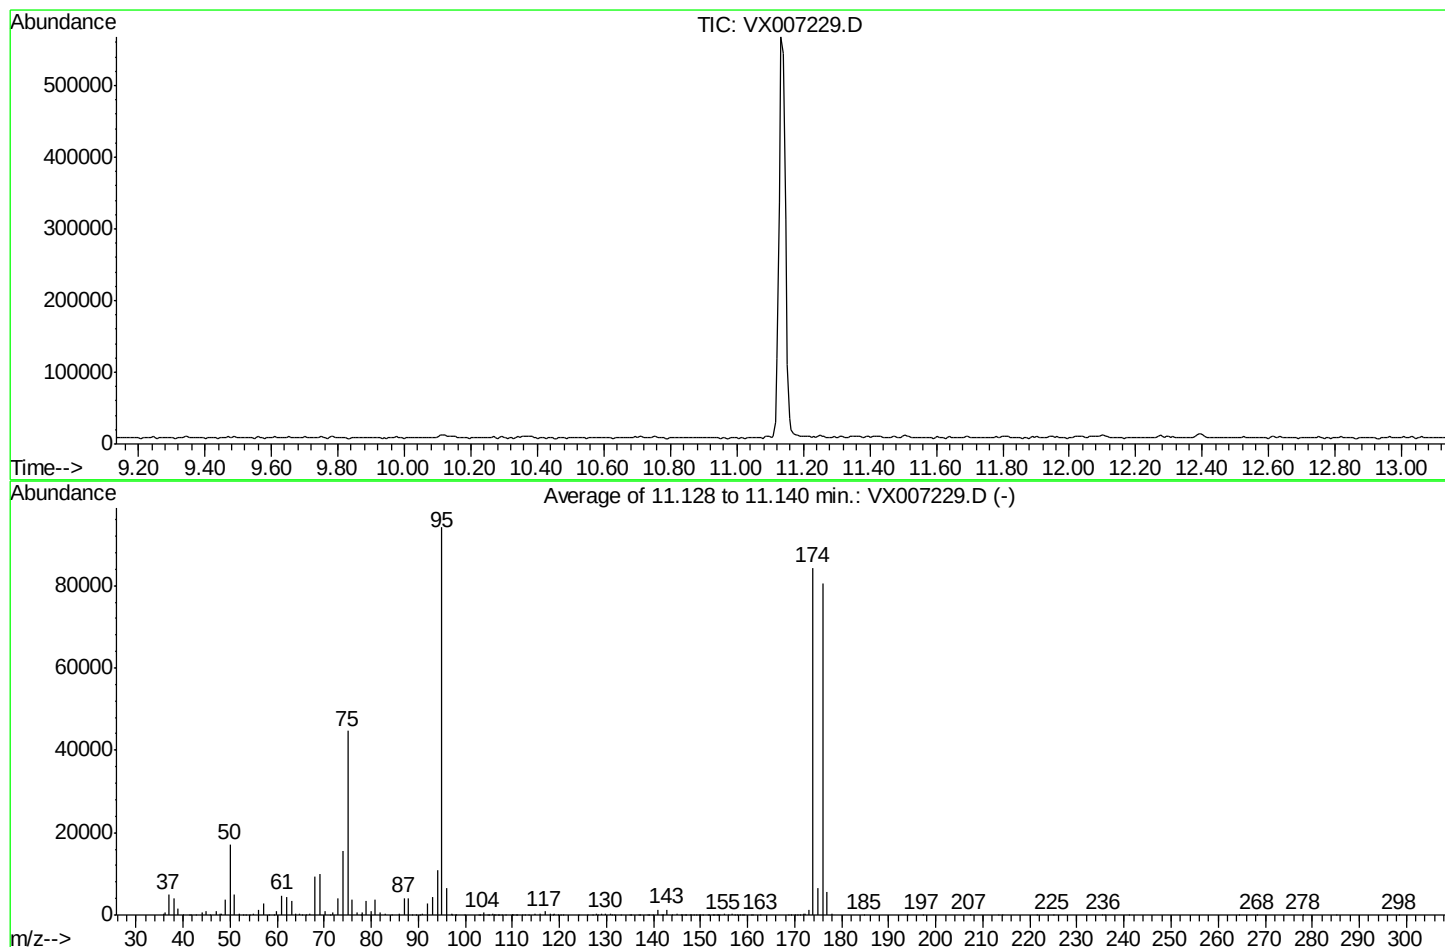

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	17089	PASS
75	95	30	60	47.5	44730	PASS
95	95	100	100	100.0	94133	PASS
96	95	5	9	6.9	6481	PASS
173	174	0.00	2	1.4	1141	PASS
174	95	50	100	89.7	84392	PASS
175	174	5	9	7.6	6401	PASS
176	174	95	101	95.2	80381	PASS
177	176	5	9	7.0	5598	PASS