

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
 Data File : VX020750.D
 Acq On : 26 Jan 2021 13:57
 Operator : JC/SP
 Sample : M1192-04DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 26 14:42:02 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.623	168	287287	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.824	114	495094	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.092	117	495533	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	226301	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.025	65	191314	48.82	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	97.64%
35) Dibromofluoromethane	5.465	113	162792	48.00	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.00%
50) Toluene-d8	8.696	98	625951	50.35	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.70%
62) 4-Bromofluorobenzene	11.122	95	247240	51.21	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	102.42%

Target Compounds						Qvalue
5) Bromomethane	1.618	94	641	0.33	ug/l	87
10) Methyl Iodide	2.483	142	923	0.24	ug/l	96
11) Tert butyl alcohol	2.989	59	9783	13.37	ug/l #	73
13) Acrolein	2.282	56	160	0.29	ug/l #	49
16) Acetone	2.429	43	15356	10.34	ug/l	97
17) Carbon Disulfide	2.544	76	887	1.00	ug/l	95
18) Methyl Acetate	2.746	43	1230	0.32	ug/l	91
19) Methyl tert-butyl Ether	3.166	73	5994	0.58	ug/l	98
20) Methylene Chloride	2.831	84	1130	0.30	ug/l #	93
22) Diisopropyl ether	3.825	45	5741	0.57	ug/l #	80
23) Vinyl Acetate	3.831	43	2925	0.35	ug/l #	68
25) 2-Butanone	4.654	43	4272	1.84	ug/l	96
29) Tetrahydrofuran	5.105	42	375	0.25	ug/l #	31
36) 1,1-Dichloropropene	5.617	75	22693	4.57	ug/l #	48
37) Ethyl Acetate	4.794	43	2239	0.48	ug/l #	84
38) Carbon Tetrachloride	5.623	117	30006	5.74	ug/l #	17
39) Methylcyclohexane	7.434	83	3166	0.56	ug/l	93
40) Benzene	6.105	78	70362	4.81	ug/l	97
51) 4-Methyl-2-Pentanone	8.629	43	1023	0.22	ug/l #	71
52) Toluene	8.763	92	342133	37.18	ug/l	99
53) t-1,3-Dichloropropene	8.763	75	3971	0.70	ug/l #	1
55) 1,1,2-Trichloroethane	9.141	97	1002	0.26	ug/l #	22
56) Ethyl methacrylate	9.159	69	2465	3.16	ug/l #	83
67) Ethyl Benzene	10.232	91	57035	3.07	ug/l	100
68) m/p-Xylenes	10.342	106	200144	28.87	ug/l	97
69) o-Xylene	10.683	106	108251	16.60	ug/l	98
70) Styrene	10.683	104	6044	0.54	ug/l #	1
73) Isopropylbenzene	11.000	105	3544	0.22	ug/l	95
74) N-amyl acetate	10.897	43	826	2.13	ug/l #	1
76) 1,2,3-Trichloropropane	11.122	75	120819	23.02	ug/l #	40
78) n-propylbenzene	11.342	91	10805	0.57	ug/l	99
79) 2-Chlorotoluene	11.415	91	24872	2.16	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.488	105	69212	4.95	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.122	75	120819	64.51	ug/l #	12
82) 4-Chlorotoluene	11.488	91	7409	0.54	ug/l #	45
83) tert-Butylbenzene	11.787	119	31323	2.32	ug/l #	51

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
 Data File : VX020750.D
 Acq On : 26 Jan 2021 13:57
 Operator : JC/SP
 Sample : M1192-04DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 26 14:42:02 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
84) 1,2,4-Trimethylbenzene	11.793	105	265462	18.83	ug/l	99
85) sec-Butylbenzene	11.793	105	265462	17.01	ug/l #	57
86) p-Isopropyltoluene	12.049	119	5584	0.39	ug/l	89
89) n-Butylbenzene	12.360	91	14254	1.10	ug/l #	22
90) Hexachloroethane	12.567	117	3099	1.19	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.963	75	390	0.32	ug/l #	1
95) Naphthalene	13.817	128	90011	7.76	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
Data File : VX020750.D
Acq On : 26 Jan 2021 13:57
Operator : JC/SP
Sample : M1192-04DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 26 14:42:02 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration




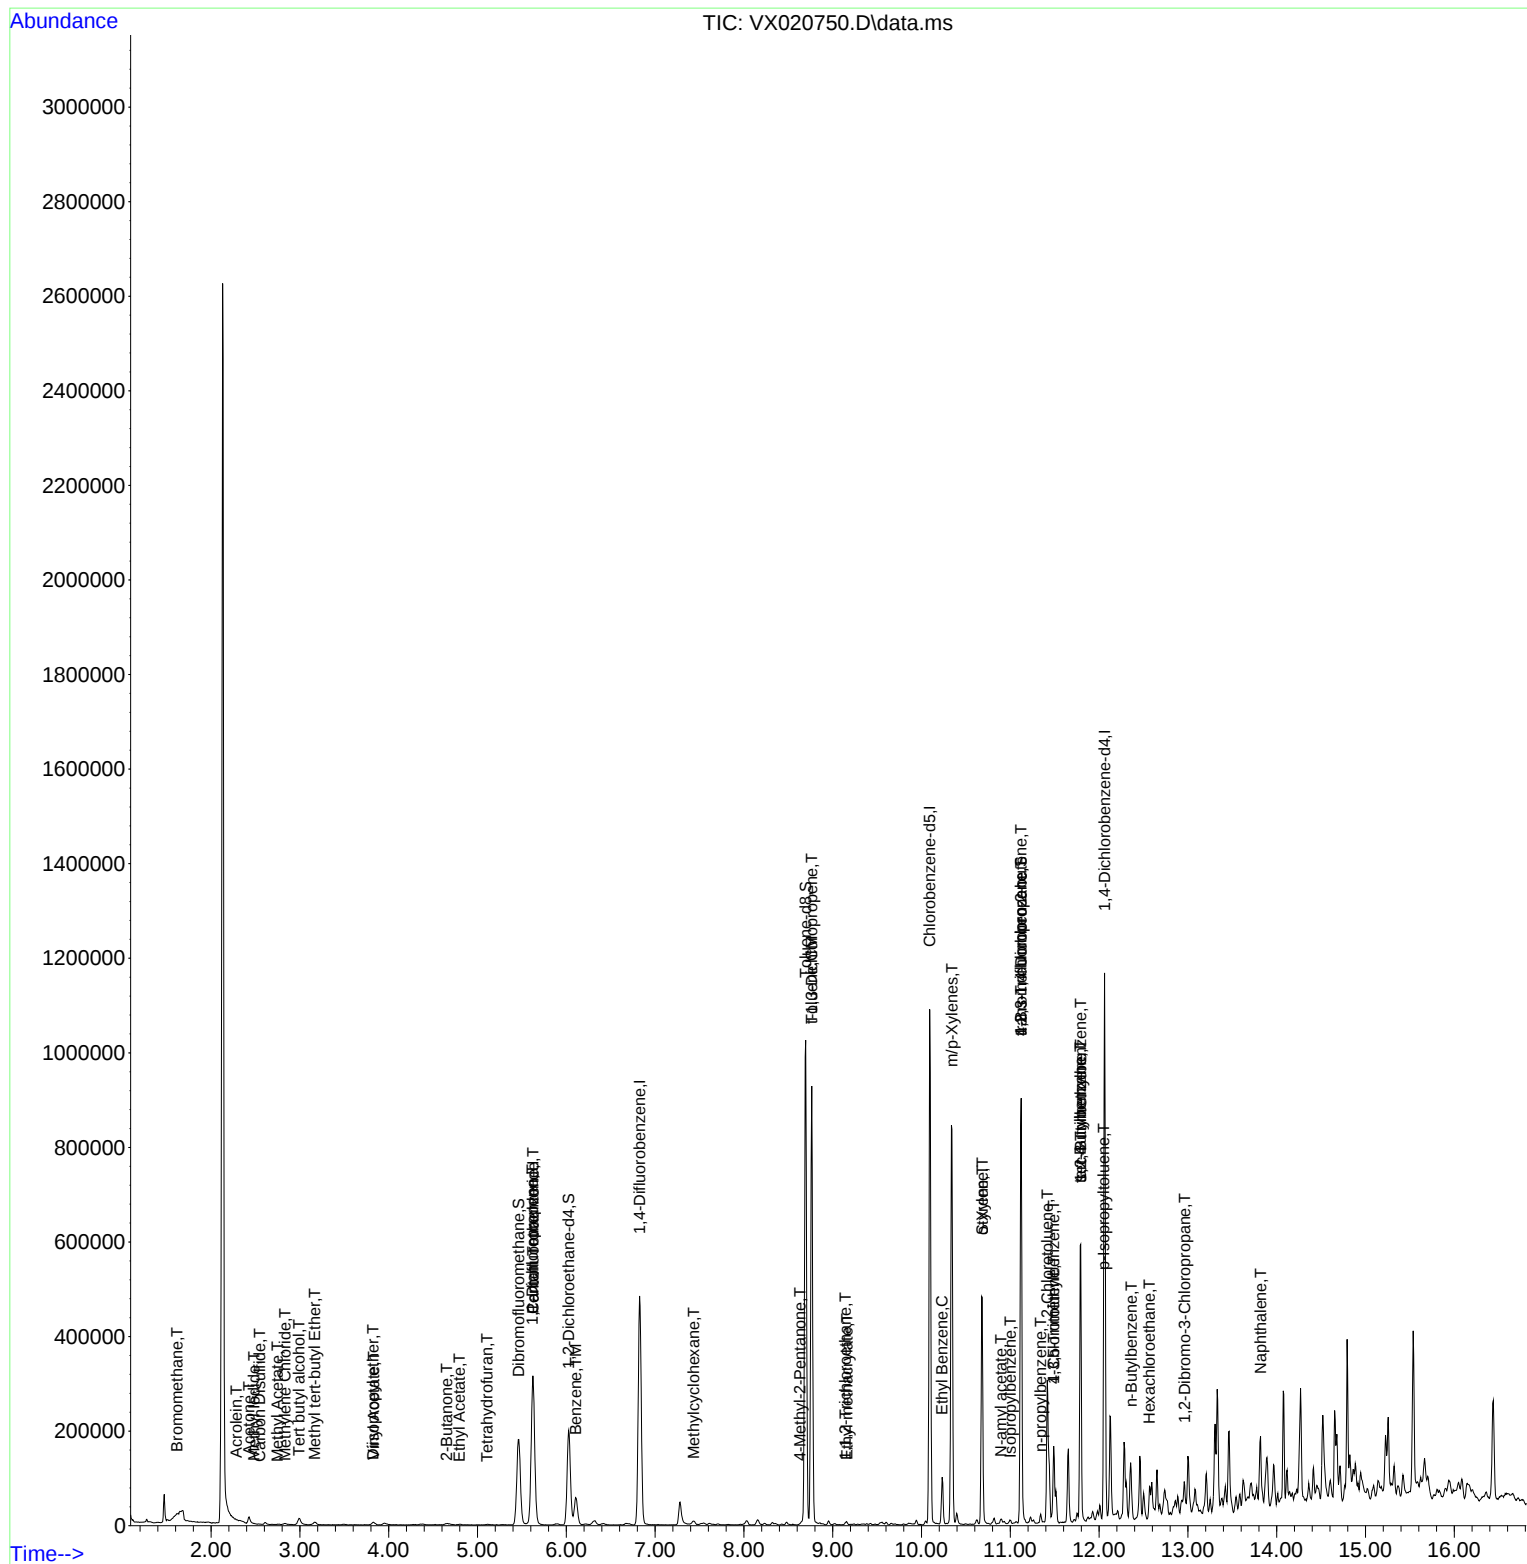




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.006 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:168 Resp: 287287
Ion Ratio Lower Upper
168 100
99 59.6 45.8 68.6

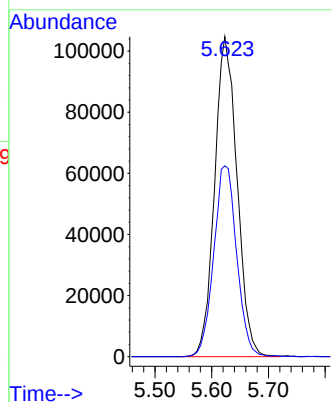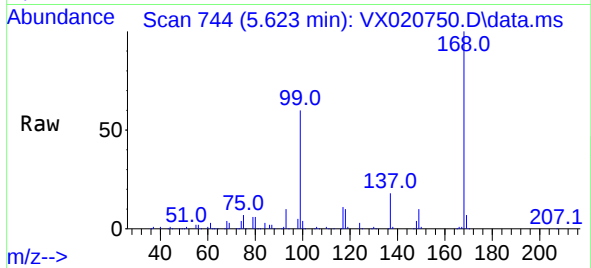

#5
Bromomethane
Concen: 0.33 ug/l
RT: 1.618 min Scan# 87
Delta R.T. -0.006 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 94 Resp: 641
Ion Ratio Lower Upper
94 100
96 83.3 76.4 114.6


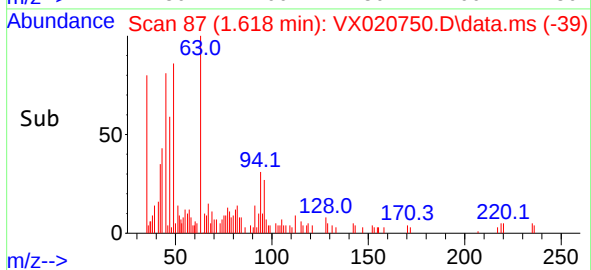
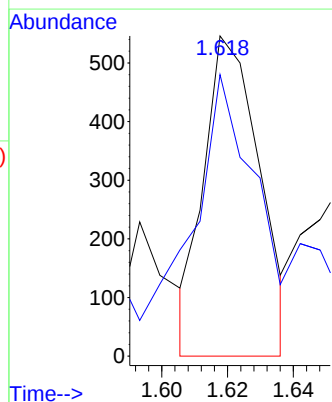
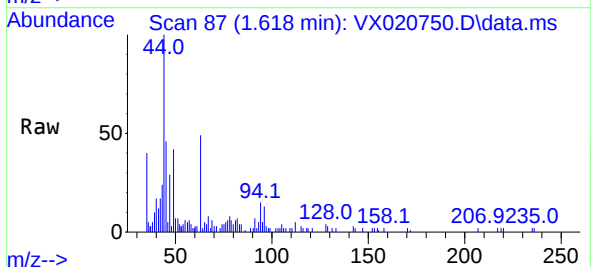




#10
Methyl Iodide
Concen: 0.24 ug/l
RT: 2.483 min Scan# 229
Delta R.T. -0.006 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:	142	Resp:	923
Ion	Ratio	Lower	Upper
142	100		
127	43.9	33.3	49.9
141	12.9	11.4	17.0

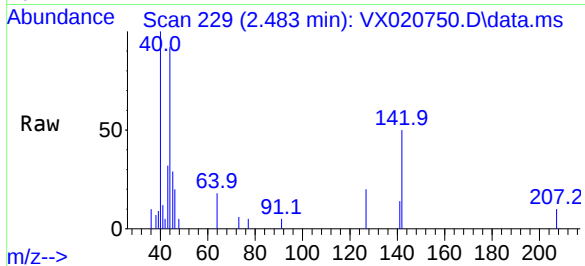

#11
Tert butyl alcohol
Concen: 13.37 ug/l
RT: 2.989 min Scan# 312
Delta R.T. -0.031 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion:	59	Resp:	9783
Ion	Ratio	Lower	Upper
59	100		
57	0.0	7.8	11.8#


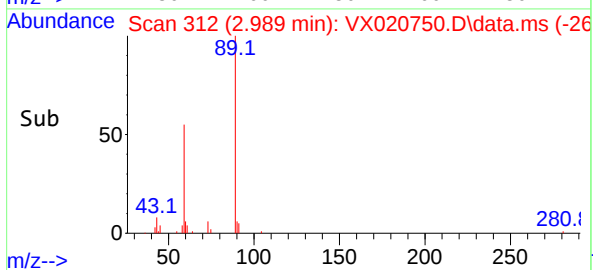

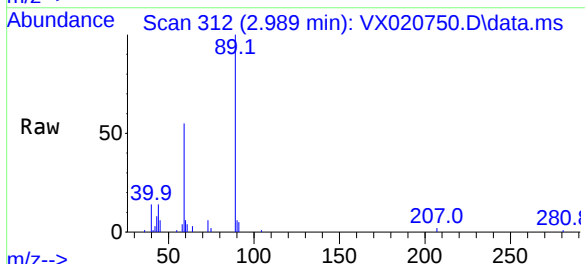




#13
Acrolein
Concen: 0.29 ug/l
RT: 2.282 min Scan# 196
Delta R.T. 0.012 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 56 Resp: 160
Ion Ratio Lower Upper
56 100
55 112.5 56.4 84.6#

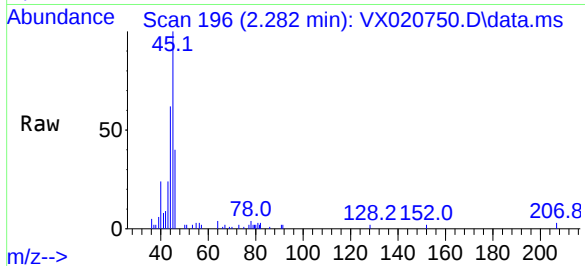

#16
Acetone
Concen: 10.34 ug/l
RT: 2.429 min Scan# 220
Delta R.T. 0.007 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 43 Resp: 15356
Ion Ratio Lower Upper
43 100
58 33.2 27.8 41.8

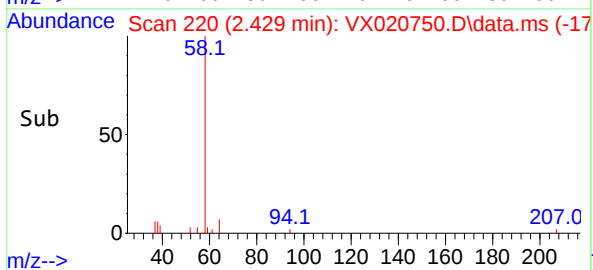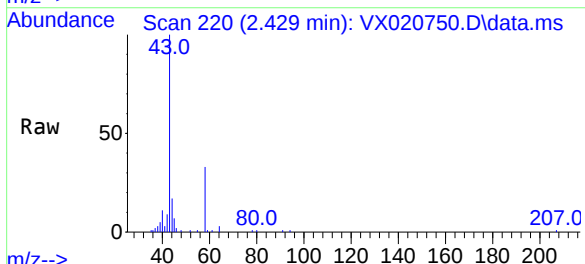



#17

Carbon Disulfide

Concen: 1.00 ug/l

RT: 2.544 min Scan# 239

Delta R.T. 0.000 min

Lab File: VX020750.D





Acq: 26 Jan 2021 13:57

Tgt Ion: 76 Resp: 887

Ion Ratio Lower Upper

76 100

78 10.7 7.2 10.8

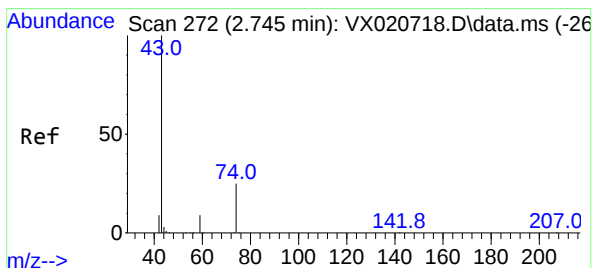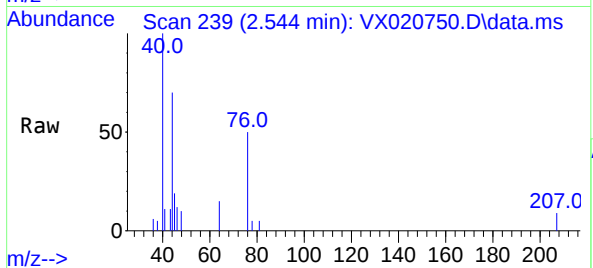

#18

Methyl Acetate

Concen: 0.32 ug/l

RT: 2.746 min Scan# 272

Delta R.T. 0.001 min

Lab File: VX020750.D




Acq: 26 Jan 2021 13:57


Tgt Ion: 43 Resp: 1230

Ion Ratio Lower Upper

43 100

74 22.6 21.9 32.9

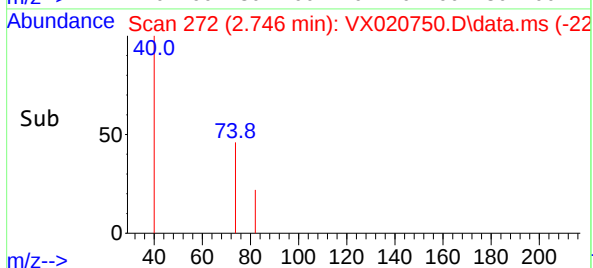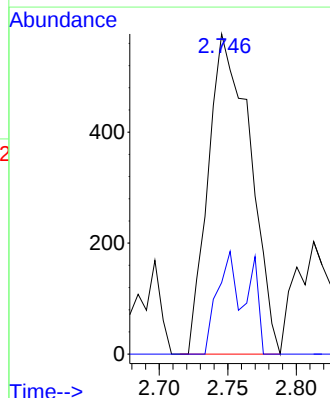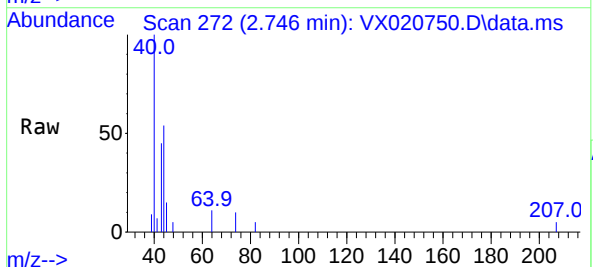







#19

Methyl tert-butyl Ether
Concen: 0.58 ug/l
RT: 3.166 min Scan# 341
Delta R.T. 0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 73 Resp: 5994
Ion Ratio Lower Upper
73 100
57 20.5 17.1 25.7

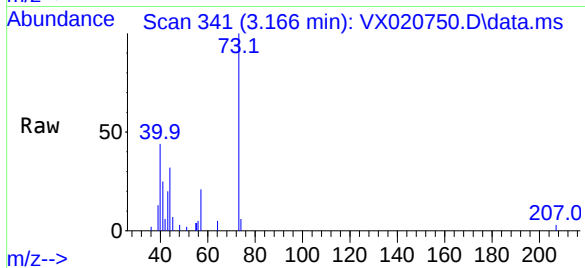


#20

Methylene Chloride
Concen: 0.30 ug/l
RT: 2.831 min Scan# 286
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 84 Resp: 1130
Ion Ratio Lower Upper
84 100
49 108.0 88.6 132.8
51 45.1 27.0 40.6#
86 56.1 50.3 75.5


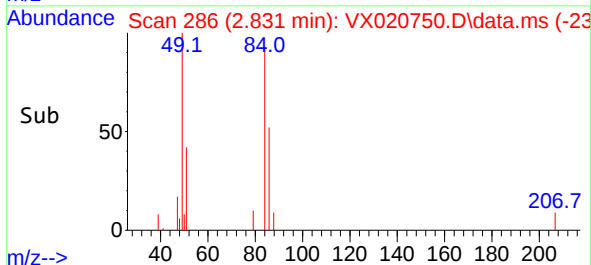
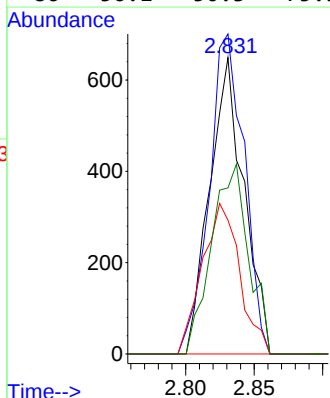
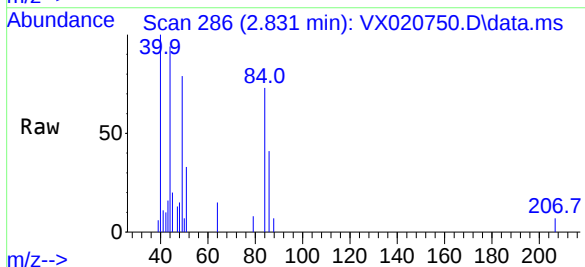




#22
Diisopropyl ether
Concen: 0.57 ug/l
RT: 3.825 min Scan# 449
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:	45	Resp:	5741
Ion	Ratio	Lower	Upper
45	100		
43	46.4	58.0	87.0#
87	32.4	25.4	38.0
59	13.7	10.2	15.2



#23
Vinyl Acetate
Concen: 0.35 ug/l
RT: 3.831 min Scan# 450
Delta R.T. 0.049 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion:	43	Resp:	2925
Ion	Ratio	Lower	Upper
43	100		
86	0.0	9.9	14.9#


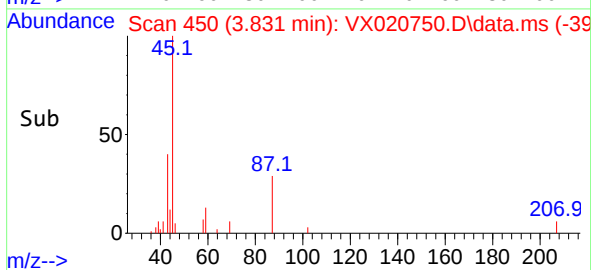






#25
2-Butanone
Concen: 1.84 ug/l
RT: 4.654 min Scan# 585
Delta R.T. 0.019 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 4272
Ion Ratio Lower Upper
43 100
72 27.2 23.7 35.5

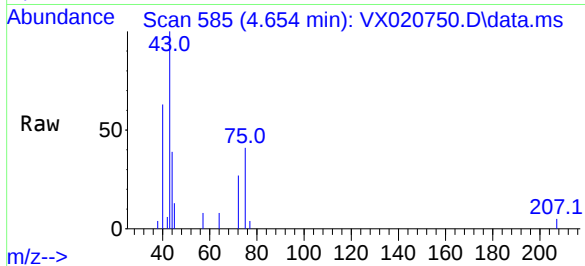

#29
Tetrahydrofuran
Concen: 0.25 ug/l
RT: 5.105 min Scan# 659
Delta R.T. 0.019 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 42 Resp: 375
Ion Ratio Lower Upper
42 100
72 0.0 41.7 62.5#
71 5.3 38.4 57.6#

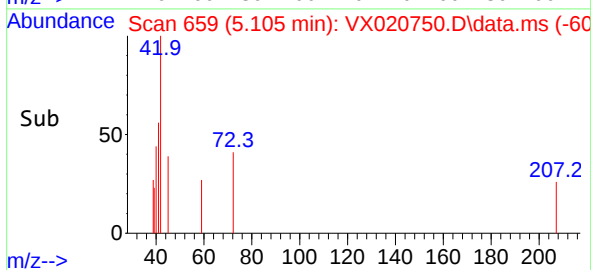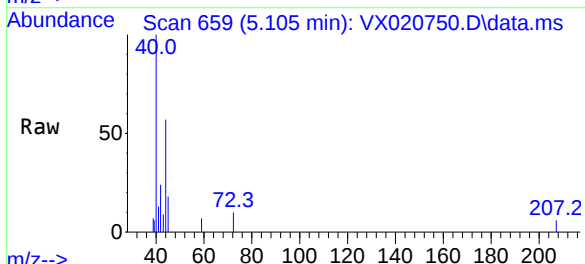







#33

1,2-Dichloroethane-d4
Concen: 48.82 ug/l
RT: 6.025 min Scan# 810
Delta R.T. 0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 65 Resp: 191314
Ion Ratio Lower Upper
65 100
67 53.4 0.0 105.4

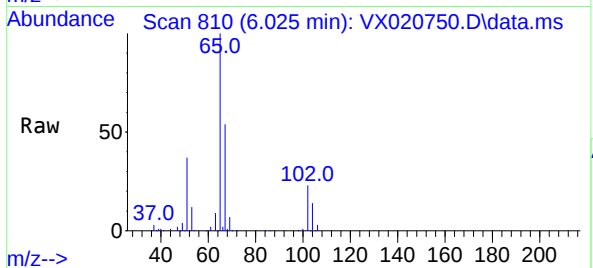


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.824 min Scan# 941
Delta R.T. -0.006 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57


Tgt Ion: 114 Resp: 495094
Ion Ratio Lower Upper
114 100
63 20.2 0.0 40.8
88 17.1 0.0 32.8

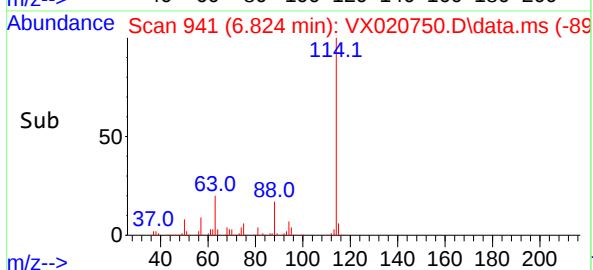






#35
Dibromofluoromethane
Concen: 48.00 ug/l
RT: 5.465 min Scan# 718
Delta R.T. 0.001 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57


Instrument :
MSVOA_X
ClientSampleId :

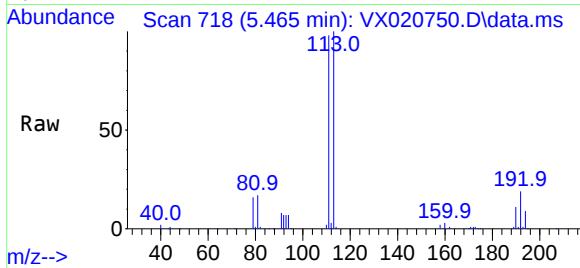



Tgt Ion:113 Resp: 162792
Ion Ratio Lower Upper
113 100
111 102.4 81.9 122.9
192 19.7 16.7 25.1

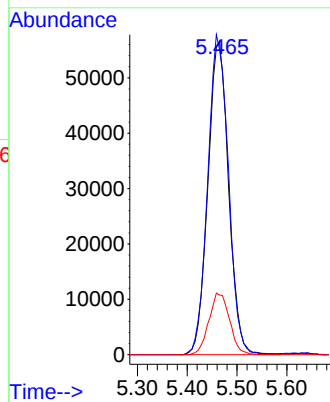


#36
1,1-Dichloropropene
Concen: 4.57 ug/l
RT: 5.617 min Scan# 743
Delta R.T. -0.152 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

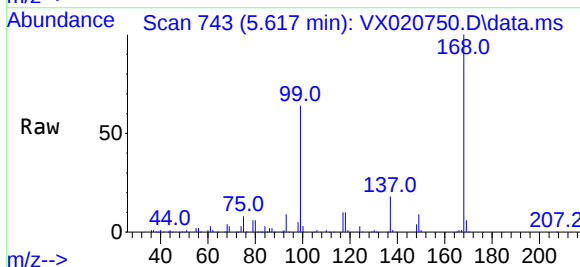

Tgt Ion: 75 Resp: 22693
Ion Ratio Lower Upper
75 100
110 8.6 18.1 54.4#
77 0.0 25.3 37.9#

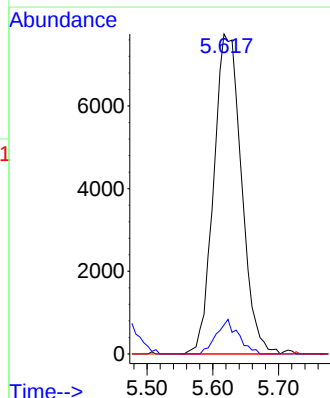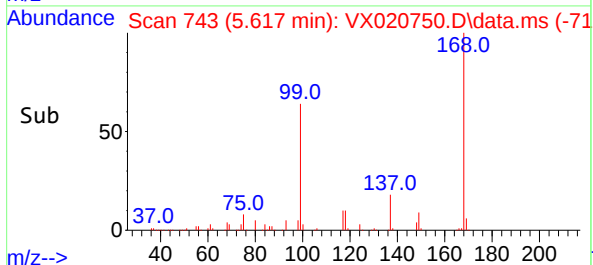







#37
Ethyl Acetate
Concen: 0.48 ug/l
RT: 4.794 min Scan# 608
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 43 Resp: 2239




Ion	Ratio	Lower	Upper
43	100		
61	7.8	12.8	19.2#
70	8.1	10.5	15.7#

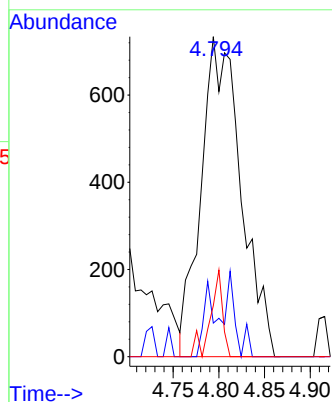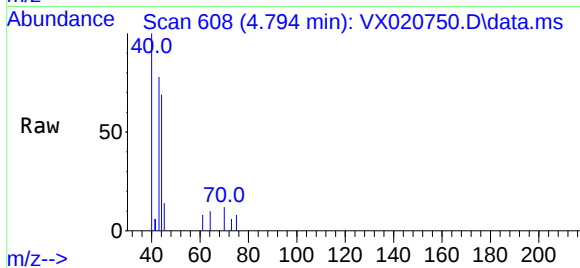


#38
Carbon Tetrachloride
Concen: 5.74 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.128 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 117 Resp: 30006

Ion	Ratio	Lower	Upper
117	100		
119	5.6	76.2	114.2#
121	0.0	24.8	37.2#

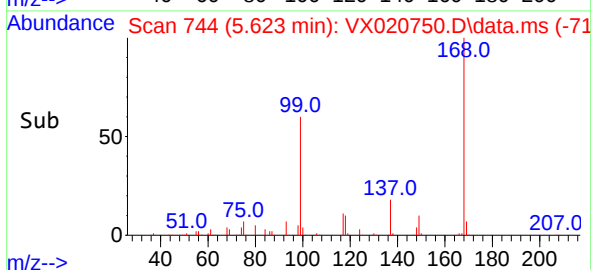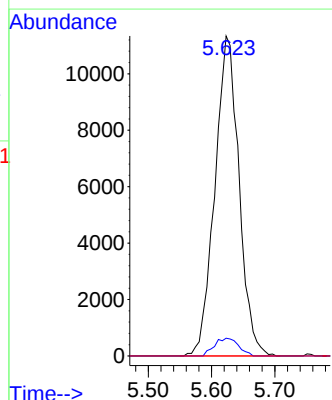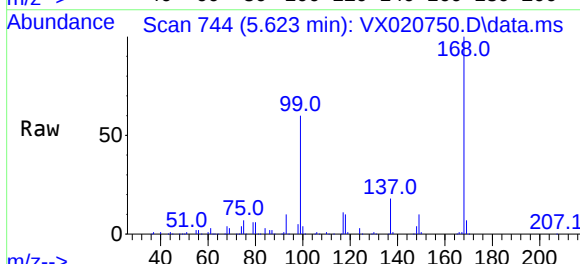



#39

Methylcyclohexane

Concen: 0.56 ug/l

RT: 7.434 min Scan# 1041





Delta R.T. -0.006 min

Lab File: VX020750.D

Acq: 26 Jan 2021 13:57

Tgt Ion: 83	Resp: 3166
Ion Ratio	Lower Upper
83 100	
55 81.5	58.9 88.3
98 45.2	38.1 57.1

Instrument :
MSVOA_X
ClientSampleId :

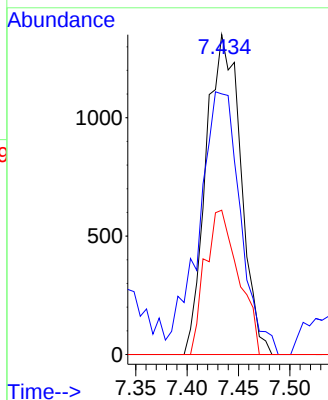

#40

Benzene

Concen: 4.81 ug/l




RT: 6.105 min Scan# 823


Delta R.T. -0.006 min

Lab File: VX020750.D

Acq: 26 Jan 2021 13:57

Tgt Ion: 78	Resp: 70362
Ion Ratio	Lower Upper
78 100	
77 21.9	18.9 28.3


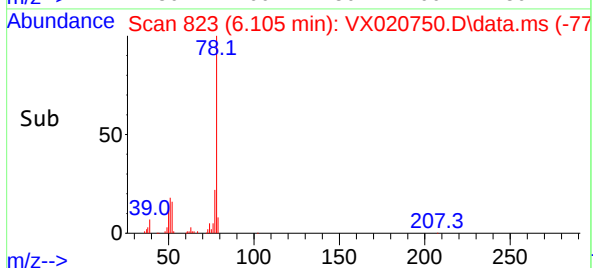
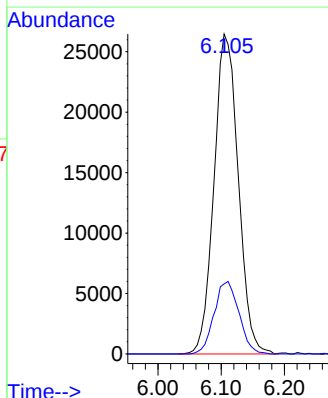





#50
Toluene-d8
Concen: 50.35 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 625951
Ion Ratio Lower Upper
98 100
100 65.1 51.9 77.9

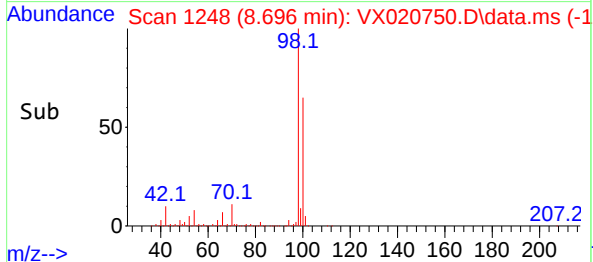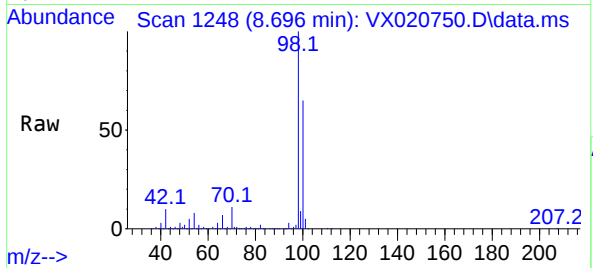

#51
4-Methyl-2-Pentanone
Concen: 0.22 ug/l
RT: 8.629 min Scan# 1237
Delta R.T. 0.013 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 43 Resp: 1023
Ion Ratio Lower Upper
43 100
58 25.4 35.4 53.0#


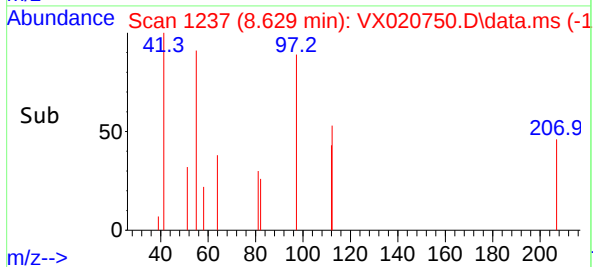

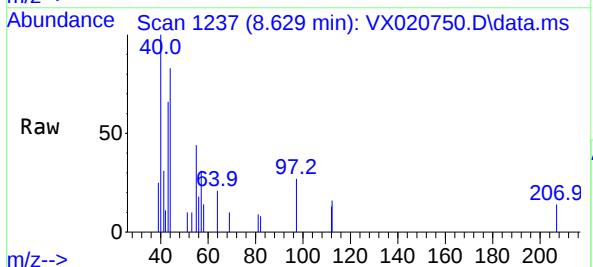




#52
Toluene
Concen: 37.18 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 92 Resp: 342133
Ion Ratio Lower Upper
92 100
91 170.1 137.1 205.7

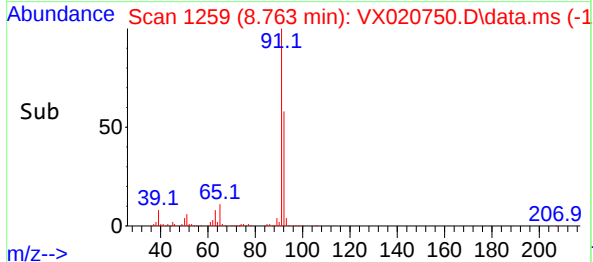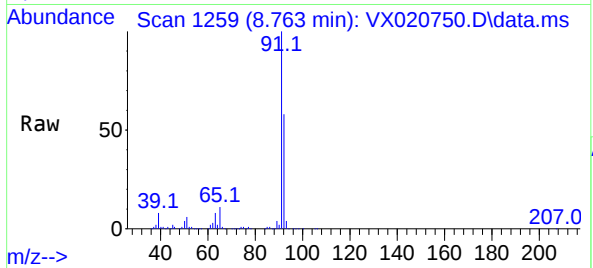

#53
t-1,3-Dichloropropene
Concen: 0.70 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. -0.256 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 75 Resp: 3971
Ion Ratio Lower Upper
75 100
77 182.9 24.9 37.3#


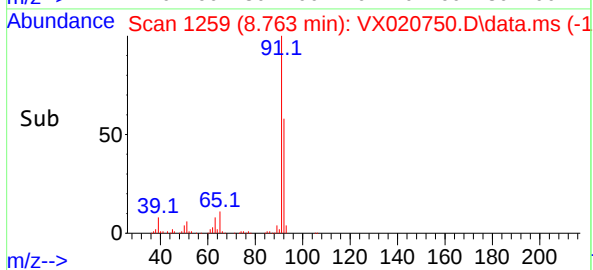






#55
1,1,2-Trichloroethane
Concen: 0.26 ug/l
RT: 9.141 min Scan# 1321
Delta R.T. -0.054 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 97	Resp: 1002
Ion Ratio	Lower Upper
97 100	
83 0.0	69.3 103.9#
85 18.4	44.3 66.5#
99 0.0	50.3 75.5#

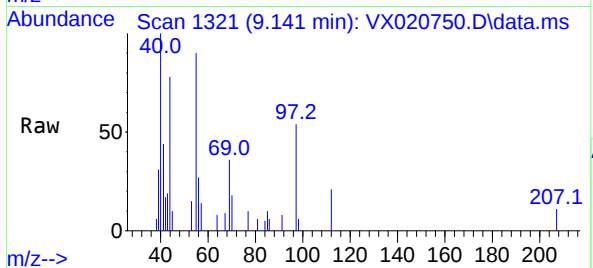

#56
Ethyl methacrylate
Concen: 3.16 ug/l
RT: 9.159 min Scan# 1324
Delta R.T. 0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 69	Resp: 2465
Ion Ratio	Lower Upper
69 100	
41 69.0	46.8 70.2
39 43.4	24.7 37.1#


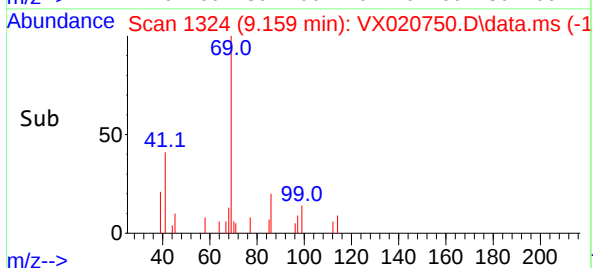
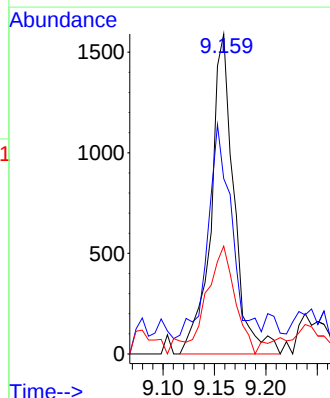





#62
4-Bromofluorobenzene
Concen: 51.21 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. 0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 247240
Ion Ratio Lower Upper
95 100
174 75.4 0.0 154.6
176 75.1 0.0 155.8

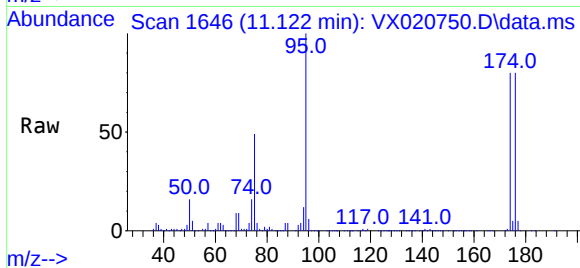

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.092 min Scan# 1477
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 117 Resp: 495533
Ion Ratio Lower Upper
117 100
82 56.4 47.4 71.2
119 30.9 26.6 39.8


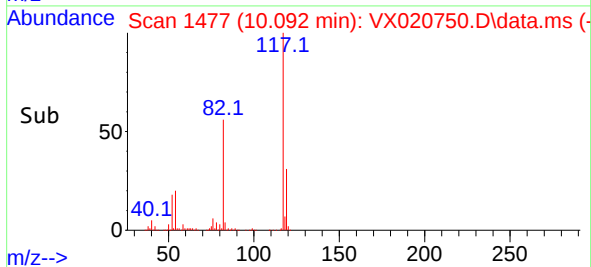

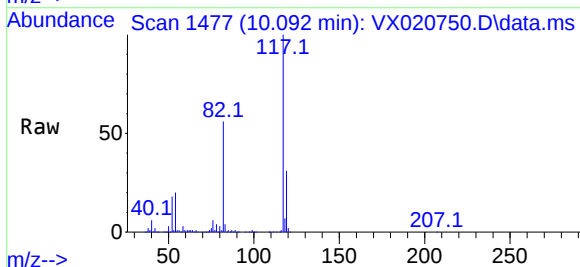


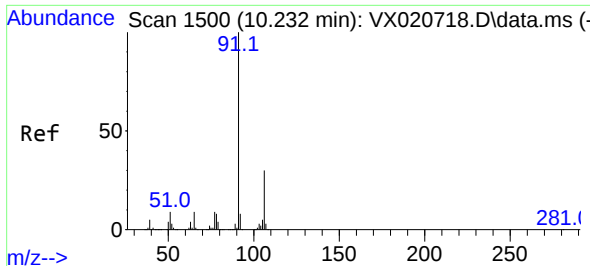

#67
Ethyl Benzene
Concen: 3.07 ug/l
RT: 10.232 min Scan# 1500
Delta R.T. 0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 57035
Ion Ratio Lower Upper
91 100
106 31.0 24.6 37.0

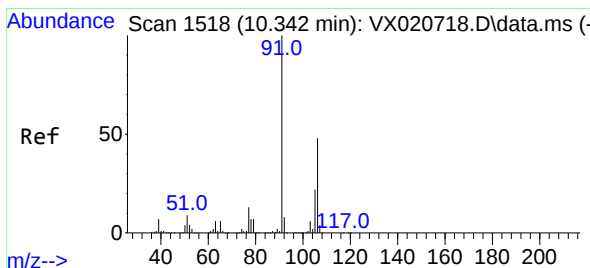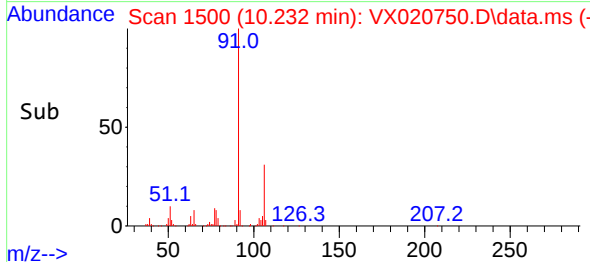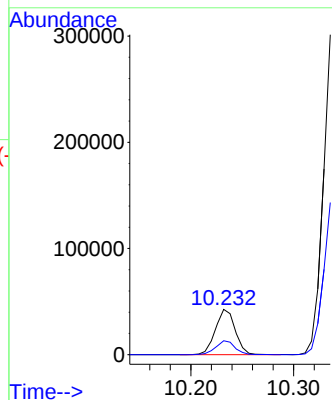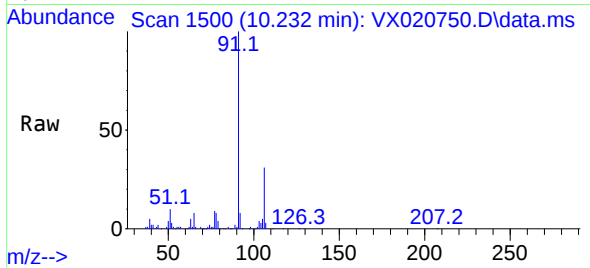

#68
m/p-Xylenes
Concen: 28.87 ug/l
RT: 10.342 min Scan# 1518
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion:106 Resp: 200144
Ion Ratio Lower Upper
106 100
91 208.4 162.8 244.2


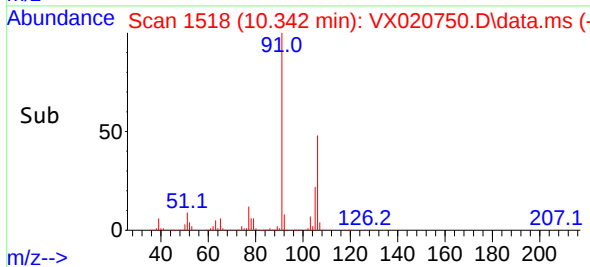
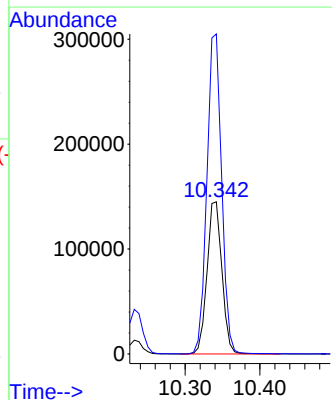
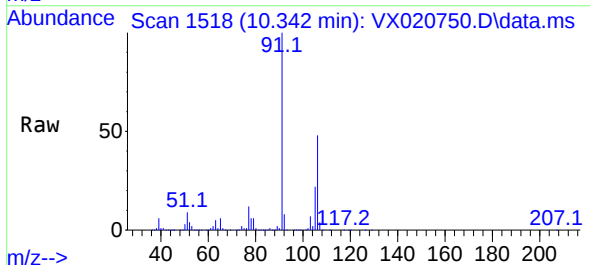




#69
o-Xylene
Concen: 16.60 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. 0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:106 Resp: 108251
Ion Ratio Lower Upper
106 100
91 219.4 108.1 324.2

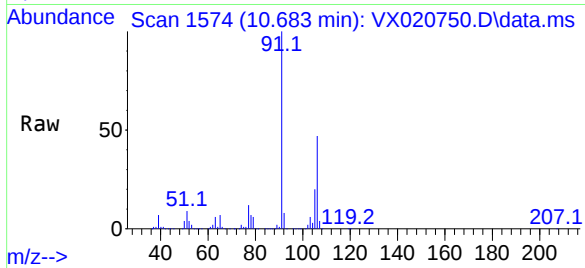

#70
Styrene
Concen: 0.54 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. -0.012 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion:104 Resp: 6044
Ion Ratio Lower Upper
104 100
78 270.4 40.0 60.0#
103 243.4 43.4 65.0#


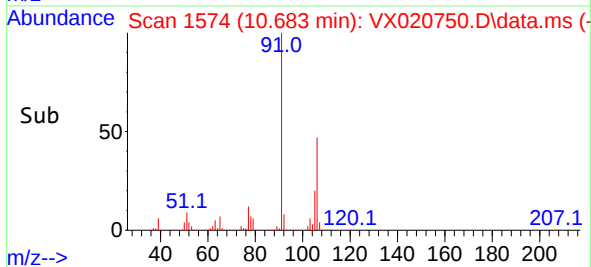

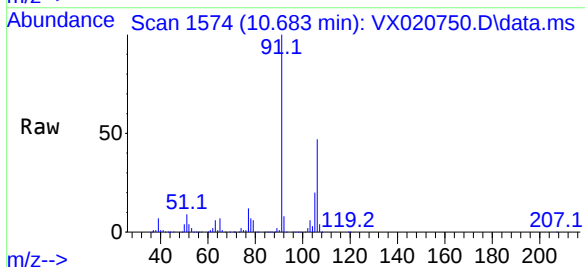




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:152 Resp: 226301
Ion Ratio Lower Upper
152 100
115 62.0 41.1 123.3
150 160.6 0.0 349.0

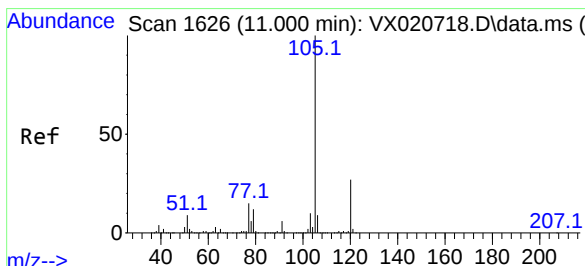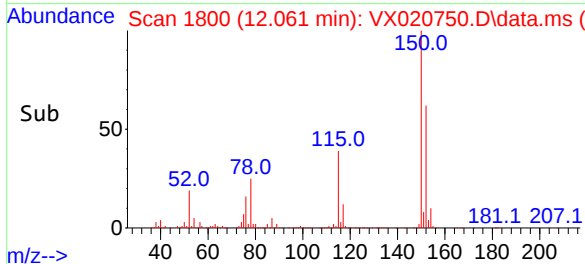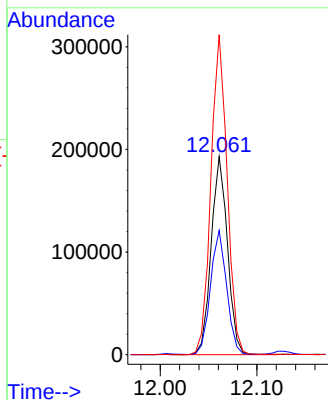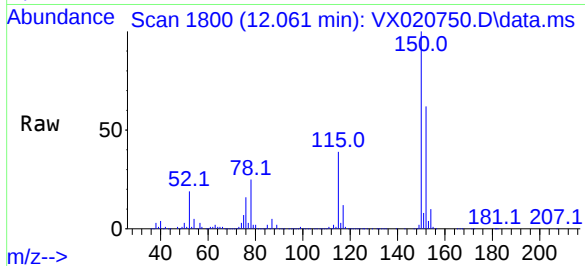

#73
Isopropylbenzene
Concen: 0.22 ug/l
RT: 11.000 min Scan# 1626
Delta R.T. 0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57


Tgt Ion:105 Resp: 3544
Ion Ratio Lower Upper
105 100
120 28.9 13.2 39.6

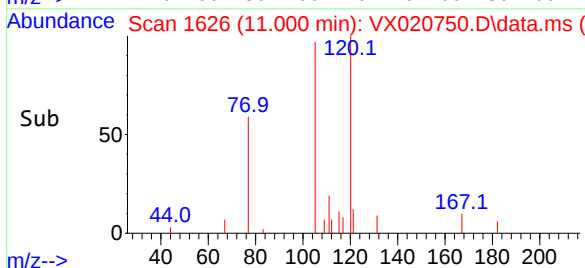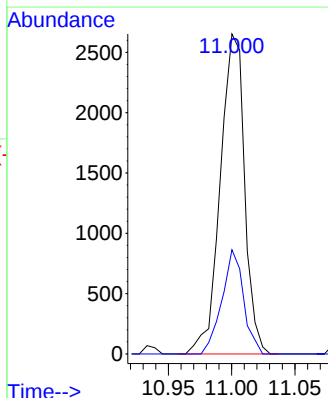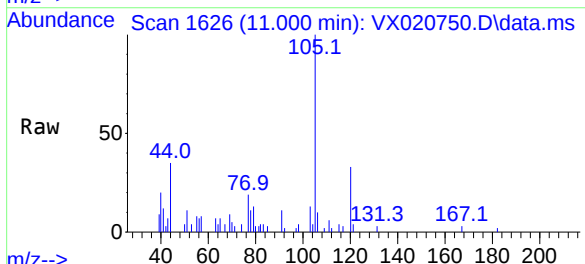






#74
N-amy1 acetate
Concen: 2.13 ug/l
RT: 10.897 min Scan# 1609
Delta R.T. 0.019 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Instrument :
MSVOA_X
ClientSampleId :

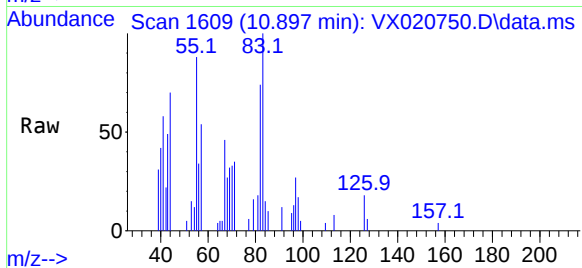

Tgt Ion: 43 Resp: 826




Ion	Ratio	Lower	Upper
43	100		
70	49.0	39.0	58.6
55	352.3	21.5	32.3#
61	0.0	22.1	33.1#

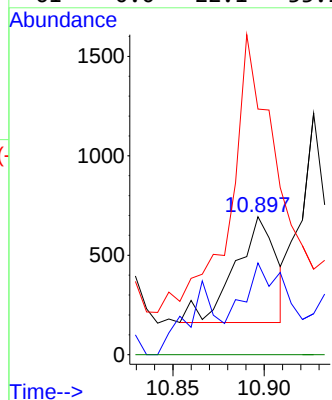


#76
1,2,3-Trichloropropane
Concen: 23.02 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.158 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 75 Resp: 120819

Ion	Ratio	Lower	Upper
75	100		
77	1.7	19.1	57.5#


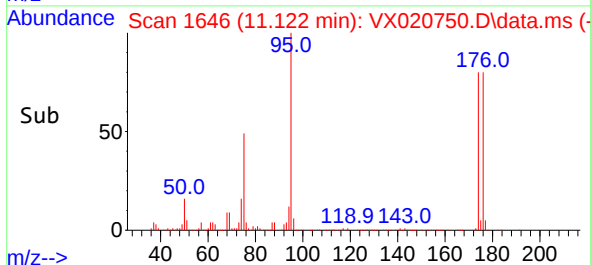
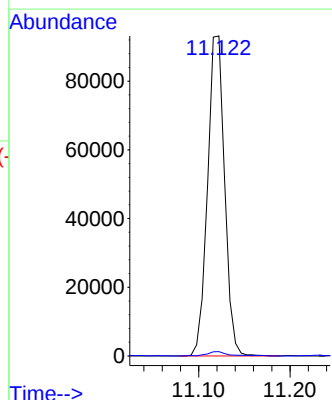
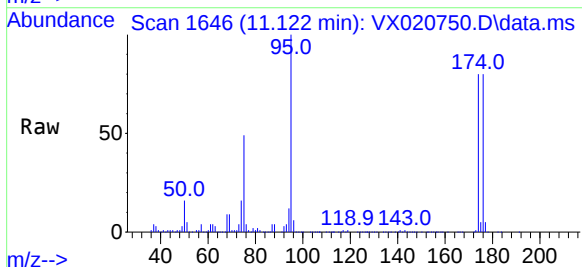




#78
n-propylbenzene
Concen: 0.57 ug/l
RT: 11.342 min Scan# 1682
Delta R.T. 0.001 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 10805
Ion Ratio Lower Upper
91 100
120 22.7 11.5 34.5

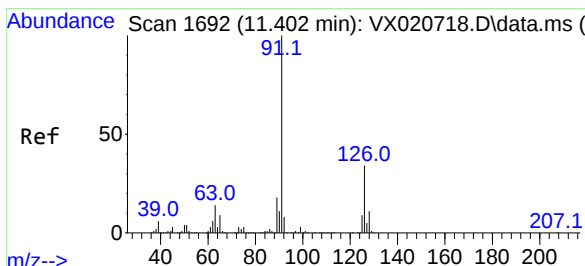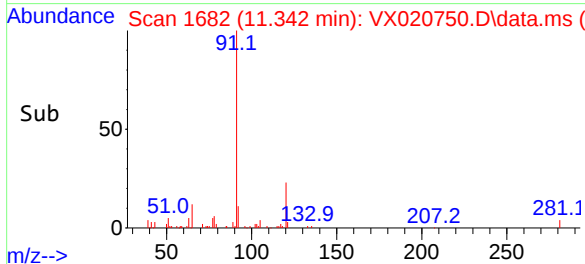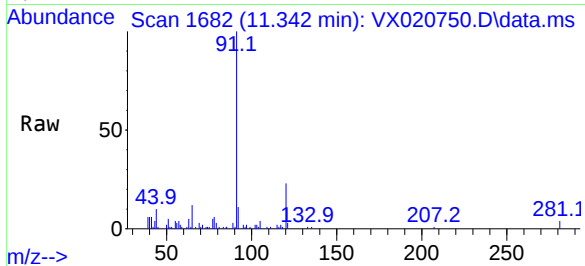

#79
2-Chlorotoluene
Concen: 2.16 ug/l
RT: 11.415 min Scan# 1694
Delta R.T. 0.013 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 91 Resp: 24872
Ion Ratio Lower Upper
91 100
126 0.2 16.6 49.8#


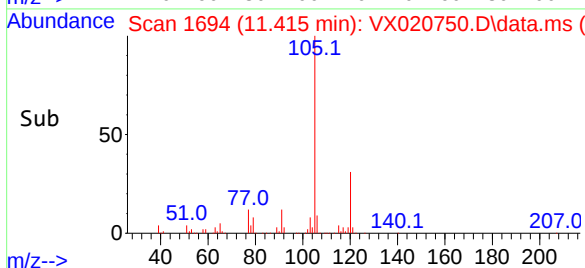
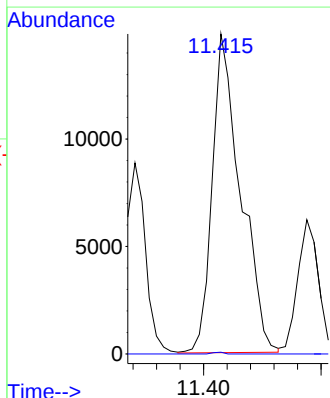
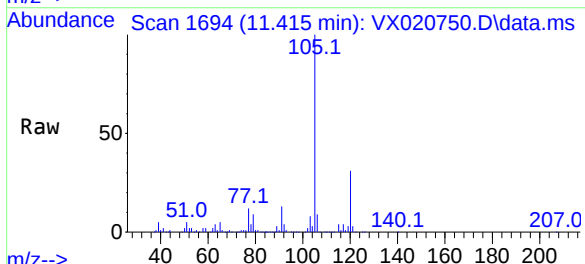




#80
1,3,5-Trimethylbenzene
Concen: 4.95 ug/l
RT: 11.488 min Scan# 1706
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 69212
Ion Ratio Lower Upper
105 100
120 47.5 23.8 71.5

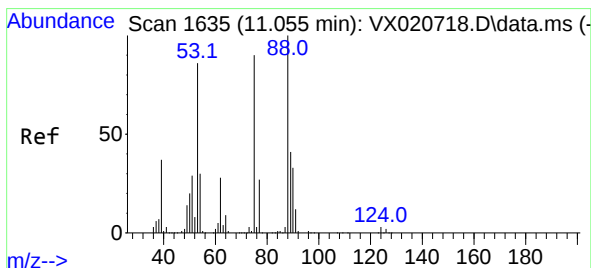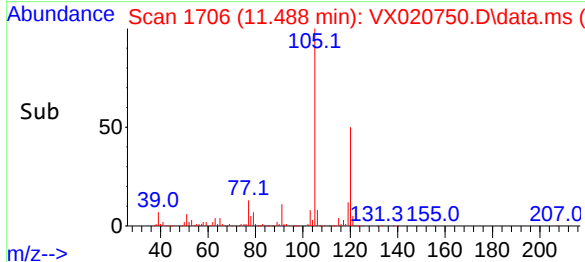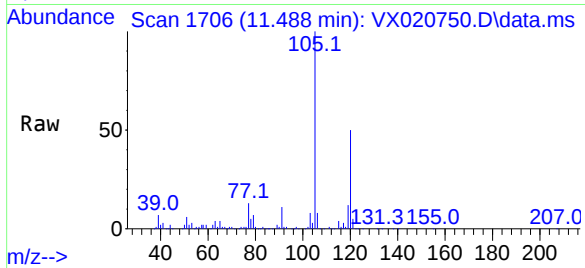

#81
trans-1,4-Dichloro-2-butene
Concen: 64.51 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. 0.067 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 75 Resp: 120819
Ion Ratio Lower Upper
75 100
53 0.5 74.5 111.7#
89 0.0 37.9 56.9#


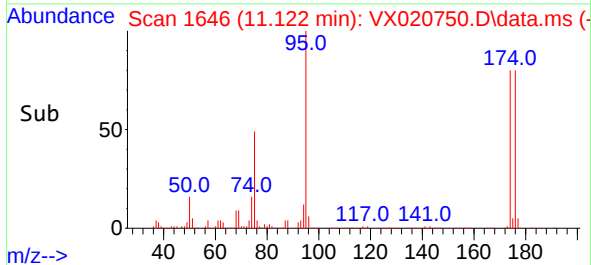

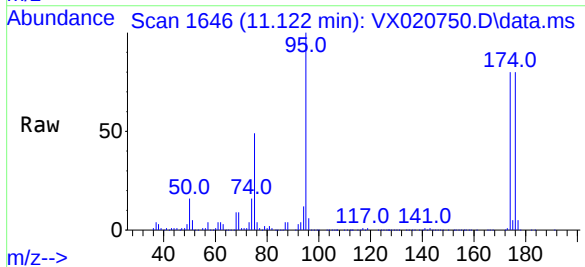




#82
4-Chlorotoluene
Concen: 0.54 ug/l
RT: 11.488 min Scan# 1706
Delta R.T. -0.006 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 7409
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

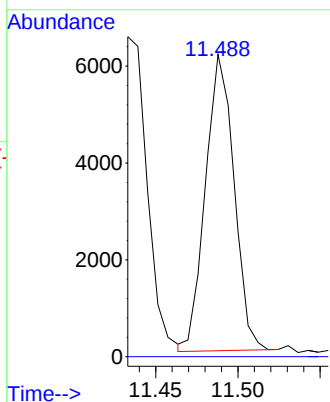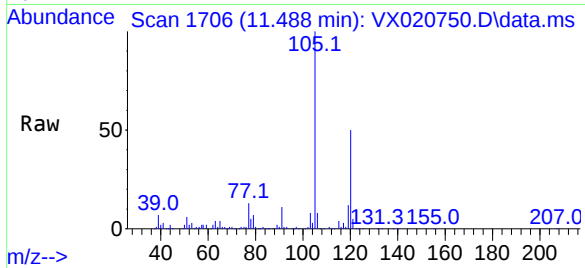

#83
tert-Butylbenzene
Concen: 2.32 ug/l
RT: 11.787 min Scan# 1755
Delta R.T. 0.037 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 119 Resp: 31323
Ion Ratio Lower Upper
119 100
91 92.3 27.9 83.7#
134 0.3 11.3 33.9#


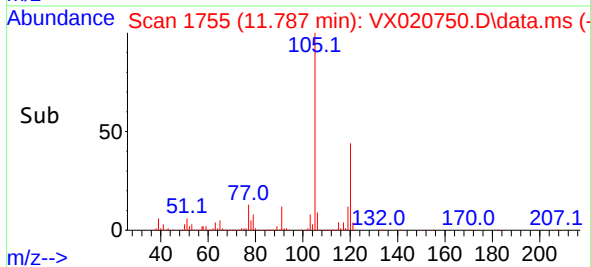

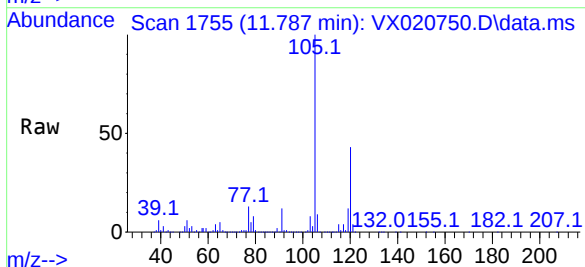




#84
1,2,4-Trimethylbenzene
Concen: 18.83 ug/l
RT: 11.793 min Scan# 1756
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 265462
Ion Ratio Lower Upper
105 100
120 44.3 22.4 67.3

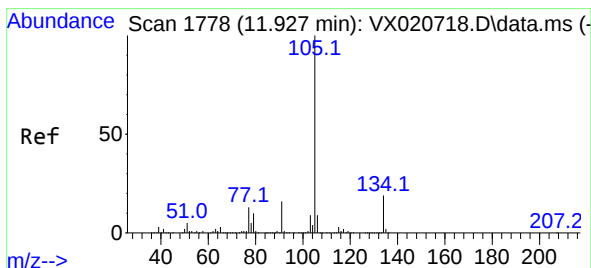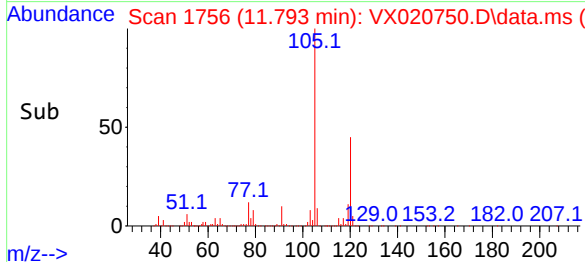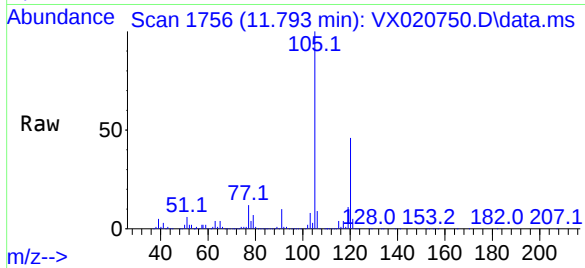

#85
sec-Butylbenzene
Concen: 17.01 ug/l
RT: 11.793 min Scan# 1756
Delta R.T. -0.134 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion:105 Resp: 265462
Ion Ratio Lower Upper
105 100
134 0.0 10.0 29.8#


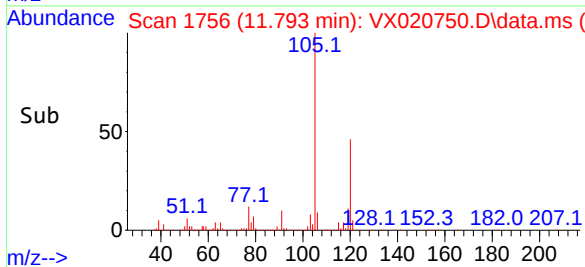

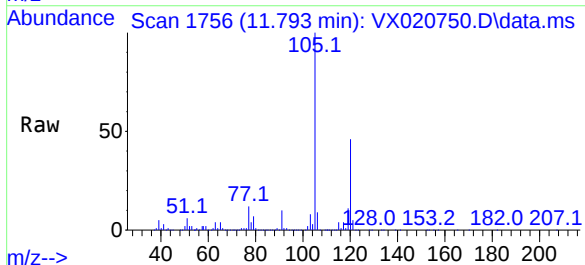




#86
p-Isopropyltoluene
Concen: 0.39 ug/l
RT: 12.049 min Scan# 1798
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:	119	Resp:	5584
Ion	Ratio	Lower	Upper
119	100		
134	28.1	12.9	38.7
91	32.5	11.7	35.0

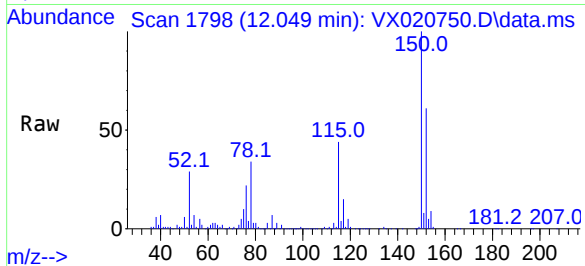

#89
n-Butylbenzene
Concen: 1.10 ug/l
RT: 12.360 min Scan# 1849
Delta R.T. -0.012 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion:	91	Resp:	14254
Ion	Ratio	Lower	Upper
91	100		
92	30.0	27.4	82.0
134	113.5	13.2	39.5#


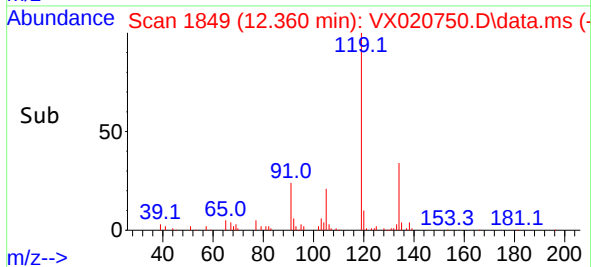

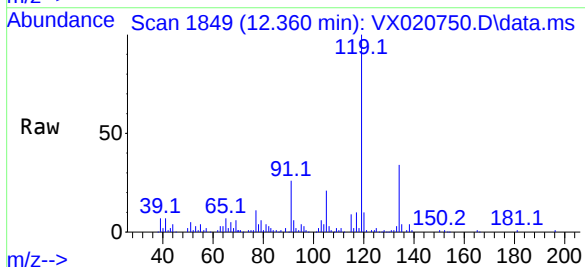




#90
Hexachloroethane
Concen: 1.19 ug/l
RT: 12.567 min Scan# 1883
Delta R.T. -0.012 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:117 Resp: 3099
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

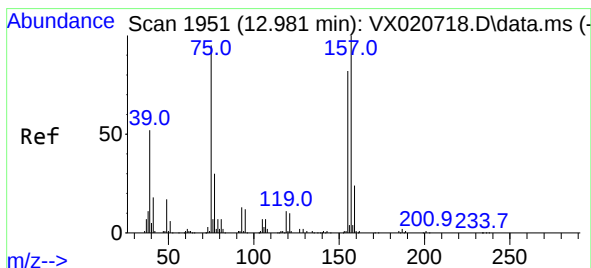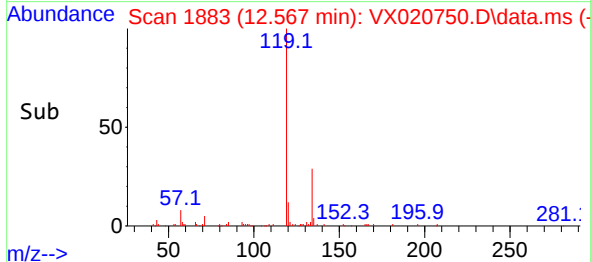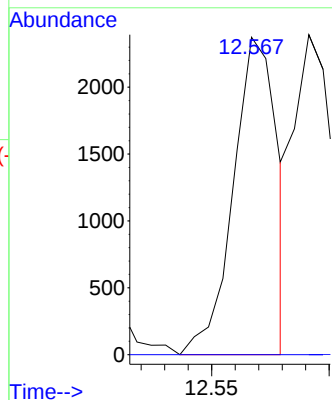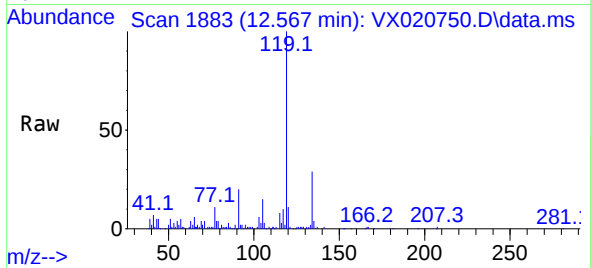

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.32 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. -0.018 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Tgt Ion: 75 Resp: 390
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

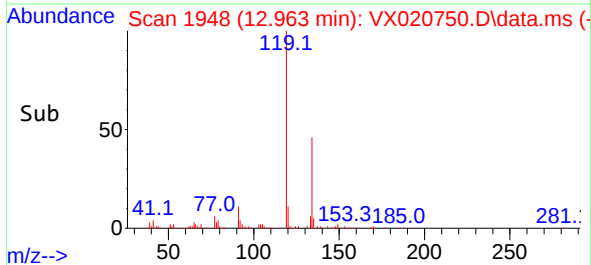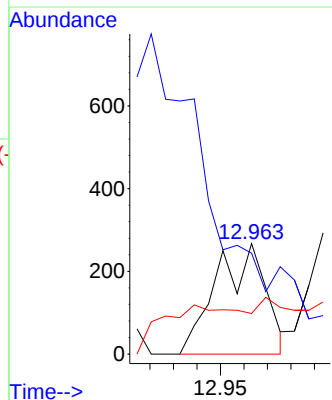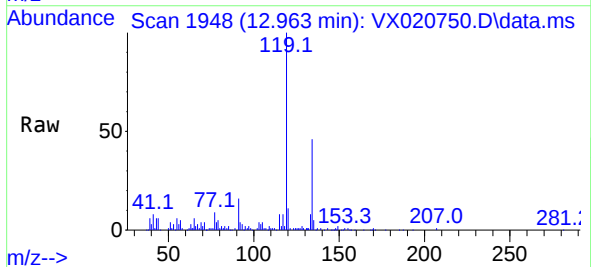

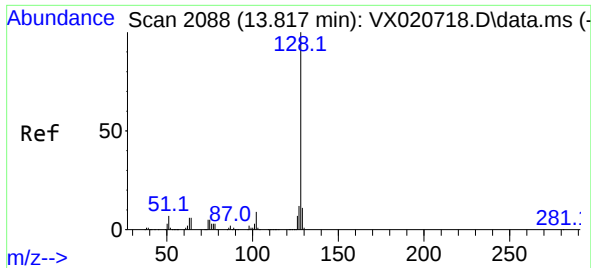

#95
Naphthalene
Concen: 7.76 ug/l
RT: 13.817 min Scan# 2088
Delta R.T. -0.000 min
Lab File: VX020750.D
Acq: 26 Jan 2021 13:57

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:	128	Resp:	90011
Ion	Ratio	Lower	Upper
128	100		
127	12.3	10.3	15.5
129	11.3	8.8	13.2

