

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
 Data File : VX020753.D
 Acq On : 26 Jan 2021 15:07
 Operator : JC/SP
 Sample : M1189-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 27 00:55:36 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	332847	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	562156	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	537744	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	248444	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	214591	47.27	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	94.54%		
35) Dibromofluoromethane	5.464	113	182042	47.28	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	94.56%		
50) Toluene-d8	8.695	98	693811	49.15	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	98.30%		
62) 4-Bromofluorobenzene	11.122	95	261902	47.77	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	95.54%		
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.185	85	23	1.20	ug/l #	42
5) Bromomethane	1.636	94	477	0.21	ug/l	93
11) Tert butyl alcohol	3.014	59	15732	18.56	ug/l	95
13) Acrolein	2.282	56	608	0.95	ug/l	83
14) Allyl chloride	2.831	41	40984	6.88	ug/l #	27
16) Acetone	2.416	43	45054	26.17	ug/l	99
17) Carbon Disulfide	2.544	76	966	0.99	ug/l	96
18) Methyl Acetate	2.751	43	7437	1.69	ug/l	92
20) Methylene Chloride	2.831	84	1110926	255.74	ug/l	97
22) Diisopropyl ether	3.757	45	5567	0.48	ug/l #	1
25) 2-Butanone	4.641	43	42615	15.81	ug/l	98
29) Tetrahydrofuran	5.111	42	526	0.30	ug/l #	53
36) 1,1-Dichloropropene	5.629	75	26011	4.61	ug/l #	49
37) Ethyl Acetate	4.641	43	42615	7.97	ug/l #	65
38) Carbon Tetrachloride	5.623	117	33923	5.72	ug/l #	17
40) Benzene	6.104	78	21027	1.27	ug/l	95
44) Trichloroethene	7.190	130	904	0.20	ug/l	89
48) Methyl methacrylate	7.738	41	884	0.21	ug/l #	13
49) 1,4-Dioxane	7.720	88	789	7.81	ug/l #	81
51) 4-Methyl-2-Pentanone	8.616	43	2074	0.39	ug/l	88
52) Toluene	8.762	92	88833	8.50	ug/l	99
56) Ethyl methacrylate	9.183	69	83	2.79	ug/l #	29
59) 2-Hexanone	9.464	43	998	0.25	ug/l	82
67) Ethyl Benzene	10.232	91	9692	0.48	ug/l	93
68) m/p-Xylenes	10.341	106	18603	2.47	ug/l	94
69) o-Xylene	10.683	106	9498	1.34	ug/l	98
70) Styrene	10.695	104	3338	0.27	ug/l #	69
74) N-amyl acetate	10.927	43	376	2.06	ug/l #	60
76) 1,2,3-Trichloropropane	11.122	75	128605	22.32	ug/l #	39
80) 1,3,5-Trimethylbenzene	11.488	105	4233	0.28	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.122	75	128605	62.54	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.792	105	12676	0.82	ug/l	98
95) Naphthalene	13.816	128	47640	5.23	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
Data File : VX020753.D
Acq On : 26 Jan 2021 15:07
Operator : JC/SP
Sample : M1189-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 27 00:55:36 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration




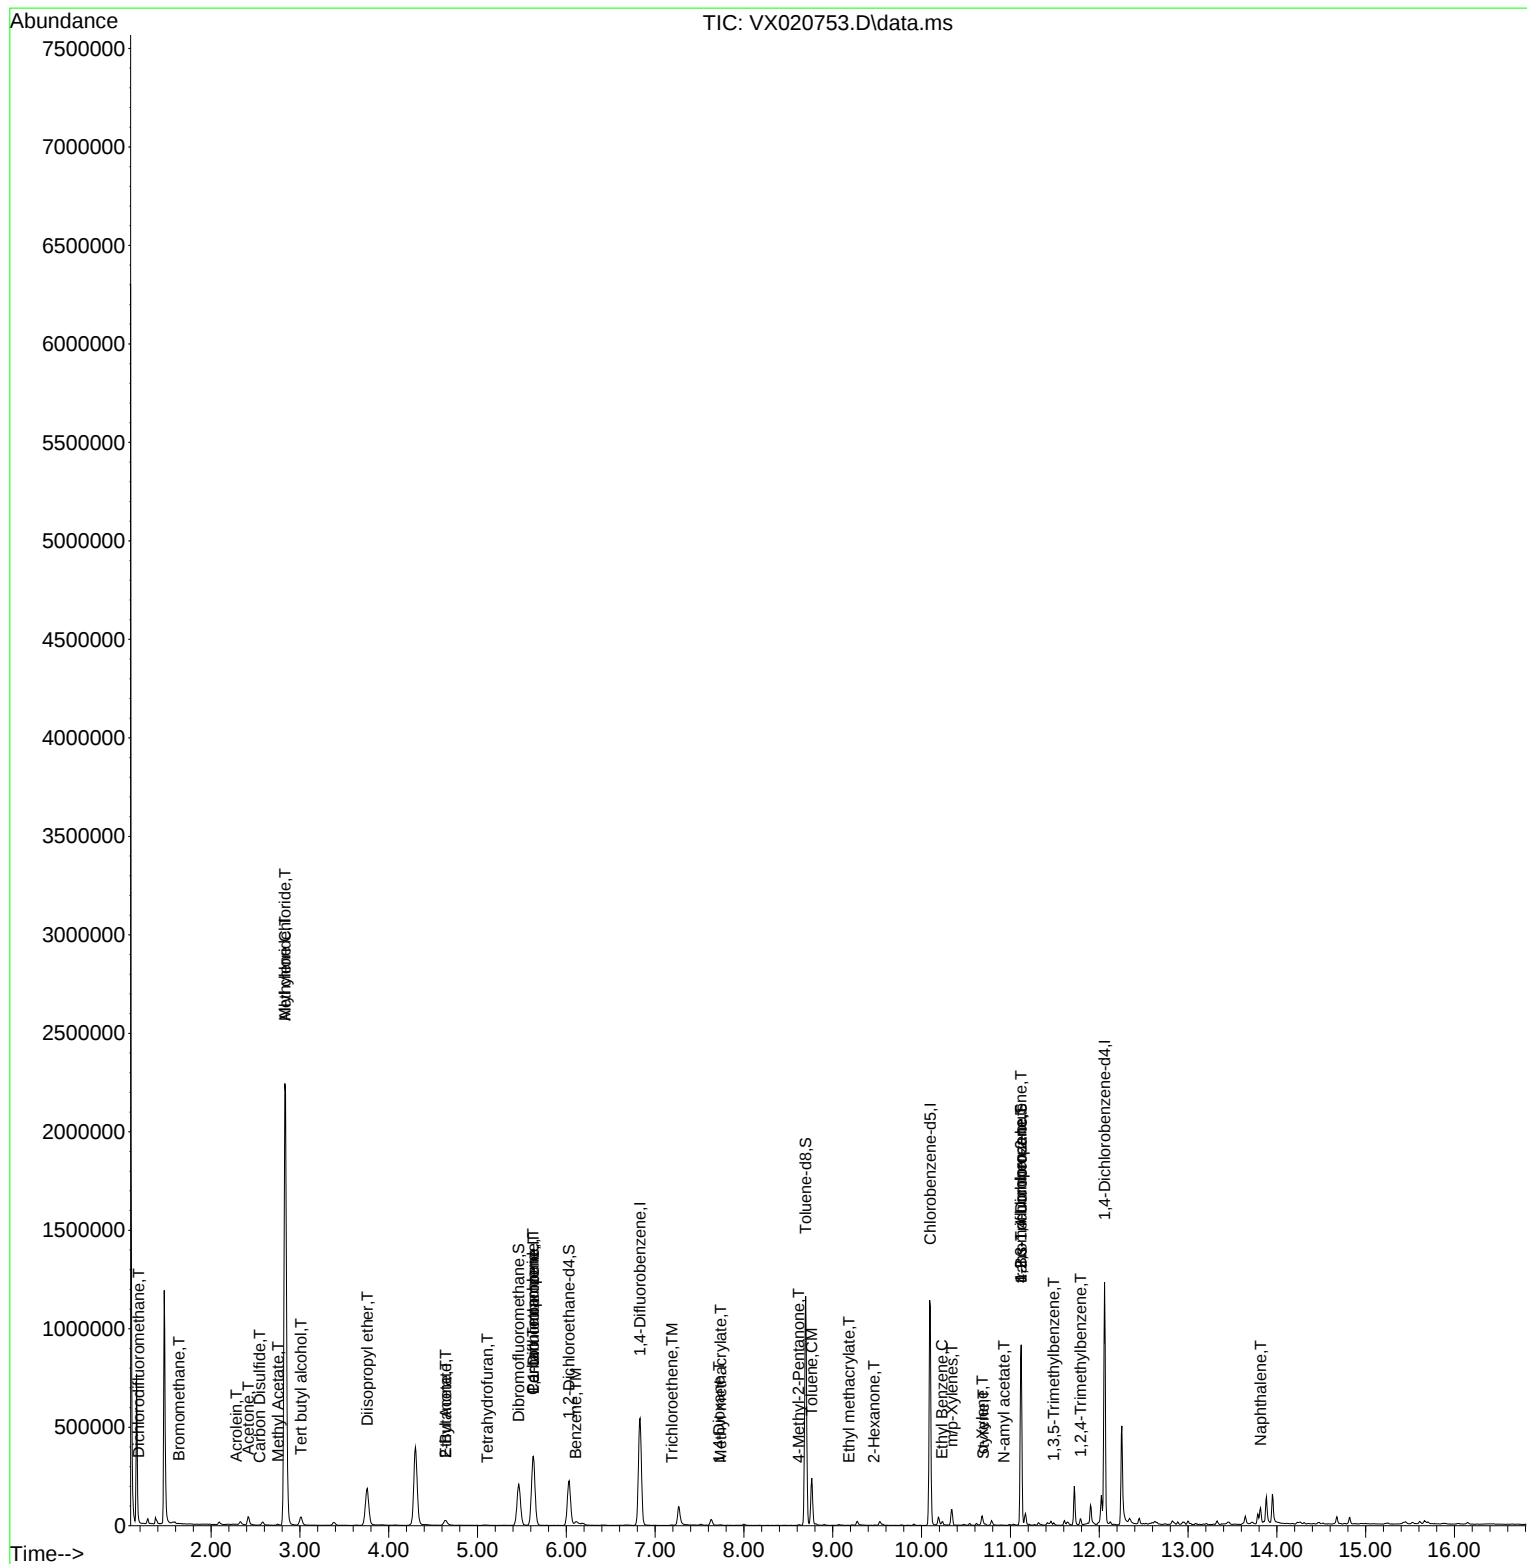




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 332847
Ion Ratio Lower Upper
168 100
99 60.2 45.8 68.6



#2
Dichlorodifluoromethane
Concen: 1.20 ug/l
RT: 1.185 min Scan# 16
Delta R.T. -0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 85 Resp: 23
Ion Ratio Lower Upper
85 100
87 0.0 16.4 49.2#







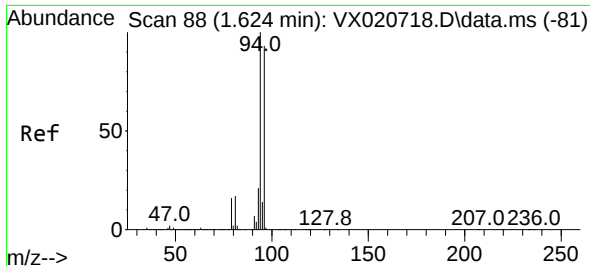

#5
Bromomethane
Concen: 0.21 ug/l
RT: 1.636 min Scan# 90
Delta R.T. 0.012 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 94 Resp: 477
Ion Ratio Lower Upper
94 100
96 89.0 76.4 114.6

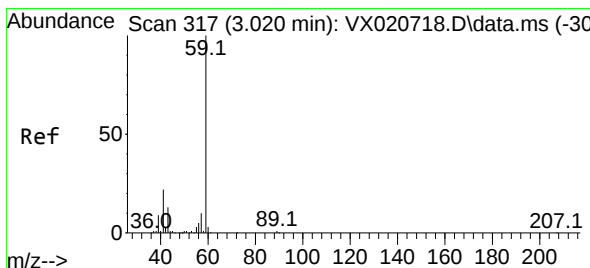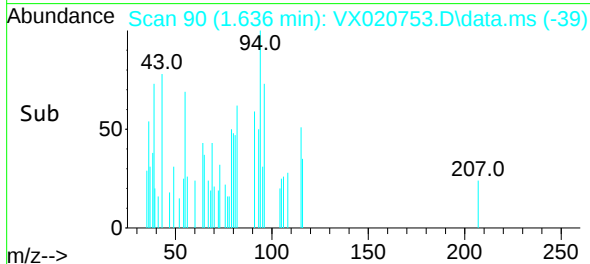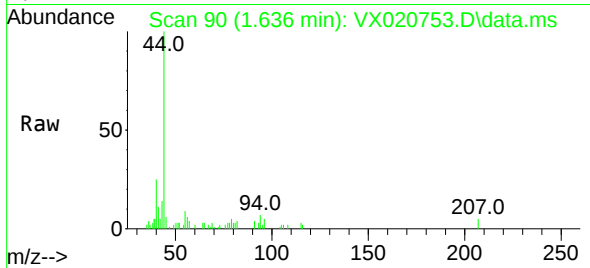

#11
Tert butyl alcohol
Concen: 18.56 ug/l
RT: 3.014 min Scan# 316
Delta R.T. -0.006 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 59 Resp: 15732
Ion Ratio Lower Upper
59 100
57 11.6 7.8 11.8


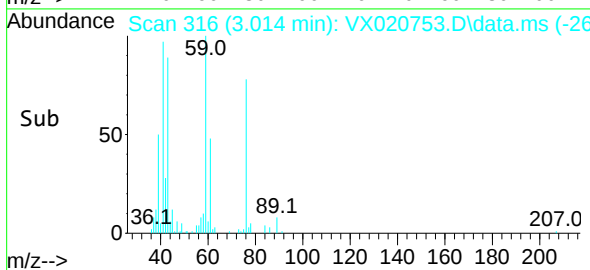

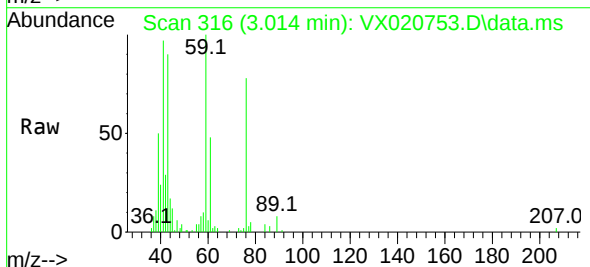


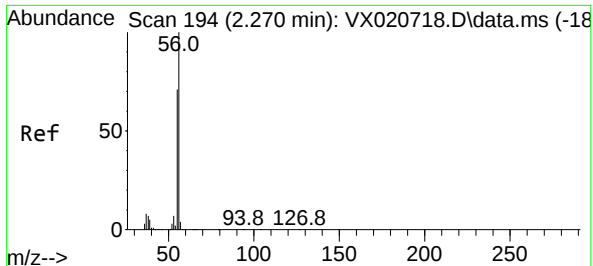

#13
Acrolein
Concen: 0.95 ug/l
RT: 2.282 min Scan# 196
Delta R.T. 0.012 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 56 Resp: 608
Ion Ratio Lower Upper
56 100
55 84.4 56.4 84.6

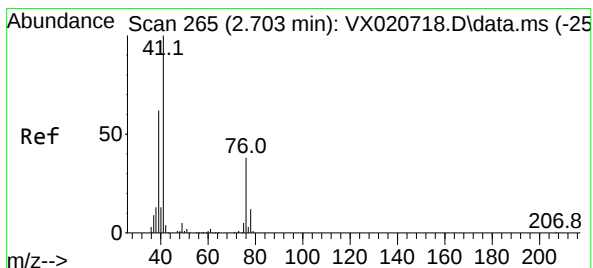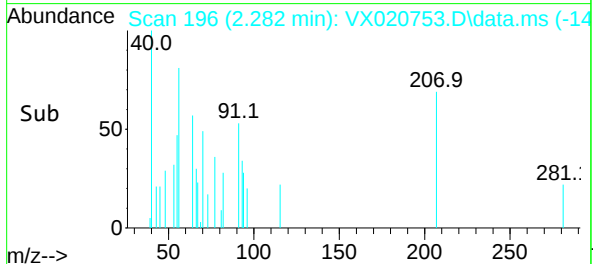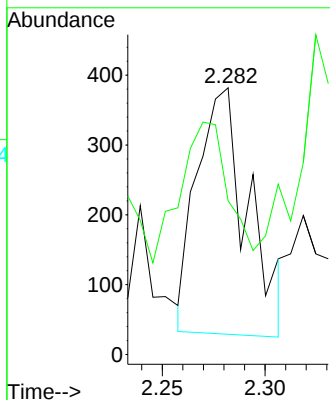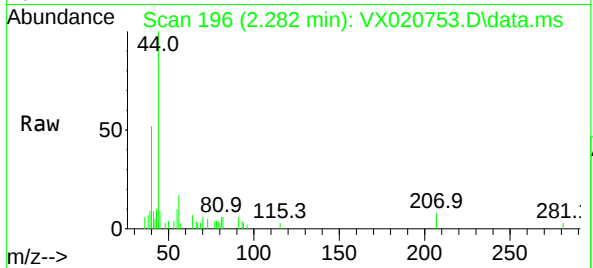

#14
Allyl chloride
Concen: 6.88 ug/l
RT: 2.831 min Scan# 286
Delta R.T. 0.128 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 41 Resp: 40984
Ion Ratio Lower Upper
41 100
39 2.3 51.6 77.4#
76 0.0 30.5 45.7#


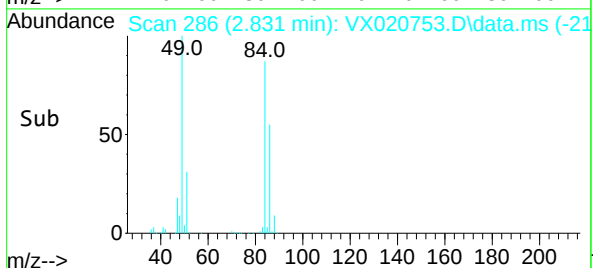
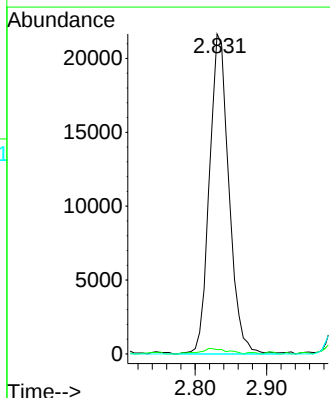
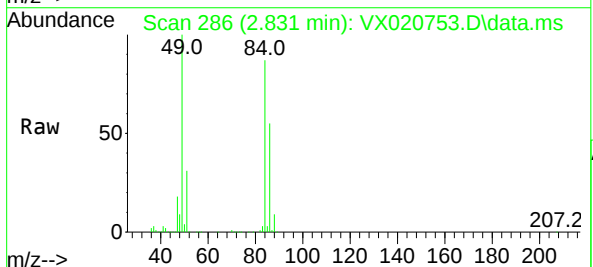




#16
Acetone
Concen: 26.17 ug/l
RT: 2.416 min Scan# 218
Delta R.T. -0.006 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 45054
Ion Ratio Lower Upper
43 100
58 35.6 27.8 41.8

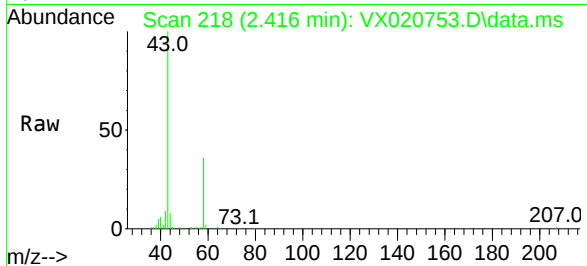

#17
Carbon Disulfide
Concen: 0.99 ug/l
RT: 2.544 min Scan# 239
Delta R.T. 0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 76 Resp: 966
Ion Ratio Lower Upper
76 100
78 10.6 7.2 10.8

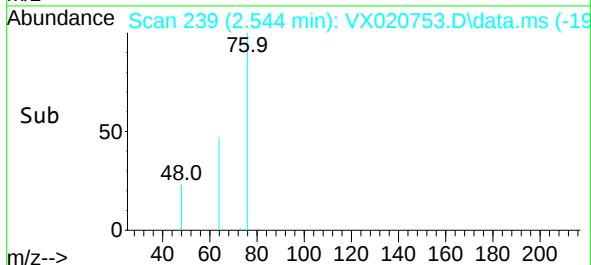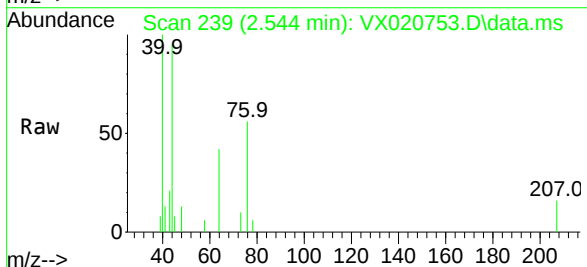



#18

Methyl Acetate

Concen: 1.69 ug/l

RT: 2.751 min Scan# 273

Delta R.T. 0.006 min

Lab File: VX020753.D





Acq: 26 Jan 2021 15:07

Tgt Ion: 43 Resp: 7437

Ion Ratio Lower Upper

43 100

74 23.0 21.9 32.9

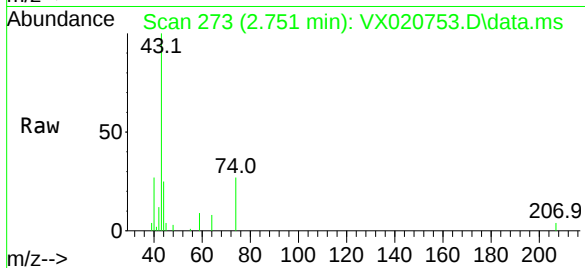

#20

Methylene Chloride

Concen: 255.74 ug/l

RT: 2.831 min Scan# 286

Delta R.T. -0.000 min

Lab File: VX020753.D

Acq: 26 Jan 2021 15:07

Tgt Ion: 84 Resp: 1110926




Ion Ratio Lower Upper


84 100

49 115.1 88.6 132.8

51 35.9 27.0 40.6


86 63.4 50.3 75.5

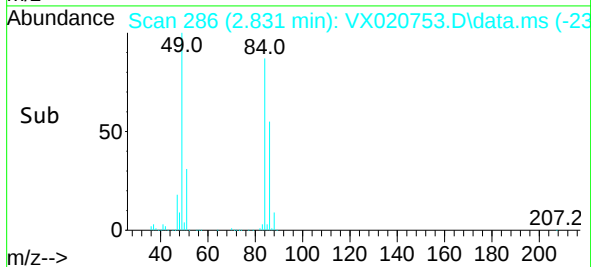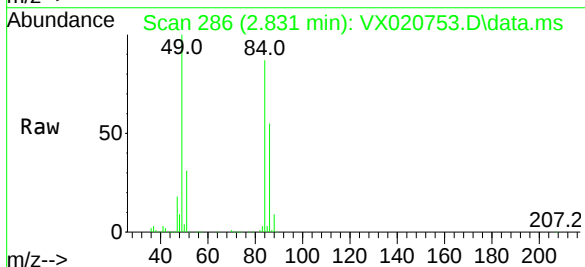






#22
Diisopropyl ether
Concen: 0.48 ug/l
RT: 3.757 min Scan# 438
Delta R.T. -0.068 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07


Instrument :
MSVOA_X
ClientSampled :

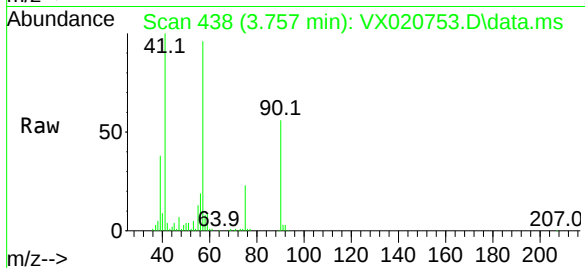



Tgt Ion: 45	Resp: 5567
Ion Ratio	Lower Upper
45	100
43	17.2 58.0 87.0#
87	0.0 25.4 38.0#
59	201.2 10.2 15.2#

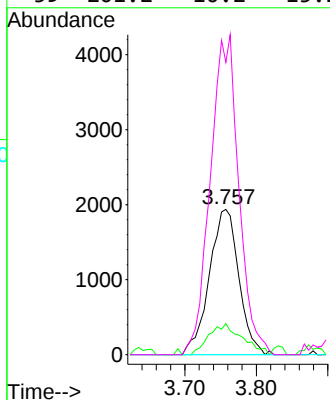


#25
2-Butanone
Concen: 15.81 ug/l
RT: 4.641 min Scan# 583
Delta R.T. 0.006 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

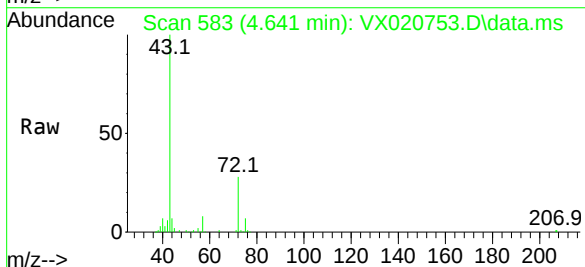

Tgt Ion: 43	Resp: 42615
Ion Ratio	Lower Upper
43	100
72	28.5 23.7 35.5

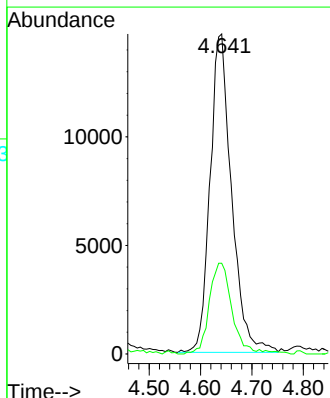



#29

Tetrahydrofuran

Concen: 0.30 ug/l

RT: 5.111 min Scan# 660





Delta R.T. 0.025 min

Lab File: VX020753.D

Acq: 26 Jan 2021 15:07

Tgt Ion:	42	Resp:	526
Ion	Ratio	Lower	Upper
42	100		
72	26.8	41.7	62.5#
71	7.6	38.4	57.6#

Instrument :
MSVOA_X
ClientSampleId :

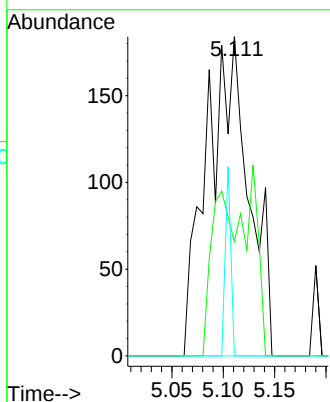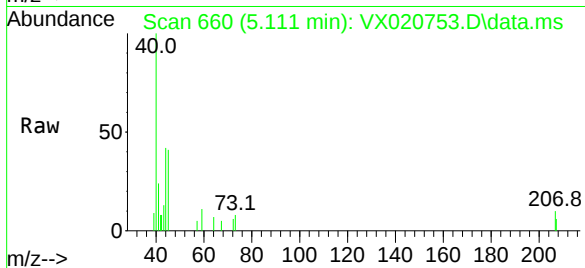

#33

1,2-Dichloroethane-d4

Concen: 47.27 ug/l




RT: 6.031 min Scan# 811


Delta R.T. 0.006 min

Lab File: VX020753.D

Acq: 26 Jan 2021 15:07

Tgt Ion:	65	Resp:	214591
Ion	Ratio	Lower	Upper
65	100		
67	52.5	0.0	105.4


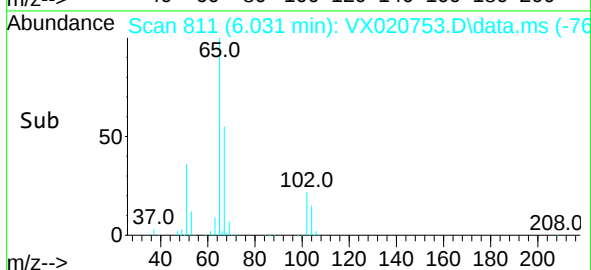
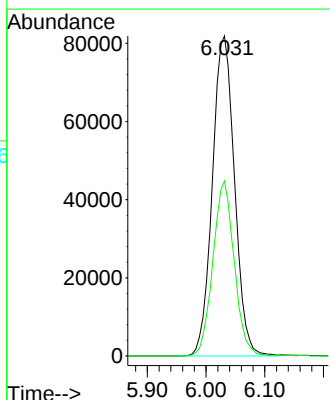
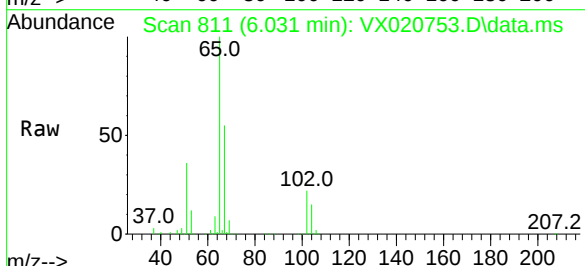




#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. -0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 562156
Ion Ratio Lower Upper
114 100
63 20.4 0.0 40.8
88 17.2 0.0 32.8



#35
Dibromofluoromethane
Concen: 47.28 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07


Tgt Ion:113 Resp: 182042
Ion Ratio Lower Upper
113 100
111 103.5 81.9 122.9
192 19.5 16.7 25.1

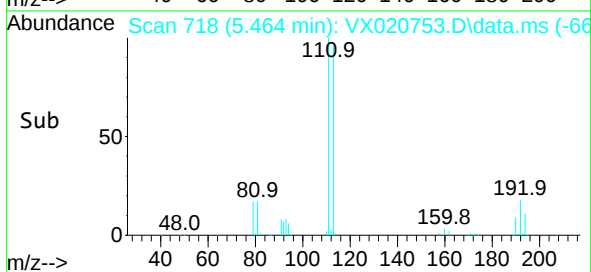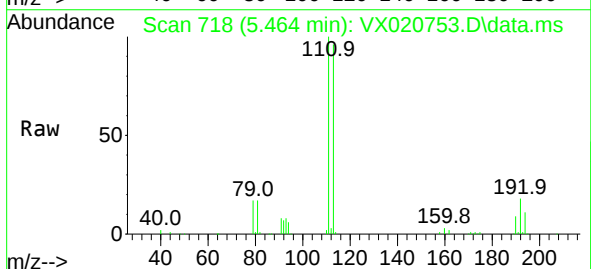






#36
1,1-Dichloropropene
Concen: 4.61 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.140 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 75 Resp: 26011
Ion Ratio Lower Upper
75 100
110 9.6 18.1 54.4#
77 0.0 25.3 37.9#




#37
Ethyl Acetate
Concen: 7.97 ug/l
RT: 4.641 min Scan# 583
Delta R.T. -0.153 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Tgt Ion: 43 Resp: 42615
Ion Ratio Lower Upper
43 100
61 0.2 12.8 19.2#
70 0.1 10.5 15.7#

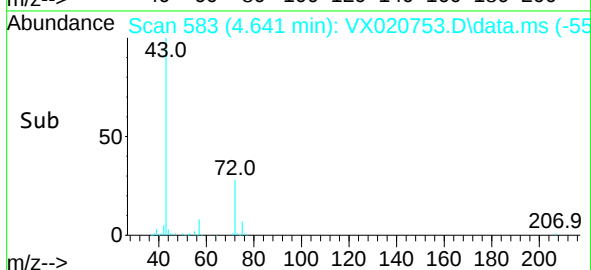






#38
Carbon Tetrachloride
Concen: 5.72 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.128 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:117 Resp: 33923
Ion Ratio Lower Upper
117 100
119 5.5 76.2 114.2#
121 0.0 24.8 37.2#




#40
Benzene
Concen: 1.27 ug/l
RT: 6.104 min Scan# 823
Delta R.T. -0.007 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07



Tgt Ion: 78 Resp: 21027
Ion Ratio Lower Upper
78 100
77 21.1 18.9 28.3




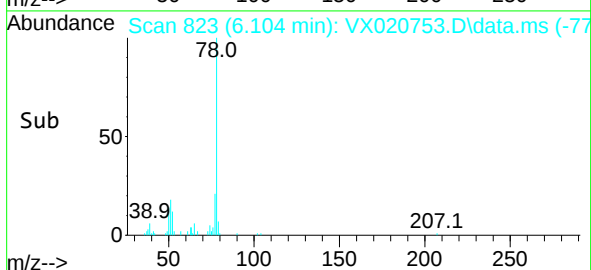


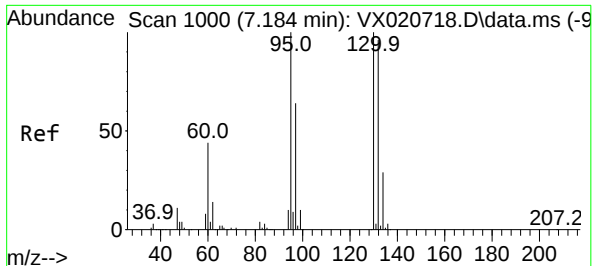

#44
Trichloroethene
Concen: 0.20 ug/l
RT: 7.190 min Scan# 1001
Delta R.T. 0.006 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:130 Resp: 904
Ion Ratio Lower Upper
130 100
95 88.3 0.0 198.0

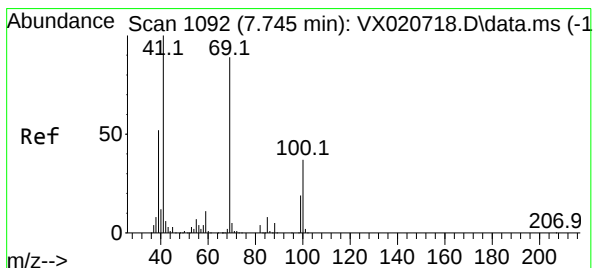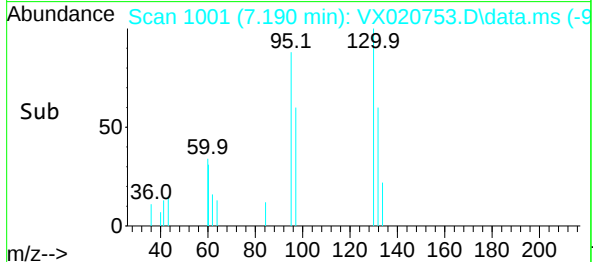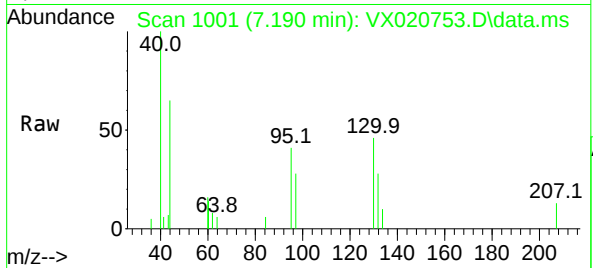

#48
Methyl methacrylate
Concen: 0.21 ug/l
RT: 7.738 min Scan# 1091
Delta R.T. -0.007 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 41 Resp: 884
Ion Ratio Lower Upper
41 100
69 5.0 76.0 114.0#
39 0.0 44.6 67.0#

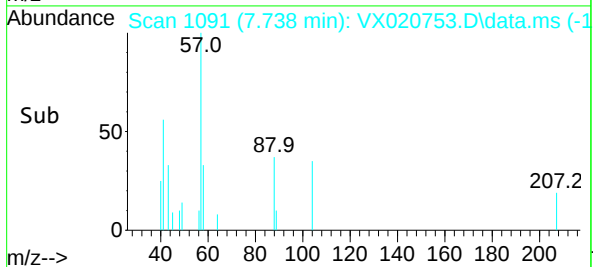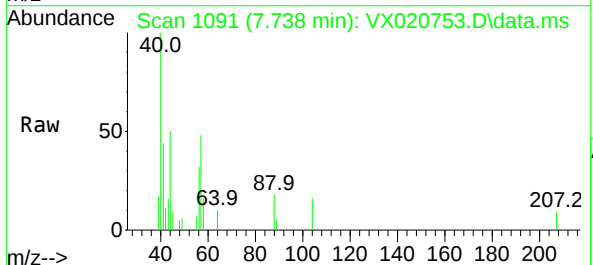



#49

1,4-Dioxane

Concen: 7.81 ug/l

RT: 7.720 min Scan# 1088





Delta R.T. 0.006 min

Lab File: VX020753.D

Acq: 26 Jan 2021 15:07

Tgt Ion: 88 Resp: 789

Ion	Ratio	Lower	Upper
88	100		
43	0.0	23.2	34.8#
58	72.1	55.0	82.4



#50

Toluene-d8

Concen: 49.15 ug/l

RT: 8.695 min Scan# 1248




Delta R.T. -0.001 min

Lab File: VX020753.D


Acq: 26 Jan 2021 15:07

Tgt Ion: 98 Resp: 693811

Ion	Ratio	Lower	Upper
98	100		
100	66.0	51.9	77.9

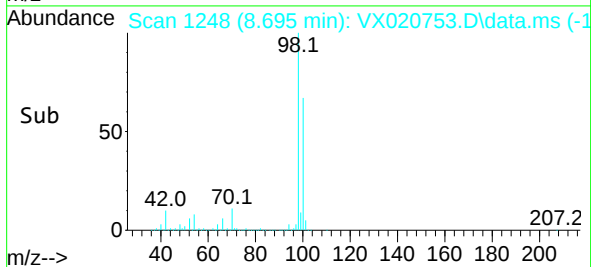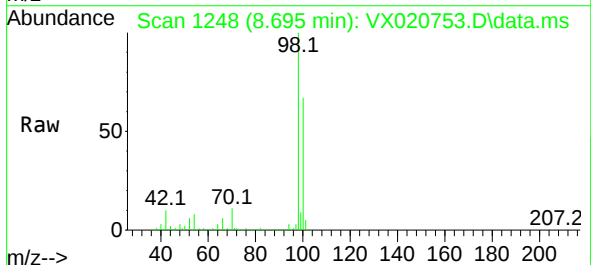





Instrument :
MSVOA_X
ClientSampleId :



#51
4-Methyl-2-Pentanone
Concen: 0.39 ug/l
RT: 8.616 min Scan# 1235
Delta R.T. 0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 2074
Ion Ratio Lower Upper
43 100
58 36.5 35.4 53.0



#52
Toluene
Concen: 8.50 ug/l
RT: 8.762 min Scan# 1259
Delta R.T. -0.001 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 92 Resp: 88833
Ion Ratio Lower Upper
92 100
91 172.7 137.1 205.7




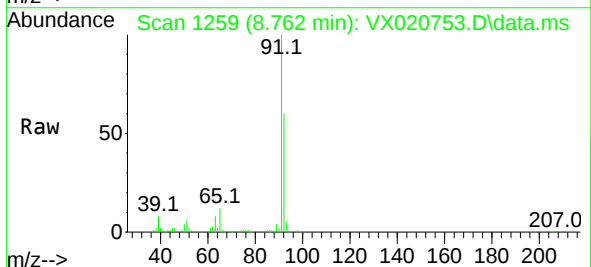


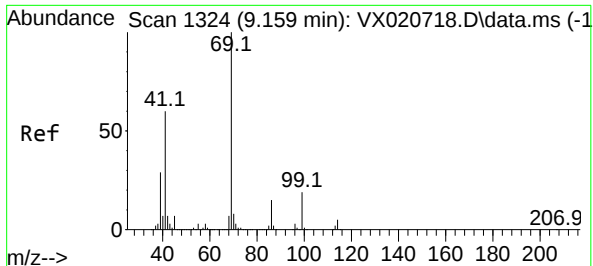

#56
Ethyl methacrylate
Concen: 2.79 ug/l
RT: 9.183 min Scan# 1328
Delta R.T. 0.024 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 69 Resp: 83
Ion Ratio Lower Upper
69 100
41 0.0 46.8 70.2#
39 0.0 24.7 37.1#

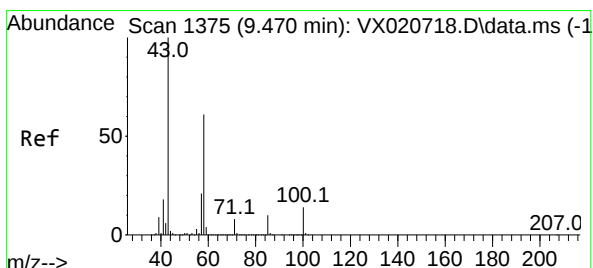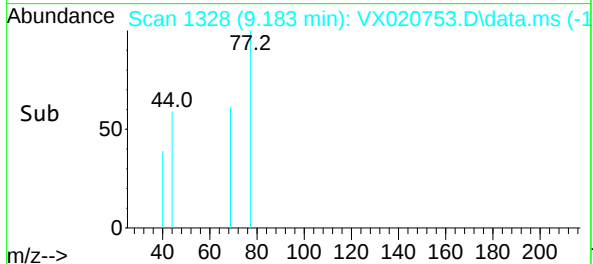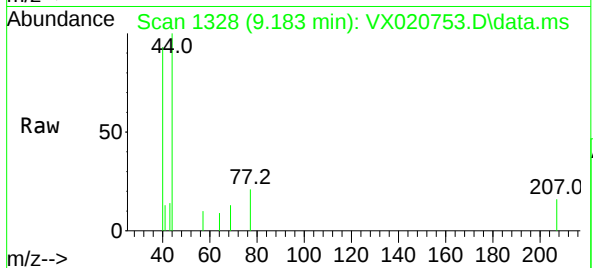

#59
2-Hexanone
Concen: 0.25 ug/l
RT: 9.464 min Scan# 1374
Delta R.T. -0.006 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 43 Resp: 998
Ion Ratio Lower Upper
43 100
58 47.9 30.9 92.8


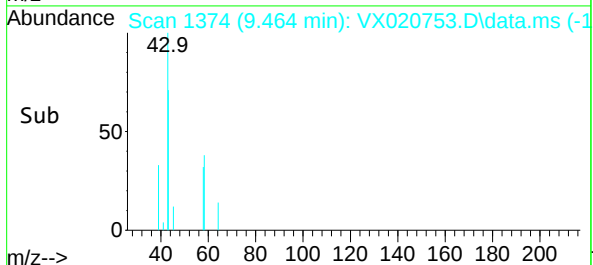

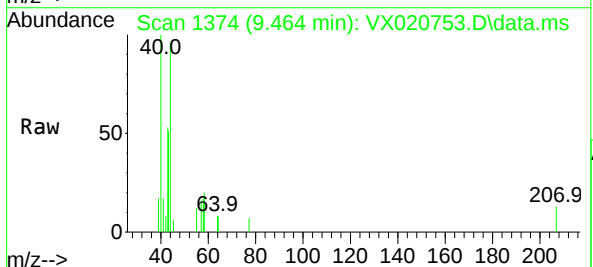




#62
4-Bromofluorobenzene
Concen: 47.77 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 261902
Ion Ratio Lower Upper
95 100
174 77.1 0.0 154.6
176 73.1 0.0 155.8

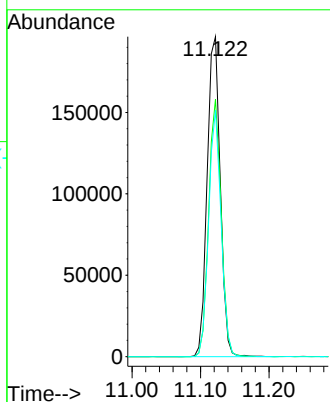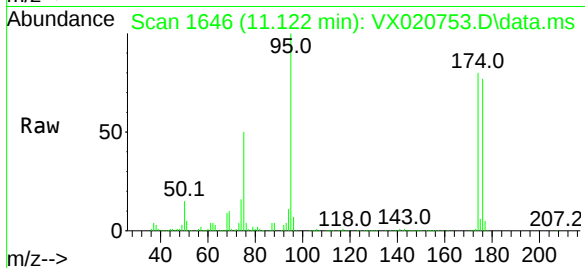

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 117 Resp: 537744
Ion Ratio Lower Upper
117 100
82 56.1 47.4 71.2
119 32.1 26.6 39.8


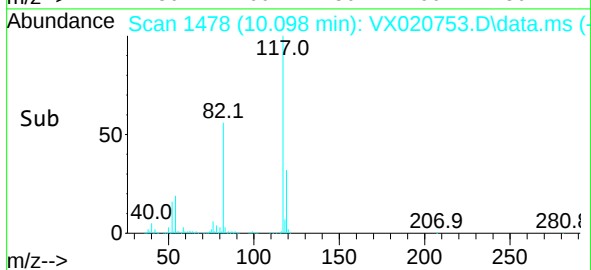
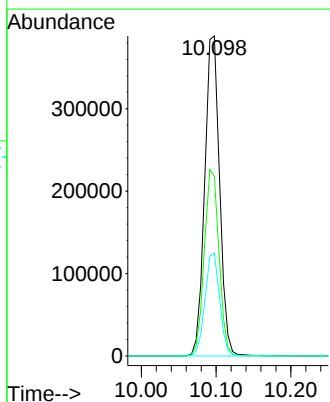
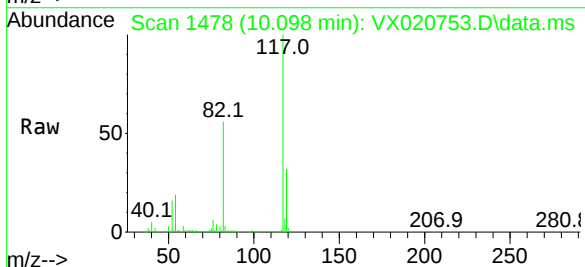


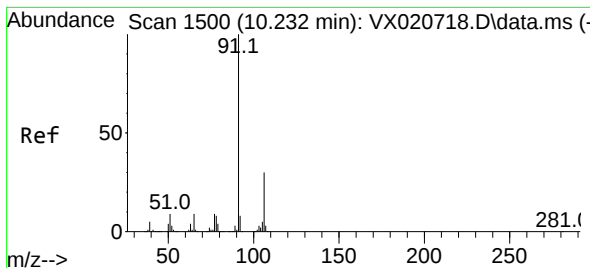

#67
Ethyl Benzene
Concen: 0.48 ug/l
RT: 10.232 min Scan# 1500
Delta R.T. -0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 9692
Ion Ratio Lower Upper
91 100
106 34.5 24.6 37.0

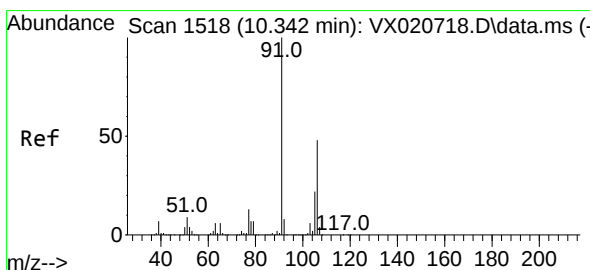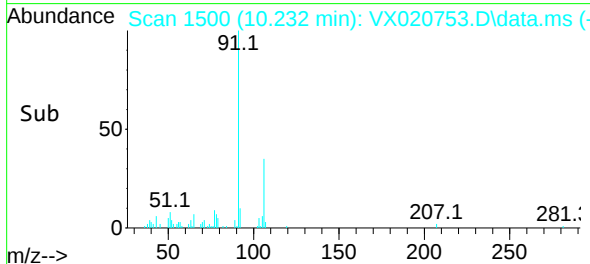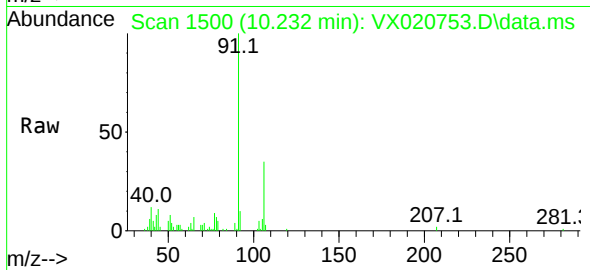

#68
m/p-Xylenes
Concen: 2.47 ug/l
RT: 10.341 min Scan# 1518
Delta R.T. -0.001 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 106 Resp: 18603
Ion Ratio Lower Upper
106 100
91 212.5 162.8 244.2


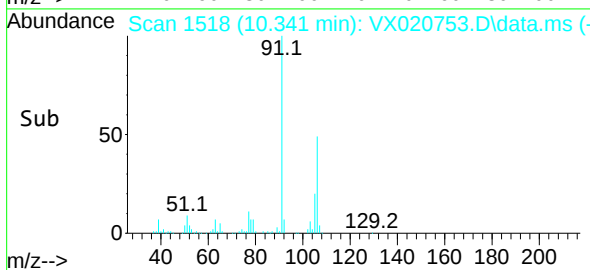

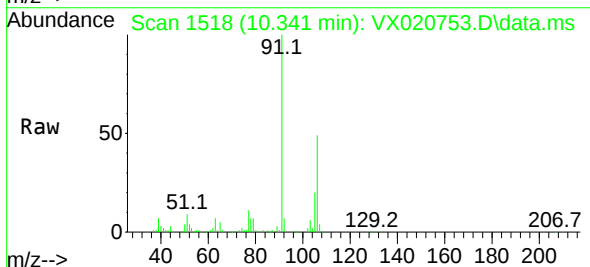




#69
o-Xylene
Concen: 1.34 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. -0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:106 Resp: 9498
Ion Ratio Lower Upper
106 100
91 212.7 108.1 324.2

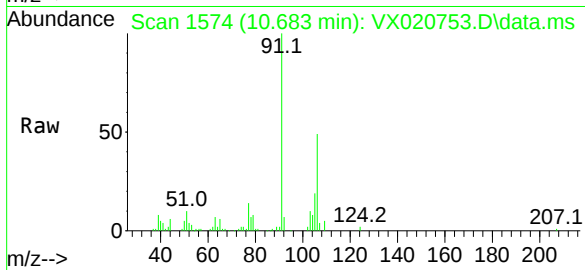

#70
Styrene
Concen: 0.27 ug/l
RT: 10.695 min Scan# 1576
Delta R.T. 0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion:104 Resp: 3338
Ion Ratio Lower Upper
104 100
78 72.2 40.0 60.0#
103 75.0 43.4 65.0#


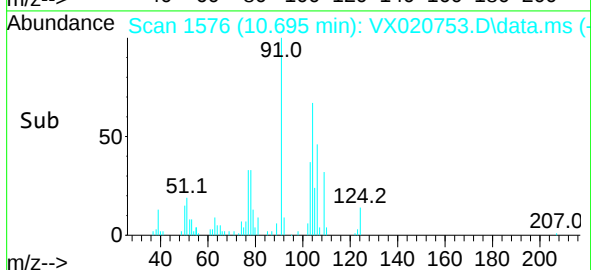

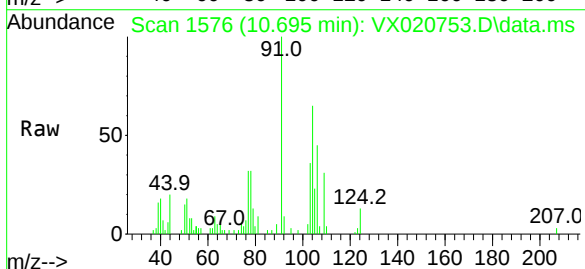


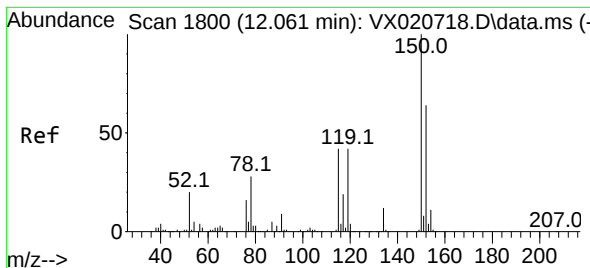

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 248444
Ion Ratio Lower Upper
152 100
115 61.7 41.1 123.3
150 158.3 0.0 349.0

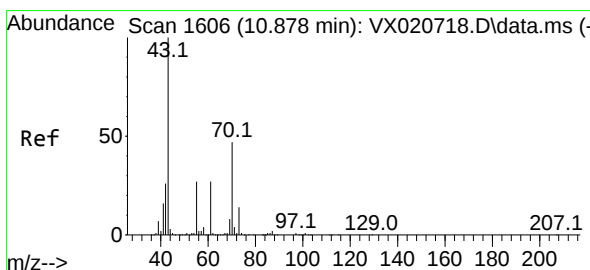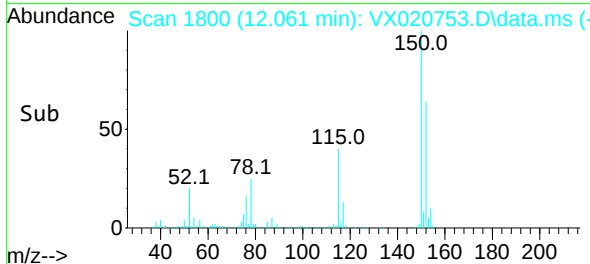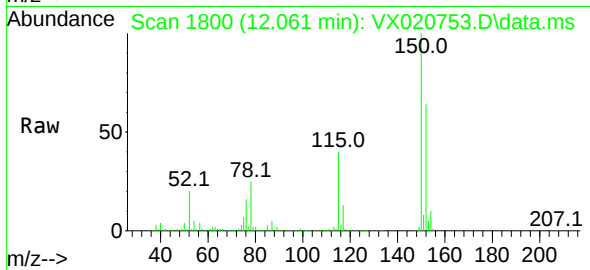

#74
N-ethyl acetate
Concen: 2.06 ug/l
RT: 10.927 min Scan# 1614
Delta R.T. 0.049 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 43 Resp: 376
Ion Ratio Lower Upper
43 100
70 30.3 39.0 58.6#
55 0.0 21.5 32.3#
61 0.0 22.1 33.1#


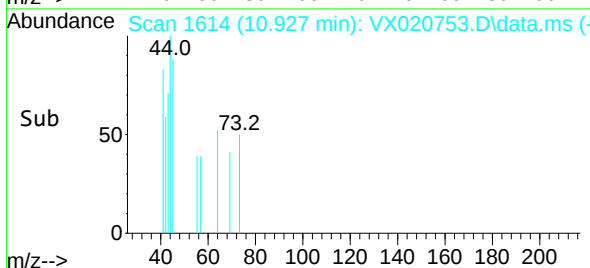

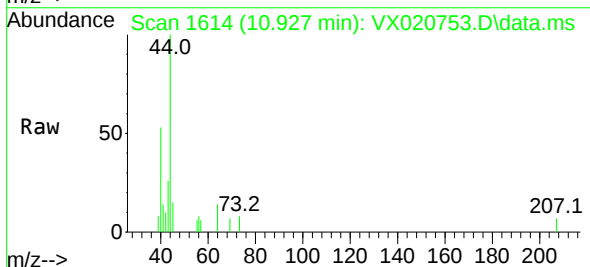


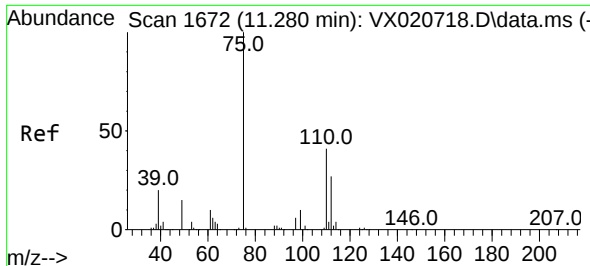

#76
1,2,3-Trichloropropane
Concen: 22.32 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.158 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 128605
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#

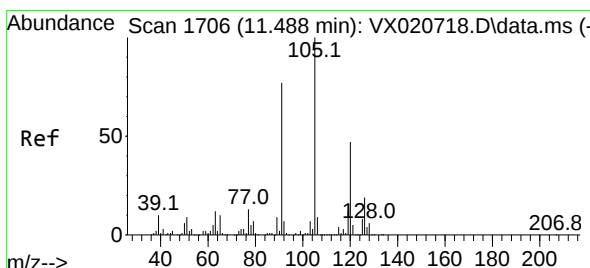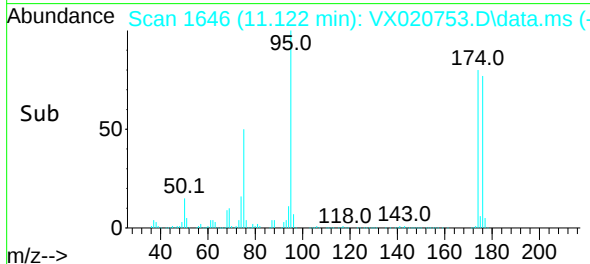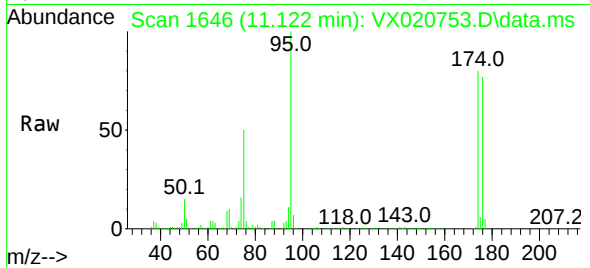

#80
1,3,5-Trimethylbenzene
Concen: 0.28 ug/l
RT: 11.488 min Scan# 1706
Delta R.T. -0.000 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07


Tgt Ion:105 Resp: 4233
Ion Ratio Lower Upper
105 100
120 47.4 23.8 71.5

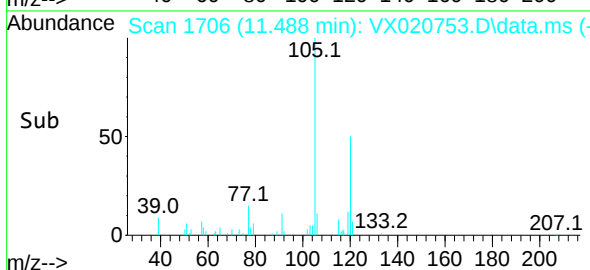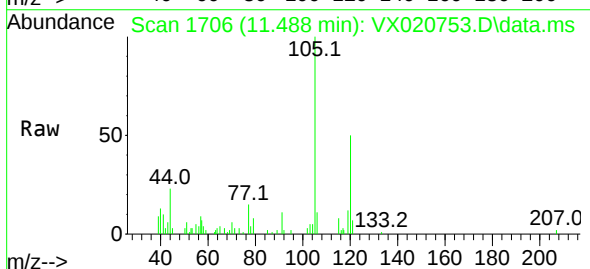






#81
trans-1,4-Dichloro-2-butene
Concen: 62.54 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. 0.067 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Instrument :
MSVOA_X
ClientSampled :



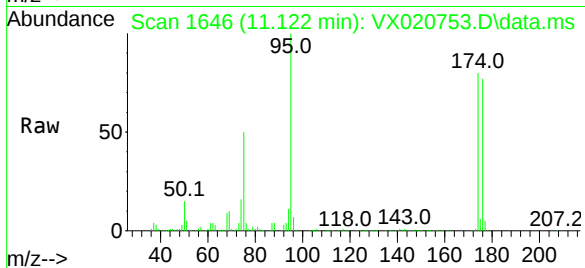



Tgt Ion: 75 Resp: 128605
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#

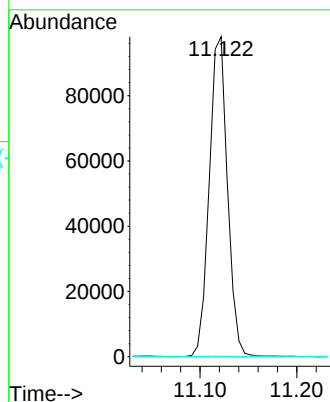

#84
1,2,4-Trimethylbenzene
Concen: 0.82 ug/l
RT: 11.792 min Scan# 1756
Delta R.T. -0.001 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Tgt Ion: 105 Resp: 12676
Ion Ratio Lower Upper
105 100
120 43.5 22.4 67.3

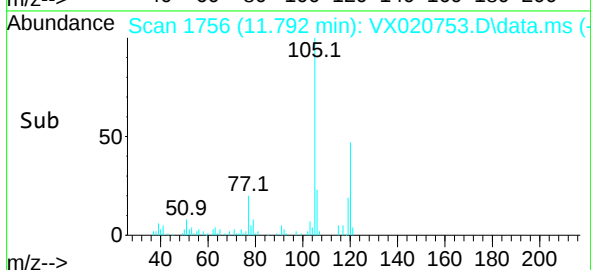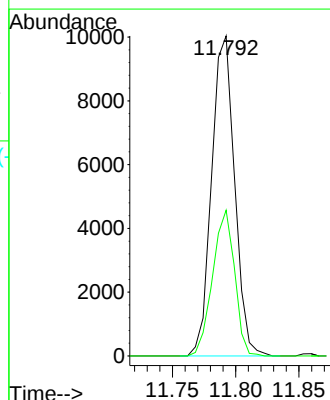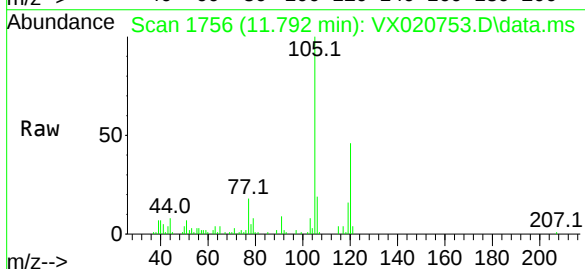

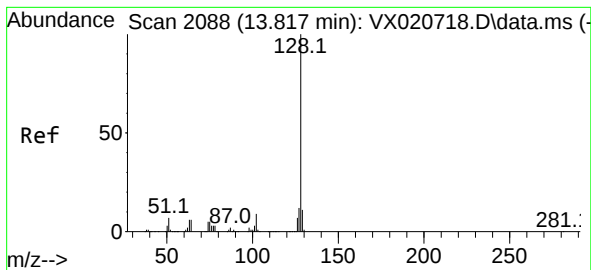

#95
Naphthalene
Concen: 5.23 ug/l
RT: 13.816 min Scan# 2088
Delta R.T. -0.001 min
Lab File: VX020753.D
Acq: 26 Jan 2021 15:07

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:128 Resp: 47640
Ion Ratio Lower Upper
128 100
127 12.7 10.3 15.5
129 12.0 8.8 13.2

