

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
 Data File : VX020746.D
 Acq On : 26 Jan 2021 12:23
 Operator : JC/SP
 Sample : M1192-04DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 41623DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Title : SW846 8260

Signal : TIC: VX020746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.630	82	89	90	rVV6	8549	15881	1.05%	0.155%
2	2.130	164	171	178	rBV	135584	193246	12.72%	1.880%
3	2.989	303	312	329	rBV	14739	40804	2.69%	0.397%
4	5.464	702	718	732	rBV2	177449	515798	33.94%	5.019%
5	5.623	733	744	761	rVB	304277	846521	55.71%	8.237%
6	6.025	799	810	827	rBV	192001	512889	33.75%	4.991%
7	6.824	931	941	958	rBV	458853	1099225	72.34%	10.696%
8	8.696	1239	1248	1254	rBV	970241	1519582	100.00%	14.786%
9	8.763	1254	1259	1270	rVB	65191	104615	6.88%	1.018%
10	10.092	1471	1477	1493	rBV	979077	1328922	87.45%	12.931%
11	10.232	1495	1500	1508	rVB	36430	48376	3.18%	0.471%
12	10.336	1510	1517	1527	rVB	124197	176580	11.62%	1.718%
13	10.683	1568	1574	1584	rBV	75907	101728	6.69%	0.990%
14	11.122	1640	1646	1657	rBV	781089	983806	64.74%	9.573%
15	11.341	1678	1682	1687	rVB	18382	22493	1.48%	0.219%
16	11.415	1687	1694	1702	rVV	63656	118555	7.80%	1.154%
17	11.488	1702	1706	1714	rVB	40735	51600	3.40%	0.502%
18	11.652	1728	1733	1739	rVB	31434	42182	2.78%	0.410%
19	11.786	1751	1755	1763	rVB	118695	152652	10.05%	1.485%
20	12.061	1794	1800	1806	rVV	992823	1188475	78.21%	11.565%
21	12.128	1806	1811	1819	rVB	51730	70011	4.61%	0.681%
22	12.280	1829	1836	1839	rBV2	44936	66230	4.36%	0.644%
23	12.360	1844	1849	1855	rVB4	39619	64175	4.22%	0.624%
24	12.567	1879	1883	1885	rBV	20386	25792	1.70%	0.251%
25	12.591	1885	1887	1892	rVB	22339	24092	1.59%	0.234%
26	12.652	1892	1897	1900	rBV	42896	52469	3.45%	0.511%
27	12.738	1906	1911	1920	rBV3	21608	40409	2.66%	0.393%
28	12.884	1931	1935	1941	rVB2	14247	18775	1.24%	0.183%
29	12.957	1941	1947	1951	rBV	30775	40803	2.69%	0.397%
30	13.000	1951	1954	1960	rVB	45571	54238	3.57%	0.528%
31	13.207	1980	1988	1992	rBV2	32286	47467	3.12%	0.462%
32	13.329	2004	2008	2013	rVB2	75982	105254	6.93%	1.024%
33	13.463	2025	2030	2039	rVB	35806	47964	3.16%	0.467%
34	13.579	2046	2049	2052	rVV	15038	21077	1.39%	0.205%
35	13.622	2052	2056	2062	rVV3	30604	60268	3.97%	0.586%
36	13.707	2062	2070	2076	rVB2	20127	47182	3.10%	0.459%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
 Data File : VX020746.D
 Acq On : 26 Jan 2021 12:23
 Operator : JC/SP
 Sample : M1192-04DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 41623DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M

Title : SW846 8260

37	13.817	2082	2088	2095	rVB	27400	41517	2.73%	0.404%
38	13.896	2095	2101	2105	rVB2	18087	27904	1.84%	0.272%
39	13.963	2105	2112	2116	rBV2	24108	37322	2.46%	0.363%
40	14.006	2116	2119	2123	rVB2	12704	16360	1.08%	0.159%
41	14.115	2132	2137	2141	rVB	22593	26474	1.74%	0.258%
42	14.268	2154	2162	2168	rBV2	45064	83500	5.49%	0.813%
43	14.414	2182	2186	2190	rVB2	19617	25593	1.68%	0.249%
44	14.518	2199	2203	2209	rBV2	32462	46061	3.03%	0.448%
45	14.658	2221	2226	2227	rBV3	19233	24841	1.63%	0.242%
46	14.676	2227	2229	2232	rVV	22685	27426	1.80%	0.267%
47	14.713	2232	2235	2239	rVB	14256	18817	1.24%	0.183%
48	14.944	2268	2273	2278	rBV3	8611	16384	1.08%	0.159%
49	15.225	2315	2319	2327	rBV2	18453	34564	2.27%	0.336%


Sum of corrected areas: 10276899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
Data File : VX020746.D
Acq On : 26 Jan 2021 12:23
Operator : JC/SP
Sample : M1192-04DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41623DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

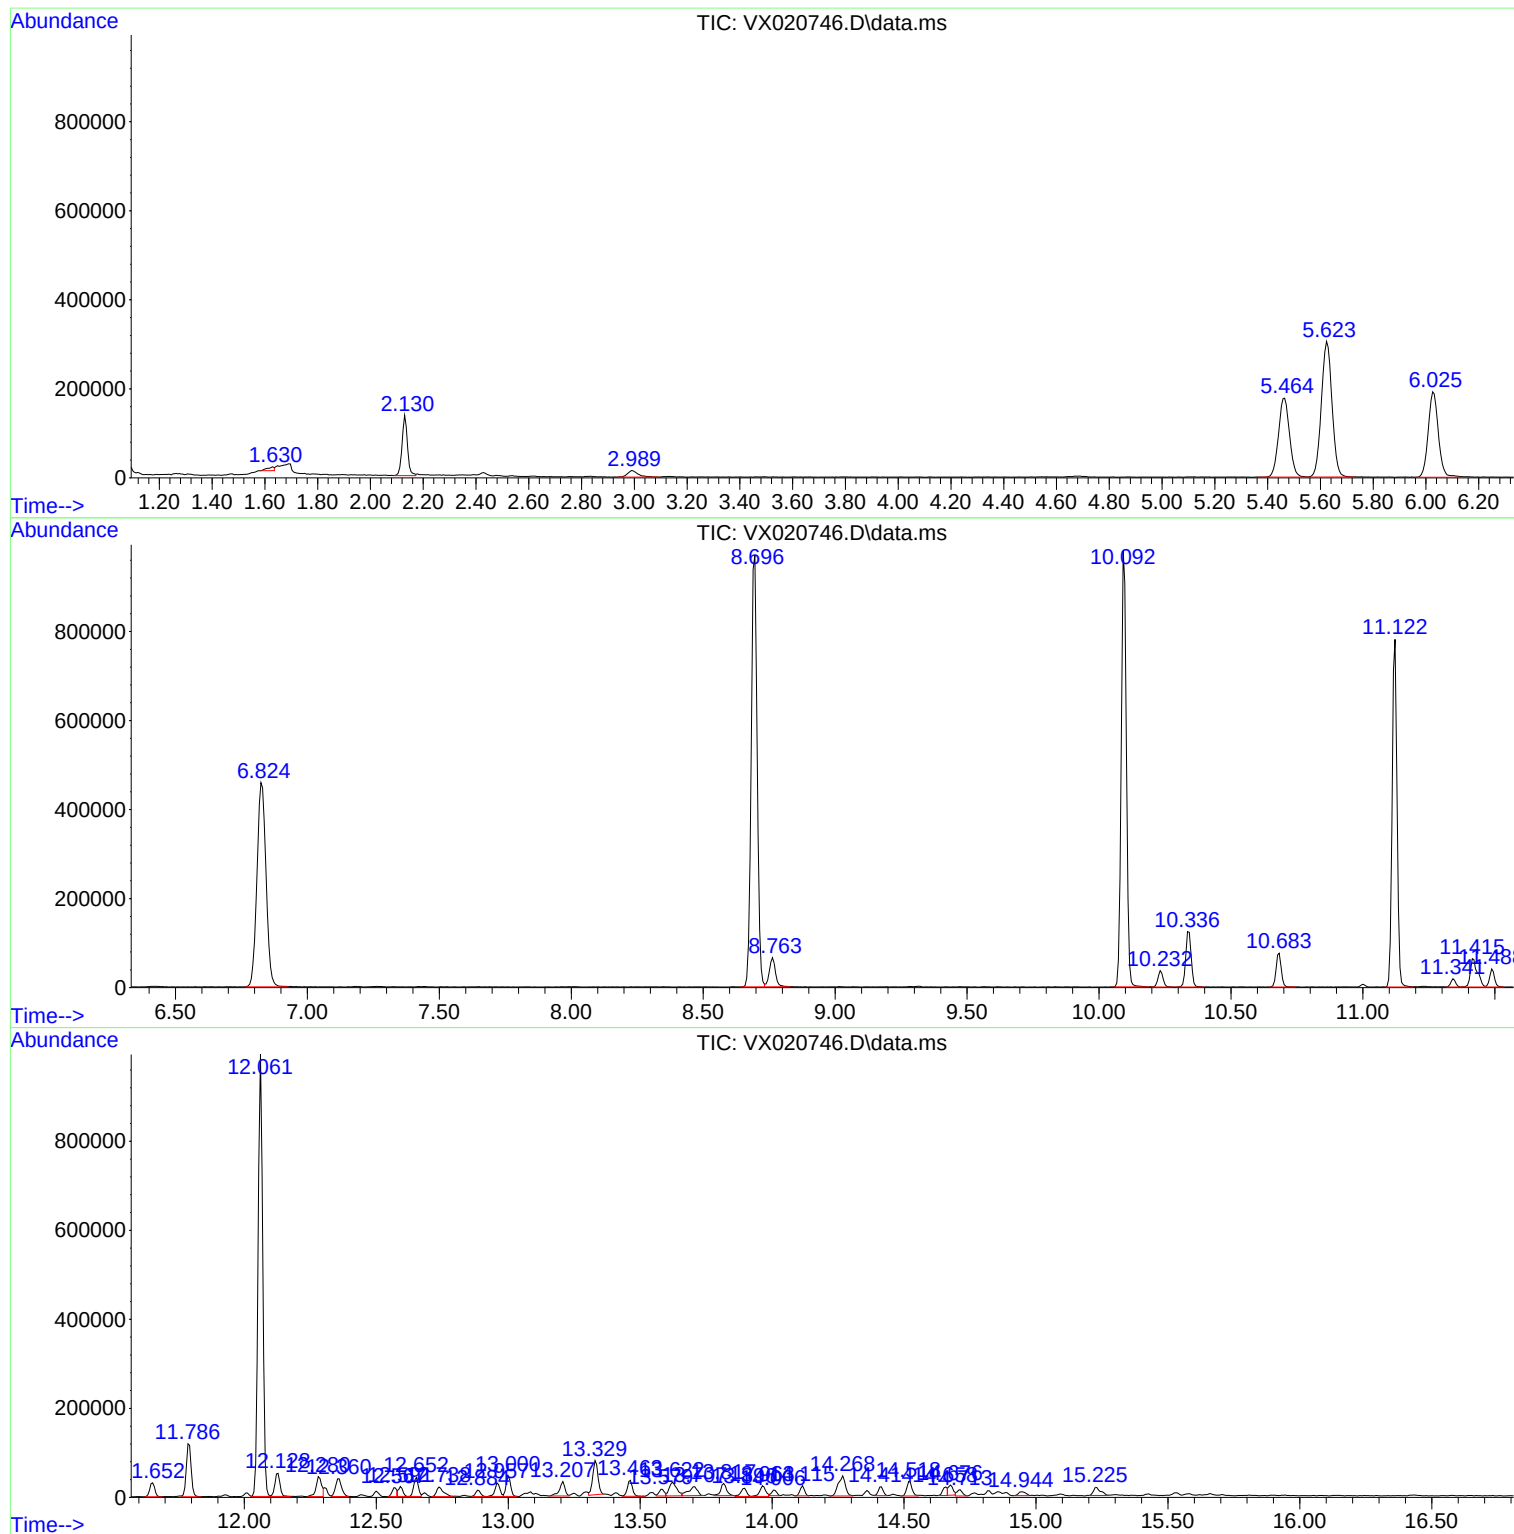

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
Data File : VX020746.D
Acq On : 26 Jan 2021 12:23
Operator : JC/SP
Sample : M1192-04DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41623DL










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.130	11.41 ug/l	193246	Pentafluorobenzene	5.623

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol	46	C2H6O	000064-17-5	64
2			Dimethyl ether	46	C2H6O	000115-10-6	9
3			Methane, nitroso-	45	CH3NO	000865-40-7	4
4			Formic acid	46	CH2O2	000064-18-6	4
5			Oxalic acid	90	C2H2O4	000144-62-7	4

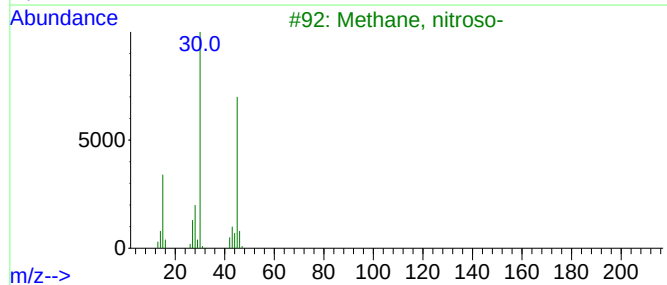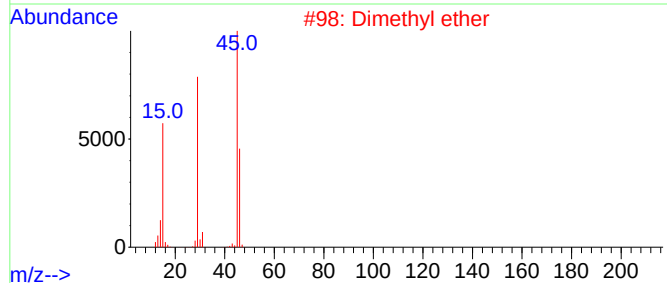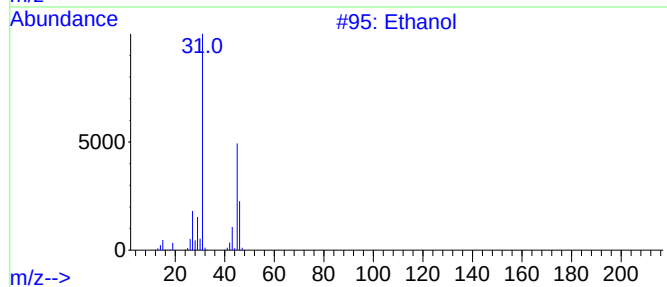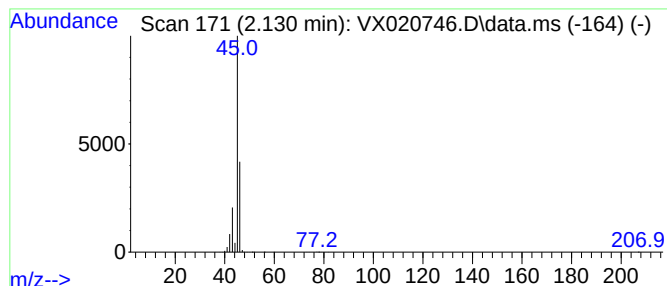

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012621\
Data File : VX020746.D
Acq On : 26 Jan 2021 12:23
Operator : JC/SP
Sample : M1192-04DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
41623DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol	2.130	11.4	ug/l	193246	1	5.623	846521	50.0