
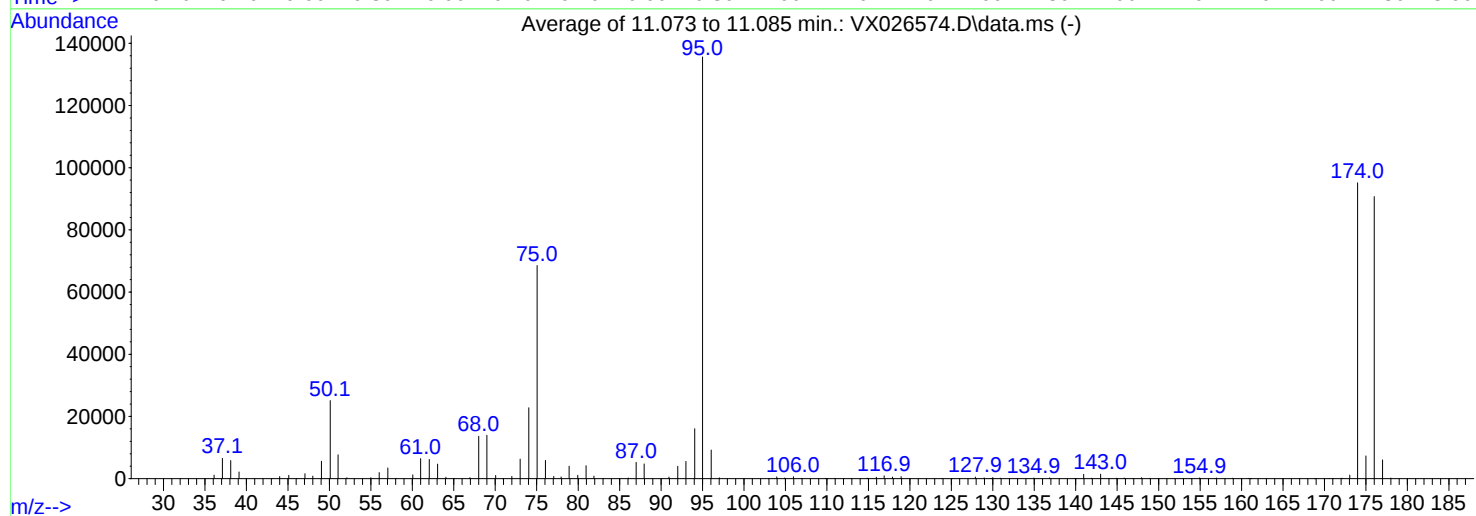


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012622\
 Data File : VX026574.D
 Acq On : 25 Jan 2022 17:12
 Operator : JC/MD
 Sample : BFB614
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB614

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXTR012622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Jan 26 03:14:49 2022

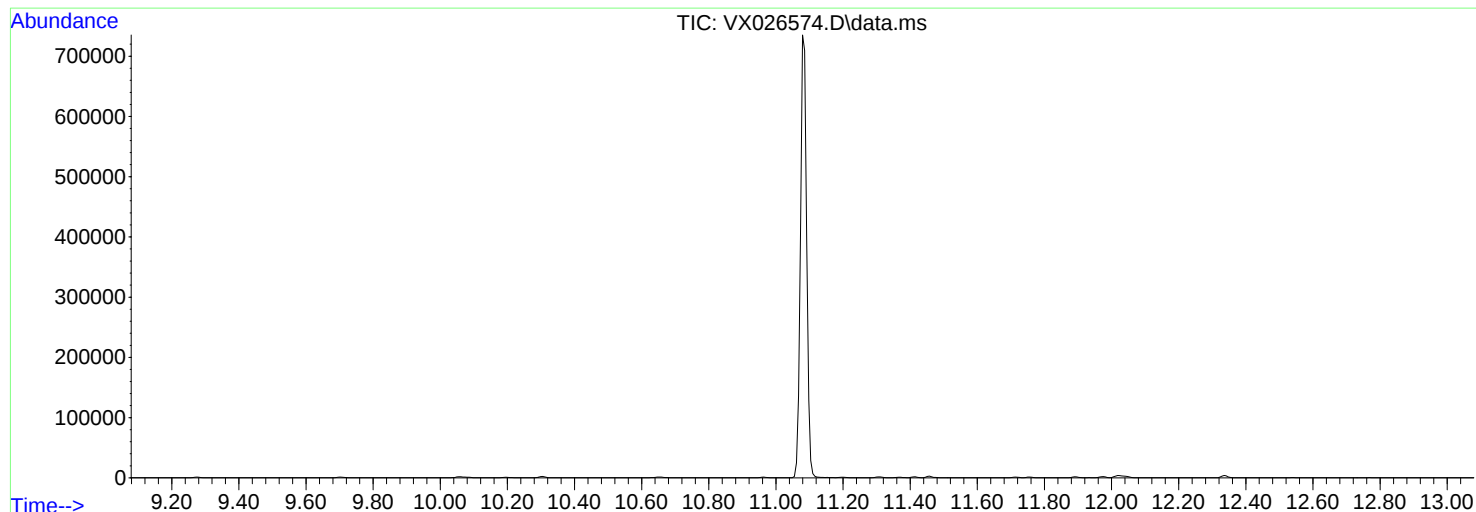

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	25123	PASS
75	95	30	80	50.5	68560	PASS
95	95	100	100	100.0	135664	PASS
96	95	5	9	6.8	9202	PASS
173	174	0.00	2	1.2	1120	PASS
174	95	50	120	70.1	95131	PASS
175	174	5	9	7.7	7333	PASS
176	174	95	105	95.3	90704	PASS
177	176	5	10	6.6	6011	PASS

m/z	Abundance
40.00	177.0
44.00	101.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

m/z	Abundance
36.10	929.0
37.10	5298.0
38.10	4649.0
39.10	1790.0
40.10	279.0
43.20	53.0
44.00	521.0
45.10	894.0
46.10	85.0
47.00	1276.0
48.00	616.0
49.10	4314.0
50.10	19656.0
51.00	5869.0
52.10	297.0
55.00	226.0
56.00	1405.0
57.10	2700.0
58.00	101.0
60.10	990.0
61.00	5032.0
62.00	4913.0
63.10	3742.0
64.10	445.0
65.00	64.0
66.90	218.0
68.00	9925.0
69.00	10400.0
70.00	694.0
72.00	561.0
73.00	4528.0
74.10	16544.0
75.00	50704.0
76.00	4420.0
77.10	558.0
78.00	443.0
78.90	2874.0
79.90	705.0
80.90	3002.0
81.90	634.0
83.10	68.0
86.00	124.0
87.00	3582.0
87.90	3051.0
90.90	377.0
92.00	2926.0
93.00	4115.0
94.00	11352.0
95.00	95376.0
96.00	6963.0
97.10	227.0
103.90	405.0
104.80	120.0
106.00	366.0
107.00	87.0
109.80	72.0
111.00	75.0
112.00	55.0
112.90	87.0
114.80	92.0
116.00	325.0
116.90	599.0
117.90	286.0
119.00	448.0
123.80	56.0
127.90	362.0
128.90	163.0
129.80	292.0
130.90	127.0
134.90	151.0
136.90	184.0
140.10	63.0
140.90	987.0
141.90	105.0
143.00	944.0
144.10	65.0
145.00	107.0
145.80	147.0
147.90	205.0
150.00	65.0
152.90	70.0
155.00	167.0
156.80	131.0
158.90	78.0
161.10	65.0
171.00	66.0
172.00	171.0
173.00	629.0
174.00	54488.0
175.00	4433.0
176.00	52584.0
177.00	3706.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

178.00

119.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

m/z	Abundance
36.10	1292.0
37.10	7730.0
38.10	7058.0
39.10	2601.0
40.00	327.0
44.10	958.0
45.10	1306.0
46.00	109.0
47.10	2017.0
48.00	1121.0
49.00	6724.0
50.10	30584.0
51.10	8760.0
52.10	372.0
55.00	462.0
56.00	2459.0
57.10	4229.0
58.10	187.0
60.00	1425.0
61.00	7520.0
62.10	7454.0
63.00	5383.0
64.10	511.0
65.10	85.0
67.00	434.0
68.00	16480.0
69.00	16616.0
70.00	1305.0
72.00	900.0
73.00	7506.0
74.00	27592.0
75.00	81680.0
76.00	7014.0
77.00	893.0
77.90	640.0
78.90	4908.0
80.00	1300.0
81.00	5040.0
81.90	1020.0
83.00	120.0
86.10	287.0
87.00	6232.0
88.00	5648.0
90.90	708.0
92.00	4856.0
93.00	6461.0
94.10	19208.0
95.00	160896.0
96.10	10889.0
97.10	299.0
102.90	76.0
103.90	667.0
104.90	215.0
105.90	684.0
106.90	145.0
110.00	93.0
111.00	111.0
112.00	79.0
112.90	139.0
114.90	152.0
115.90	522.0
116.90	1098.0
117.90	593.0
118.90	815.0
123.80	73.0
127.90	601.0
128.90	263.0
130.00	587.0
130.90	183.0
134.90	254.0
136.90	294.0
140.00	117.0
140.90	1715.0
141.90	187.0
143.00	1685.0
144.00	114.0
145.00	199.0
145.80	211.0
146.90	73.0
148.00	374.0
149.00	144.0
150.00	125.0
151.90	79.0
153.00	145.0
153.90	72.0
155.00	289.0
157.00	247.0
158.90	188.0
160.80	119.0
168.80	51.0
170.00	85.0
170.60	63.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

172.20	309.0
173.10	1403.0
174.00	109192.0
175.00	8591.0
176.00	104600.0
177.00	7311.0
178.00	245.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

m/z	Abundance
36.10	1239.0
37.10	6591.0
38.10	5790.0
39.10	2059.0
40.00	204.0
43.00	52.0
44.10	794.0
45.10	1128.0
46.10	94.0
47.00	1546.0
48.00	779.0
49.10	5771.0
50.10	25128.0
51.10	8339.0
52.10	316.0
55.00	329.0
56.00	2072.0
57.00	3395.0
58.00	96.0
60.00	1304.0
61.00	6695.0
62.00	6098.0
63.10	4918.0
64.00	475.0
67.00	271.0
68.00	14535.0
69.00	14792.0
70.10	1146.0
70.90	51.0
72.00	787.0
73.00	6734.0
74.00	24320.0
75.10	73296.0
76.10	6183.0
77.10	777.0
78.00	671.0
78.90	4208.0
80.00	1219.0
81.00	4510.0
81.90	854.0
83.00	72.0
86.00	150.0
87.00	5936.0
88.00	5495.0
91.00	513.0
92.00	4181.0
93.00	6042.0
94.00	17688.0
95.00	150720.0
96.00	9753.0
97.00	254.0
103.00	61.0
104.00	585.0
105.00	217.0
105.90	759.0
106.80	152.0
109.80	101.0
110.90	130.0
112.10	77.0
113.00	148.0
114.90	198.0
115.90	566.0
116.90	1018.0
117.90	652.0
118.90	826.0
123.90	76.0
125.00	60.0
127.90	594.0
129.00	327.0
130.00	548.0
130.90	171.0
135.00	301.0
136.80	297.0
139.80	127.0
141.00	1557.0
141.90	210.0
143.00	1710.0
143.90	77.0
144.90	187.0
145.90	260.0
146.90	80.0
147.90	301.0
148.90	120.0
149.90	208.0
151.90	78.0
152.90	129.0
154.00	120.0
154.90	354.0
157.00	334.0
159.00	233.0
160.90	159.0
170.00	73.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614

170.50	127.0
171.10	163.0
172.00	364.0
173.10	1327.0
174.00	121712.0
175.00	8974.0
176.00	114928.0
177.00	7016.0
178.00	229.0

Instrument :
MSVOA_X
ClientSampleId :
BFB614