

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
 Data File : VX033920.D
 Acq On : 26 Jan 2023 19:24
 Operator : JC/MD
 Sample : 01321-02 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 33903

Quant Time: Jan 27 03:00:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 11 14:48:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	157833	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	226690	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	202711	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	98618	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	75193	45.247	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	90.500%
35) Dibromofluoromethane	5.385	113	68928	48.968	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.940%
50) Toluene-d8	8.647	98	258753	50.452	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.900%
62) 4-Bromofluorobenzene	11.079	95	90365	47.456	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.920%
Target Compounds						Qvalue
11) Tert butyl alcohol	2.947	59	1052	3.644	ug/l #	86
16) Acetone	2.374	43	4912	Below Cal	#	87
17) Carbon Disulfide	2.520	76	90	1.849	ug/l #	76
18) Methyl Acetate	2.703	43	1462	0.630	ug/l #	85
19) Methyl tert-butyl Ether	3.111	73	10374	2.326	ug/l	100
20) Methylene Chloride	2.788	84	610	Below Cal	#	85
22) Diisopropyl ether	3.751	45	1304	0.268	ug/l #	70
25) 2-Butanone	4.580	43	1155	1.064	ug/l	99
27) cis-1,2-Dichloroethene	4.501	96	762	0.441	ug/l	91
31) Cyclohexane	5.550	56	2198	0.899	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	9432	4.591	ug/l #	49
37) Ethyl Acetate	4.721	43	1897	Below Cal	#	84
38) Carbon Tetrachloride	5.550	117	13511	6.350	ug/l #	16
40) Benzene	6.037	78	11282	1.884	ug/l	97
52) Toluene	8.720	92	10251	2.651	ug/l	98
67) Ethyl Benzene	10.195	91	3868	0.537	ug/l #	88
68) m/p-Xylenes	10.305	106	5839	2.072	ug/l	97
69) o-Xylene	10.646	106	4263	1.525	ug/l	93
73) Isopropylbenzene	10.963	105	2032	Below Cal		92
75) 1,1,2,2-Tetrachloroethane	11.085	83	20	Below Cal	#	1
76) 1,2,3-Trichloropropane	11.079	75	41692	23.009	ug/l #	34
78) n-propylbenzene	11.305	91	2025	0.252	ug/l	96
79) 2-Chlorotoluene	11.378	91	1341	Below Cal	#	39
80) 1,3,5-Trimethylbenzene	11.451	105	4121	0.694	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	41692	71.510	ug/l #	8
82) 4-Chlorotoluene	11.451	91	513	Below Cal	#	43
83) tert-Butylbenzene	11.750	119	2011	0.341	ug/l #	61
84) 1,2,4-Trimethylbenzene	11.750	105	15189	2.706	ug/l	98
89) n-Butylbenzene	12.329	91	1309	0.265	ug/l #	21
90) Hexachloroethane	12.530	117	283	0.285	ug/l #	4
95) Naphthalene	13.780	128	10690	1.716	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
Data File : VX033920.D
Acq On : 26 Jan 2023 19:24
Operator : JC/MD
Sample : 01321-02 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33903

Quant Time: Jan 27 03:00:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 11 14:48:42 2023
Response via : Initial Calibration

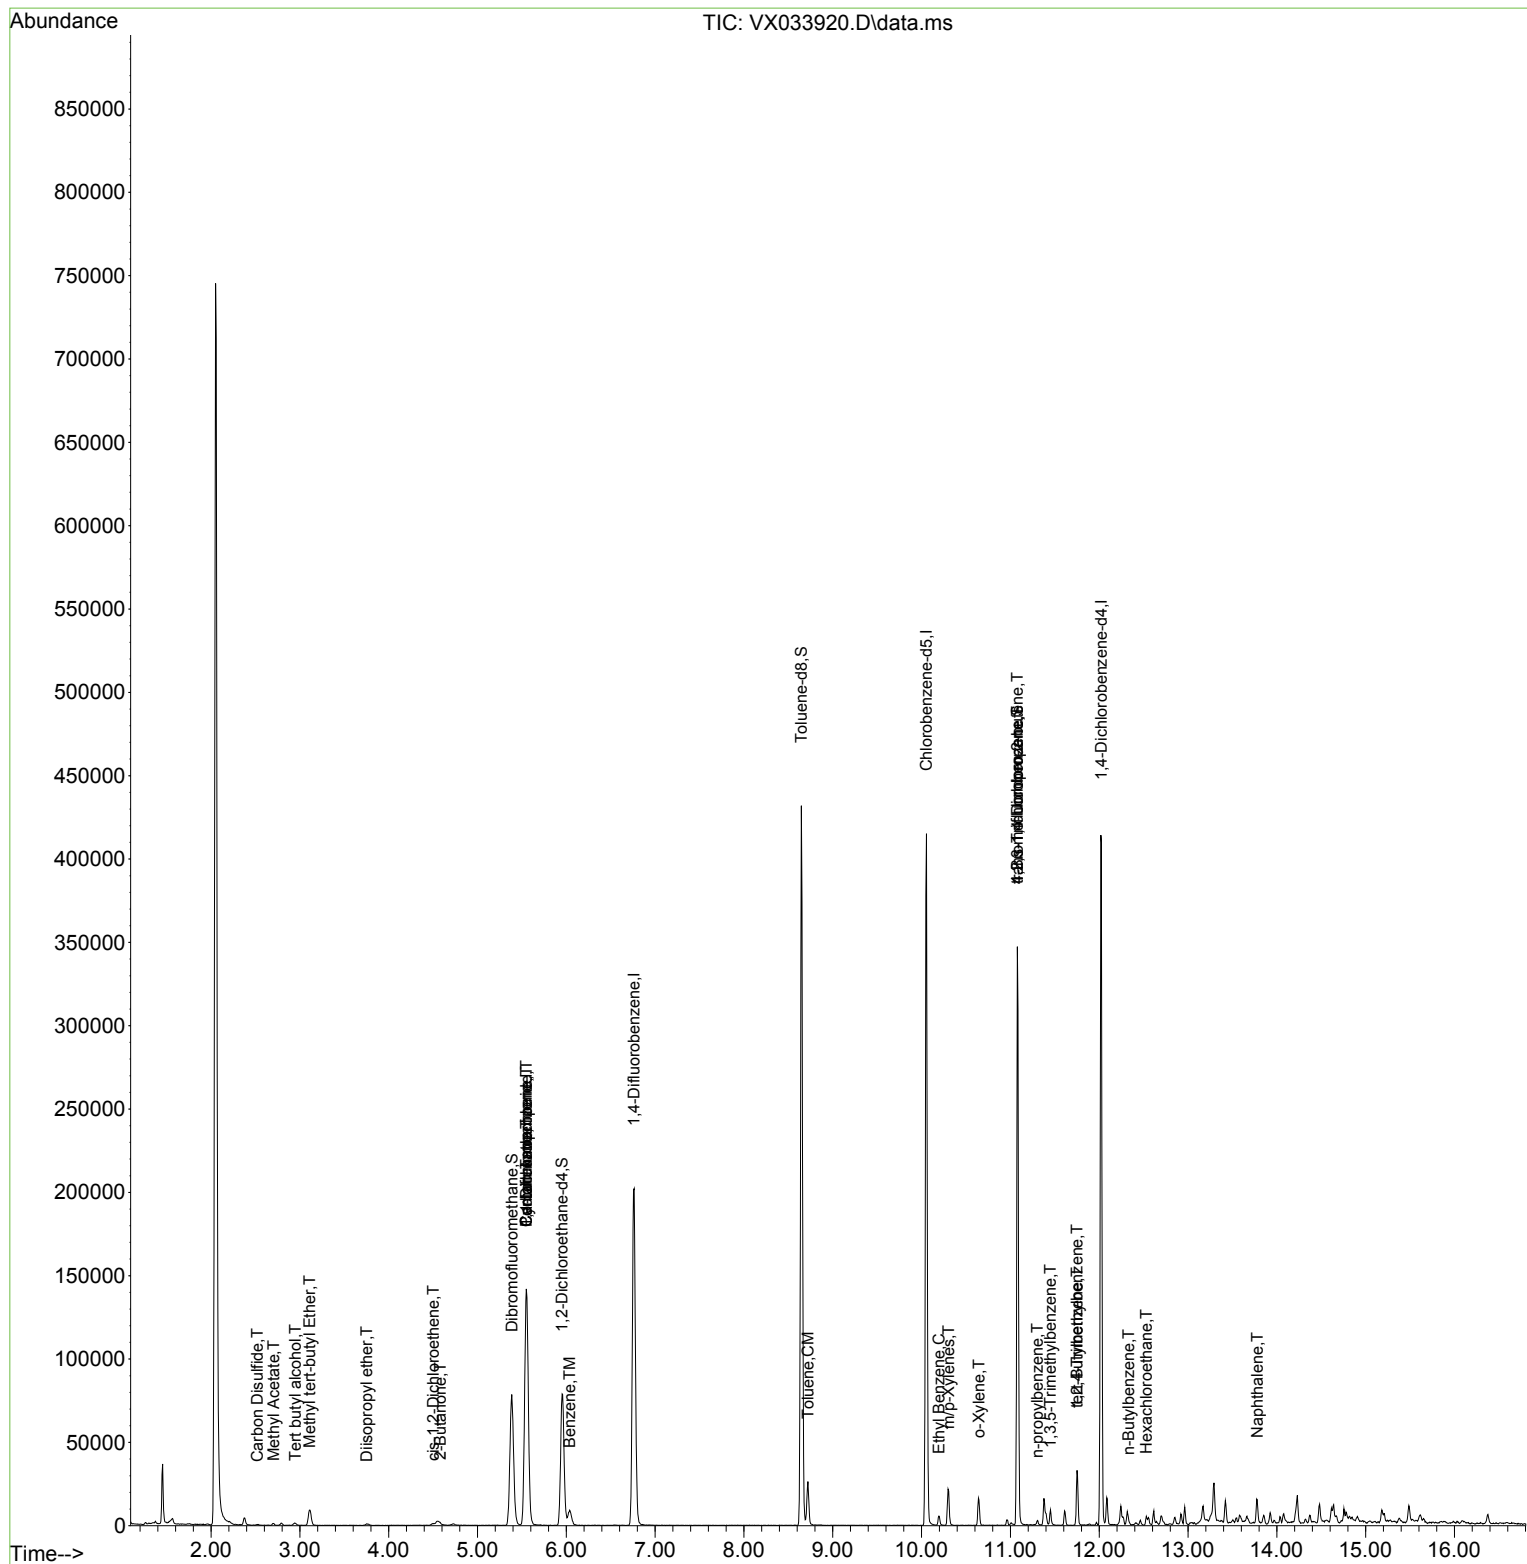

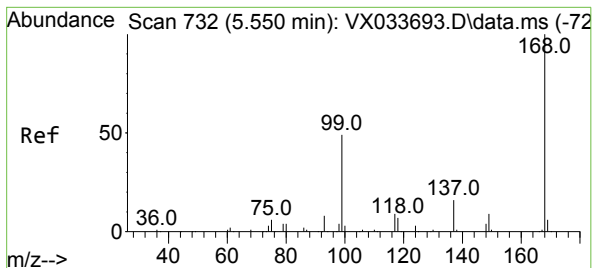

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :





33903

Tgt Ion:168 Resp: 157833

Ion Ratio Lower Upper

168 100

99 48.3 39.6 59.4

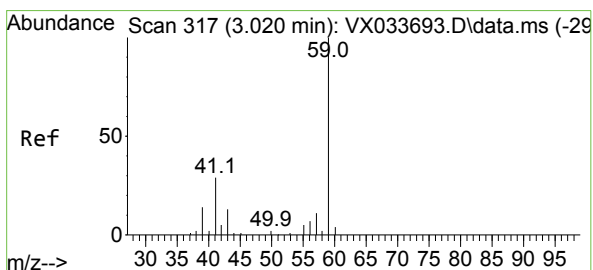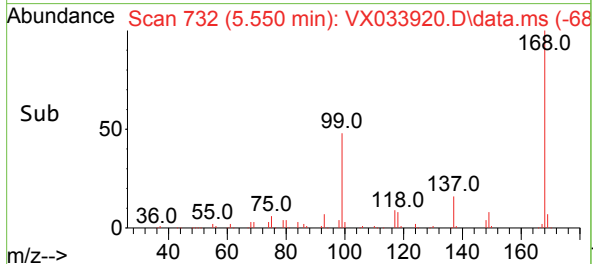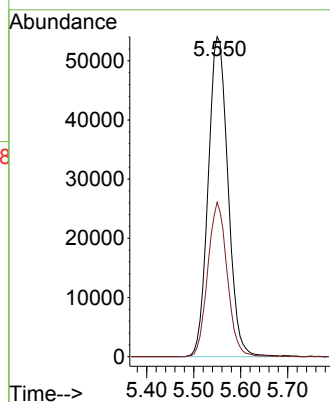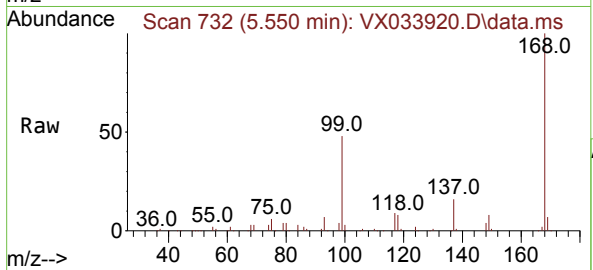

#11

Tert butyl alcohol

Concen: 3.644 ug/l

RT: 2.947 min Scan# 305

Delta R.T. -0.073 min

Lab File: VX033920.D




Acq: 26 Jan 2023 19:24

Tgt Ion: 59 Resp: 1052

Ion Ratio Lower Upper

59 100

57 0.0 3.7 5.5#

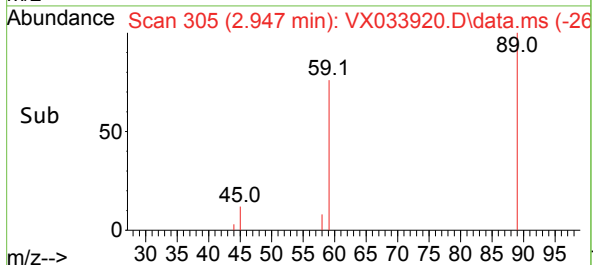

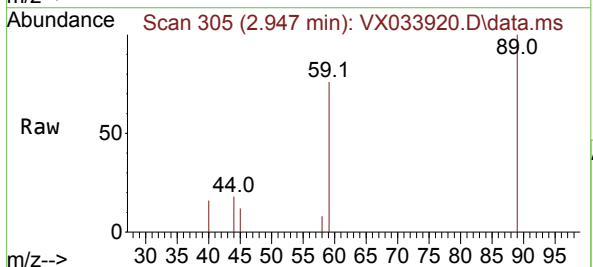




#16
Acetone
Concen: Below Cal
RT: 2.374 min Scan# 215
Delta R.T. -0.024 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion: 43 Resp: 4912
Ion Ratio Lower Upper
43 100
58 35.1 22.6 33.8#

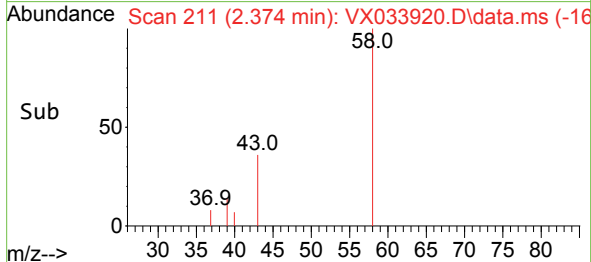

#17
Carbon Disulfide
Concen: 1.849 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.006 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 76 Resp: 90
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#

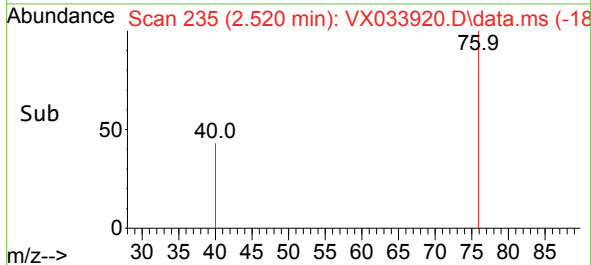



#18

Methyl Acetate

Concen: 0.630 ug/l

RT: 2.703 min Scan# 2

Delta R.T. -0.006 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :





33903

Tgt Ion: 43 Resp: 1462

Ion Ratio Lower Upper

43 100

74 15.5 18.2 27.4#

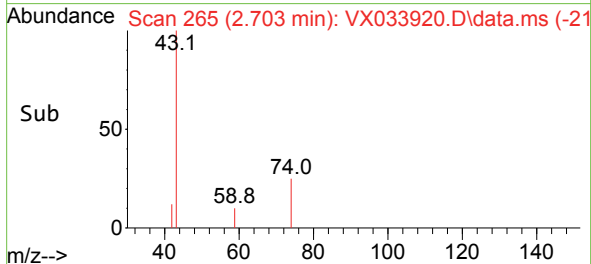

#19

Methyl tert-butyl Ether

Concen: 2.326 ug/l

RT: 3.111 min Scan# 332

Delta R.T. -0.000 min

Lab File: VX033920.D




Acq: 26 Jan 2023 19:24


Tgt Ion: 73 Resp: 10374

Ion Ratio Lower Upper

73 100

57 21.8 17.4 26.0



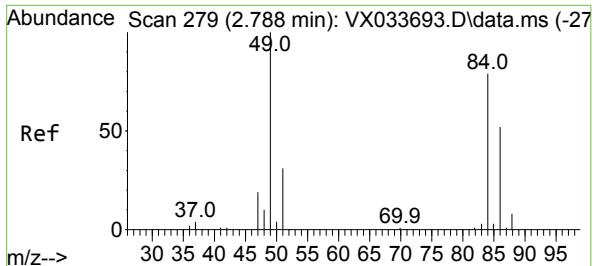

#20

Methylene Chloride

Concen: Below Cal

RT: 2.788 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :

33903

Tgt Ion: 84 Resp: 610





Ion Ratio Lower Upper

84 100

49 147.0 101.1 151.7

51 49.7 31.0 46.6#

86 71.3 52.6 79.0

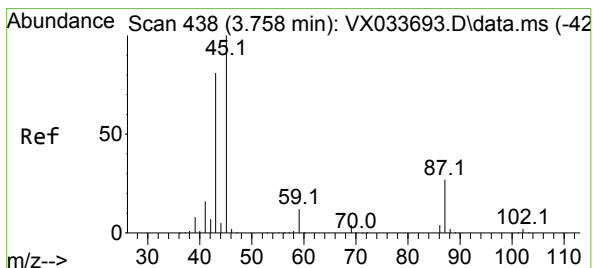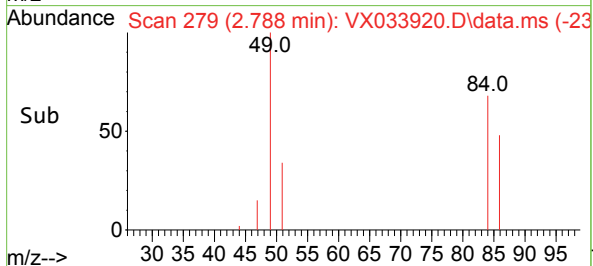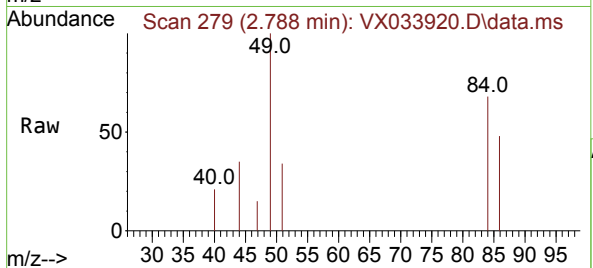

#22

Diisopropyl ether

Concen: 0.268 ug/l

RT: 3.751 min Scan# 437

Delta R.T. -0.006 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Tgt Ion: 45 Resp: 1304




Ion Ratio Lower Upper


45 100

43 46.3 64.6 97.0#

87 30.1 21.9 32.9

59 0.0 9.2 13.8#


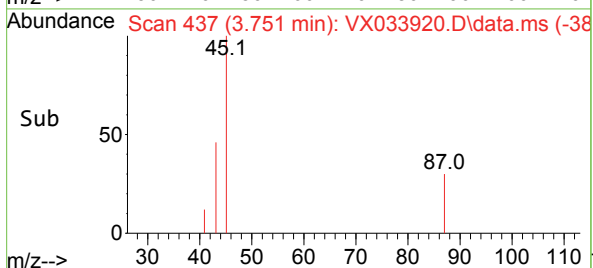
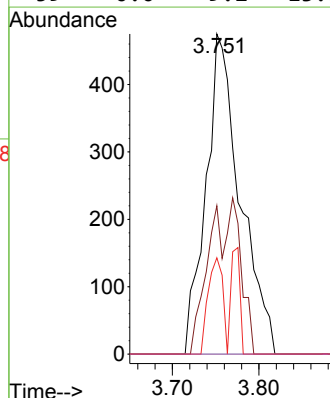
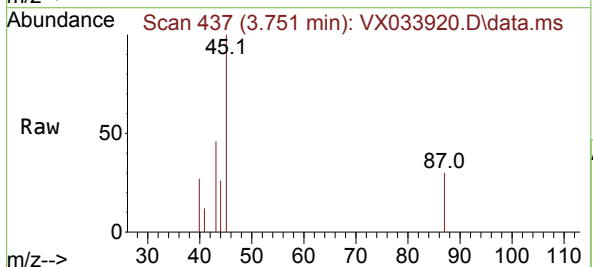




#25
2-Butanone
Concen: 1.064 ug/l
RT: 4.580 min Scan# 51
Delta R.T. 0.012 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion: 43 Resp: 1155
Ion Ratio Lower Upper
43 100
72 24.9 19.4 29.2

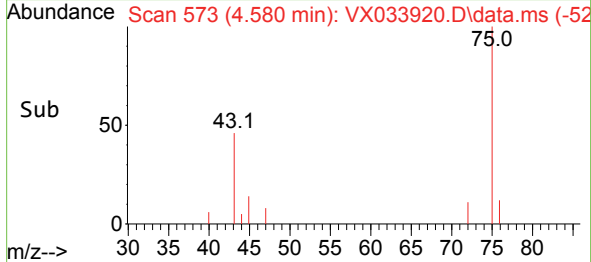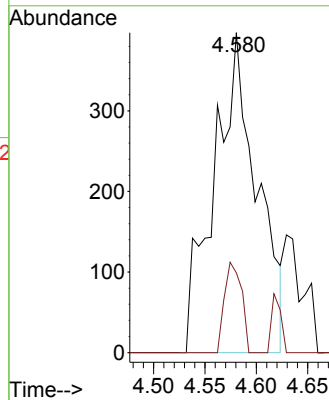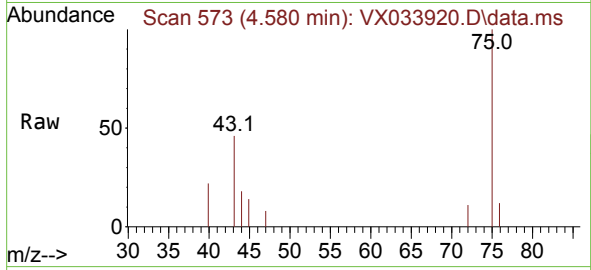

#27
cis-1,2-Dichloroethene
Concen: 0.441 ug/l
RT: 4.501 min Scan# 560
Delta R.T. 0.012 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 96 Resp: 762
Ion Ratio Lower Upper
96 100
61 126.8 0.0 277.6
98 57.7 0.0 128.0



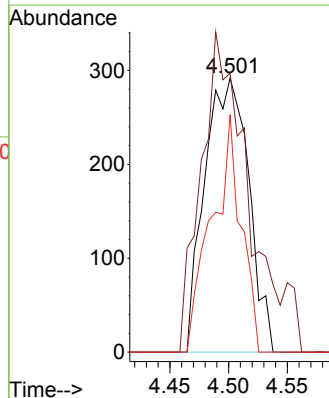



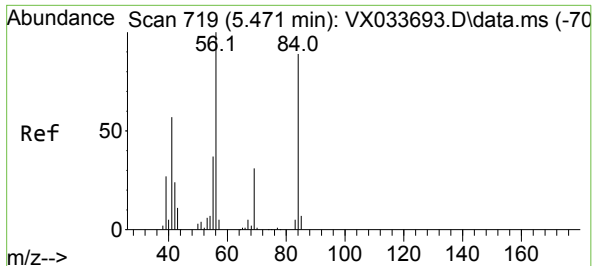

#31
Cyclohexane
Concen: 0.899 ug/l
RT: 5.550 min Scan# 719
Delta R.T. 0.079 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion: 56 Resp: 2198
Ion Ratio Lower Upper
56 100
69 209.5 24.6 37.0#
84 211.0 71.0 106.6#

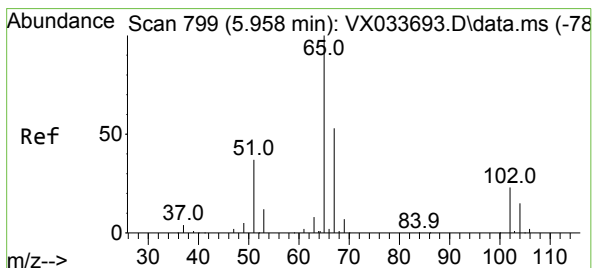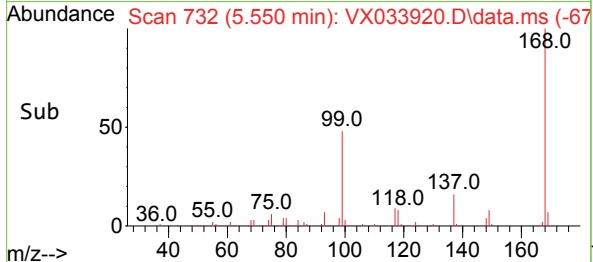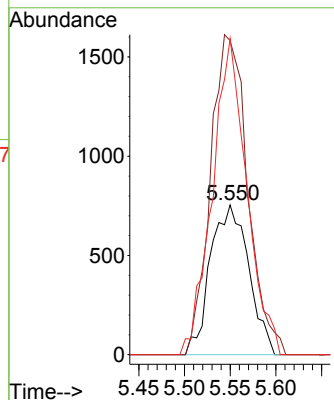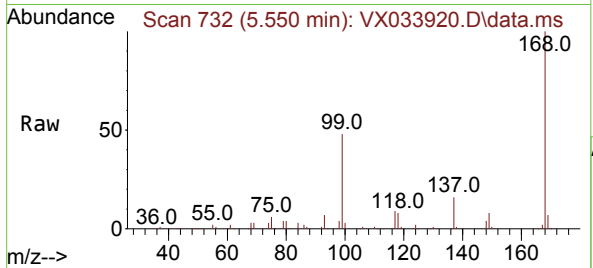

#33
1,2-Dichloroethane-d4
Concen: 45.247 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 65 Resp: 75193
Ion Ratio Lower Upper
65 100
67 54.0 0.0 104.8


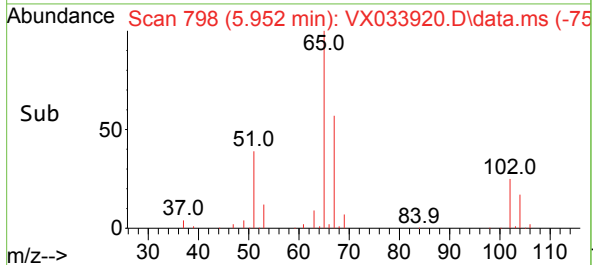
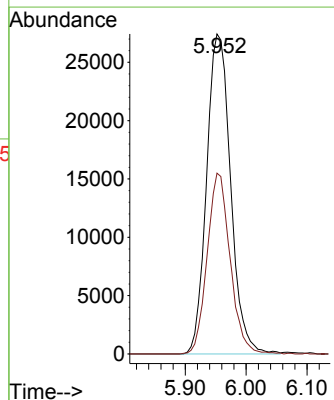
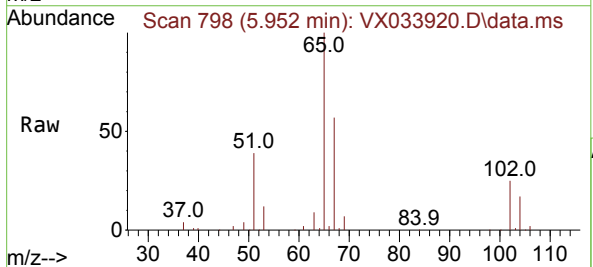




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion:114 Resp: 226690
Ion Ratio Lower Upper
114 100
63 18.5 0.0 37.4
88 16.1 0.0 30.6

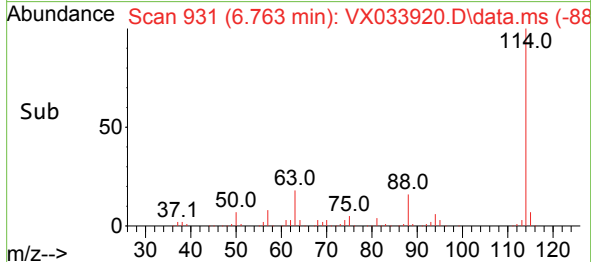

#35
Dibromofluoromethane
Concen: 48.968 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion:113 Resp: 68928
Ion Ratio Lower Upper
113 100
111 101.5 83.0 124.6
192 24.6 19.0 28.4




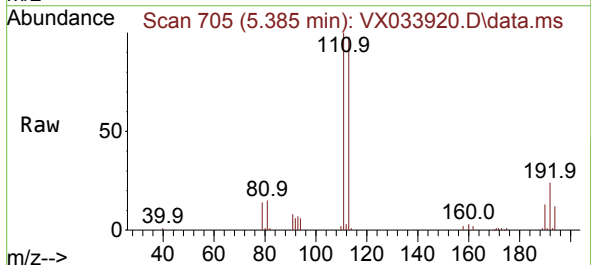




#36
1,1-Dichloropropene
Concen: 4.591 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion: 75 Resp: 9432
Ion Ratio Lower Upper
75 100
110 9.4 18.8 56.4#
77 0.0 25.1 37.7#

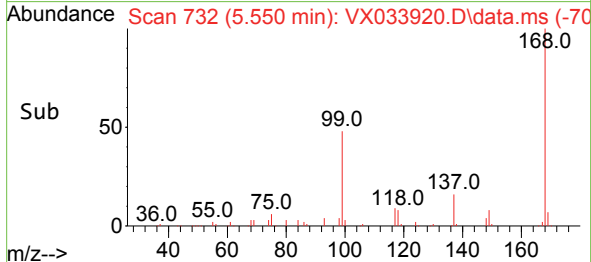

#37
Ethyl Acetate
Concen: Below Cal
RT: 4.721 min Scan# 596
Delta R.T. 0.006 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 43 Resp: 1897
Ion Ratio Lower Upper
43 100
61 7.3 11.1 16.7#
70 5.0 8.5 12.7#




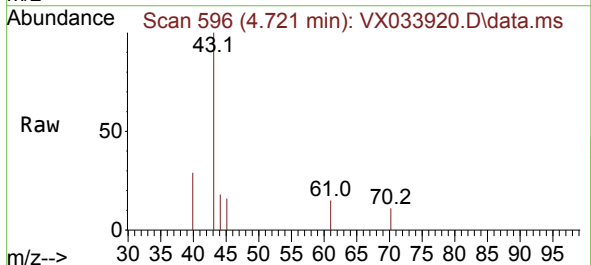




#38
Carbon Tetrachloride
Concen: 6.350 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion:117 Resp: 13511
Ion Ratio Lower Upper
117 100
119 6.0 78.0 117.0#
121 0.0 24.4 36.6#

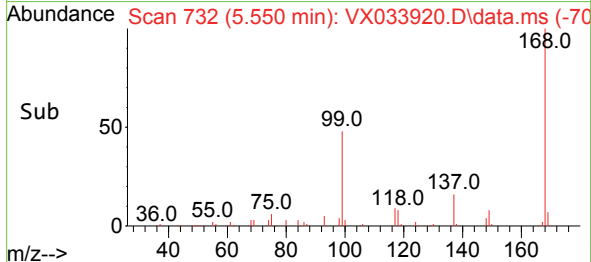

#40
Benzene
Concen: 1.884 ug/l
RT: 6.037 min Scan# 812
Delta R.T. -0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 78 Resp: 11282
Ion Ratio Lower Upper
78 100
77 25.4 19.0 28.4




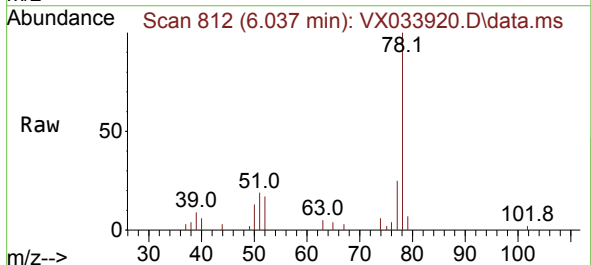




#50
Toluene-d8
Concen: 50.452 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion: 98 Resp: 258753
Ion Ratio Lower Upper
98 100
100 66.8 53.6 80.4

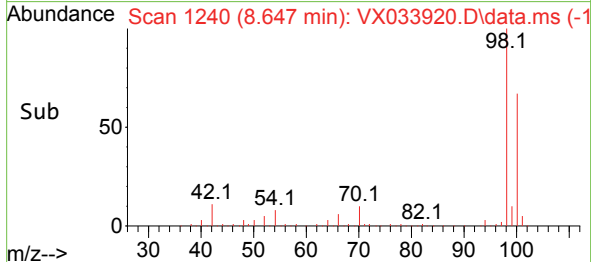

#52
Toluene
Concen: 2.651 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 92 Resp: 10251
Ion Ratio Lower Upper
92 100
91 167.1 135.5 203.3




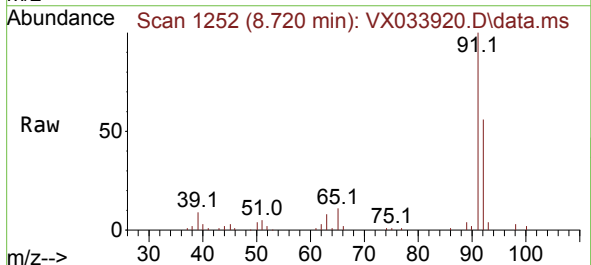




#62
4-Bromofluorobenzene
Concen: 47.456 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion: 95 Resp: 90365
Ion Ratio Lower Upper
95 100
174 95.5 0.0 184.4
176 93.7 0.0 178.8

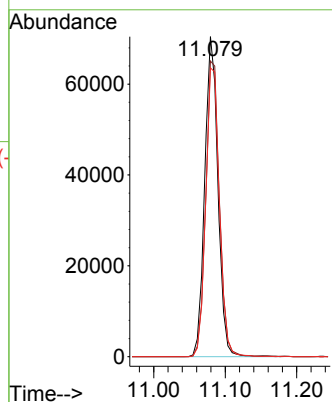

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 117 Resp: 202711
Ion Ratio Lower Upper
117 100
82 50.4 40.6 60.8
119 32.2 25.6 38.4


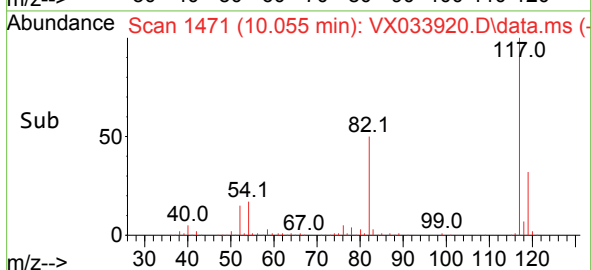






#67
Ethyl Benzene
Concen: 0.537 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion: 91 Resp: 3868
Ion Ratio Lower Upper
91 100
106 25.3 25.8 38.8#

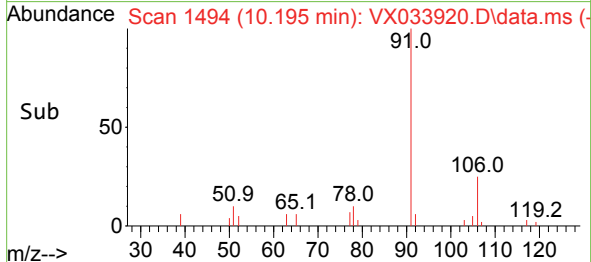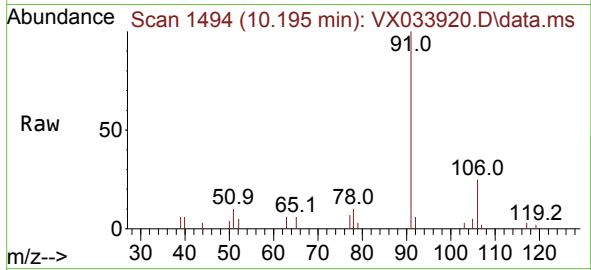

#68
m/p-Xylenes
Concen: 2.072 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 106 Resp: 5839
Ion Ratio Lower Upper
106 100
91 200.3 156.4 234.6

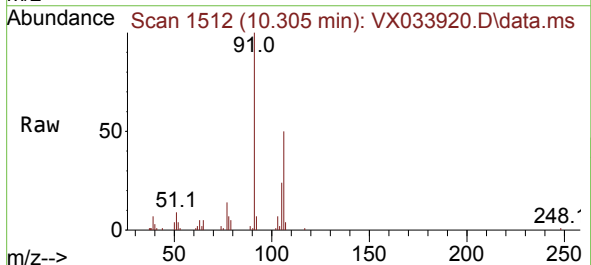



#69

o-Xylene

Concen: 1.525 ug/l

RT: 10.646 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :





33903

Tgt Ion:106 Resp: 4263

Ion Ratio Lower Upper

106 100

91 194.8 103.1 309.3

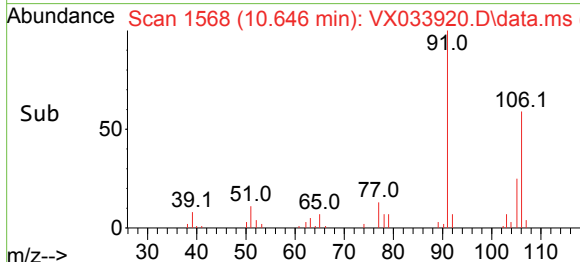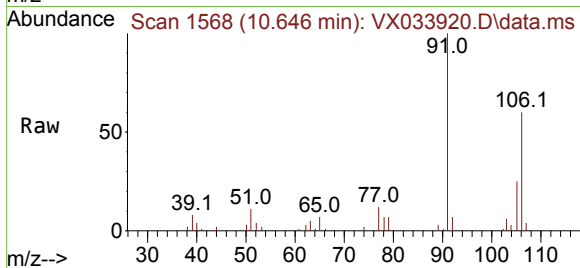

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24




Tgt Ion:152 Resp: 98618


Ion Ratio Lower Upper

152 100

115 53.5 38.7 116.1

150 156.9 0.0 348.2

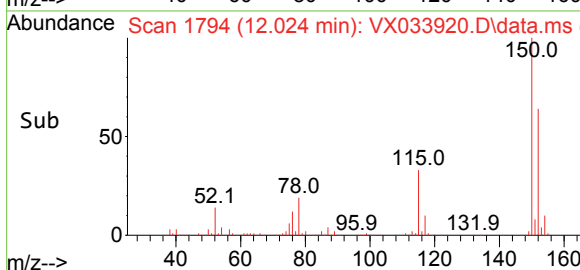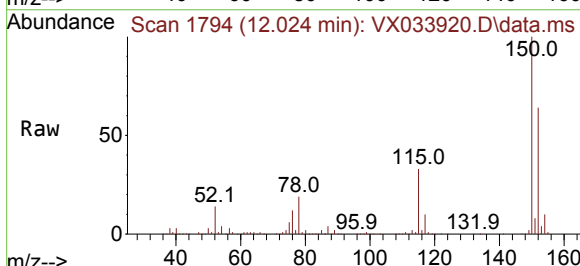



#73

Isopropylbenzene

Concen: Below Cal

RT: 10.963 min Scan# 1

Delta R.T. -0.001 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :





33903

Tgt Ion:105 Resp: 2032

Ion Ratio Lower Upper

105 100

120 31.2 13.6 40.8

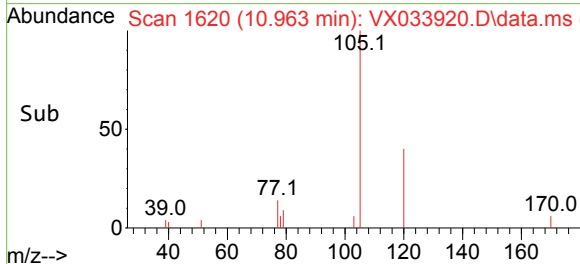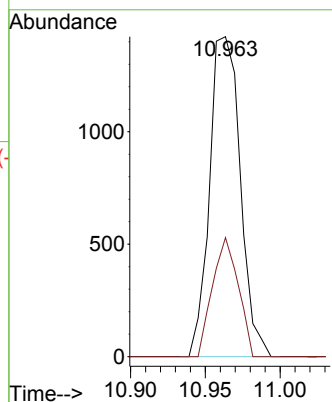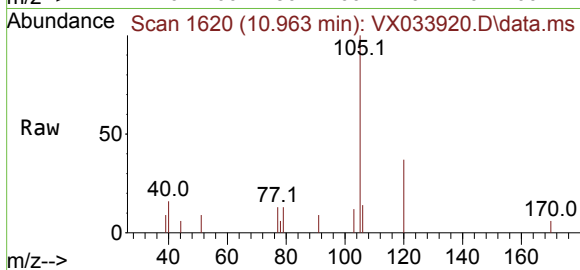

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 11.085 min Scan# 1640

Delta R.T. -0.128 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24




Tgt Ion: 83 Resp: 20


Ion Ratio Lower Upper

83 100

131 665.0 5.5 16.7#

85 0.0 32.3 96.9#

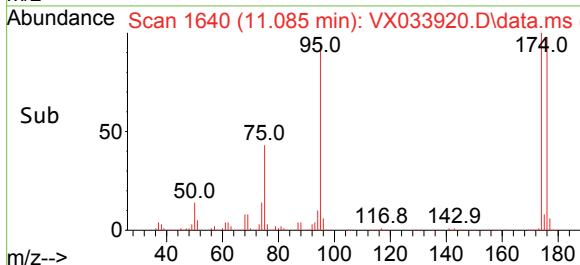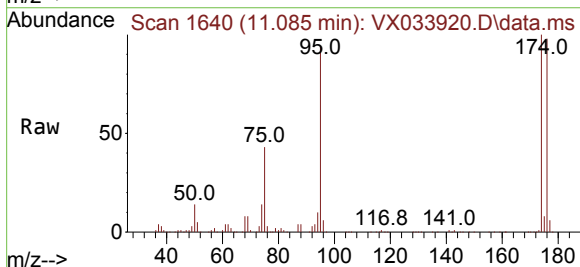



#76

1,2,3-Trichloropropane

Concen: 23.009 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.159 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :





33903

Tgt Ion: 75 Resp: 41692

Ion Ratio Lower Upper

75 100

77 1.1 21.8 65.4#

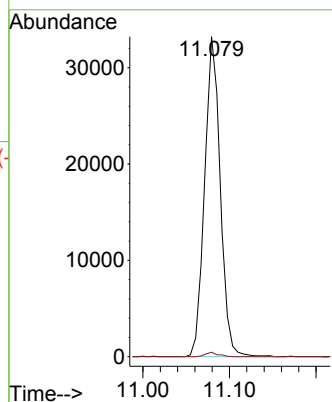

#78

n-propylbenzene

Concen: 0.252 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX033920.D




Acq: 26 Jan 2023 19:24


Tgt Ion: 91 Resp: 2025

Ion Ratio Lower Upper

91 100

120 26.6 12.3 36.8

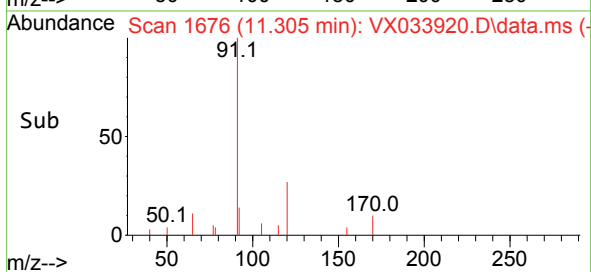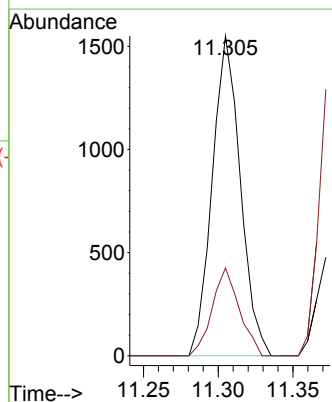



#79

2-Chlorotoluene

Concen: Below Cal

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :





33903

Tgt Ion: 91 Resp: 1341

Ion Ratio Lower Upper

91 100

126 0.0 18.1 54.1#

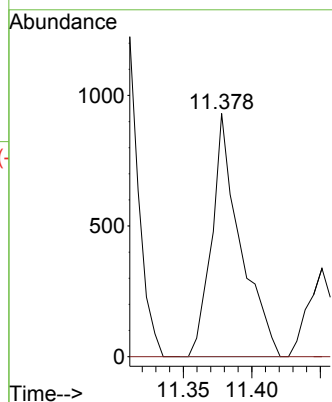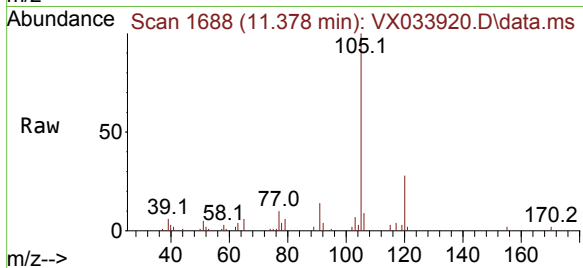

#80

1,3,5-Trimethylbenzene

Concen: 0.694 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX033920.D




Acq: 26 Jan 2023 19:24


Tgt Ion: 105 Resp: 4121

Ion Ratio Lower Upper

105 100

120 49.6 25.6 76.8


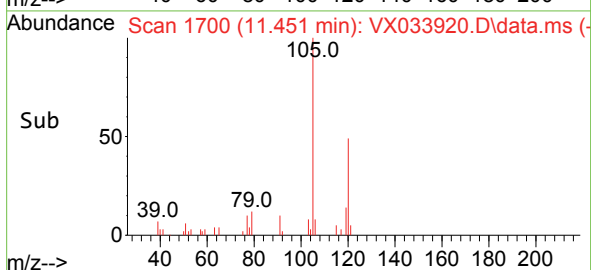

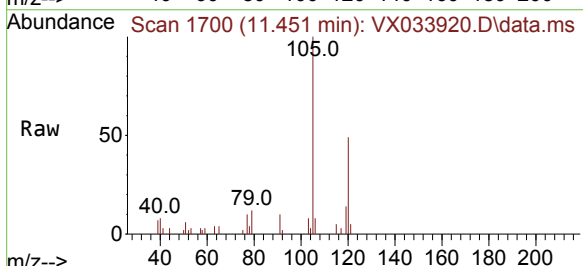




#81
trans-1,4-Dichloro-2-butene
Concen: 71.510 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24




Instrument :
MSVOA_X
ClientSampleId :
33903


Tgt Ion: 75 Resp: 41692
Ion Ratio Lower Upper
75 100
53 0.0 83.0 124.6#
89 0.0 37.7 56.5#

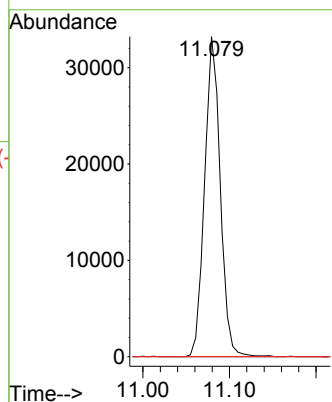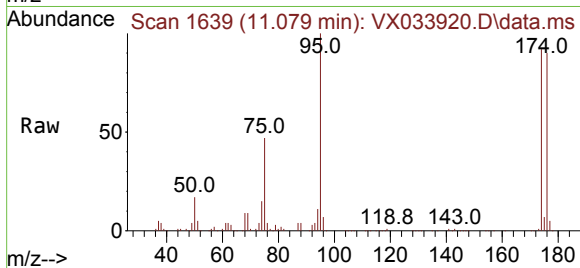

#82
4-Chlorotoluene
Concen: Below Cal
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX033920.D
Acq: 26 Jan 2023 19:24

Tgt Ion: 91 Resp: 513
Ion Ratio Lower Upper
91 100
126 0.0 15.8 47.4#

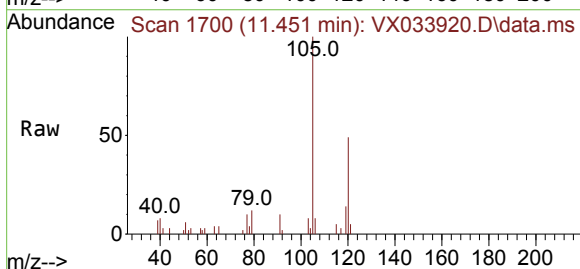



#83

tert-Butylbenzene

Concen: 0.341 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.036 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :

33903





Tgt Ion:119 Resp: 2011

Ion Ratio Lower Upper

119 100

91 77.9 26.9 80.7

134 0.0 12.3 36.8#

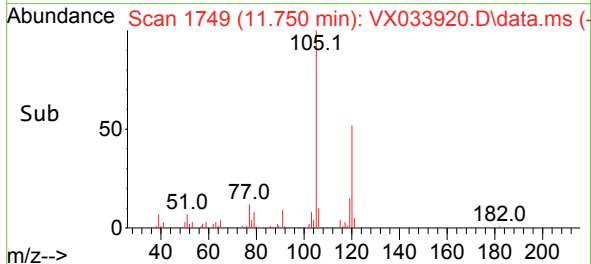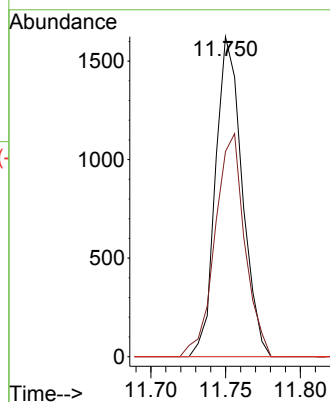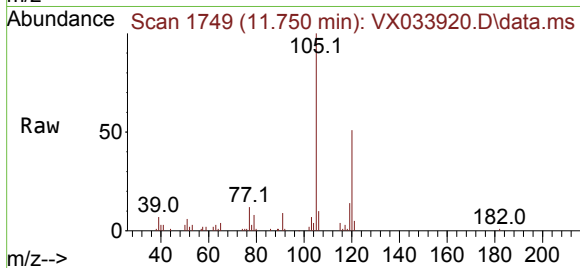

#84

1,2,4-Trimethylbenzene

Concen: 2.706 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX033920.D




Acq: 26 Jan 2023 19:24


Tgt Ion:105 Resp: 15189

Ion Ratio Lower Upper

105 100

120 48.1 23.4 70.2

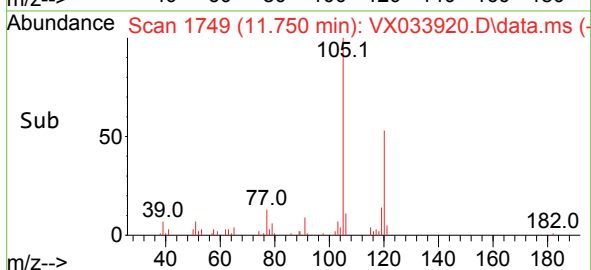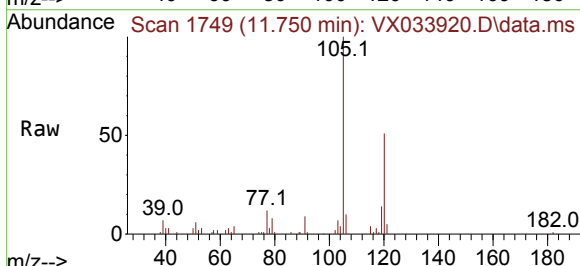



#89

n-Butylbenzene

Concen: 0.265 ug/l

RT: 12.329 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX033920.D

Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :

33903





Tgt Ion: 91 Resp: 1309

Ion Ratio Lower Upper

91 100

92 28.0 27.5 82.5

134 113.0 14.3 42.9#

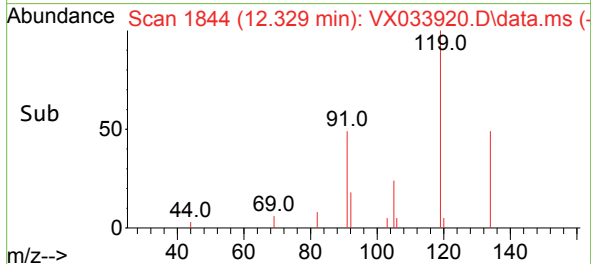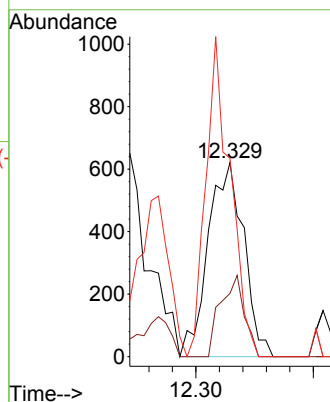

#90

Hexachloroethane

Concen: 0.285 ug/l

RT: 12.530 min Scan# 1877

Delta R.T. -0.006 min

Lab File: VX033920.D




Acq: 26 Jan 2023 19:24


Tgt Ion: 117 Resp: 283

Ion Ratio Lower Upper

117 100

201 0.0 45.1 135.3#

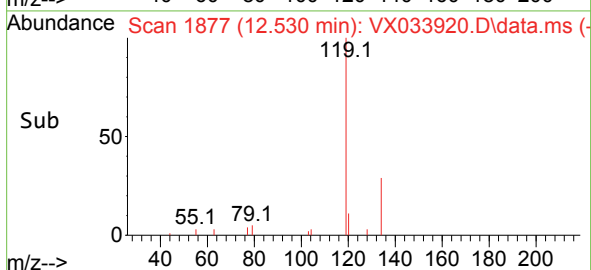



#95

Naphthalene

Concen: 1.716 ug/l

RT: 13.780 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX033920.D


Acq: 26 Jan 2023 19:24

Instrument :

MSVOA_X

ClientSampleId :

33903

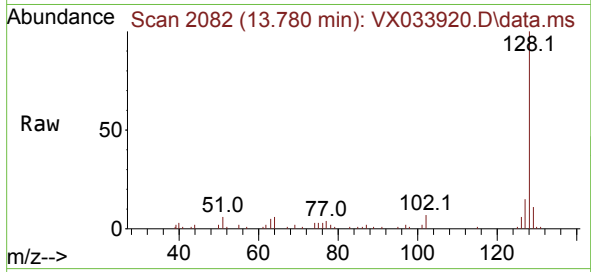

Tgt Ion:128 Resp: 10690

Ion Ratio Lower Upper

128 100

127 13.3 10.3 15.5

129 11.0 8.7 13.1

