

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
 Data File : VX033907.D
 Acq On : 26 Jan 2023 13:41
 Operator : JC/MD
 Sample : 01308-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LEA-13I

Quant Time: Jan 27 02:54:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 11 14:48:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	156135	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	220107	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	189257	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	82028	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	73141	44.491	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	88.980%
35) Dibromofluoromethane	5.385	113	67875	49.662	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.320%
50) Toluene-d8	8.647	98	250153	50.234	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.460%
62) 4-Bromofluorobenzene	11.079	95	80617	43.603	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	87.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
Data File : VX033907.D
Acq On : 26 Jan 2023 13:41
Operator : JC/MD
Sample : 01308-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-13I

Quant Time: Jan 27 02:54:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 11 14:48:42 2023
Response via : Initial Calibration




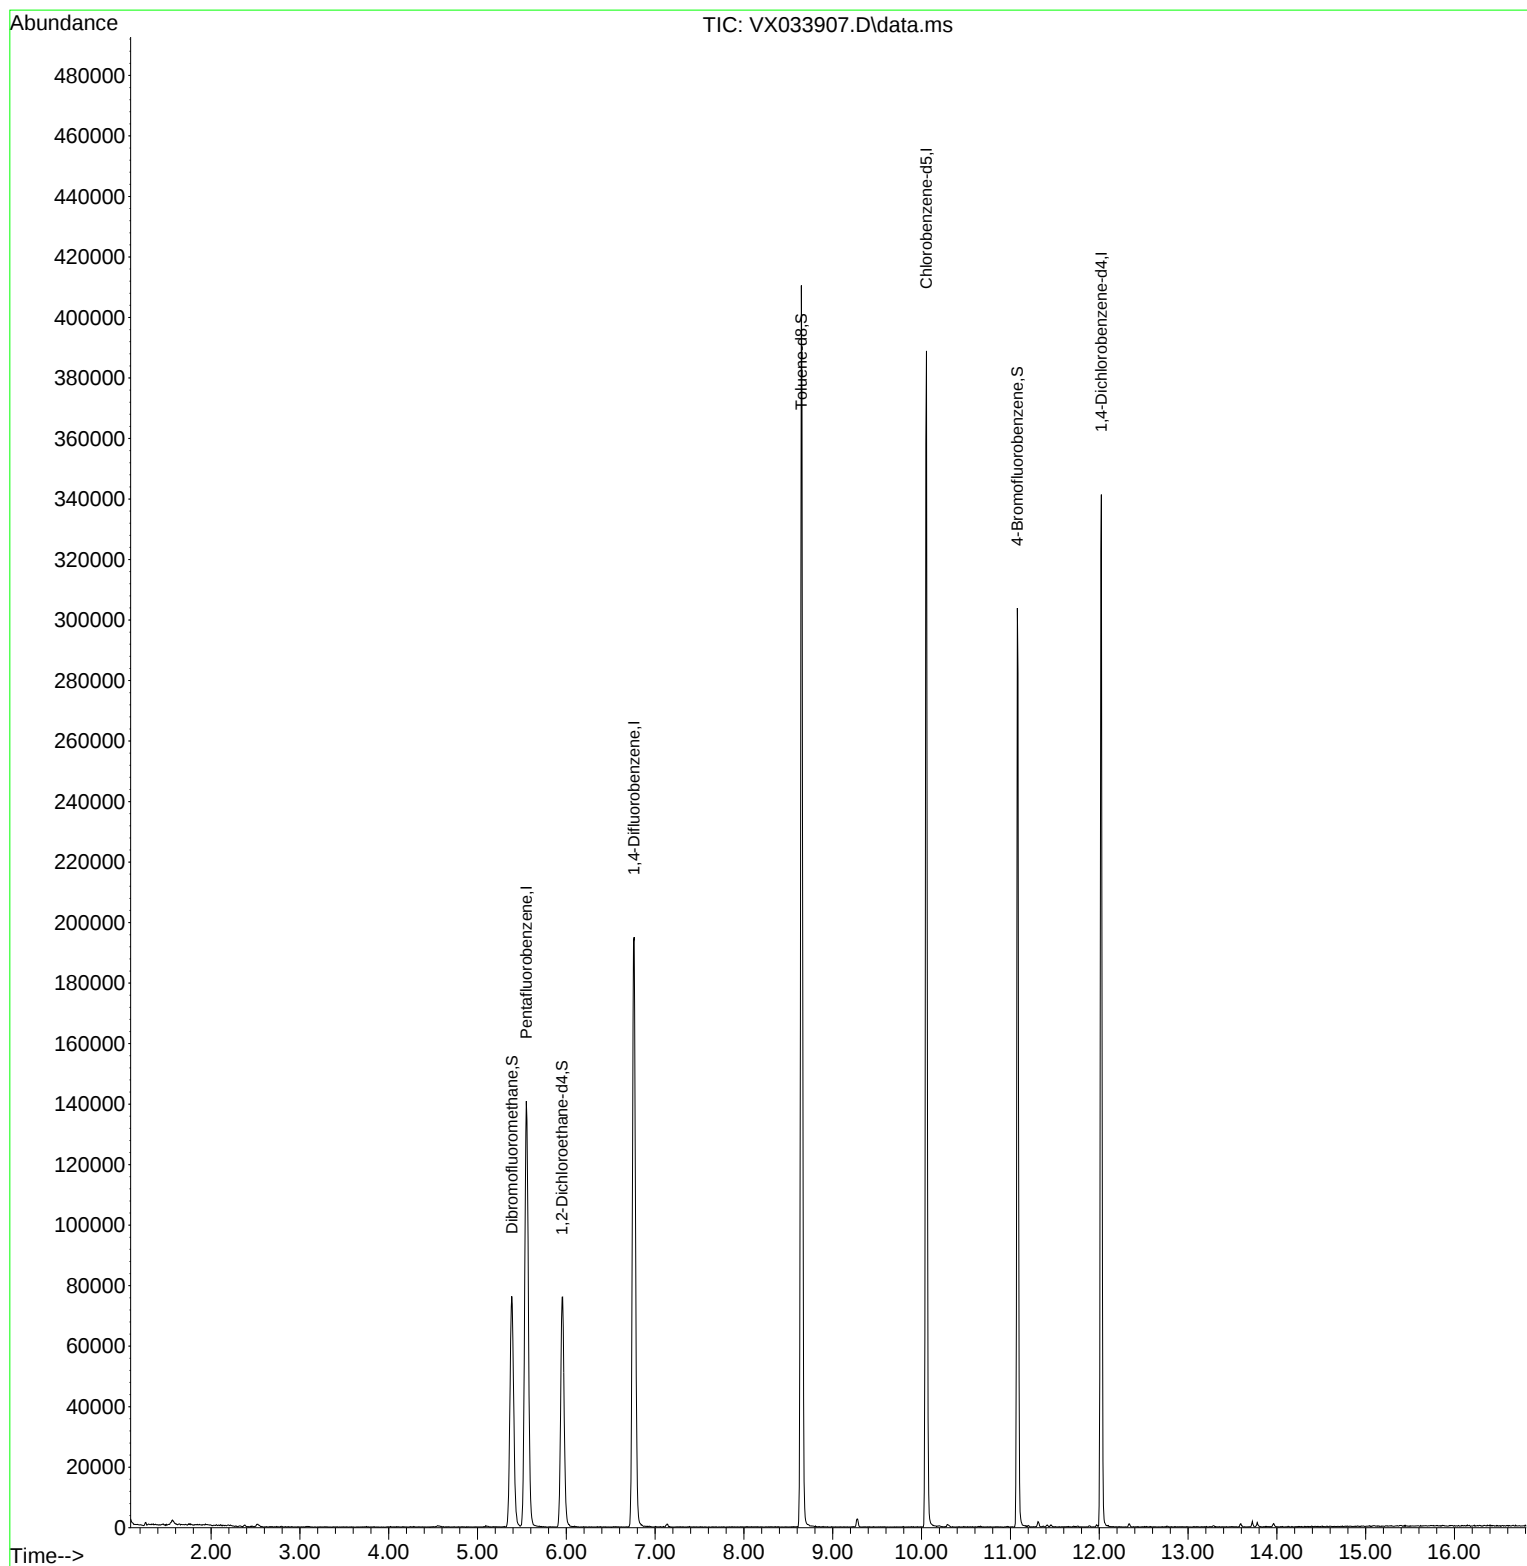


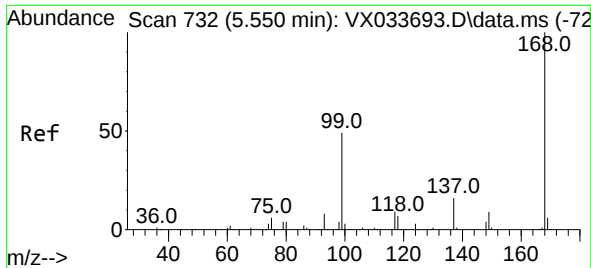

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX033907.D
Acq: 26 Jan 2023 13:41




Instrument :
MSVOA_X
ClientSampleId :
LEA-13I


Tgt Ion:168 Resp: 156135
Ion Ratio Lower Upper
168 100
99 46.4 39.6 59.4

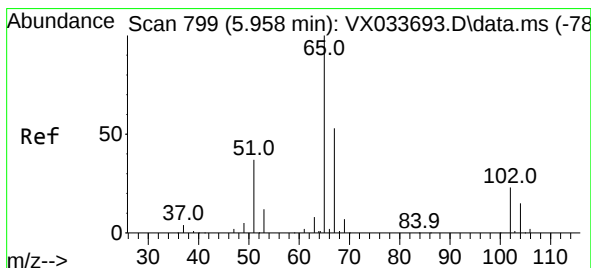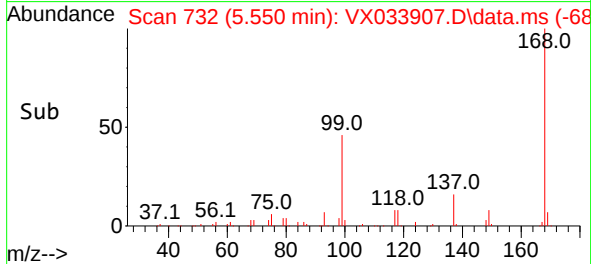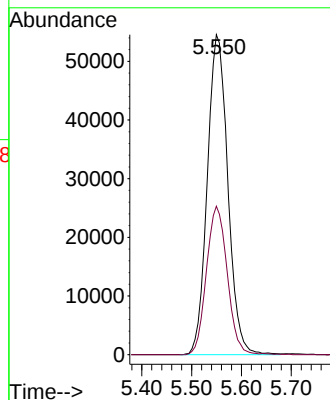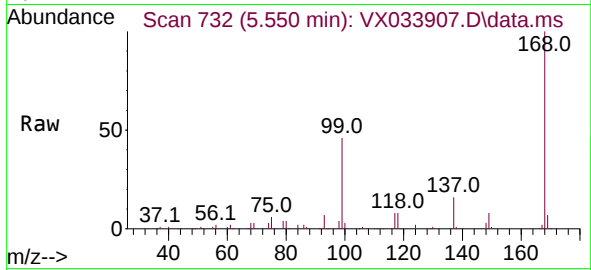

#33
1,2-Dichloroethane-d4
Concen: 44.491 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX033907.D
Acq: 26 Jan 2023 13:41

Tgt Ion: 65 Resp: 73141
Ion Ratio Lower Upper
65 100
67 53.4 0.0 104.8


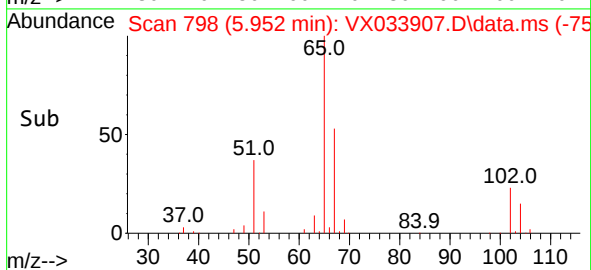
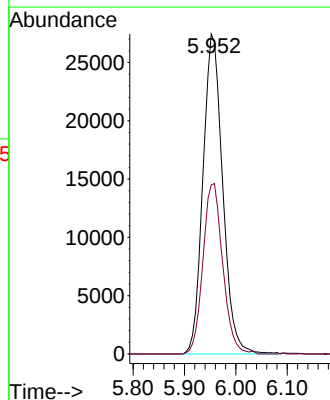
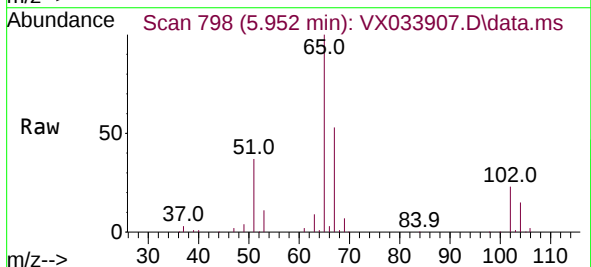


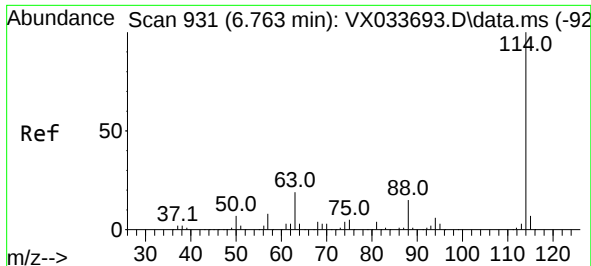

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX033907.D
Acq: 26 Jan 2023 13:41




Instrument :
MSVOA_X
ClientSampleId :
LEA-13I


Tgt Ion:114 Resp: 220107
Ion Ratio Lower Upper
114 100
63 18.6 0.0 37.4
88 14.6 0.0 30.6

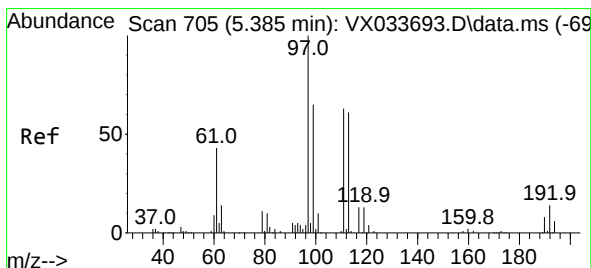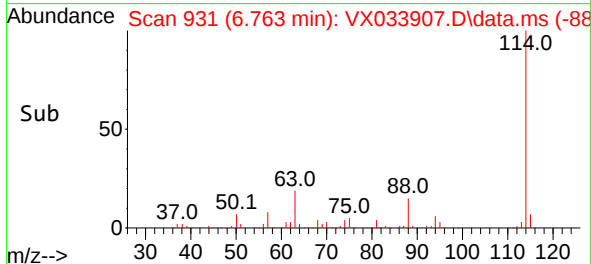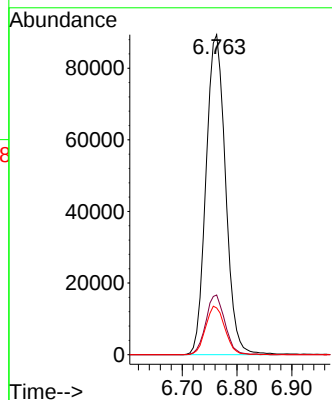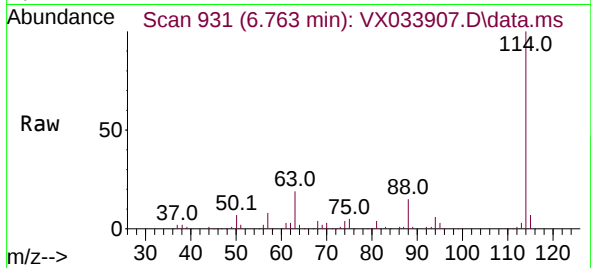

#35
Dibromofluoromethane
Concen: 49.662 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX033907.D
Acq: 26 Jan 2023 13:41

Tgt Ion:113 Resp: 67875
Ion Ratio Lower Upper
113 100
111 102.0 83.0 124.6
192 24.7 19.0 28.4


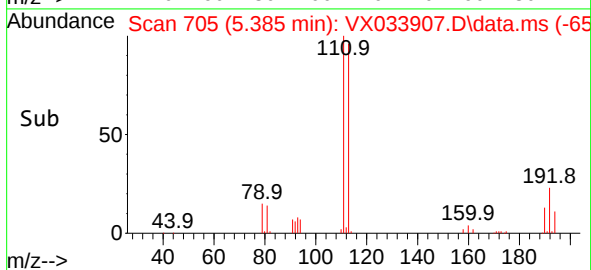
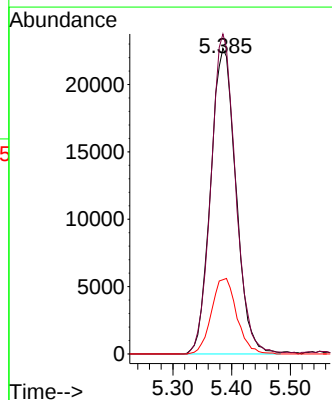
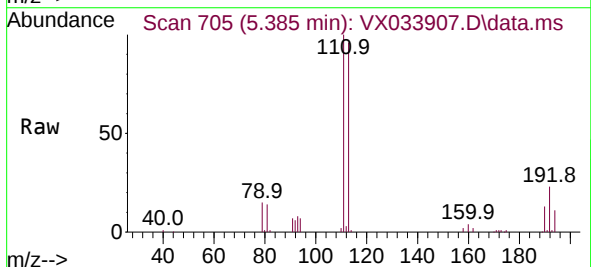


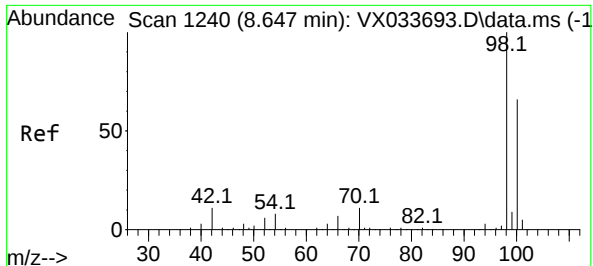

#50
Toluene-d8
Concen: 50.234 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033907.D
Acq: 26 Jan 2023 13:41




Instrument :
MSVOA_X
ClientSampleId :
LEA-13I


Tgt Ion: 98 Resp: 250153
Ion Ratio Lower Upper
98 100
100 66.7 53.6 80.4

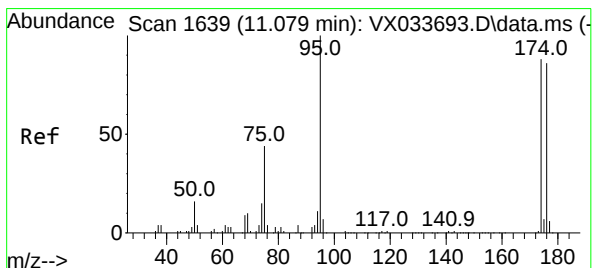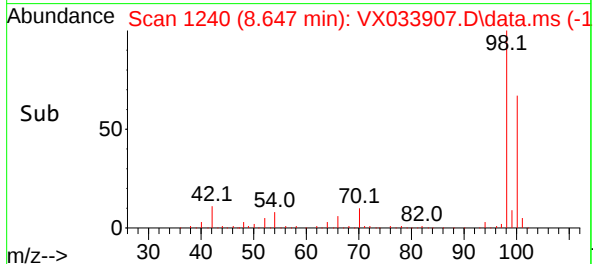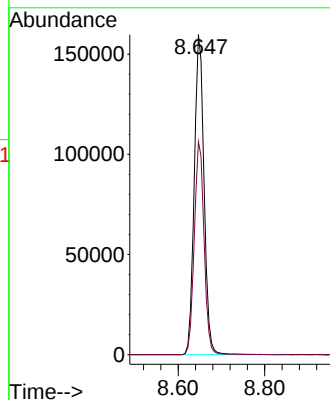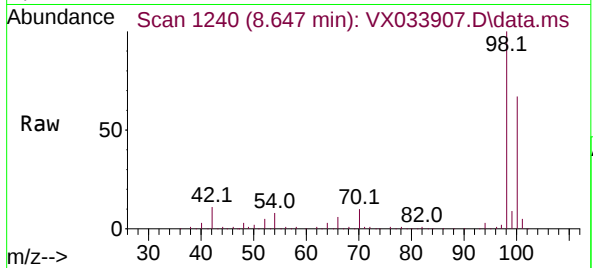

#62
4-Bromofluorobenzene
Concen: 43.603 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX033907.D
Acq: 26 Jan 2023 13:41

Tgt Ion: 95 Resp: 80617
Ion Ratio Lower Upper
95 100
174 96.1 0.0 184.4
176 92.5 0.0 178.8


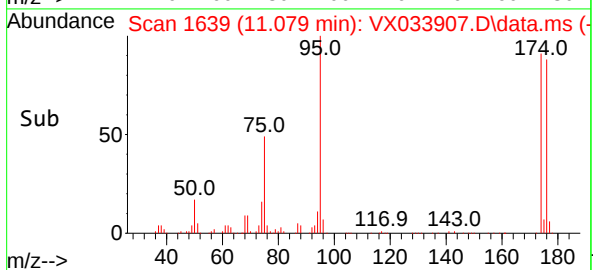
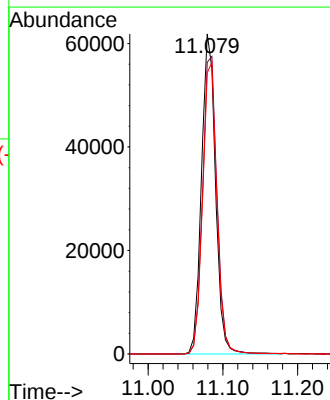
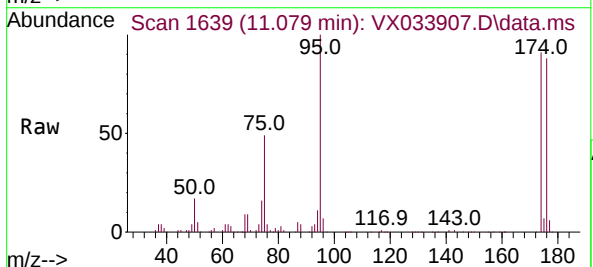


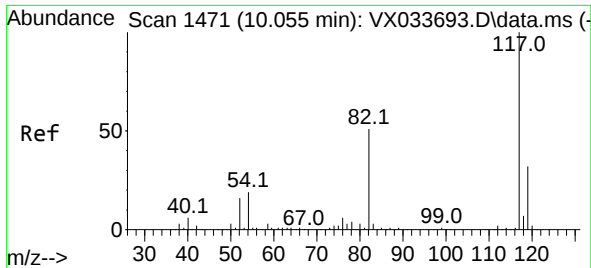

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX033907.D
Acq: 26 Jan 2023 13:41

Instrument :
MSVOA_X
ClientSampleId :
LEA-13I

Tgt Ion:117 Resp: 189257
Ion Ratio Lower Upper
117 100
82 49.7 40.6 60.8
119 31.7 25.6 38.4

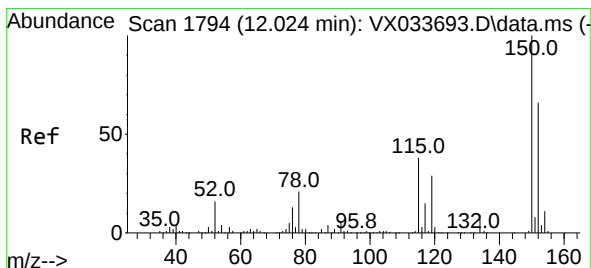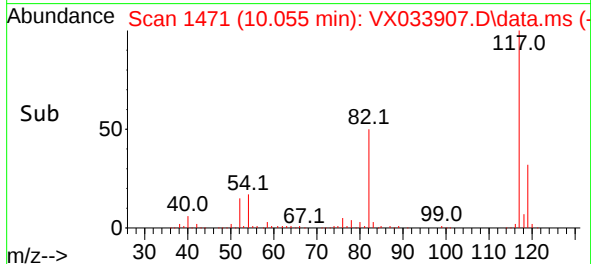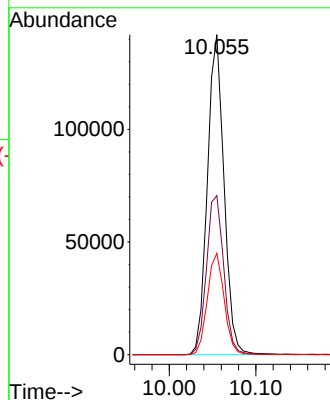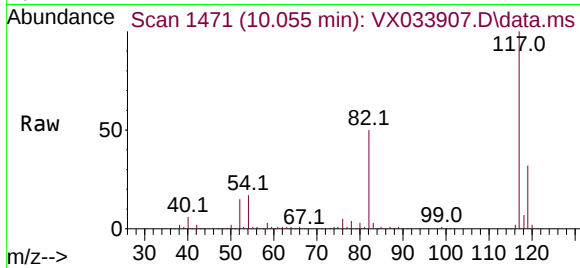

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX033907.D
Acq: 26 Jan 2023 13:41

Tgt Ion:152 Resp: 82028
Ion Ratio Lower Upper
152 100
115 53.3 38.7 116.1
150 154.2 0.0 348.2

