

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX012623\  
Data File : VX033913.D  
Acq On : 26 Jan 2023 16:42  
Operator : JC/MD  
Sample : 01323-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
22-MW-01S

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M

Title : SW846 8260

Signal : TIC: VX033913.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 694           | 705         | 721          | rBV      | 82381          | 236454        | 34.66%          | 6.551%        |
| 2         | 5.550       | 721           | 732         | 747          | rVV      | 147593         | 417243        | 61.15%          | 11.560%       |
| 3         | 5.952       | 787           | 798         | 816          | rBV      | 82297          | 220251        | 32.28%          | 6.102%        |
| 4         | 6.763       | 920           | 931         | 944          | rBV      | 209155         | 505108        | 74.03%          | 13.994%       |
| 5         | 8.647       | 1234          | 1240        | 1258         | rBV      | 443079         | 682286        | 100.00%         | 18.903%       |
| 6         | 10.055      | 1465          | 1471        | 1482         | rBV      | 424612         | 583175        | 85.47%          | 16.157%       |
| 7         | 11.079      | 1634          | 1639        | 1648         | rBV      | 356240         | 450746        | 66.06%          | 12.488%       |
| 8         | 12.024      | 1788          | 1794        | 1807         | rBV      | 405787         | 514121        | 75.35%          | 14.244%       |




Sum of corrected areas: 3609384

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX012623\  
Data File : VX033913.D  
Acq On : 26 Jan 2023 16:42  
Operator : JC/MD  
Sample : 01323-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
22-MW-01S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

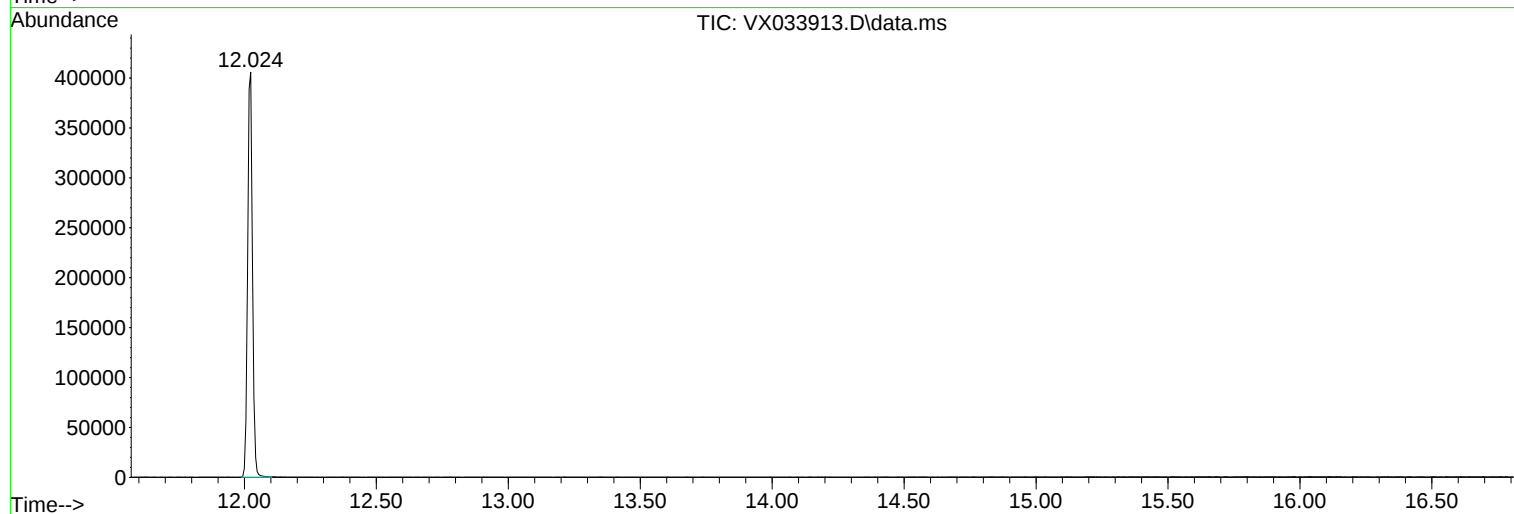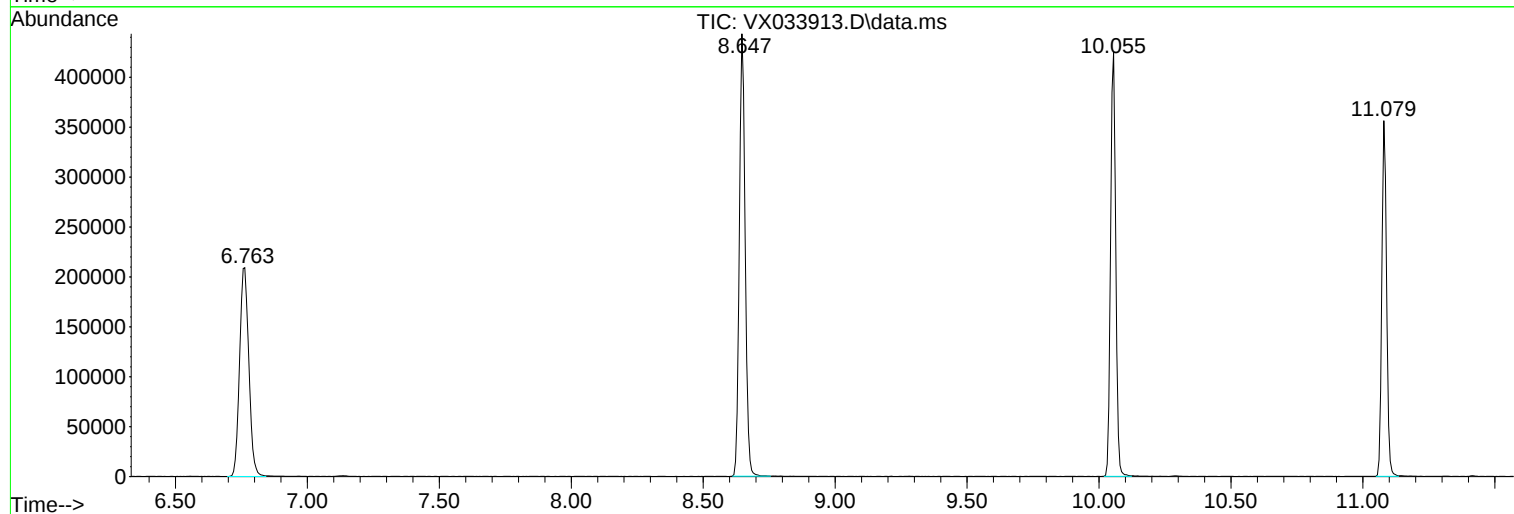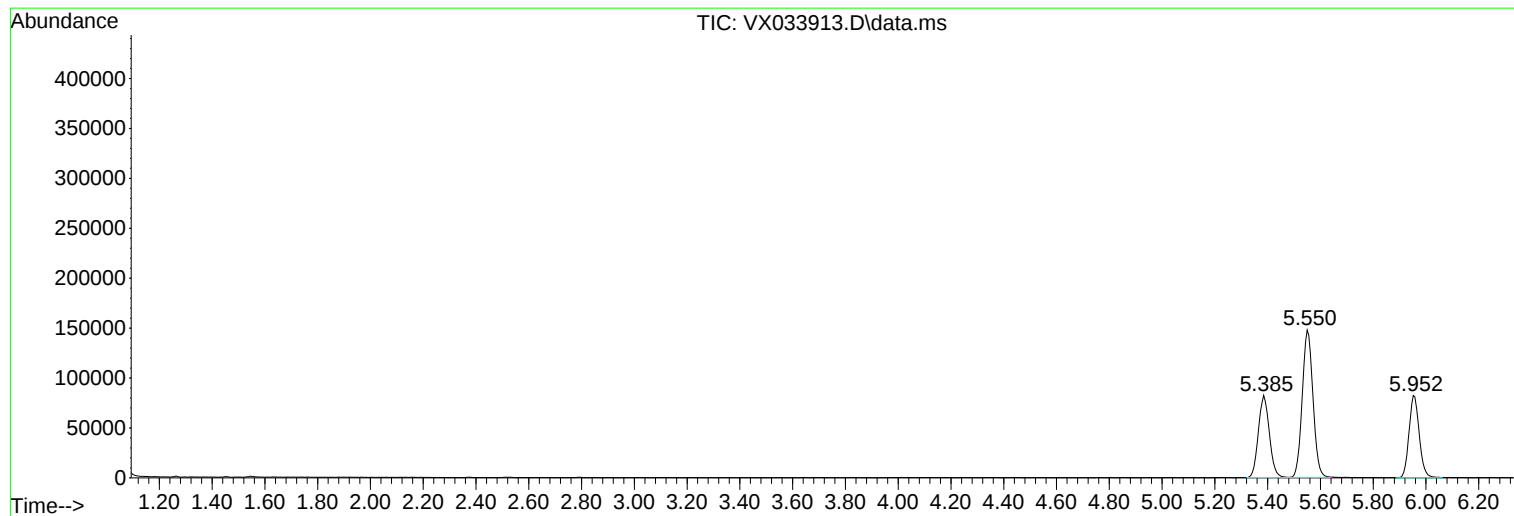

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX012623\  
Data File : VX033913.D  
Acq On : 26 Jan 2023 16:42  
Operator : JC/MD  
Sample : 01323-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
22-MW-01S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX012623\  
Data File : VX033913.D  
Acq On : 26 Jan 2023 16:42  
Operator : JC/MD  
Sample : 01323-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
22-MW-01S

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|