

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX012623\  
Data File : VX033915.D  
Acq On : 26 Jan 2023 17:28  
Operator : JC/MD  
Sample : 01323-16  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-22

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M

Title : SW846 8260

Signal : TIC: VX033915.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.374       | 43            | 47          | 71           | rBV      | 3412769        | 4084869       | 15.08%          | 11.943%       |
| 2         | 4.495       | 544           | 559         | 596          | rBV      | 9356131        | 27090545      | 100.00%         | 79.205%       |
| 3         | 5.550       | 721           | 732         | 748          | rVV      | 142755         | 402668        | 1.49%           | 1.177%        |
| 4         | 6.763       | 920           | 931         | 947          | rBV      | 201474         | 484631        | 1.79%           | 1.417%        |
| 5         | 8.647       | 1233          | 1240        | 1260         | rBV      | 413398         | 655427        | 2.42%           | 1.916%        |
| 6         | 10.055      | 1465          | 1471        | 1483         | rVB      | 399674         | 551473        | 2.04%           | 1.612%        |
| 7         | 11.079      | 1634          | 1639        | 1651         | rBV      | 337583         | 432224        | 1.60%           | 1.264%        |
| 8         | 12.018      | 1788          | 1793        | 1806         | rBV      | 380964         | 501071        | 1.85%           | 1.465%        |




Sum of corrected areas: 34202908

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX012623\  
Data File : VX033915.D  
Acq On : 26 Jan 2023 17:28  
Operator : JC/MD  
Sample : 01323-16  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

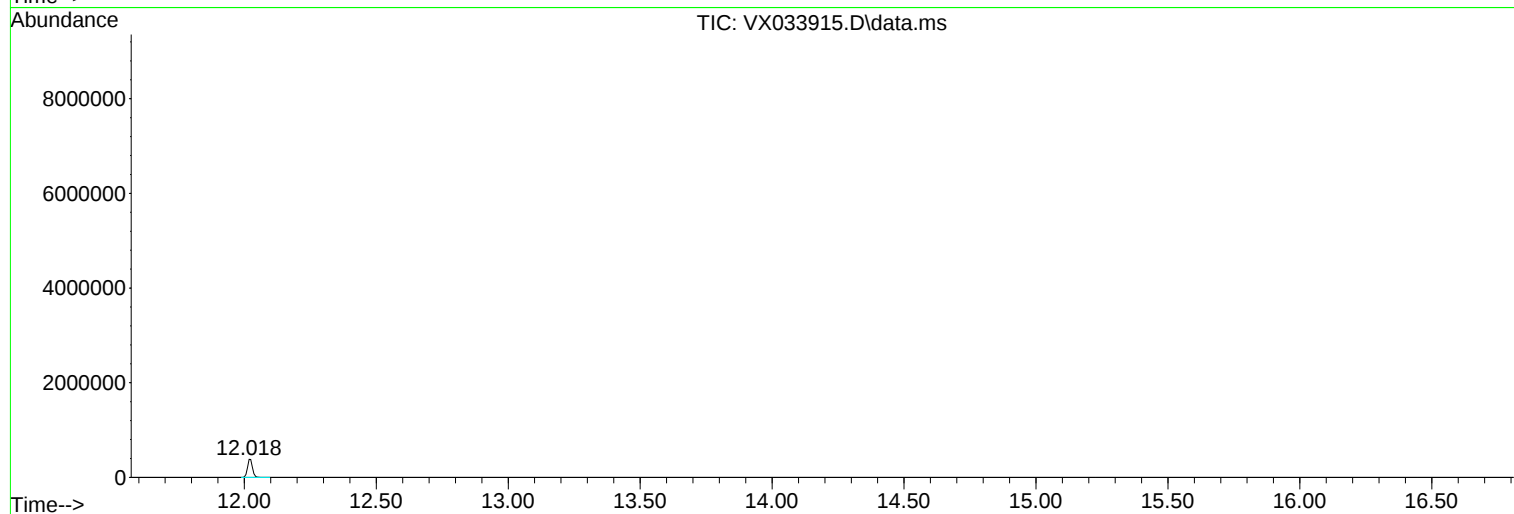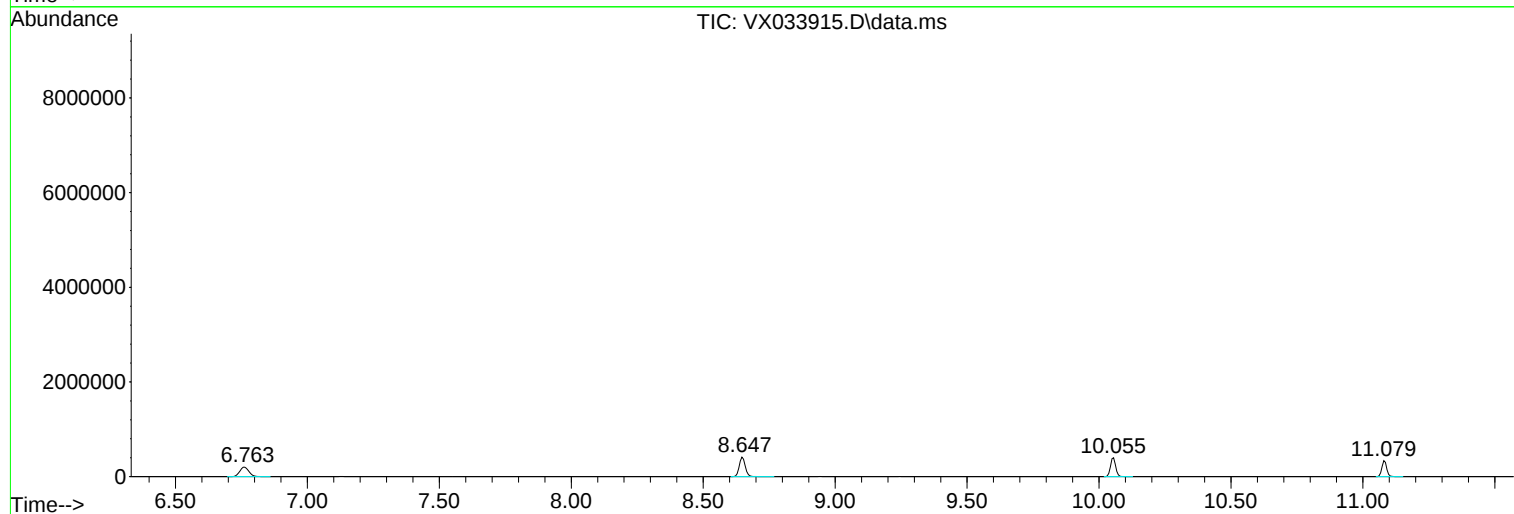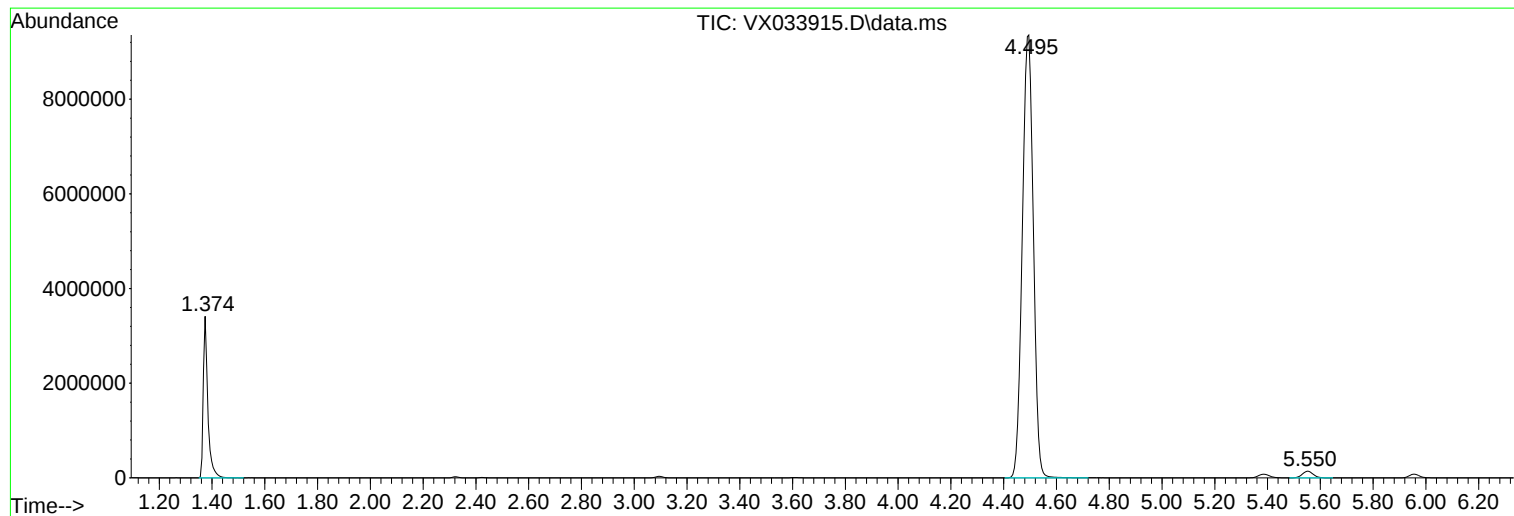

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX012623\  
Data File : VX033915.D  
Acq On : 26 Jan 2023 17:28  
Operator : JC/MD  
Sample : 01323-16  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX012623\  
Data File : VX033915.D  
Acq On : 26 Jan 2023 17:28  
Operator : JC/MD  
Sample : 01323-16  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X011123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|