

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
 Data File : VX033916.D
 Acq On : 26 Jan 2023 17:52
 Operator : JC/MD
 Sample : 01323-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LEA-5SR

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Title : SW846 8260

Signal : TIC: VX033916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.373	203	211	220	rBV	12346	20669	3.09%	0.557%
2	2.946	296	305	315	rVB	7339	17109	2.56%	0.461%
3	4.489	547	558	562	rBV	16038	41261	6.17%	1.112%
4	4.544	562	567	579	rVB	17935	60177	8.99%	1.622%
5	5.385	694	705	720	rBV	80204	232668	34.77%	6.271%
6	5.550	720	732	748	rVV	146488	411039	61.42%	11.078%
7	5.952	786	798	814	rBV	79459	215188	32.16%	5.799%
8	6.763	920	931	944	rBV	203954	497442	74.33%	13.406%
9	8.647	1233	1240	1256	rBV	425792	669214	100.00%	18.036%
10	10.055	1465	1471	1480	rBV	414957	563515	84.21%	15.187%
11	11.079	1634	1639	1656	rBV	354590	451886	67.52%	12.179%
12	12.024	1788	1794	1806	rBV	407944	530298	79.24%	14.292%




Sum of corrected areas: 3710466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
Data File : VX033916.D
Acq On : 26 Jan 2023 17:52
Operator : JC/MD
Sample : 01323-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-5SR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

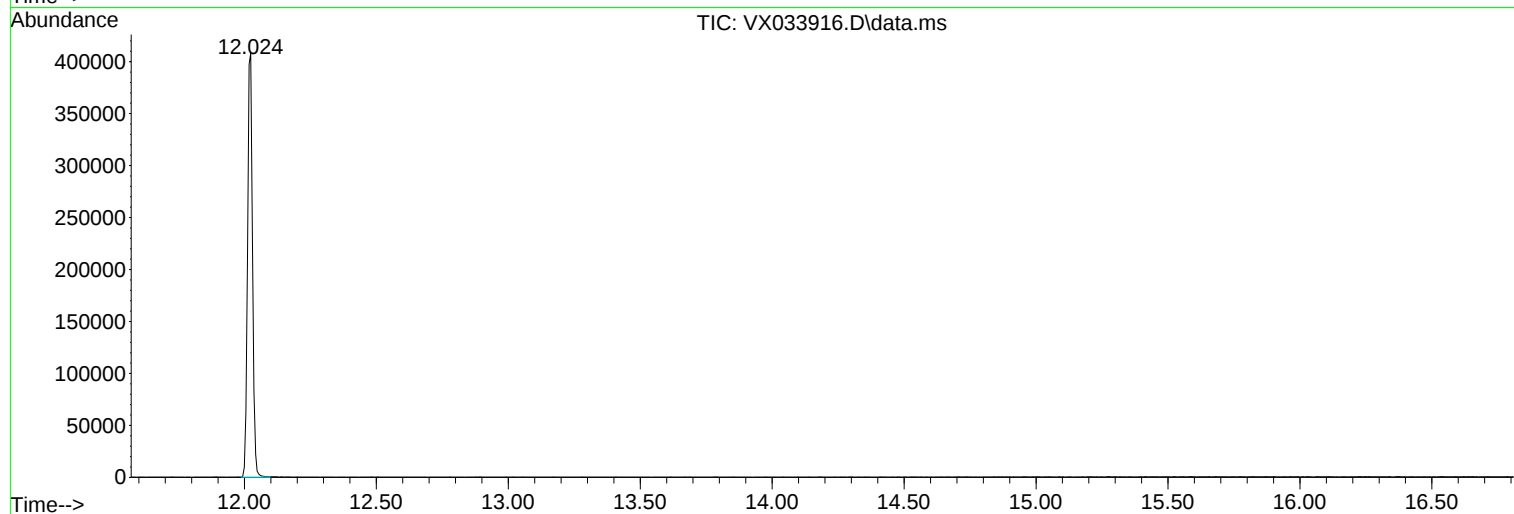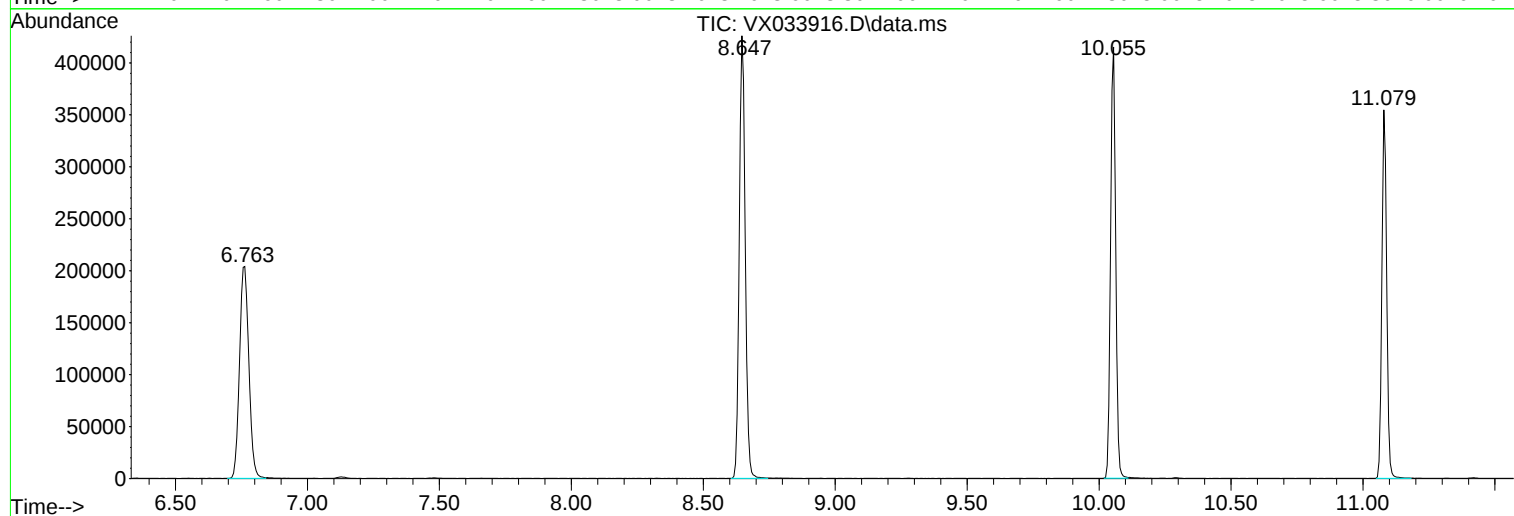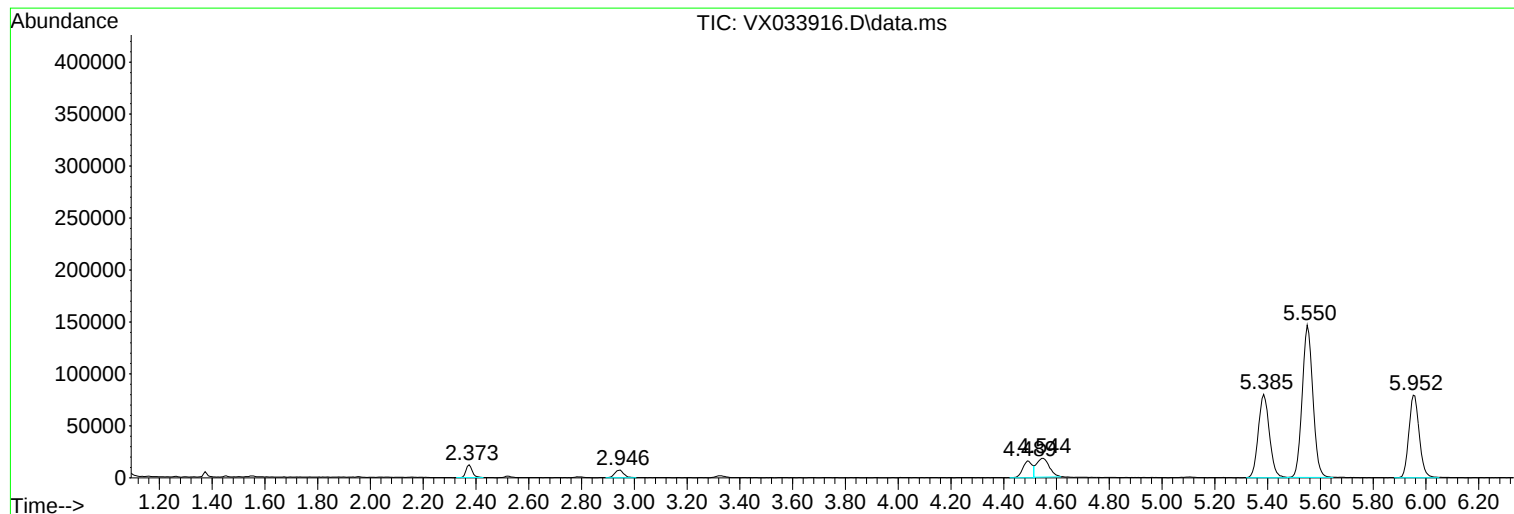

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
Data File : VX033916.D
Acq On : 26 Jan 2023 17:52
Operator : JC/MD
Sample : 01323-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-5SR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
Data File : VX033916.D
Acq On : 26 Jan 2023 17:52
Operator : JC/MD
Sample : 01323-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-5SR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------