

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
 Data File : VX033917.D
 Acq On : 26 Jan 2023 18:15
 Operator : JC/MD
 Sample : 01320-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOTE-COMP-0126

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Title : SW846 8260

Signal : TIC: VX033917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	32	rBV	13215	13820	2.02%	0.343%
2	2.374	206	211	222	rVB	5610	9020	1.32%	0.224%
3	4.495	549	559	567	rBV3	4378	12487	1.83%	0.310%
4	5.093	646	657	667	rBV2	3549	9855	1.44%	0.245%
5	5.385	692	705	719	rBV	82063	236401	34.62%	5.873%
6	5.550	721	732	751	rVB	143768	413354	60.54%	10.270%
7	5.952	788	798	813	rBV	81553	219270	32.11%	5.448%
8	6.763	921	931	948	rBV	209710	501528	73.45%	12.461%
9	8.647	1233	1240	1248	rBV	452836	682822	100.00%	16.965%
10	8.720	1248	1252	1260	rVB	20479	31763	4.65%	0.789%
11	10.055	1465	1471	1486	rBV	419976	583917	85.52%	14.508%
12	11.079	1634	1639	1651	rBV	359073	461593	67.60%	11.468%
13	11.366	1680	1686	1692	rBV	121933	163307	23.92%	4.057%
14	11.457	1696	1701	1708	rVB	46524	61212	8.96%	1.521%
15	12.024	1788	1794	1803	rBV	437835	567045	83.04%	14.088%
16	12.439	1857	1862	1869	rBV	46256	57509	8.42%	1.429%




Sum of corrected areas: 4024903

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
Data File : VX033917.D
Acq On : 26 Jan 2023 18:15
Operator : JC/MD
Sample : 01320-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP-0126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

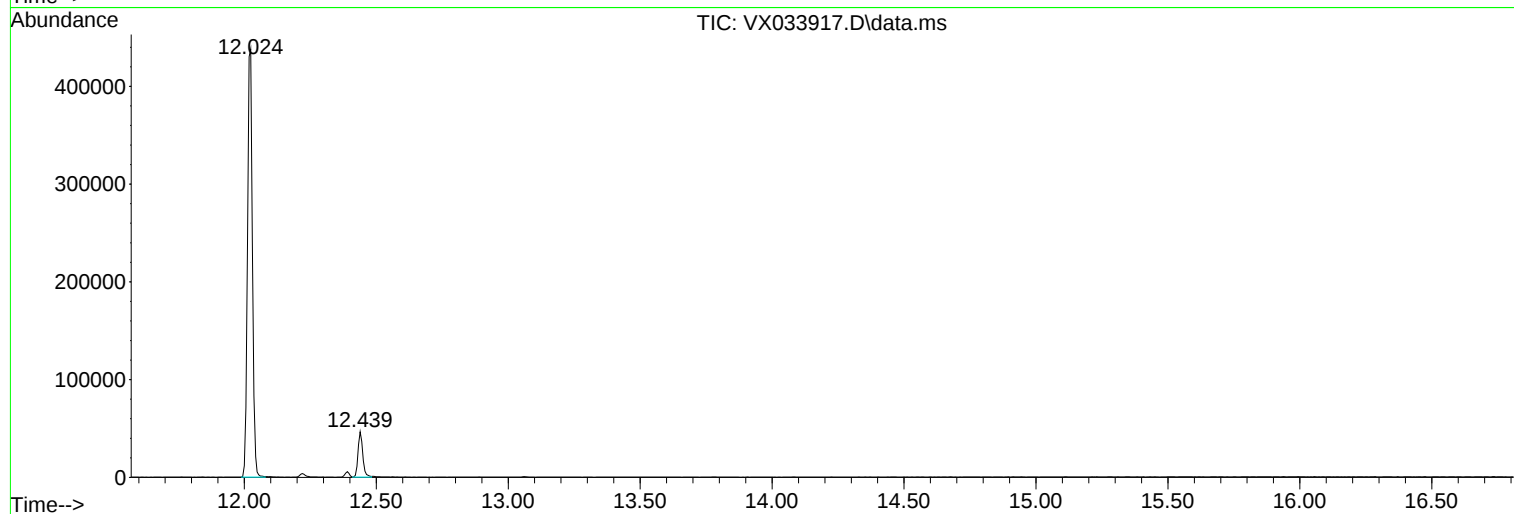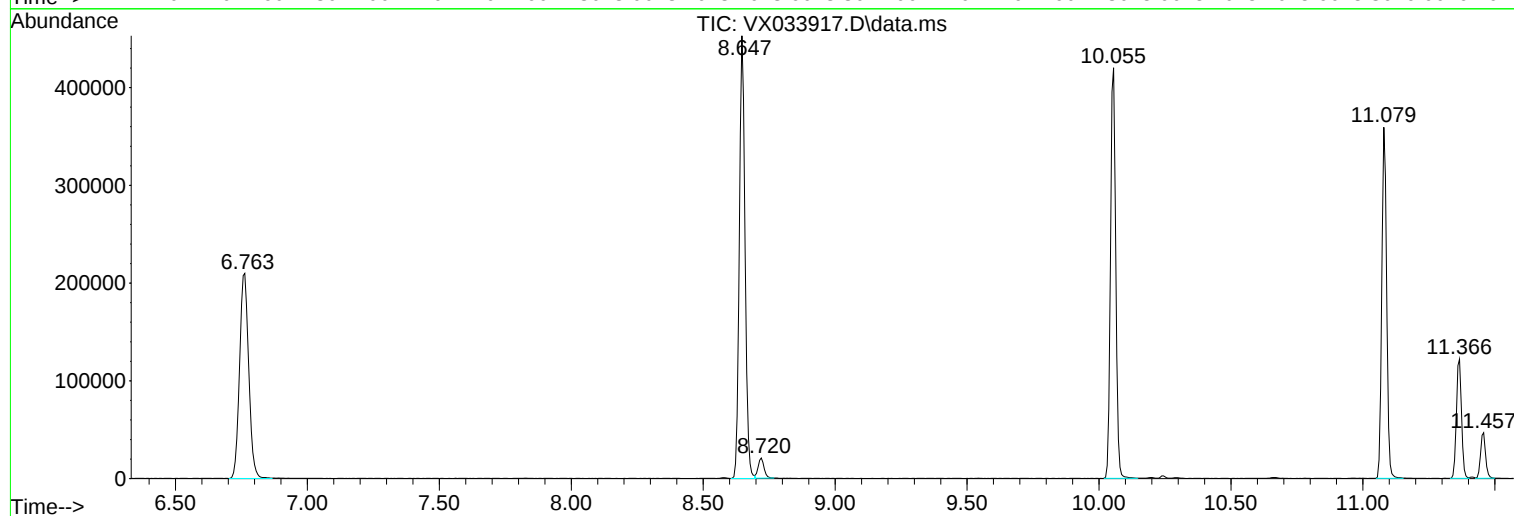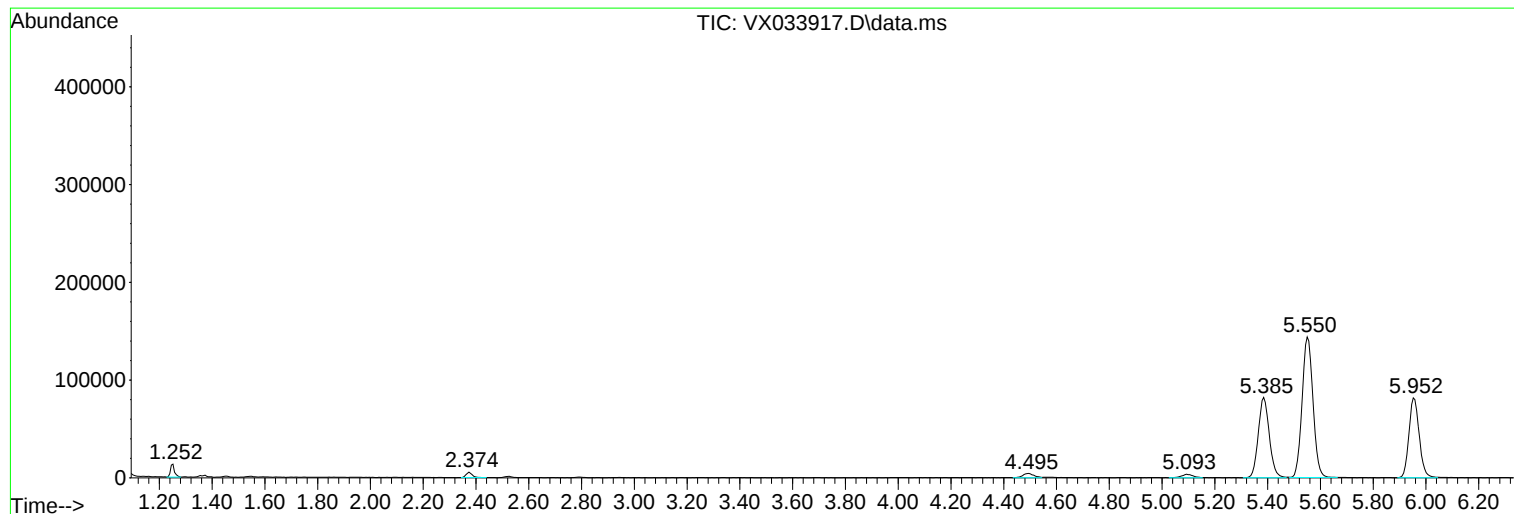

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
Data File : VX033917.D
Acq On : 26 Jan 2023 18:15
Operator : JC/MD
Sample : 01320-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP-0126










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, (ethoxymethyl)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.439	5.07 ug/l	57509	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, (ethoxymethyl)-	136	C9H12O	000539-30-0	96
2			Benzeneacetamide	135	C8H9NO	000103-81-1	52
3			Benzeneethanol, .alpha.-methyl-	136	C9H12O	000698-87-3	52
4			Toluene	92	C7H8	000108-88-3	50
5			2-Propanone, 1-(4-pyridinyl)-	135	C8H9NO	006304-16-1	46

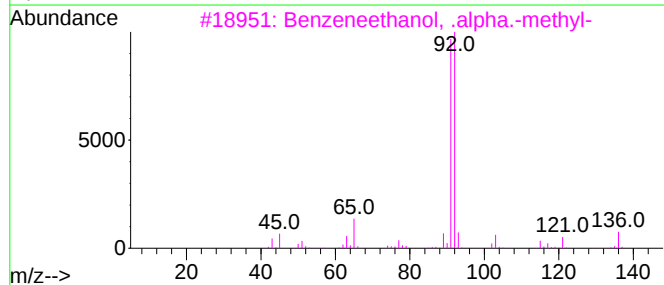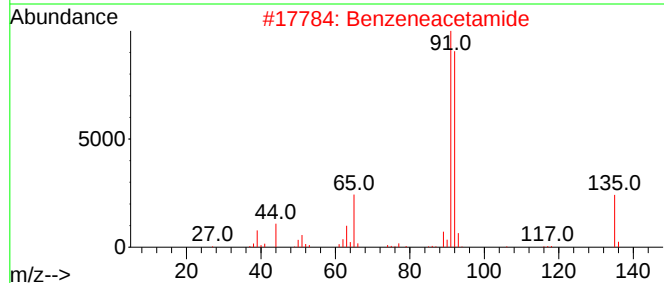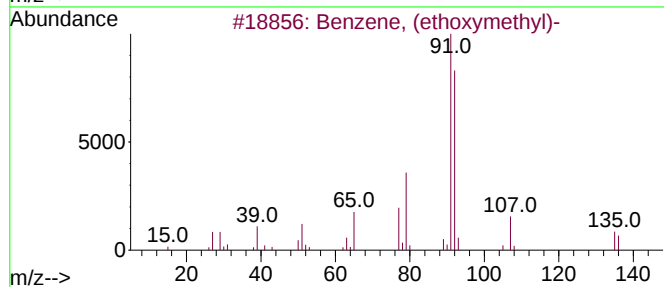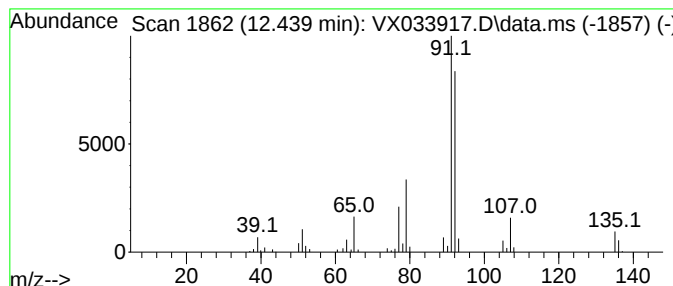

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012623\
Data File : VX033917.D
Acq On : 26 Jan 2023 18:15
Operator : JC/MD
Sample : 01320-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP-0126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, (ethox...	12.439	5.1	ug/l	57509	4	12.024	567045	50.0