
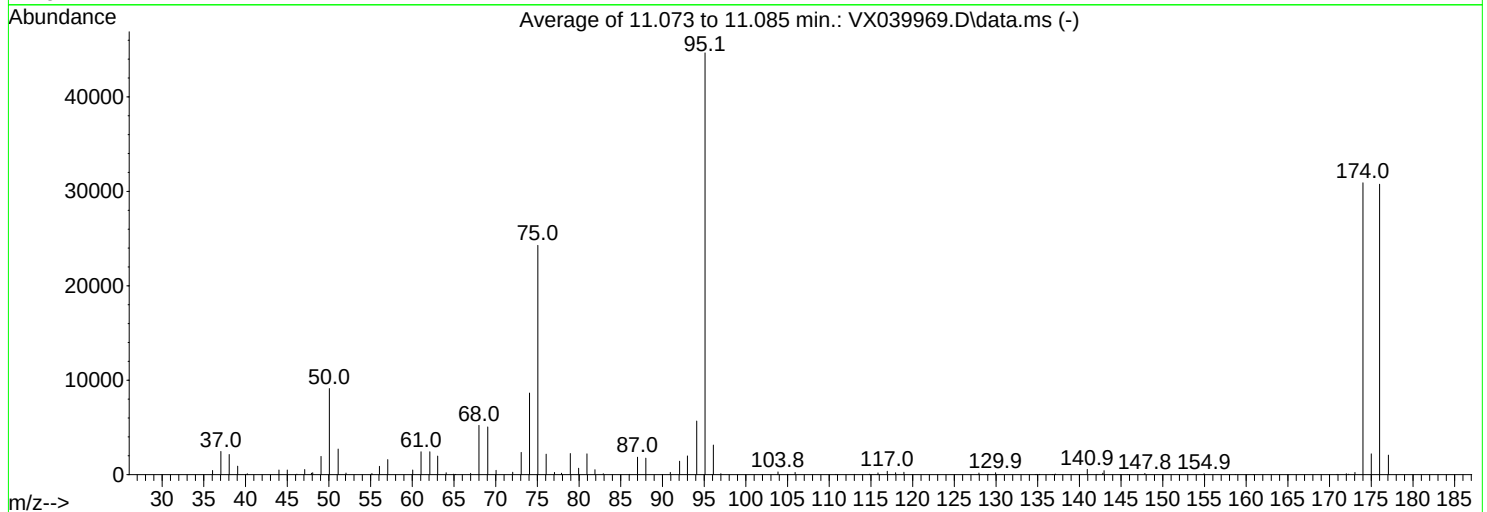


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012624\
Data File : VX039969.D
Acq On : 26 Jan 2024 08:26
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011024W.M
Title : SW846 8260
Last Update : Thu Jan 11 03:51:26 2024

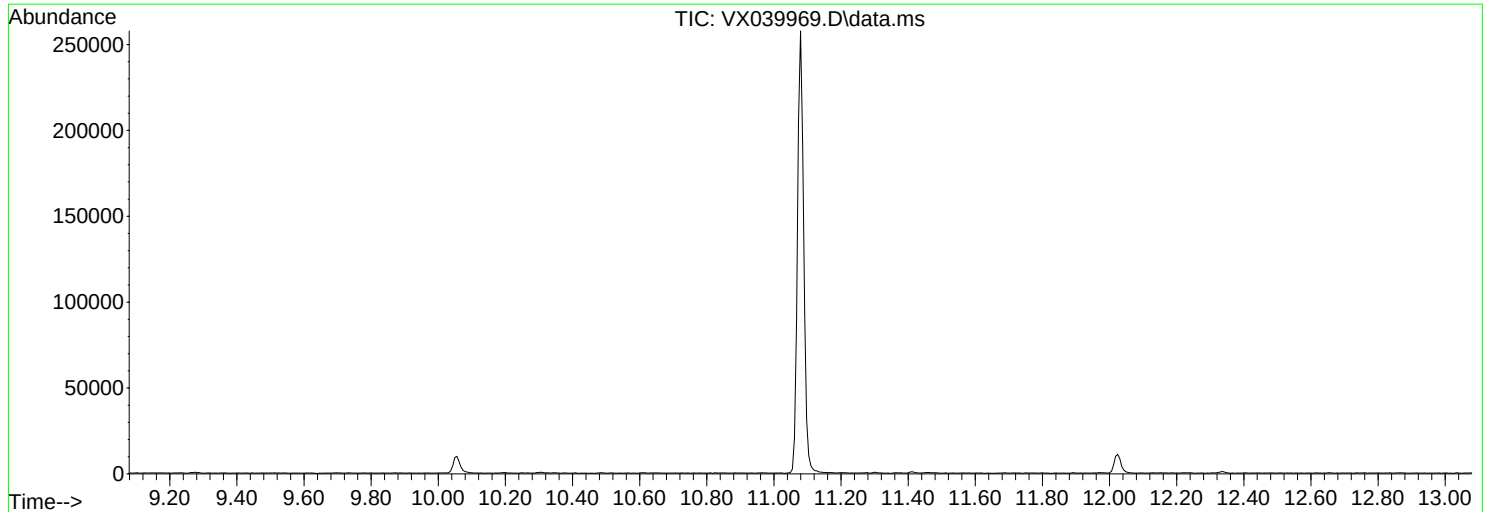

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	9123	PASS
75	95	30	60	54.4	24285	PASS
95	95	100	100	100.0	44669	PASS
96	95	5	9	7.0	3131	PASS
173	174	0.00	2	0.8	236	PASS
174	95	50	100	69.2	30901	PASS
175	174	5	9	7.1	2200	PASS
176	174	95	101	99.5	30755	PASS
177	176	5	9	6.7	2064	PASS