

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012720\
 Data File : VX014731.D
 Acq On : 27 Jan 2020 17:04
 Operator : JC/SP
 Sample : L1245-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 20200066-AMENDED-COMP-4

Quant Time: Jan 28 05:51:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 22 12:35:15 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	437720	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	692699	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	631463	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	295800	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	254957	49.88	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.76%	
35) Dibromofluoromethane	5.49	113	131274	30.03	ug/l	0.00
Spiked Amount 50.000			Recovery	=	60.06%	
50) Toluene-d8	8.71	98	825665	49.14	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.28%	
62) 4-Bromofluorobenzene	11.13	95	283610	47.38	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.76%	
Target Compounds						
16) Acetone	2.43	43	55700	20.021	ug/l	97
20) Methylene Chloride	2.85	84	14278	2.754	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012720\
Data File : VX014731.D
Acq On : 27 Jan 2020 17:04
Operator : JC/SP
Sample : L1245-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20200066-AMENDED-COMP-4

Quant Time: Jan 28 05:51:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 22 12:35:15 2020
Response via : Initial Calibration

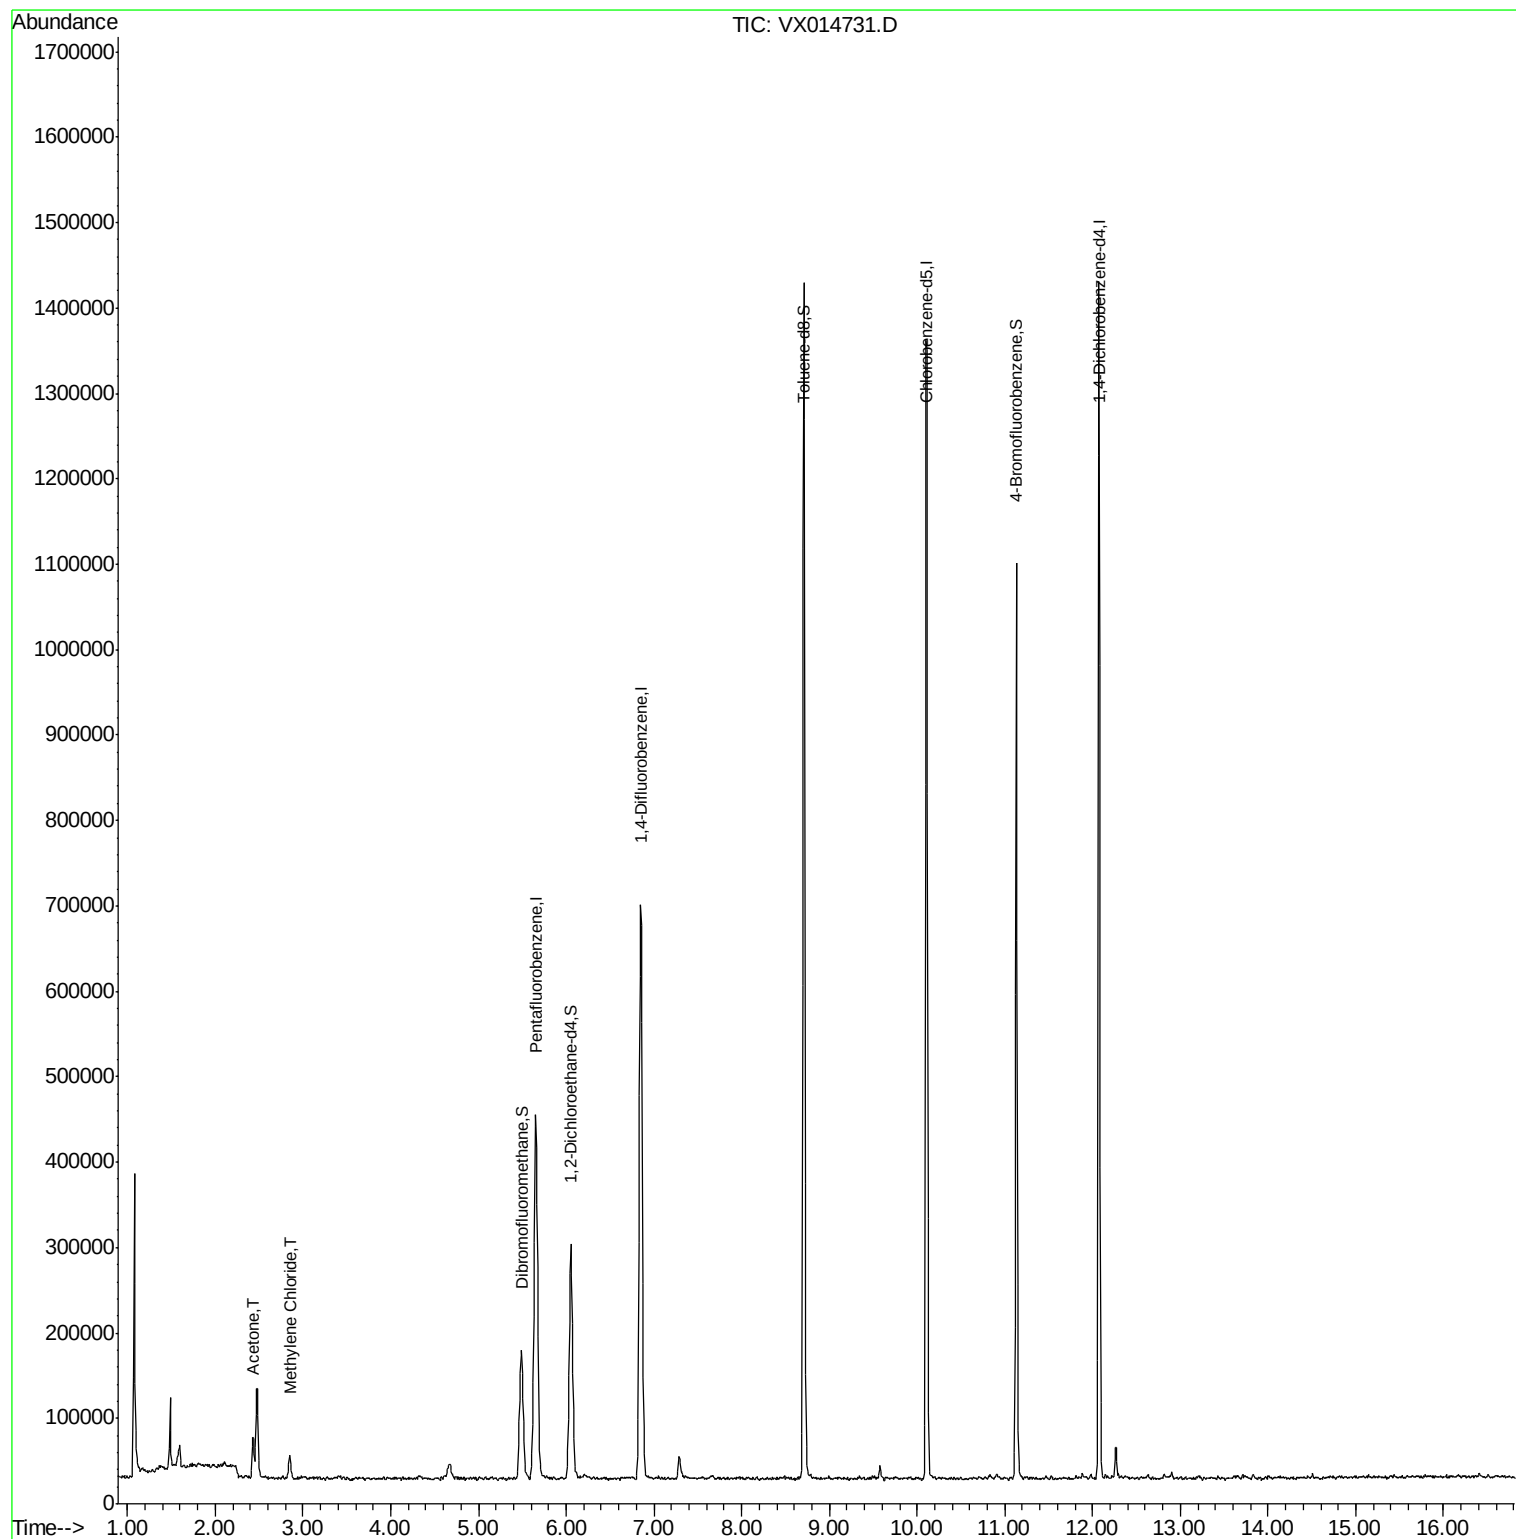

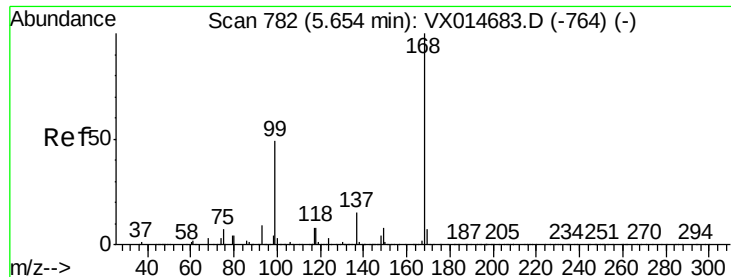

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 782

Delta R.T. 0.00 min

Lab File: VX014731.D

Acq: 27 Jan 2020 17:04

Instrument :

MSVOA_X

ClientSampleId :


20200066-AMENDED-COMP-4

Tot Ion:168 Resp: 437720

Ion Ratio Lower Upper

168 100

99 53.4 39.8 59.6

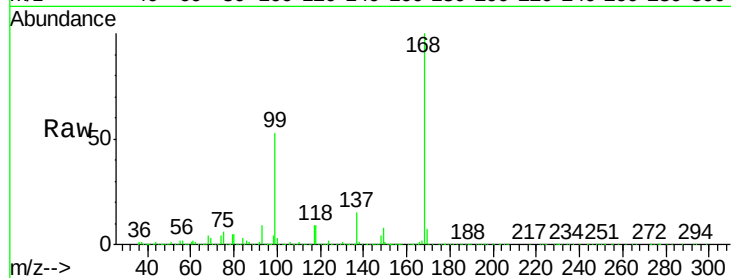

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

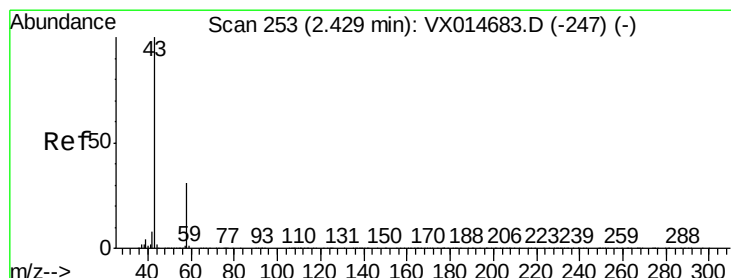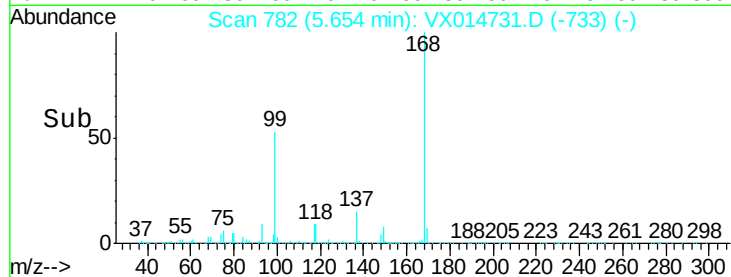

#16

Acetone

Concen: 20.021 ug/l

RT: 2.43 min Scan# 253

Delta R.T. 0.00 min

Lab File: VX014731.D


Acq: 27 Jan 2020 17:04

Tgt Ion: 43 Resp: 55700

Ion Ratio Lower Upper

43 100

58 29.1 24.5 36.7

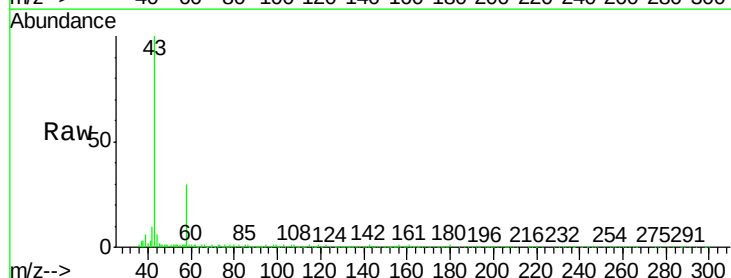

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.43

30000


20000


10000

0

Time-->

2.35 2.40 2.45 2.50




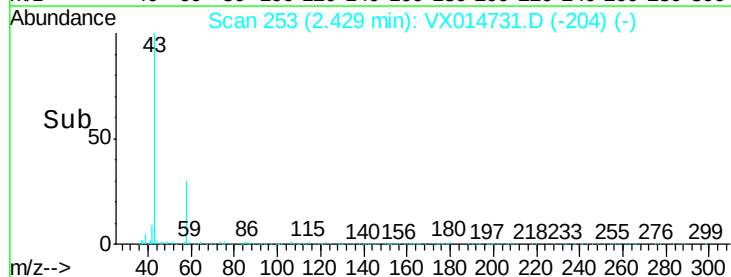


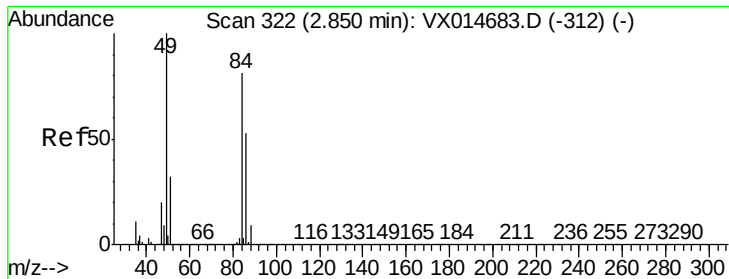

#20
Methylene Chloride
Concen: 2.754 ug/l
RT: 2.85 min Scan# 322
Delta R.T. 0.00 min
Lab File: VX014731.D
Acq: 27 Jan 2020 17:04




Instrument :
MSVOA_X
ClientSampleId :
20200066-AMENDED-COMP-4


Tot Ion:	84	Resp:	14278
Ion	Ratio	Lower	Upper
84	100		
49	122.3	98.2	147.4
51	36.5	31.3	46.9
86	60.9	51.8	77.6

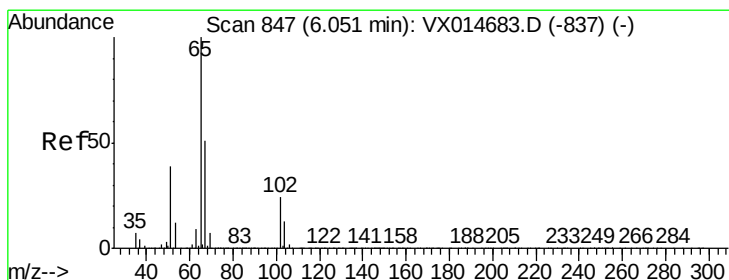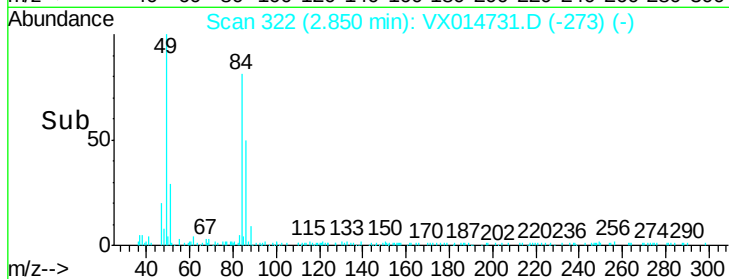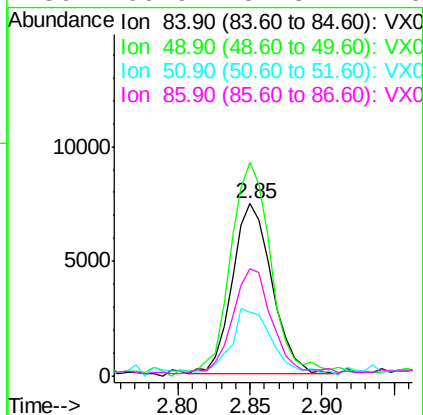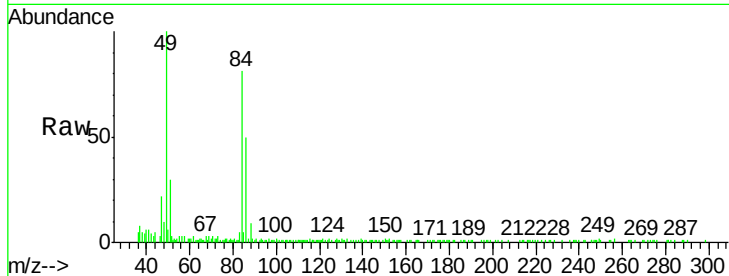

#33
1,2-Dichloroethane-d4
Concen: 49.879 ug/l
RT: 6.05 min Scan# 847
Delta R.T. 0.00 min
Lab File: VX014731.D
Acq: 27 Jan 2020 17:04

Tgt Ion:	65	Resp:	254957
Ion	Ratio	Lower	Upper
65	100		
67	52.9	0.0	107.4

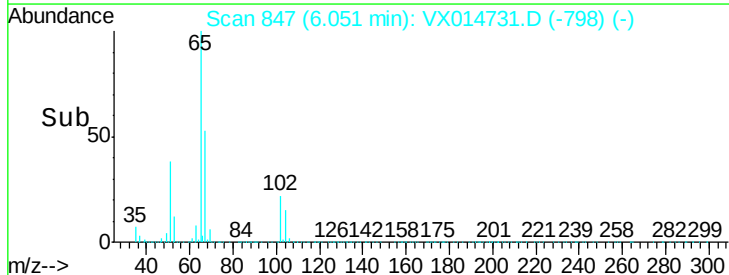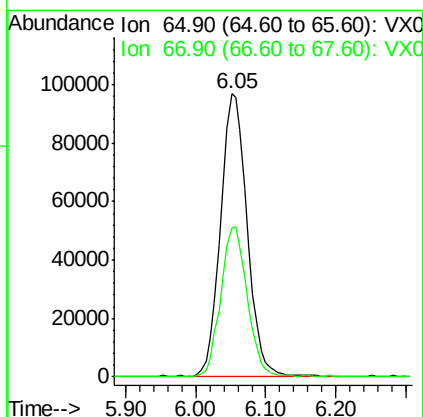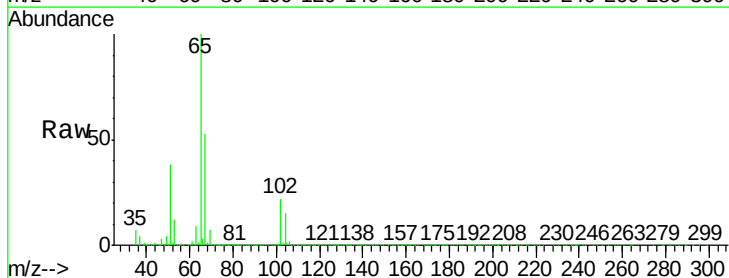

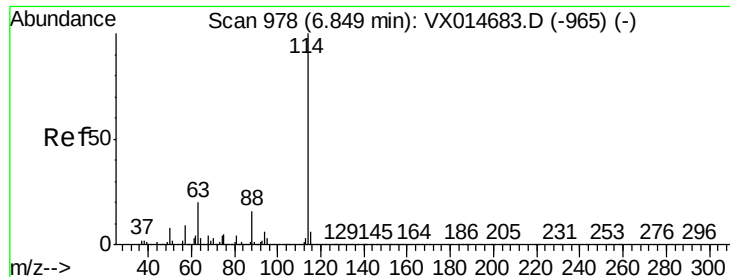

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. 0.00 min

Lab File: VX014731.D

Acq: 27 Jan 2020 17:04

Instrument :

MSVOA_X

ClientSampleId :

20200066-AMENDED-COMP-4


Tot Ion:114 Resp: 692699

Ion Ratio Lower Upper

114 100

63 20.5 0.0 40.6




88 15.3 0.0 31.2

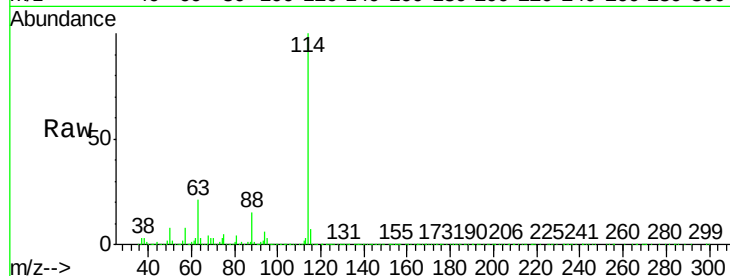

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

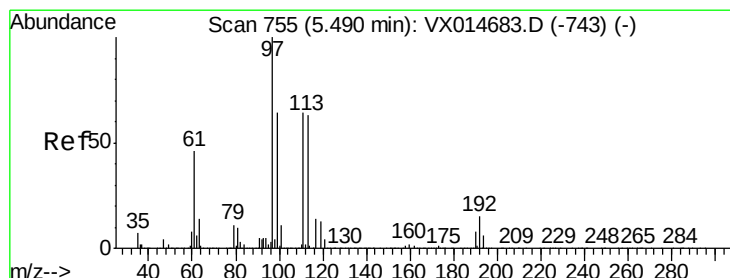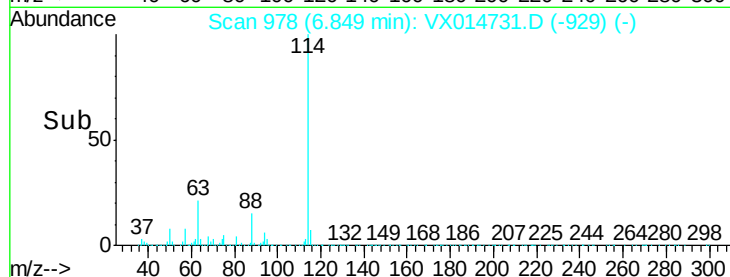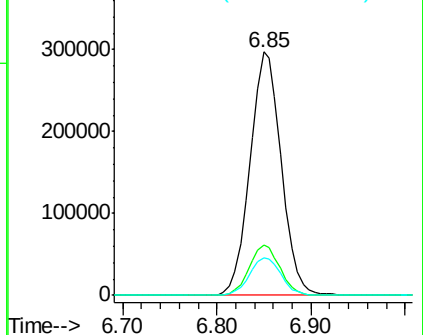

#35

Dibromofluoromethane

Concen: 30.034 ug/l

RT: 5.49 min Scan# 755

Delta R.T. 0.00 min

Lab File: VX014731.D

Acq: 27 Jan 2020 17:04


Tgt Ion:113 Resp: 131274

Ion Ratio Lower Upper

113 100

111 103.1 80.7 121.1



192 23.8 18.5 27.7

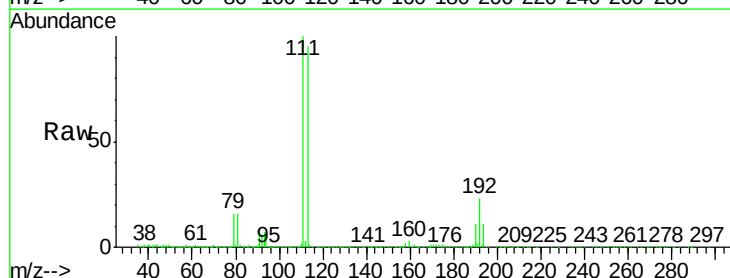


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

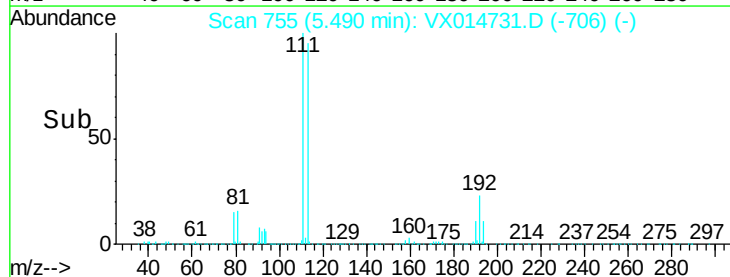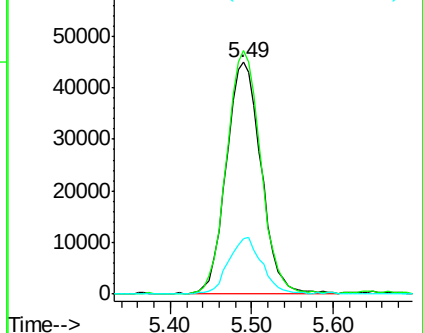

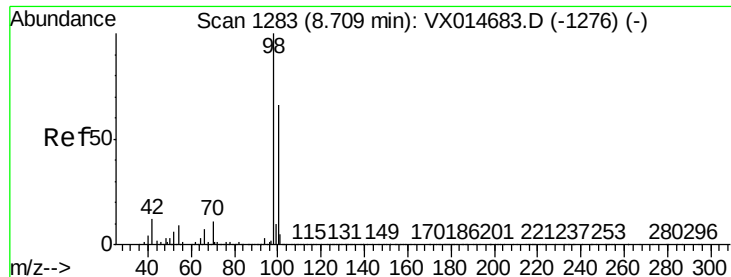

#50

Toluene-d8

Concen: 49.137 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. 0.00 min

Lab File: VX014731.D

Acq: 27 Jan 2020 17:04

Instrument :

MSVOA_X

ClientSampleId :





20200066-AMENDED-COMP-4

Tot Ion: 98 Resp: 825665

Ion Ratio Lower Upper

98 100

100 65.7 53.0 79.6

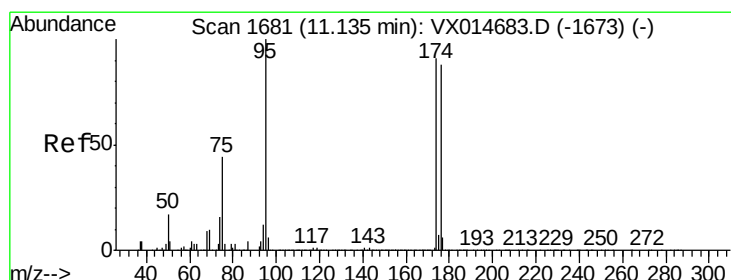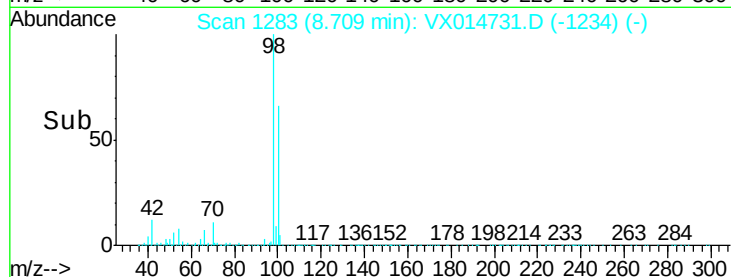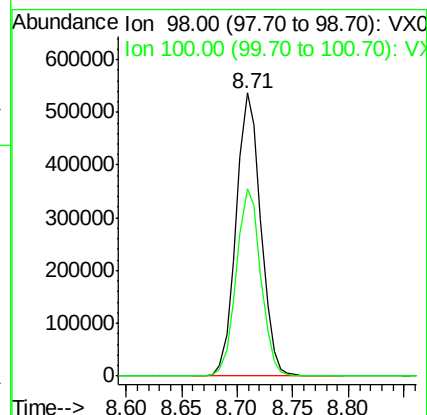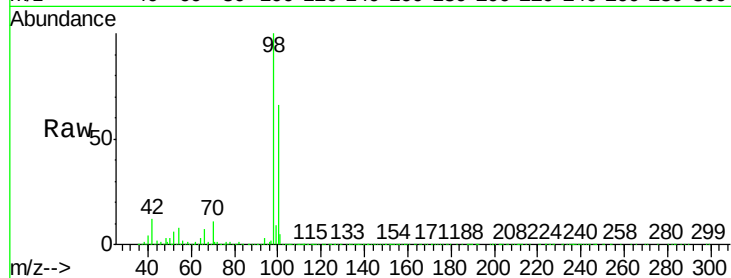

#62

4-Bromofluorobenzene

Concen: 47.381 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.01 min

Lab File: VX014731.D

Acq: 27 Jan 2020 17:04




Tgt Ion: 95 Resp: 283610


Ion Ratio Lower Upper

95 100

174 89.2 0.0 176.0

176 85.3 0.0 172.2


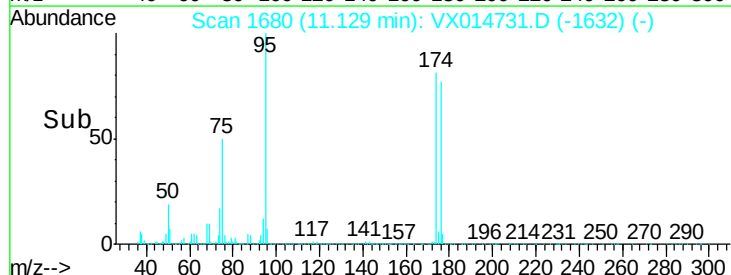
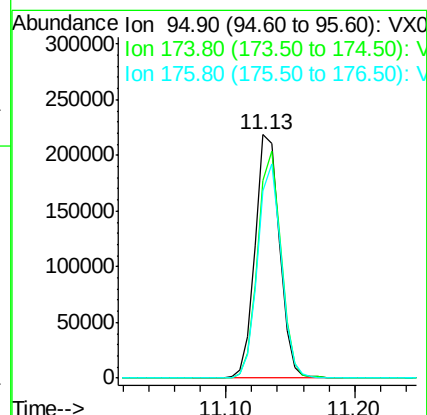
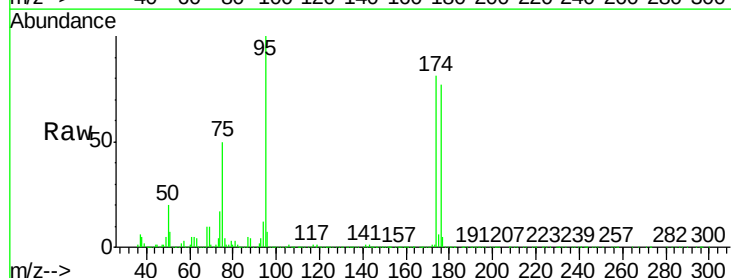


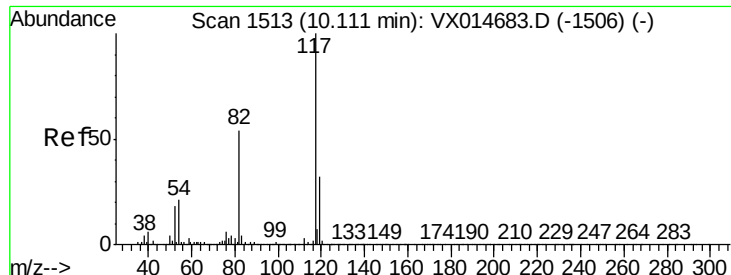

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. 0.00 min
Lab File: VX014731.D
Acq: 27 Jan 2020 17:04

Instrument :
MSVOA_X
ClientSampleId :
20200066-AMENDED-COMP-4

Tot Ion	Ratio	Lower	Upper
117	100		
82	52.5	43.2	64.8
119	32.5	25.8	38.6

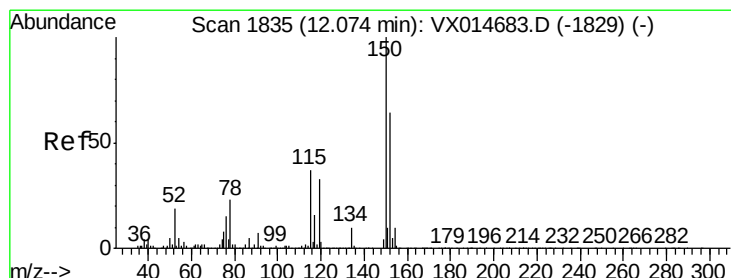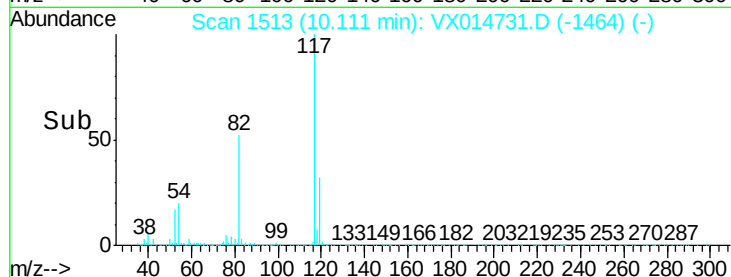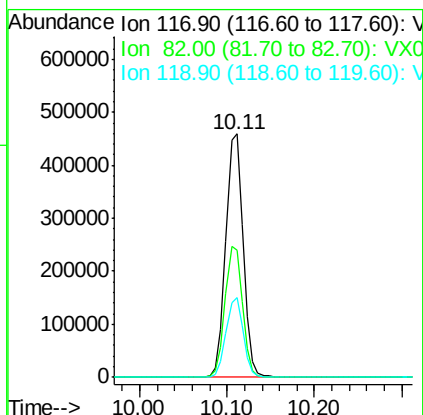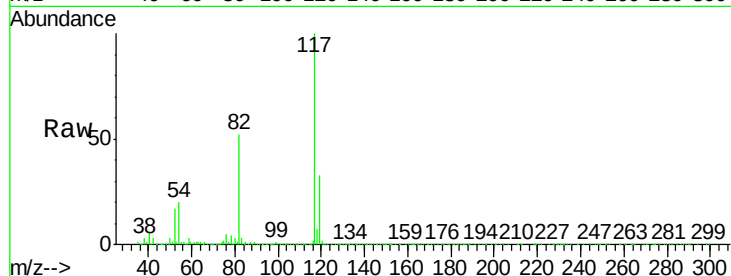

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX014731.D
Acq: 27 Jan 2020 17:04

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.4	39.4	118.1
150	156.7	0.0	351.2

