

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX012720\
 Data File : VX014720.D
 Acq On : 27 Jan 2020 12:48
 Operator : JC/SP
 Sample : L1264-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CTY-GW-01-12

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	41	rBV	1485900	1758890	80.29%	12.770%
2	1.168	43	46	51	rVB2	19051	22648	1.03%	0.164%
3	1.265	59	62	65	rBV	21621	28825	1.32%	0.209%
4	1.607	109	118	119	rBV8	33216	74465	3.40%	0.541%
5	2.430	247	253	259	rBV	24773	39982	1.83%	0.290%
6	4.667	614	620	626	rBV8	7981	24065	1.10%	0.175%
7	5.490	744	755	766	rBV	252081	715818	32.68%	5.197%
8	5.649	771	781	795	rVB	435634	1215831	55.50%	8.827%
9	6.051	837	847	855	rBV	279637	734383	33.52%	5.332%
10	6.136	855	861	869	rVB2	44123	118432	5.41%	0.860%
11	6.849	969	978	991	rBV	681487	1587957	72.49%	11.529%
12	7.453	1071	1077	1082	rBV10	8477	21977	1.00%	0.160%
13	8.709	1277	1283	1291	rBV	1440972	2190609	100.00%	15.905%
14	10.105	1506	1512	1522	rBV	1403543	1893030	86.42%	13.744%
15	10.355	1549	1553	1560	rVB2	15748	23272	1.06%	0.169%
16	10.696	1605	1609	1617	rVB2	14968	24530	1.12%	0.178%
17	11.135	1675	1681	1692	rVB	1082397	1423367	64.98%	10.334%
18	12.074	1830	1835	1842	rBV	1391420	1732365	79.08%	12.578%
19	12.294	1868	1871	1877	rVB2	19332	26071	1.19%	0.189%
20	13.568	2075	2080	2083	rBV3	20445	29907	1.37%	0.217%
21	13.830	2118	2123	2129	rVB	70860	86916	3.97%	0.631%


Sum of corrected areas: 13773340

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012720\
Data File : VX014720.D
Acq On : 27 Jan 2020 12:48
Operator : JC/SP
Sample : L1264-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CTY-GW-01-12

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

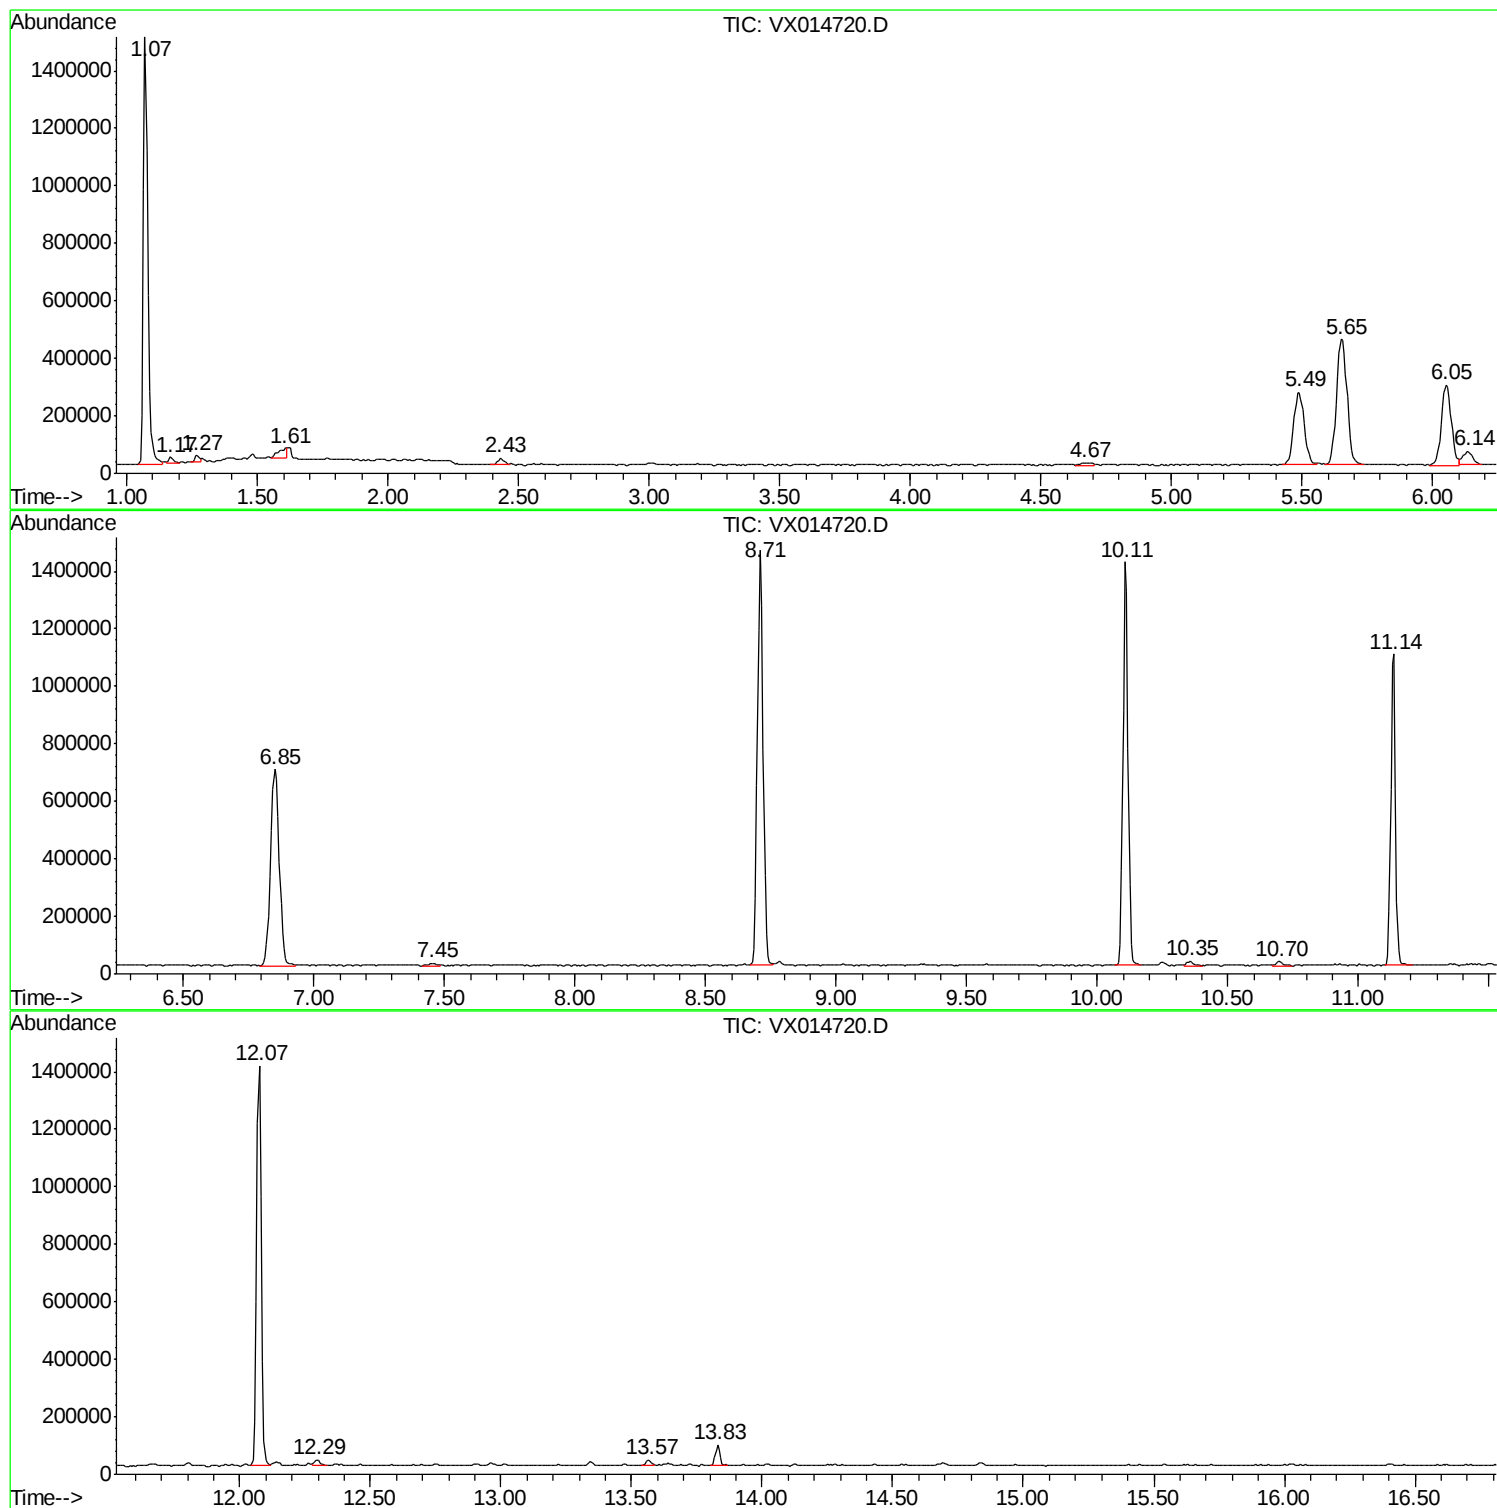

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX012720\
Data File : VX014720.D
Acq On : 27 Jan 2020 12:48
Operator : JC/SP
Sample : L1264-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CTY-GW-01-12

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX012720\
Data File : VX014720.D
Acq On : 27 Jan 2020 12:48
Operator : JC/SP
Sample : L1264-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CTY-GW-01-12

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc