

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012721\
 Data File : VX020775.D
 Acq On : 27 Jan 2021 17:14
 Operator : JC/SP
 Sample : M1189-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 28 00:45:24 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.629	168	319297	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	553780	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	514621	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	224953	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	215472	49.48	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.96%
35) Dibromofluoromethane	5.464	113	185370	48.87	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.74%
50) Toluene-d8	8.696	98	669422	48.14	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.28%
62) 4-Bromofluorobenzene	11.122	95	244152	45.21	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	90.42%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.435	85	19	1.20	ug/l #	42
10) Methyl Iodide	2.495	142	968	0.22	ug/l #	77
11) Tert butyl alcohol	3.001	59	10008	12.31	ug/l	95
13) Acrolein	2.270	56	206	0.34	ug/l #	1
16) Acetone	2.416	43	56015	33.92	ug/l	98
17) Carbon Disulfide	2.550	76	1365	1.04	ug/l #	75
18) Methyl Acetate	2.745	43	925	0.22	ug/l #	67
20) Methylene Chloride	2.831	84	2628	0.63	ug/l #	96
25) 2-Butanone	4.635	43	15857	6.13	ug/l	91
29) Tetrahydrofuran	5.099	42	930	0.56	ug/l #	75
31) Cyclohexane	5.623	56	6882	1.18	ug/l #	6
36) 1,1-Dichloropropene	5.623	75	24090	4.33	ug/l #	49
37) Ethyl Acetate	4.635	43	15857	3.01	ug/l #	66
38) Carbon Tetrachloride	5.629	117	32931	5.64	ug/l #	17
49) 1,4-Dioxane	7.732	88	43	0.43	ug/l #	1
51) 4-Methyl-2-Pentanone	8.616	43	2147	0.40	ug/l	87
52) Toluene	8.763	92	2134	0.21	ug/l	82
59) 2-Hexanone	9.470	43	2012	0.51	ug/l	77
67) Ethyl Benzene	10.232	91	10351	0.54	ug/l	98
68) m/p-Xylenes	10.342	106	17754	2.47	ug/l	100
69) o-Xylene	10.683	106	13135	1.94	ug/l	93
74) N-amyl acetate	10.866	43	70	2.02	ug/l #	40
76) 1,2,3-Trichloropropane	11.116	75	118377	22.69	ug/l #	39
78) n-propylbenzene	11.341	91	7416	0.40	ug/l	98
79) 2-Chlorotoluene	11.421	91	5698	0.50	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.488	105	16402	1.18	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.116	75	118377	63.58	ug/l #	12
83) tert-Butylbenzene	12.006	119	2718	0.20	ug/l	71
84) 1,2,4-Trimethylbenzene	11.793	105	66397	4.74	ug/l	99
85) sec-Butylbenzene	11.793	105	66397	4.28	ug/l #	57
89) n-Butylbenzene	12.360	91	4521	0.35	ug/l #	31
90) Hexachloroethane	12.567	117	1249	0.48	ug/l #	9
95) Naphthalene	13.817	128	31088	4.57	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 28 00:45:24 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration








#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Instrument :
MSVOA_X
ClientSampleId :



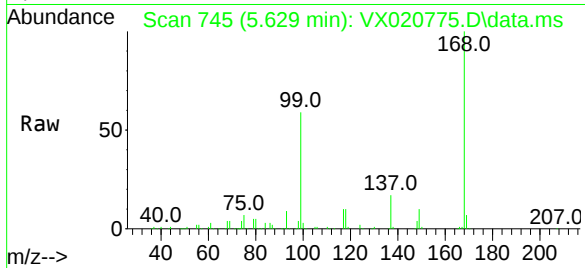



Tgt Ion:168 Resp: 319297
Ion Ratio Lower Upper
168 100
99 59.0 45.8 68.6

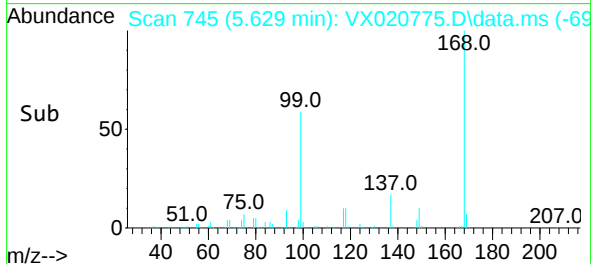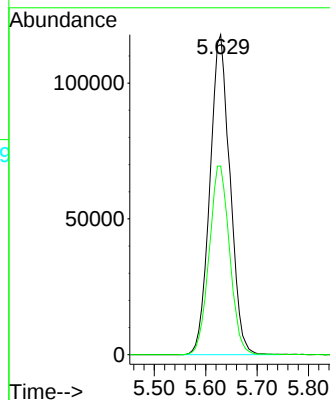

#2
Dichlorodifluoromethane
Concen: 1.20 ug/l
RT: 1.435 min Scan# 57
Delta R.T. 0.250 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14


Tgt Ion: 85 Resp: 19
Ion Ratio Lower Upper
85 100
87 0.0 16.4 49.2#

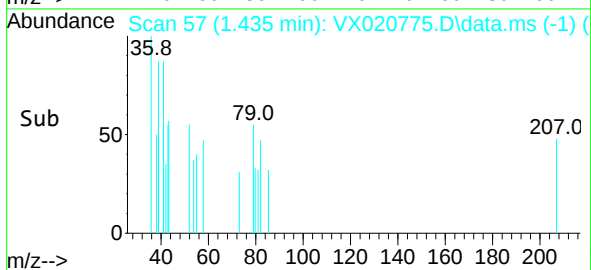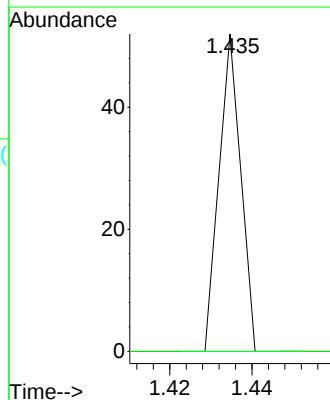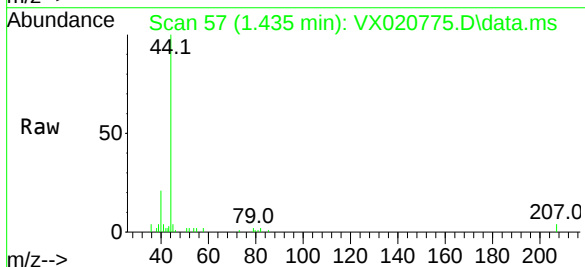



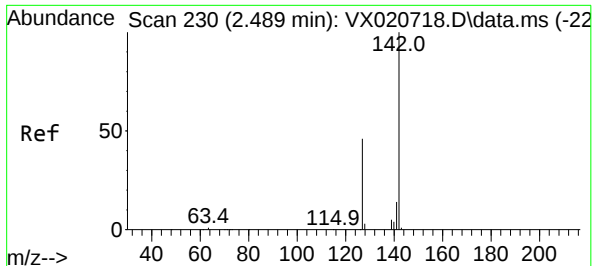


#10
Methyl Iodide
Concen: 0.22 ug/l
RT: 2.495 min Scan# 231
Delta R.T. 0.006 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14


Instrument :
MSVOA_X
ClientSampled :

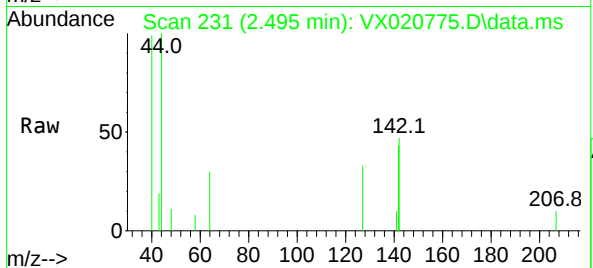



Tgt Ion:142 Resp: 968
Ion Ratio Lower Upper
142 100
127 57.4 33.3 49.9#
141 7.6 11.4 17.0#

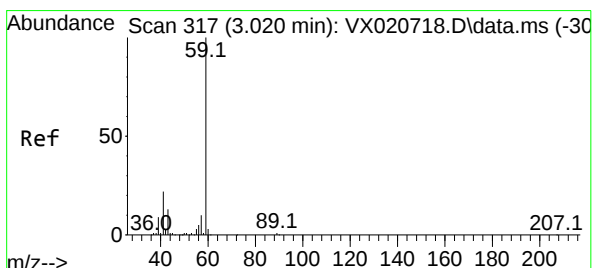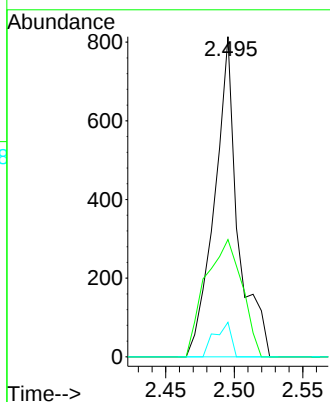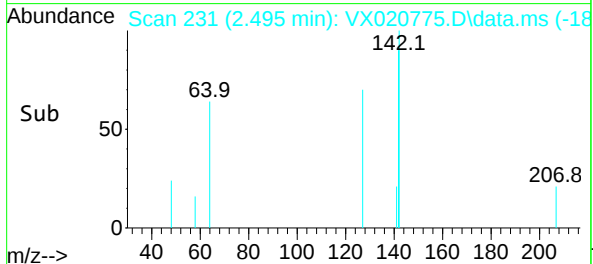


#11
Tert butyl alcohol
Concen: 12.31 ug/l
RT: 3.001 min Scan# 314
Delta R.T. -0.019 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

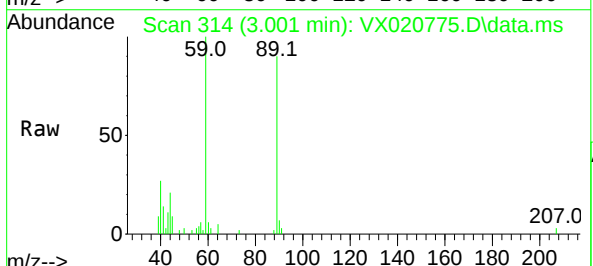

Tgt Ion: 59 Resp: 10008
Ion Ratio Lower Upper
59 100
57 7.9 7.8 11.8



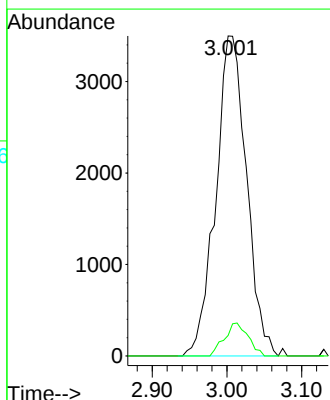
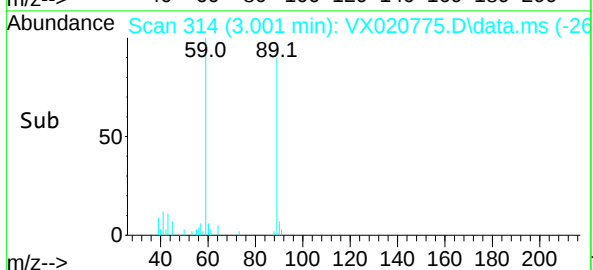


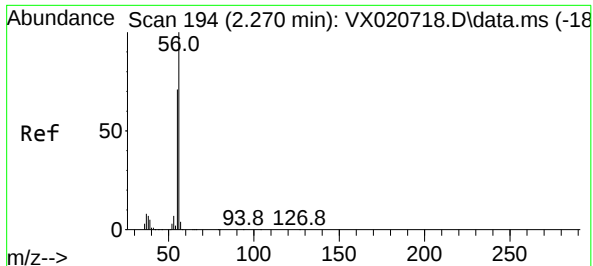

#13
Acrolein
Concen: 0.34 ug/l
RT: 2.270 min Scan# 194
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 56 Resp: 206
Ion Ratio Lower Upper
56 100
55 261.2 56.4 84.6#

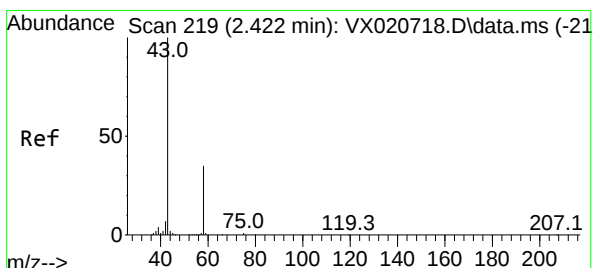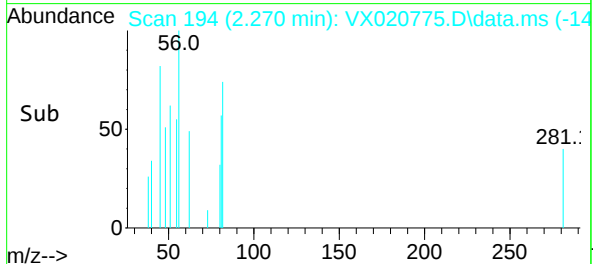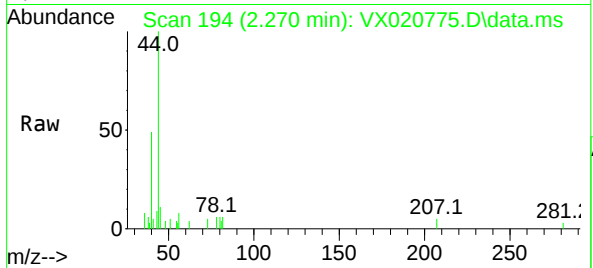

#16
Acetone
Concen: 33.92 ug/l
RT: 2.416 min Scan# 218
Delta R.T. -0.006 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 43 Resp: 56015
Ion Ratio Lower Upper
43 100
58 36.2 27.8 41.8


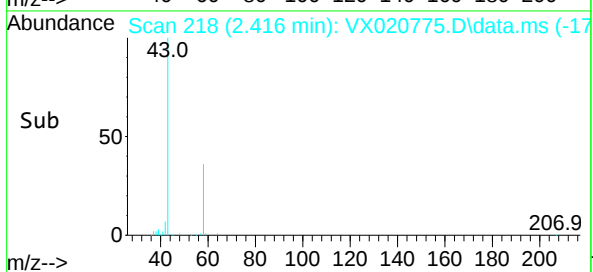

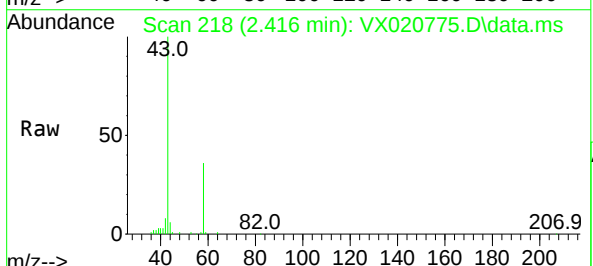


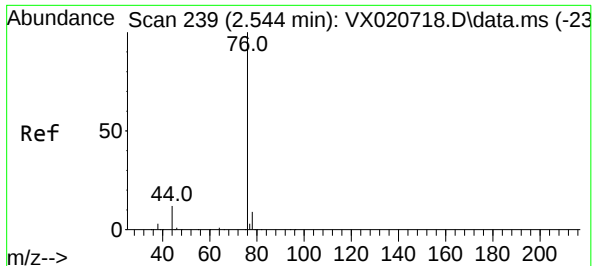

#17
Carbon Disulfide
Concen: 1.04 ug/l
RT: 2.550 min Scan# 240
Delta R.T. 0.006 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 76 Resp: 1365
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

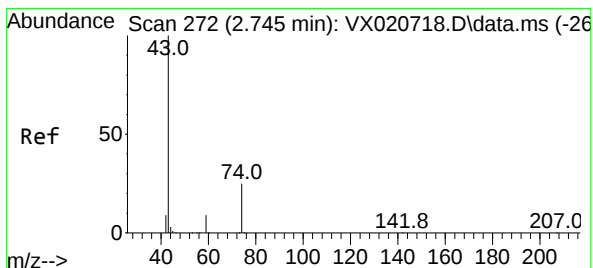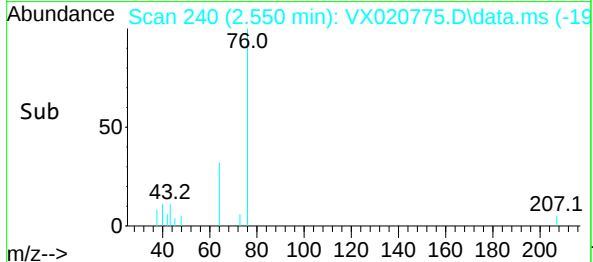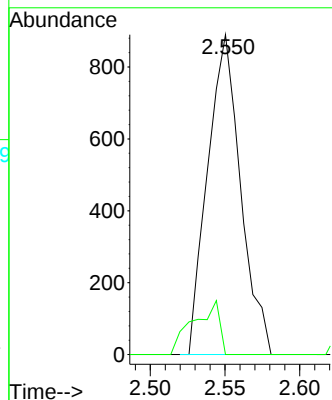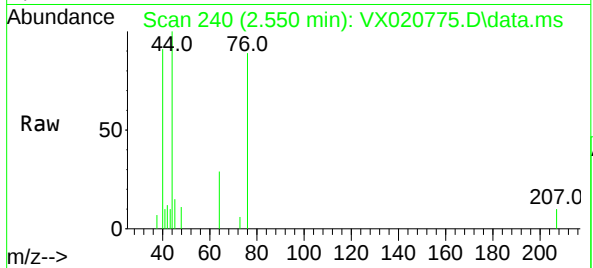

#18
Methyl Acetate
Concen: 0.22 ug/l
RT: 2.745 min Scan# 272
Delta R.T. 0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14


Tgt Ion: 43 Resp: 925
Ion Ratio Lower Upper
43 100
74 10.4 21.9 32.9#

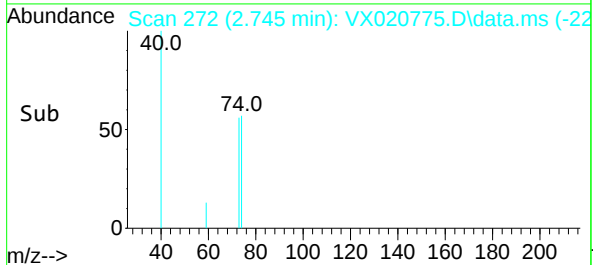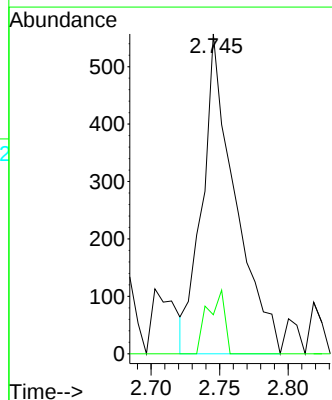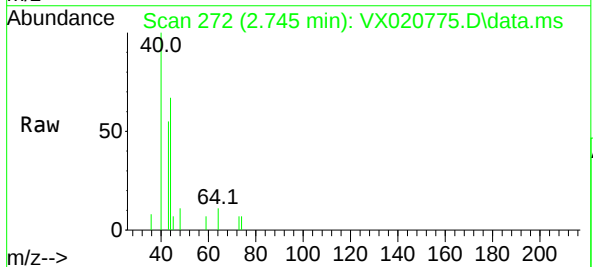






#20
Methylene Chloride
Concen: 0.63 ug/l
RT: 2.831 min Scan# 286
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion: 84 Resp: 2628




Ion	Ratio	Lower	Upper
84	100		
49	111.1	88.6	132.8
51	40.8	27.0	40.6#
86	67.5	50.3	75.5

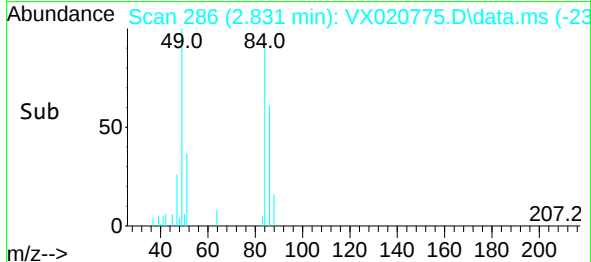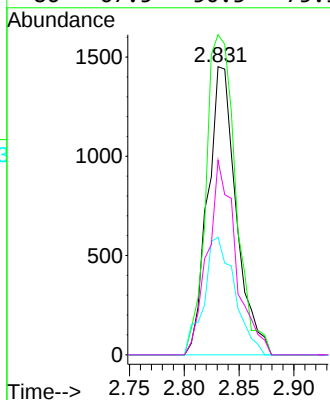


#25
2-Butanone
Concen: 6.13 ug/l
RT: 4.635 min Scan# 582
Delta R.T. 0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 43 Resp: 15857

Ion	Ratio	Lower	Upper
43	100		
72	25.0	23.7	35.5

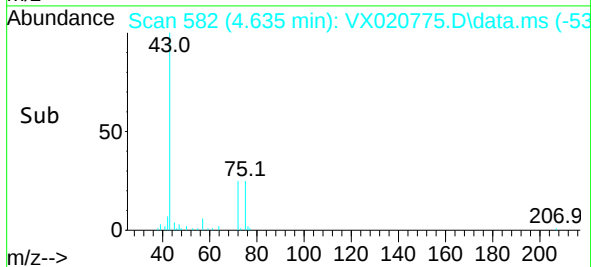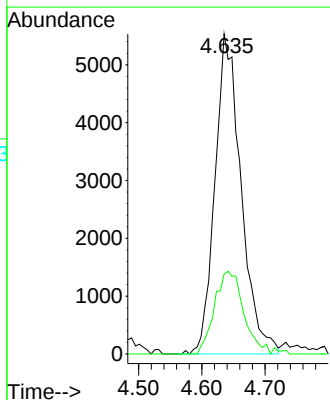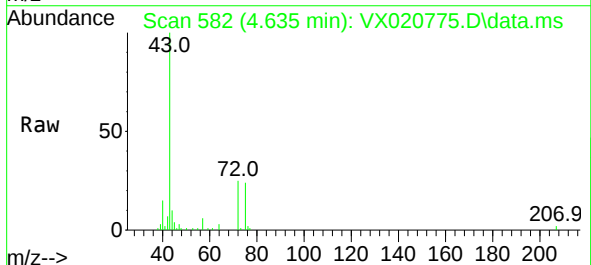

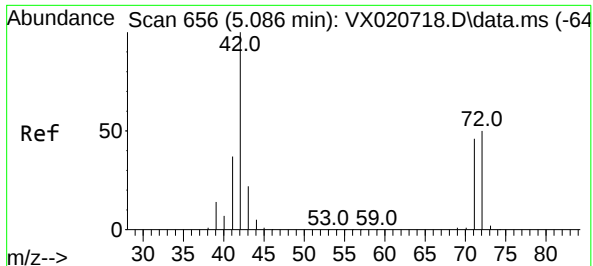

#29

Tetrahydrofuran

Concen: 0.56 ug/l

RT: 5.099 min Scan# 658





Delta R.T. 0.013 min

Lab File: VX020775.D

Acq: 27 Jan 2021 17:14

Tgt Ion:	42	Resp:	930
Ion	Ratio	Lower	Upper
42	100		
72	34.8	41.7	62.5#
71	31.3	38.4	57.6#

Instrument :
MSVOA_X
ClientSampled :

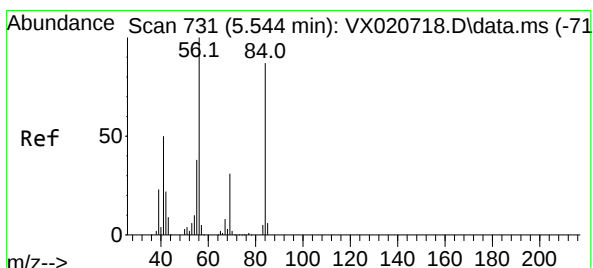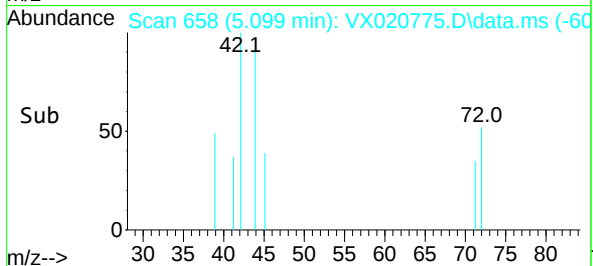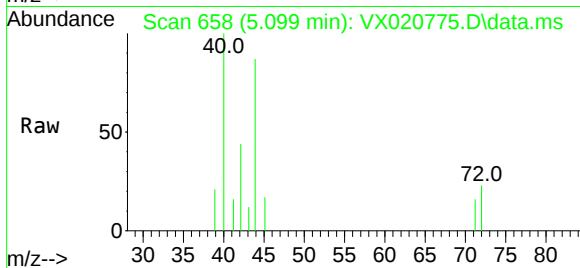

#31

Cyclohexane

Concen: 1.18 ug/l




RT: 5.623 min Scan# 744


Delta R.T. 0.079 min

Lab File: VX020775.D

Acq: 27 Jan 2021 17:14

Tgt Ion:	56	Resp:	6882
Ion	Ratio	Lower	Upper
56	100		
69	160.3	25.3	37.9#
84	131.6	71.4	107.0#

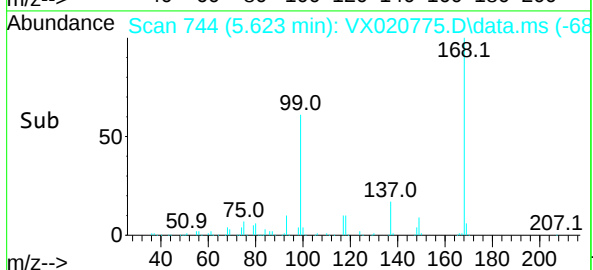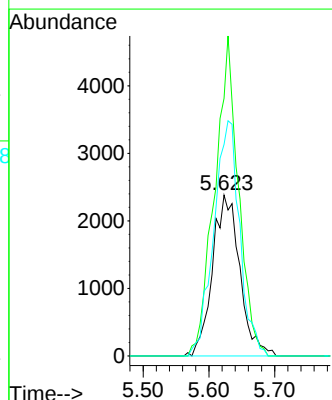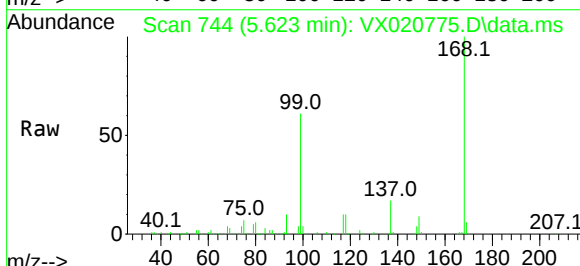



#33

1,2-Dichloroethane-d4

Concen: 49.48 ug/l

RT: 6.031 min Scan# 811

Delta R.T. 0.006 min

Lab File: VX020775.D





Acq: 27 Jan 2021 17:14

Tgt Ion: 65 Resp: 215472

Ion Ratio Lower Upper

65 100

67 52.6 0.0 105.4

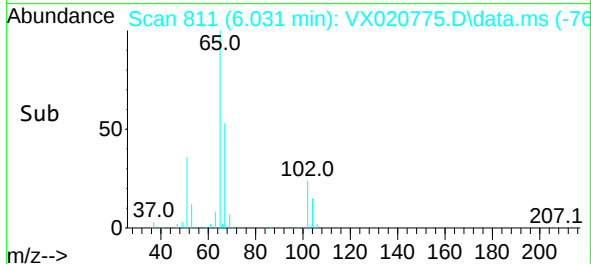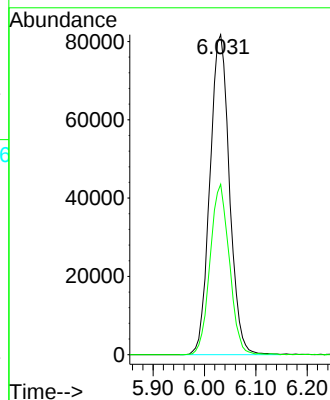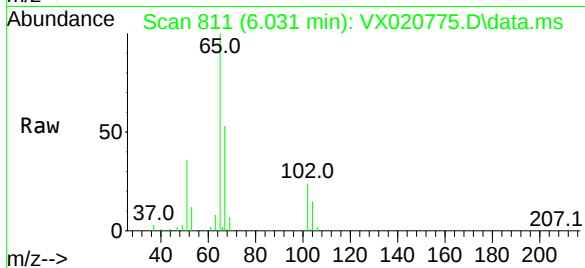

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.830 min Scan# 942

Delta R.T. 0.000 min

Lab File: VX020775.D

Acq: 27 Jan 2021 17:14




Tgt Ion: 114 Resp: 553780


Ion Ratio Lower Upper

114 100

63 20.2 0.0 40.8


88 16.7 0.0 32.8

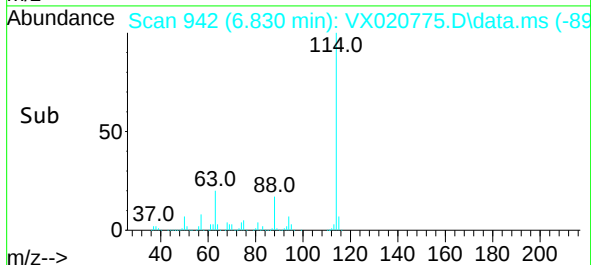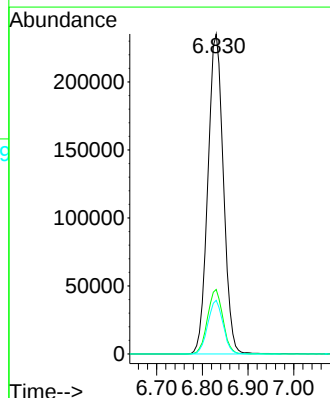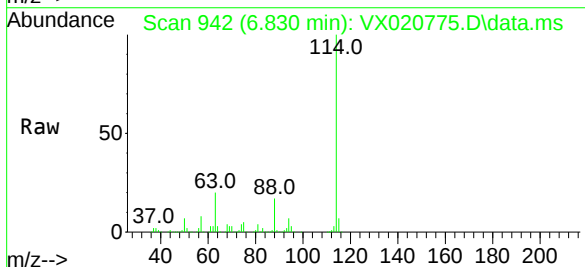






#35
Dibromofluoromethane
Concen: 48.87 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14


Instrument :
MSVOA_X
ClientSampleId :

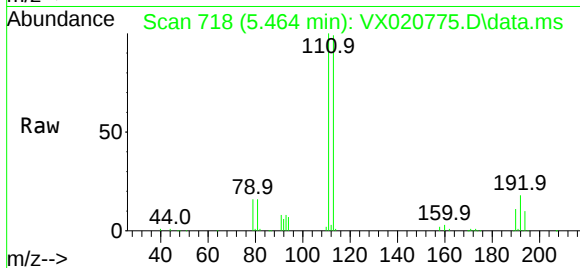



Tgt Ion:113 Resp: 185370
Ion Ratio Lower Upper
113 100
111 102.5 81.9 122.9
192 19.7 16.7 25.1




#36
1,1-Dichloropropene
Concen: 4.33 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.146 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

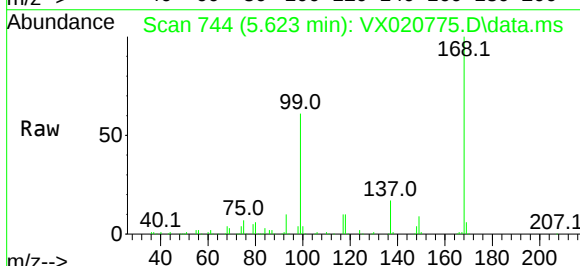

Tgt Ion: 75 Resp: 24090
Ion Ratio Lower Upper
75 100
110 9.8 18.1 54.4#
77 0.0 25.3 37.9#

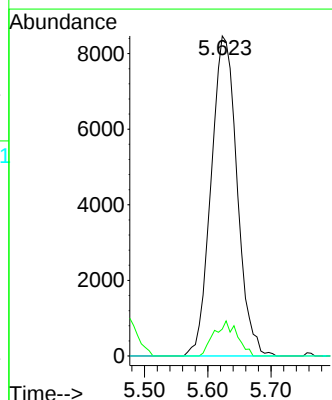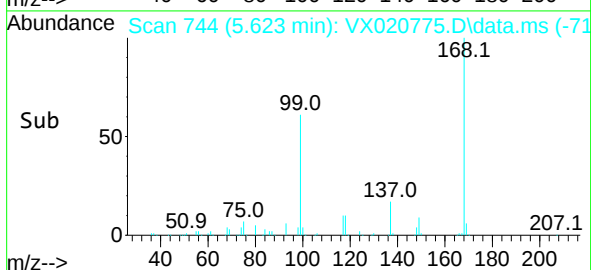



#37

Ethyl Acetate


Concen: 3.01 ug/l

RT: 4.635 min Scan# 582




Delta R.T. -0.159 min

Lab File: VX020775.D

Acq: 27 Jan 2021 17:14



Tgt Ion:	43	Resp:	15857
Ion	Ratio	Lower	Upper
43	100		
61	1.1	12.8	19.2#
70	0.0	10.5	15.7#

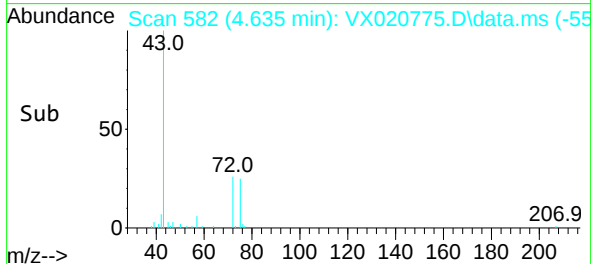

#38

Carbon Tetrachloride


Concen: 5.64 ug/l

RT: 5.629 min Scan# 745



Delta R.T. -0.122 min


Lab File: VX020775.D

Acq: 27 Jan 2021 17:14



Tgt Ion:	117	Resp:	32931
Ion	Ratio	Lower	Upper
117	100		
119	5.4	76.2	114.2#
121	0.0	24.8	37.2#



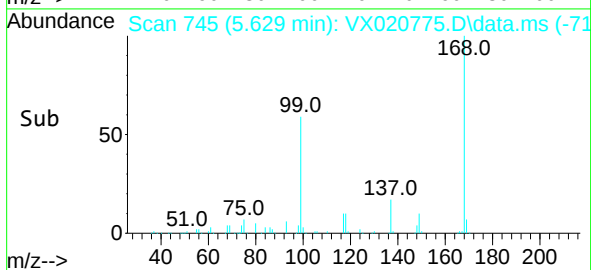





#49
1,4-Dioxane
Concen: 0.43 ug/l
RT: 7.732 min Scan# 1090
Delta R.T. 0.018 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 88 Resp: 43
Ion Ratio Lower Upper
88 100
43 581.4 23.2 34.8#
58 114.0 55.0 82.4#

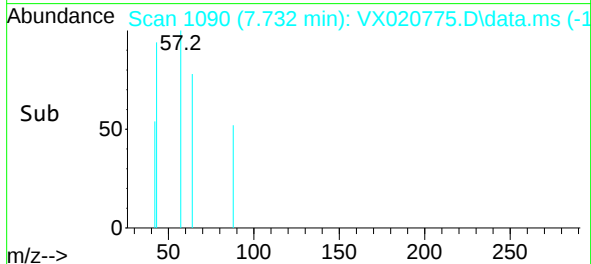

#50
Toluene-d8
Concen: 48.14 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 98 Resp: 669422
Ion Ratio Lower Upper
98 100
100 66.0 51.9 77.9


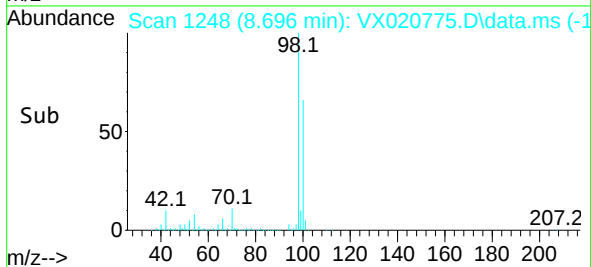

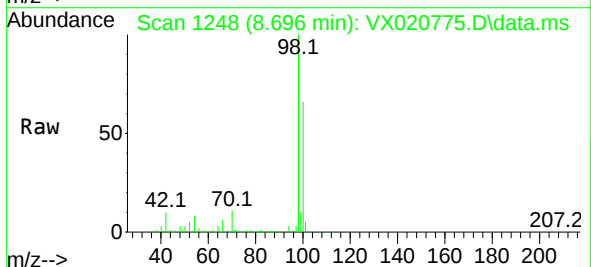




#51
4-Methyl-2-Pentanone
Concen: 0.40 ug/l
RT: 8.616 min Scan# 1235
Delta R.T. 0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 2147
Ion Ratio Lower Upper
43 100
58 36.1 35.4 53.0

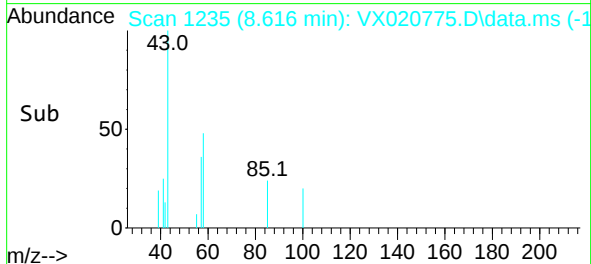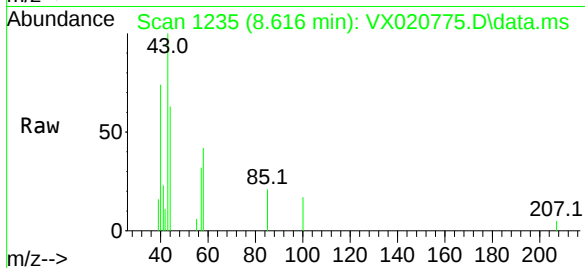

#52
Toluene
Concen: 0.21 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 92 Resp: 2134
Ion Ratio Lower Upper
92 100
91 196.3 137.1 205.7



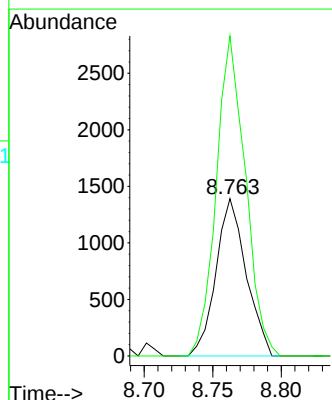
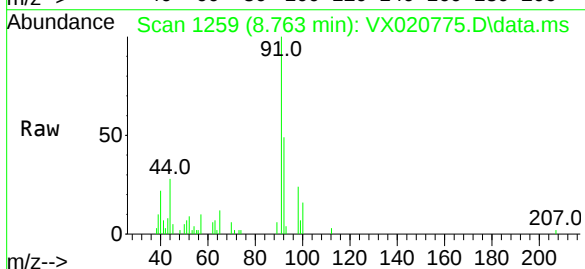




#59
2-Hexanone
Concen: 0.51 ug/l
RT: 9.470 min Scan# 1375
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 2012
Ion Ratio Lower Upper
43 100
58 44.3 30.9 92.8

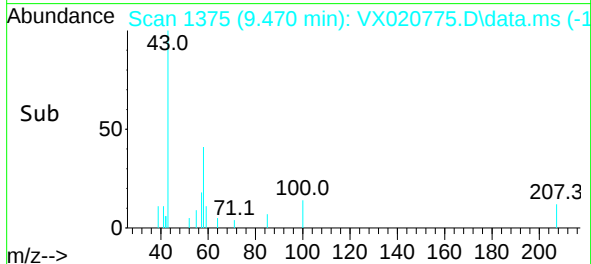

#62
4-Bromofluorobenzene
Concen: 45.21 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 95 Resp: 244152
Ion Ratio Lower Upper
95 100
174 77.6 0.0 154.6
176 75.7 0.0 155.8


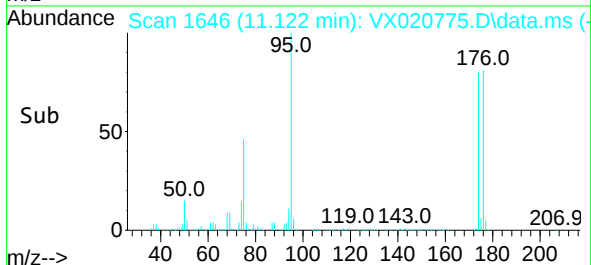
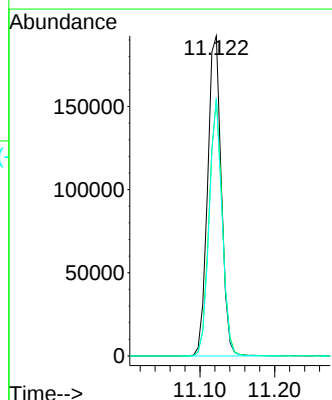
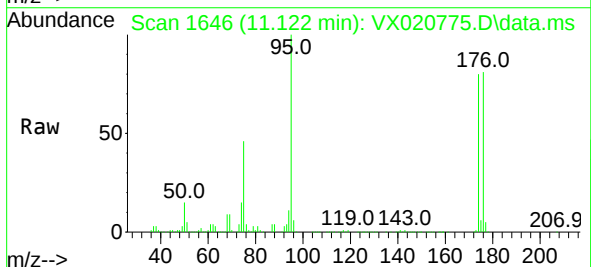




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 514621
Ion Ratio Lower Upper
117 100
82 55.9 47.4 71.2
119 32.0 26.6 39.8

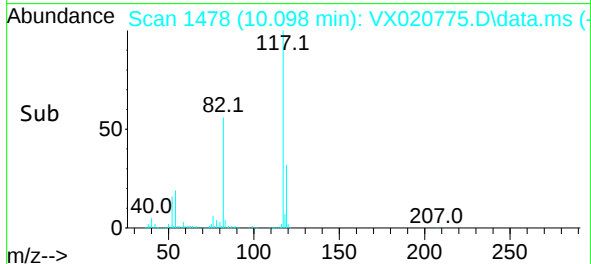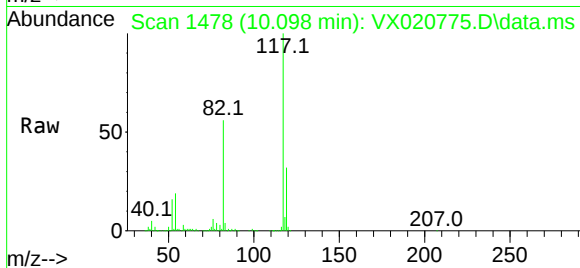

#67
Ethyl Benzene
Concen: 0.54 ug/l
RT: 10.232 min Scan# 1500
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 91 Resp: 10351
Ion Ratio Lower Upper
91 100
106 29.6 24.6 37.0


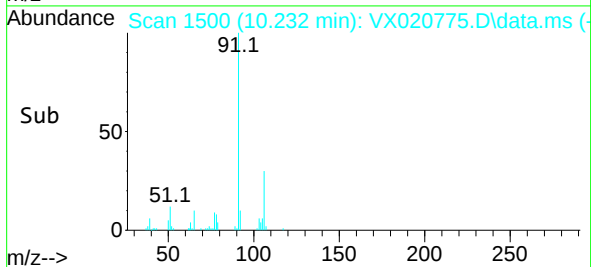

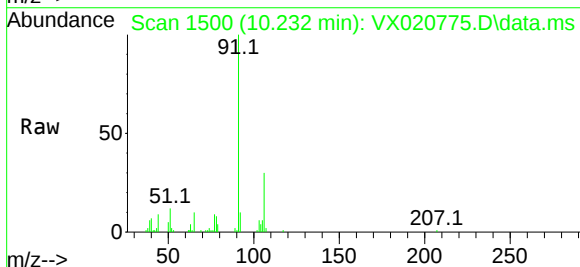




#68
m/p-Xylenes
Concen: 2.47 ug/l
RT: 10.342 min Scan# 1518
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 17754
Ion Ratio Lower Upper
106 100
91 203.2 162.8 244.2

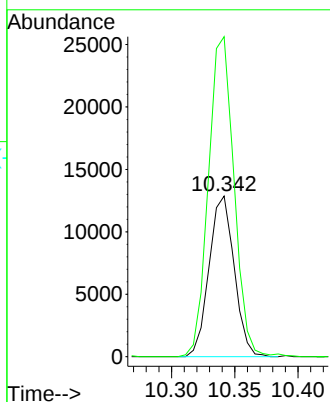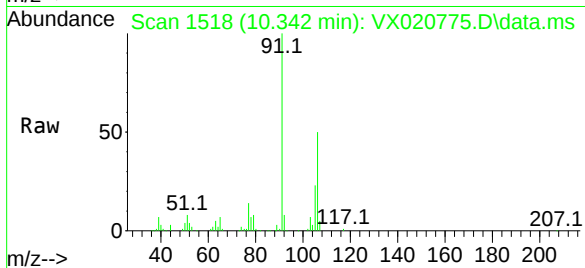

#69
o-Xylene
Concen: 1.94 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. 0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion:106 Resp: 13135
Ion Ratio Lower Upper
106 100
91 226.8 108.1 324.2


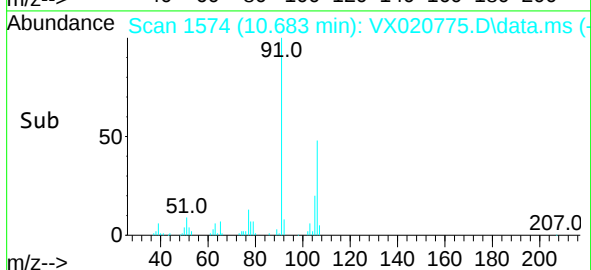
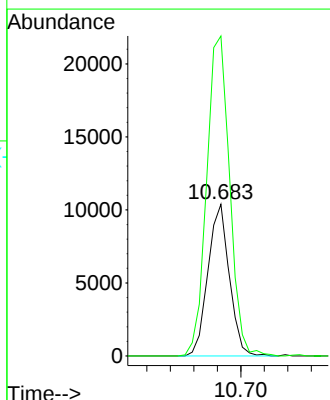
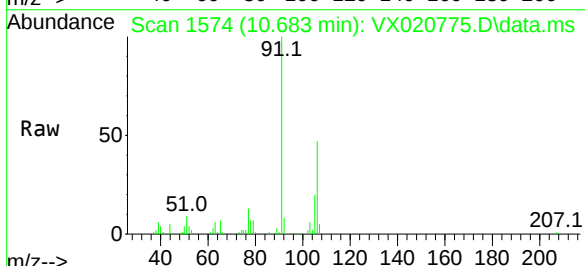


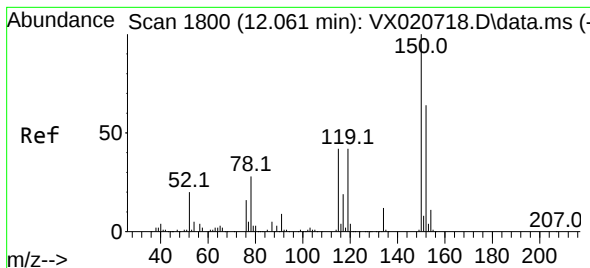

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 224953
Ion Ratio Lower Upper
152 100
115 62.3 41.1 123.3
150 158.9 0.0 349.0

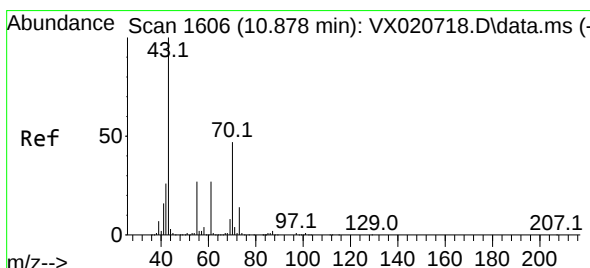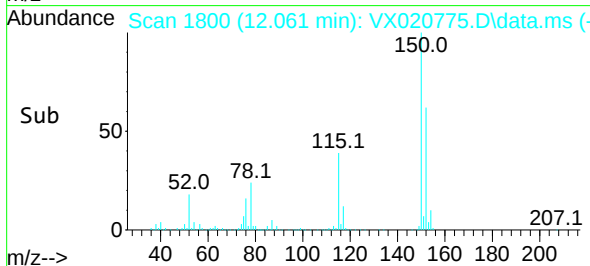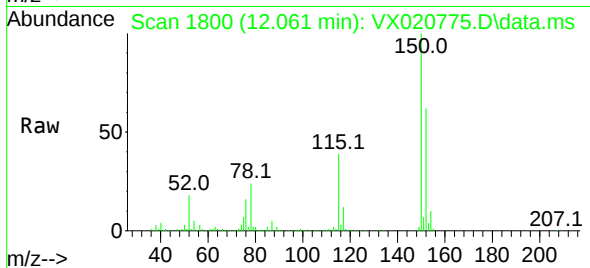

#74
N-ethyl acetate
Concen: 2.02 ug/l
RT: 10.866 min Scan# 1604
Delta R.T. -0.012 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 43 Resp: 70
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.6#
55 51.4 21.5 32.3#
61 0.0 22.1 33.1#


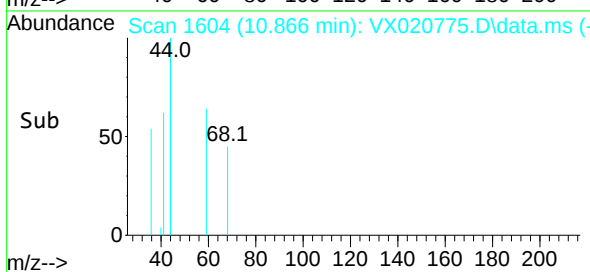
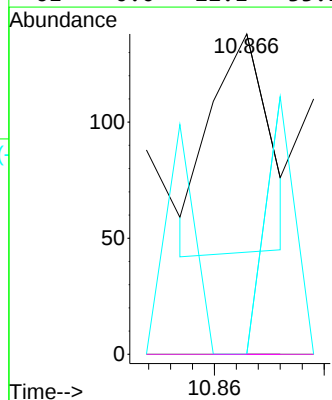
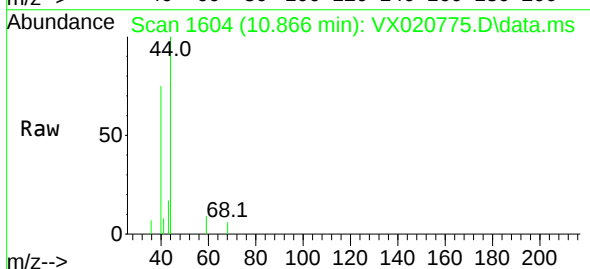


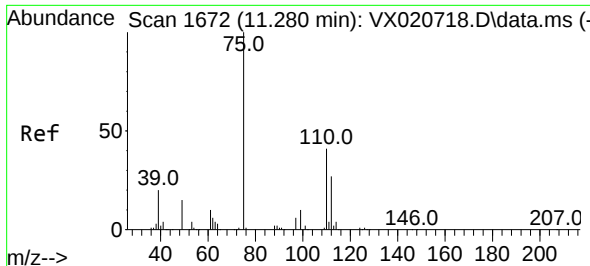

#76
1,2,3-Trichloropropane
Concen: 22.69 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.164 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 118377
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#

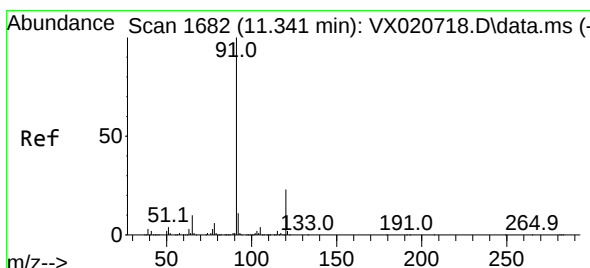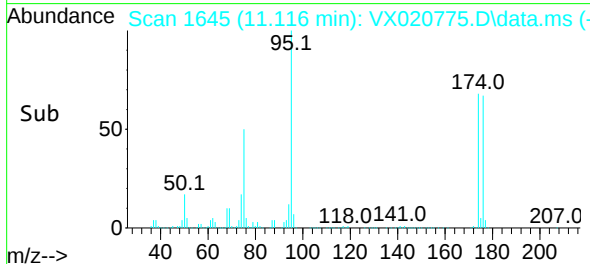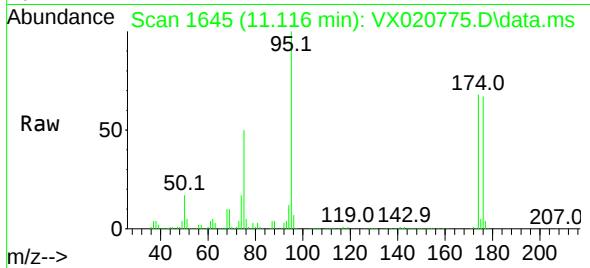

#78
n-propylbenzene
Concen: 0.40 ug/l
RT: 11.341 min Scan# 1682
Delta R.T. 0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 91 Resp: 7416
Ion Ratio Lower Upper
91 100
120 22.0 11.5 34.5


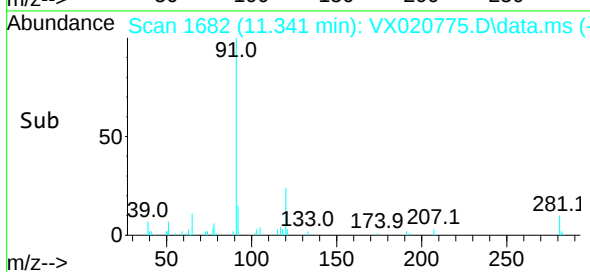

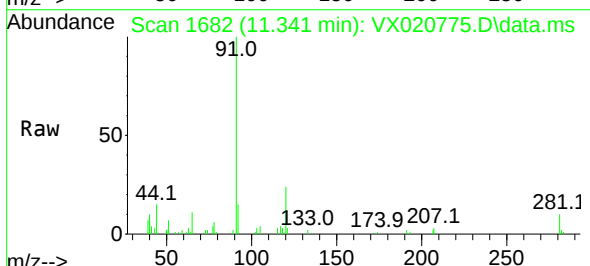


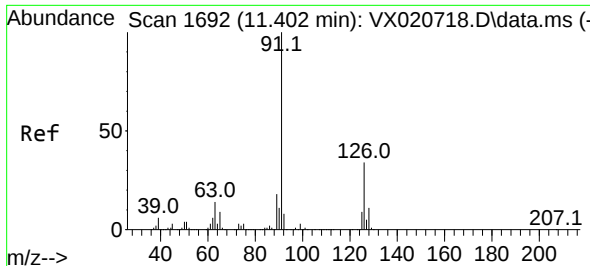

#79
2-Chlorotoluene
Concen: 0.50 ug/l
RT: 11.421 min Scan# 1695
Delta R.T. 0.019 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 5698
Ion Ratio Lower Upper
91 100
126 0.4 16.6 49.8#

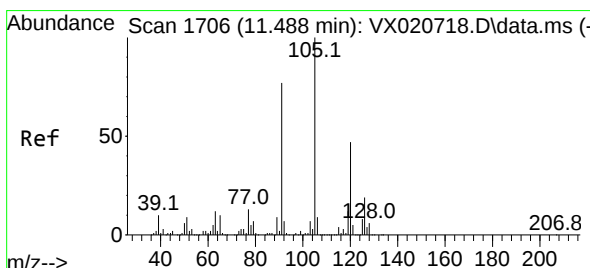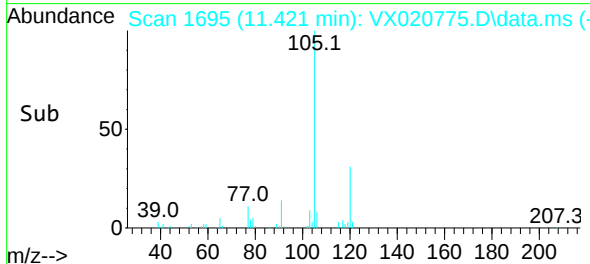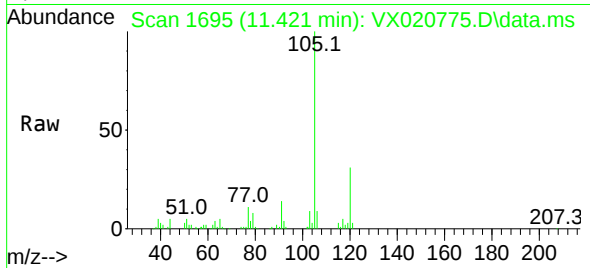

#80
1,3,5-Trimethylbenzene
Concen: 1.18 ug/l
RT: 11.488 min Scan# 1706
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14


Tgt Ion: 105 Resp: 16402
Ion Ratio Lower Upper
105 100
120 46.6 23.8 71.5

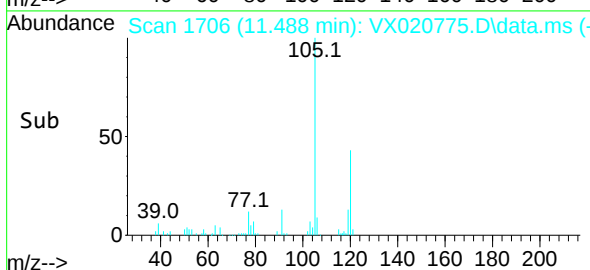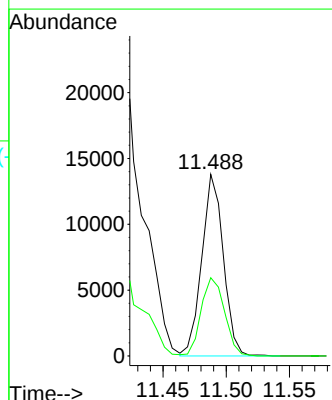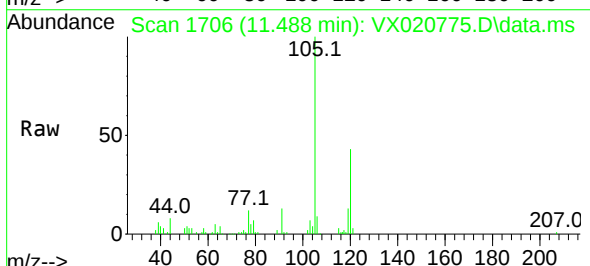






#81
trans-1,4-Dichloro-2-butene
Concen: 63.58 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. 0.061 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Instrument :
MSVOA_X
ClientSampleId :



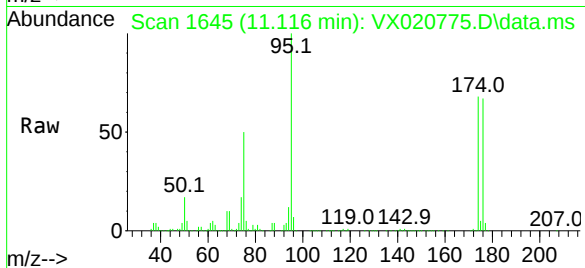



Tgt Ion: 75 Resp: 118377
Ion Ratio Lower Upper
75 100
53 0.1 74.5 111.7#
89 0.0 37.9 56.9#

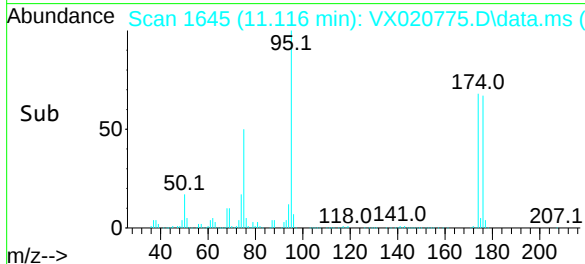

#83
tert-Butylbenzene
Concen: 0.20 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.256 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 119 Resp: 2718
Ion Ratio Lower Upper
119 100
91 28.7 27.9 83.7
134 26.3 11.3 33.9


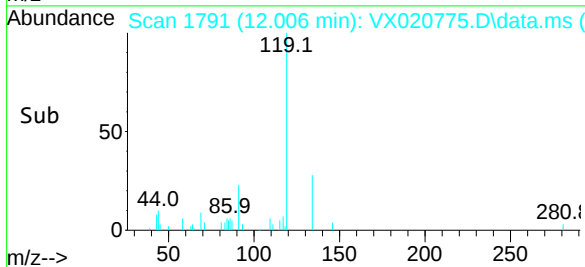

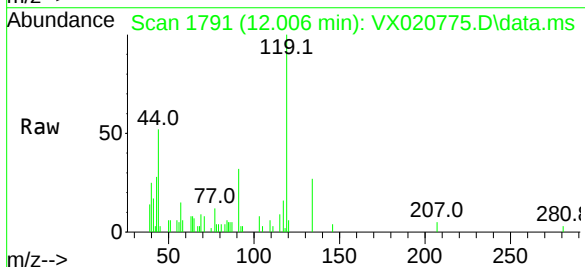




#84
1,2,4-Trimethylbenzene
Concen: 4.74 ug/l
RT: 11.793 min Scan# 1756
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 66397
Ion Ratio Lower Upper
105 100
120 44.1 22.4 67.3

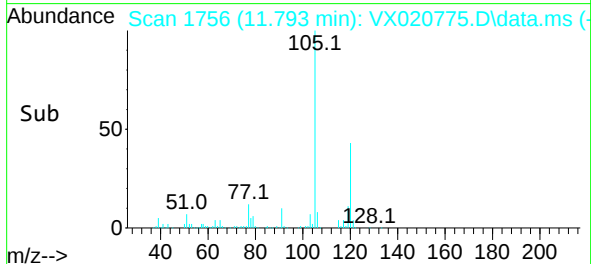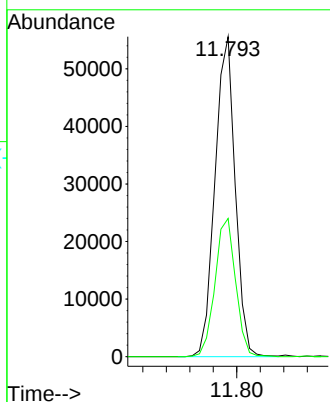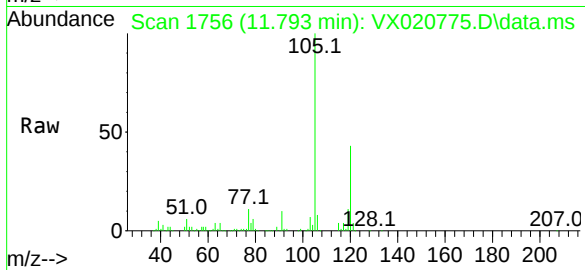

#85
sec-Butylbenzene
Concen: 4.28 ug/l
RT: 11.793 min Scan# 1756
Delta R.T. -0.134 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion:105 Resp: 66397
Ion Ratio Lower Upper
105 100
134 0.1 10.0 29.8#



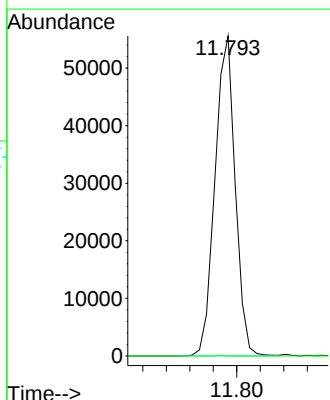
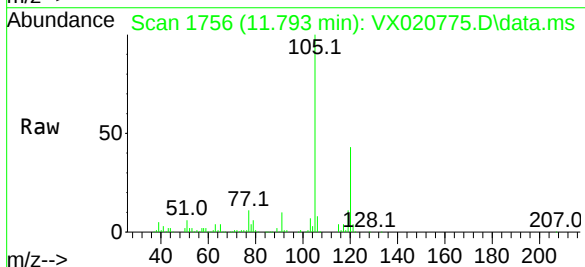




#89
n-Butylbenzene
Concen: 0.35 ug/l
RT: 12.360 min Scan# 1849
Delta R.T. -0.012 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 4521
Ion Ratio Lower Upper
91 100
92 30.4 27.4 82.0
134 98.8 13.2 39.5#

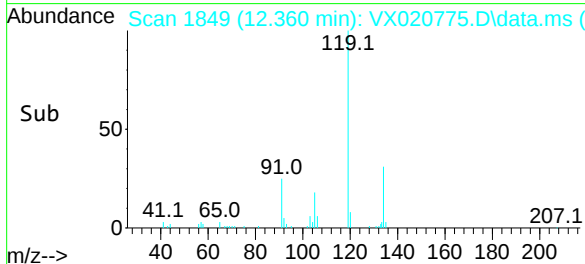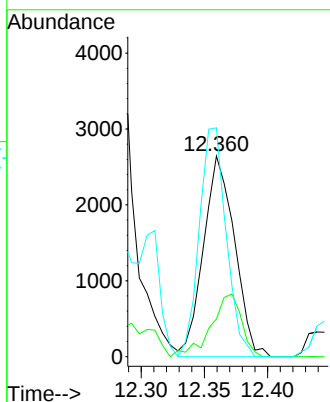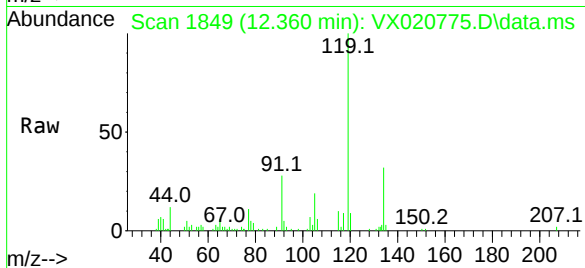

#90
Hexachloroethane
Concen: 0.48 ug/l
RT: 12.567 min Scan# 1883
Delta R.T. -0.012 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Tgt Ion: 117 Resp: 1249
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

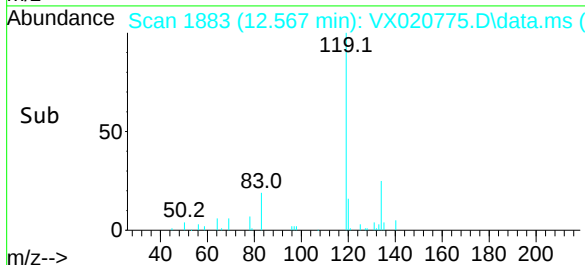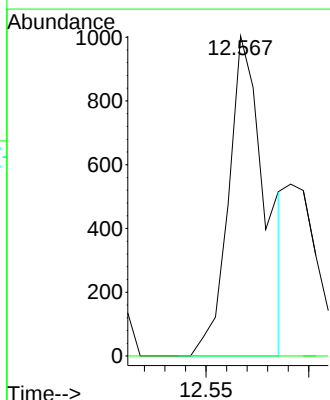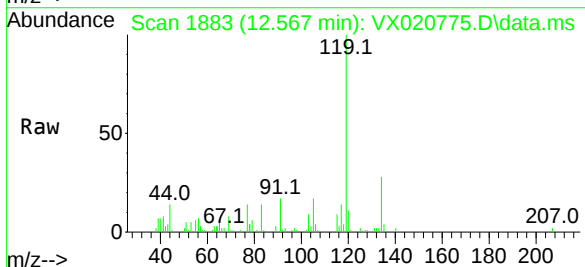

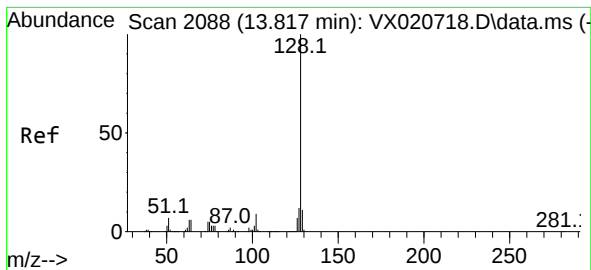

#95
Naphthalene
Concen: 4.57 ug/l
RT: 13.817 min Scan# 2088
Delta R.T. -0.000 min
Lab File: VX020775.D
Acq: 27 Jan 2021 17:14

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:128 Resp: 31088
Ion Ratio Lower Upper
128 100
127 14.0 10.3 15.5
129 12.5 8.8 13.2

