

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012721\
 Data File : VX020777.D
 Acq On : 27 Jan 2021 18:01
 Operator : JC/SP
 Sample : M1217-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 28 00:46:03 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	294261	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	497114	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	455009	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.067	152	170874	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	189537	47.22	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	94.44%		
35) Dibromofluoromethane	5.471	113	19131	5.62	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	11.24%#		
50) Toluene-d8	8.696	98	603369	48.33	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	96.66%		
62) 4-Bromofluorobenzene	11.122	95	160130	33.03	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	66.06%		
Target Compounds						
					Qvalue	
5) Bromomethane	1.630	94	684	0.35	ug/l #	56
13) Acrolein	2.270	56	208	0.37	ug/l #	14
14) Allyl chloride	2.611	41	2711518	515.22	ug/l #	68
16) Acetone	2.428	43	939323	617.25	ug/l	99
17) Carbon Disulfide	2.544	76	675	0.97	ug/l #	75
18) Methyl Acetate	2.611	43	6901629	1775.07	ug/l #	47
20) Methylene Chloride	2.831	84	2808	0.73	ug/l	87
25) 2-Butanone	4.660	43	6993	2.93	ug/l #	81
36) 1,1-Dichloropropene	5.629	75	22325	4.48	ug/l #	49
38) Carbon Tetrachloride	5.623	117	29749	5.67	ug/l #	17
43) Isopropyl Acetate	6.220	43	20899	2.77	ug/l #	57
49) 1,4-Dioxane	7.720	88	1128	12.62	ug/l #	24
51) 4-Methyl-2-Pentanone	8.616	43	6068	1.28	ug/l	96
52) Toluene	8.763	92	37253	4.03	ug/l	99
56) Ethyl methacrylate	9.134	69	937	2.93	ug/l #	1
59) 2-Hexanone	9.561	43	980	0.28	ug/l	90
67) Ethyl Benzene	10.232	91	15468	0.91	ug/l	94
68) m/p-Xylenes	10.342	106	24379	3.83	ug/l	95
69) o-Xylene	10.683	106	12260	2.05	ug/l	97
73) Isopropylbenzene	11.000	105	2530	0.20	ug/l #	49
75) 1,1,2,2-Tetrachloroethane	11.268	83	970	0.23	ug/l #	26
76) 1,2,3-Trichloropropane	11.177	75	25681385	6480.23	ug/l #	38
78) n-propylbenzene	11.360	91	8862	0.62	ug/l	99
79) 2-Chlorotoluene	11.433	91	4331	0.50	ug/l #	45
80) 1,3,5-Trimethylbenzene	11.500	105	12448	1.18	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.177	75	25681081	18158.90	ug/l #	22
82) 4-Chlorotoluene	11.506	91	2169	0.21	ug/l #	62
83) tert-Butylbenzene	12.012	119	3411	0.33	ug/l	79
84) 1,2,4-Trimethylbenzene	11.799	105	38076	3.58	ug/l	98
85) sec-Butylbenzene	11.939	105	3445	0.29	ug/l	83
86) p-Isopropyltoluene	12.055	119	5626	0.51	ug/l	86
89) n-Butylbenzene	12.353	91	14722	1.50	ug/l	69
90) Hexachloroethane	12.573	117	1230	0.62	ug/l #	9
95) Naphthalene	13.817	128	7556	3.42	ug/l #	60

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012721\
Data File : VX020777.D
Acq On : 27 Jan 2021 18:01
Operator : JC/SP
Sample : M1217-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 28 00:46:03 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012721\
Data File : VX020777.D
Acq On : 27 Jan 2021 18:01
Operator : JC/SP
Sample : M1217-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 28 00:46:03 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration

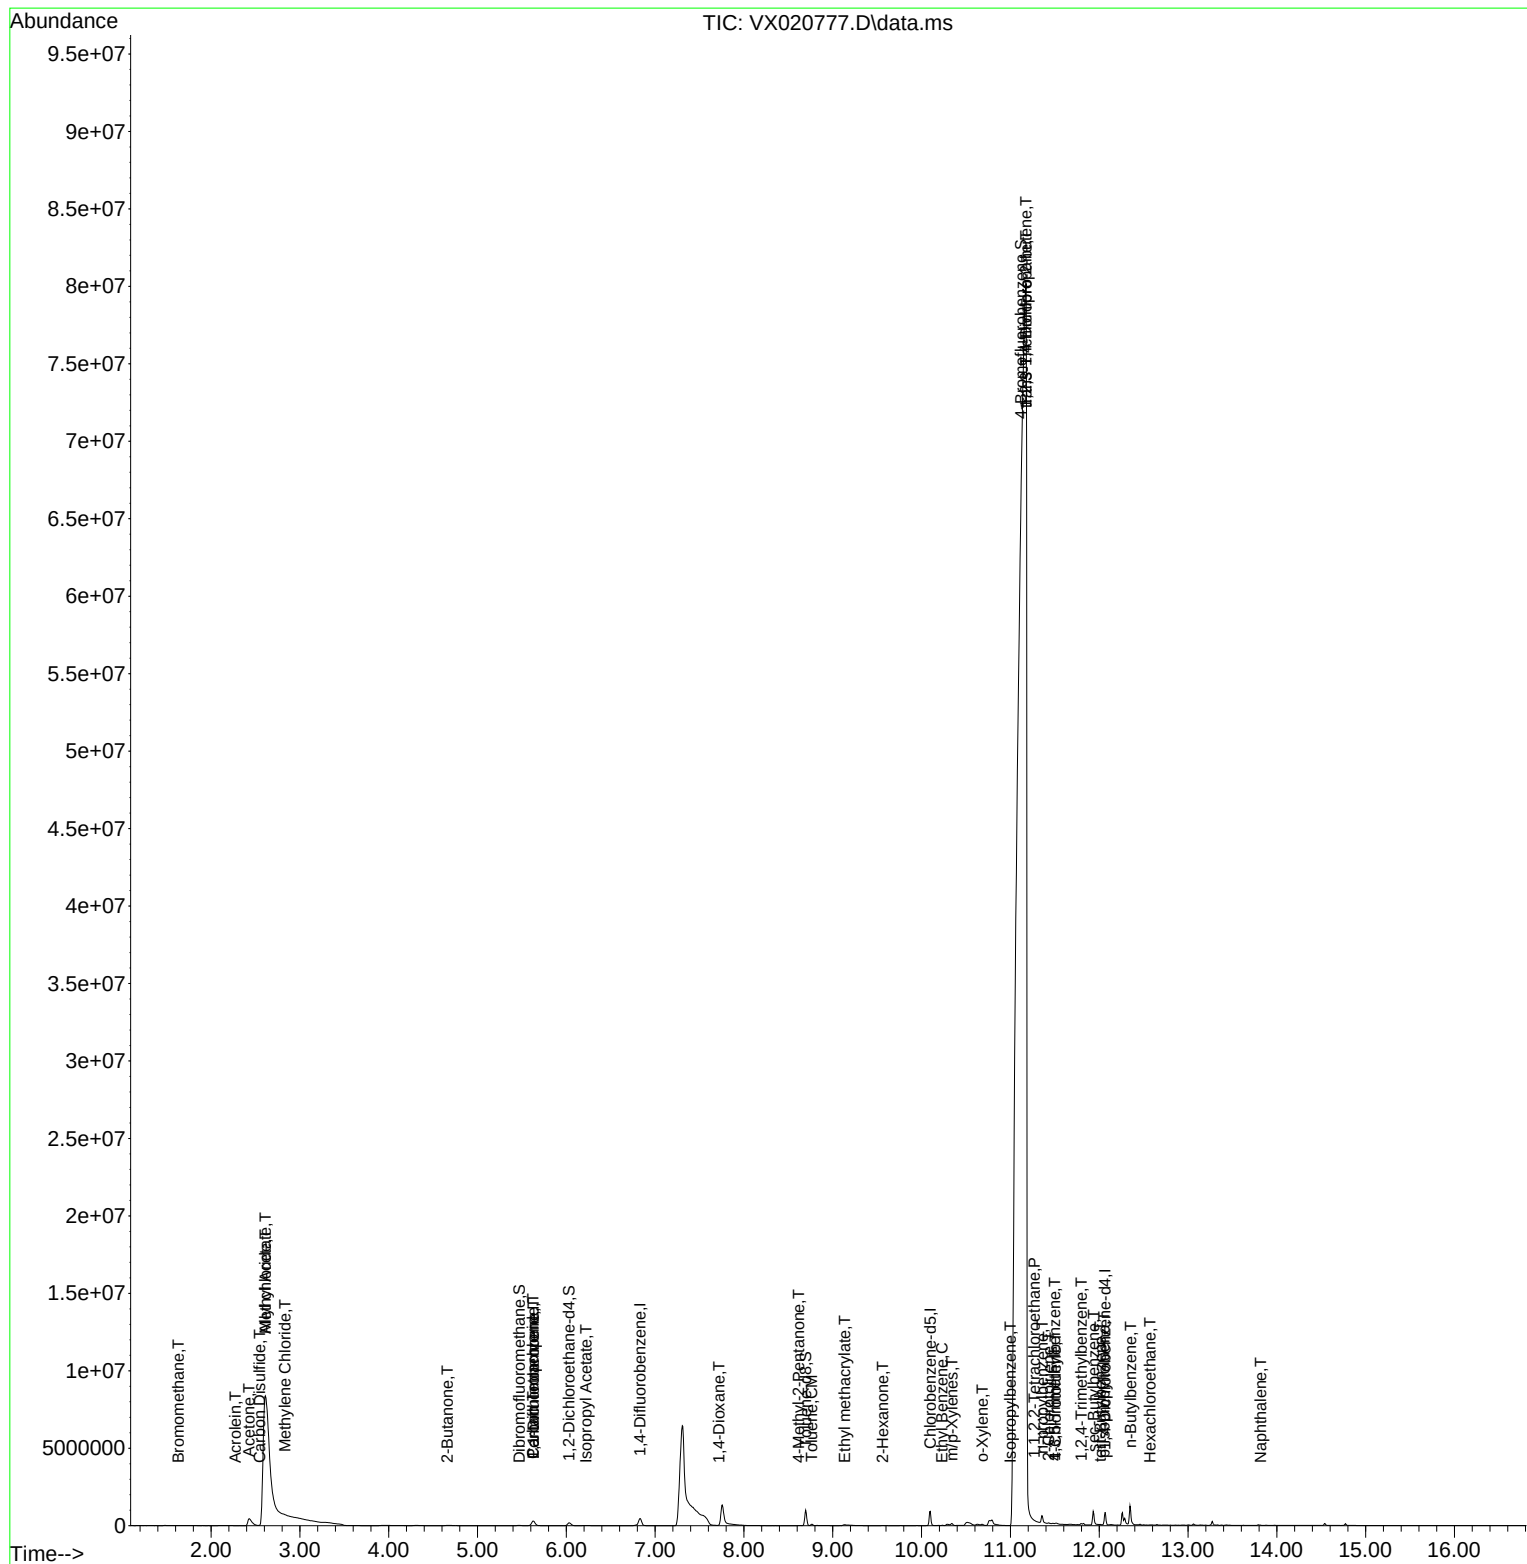






#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01


Instrument :
MSVOA_X
ClientSampled :

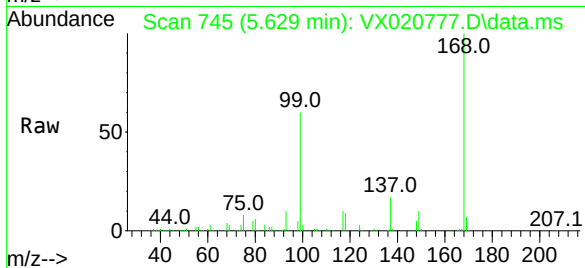



Tgt Ion:168 Resp: 294261
Ion Ratio Lower Upper
168 100
99 60.1 45.8 68.6

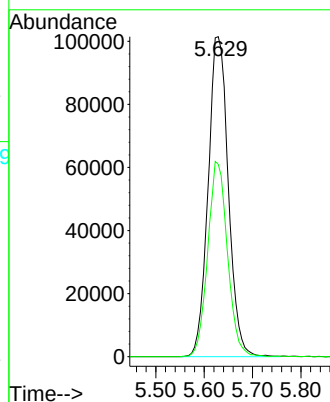


#5
Bromomethane
Concen: 0.35 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.006 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

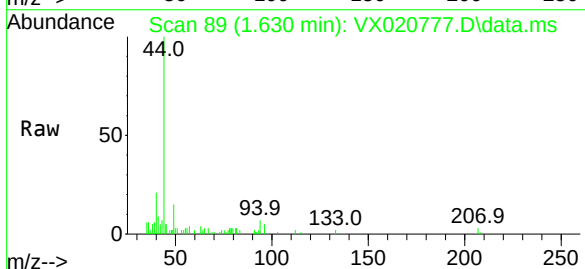

Tgt Ion: 94 Resp: 684
Ion Ratio Lower Upper
94 100
96 52.9 76.4 114.6#



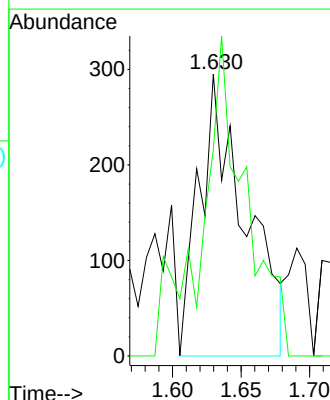
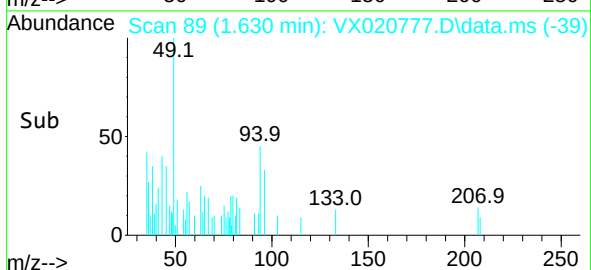


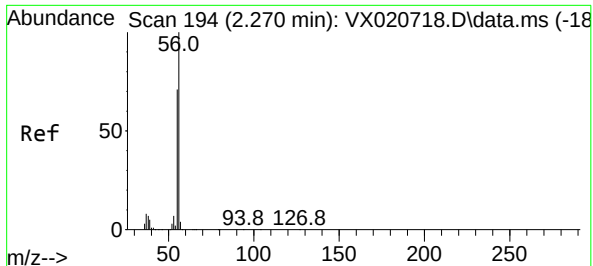

#13
Acrolein
Concen: 0.37 ug/l
RT: 2.270 min Scan# 194
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 56 Resp: 208
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#

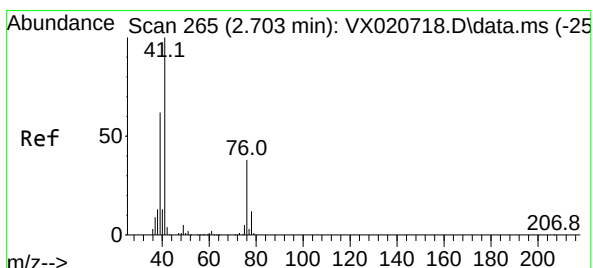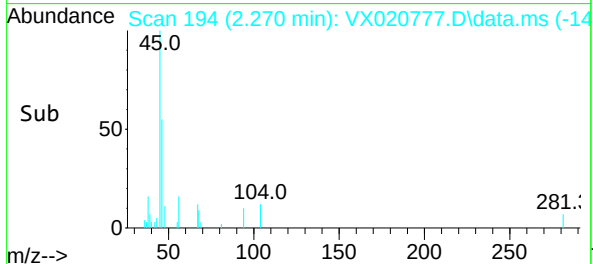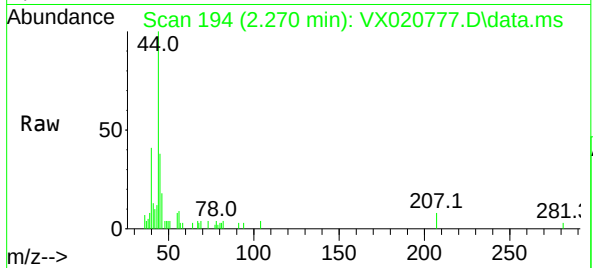

#14
Allyl chloride
Concen: 515.22 ug/l
RT: 2.611 min Scan# 250
Delta R.T. -0.092 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 41 Resp: 2711518
Ion Ratio Lower Upper
41 100
39 75.5 51.6 77.4
76 0.0 30.5 45.7#


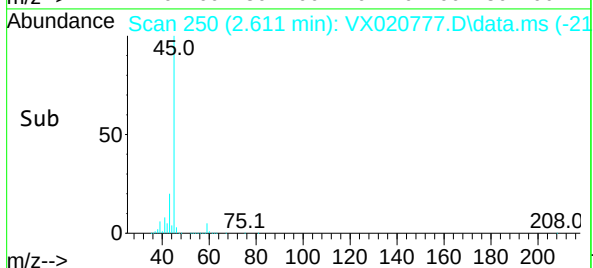

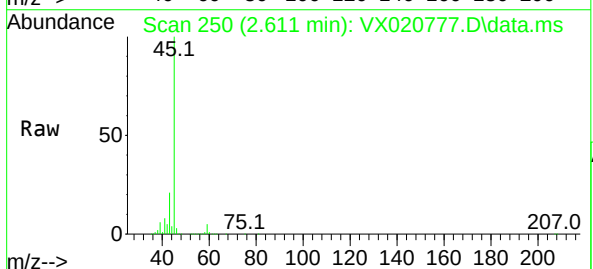




#16
Acetone
Concen: 617.25 ug/l
RT: 2.428 min Scan# 220
Delta R.T. 0.006 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 939323
Ion Ratio Lower Upper
43 100
58 35.7 27.8 41.8



#17
Carbon Disulfide
Concen: 0.97 ug/l
RT: 2.544 min Scan# 239
Delta R.T. 0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 76 Resp: 675
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#




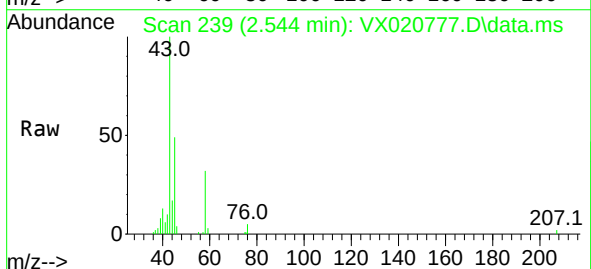




#18
Methyl Acetate
Concen: 1775.07 ug/l
RT: 2.611 min Scan# 250
Delta R.T. -0.134 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 6901629
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

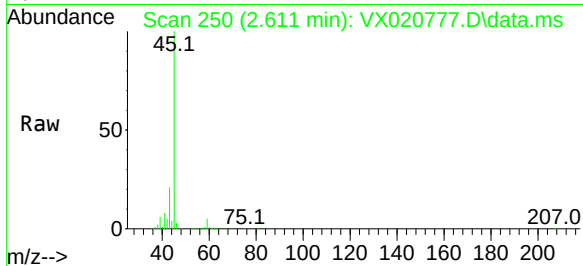

#20
Methylene Chloride
Concen: 0.73 ug/l
RT: 2.831 min Scan# 286
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 84 Resp: 2808
Ion Ratio Lower Upper
84 100
49 131.5 88.6 132.8
51 37.2 27.0 40.6
86 59.7 50.3 75.5


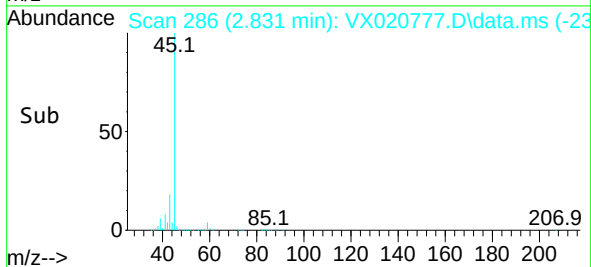

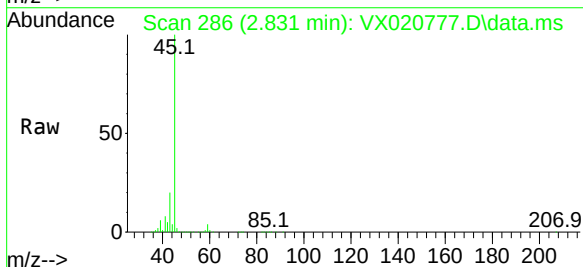




#25
2-Butanone
Concen: 2.93 ug/l
RT: 4.660 min Scan# 586
Delta R.T. 0.025 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 6993
Ion Ratio Lower Upper
43 100
72 19.5 23.7 35.5#

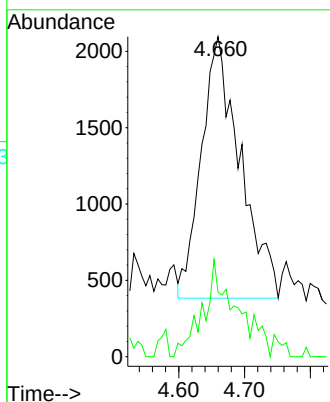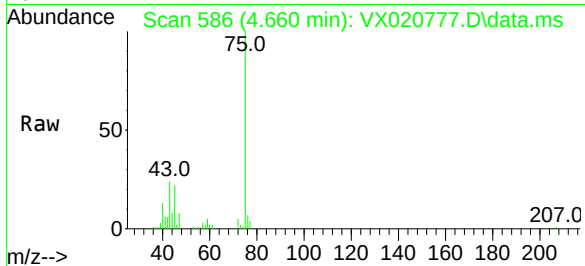

#33
1,2-Dichloroethane-d4
Concen: 47.22 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 65 Resp: 189537
Ion Ratio Lower Upper
65 100
67 53.0 0.0 105.4

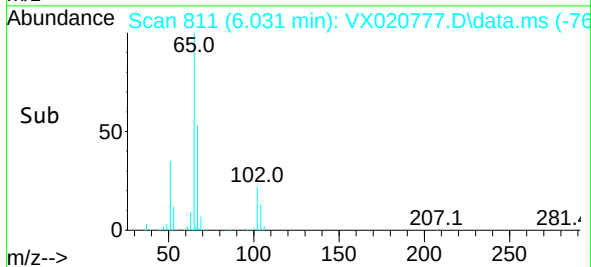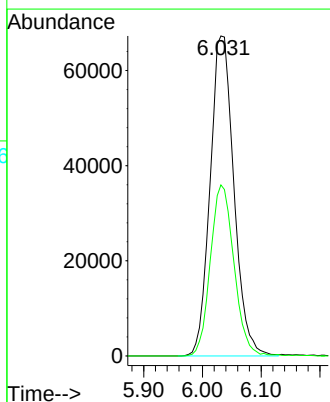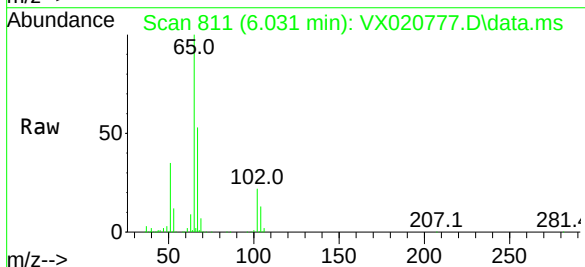

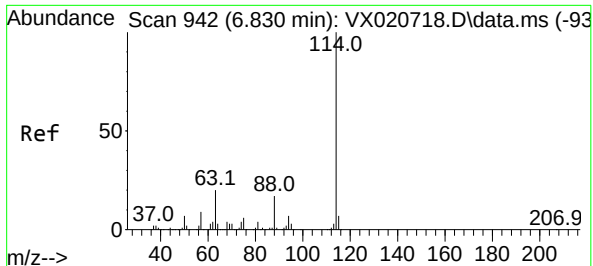

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.830 min Scan# 942

Delta R.T. 0.000 min

Lab File: VX020777.D

Acq: 27 Jan 2021 18:01





Tgt Ion:114 Resp: 497114

Ion Ratio Lower Upper

114 100

63 20.7 0.0 40.8

88 17.4 0.0 32.8

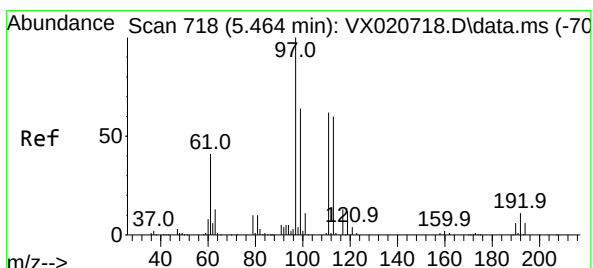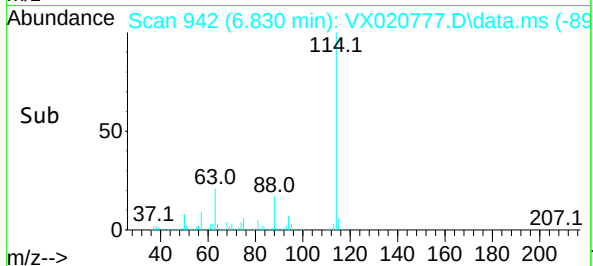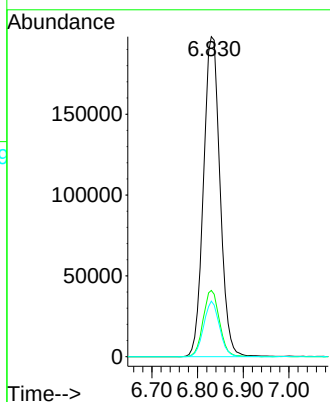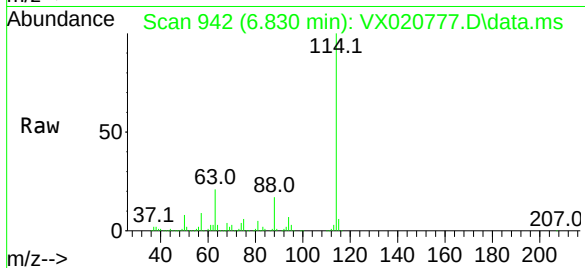

#35

Dibromofluoromethane

Concen: 5.62 ug/l

RT: 5.471 min Scan# 719

Delta R.T. 0.006 min

Lab File: VX020777.D

Acq: 27 Jan 2021 18:01




Tgt Ion:113 Resp: 19131


Ion Ratio Lower Upper

113 100

111 102.7 81.9 122.9


192 20.1 16.7 25.1

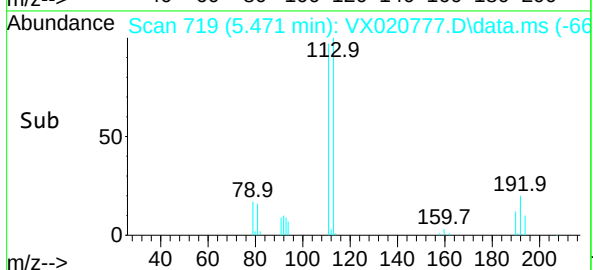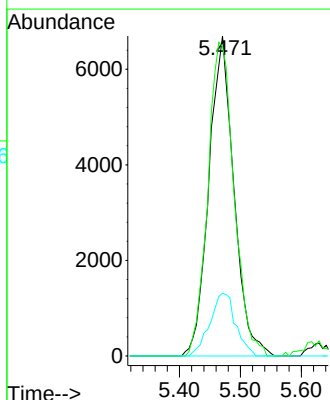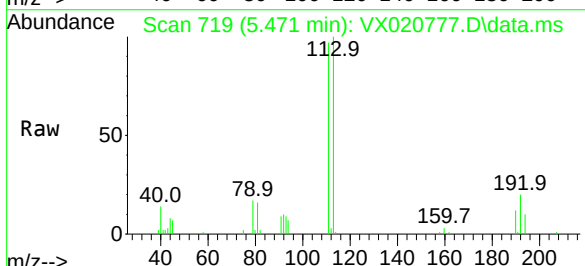






#36
1,1-Dichloropropene
Concen: 4.48 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.140 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Instrument :
MSVOA_X
ClientSampled :



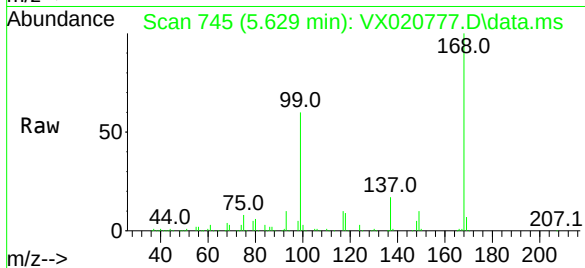



Tgt Ion: 75 Resp: 22325
Ion Ratio Lower Upper
75 100
110 9.5 18.1 54.4#
77 0.0 25.3 37.9#

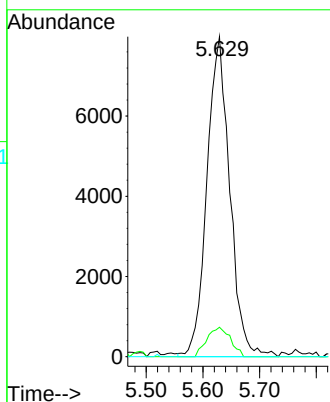

#38
Carbon Tetrachloride
Concen: 5.67 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.128 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 117 Resp: 29749
Ion Ratio Lower Upper
117 100
119 5.8 76.2 114.2#
121 0.0 24.8 37.2#


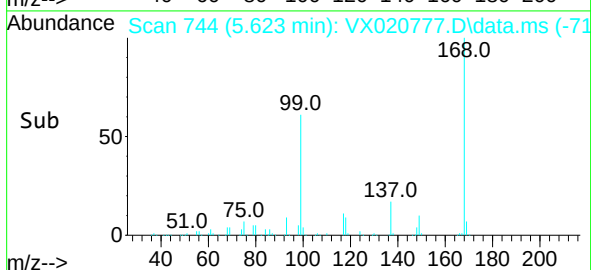
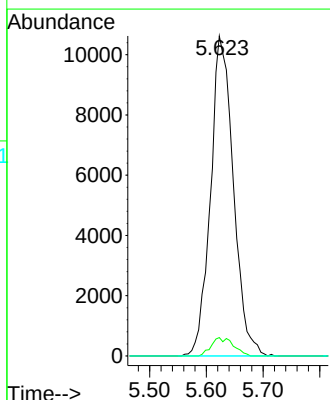
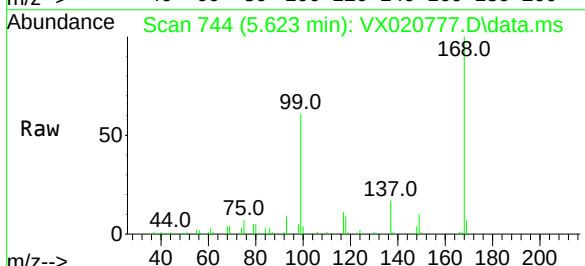


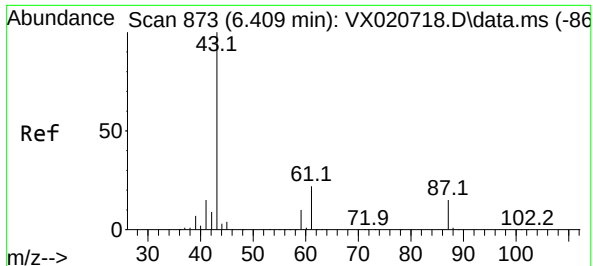

#43
Isopropyl Acetate
Concen: 2.77 ug/l
RT: 6.220 min Scan# 842
Delta R.T. -0.189 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 20899
Ion Ratio Lower Upper
43 100
61 0.0 18.2 27.4#
87 0.0 12.5 18.7#

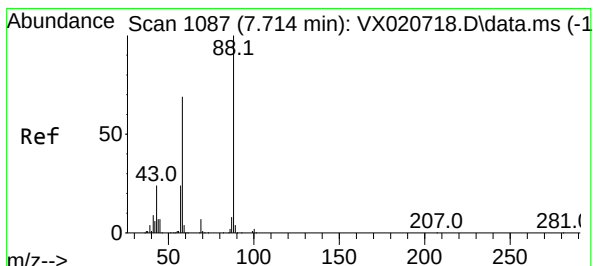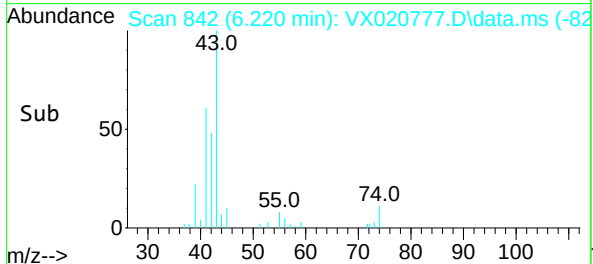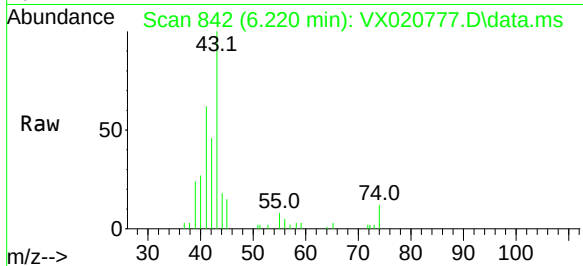

#49
1,4-Dioxane
Concen: 12.62 ug/l
RT: 7.720 min Scan# 1088
Delta R.T. 0.006 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 88 Resp: 1128
Ion Ratio Lower Upper
88 100
43 0.0 23.2 34.8#
58 0.0 55.0 82.4#


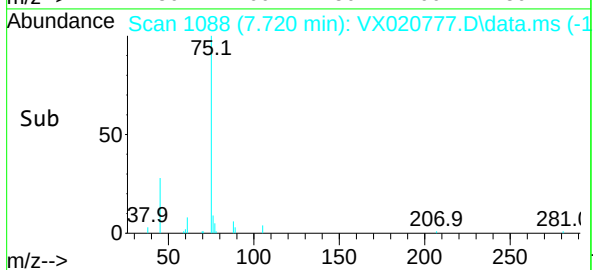

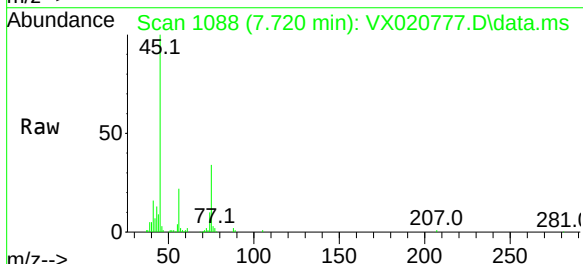




#50
Toluene-d8
Concen: 48.33 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 603369
Ion Ratio Lower Upper
98 100
100 65.9 51.9 77.9



#51
4-Methyl-2-Pentanone
Concen: 1.28 ug/l
RT: 8.616 min Scan# 1235
Delta R.T. 0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 43 Resp: 6068
Ion Ratio Lower Upper
43 100
58 46.6 35.4 53.0


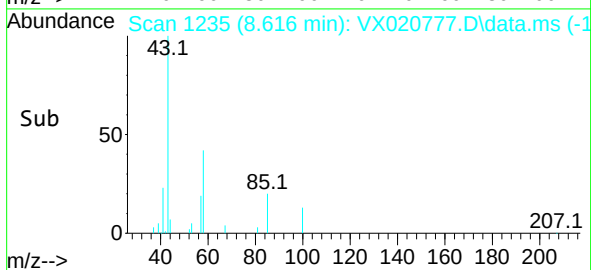

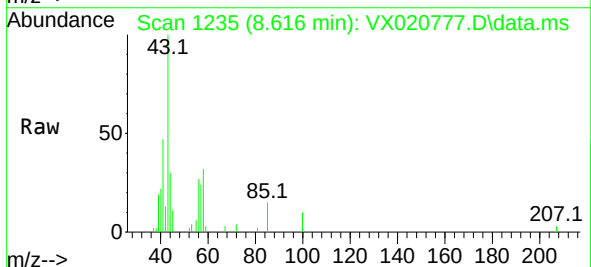




#52
Toluene
Concen: 4.03 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 92 Resp: 37253
Ion Ratio Lower Upper
92 100
91 173.4 137.1 205.7



#56
Ethyl methacrylate
Concen: 2.93 ug/l
RT: 9.134 min Scan# 1320
Delta R.T. -0.025 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 69 Resp: 937
Ion Ratio Lower Upper
69 100
41 1659.4 46.8 70.2#
39 1831.9 24.7 37.1#


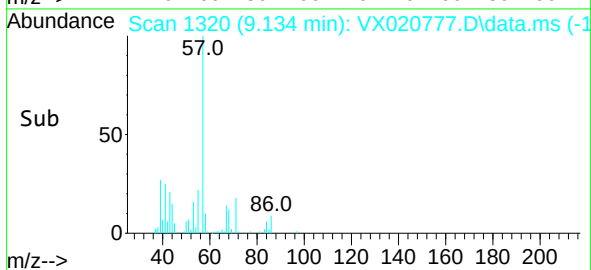

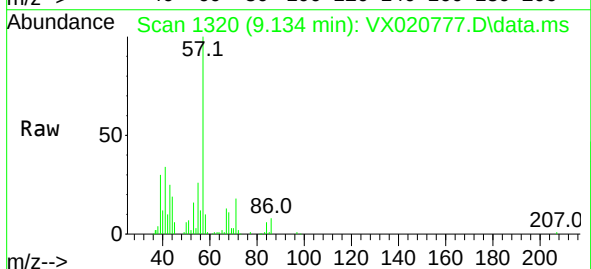




#59
2-Hexanone
Concen: 0.28 ug/l
RT: 9.561 min Scan# 1390
Delta R.T. 0.091 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 980
Ion Ratio Lower Upper
43 100
58 54.6 30.9 92.8



#62
4-Bromofluorobenzene
Concen: 33.03 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 95 Resp: 160130
Ion Ratio Lower Upper
95 100
174 81.9 0.0 154.6
176 78.9 0.0 155.8


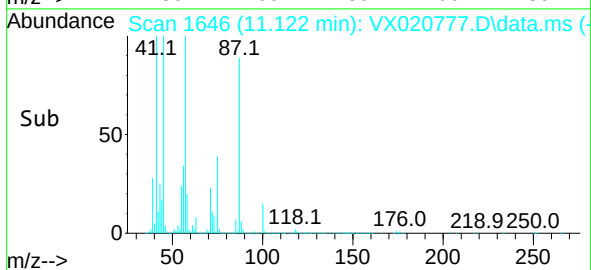

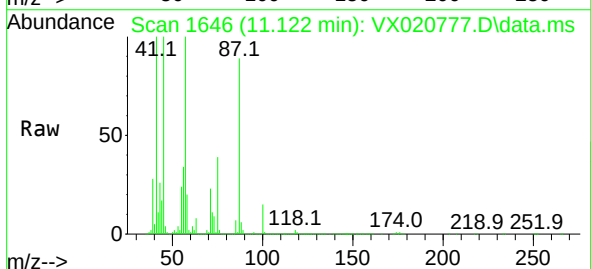




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 455009
Ion Ratio Lower Upper
117 100
82 57.3 47.4 71.2
119 33.5 26.6 39.8

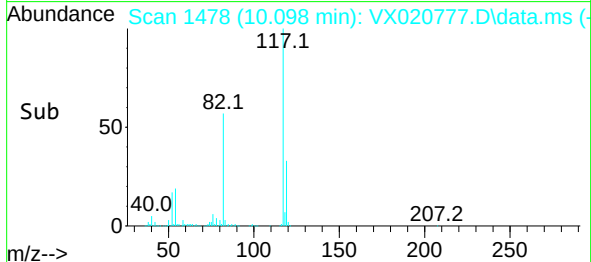

#67
Ethyl Benzene
Concen: 0.91 ug/l
RT: 10.232 min Scan# 1500
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 91 Resp: 15468
Ion Ratio Lower Upper
91 100
106 34.0 24.6 37.0


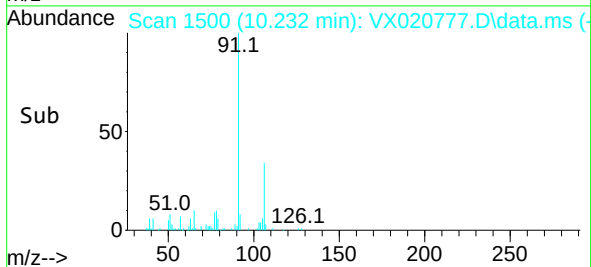

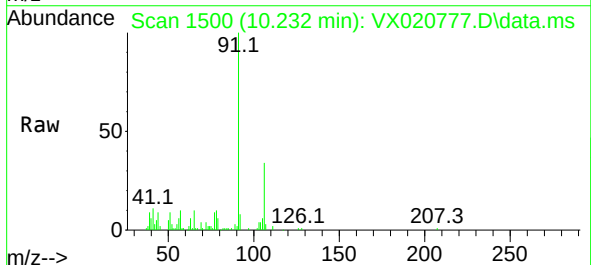




#68
m/p-Xylenes
Concen: 3.83 ug/l
RT: 10.342 min Scan# 1518
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 24379
Ion Ratio Lower Upper
106 100
91 211.4 162.8 244.2



#69
o-Xylene
Concen: 2.05 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion:106 Resp: 12260
Ion Ratio Lower Upper
106 100
91 210.8 108.1 324.2




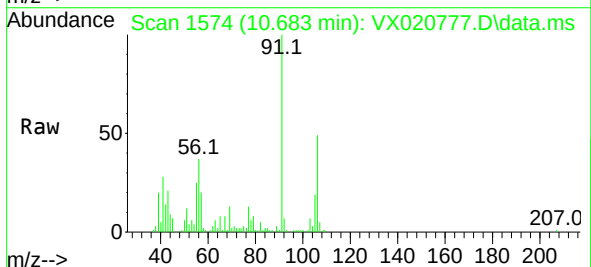




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.067 min Scan# 1801
Delta R.T. 0.006 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:152 Resp: 170874
Ion Ratio Lower Upper
152 100
115 60.9 41.1 123.3
150 158.1 0.0 349.0

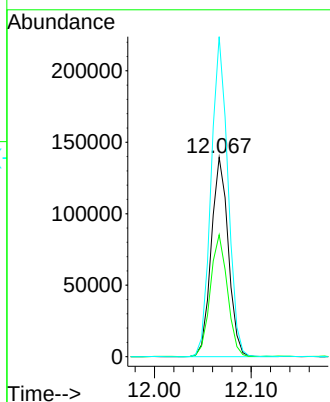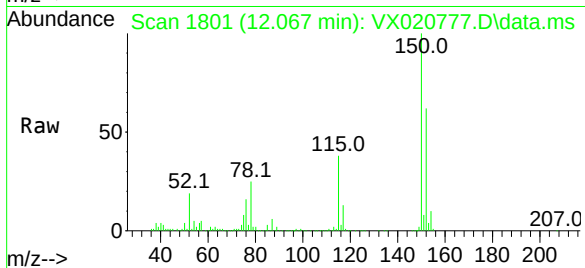

#73
Isopropylbenzene
Concen: 0.20 ug/l
RT: 11.000 min Scan# 1626
Delta R.T. 0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion:105 Resp: 2530
Ion Ratio Lower Upper
105 100
120 0.0 13.2 39.6#


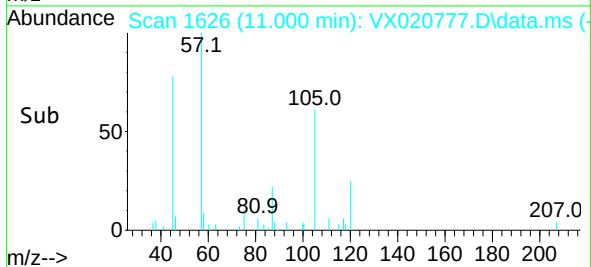
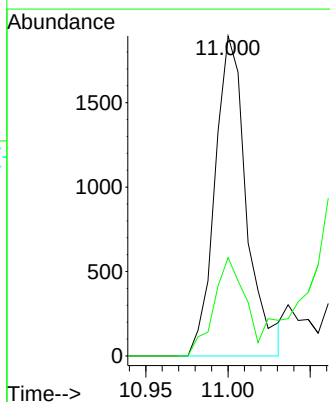
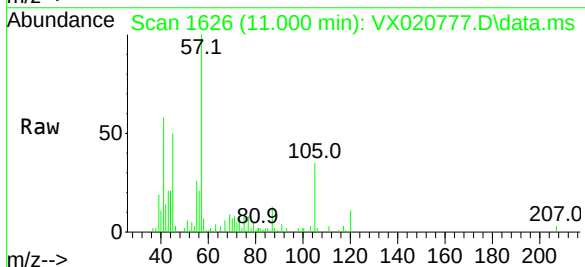




#75
1,1,2,2-Tetrachloroethane
Concen: 0.23 ug/l
RT: 11.268 min Scan# 1670
Delta R.T. 0.018 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 83 Resp: 970
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.2#
85 0.0 31.8 95.4#



#76
1,2,3-Trichloropropane
Concen: 6480.23 ug/l
RT: 11.177 min Scan# 1655
Delta R.T. -0.103 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 75 Resp: 25681385
Ion Ratio Lower Upper
75 100
77 0.6 19.1 57.5#

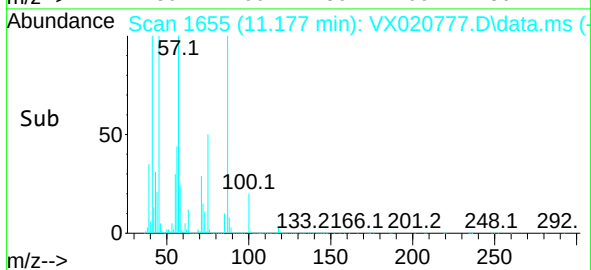



#78

n-propylbenzene

Concen: 0.62 ug/l

RT: 11.360 min Scan# 1685

Delta R.T. 0.019 min

Lab File: VX020777.D





Acq: 27 Jan 2021 18:01

Tgt Ion: 91 Resp: 8862

Ion Ratio Lower Upper

91 100

120 22.7 11.5 34.5

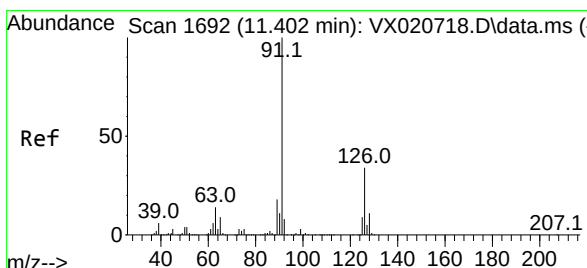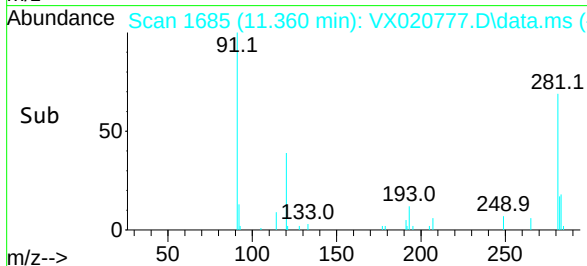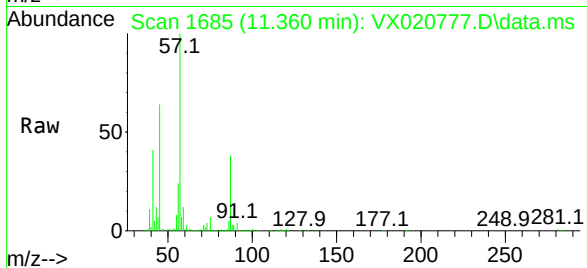

#79

2-Chlorotoluene

Concen: 0.50 ug/l

RT: 11.433 min Scan# 1697

Delta R.T. 0.031 min

Lab File: VX020777.D




Acq: 27 Jan 2021 18:01


Tgt Ion: 91 Resp: 4331

Ion Ratio Lower Upper

91 100

126 2.1 16.6 49.8#


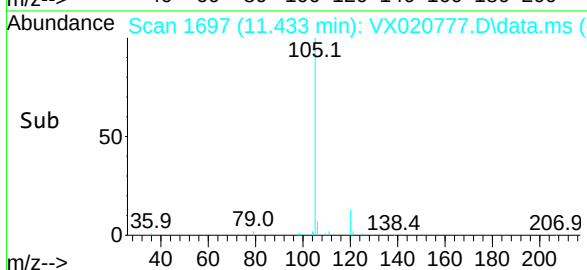

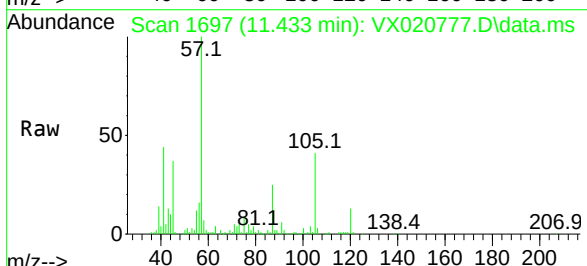




#80
1,3,5-Trimethylbenzene
Concen: 1.18 ug/l
RT: 11.500 min Scan# 1708
Delta R.T. 0.012 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:105 Resp: 12448
Ion Ratio Lower Upper
105 100
120 45.5 23.8 71.5

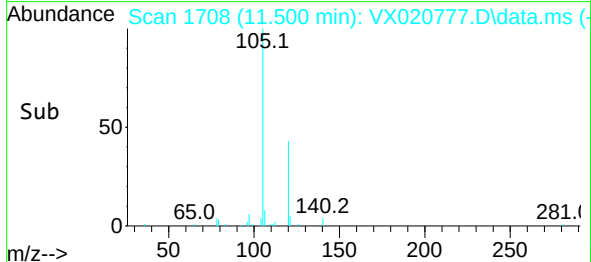

#81
trans-1,4-Dichloro-2-butene
Concen: 18158.90 ug/l
RT: 11.177 min Scan# 1655
Delta R.T. 0.122 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 75 Resp:25681081
Ion Ratio Lower Upper
75 100
53 10.6 74.5 111.7#
89 6.0 37.9 56.9#


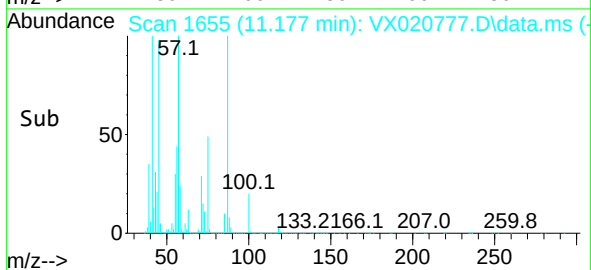




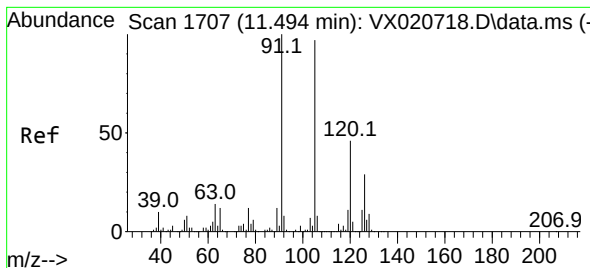

#82
4-Chlorotoluene
Concen: 0.21 ug/l
RT: 11.506 min Scan# 1709
Delta R.T. 0.012 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 2169
Ion Ratio Lower Upper
91 100
126 9.2 14.9 44.5#

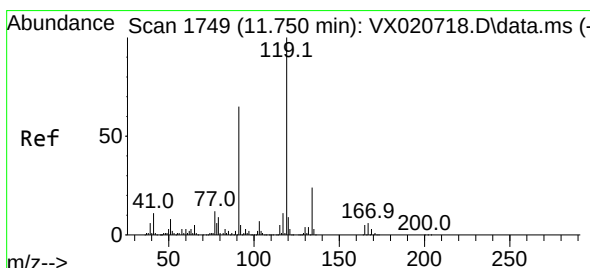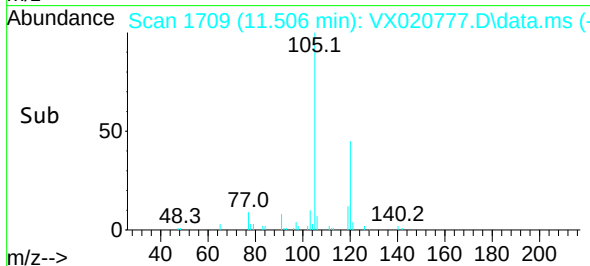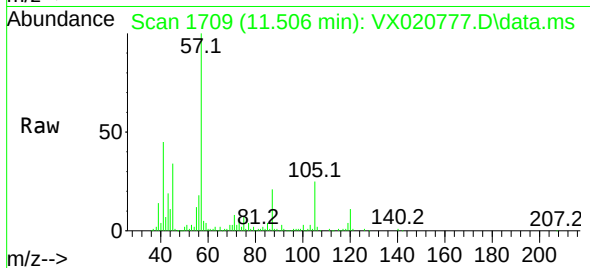

#83
tert-Butylbenzene
Concen: 0.33 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.262 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion: 119 Resp: 3411
Ion Ratio Lower Upper
119 100
91 36.8 27.9 83.7
134 25.9 11.3 33.9

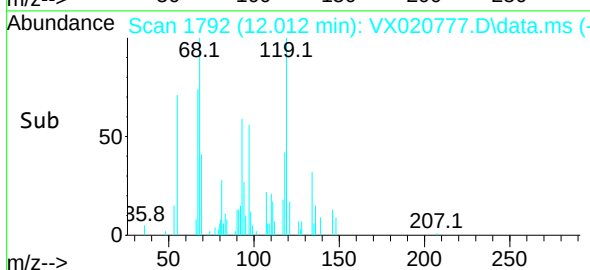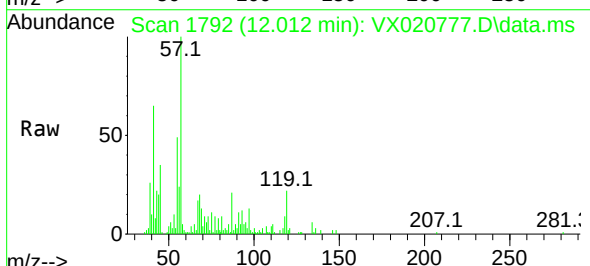



#84

1,2,4-Trimethylbenzene

Concen: 3.58 ug/l

RT: 11.799 min Scan# 1757

Delta R.T. 0.006 min

Lab File: VX020777.D





Acq: 27 Jan 2021 18:01

Tgt Ion:105 Resp: 38076

Ion Ratio Lower Upper

105 100

120 46.3 22.4 67.3

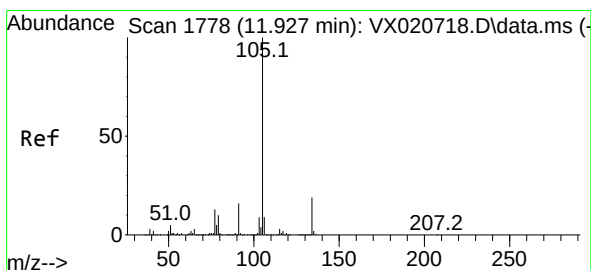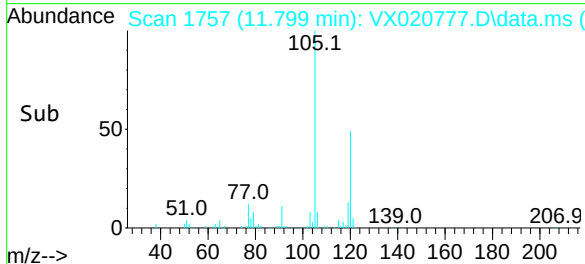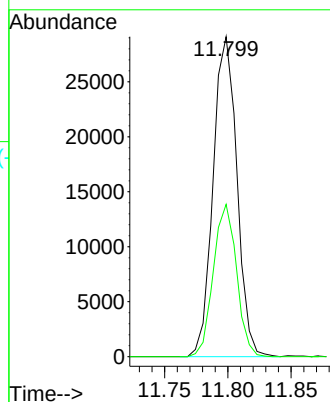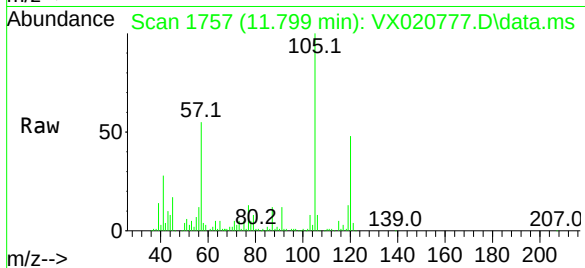

#85

sec-Butylbenzene

Concen: 0.29 ug/l

RT: 11.939 min Scan# 1780

Delta R.T. 0.012 min

Lab File: VX020777.D




Acq: 27 Jan 2021 18:01


Tgt Ion:105 Resp: 3445

Ion Ratio Lower Upper

105 100

134 27.9 10.0 29.8


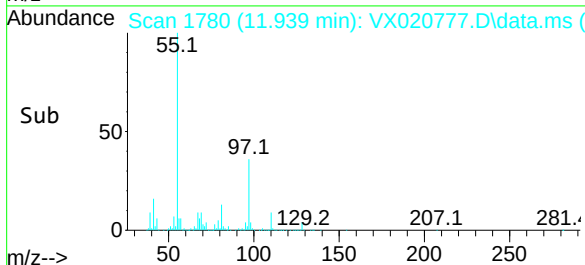
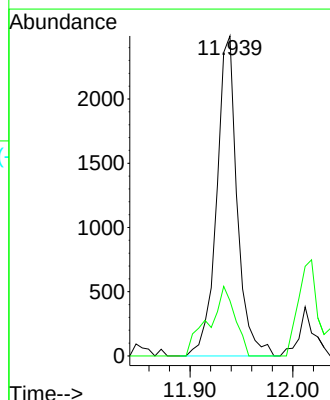
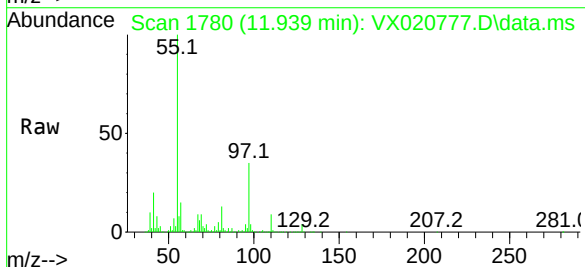




#86
p-Isopropyltoluene
Concen: 0.51 ug/l
RT: 12.055 min Scan# 1799
Delta R.T. 0.006 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:	119	Resp:	5626
Ion	Ratio	Lower	Upper
119	100		
134	29.5	12.9	38.7
91	33.8	11.7	35.0

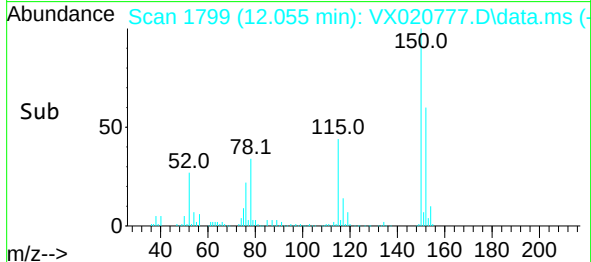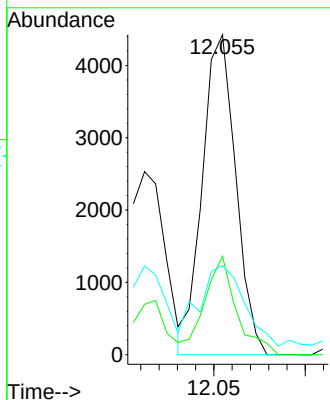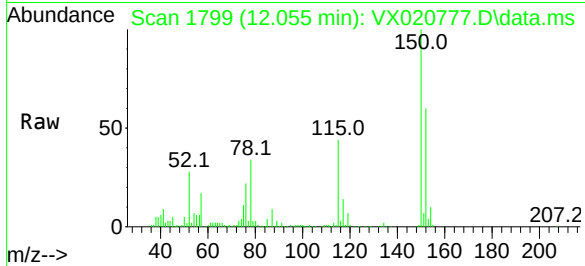

#89
n-Butylbenzene
Concen: 1.50 ug/l
RT: 12.353 min Scan# 1848
Delta R.T. -0.019 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion:	91	Resp:	14722
Ion	Ratio	Lower	Upper
91	100		
92	27.5	27.4	82.0
134	34.2	13.2	39.5


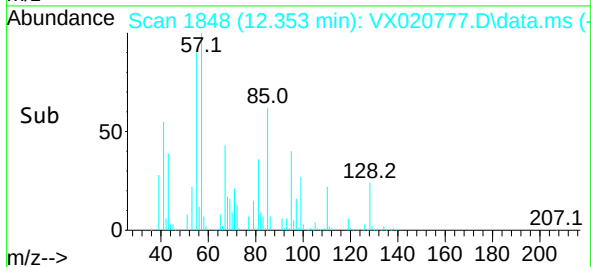
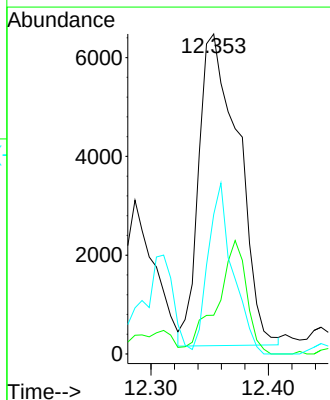
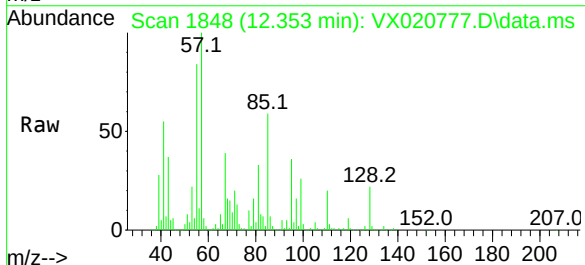




#90
Hexachloroethane
Concen: 0.62 ug/l
RT: 12.573 min Scan# 1884
Delta R.T. -0.006 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 1230
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

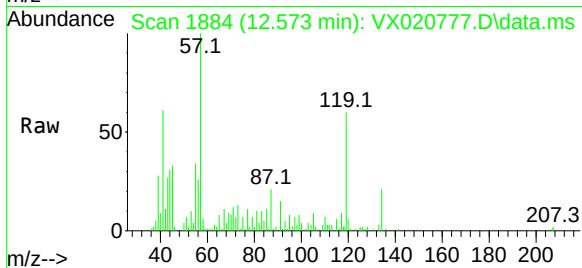

#95
Naphthalene
Concen: 3.42 ug/l
RT: 13.817 min Scan# 2088
Delta R.T. -0.000 min
Lab File: VX020777.D
Acq: 27 Jan 2021 18:01

Tgt Ion:128 Resp: 7556
Ion Ratio Lower Upper
128 100
127 32.5 10.3 15.5#
129 0.0 8.8 13.2#

