

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012722\
 Data File : VX026620.D
 Acq On : 27 Jan 2022 13:36
 Operator : JC/MD
 Sample : N1286-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-30

Quant Time: Jan 28 04:25:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	141808	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	240948	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	216579	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	90377	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	92002	46.443	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.880%
35) Dibromofluoromethane	5.391	113	74511	47.887	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.780%
50) Toluene-d8	8.653	98	284140	50.676	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	101.360%
62) 4-Bromofluorobenzene	11.079	95	102625	51.523	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.040%

Target Compounds					Qvalue	
6) Chloroethane	1.593	64	3186	3.909	ug/l #	43
10) Methyl Iodide	2.465	142	178	4.542	ug/l #	37
13) Acrolein	2.343	56	614	2.097	ug/l #	74
15) Acrylonitrile	3.111	53	256	0.302	ug/l #	29
16) Acetone	2.392	43	7127	7.055	ug/l #	88
18) Methyl Acetate	2.788	43	17026	8.478	ug/l #	53
19) Methyl tert-butyl Ether	3.111	73	8979	1.671	ug/l #	1
20) Methylene Chloride	2.794	84	487	0.292	ug/l #	67
22) Diisopropyl ether	3.764	45	2433	0.440	ug/l #	82
23) Vinyl Acetate	3.764	43	1359	0.298	ug/l #	73
25) 2-Butanone	4.727	43	11509	8.760	ug/l #	50
29) Tetrahydrofuran	5.013	42	183	0.235	ug/l #	78
31) Cyclohexane	5.471	56	2429	0.831	ug/l	87
36) 1,1-Dichloropropene	5.556	75	11269	4.588	ug/l #	51
37) Ethyl Acetate	4.727	43	11509	4.632	ug/l	99
38) Carbon Tetrachloride	5.556	117	14665	5.804	ug/l #	17
39) Methylcyclohexane	7.385	83	1048	0.354	ug/l	92
40) Benzene	6.044	78	24978	3.679	ug/l	96
52) Toluene	8.720	92	5822	1.398	ug/l	99
67) Ethyl Benzene	10.195	91	96776	11.677	ug/l	100
68) m/p-Xylenes	10.305	106	2808	0.905	ug/l	95
69) o-Xylene	10.646	106	1457	0.487	ug/l	95
73) Isopropylbenzene	10.963	105	9349	1.262	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	51414	25.837	ug/l #	40
78) n-propylbenzene	11.305	91	22625	2.678	ug/l	100
79) 2-Chlorotoluene	11.378	91	1483	0.289	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	8421	1.379	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.079	75	51414	78.369	ug/l #	3
83) tert-Butylbenzene	11.756	119	3718	0.652	ug/l #	59
84) 1,2,4-Trimethylbenzene	11.756	105	32336	5.293	ug/l	98
85) sec-Butylbenzene	11.896	105	1488	0.202	ug/l	99
89) n-Butylbenzene	12.317	91	1757	0.331	ug/l #	11
90) Hexachloroethane	12.616	117	1067	3.166	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	13.170	75	101	0.210	ug/l #	3
95) Naphthalene	13.780	128	5458	0.849	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012722\
Data File : VX026620.D
Acq On : 27 Jan 2022 13:36
Operator : JC/MD
Sample : N1286-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-30

Quant Time: Jan 28 04:25:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012722\
Data File : VX026620.D
Acq On : 27 Jan 2022 13:36
Operator : JC/MD
Sample : N1286-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-30

Quant Time: Jan 28 04:25:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




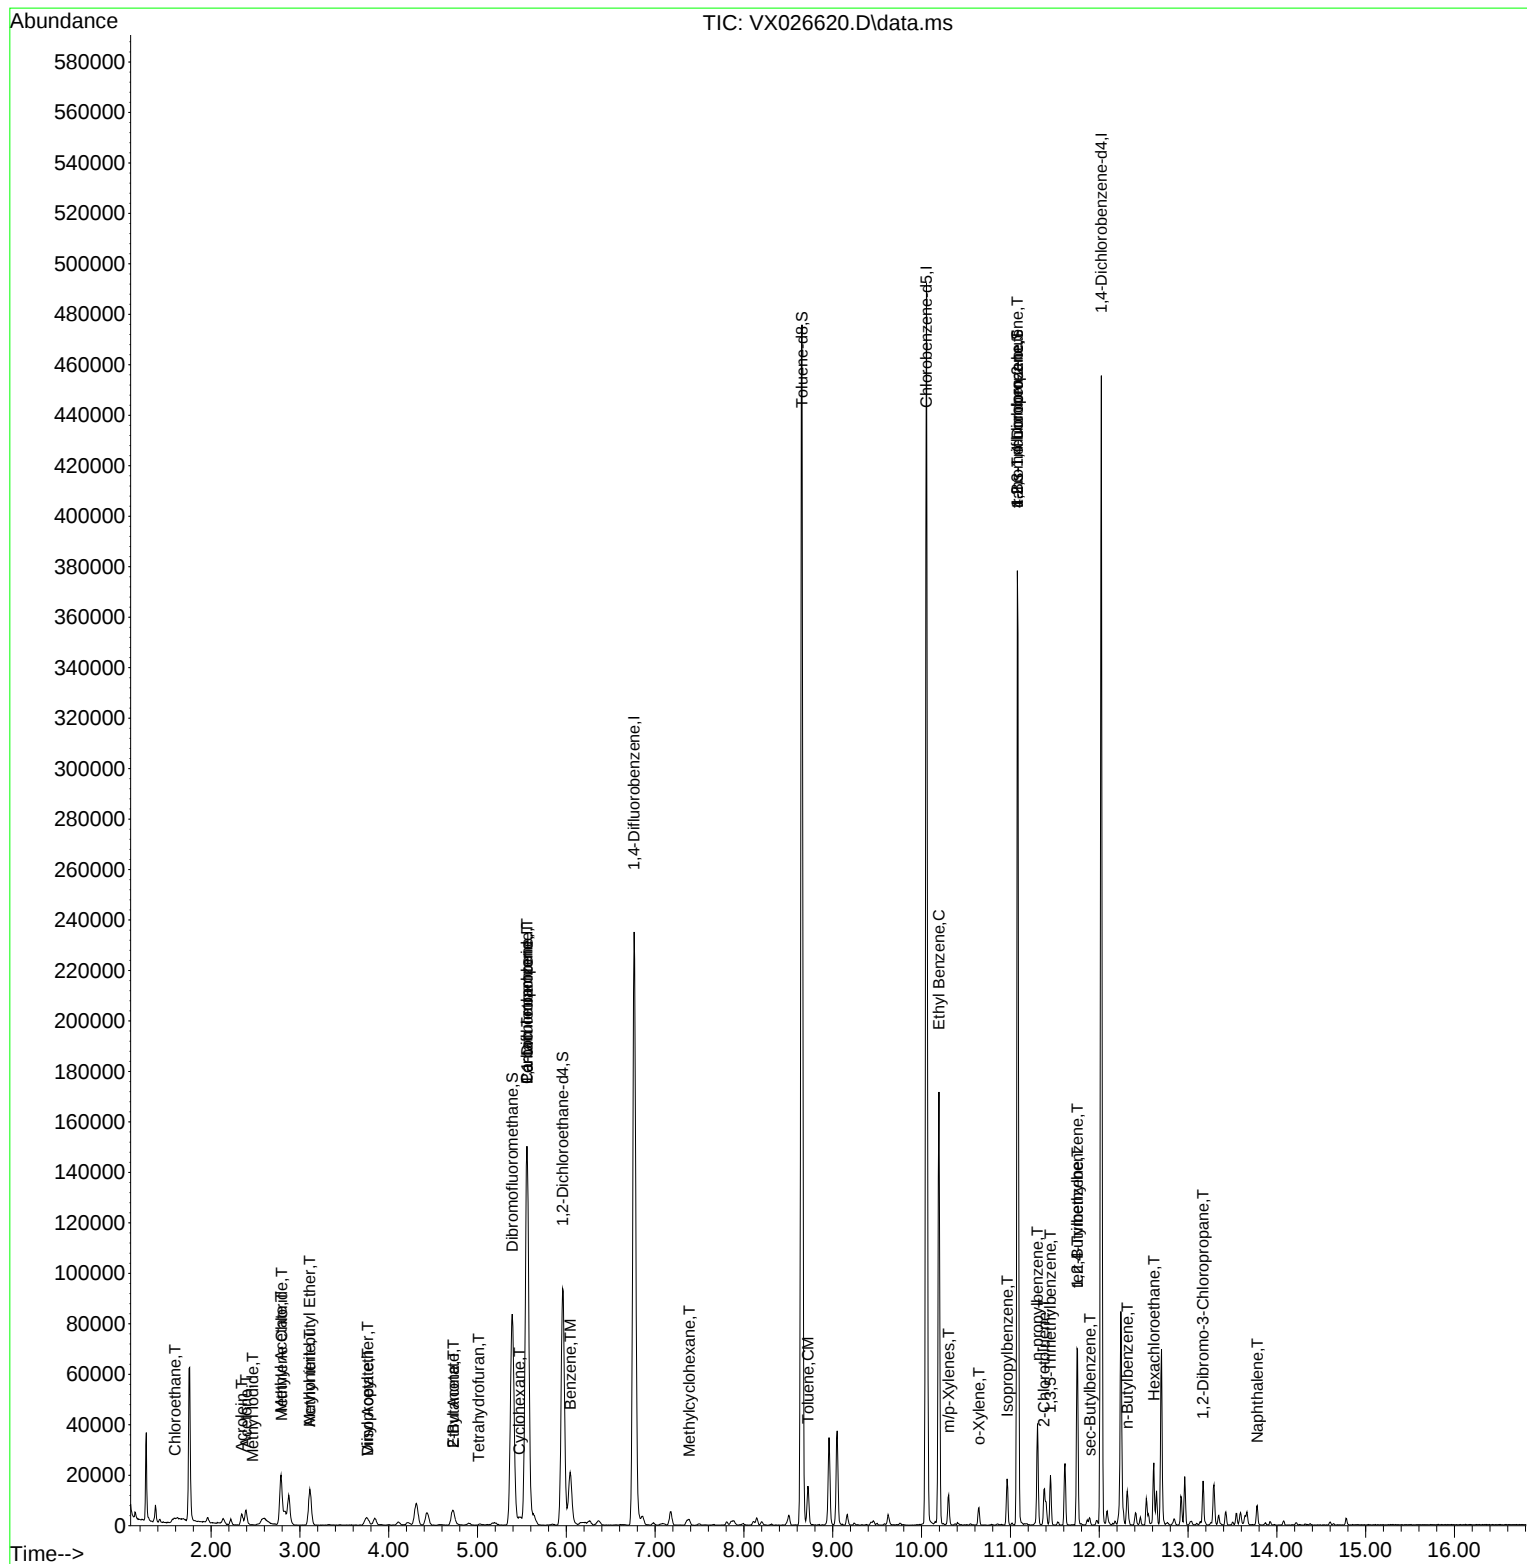




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion:168 Resp: 141808
Ion Ratio Lower Upper
168 100
99 62.0 50.3 75.5



#6
Chloroethane
Concen: 3.909 ug/l
RT: 1.593 min Scan# 83
Delta R.T. -0.098 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 64 Resp: 3186
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#


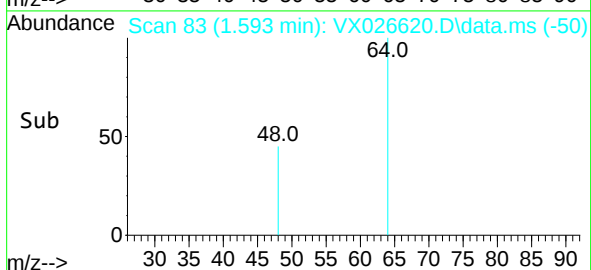






#10
Methyl Iodide
Concen: 4.542 ug/l
RT: 2.465 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion:142 Resp: 178
Ion Ratio Lower Upper
142 100
127 0.0 38.1 57.1#
141 0.0 11.2 16.8#

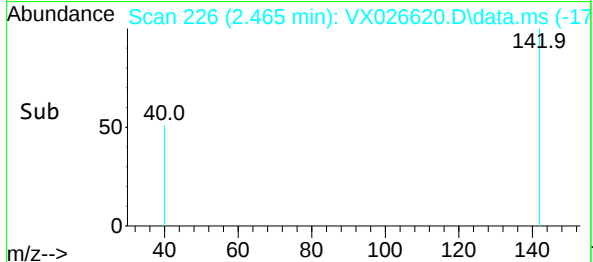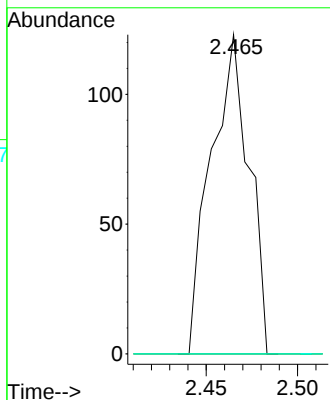

#13
Acrolein
Concen: 2.097 ug/l
RT: 2.343 min Scan# 206
Delta R.T. 0.104 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 56 Resp: 614
Ion Ratio Lower Upper
56 100
55 49.8 56.9 85.3#

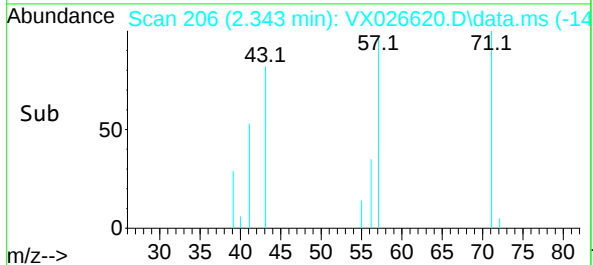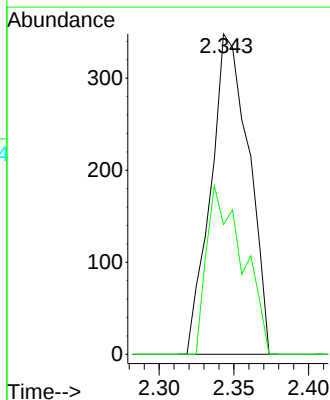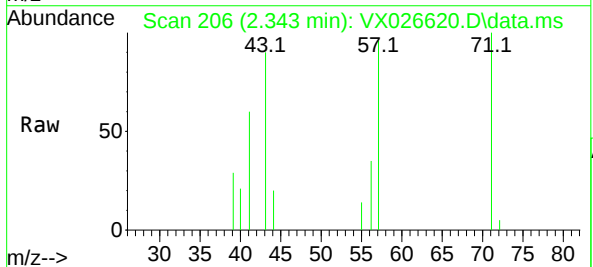



#15

Acrylonitrile

Concen: 0.302 ug/l

RT: 3.111 min Scan# 31

Delta R.T. 0.043 min

Lab File: VX026620.D

Acq: 27 Jan 2022 13:36

Instrument :

MSVOA_X

ClientSampleId :

MW-30





Tgt Ion: 53 Resp: 256

Ion Ratio Lower Upper

53 100

52 0.0 66.6 100.0#

51 49.6 29.5 44.3#



#16

Acetone

Concen: 7.055 ug/l

RT: 2.392 min Scan# 214

Delta R.T. 0.000 min

Lab File: VX026620.D




Acq: 27 Jan 2022 13:36


Tgt Ion: 43 Resp: 7127

Ion Ratio Lower Upper

43 100

58 35.3 23.0 34.6#


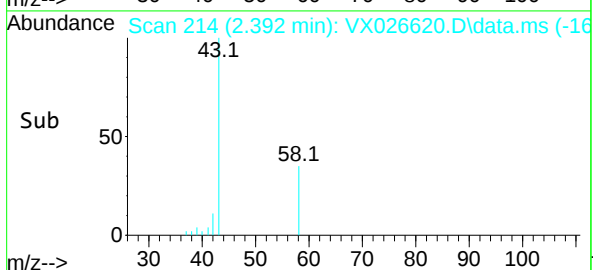

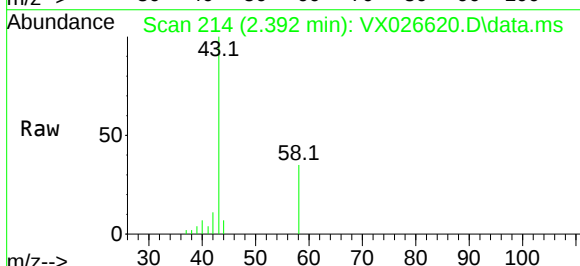




#18
Methyl Acetate
Concen: 8.478 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.079 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion: 43 Resp: 17026
Ion Ratio Lower Upper
43 100
74 0.0 18.3 27.5#

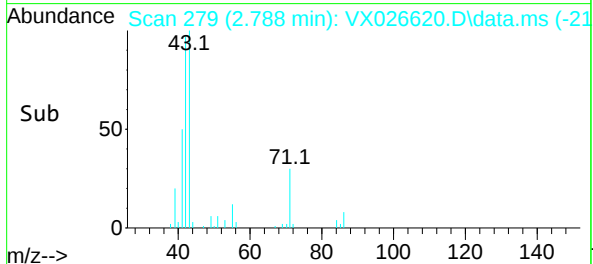

#19
Methyl tert-butyl Ether
Concen: 1.671 ug/l
RT: 3.111 min Scan# 332
Delta R.T. -0.006 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36


Tgt Ion: 73 Resp: 8979
Ion Ratio Lower Upper
73 100
57 69.9 17.4 26.2#

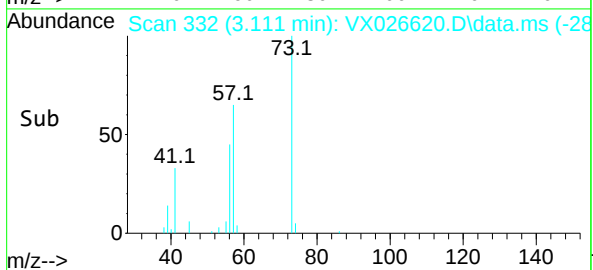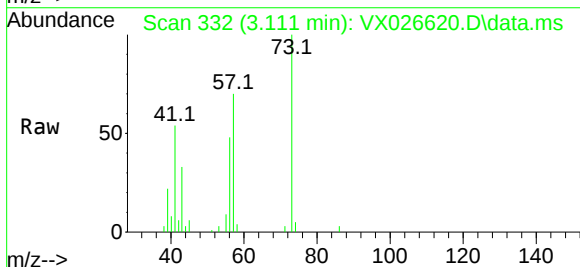






#20
Methylene Chloride
Concen: 0.292 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Instrument :
MSVOA_X
ClientSampleId :
MW-30







Tgt Ion:	84	Resp:	487
Ion	Ratio	Lower	Upper
84	100		
49	100.7	101.5	152.3#
51	59.3	31.2	46.8#
86	104.7	51.3	76.9#



#22
Diisopropyl ether
Concen: 0.440 ug/l
RT: 3.764 min Scan# 439
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion:	45	Resp:	2433
Ion	Ratio	Lower	Upper
45	100		
43	56.5	60.6	91.0#
87	23.4	22.0	33.0
59	16.2	9.0	13.4#


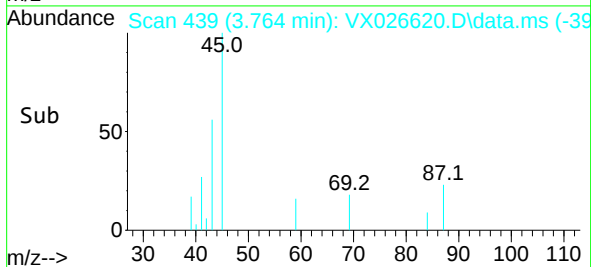

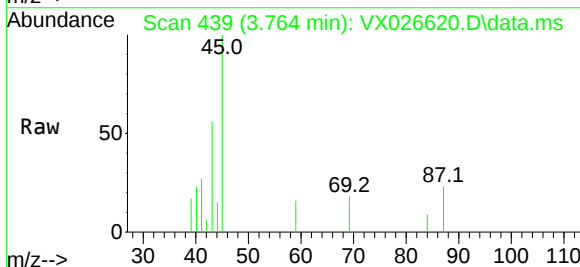




#23
 Vinyl Acetate
 Concen: 0.298 ug/l
 RT: 3.764 min Scan# 41
 Delta R.T. 0.037 min
 Lab File: VX026620.D
 Acq: 27 Jan 2022 13:36




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-30


Tgt Ion: 43 Resp: 1359
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.1 12.1#

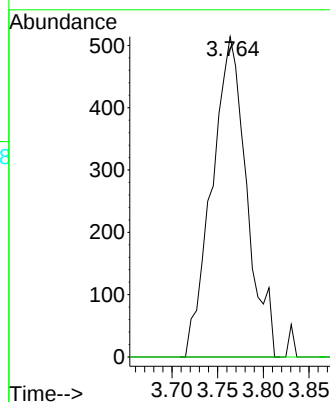

#25
 2-Butanone
 Concen: 8.760 ug/l
 RT: 4.727 min Scan# 597
 Delta R.T. 0.165 min
 Lab File: VX026620.D
 Acq: 27 Jan 2022 13:36

Tgt Ion: 43 Resp: 11509
 Ion Ratio Lower Upper
 43 100
 72 0.0 20.4 30.6#

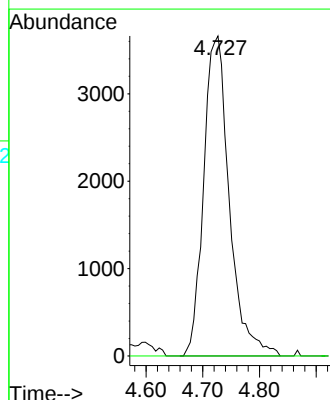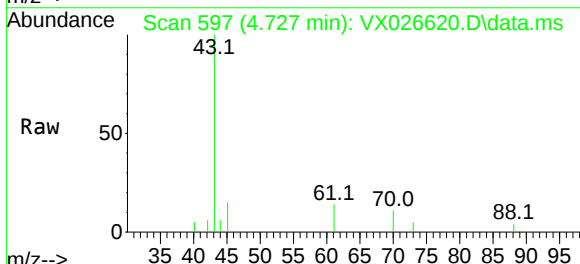



#29

Tetrahydrofuran

Concen: 0.235 ug/l

RT: 5.013 min Scan# 644

Delta R.T. 0.000 min

Lab File: VX026620.D

Acq: 27 Jan 2022 13:36

Instrument :

MSVOA_X

ClientSampleId :

MW-30





Tgt Ion: 42 Resp: 183

Ion Ratio Lower Upper

42 100

72 35.5 34.6 52.0

71 60.1 31.8 47.8#

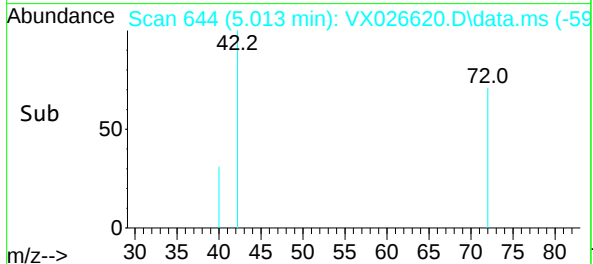

#31

Cyclohexane

Concen: 0.831 ug/l

RT: 5.471 min Scan# 719

Delta R.T. -0.006 min

Lab File: VX026620.D

Acq: 27 Jan 2022 13:36




Tgt Ion: 56 Resp: 2429


Ion Ratio Lower Upper

56 100

69 28.8 25.8 38.6

84 71.2 68.9 103.3


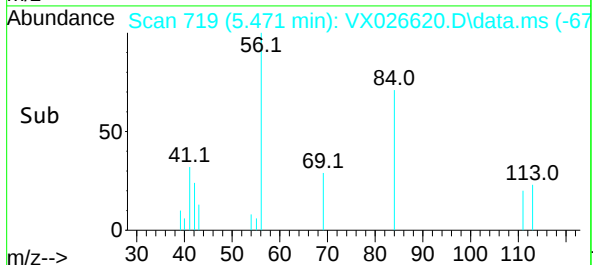

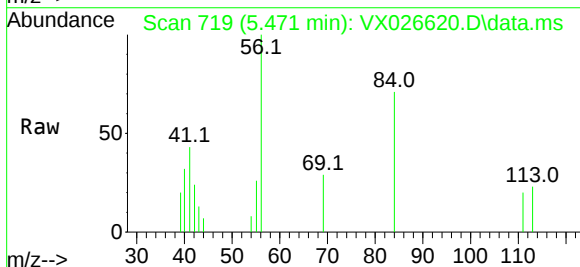




#33
 1,2-Dichloroethane-d4
 Concen: 46.443 ug/l
 RT: 5.958 min Scan# 799
 Delta R.T. 0.000 min
 Lab File: VX026620.D
 Acq: 27 Jan 2022 13:36




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-30


Tgt Ion: 65 Resp: 92002
 Ion Ratio Lower Upper
 65 100
 67 51.8 0.0 100.8

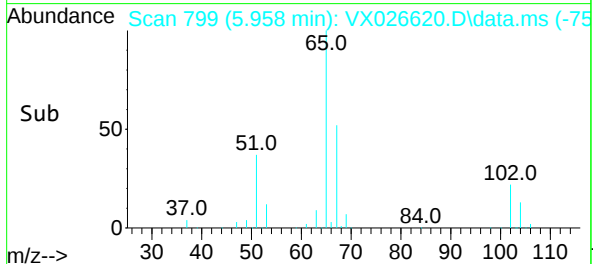

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. 0.000 min
 Lab File: VX026620.D
 Acq: 27 Jan 2022 13:36

Tgt Ion: 114 Resp: 240948
 Ion Ratio Lower Upper
 114 100
 63 20.2 0.0 42.8
 88 16.3 0.0 33.0

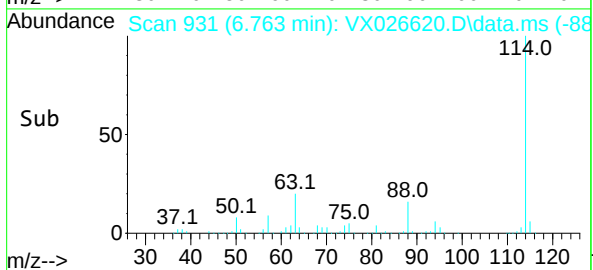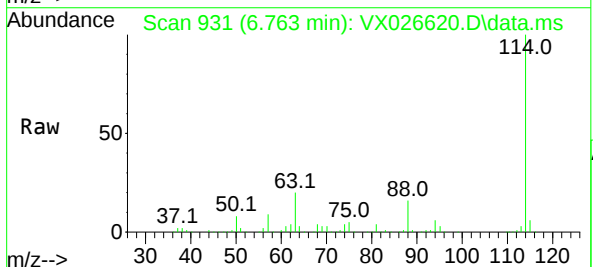



#35

Dibromofluoromethane

Concen: 47.887 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX026620.D


Acq: 27 Jan 2022 13:36

Instrument :

MSVOA_X

ClientSampleId :

MW-30






Tgt Ion:113 Resp: 74511

Ion Ratio Lower Upper

113 100

111 102.4 81.2 121.8

192 19.4 15.0 22.4



#36

1,1-Dichloropropene

Concen: 4.588 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX026620.D

Acq: 27 Jan 2022 13:36




Tgt Ion: 75 Resp: 11269


Ion Ratio Lower Upper

75 100

110 9.3 17.2 51.6#

77 0.0 24.6 36.8#

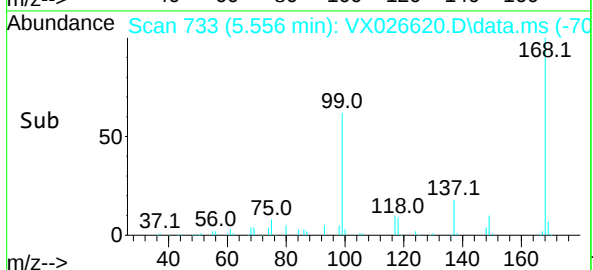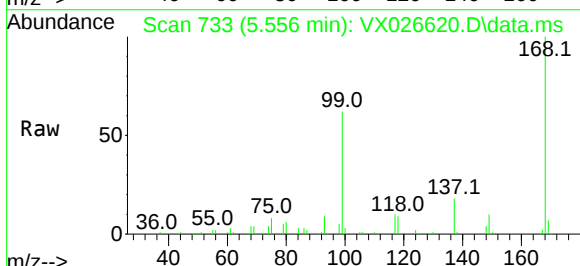



#37

Ethyl Acetate

Concen: 4.632 ug/l

RT: 4.727 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX026620.D

Acq: 27 Jan 2022 13:36

Instrument :

MSVOA_X

ClientSampleId :

MW-30





Tgt Ion: 43 Resp: 11509

Ion Ratio Lower Upper

43 100

61 13.5 10.6 16.0

70 10.9 8.5 12.7

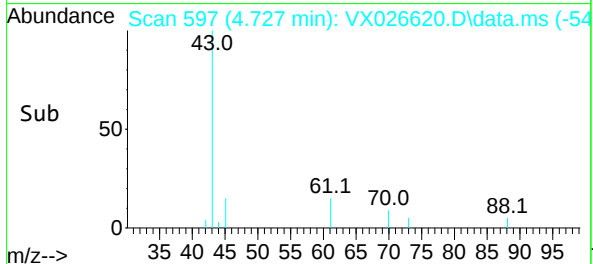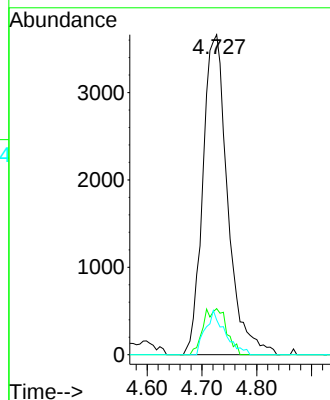

#38

Carbon Tetrachloride

Concen: 5.804 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.128 min

Lab File: VX026620.D

Acq: 27 Jan 2022 13:36




Tgt Ion: 117 Resp: 14665


Ion Ratio Lower Upper

117 100

119 4.7 74.7 112.1#

121 0.0 25.4 38.0#

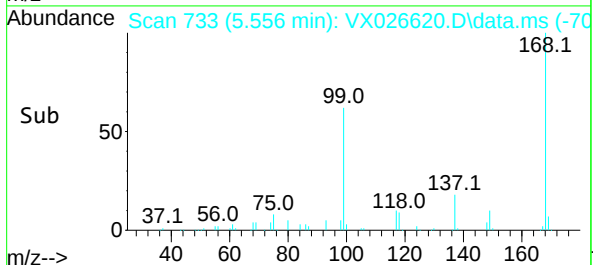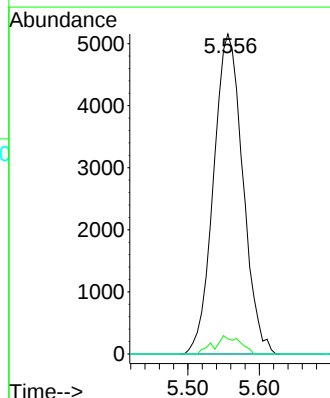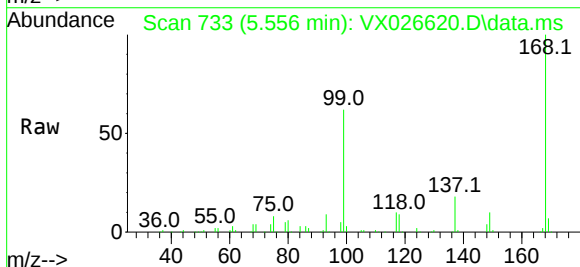



#39

Methylcyclohexane

Concen: 0.354 ug/l

RT: 7.385 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX026620.D

Acq: 27 Jan 2022 13:36

Instrument :

MSVOA_X

ClientSampleId :

MW-30





Tgt Ion: 83 Resp: 1048

Ion Ratio Lower Upper

83 100

55 87.4 63.6 95.4

98 43.3 38.4 57.6

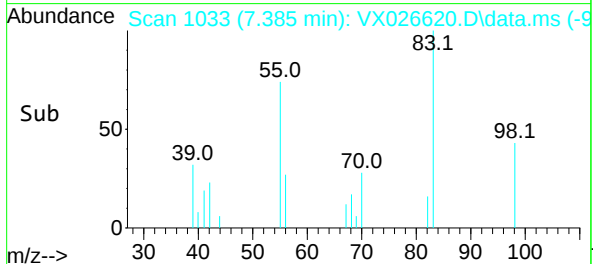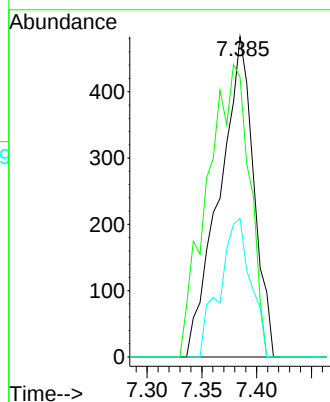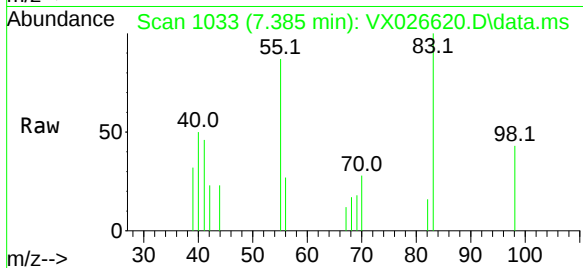

#40

Benzene

Concen: 3.679 ug/l

RT: 6.044 min Scan# 813

Delta R.T. 0.000 min

Lab File: VX026620.D




Acq: 27 Jan 2022 13:36


Tgt Ion: 78 Resp: 24978

Ion Ratio Lower Upper

78 100

77 25.5 18.9 28.3


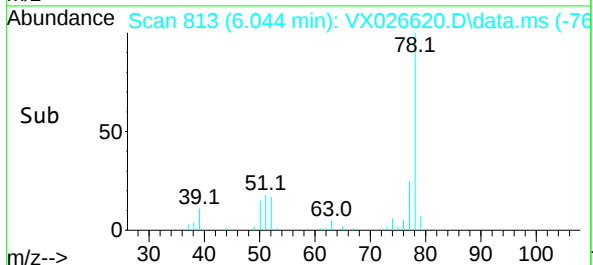
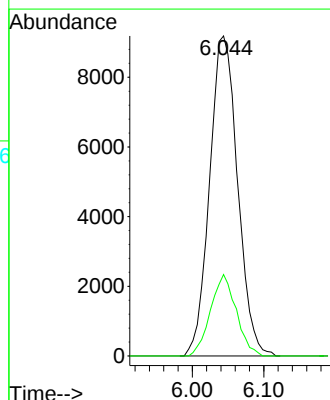
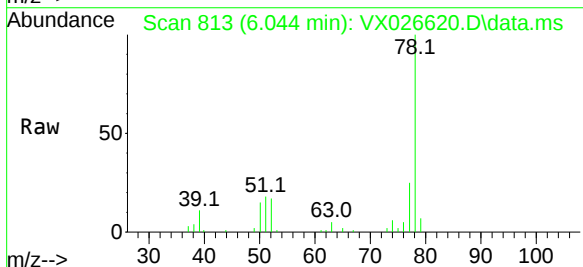




#50
Toluene-d8
Concen: 50.676 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion: 98 Resp: 284140
Ion Ratio Lower Upper
98 100
100 66.6 53.2 79.8



#52
Toluene
Concen: 1.398 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 92 Resp: 5822
Ion Ratio Lower Upper
92 100
91 171.3 135.7 203.5




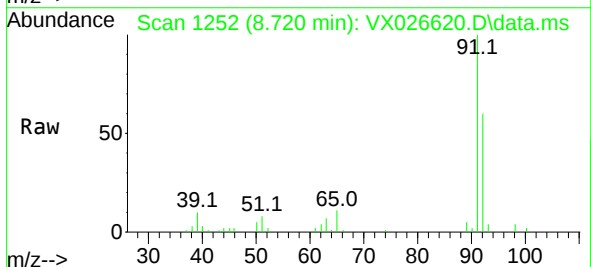




#62
4-Bromofluorobenzene
Concen: 51.523 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion: 95 Resp: 102625
Ion Ratio Lower Upper
95 100
174 74.8 0.0 148.6
176 72.8 0.0 141.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 117 Resp: 216579
Ion Ratio Lower Upper
117 100
82 57.0 45.2 67.8
119 32.1 26.2 39.2


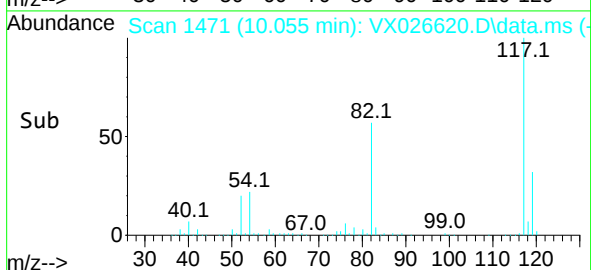

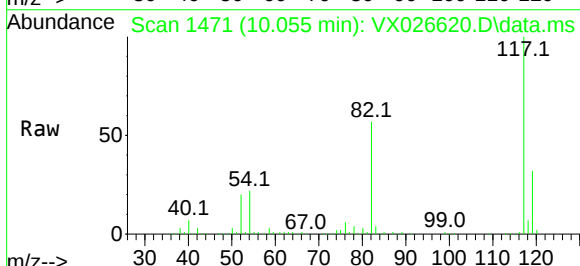




#67
Ethyl Benzene
Concen: 11.677 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion: 91 Resp: 96776
Ion Ratio Lower Upper
91 100
106 30.7 24.7 37.1

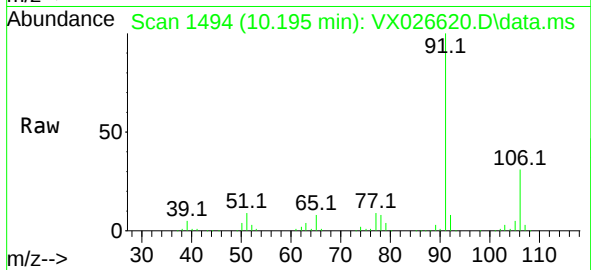

#68
m/p-Xylenes
Concen: 0.905 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 106 Resp: 2808
Ion Ratio Lower Upper
106 100
91 213.8 165.3 247.9


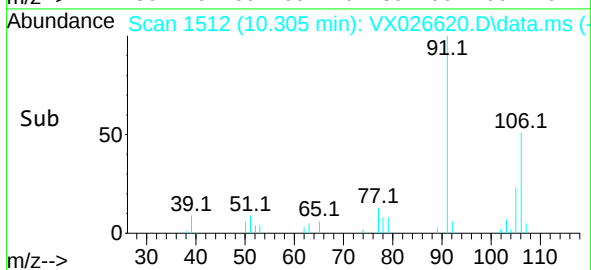

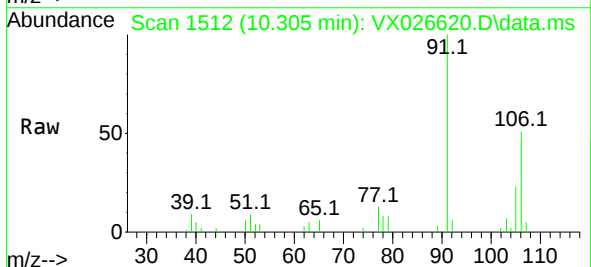




#69
o-Xylene
Concen: 0.487 ug/l
RT: 10.646 min Scan# 1567
Delta R.T. 0.006 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion:106 Resp: 1457
Ion Ratio Lower Upper
106 100
91 226.8 109.7 329.0

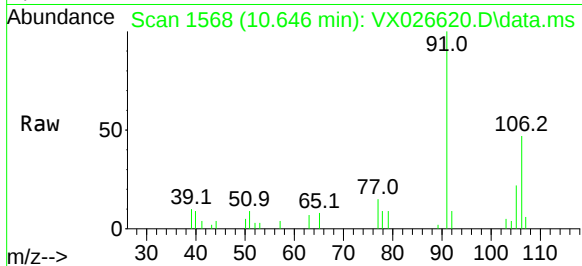

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion:152 Resp: 90377
Ion Ratio Lower Upper
152 100
115 62.1 44.2 132.6
150 158.3 0.0 348.2


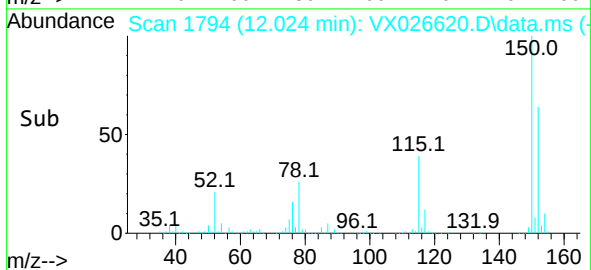

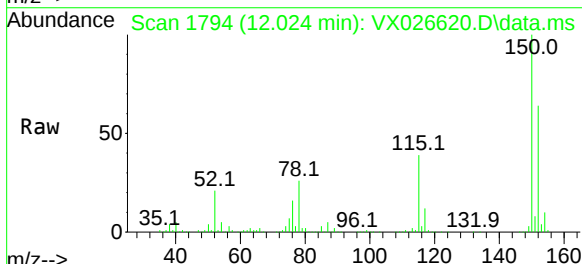




#73
Isopropylbenzene
Concen: 1.262 ug/l
RT: 10.963 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion:105 Resp: 9349
Ion Ratio Lower Upper
105 100
120 27.0 13.1 39.1

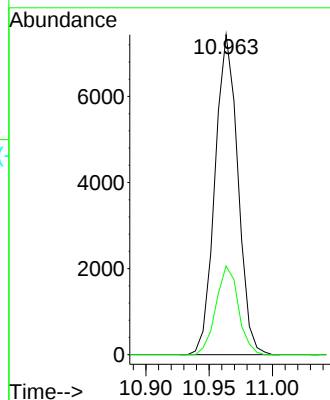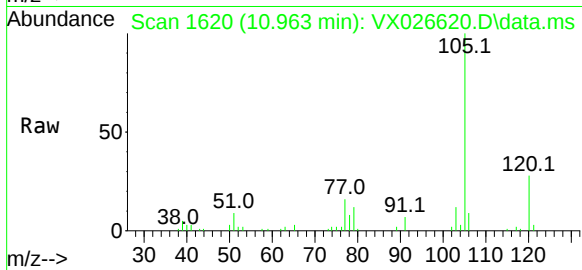

#76
1,2,3-Trichloropropane
Concen: 25.837 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 75 Resp: 51414
Ion Ratio Lower Upper
75 100
77 1.0 18.3 54.8#



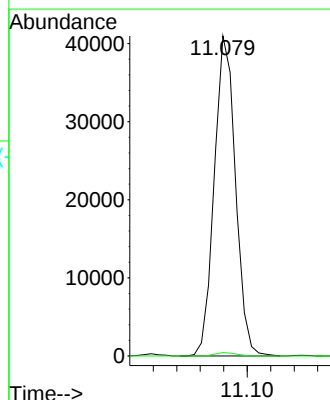
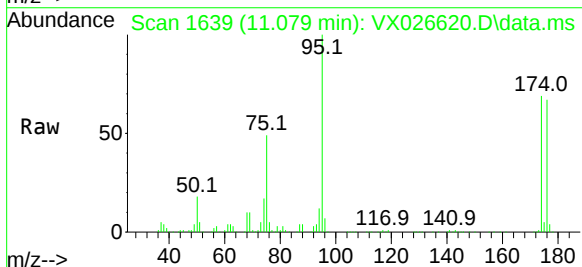




#78
n-propylbenzene
Concen: 2.678 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion: 91 Resp: 22625
Ion Ratio Lower Upper
91 100
120 22.9 11.6 34.7



#79
2-Chlorotoluene
Concen: 0.289 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 91 Resp: 1483
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.2#


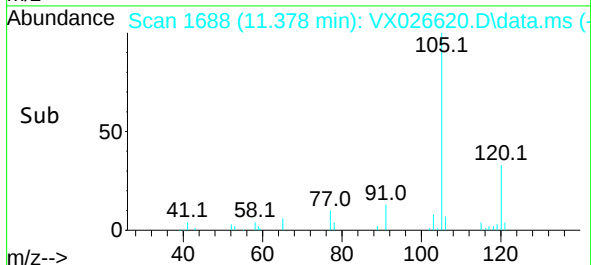

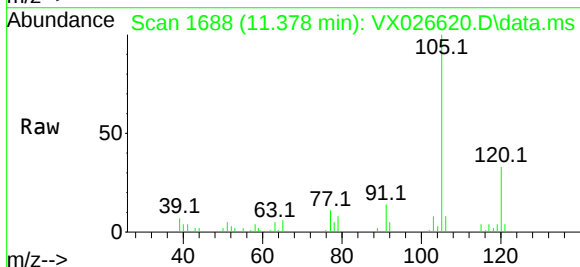




#80
1,3,5-Trimethylbenzene
Concen: 1.379 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion:105 Resp: 8421
Ion Ratio Lower Upper
105 100
120 47.3 24.0 72.0



#81
trans-1,4-Dichloro-2-butene
Concen: 78.369 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 75 Resp: 51414
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#


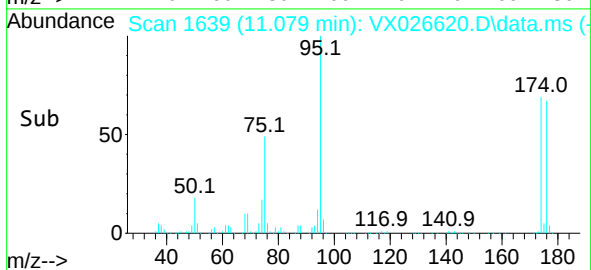

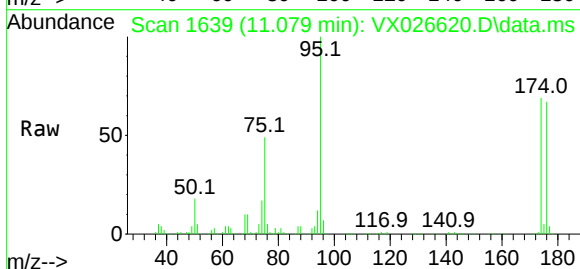




#83
 tert-Butylbenzene
 Concen: 0.652 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.043 min
 Lab File: VX026620.D
 Acq: 27 Jan 2022 13:36




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-30


Tgt Ion:119 Resp: 3718
 Ion Ratio Lower Upper
 119 100
 91 92.2 31.4 94.0
 134 0.0 11.8 35.3#

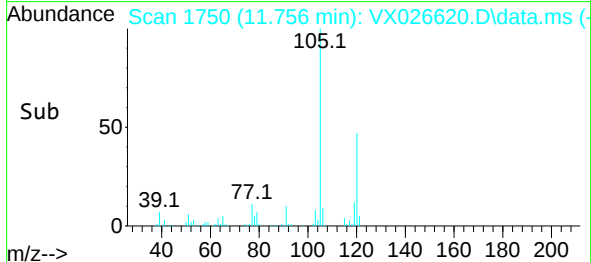

#84
 1,2,4-Trimethylbenzene
 Concen: 5.293 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.006 min
 Lab File: VX026620.D
 Acq: 27 Jan 2022 13:36

Tgt Ion:105 Resp: 32336
 Ion Ratio Lower Upper
 105 100
 120 44.7 21.9 65.5


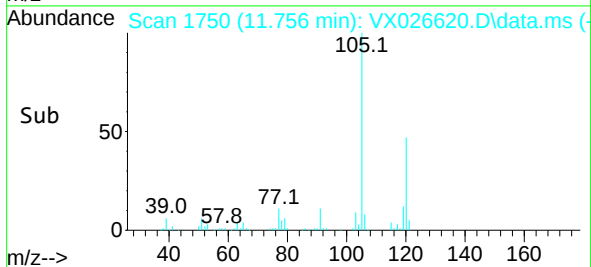

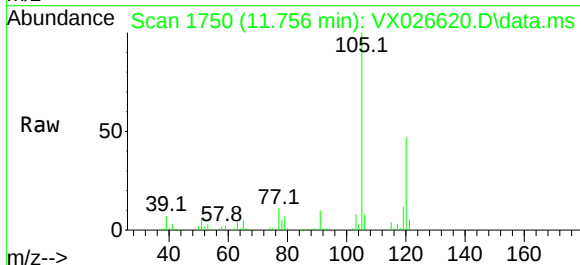




#85
 sec-Butylbenzene
 Concen: 0.202 ug/l
 RT: 11.896 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX026620.D
 Acq: 27 Jan 2022 13:36




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-30


Tgt Ion:105 Resp: 1488
 Ion Ratio Lower Upper
 105 100
 134 19.6 10.1 30.1

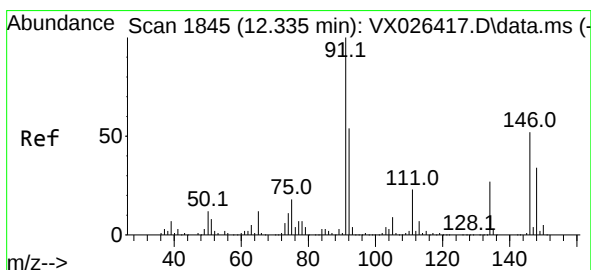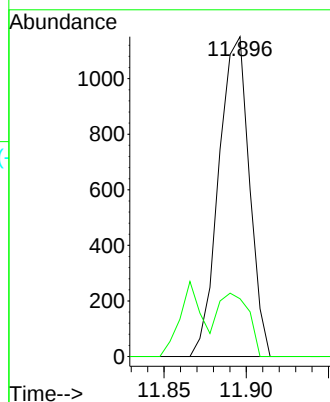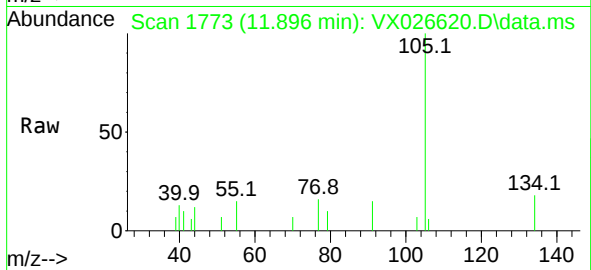

#89
 n-Butylbenzene
 Concen: 0.331 ug/l
 RT: 12.317 min Scan# 1842
 Delta R.T. -0.018 min
 Lab File: VX026620.D
 Acq: 27 Jan 2022 13:36

Tgt Ion: 91 Resp: 1757
 Ion Ratio Lower Upper
 91 100
 92 27.6 27.2 81.6
 134 126.6 13.1 39.1#


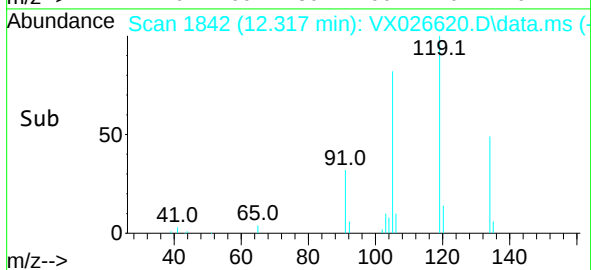
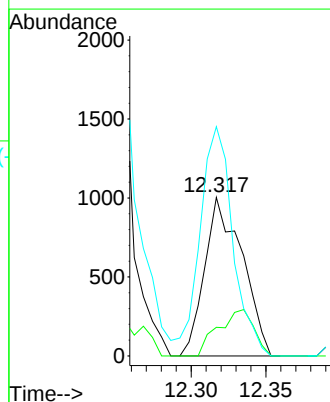
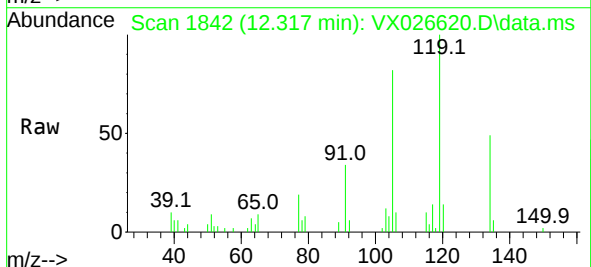




#90
Hexachloroethane
Concen: 3.166 ug/l
RT: 12.616 min Scan# 117
Delta R.T. 0.074 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36




Instrument :
MSVOA_X
ClientSampleId :
MW-30


Tgt Ion:117 Resp: 1067
Ion Ratio Lower Upper
117 100
201 0.0 35.6 106.8#

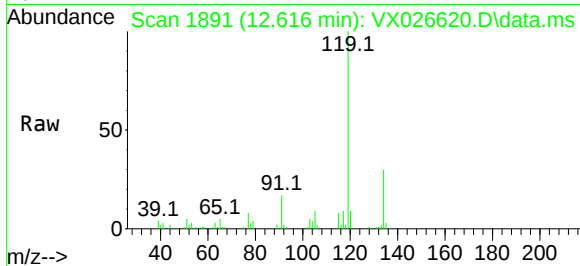

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.210 ug/l
RT: 13.170 min Scan# 1982
Delta R.T. 0.226 min
Lab File: VX026620.D
Acq: 27 Jan 2022 13:36

Tgt Ion: 75 Resp: 101
Ion Ratio Lower Upper
75 100
155 0.0 40.0 119.9#
157 0.0 51.6 154.8#

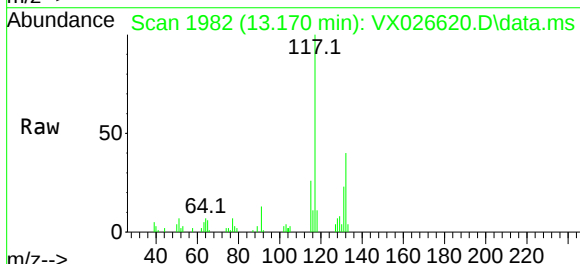



#95

Naphthalene

Concen: 0.849 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.006 min

Lab File: VX026620.D


Acq: 27 Jan 2022 13:36

Instrument :

MSVOA_X

ClientSampleId :

MW-30

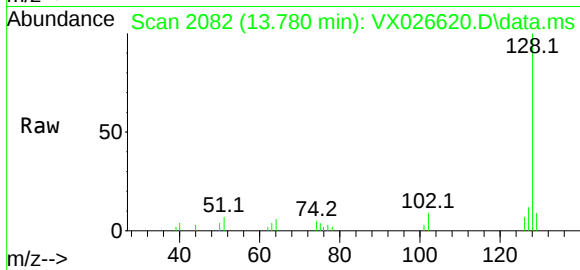

Tgt Ion:128 Resp: 5458

Ion Ratio Lower Upper

128 100

127 11.9 10.3 15.5

129 12.5 8.7 13.1

