

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012722\
 Data File : VX026637.D
 Acq On : 27 Jan 2022 20:07
 Operator : JC/MD
 Sample : N1297-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-14DA

Quant Time: Jan 28 04:28:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	126476	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	212502	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	188109	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	74537	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	83678	47.362	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.720%
35) Dibromofluoromethane	5.391	113	67266	49.018	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.040%
50) Toluene-d8	8.653	98	248890	50.331	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.660%
62) 4-Bromofluorobenzene	11.079	95	87015	49.534	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.060%


Target Compounds				Qvalue		
11) Tert butyl alcohol	3.014	59	170	0.692	ug/l #	75
13) Acrolein	2.343	56	2957	11.322	ug/l #	76
14) Allyl chloride	2.587	41	657	0.270	ug/l #	25
15) Acrylonitrile	3.111	53	2021	2.671	ug/l #	41
16) Acetone	2.392	43	1380	1.532	ug/l	99
18) Methyl Acetate	2.788	43	47713	26.637	ug/l #	53
19) Methyl tert-butyl Ether	3.117	73	6372	1.330	ug/l #	1
20) Methylene Chloride	2.794	84	423	0.284	ug/l #	1
25) 2-Butanone	4.586	43	243	0.207	ug/l #	50
27) cis-1,2-Dichloroethene	4.495	96	402	0.246	ug/l	92
30) Chloroform	5.105	83	2551	0.921	ug/l	98
31) Cyclohexane	5.483	56	1085	0.416	ug/l #	84
36) 1,1-Dichloropropene	5.556	75	9848	4.546	ug/l #	50
38) Carbon Tetrachloride	5.562	117	13095	5.877	ug/l #	16
39) Methylcyclohexane	7.379	83	1566	0.599	ug/l #	80
40) Benzene	6.044	78	10113	1.689	ug/l	98
41) Methacrylonitrile	5.141	41	1144	0.922	ug/l #	30
51) 4-Methyl-2-Pentanone	8.647	43	1394	0.664	ug/l #	1
55) 1,1,2-Trichloroethane	9.104	97	1714	1.196	ug/l #	20
60) Dibromochloromethane	9.275	129	2436	1.631	ug/l #	11
64) Tetrachloroethene	9.275	164	2561	1.441	ug/l	86
73) Isopropylbenzene	10.963	105	34209	5.599	ug/l	100
76) 1,2,3-Trichloropropane	11.079	75	43608	26.572	ug/l #	40
78) n-propylbenzene	11.305	91	2040	0.293	ug/l	95
79) 2-Chlorotoluene	11.305	91	2040	0.483	ug/l #	42
81) trans-1,4-Dichloro-2-b...	11.079	75	43608	80.455	ug/l #	3
85) sec-Butylbenzene	11.890	105	5566	0.915	ug/l	100
86) p-Isopropyltoluene	12.183	119	1049	0.206	ug/l	91
89) n-Butylbenzene	12.335	91	4070	0.929	ug/l	91
90) Hexachloroethane	12.646	117	1557	3.926	ug/l #	14
92) 1,2-Dibromo-3-Chloropr...	13.176	75	93	0.235	ug/l #	3
95) Naphthalene	13.780	128	39248	7.402	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012722\
Data File : VX026637.D
Acq On : 27 Jan 2022 20:07
Operator : JC/MD
Sample : N1297-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-14DA

Quant Time: Jan 28 04:28:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




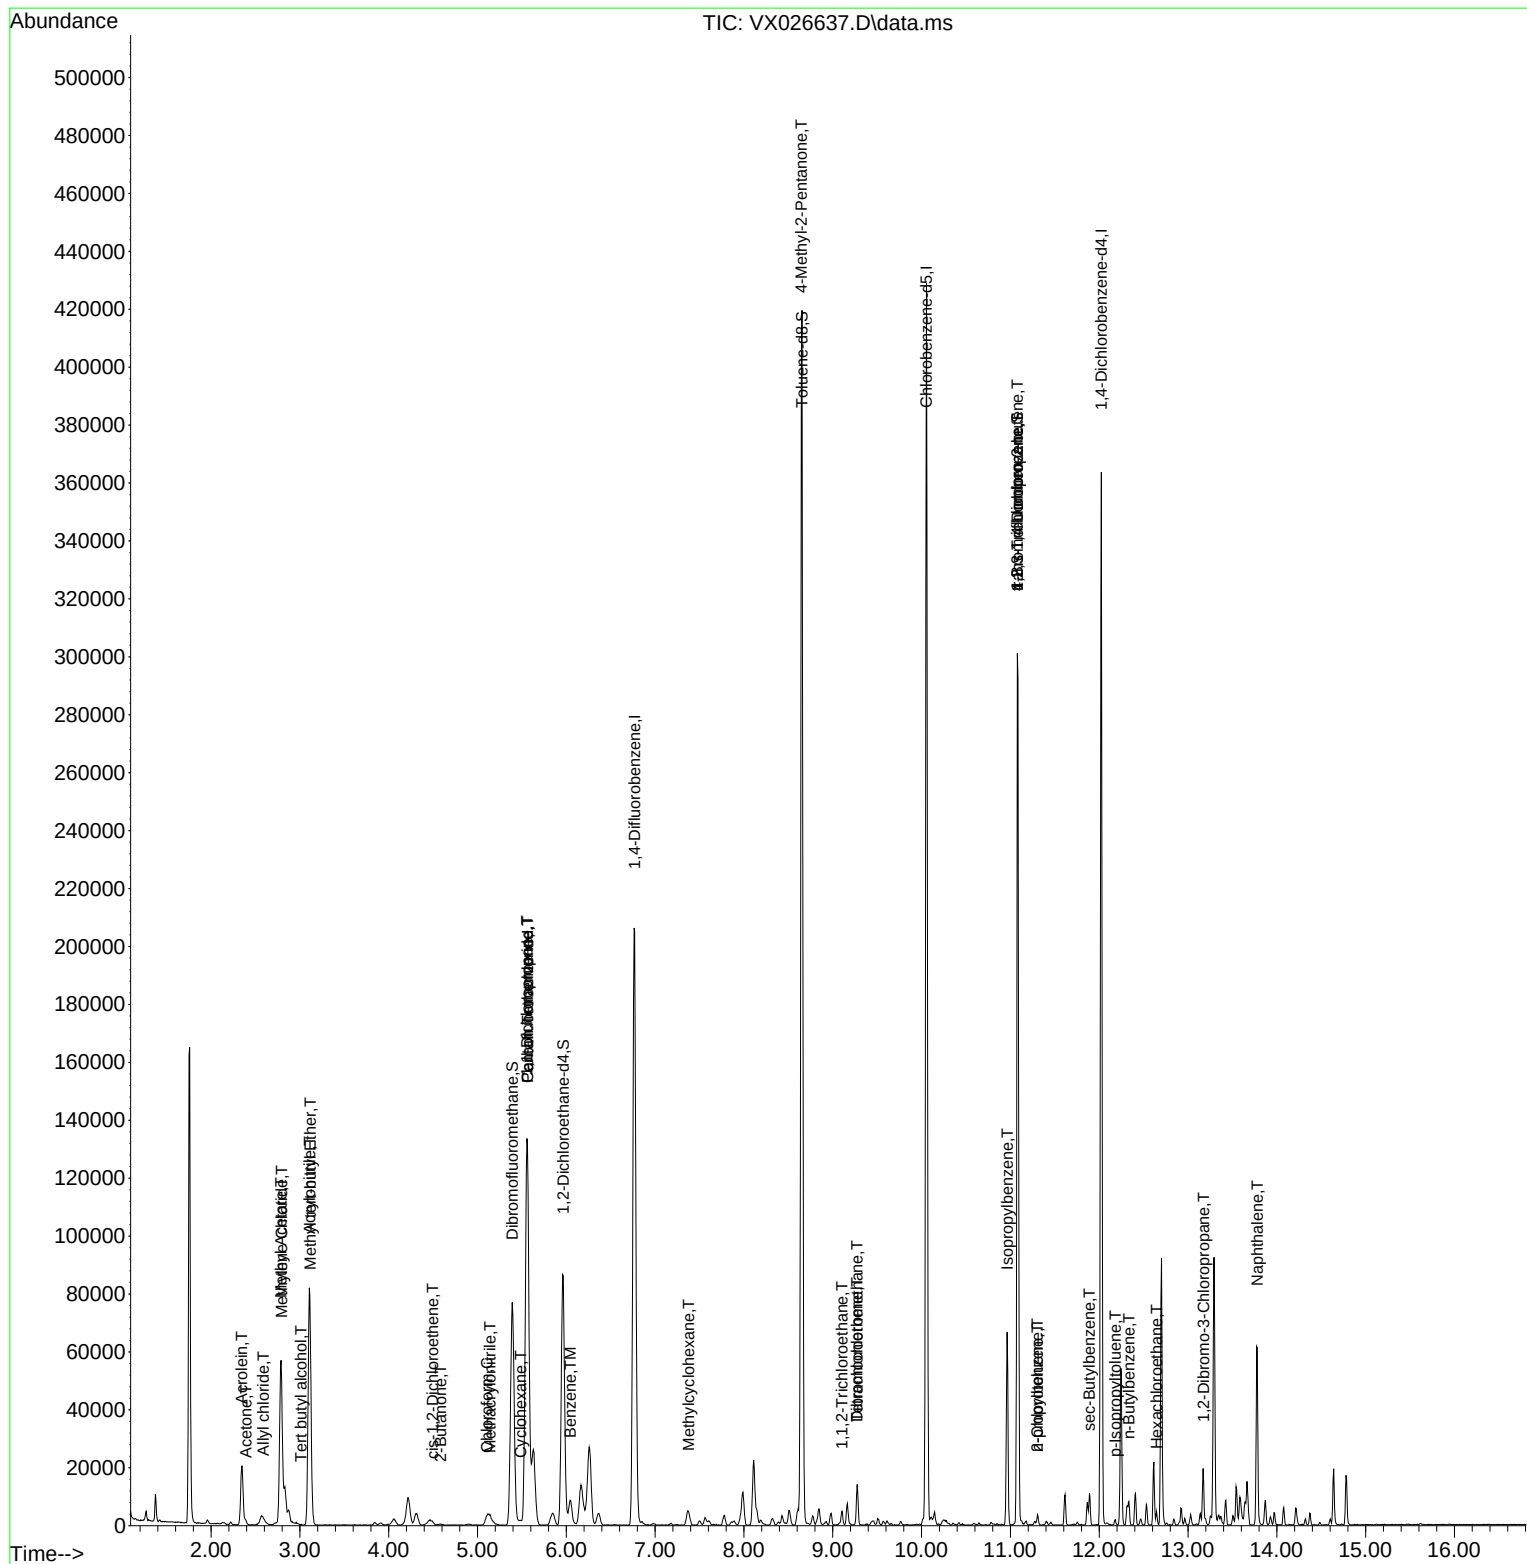




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion:168 Resp: 126476
Ion Ratio Lower Upper
168 100
99 57.7 50.3 75.5

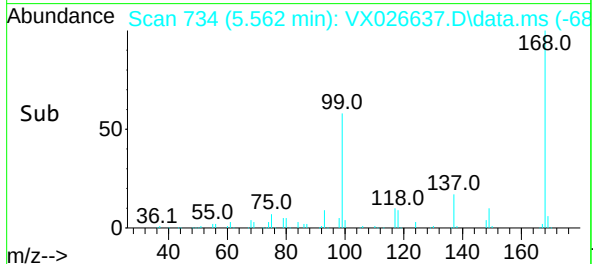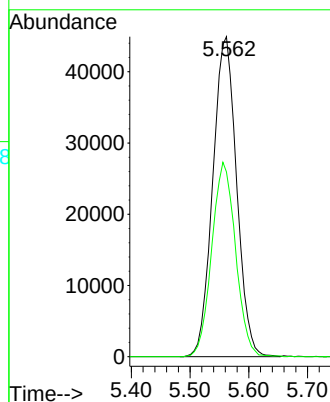

#11
Tert butyl alcohol
Concen: 0.692 ug/l
RT: 3.014 min Scan# 316
Delta R.T. 0.007 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 59 Resp: 170
Ion Ratio Lower Upper
59 100
57 0.0 7.2 10.8#


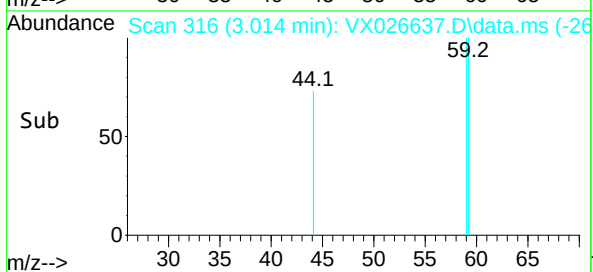
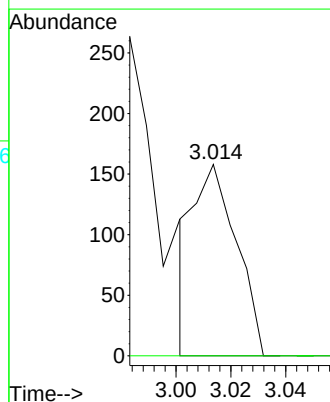





#13
Acrolein
Concen: 11.322 ug/l
RT: 2.343 min Scan# 20
Delta R.T. 0.104 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion: 56 Resp: 2957
Ion Ratio Lower Upper
56 100
55 51.6 56.9 85.3#

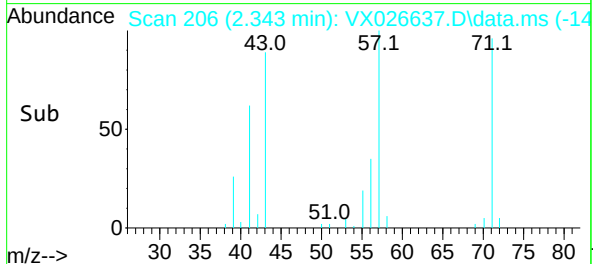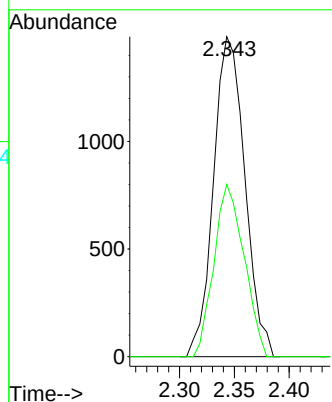

#14
Allyl chloride
Concen: 0.270 ug/l
RT: 2.587 min Scan# 246
Delta R.T. -0.085 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 41 Resp: 657
Ion Ratio Lower Upper
41 100
39 0.0 54.2 81.4#
76 0.0 25.2 37.8#

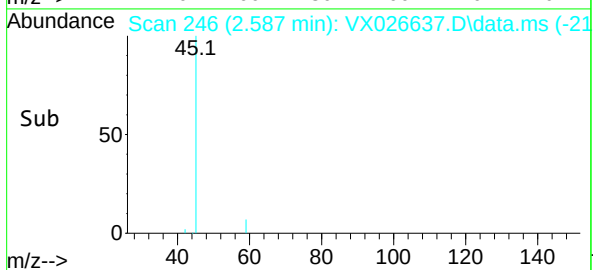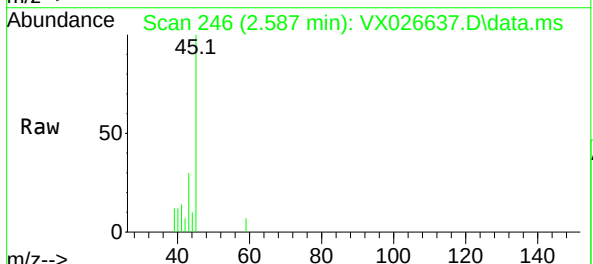



#15

Acrylonitrile

Concen: 2.671 ug/l

RT: 3.111 min Scan# 31

Delta R.T. 0.043 min

Lab File: VX026637.D

Acq: 27 Jan 2022 20:07

Instrument :

MSVOA_X

ClientSampleId :

MW-14DA





Tgt Ion: 53 Resp: 2021

Ion Ratio Lower Upper

53 100

52 18.7 66.6 100.0#

51 54.1 29.5 44.3#

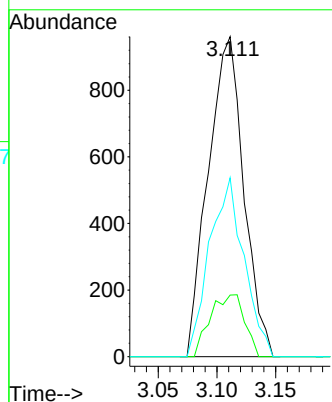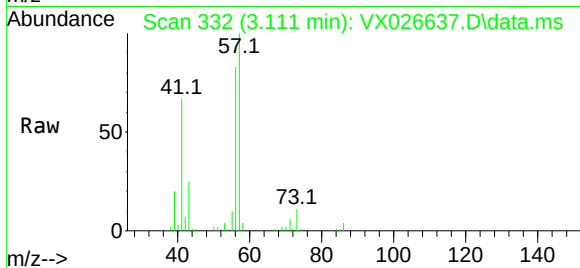

#16

Acetone

Concen: 1.532 ug/l

RT: 2.392 min Scan# 214

Delta R.T. 0.000 min

Lab File: VX026637.D




Acq: 27 Jan 2022 20:07


Tgt Ion: 43 Resp: 1380

Ion Ratio Lower Upper

43 100

58 29.6 23.0 34.6


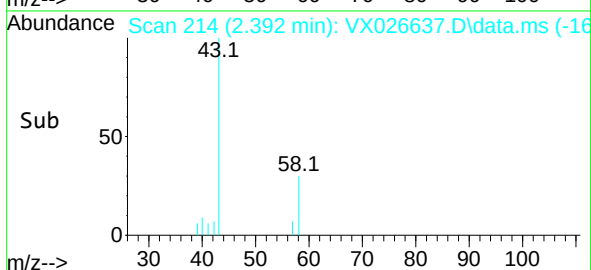
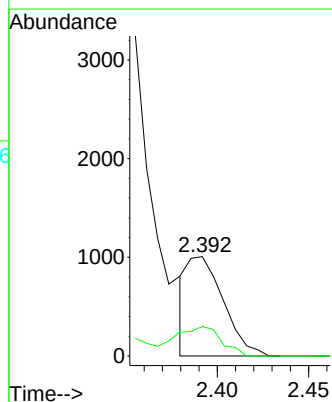
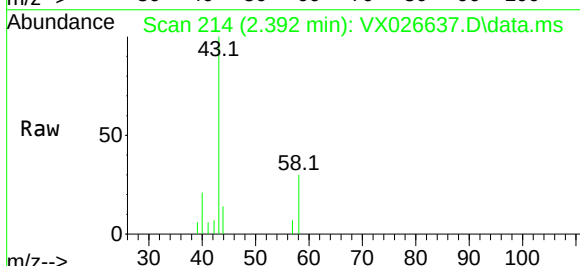




#18
Methyl Acetate
Concen: 26.637 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.079 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion: 43 Resp: 47713
Ion Ratio Lower Upper
43 100
74 0.0 18.3 27.5#

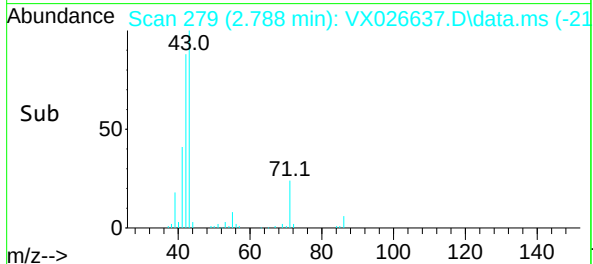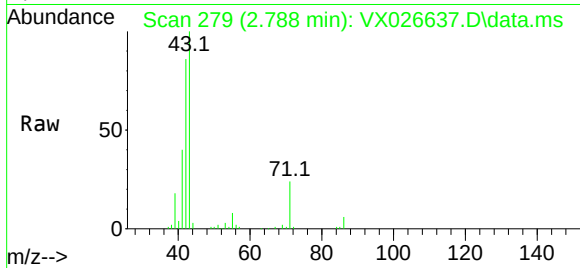

#19
Methyl tert-butyl Ether
Concen: 1.330 ug/l
RT: 3.117 min Scan# 333
Delta R.T. -0.000 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07


Tgt Ion: 73 Resp: 6372
Ion Ratio Lower Upper
73 100
57 635.5 17.4 26.2#

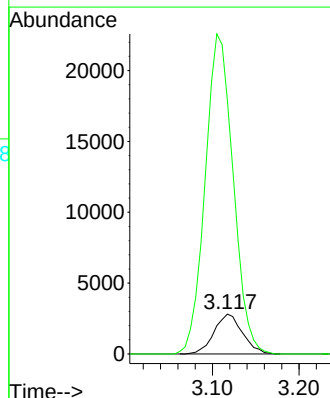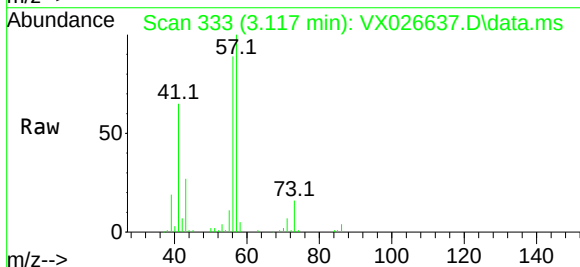





#20
Methylene Chloride
Concen: 0.284 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Instrument :
MSVOA_X
ClientSampleId :
MW-14DA



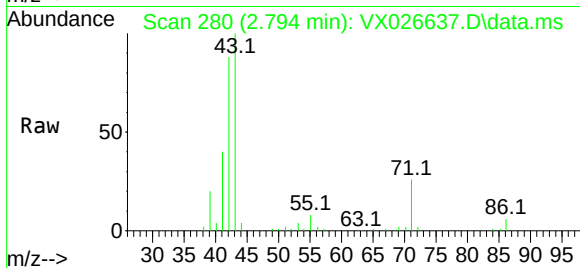



Tgt Ion: 84	Resp: 423
Ion Ratio	Lower Upper
84 100	
49 58.0	101.5 152.3#
51 137.9	31.2 46.8#
86 418.3	51.3 76.9#



#25
2-Butanone
Concen: 0.207 ug/l
RT: 4.586 min Scan# 574
Delta R.T. 0.024 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 43	Resp: 243		
Ion Ratio	Lower	Upper	
43 100			
72 0.0	20.4	30.6#	


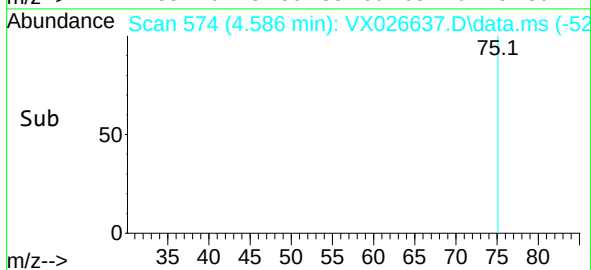
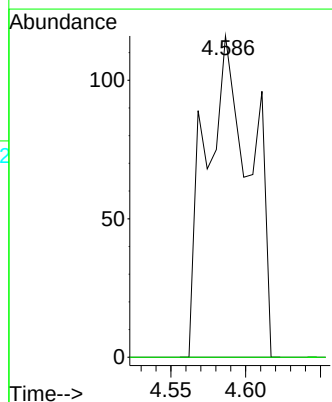
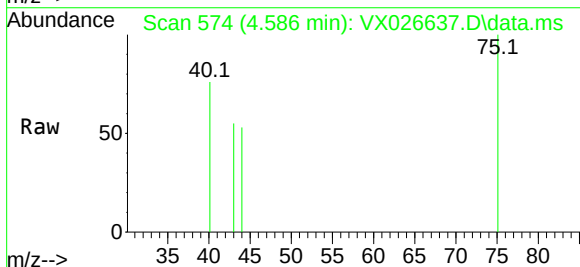




#27
 cis-1,2-Dichloroethene
 Concen: 0.246 ug/l
 RT: 4.495 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: VX026637.D
 Acq: 27 Jan 2022 20:07




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-14DA


Tgt Ion: 96	Resp:	402	
Ion	Ratio	Lower	Upper
96	100		
61	141.5	0.0	296.6
98	52.2	0.0	128.8

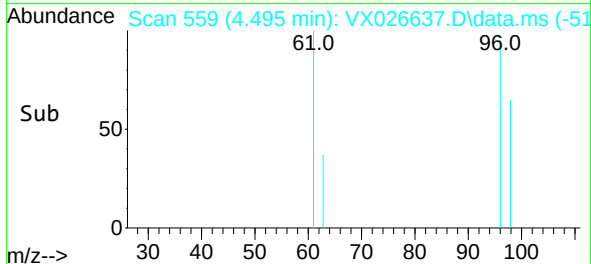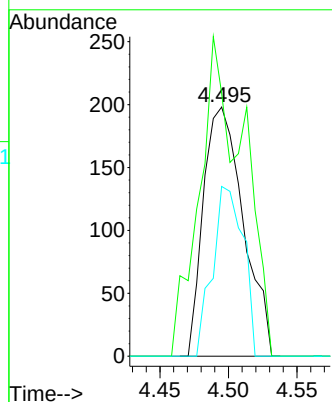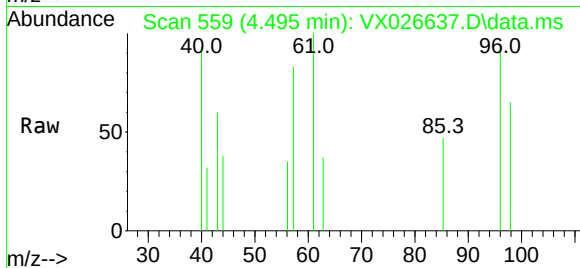

#30
 Chloroform
 Concen: 0.921 ug/l
 RT: 5.105 min Scan# 659
 Delta R.T. 0.006 min
 Lab File: VX026637.D
 Acq: 27 Jan 2022 20:07

Tgt Ion: 83	Resp:	2551	
Ion	Ratio	Lower	Upper
83	100		
85	63.1	51.6	77.4


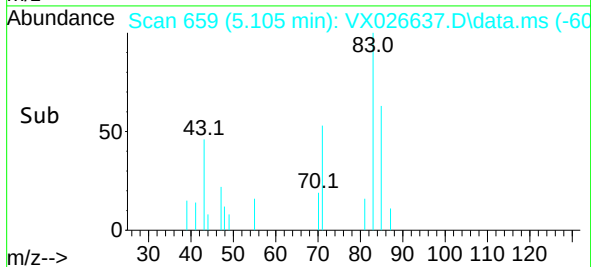
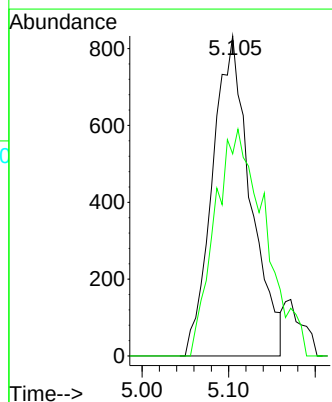
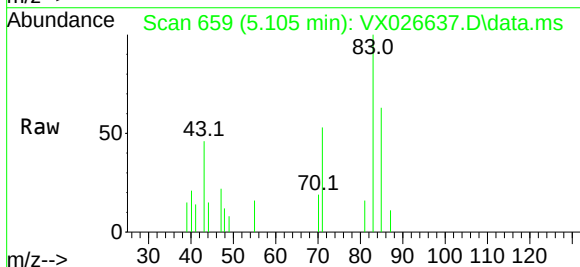




#31
Cyclohexane
Concen: 0.416 ug/l
RT: 5.483 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion: 56 Resp: 1085
Ion Ratio Lower Upper
56 100
69 47.1 25.8 38.6#
84 75.2 68.9 103.3

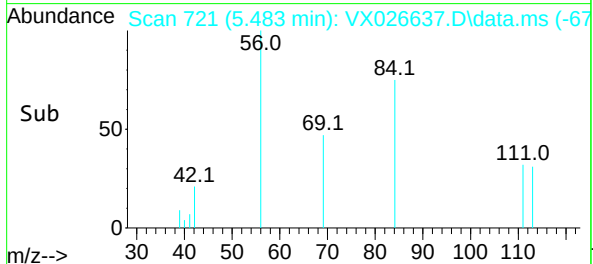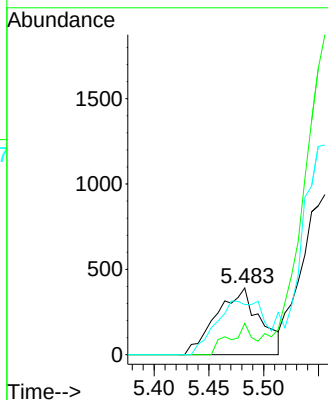

#33
1,2-Dichloroethane-d4
Concen: 47.362 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.006 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 65 Resp: 83678
Ion Ratio Lower Upper
65 100
67 52.1 0.0 100.8



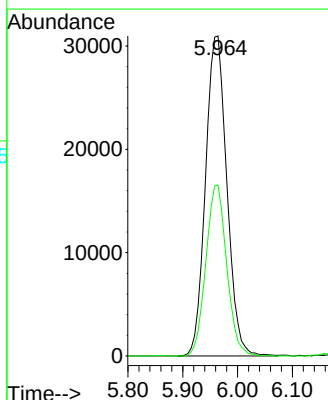
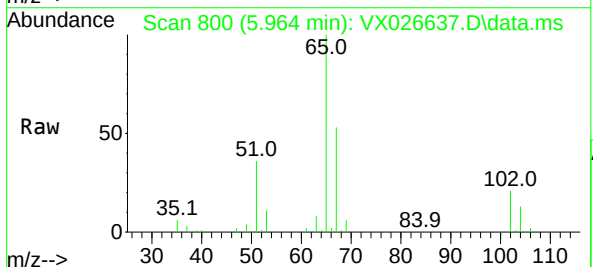




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion:114 Resp: 212502
Ion Ratio Lower Upper
114 100
63 20.6 0.0 42.8
88 16.0 0.0 33.0

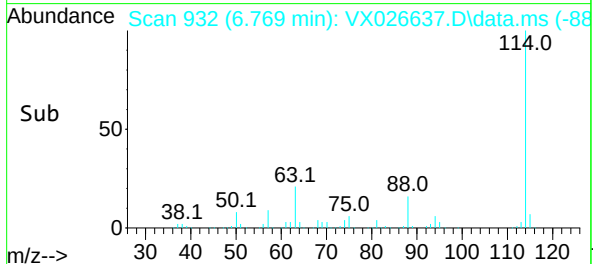

#35
Dibromofluoromethane
Concen: 49.018 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion:113 Resp: 67266
Ion Ratio Lower Upper
113 100
111 103.0 81.2 121.8
192 18.9 15.0 22.4

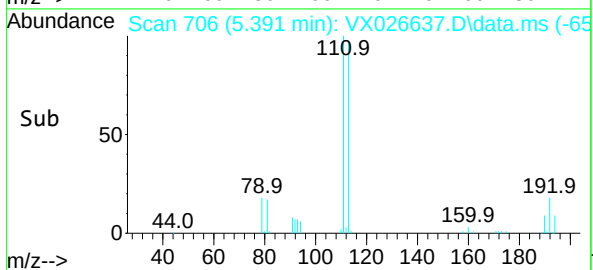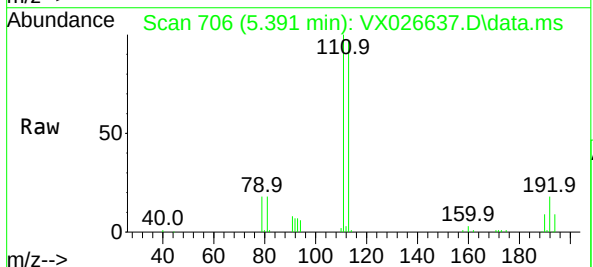



#36

1,1-Dichloropropene

Concen: 4.546 ug/l

RT: 5.556 min Scan# 71

Delta R.T. -0.140 min

Lab File: VX026637.D

Acq: 27 Jan 2022 20:07

Instrument :

MSVOA_X

ClientSampleId :

MW-14DA





Tgt Ion: 75 Resp: 9848

Ion Ratio Lower Upper

75 100

110 9.0 17.2 51.6#

77 0.0 24.6 36.8#

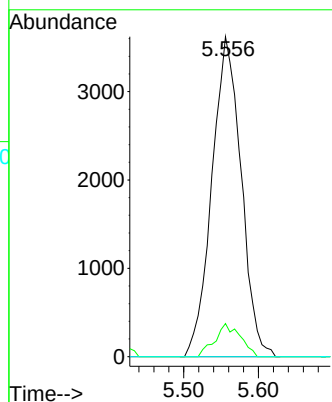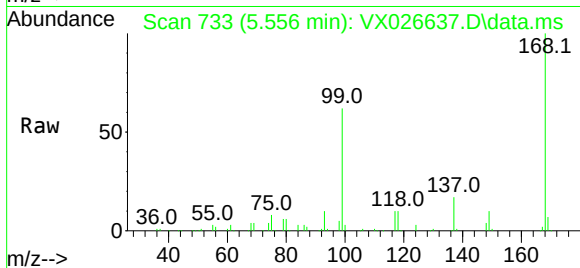

#38

Carbon Tetrachloride

Concen: 5.877 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.122 min

Lab File: VX026637.D

Acq: 27 Jan 2022 20:07




Tgt Ion: 117 Resp: 13095


Ion Ratio Lower Upper

117 100

119 4.4 74.7 112.1#

121 0.0 25.4 38.0#

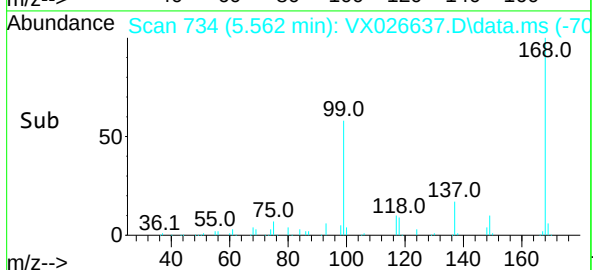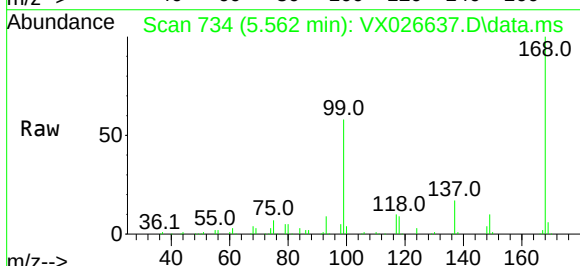



#39

Methylcyclohexane

Concen: 0.599 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. -0.006 min

Lab File: VX026637.D

Acq: 27 Jan 2022 20:07

Instrument :

MSVOA_X

ClientSampleId :

MW-14DA





Tgt Ion: 83 Resp: 1566

Ion Ratio Lower Upper

83 100

55 87.8 63.6 95.4

98 23.6 38.4 57.6#

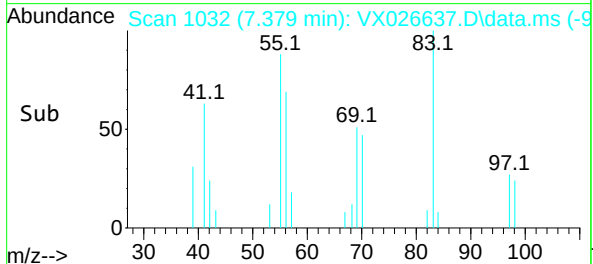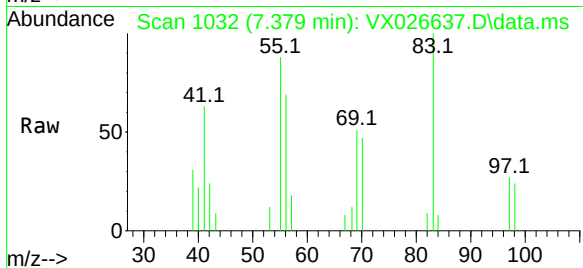

#40

Benzene

Concen: 1.689 ug/l

RT: 6.044 min Scan# 813

Delta R.T. 0.000 min

Lab File: VX026637.D




Acq: 27 Jan 2022 20:07


Tgt Ion: 78 Resp: 10113

Ion Ratio Lower Upper

78 100

77 24.6 18.9 28.3




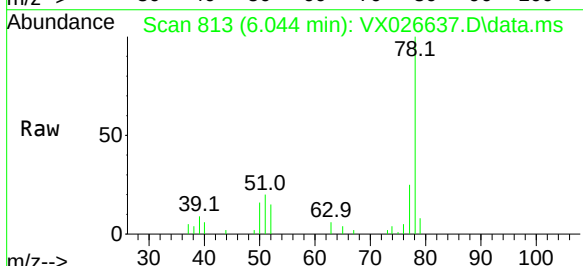




#41
Methacrylonitrile
Concen: 0.922 ug/l
RT: 5.141 min Scan# 61
Delta R.T. 0.219 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion:	41	Resp:	1144
Ion	Ratio	Lower	Upper
41	100		
39	10.2	45.4	68.0#
67	0.0	53.2	79.8#
52	0.0	23.0	34.6#

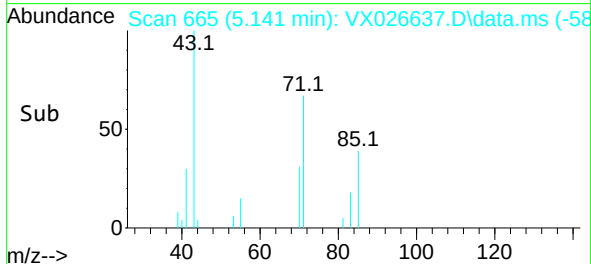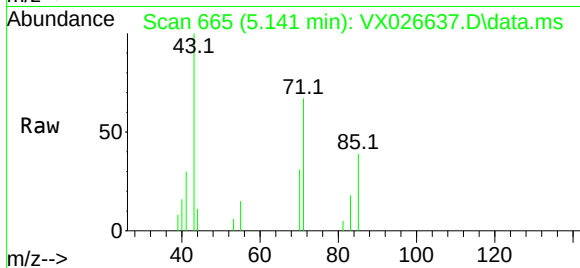

#50
Toluene-d8
Concen: 50.331 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion:	98	Resp:	248890
Ion	Ratio	Lower	Upper
98	100		
100	66.3	53.2	79.8




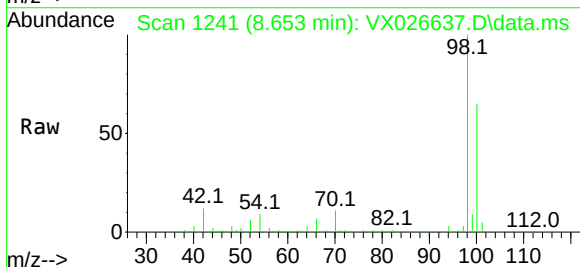




#51
4-Methyl-2-Pentanone
Concen: 0.664 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.073 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion: 43 Resp: 1394
Ion Ratio Lower Upper
43 100
58 143.7 30.5 45.7#

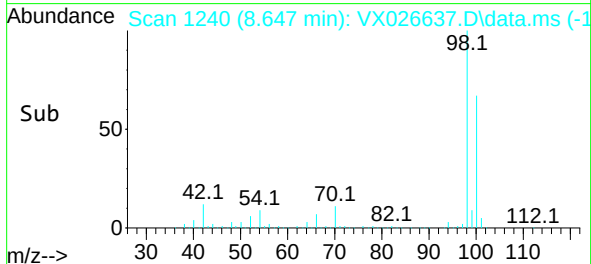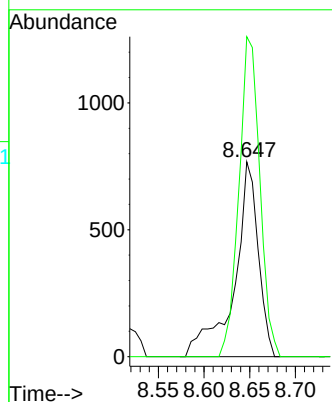

#55
1,1,2-Trichloroethane
Concen: 1.196 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 97 Resp: 1714
Ion Ratio Lower Upper
97 100
83 9.8 68.4 102.6#
85 0.0 44.0 66.0#
99 0.0 49.8 74.6#


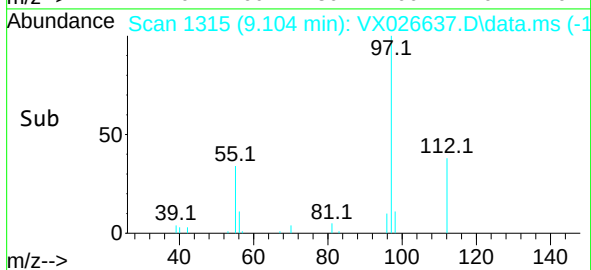

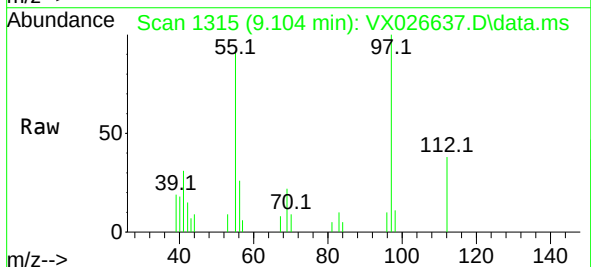




#60
Dibromochloromethane
Concen: 1.631 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.250 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion:129 Resp: 2436
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.5#

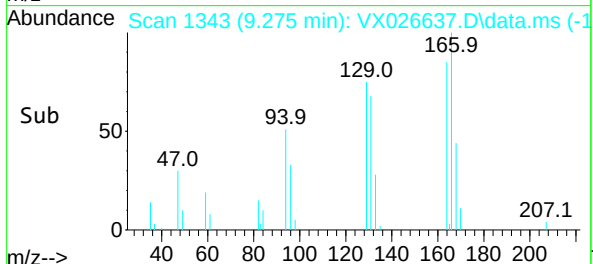

#62
4-Bromofluorobenzene
Concen: 49.534 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 95 Resp: 87015
Ion Ratio Lower Upper
95 100
174 73.6 0.0 148.6
176 71.2 0.0 141.4


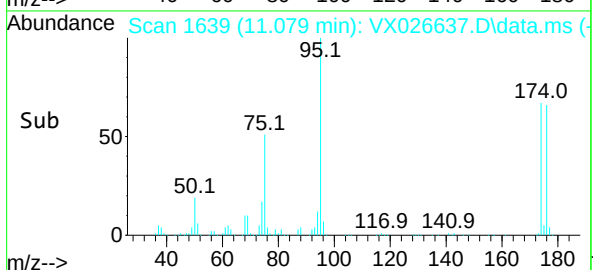

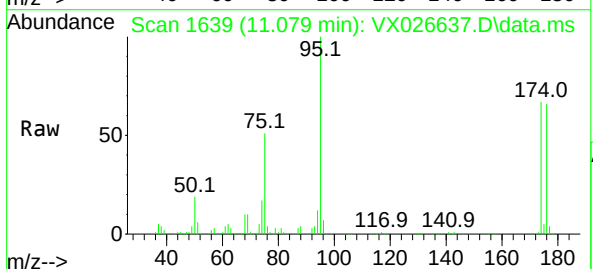




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion:117 Resp: 188109
Ion Ratio Lower Upper
117 100
82 57.5 45.2 67.8
119 32.5 26.2 39.2

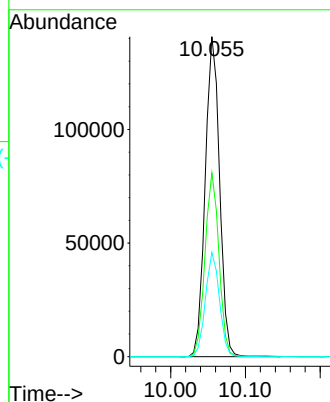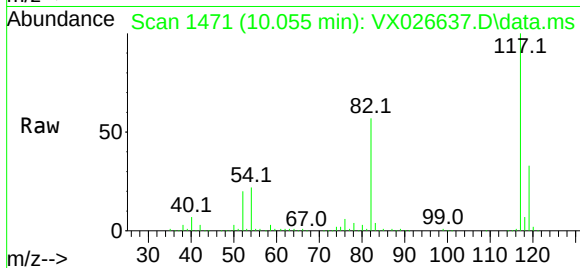

#64
Tetrachloroethene
Concen: 1.441 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion:164 Resp: 2561
Ion Ratio Lower Upper
164 100
166 117.0 101.8 152.6
129 87.8 83.3 124.9
131 79.0 78.0 117.0


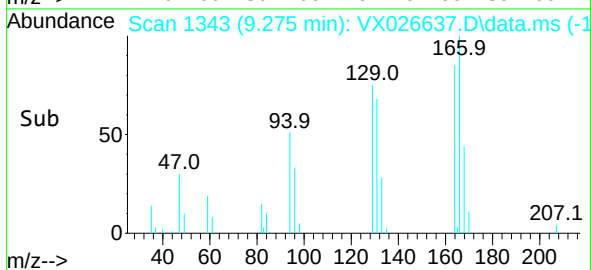

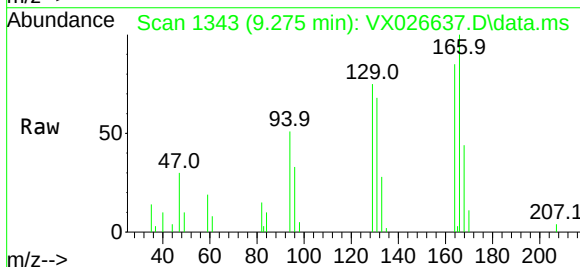




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX026637.D
 Acq: 27 Jan 2022 20:07




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-14DA


Tgt Ion:152 Resp: 74537
 Ion Ratio Lower Upper
 152 100
 115 60.8 44.2 132.6
 150 158.0 0.0 348.2

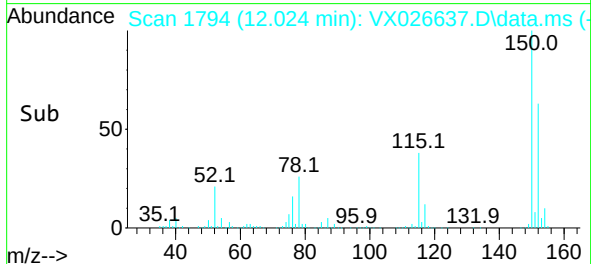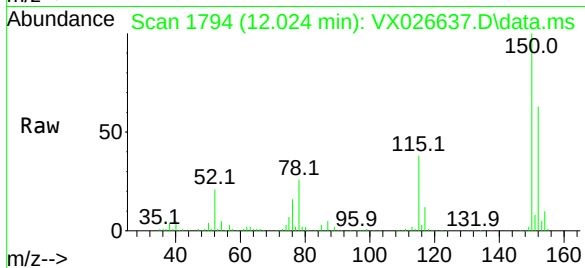

#73
 Isopropylbenzene
 Concen: 5.599 ug/l
 RT: 10.963 min Scan# 1620
 Delta R.T. 0.000 min
 Lab File: VX026637.D
 Acq: 27 Jan 2022 20:07

Tgt Ion:105 Resp: 34209
 Ion Ratio Lower Upper
 105 100
 120 25.9 13.1 39.1

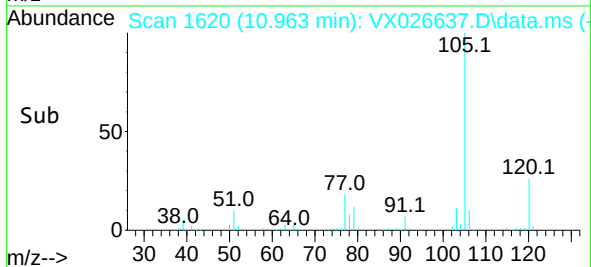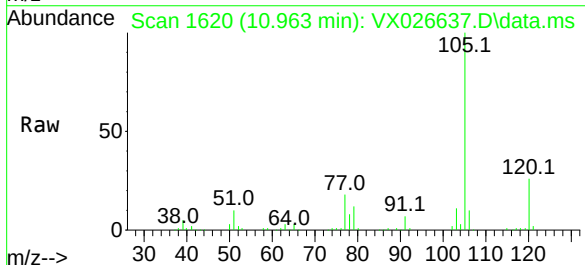



#76

1,2,3-Trichloropropane

Concen: 26.572 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.165 min

Lab File: VX026637.D

Acq: 27 Jan 2022 20:07

Instrument :

MSVOA_X

ClientSampleId :





MW-14DA

Tgt Ion: 75 Resp: 43608

Ion Ratio Lower Upper

75 100

77 1.1 18.3 54.8#

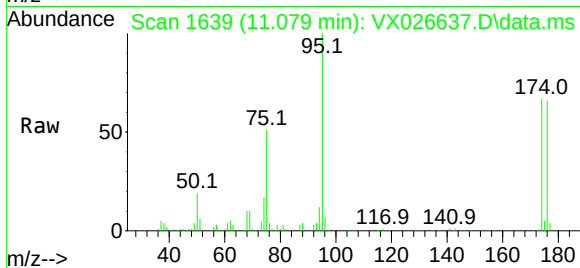

#78

n-propylbenzene

Concen: 0.293 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX026637.D




Acq: 27 Jan 2022 20:07


Tgt Ion: 91 Resp: 2040

Ion Ratio Lower Upper

91 100

120 20.9 11.6 34.7


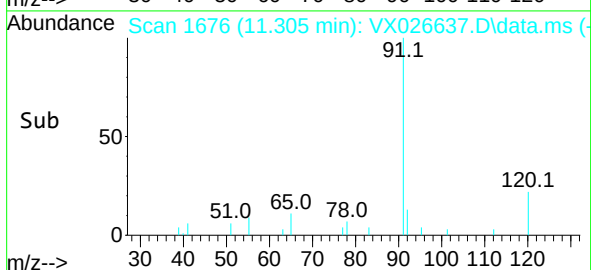

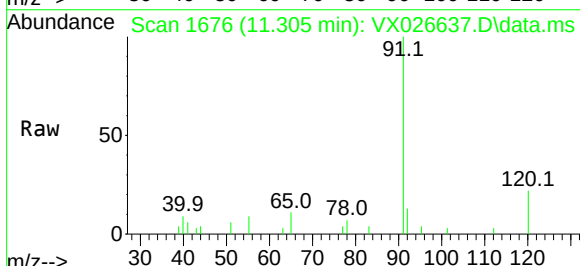




#79
2-Chlorotoluene
Concen: 0.483 ug/l
RT: 11.305 min Scan# 1639
Delta R.T. -0.061 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion: 91 Resp: 2040
Ion Ratio Lower Upper
91 100
126 0.0 16.4 49.2#

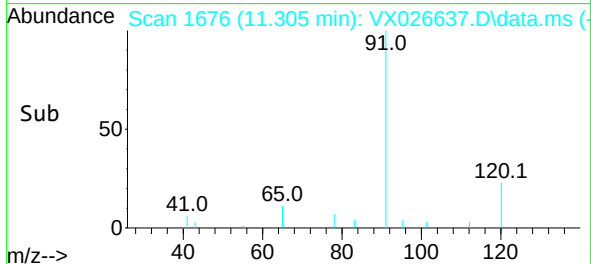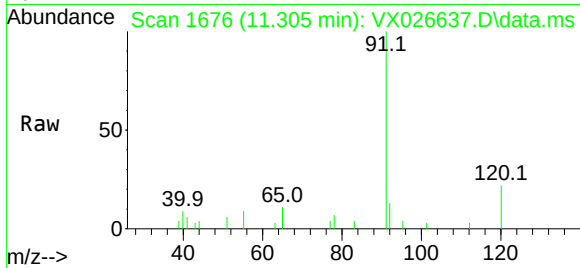

#81
trans-1,4-Dichloro-2-butene
Concen: 80.455 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 75 Resp: 43608
Ion Ratio Lower Upper
75 100
53 0.0 94.0 141.0#
89 0.0 37.0 55.4#


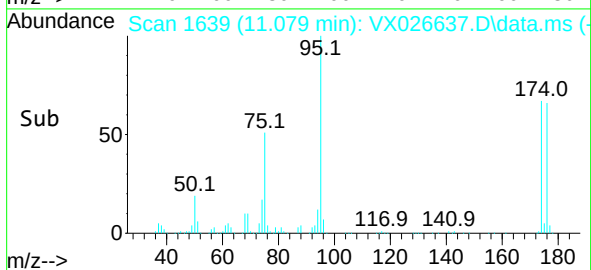

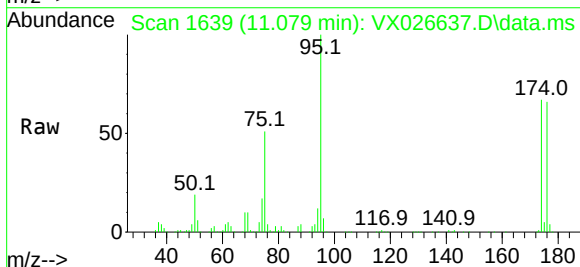




#85
 sec-Butylbenzene
 Concen: 0.915 ug/l
 RT: 11.890 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX026637.D
 Acq: 27 Jan 2022 20:07




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-14DA


Tgt Ion:105 Resp: 5566
 Ion Ratio Lower Upper
 105 100
 134 20.0 10.1 30.1

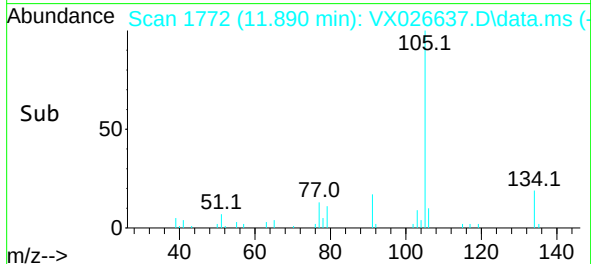

#86
 p-Isopropyltoluene
 Concen: 0.206 ug/l
 RT: 12.183 min Scan# 1820
 Delta R.T. 0.171 min
 Lab File: VX026637.D
 Acq: 27 Jan 2022 20:07

Tgt Ion:119 Resp: 1049
 Ion Ratio Lower Upper
 119 100
 134 33.7 13.0 39.0
 91 23.5 12.6 37.6


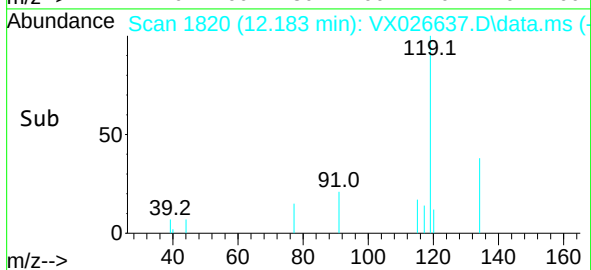

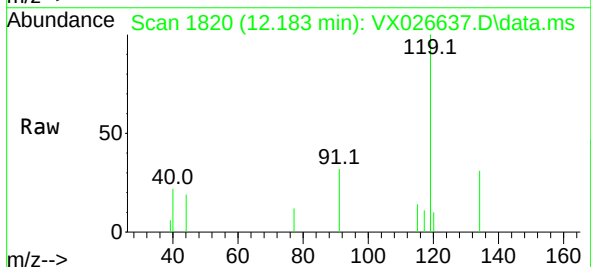


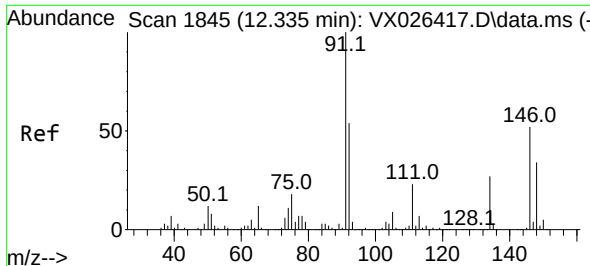

#89
n-Butylbenzene
Concen: 0.929 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07




Instrument :
MSVOA_X
ClientSampleId :
MW-14DA


Tgt Ion: 91 Resp: 4070
Ion Ratio Lower Upper
91 100
92 47.4 27.2 81.6
134 22.1 13.1 39.1

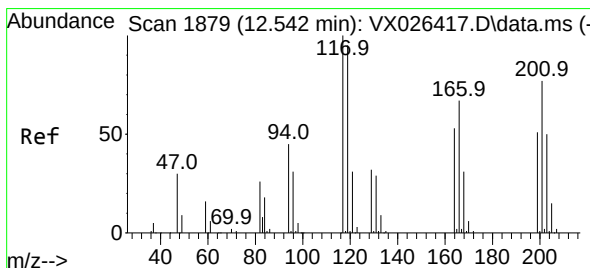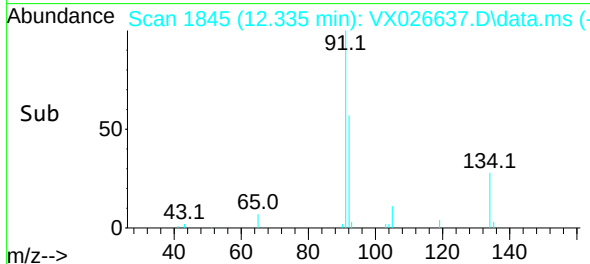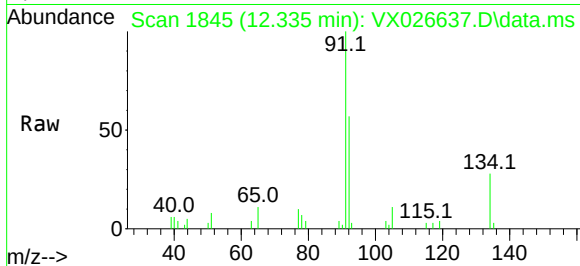

#90
Hexachloroethane
Concen: 3.926 ug/l
RT: 12.646 min Scan# 1896
Delta R.T. 0.104 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 117 Resp: 1557
Ion Ratio Lower Upper
117 100
201 0.0 35.6 106.8#


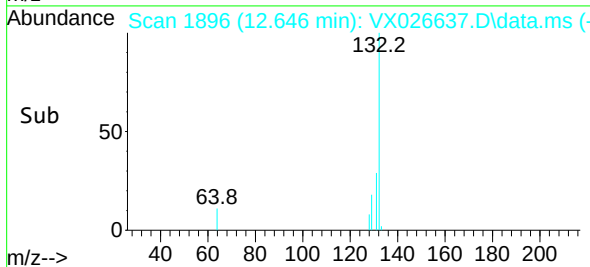

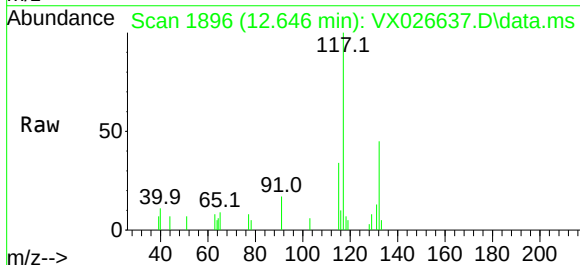


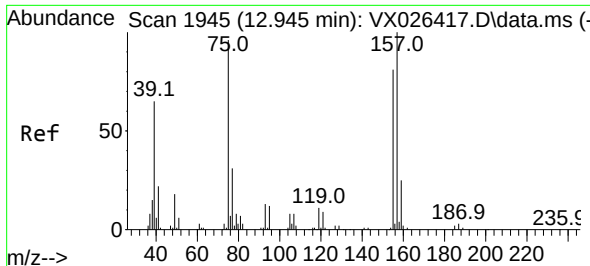

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.235 ug/l
RT: 13.176 min Scan# 1945
Delta R.T. 0.232 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Instrument :
MSVOA_X
ClientSampleId :
MW-14DA

Tgt Ion: 75 Resp: 93
Ion Ratio Lower Upper
75 100
155 0.0 40.0 119.9#
157 0.0 51.6 154.8#

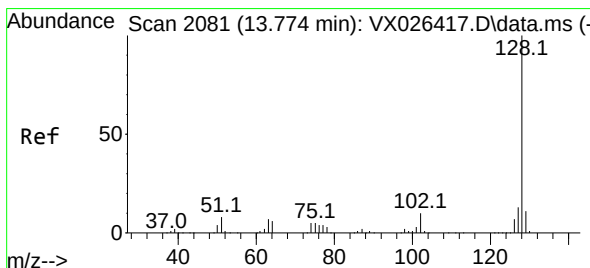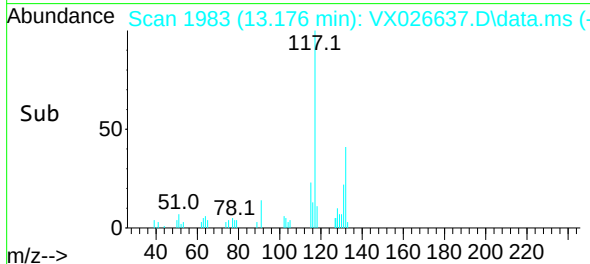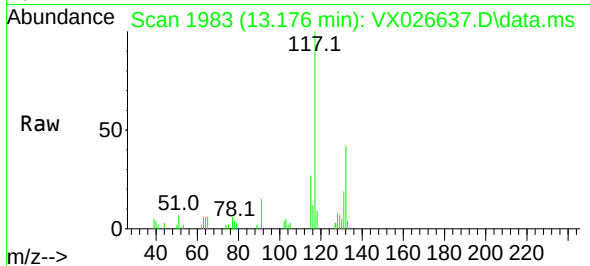

#95
Naphthalene
Concen: 7.402 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX026637.D
Acq: 27 Jan 2022 20:07

Tgt Ion: 128 Resp: 39248
Ion Ratio Lower Upper
128 100
127 13.2 10.3 15.5
129 11.7 8.7 13.1

