

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012722\
 Data File : VX026590.D
 Acq On : 26 Jan 2022 13:33
 Operator : JC/MD
 Sample : PB142265TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB142265TB

Quant Time: Jan 26 13:56:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	132691	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	222689	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	204324	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	88606	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	85425	46.086	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.180%
35) Dibromofluoromethane	5.391	113	69358	48.230	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.460%
50) Toluene-d8	8.653	98	264096	50.963	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	101.920%
62) 4-Bromofluorobenzene	11.079	95	99174	53.873	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.740%
Target Compounds						
					Qvalue	
16) Acetone	2.392	43	12287	12.999	ug/l	96
20) Methylene Chloride	2.794	84	4307	2.758	ug/l #	88
43) Isopropyl Acetate	6.348	43	13358	3.601	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012722\
Data File : VX026590.D
Acq On : 26 Jan 2022 13:33
Operator : JC/MD
Sample : PB142265TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB142265TB

Quant Time: Jan 26 13:56:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




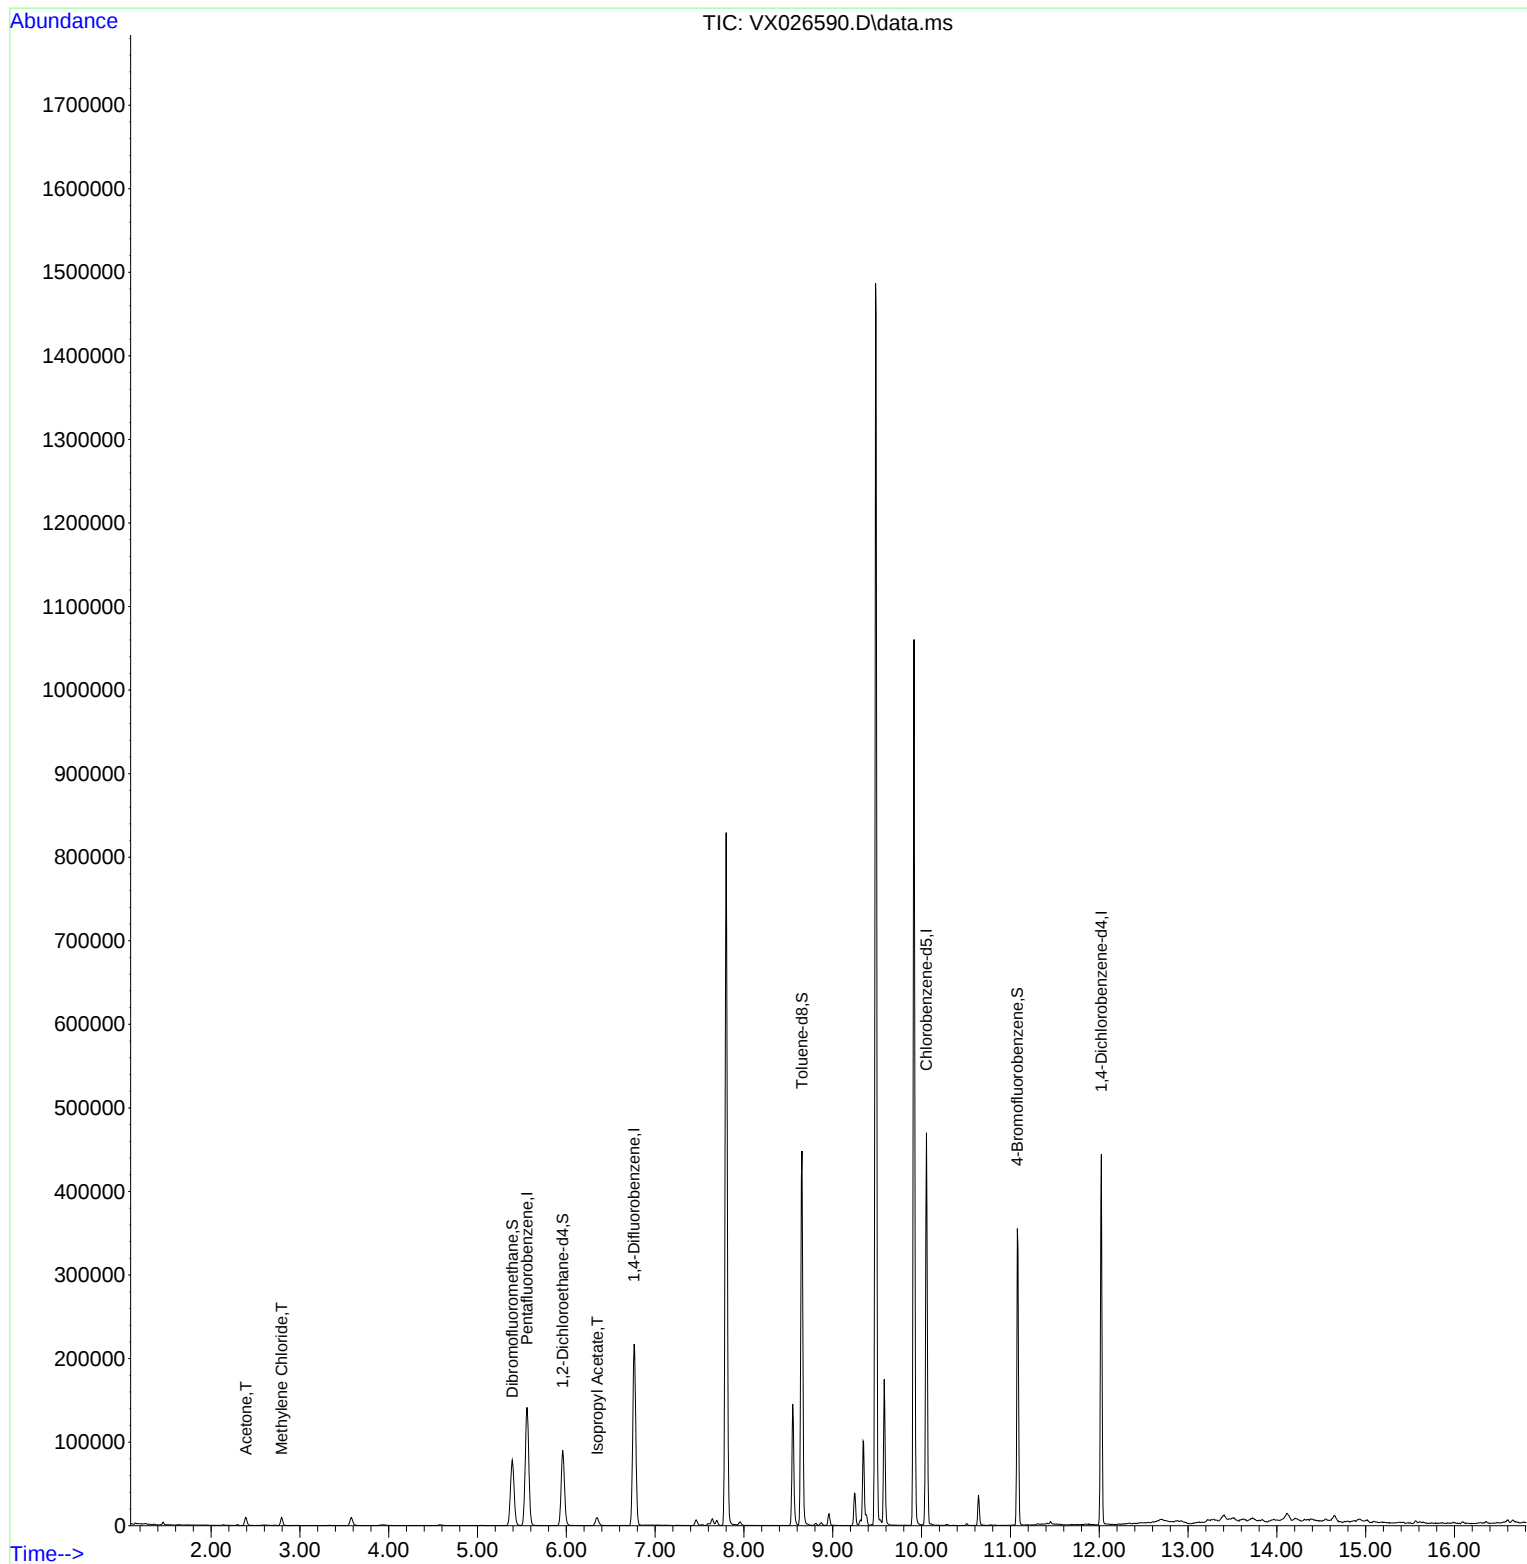


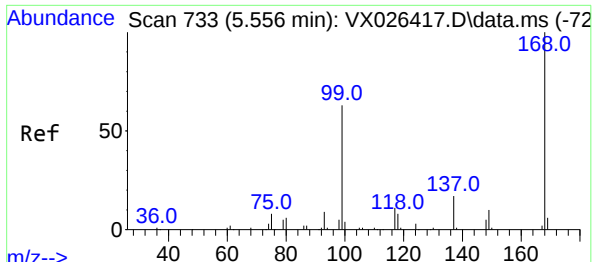

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33




Instrument :
MSVOA_X
ClientSampleId :
PB142265TB


Tgt Ion:168 Resp: 132691
Ion Ratio Lower Upper
168 100
99 60.9 50.3 75.5

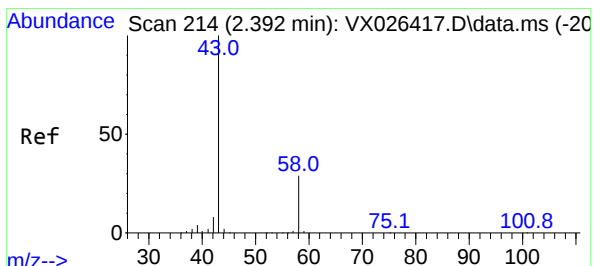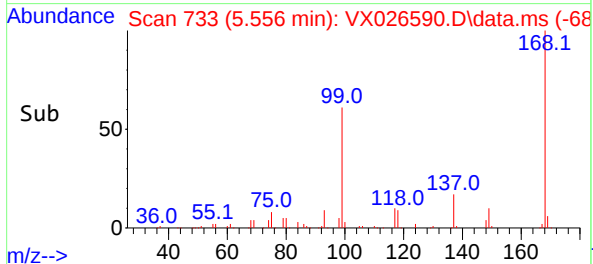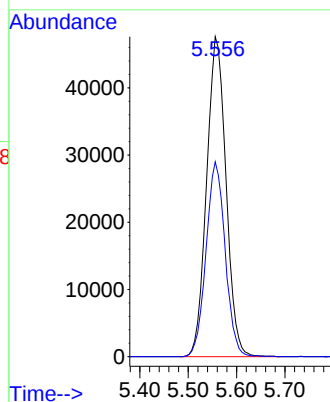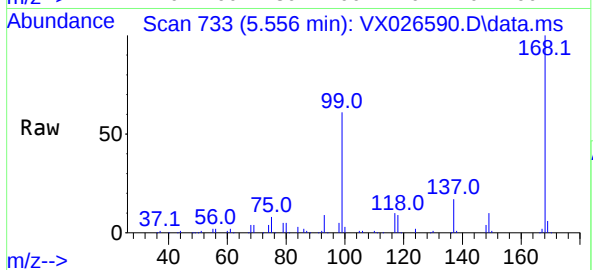

#16
Acetone
Concen: 12.999 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33

Tgt Ion: 43 Resp: 12287
Ion Ratio Lower Upper
43 100
58 31.1 23.0 34.6

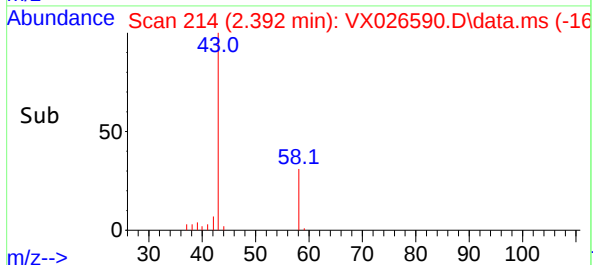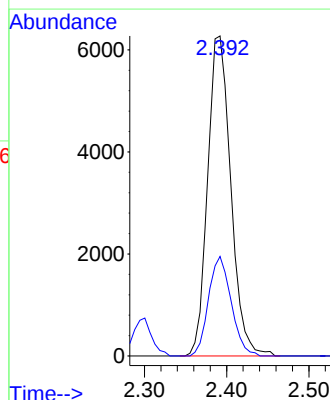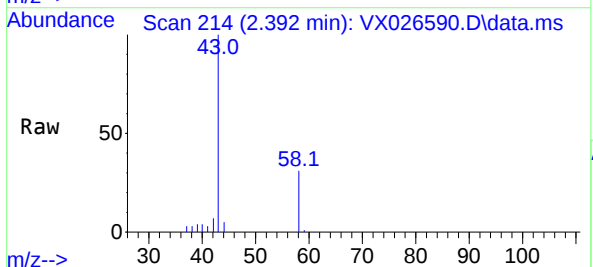




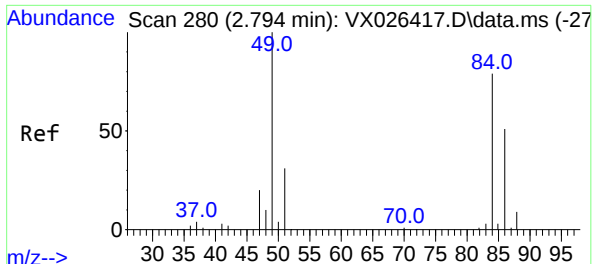


#20
Methylene Chloride
Concen: 2.758 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33

Instrument :
MSVOA_X
ClientSampleId :
PB142265TB

Tgt Ion: 84 Resp: 4307




Ion	Ratio	Lower	Upper
84	100		
49	112.1	101.5	152.3
51	30.1	31.2	46.8#
86	57.0	51.3	76.9

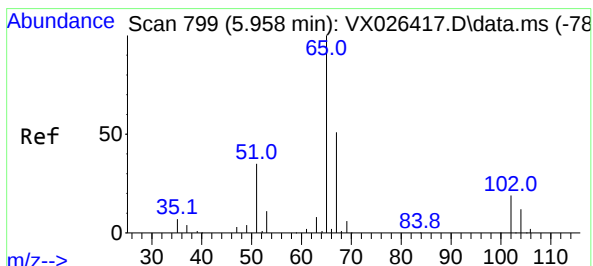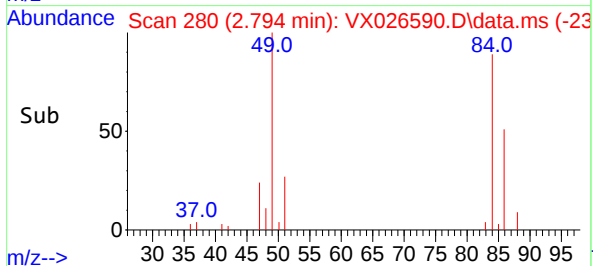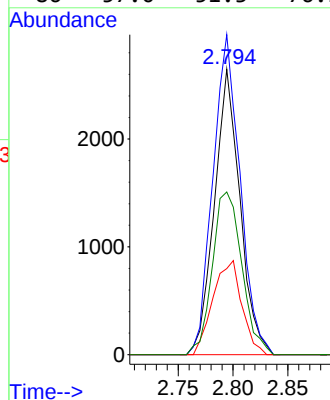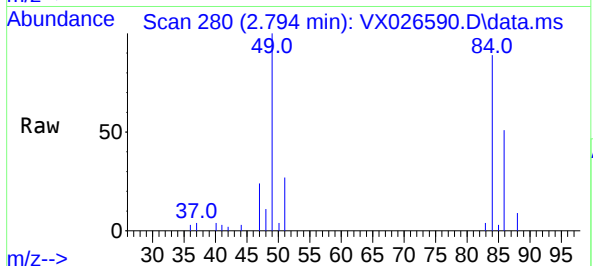


#33
1,2-Dichloroethane-d4
Concen: 46.086 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33

Tgt Ion: 65 Resp: 85425

Ion	Ratio	Lower	Upper
65	100		
67	52.8	0.0	100.8


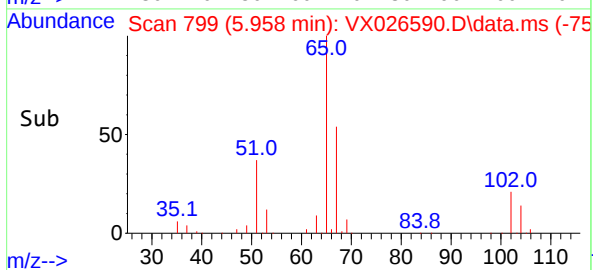
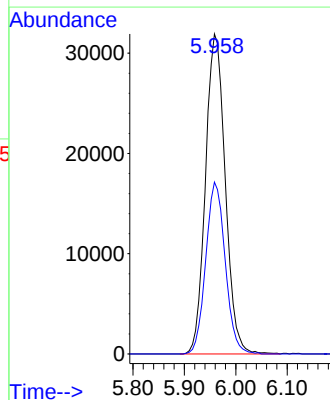
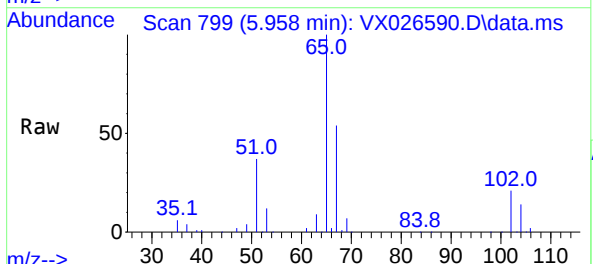


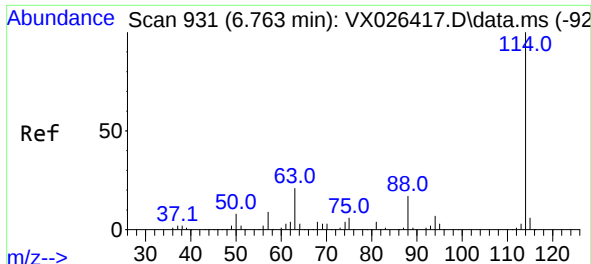

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33




Instrument :
MSVOA_X
ClientSampleId :
PB142265TB


Tgt Ion:114 Resp: 222689
Ion Ratio Lower Upper
114 100
63 20.0 0.0 42.8
88 16.2 0.0 33.0

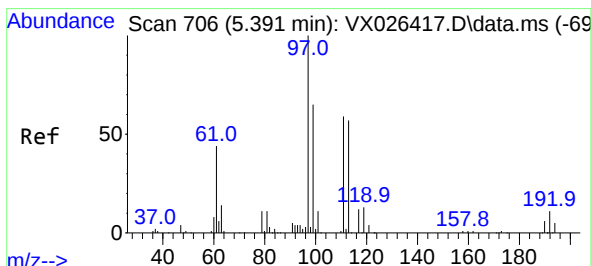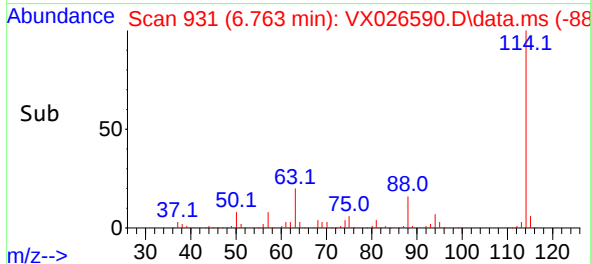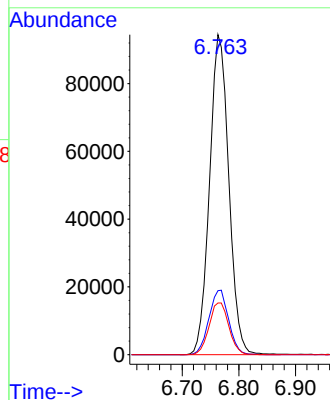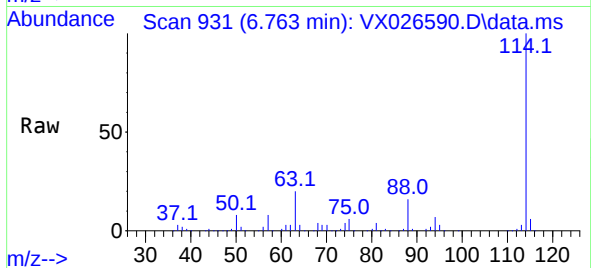

#35
Dibromofluoromethane
Concen: 48.230 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33

Tgt Ion:113 Resp: 69358
Ion Ratio Lower Upper
113 100
111 102.2 81.2 121.8
192 18.9 15.0 22.4


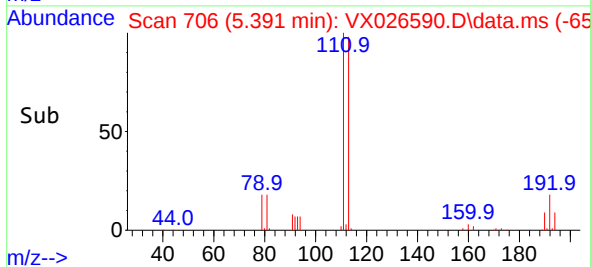
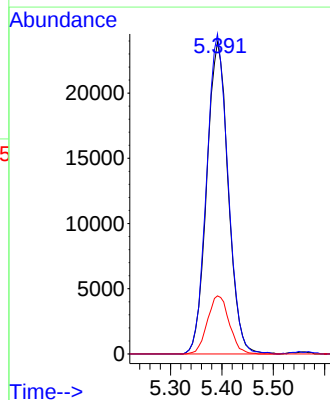
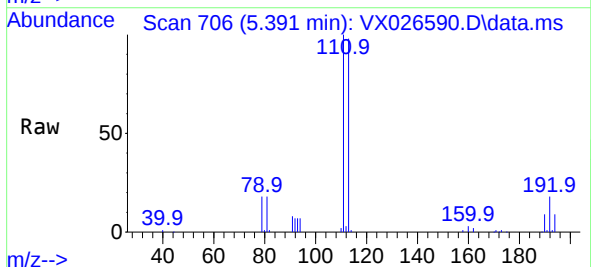


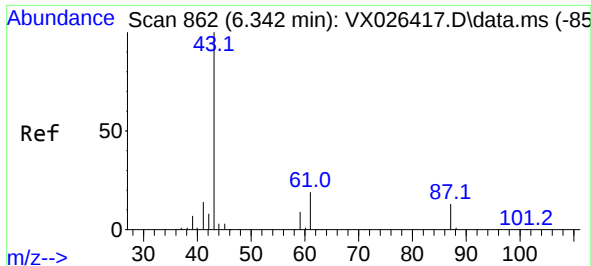

#43
Isopropyl Acetate
Concen: 3.601 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.006 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33




Instrument :
MSVOA_X
ClientSampleId :
PB142265TB


Tgt Ion: 43 Resp: 13358
Ion Ratio Lower Upper
43 100
61 19.7 15.4 23.0
87 13.5 10.2 15.2

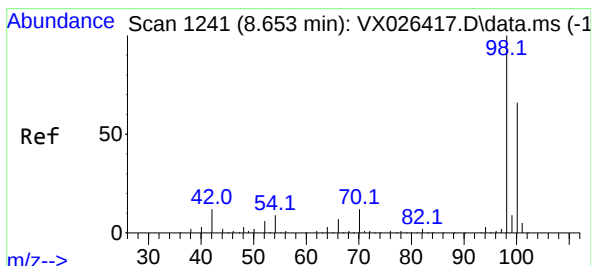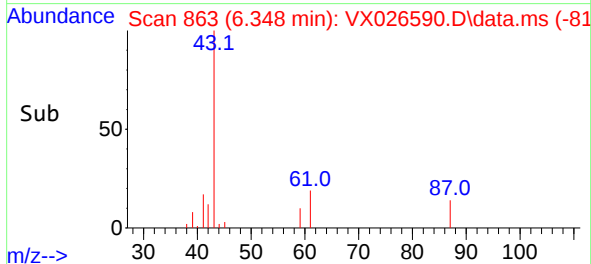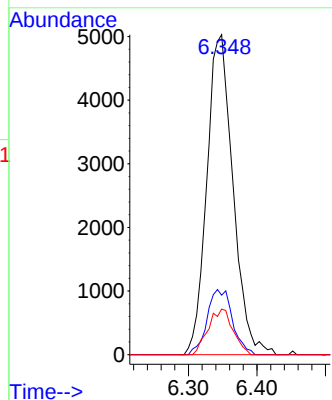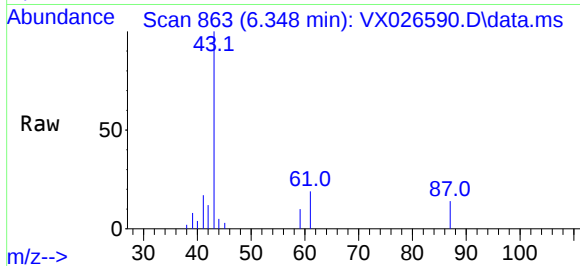

#50
Toluene-d8
Concen: 50.963 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33

Tgt Ion: 98 Resp: 264096
Ion Ratio Lower Upper
98 100
100 66.8 53.2 79.8


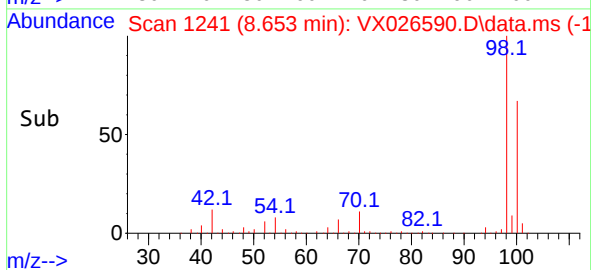
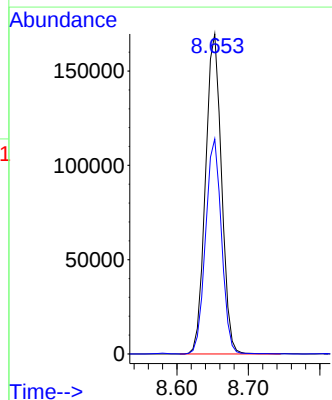
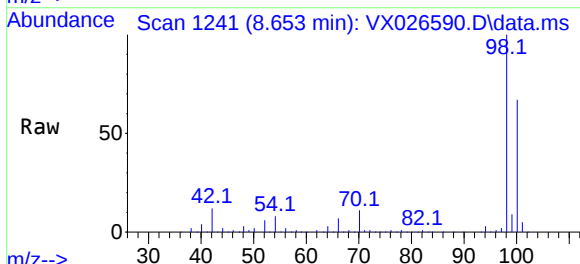


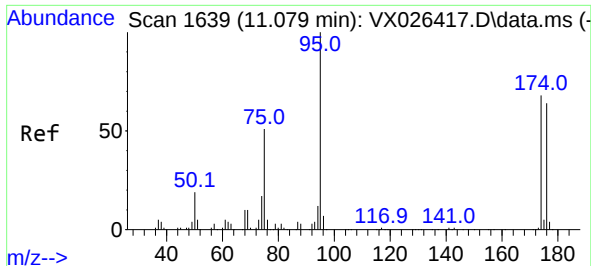

#62
4-Bromofluorobenzene
Concen: 53.873 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33




Instrument :
MSVOA_X
ClientSampleId :
PB142265TB


Tgt Ion: 95 Resp: 99174
Ion Ratio Lower Upper
95 100
174 74.1 0.0 148.6
176 71.7 0.0 141.4

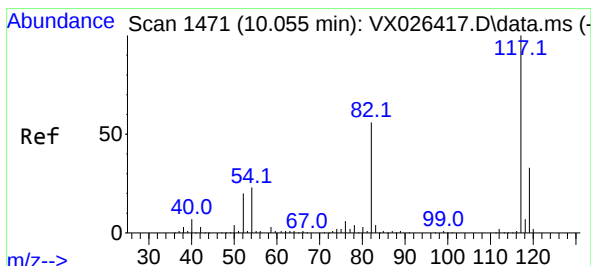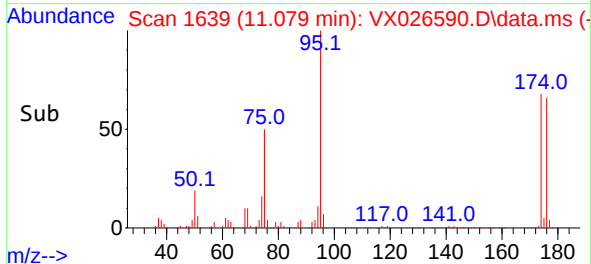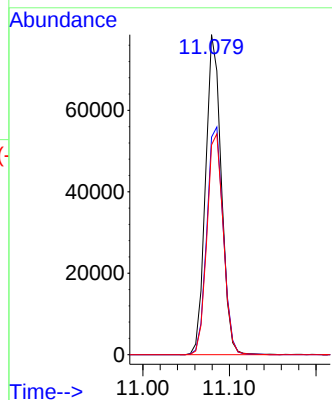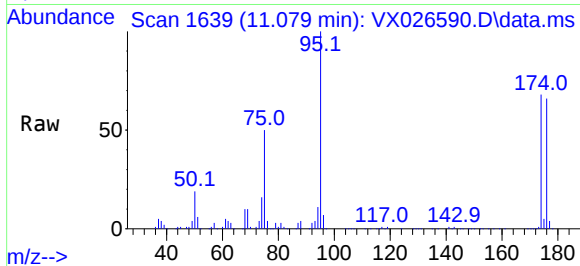

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026590.D
Acq: 26 Jan 2022 13:33


Tgt Ion: 117 Resp: 204324
Ion Ratio Lower Upper
117 100
82 57.2 45.2 67.8
119 32.0 26.2 39.2

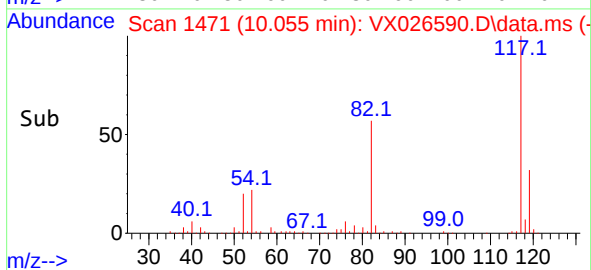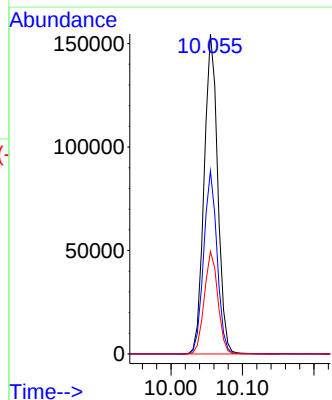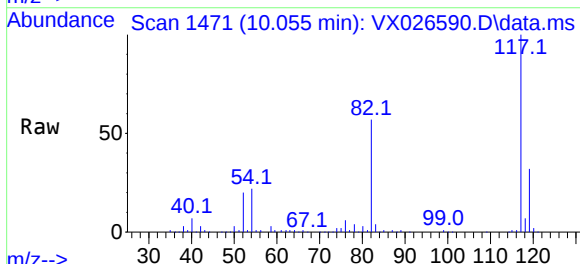

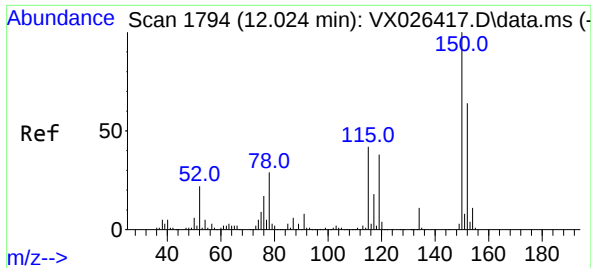

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX026590.D
 Acq: 26 Jan 2022 13:33

Instrument :
 MSVOA_X
 ClientSampleId :
 PB142265TB

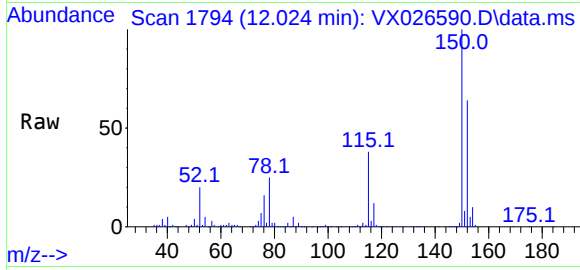

Tgt Ion:152 Resp: 88606
 Ion Ratio Lower Upper
 152 100
 115 60.5 44.2 132.6
 150 157.3 0.0 348.2

