

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012723\
 Data File : VX033931.D
 Acq On : 27 Jan 2023 12:42
 Operator : JC/MD
 Sample : 01320-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOTE-COMP-0126

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M

Title : SW846 8260

Signal : TIC: VX033931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	32	rVB	14825	15342	2.27%	0.388%
2	2.374	206	211	220	rVB	5468	8727	1.29%	0.221%
3	5.385	694	705	718	rBV2	80452	233933	34.67%	5.912%
4	5.550	721	732	754	rVB	144020	414573	61.44%	10.477%
5	5.958	789	799	817	rBV	79777	214217	31.75%	5.414%
6	6.763	920	931	945	rBV	208153	501498	74.33%	12.674%
7	8.647	1234	1240	1248	rBV	434195	674722	100.00%	17.051%
8	8.720	1248	1252	1265	rVB	20924	34076	5.05%	0.861%
9	10.055	1465	1471	1488	rBV	421214	575098	85.23%	14.534%
10	11.079	1634	1639	1649	rBV	356739	450006	66.70%	11.372%
11	11.366	1680	1686	1691	rBV	131776	169233	25.08%	4.277%
12	11.457	1696	1701	1710	rVB	49088	64177	9.51%	1.622%
13	12.024	1788	1794	1808	rBV	421230	543519	80.55%	13.736%
14	12.439	1858	1862	1874	rVV	46320	57881	8.58%	1.463%




Sum of corrected areas: 3957002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012723\
Data File : VX033931.D
Acq On : 27 Jan 2023 12:42
Operator : JC/MD
Sample : 01320-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP-0126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

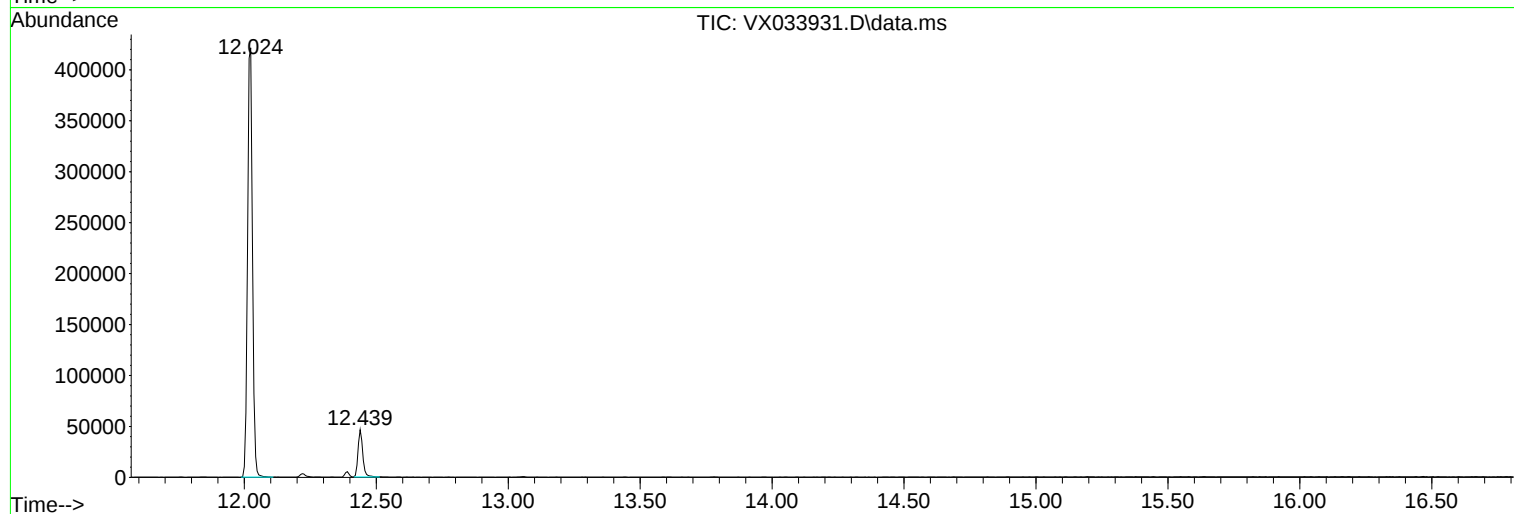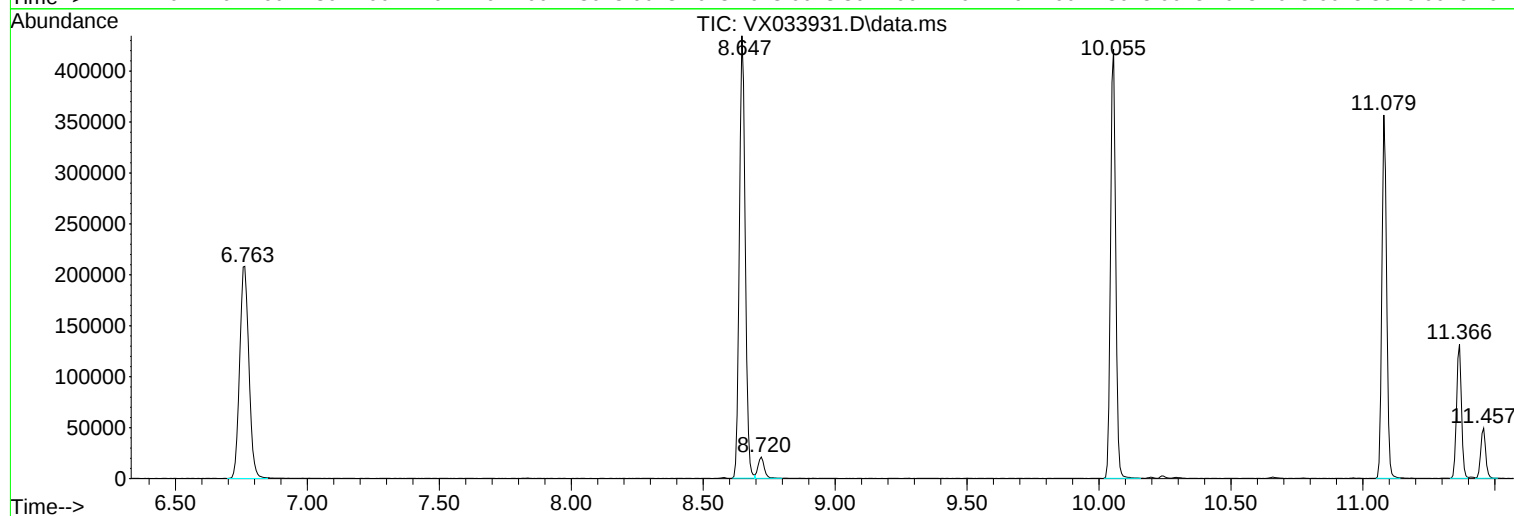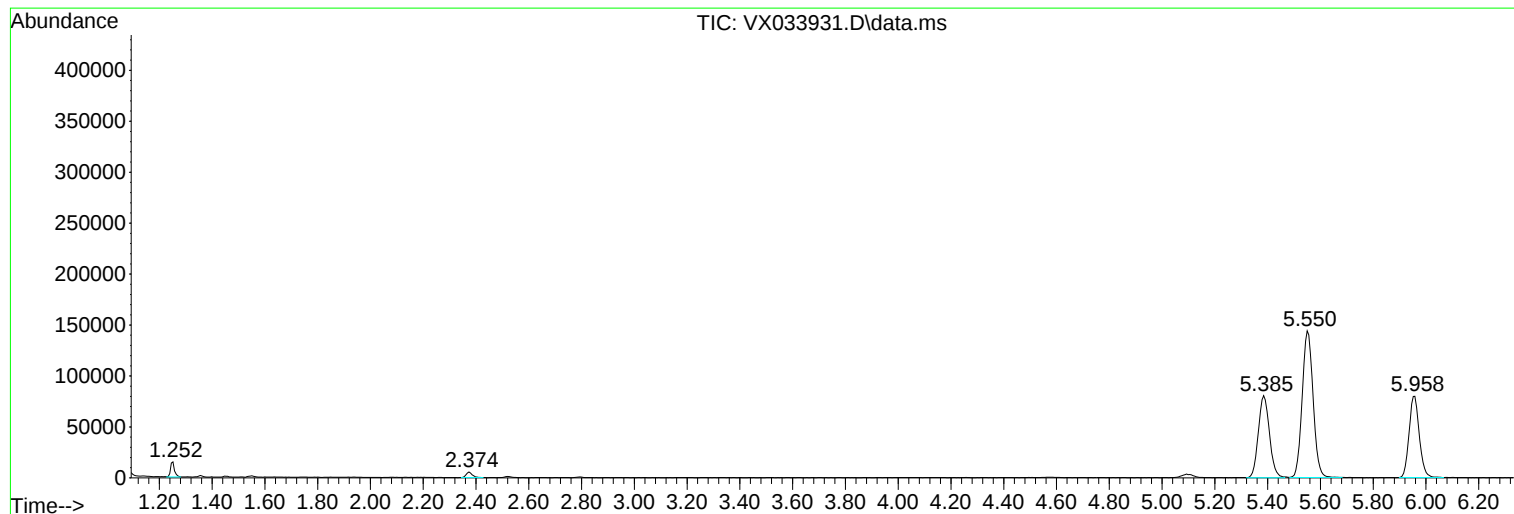

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012723\
Data File : VX033931.D
Acq On : 27 Jan 2023 12:42
Operator : JC/MD
Sample : 01320-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP-0126










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, (ethoxymethyl)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.439	5.32 ug/l	57881	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, (ethoxymethyl)-	136	C9H12O	000539-30-0	97
2			Benzeneethanol, .alpha.-methyl-	136	C9H12O	000698-87-3	58
3			Benzeneacetamide	135	C8H9NO	000103-81-1	53
4			1,5-Heptadien-3-yne	92	C7H8	003511-27-1	53
5			p-Methylbenzeneboronic acid	136	C7H9BO2	005720-05-8	53

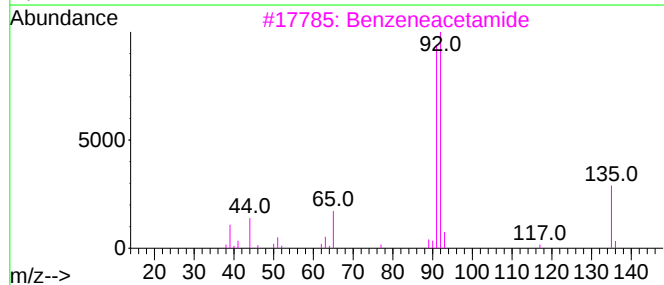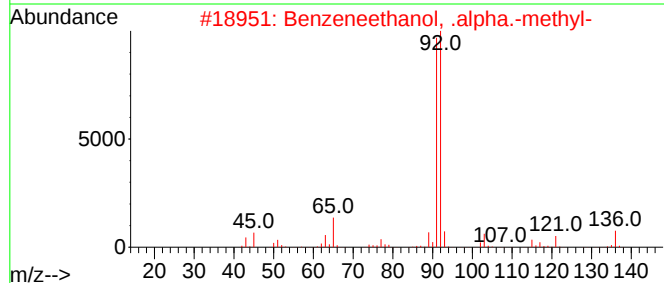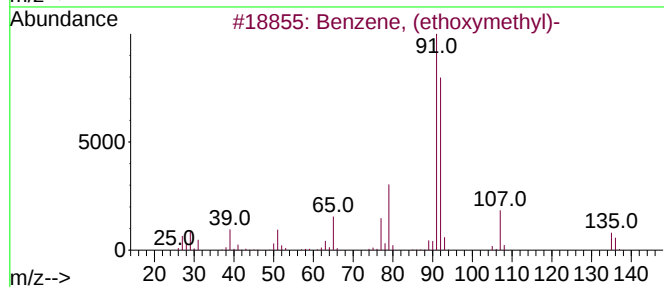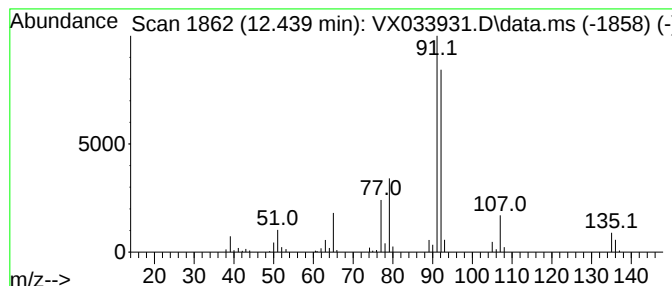

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012723\
Data File : VX033931.D
Acq On : 27 Jan 2023 12:42
Operator : JC/MD
Sample : 01320-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP-0126

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, (ethox...	12.439	5.3	ug/l	57881	4	12.024	543519	50.0