

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012725\
 Data File : VX044712.D
 Acq On : 27 Jan 2025 10:38
 Operator : JC/MD
 Sample : VX0127MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0127MBL01

Quant Time: Jan 28 04:07:40 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011525W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jan 16 01:16:09 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	156935	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	314560	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	278587	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	122776	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	113332	47.843	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	95.680%
35) Dibromofluoromethane	5.379	113	100912	50.498	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.000%
50) Toluene-d8	8.641	98	376419	54.022	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	108.040%
62) 4-Bromofluorobenzene	11.079	95	139028	53.523	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	107.040%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012725\
Data File : VX044712.D
Acq On : 27 Jan 2025 10:38
Operator : JC/MD
Sample : VX0127MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0127MBL01

Quant Time: Jan 28 04:07:40 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011525W.M
Quant Title : SW846 8260
QLast Update : Thu Jan 16 01:16:09 2025
Response via : Initial Calibration




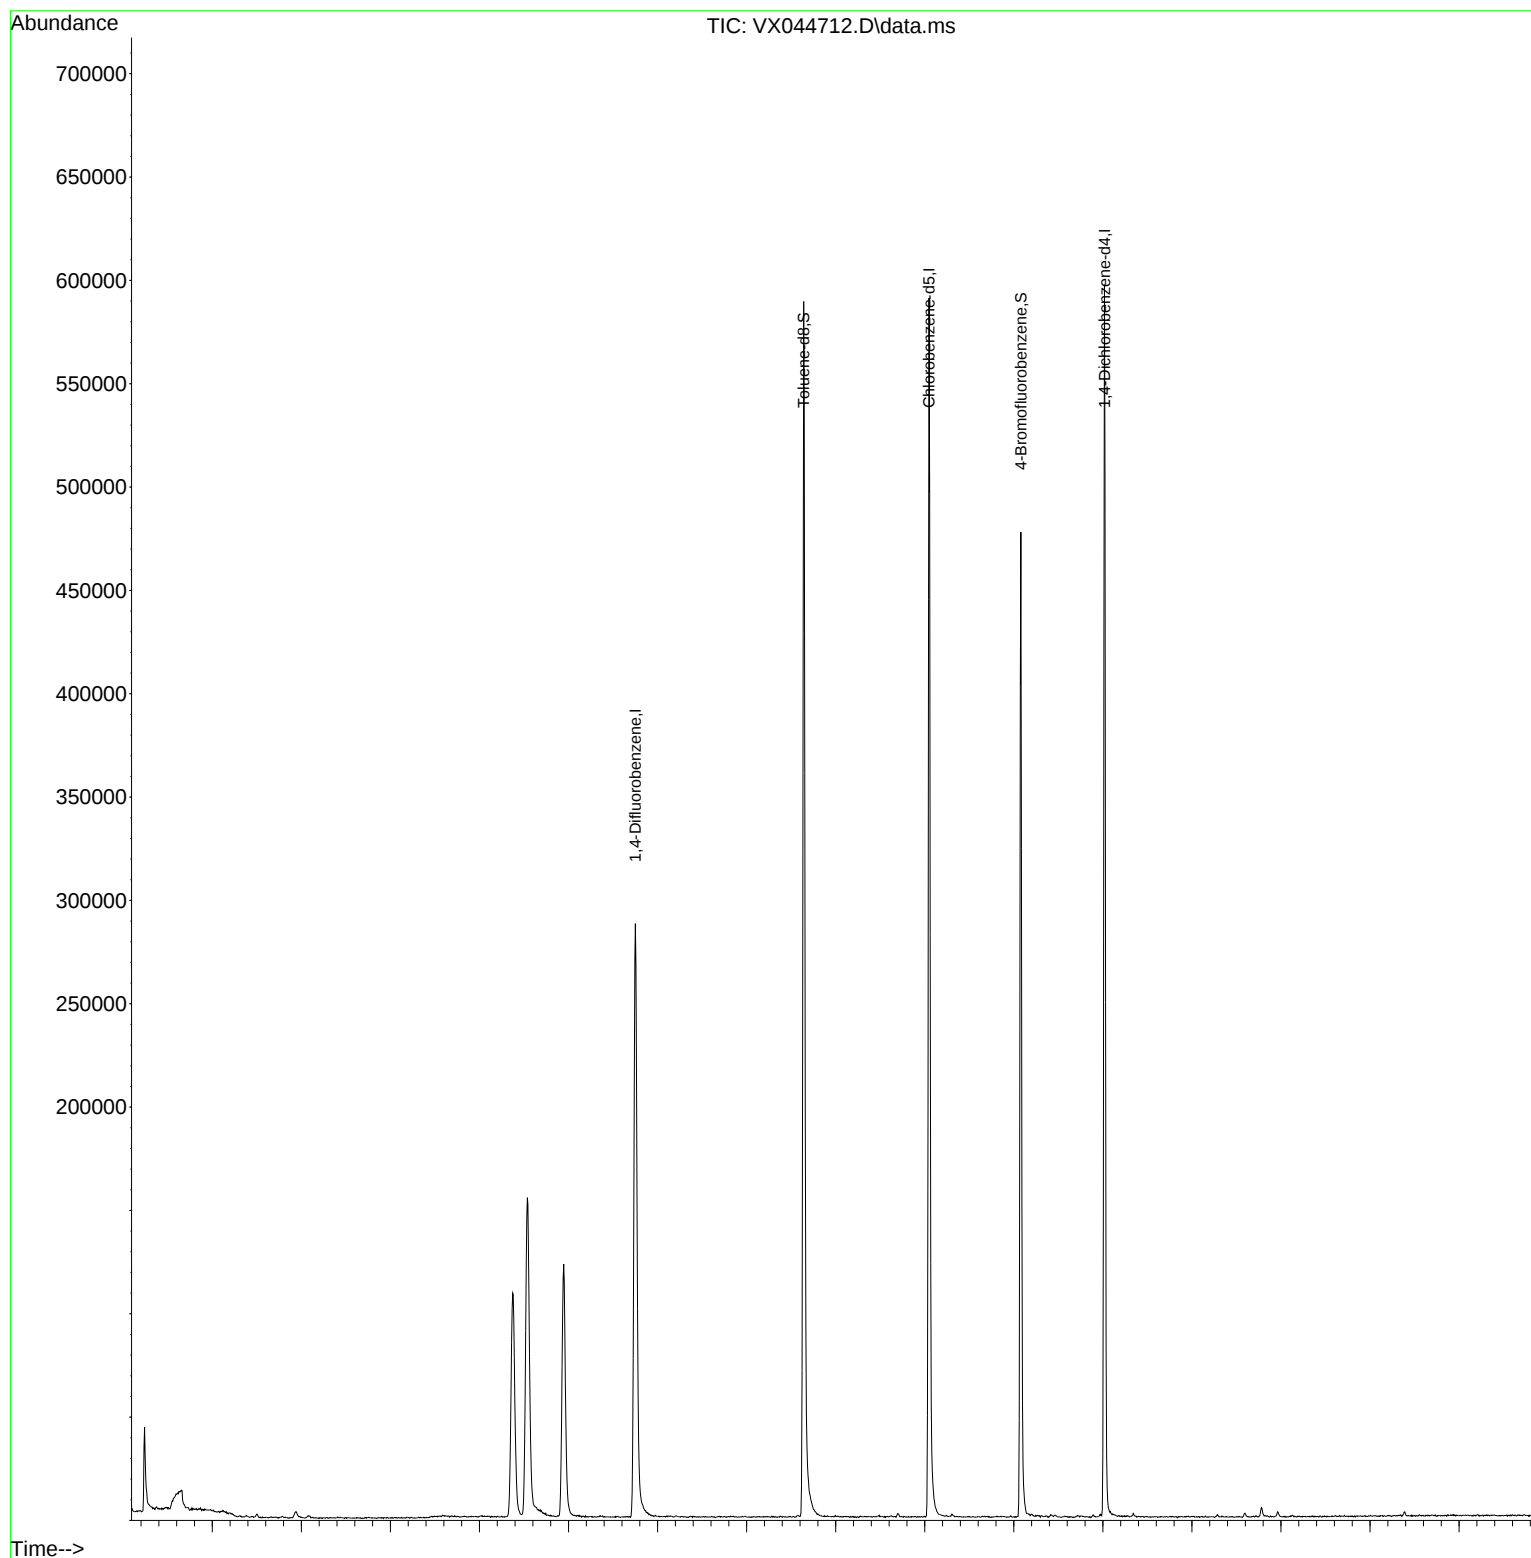


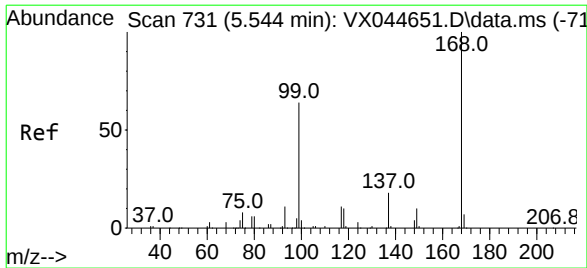

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 731
Delta R.T. -0.006 min
Lab File: VX044712.D
Acq: 27 Jan 2025 10:38




Instrument :
MSVOA_X
ClientSampleId :
VX0127MBL01


Tgt Ion:168 Resp: 156935
Ion Ratio Lower Upper
168 100
99 62.3 51.1 76.7

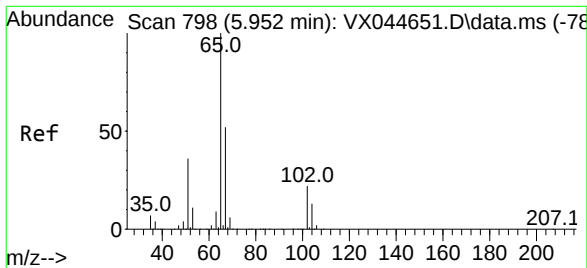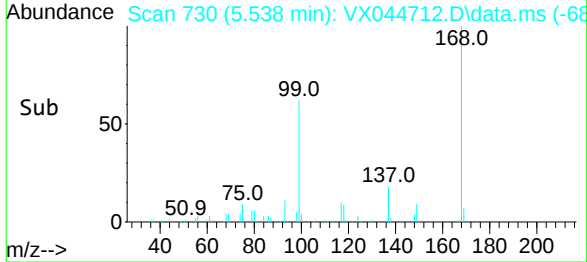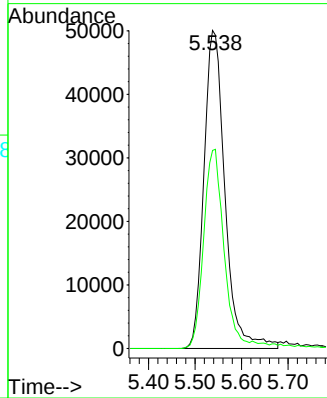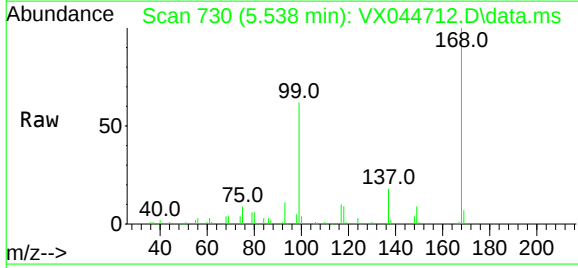

#33
1,2-Dichloroethane-d4
Concen: 47.843 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX044712.D
Acq: 27 Jan 2025 10:38

Tgt Ion: 65 Resp: 113332
Ion Ratio Lower Upper
65 100
67 54.5 0.0 103.4

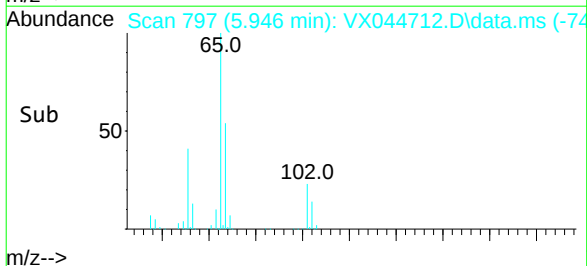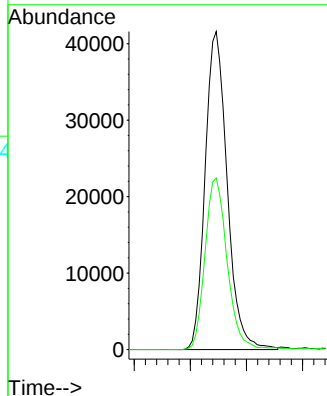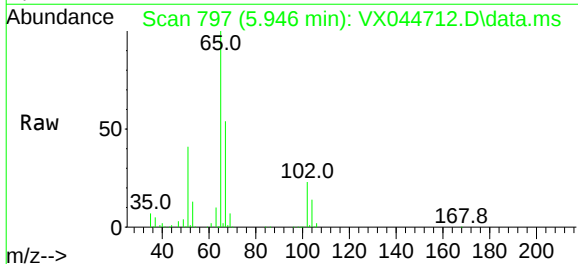

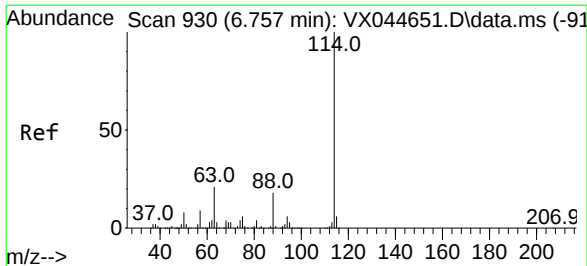

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.751 min Scan# 92

Delta R.T. -0.006 min

Lab File: VX044712.D

Acq: 27 Jan 2025 10:38

Instrument :

MSVOA_X

ClientSampleId :

VX0127MBL01





Tgt Ion:114 Resp: 314560

Ion Ratio Lower Upper

114 100

63 21.1 0.0 43.0

88 16.7 0.0 35.4

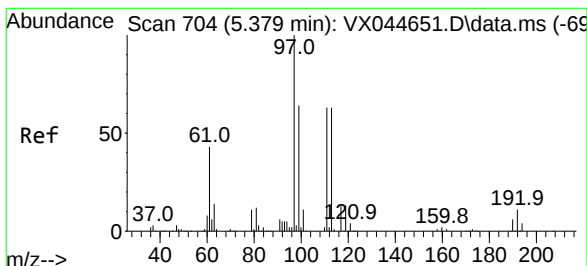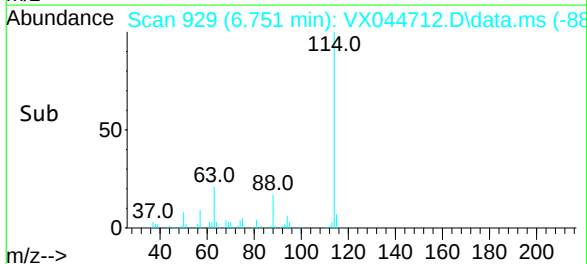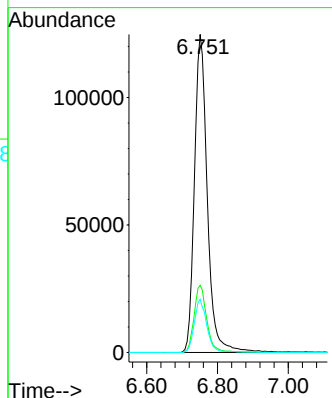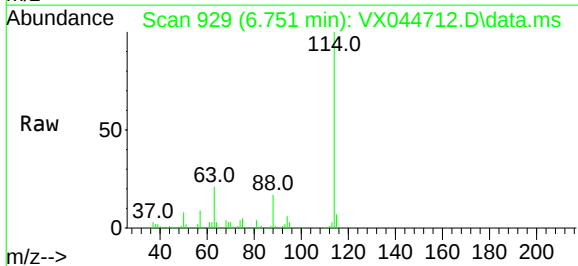

#35

Dibromofluoromethane

Concen: 50.498 ug/l

RT: 5.379 min Scan# 704

Delta R.T. 0.000 min

Lab File: VX044712.D

Acq: 27 Jan 2025 10:38




Tgt Ion:113 Resp: 100912


Ion Ratio Lower Upper

113 100

111 102.1 81.6 122.4

192 17.6 14.4 21.6

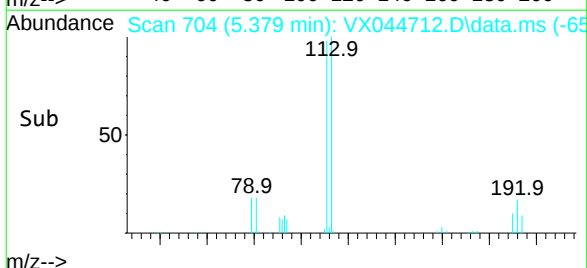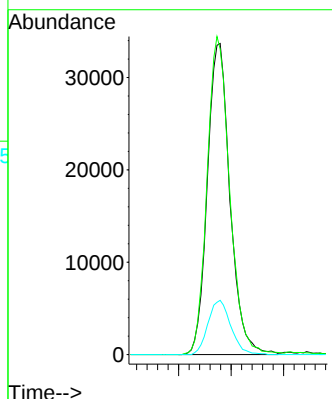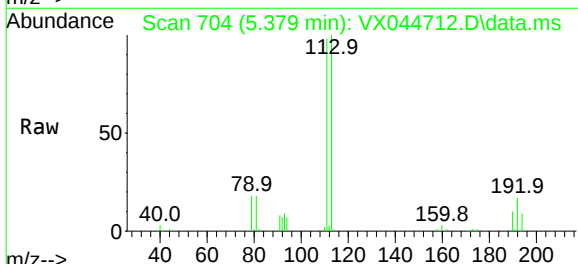

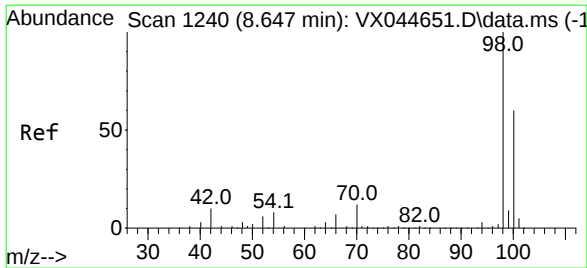

#50

Toluene-d8

Concen: 54.022 ug/l

RT: 8.641 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX044712.D

Acq: 27 Jan 2025 10:38

Instrument :

MSVOA_X

ClientSampleId :





VX0127MBL01

Tgt Ion: 98 Resp: 376419

Ion Ratio Lower Upper

98 100

100 65.8 53.2 79.8

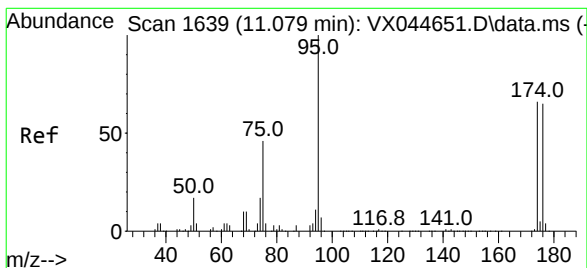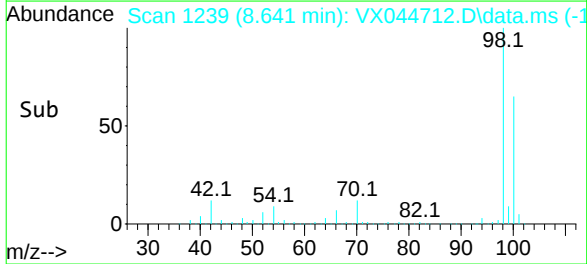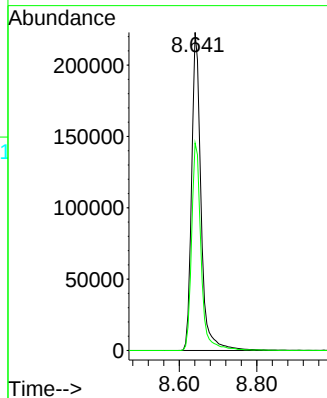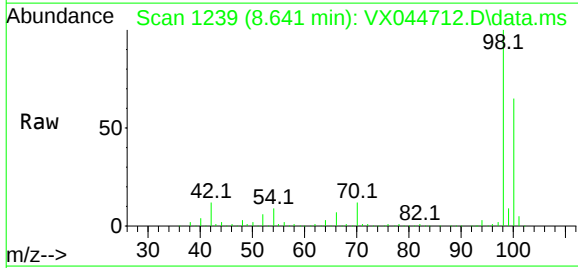

#62

4-Bromofluorobenzene

Concen: 53.523 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX044712.D

Acq: 27 Jan 2025 10:38




Tgt Ion: 95 Resp: 139028


Ion Ratio Lower Upper

95 100

174 70.5 0.0 133.0

176 67.4 0.0 129.4

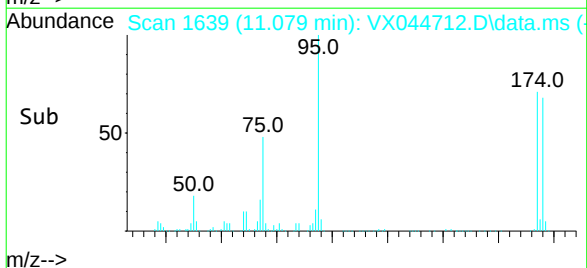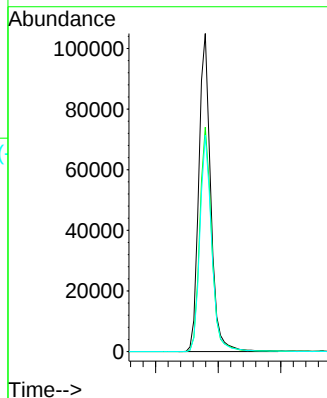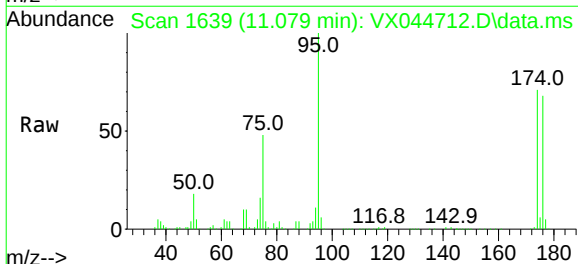

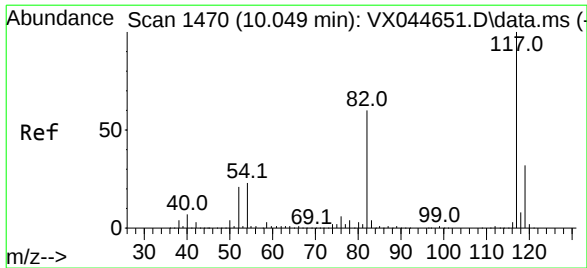

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. 0.000 min

Lab File: VX044712.D

Acq: 27 Jan 2025 10:38

Instrument :

MSVOA_X

ClientSampleId :

VX0127MBL01





Tgt Ion:117 Resp: 278587

Ion Ratio Lower Upper

117 100

82 58.0 47.6 71.4

119 32.7 25.4 38.2

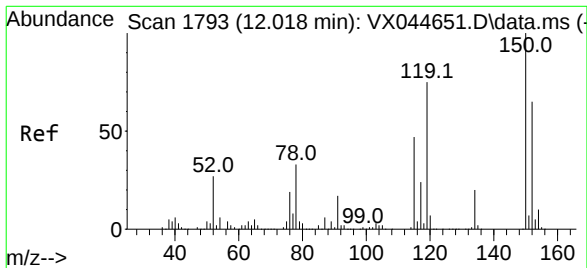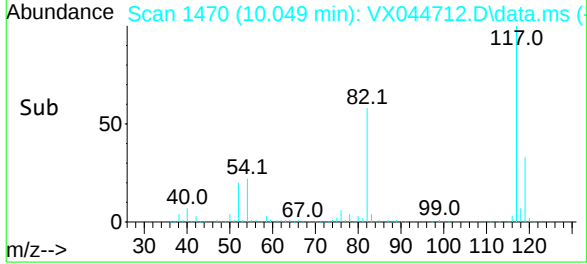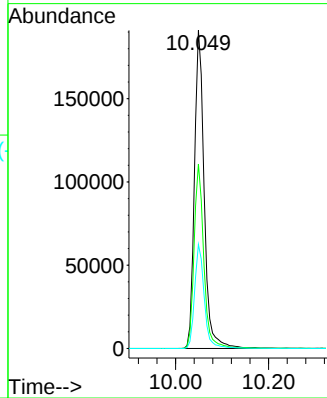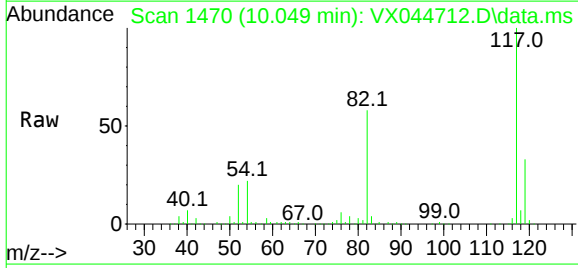

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX044712.D

Acq: 27 Jan 2025 10:38

Tgt Ion:152 Resp: 122776

Ion Ratio Lower Upper

152 100

115 62.3 43.8 131.4

150 156.8 0.0 347.8

