
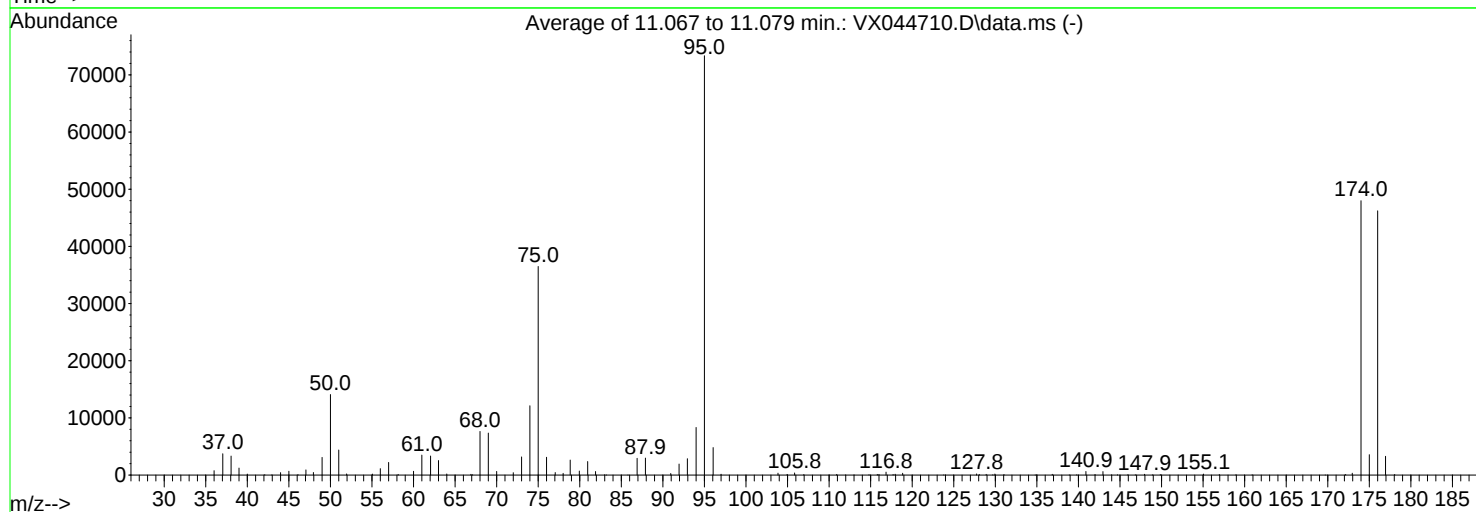


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012725\
Data File : VX044710.D
Acq On : 27 Jan 2025 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011525W.M
Title : SW846 8260
Last Update : Thu Jan 16 01:16:09 2025

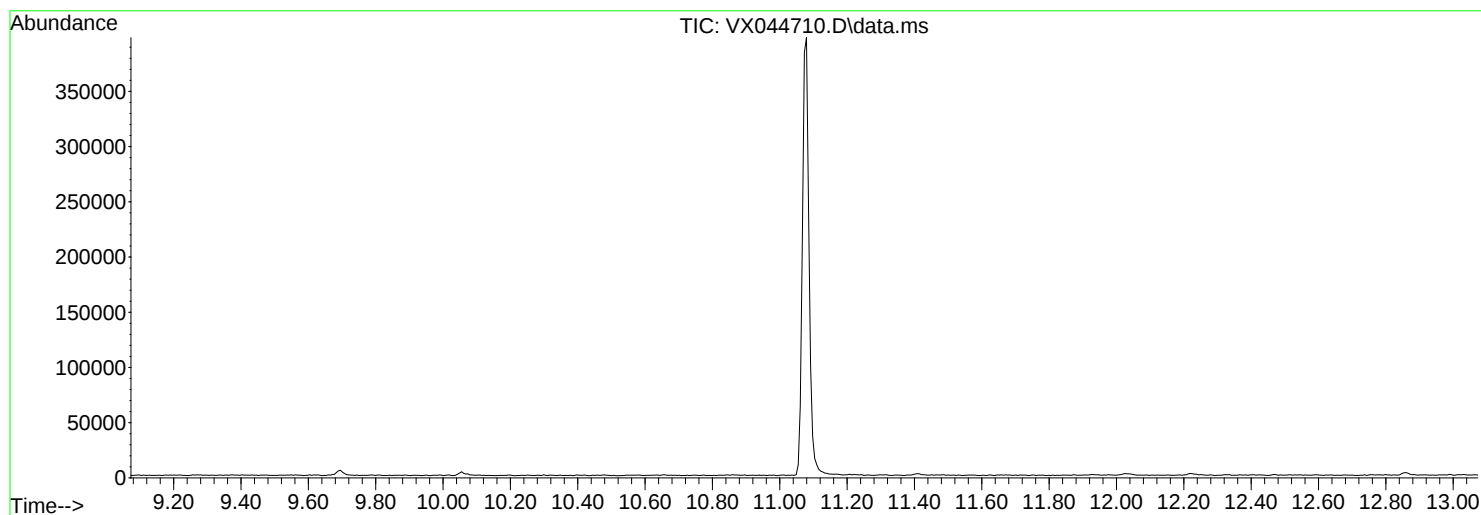

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	14088	PASS
75	95	30	60	49.7	36488	PASS
95	95	100	100	100.0	73349	PASS
96	95	5	9	6.6	4811	PASS
173	174	0.00	2	0.7	327	PASS
174	95	50	100	65.4	47992	PASS
175	174	5	9	7.4	3572	PASS
176	174	95	101	96.3	46227	PASS
177	176	5	9	7.1	3286	PASS