

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX012819\
 Data File : VX007269.D
 Acq On : 28 Jan 2019 18:58
 Operator : JC/SP
 Sample : K1011-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OR-01-012519-A

Quant Time: Jan 29 00:20:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 08 14:06:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	539282	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	826465	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	792037	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	387742	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	290565	51.56	ug/l	0.00
Spiked Amount			Recovery	=	103.12%	
35) Dibromofluoromethane	5.50	113	260116	49.15	ug/l	0.00
Spiked Amount			Recovery	=	98.30%	
50) Toluene-d8	8.71	98	1020985	52.70	ug/l	0.00
Spiked Amount			Recovery	=	105.40%	
62) 4-Bromofluorobenzene	11.13	95	359521	53.23	ug/l	0.00
Spiked Amount			Recovery	=	106.46%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.33	50	1148	0.223	ug/l	98
11) Tert butyl alcohol	3.03	59	1417	1.066	ug/l #	16
13) Acrolein	2.30	56	518	3.976	ug/l #	73
16) Acetone	2.45	43	64146	23.022	ug/l	99
18) Methyl Acetate	2.78	43	3335	0.413	ug/l #	80
20) Methylene Chloride	2.86	84	483269	91.664	ug/l	97
25) 2-Butanone	4.70	43	9656	2.422	ug/l	95
29) Tetrahydrofuran	5.17	42	3304	1.275	ug/l #	51
36) 1,1-Dichloropropene	5.67	75	34100	4.746	ug/l #	48
38) Carbon Tetrachloride	5.66	117	49294	6.819	ug/l #	14
40) Benzene	6.15	78	4508	0.206	ug/l	95
43) Isopropyl Acetate	6.46	43	18844	1.551	ug/l #	95
48) Methyl methacrylate	7.68	41	10297	1.650	ug/l #	21
49) 1,4-Dioxane	7.77	88	186	Below Cal	#	3
51) 4-Methyl-2-Pentanone	8.62	43	114153	14.618	ug/l #	50
52) Toluene	8.79	92	3893	0.276	ug/l	83
54) cis-1,3-Dichloropropene	8.62	75	54010	6.689	ug/l #	67
59) 2-Hexanone	9.54	43	116539	19.583	ug/l #	53
71) Bromoform	10.86	173	91	4.743	ug/l #	28
76) 1,2,3-Trichloropropane	11.13	75	174602	22.221	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.51	105	4572	0.200	ug/l	100
81) trans-1,4-Dichloro-2-buten	11.13	75	174602	65.770	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	5852	0.255	ug/l	92
90) Hexachloroethane	12.61	117	349	2.993	ug/l #	6
95) Naphthalene	13.83	128	35953	1.287	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX012819\
Data File : VX007269.D
Acq On : 28 Jan 2019 18:58
Operator : JC/SP
Sample : K1011-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OR-01-012519-A

Quant Time: Jan 29 00:20:36 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X010819W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 08 14:06:59 2019
Response via : Initial Calibration

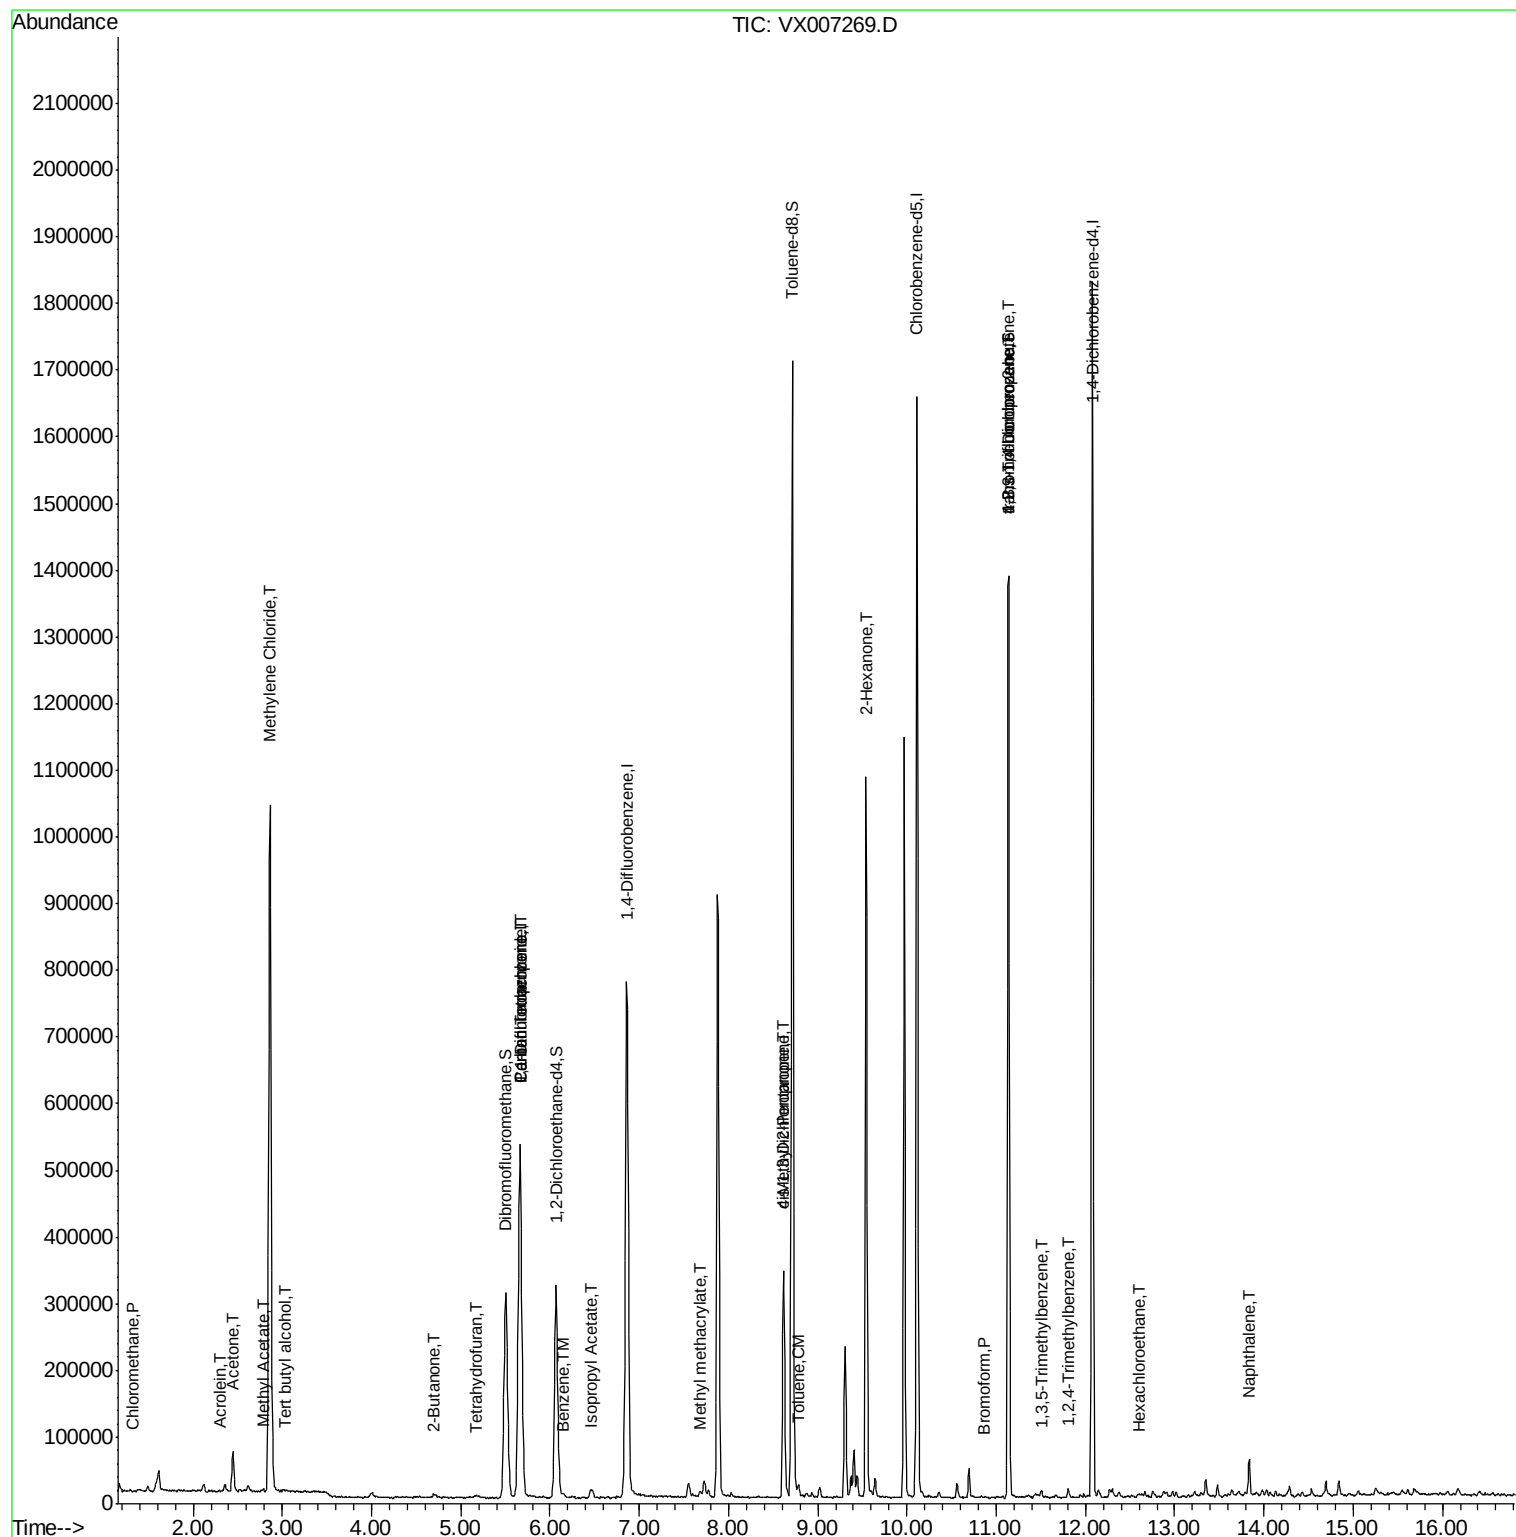

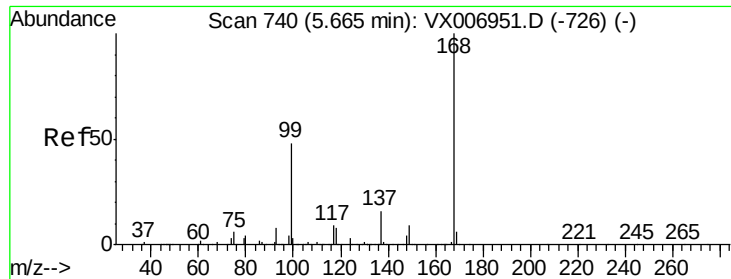

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :


OR-01-012519-A

Tot Ion:168 Resp: 539282

Ion Ratio Lower Upper

168 100

99 49.6 41.8 62.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

200000



150000

100000

50000

0

Time-->

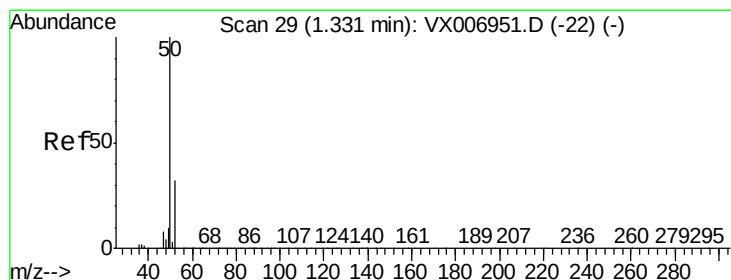

#3

Chloromethane

Concen: 0.223 ug/l

RT: 1.33 min Scan# 29

Delta R.T. -0.00 min

Lab File: VX007269.D


Acq: 28 Jan 2019 18:58

Tgt Ion: 50 Resp: 1148

Ion Ratio Lower Upper

50 100

52 30.8 25.4 38.2

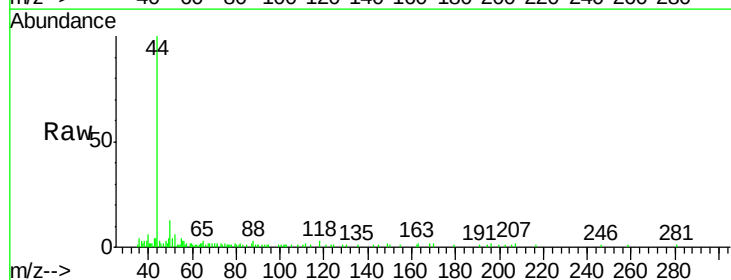

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.33

1000

800


600


400

200

0

Time-->






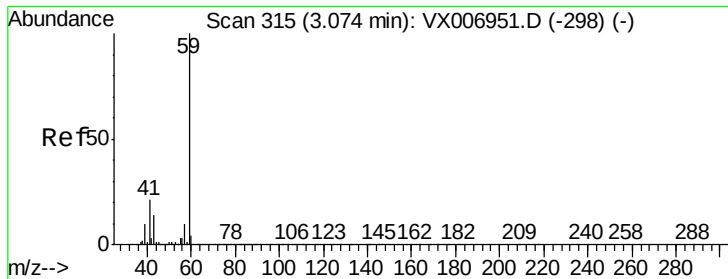


#11

Tert butyl alcohol
 Concen: 1.066 ug/l
 RT: 3.03 min Scan# 307
 Delta R.T. -0.05 min
 Lab File: VX007269.D
 Acq: 28 Jan 2019 18:58

Instrument :
 MSVOA_X
 ClientSampleId :
 OR-01-012519-A




Tot Ion: 59 Resp: 1417
 Ion Ratio Lower Upper
 59 100
 57 42.1 8.5 12.7#

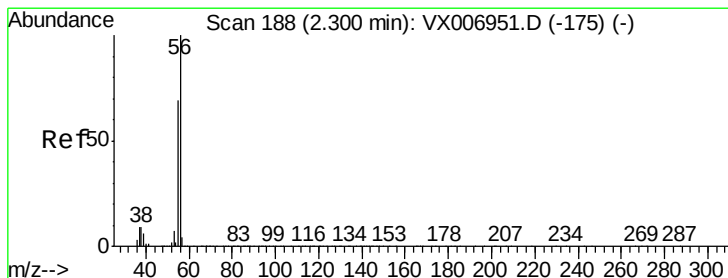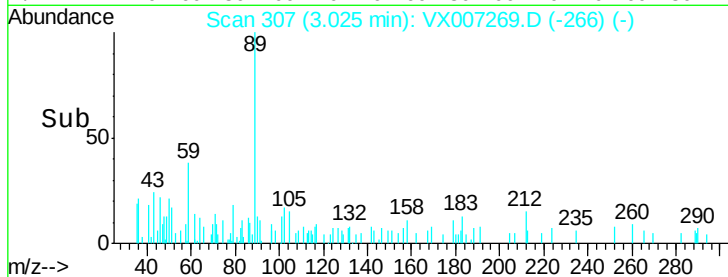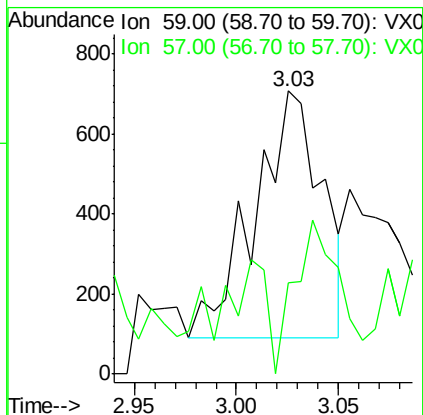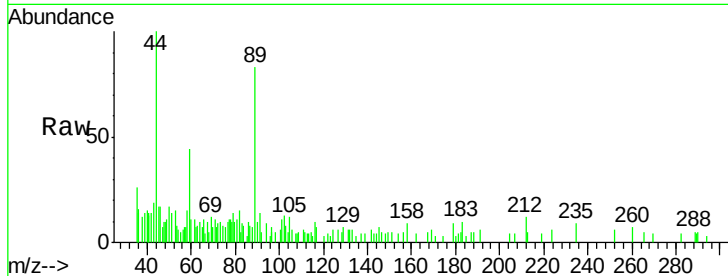


#13

Acrolein
 Concen: 3.976 ug/l
 RT: 2.30 min Scan# 188
 Delta R.T. -0.00 min
 Lab File: VX007269.D
 Acq: 28 Jan 2019 18:58

Tgt Ion: 56 Resp: 518
 Ion Ratio Lower Upper
 56 100
 55 95.4 58.2 87.4#

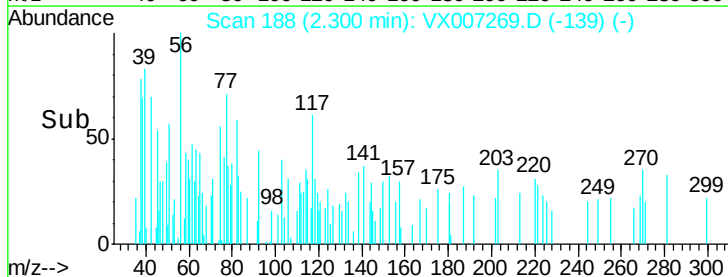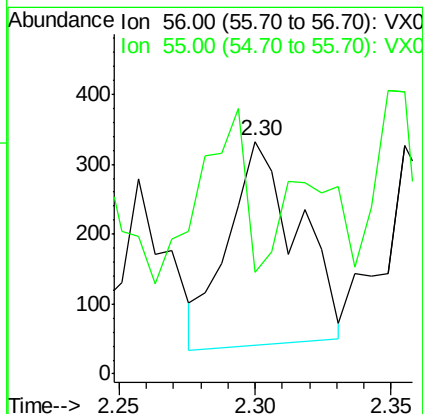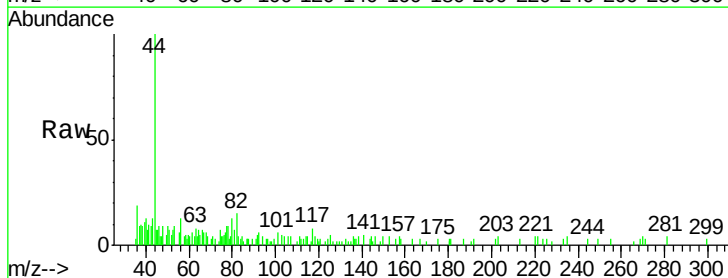



#16

Acetone

Concen: 23.022 ug/l

RT: 2.45 min Scan# 212

Delta R.T. -0.00 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :


OR-01-012519-A

Tot Ion: 43 Resp: 64146

Ion Ratio Lower Upper

43 100

58 31.6 25.0 37.6



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45

40000

30000



20000

10000

0

Time-->

2.35 2.40 2.45 2.50 2.55

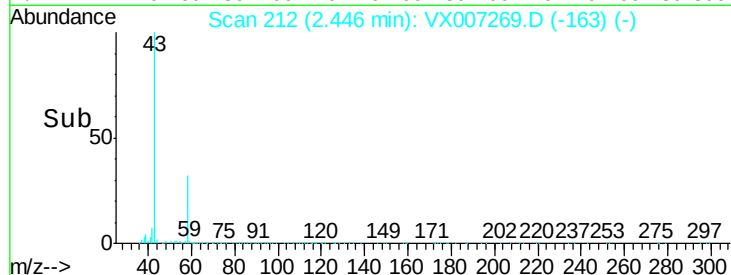

#18

Methyl Acetate

Concen: 0.413 ug/l

RT: 2.78 min Scan# 266

Delta R.T. -0.01 min

Lab File: VX007269.D


Acq: 28 Jan 2019 18:58

Tgt Ion: 43 Resp: 3335

Ion Ratio Lower Upper

43 100

74 32.9 18.6 28.0#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

2.78

2000

1500


1000


500

0

Time-->

2.70 2.75 2.80









#20
Methylene Chloride
Concen: 91.664 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.00 min
Lab File: VX007269.D
Acq: 28 Jan 2019 18:58




Instrument :
MSVOA_X
ClientSampleId :
OR-01-012519-A


Tot Ion:	84	Resp:	483269
Ion	Ratio	Lower	Upper
84	100		
49	119.6	91.8	137.6
51	37.2	28.5	42.7
86	64.1	50.2	75.2

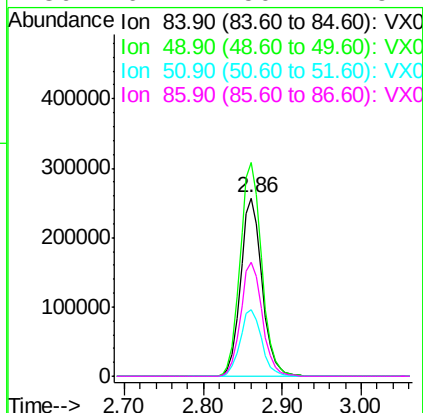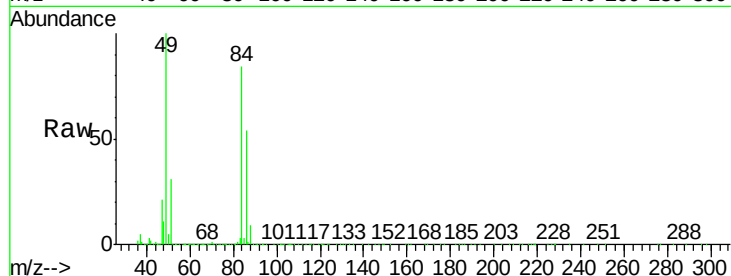

#25
2-Butanone
Concen: 2.422 ug/l
RT: 4.70 min Scan# 582
Delta R.T. -0.00 min
Lab File: VX007269.D
Acq: 28 Jan 2019 18:58

Tgt Ion:	43	Resp:	9656
Ion	Ratio	Lower	Upper
43	100		
72	25.3	22.4	33.6

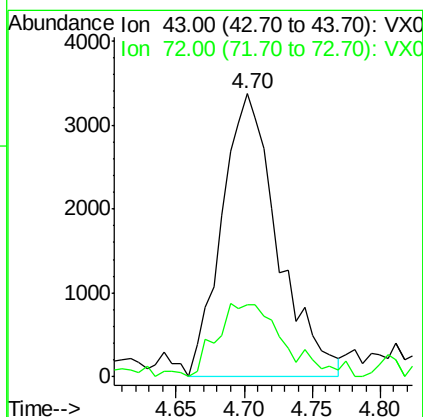

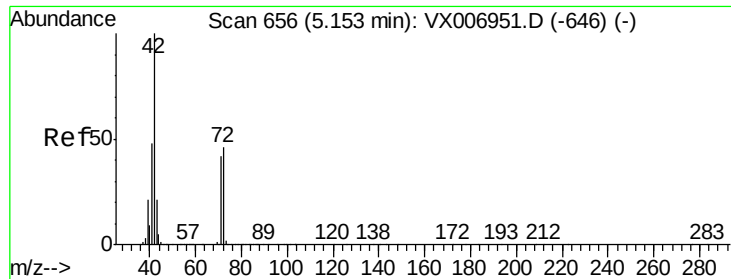

#29

Tetrahydrofuran

Concen: 1.275 ug/l

RT: 5.17 min Scan# 658

Delta R.T. 0.01 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :

OR-01-012519-A


Tot Ion: 42 Resp: 3304

Ion Ratio Lower Upper

42 100

72 28.5 38.9 58.3#




71 0.0 36.2 54.4#



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

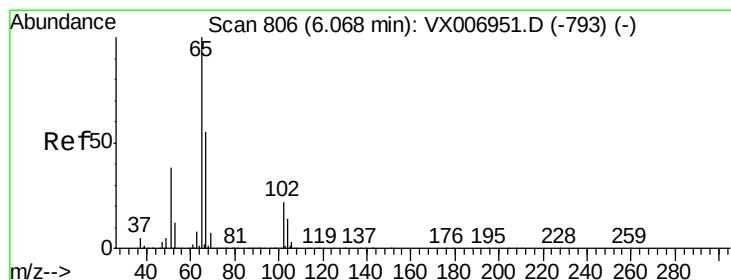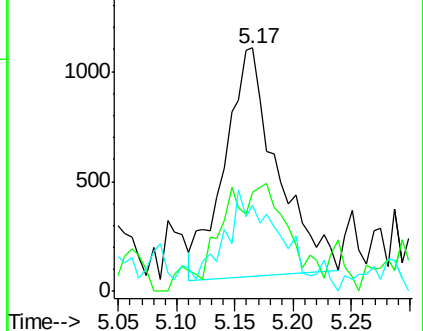

#33

1,2-Dichloroethane-d4

Concen: 51.556 ug/l

RT: 6.07 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX007269.D


Acq: 28 Jan 2019 18:58

Tgt Ion: 65 Resp: 290565

Ion Ratio Lower Upper



65 100


67 53.4 0.0 105.0



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

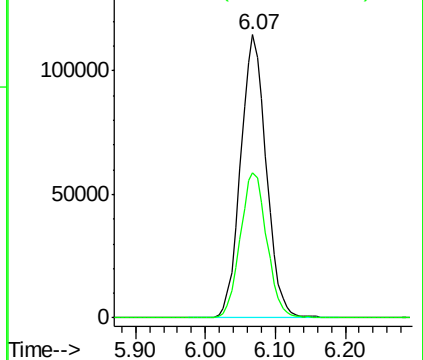




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX007269.D
 Acq: 28 Jan 2019 18:58

Instrument :
 MSVOA_X
 ClientSampleId :
 OR-01-012519-A




Tot Ion	Ratio	Lower	Upper
114	100		
63	18.5	0.0	34.8
88	14.3	0.0	28.8

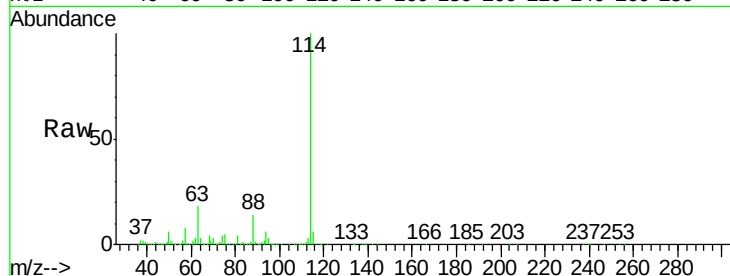

Abundance Ion 113.90 (113.60 to 114.60): V


Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

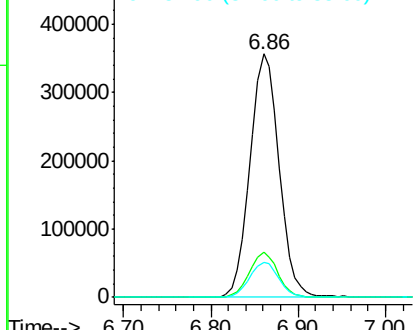

#35
 Dibromofluoromethane
 Concen: 49.147 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. -0.00 min
 Lab File: VX007269.D
 Acq: 28 Jan 2019 18:58



Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.5	81.6	122.4
192	22.1	16.7	25.1




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V




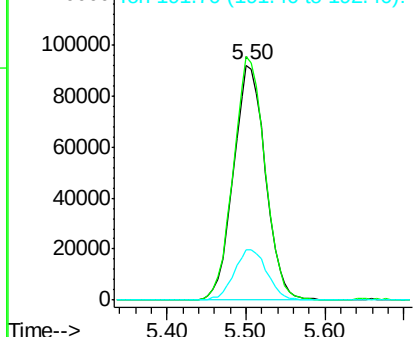


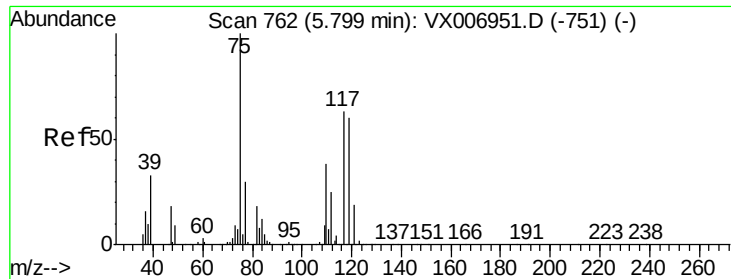

#36
 1,1-Dichloropropene
 Concen: 4.746 ug/l
 RT: 5.67 min Scan# 740
 Delta R.T. -0.13 min
 Lab File: VX007269.D
 Acq: 28 Jan 2019 18:58




Instrument :
 MSVOA_X
 ClientSampleId :
 OR-01-012519-A


Tot Ion	Ratio	Lower	Upper
75	100		
110	10.2	20.2	60.5#
77	0.4	24.8	37.2#

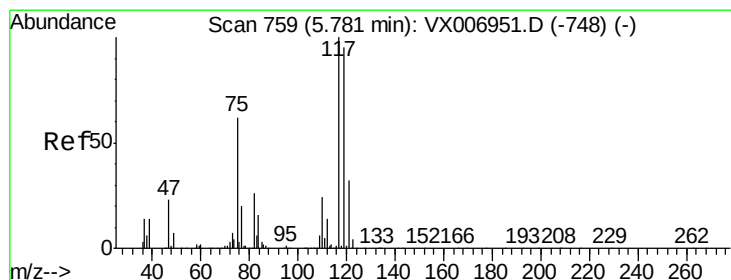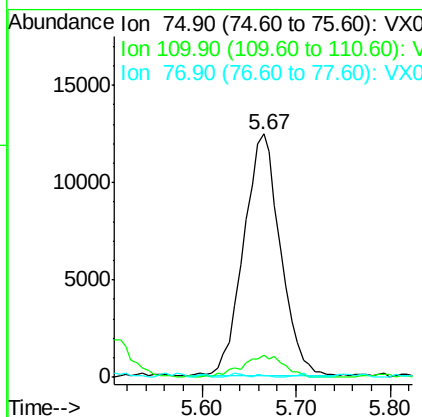

#38
 Carbon Tetrachloride
 Concen: 6.819 ug/l
 RT: 5.66 min Scan# 739
 Delta R.T. -0.12 min
 Lab File: VX007269.D
 Acq: 28 Jan 2019 18:58

Tgt Ion	Ratio	Lower	Upper
117	100		
119	4.0	79.4	119.2#
121	0.0	24.0	36.0#

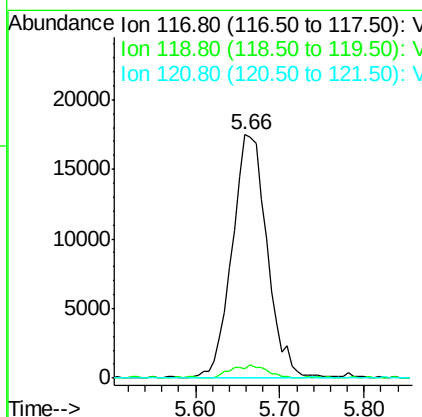

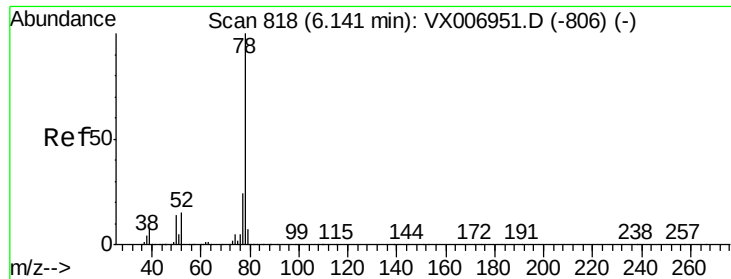

#40

Benzene

Concen: 0.206 ug/l

RT: 6.15 min Scan# 819

Delta R.T. 0.01 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :


OR-01-012519-A

Tot Ion: 78 Resp: 4508

Ion Ratio Lower Upper

78 100

77 26.5 19.2 28.8

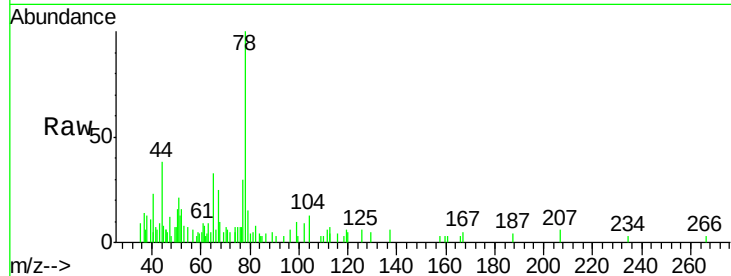

Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

6.15

2000

1500



1000

500

0

6.05 6.10 6.15 6.20 6.25

Time-->

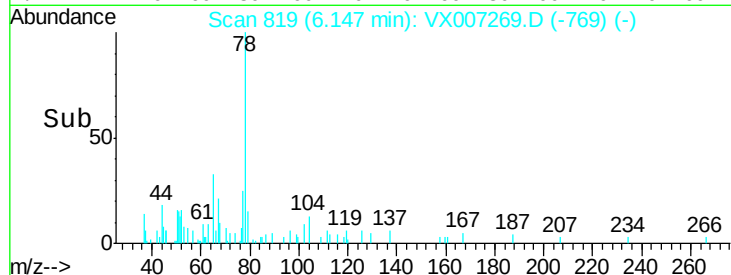

#43

Isopropyl Acetate

Concen: 1.551 ug/l

RT: 6.46 min Scan# 870

Delta R.T. -0.00 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58


Tgt Ion: 43 Resp: 18844

Ion Ratio Lower Upper

43 100

61 22.3 16.8 25.2

87 11.8 12.4 18.6#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

6.46

8000

6000


4000


2000

0

6.40 6.45 6.50 6.55 6.60

Time-->





#48

Methvl methacrylate

Concen: 1.650 ug/l

RT: 7.68 min Scan# 1071

Delta R.T. -0.09 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :

OR-01-012519-A





Tot Ion: 41 Resp: 10297

Ion Ratio Lower Upper

41 100

69 4.0 72.4 108.6#

39 14.1 45.8 68.8#

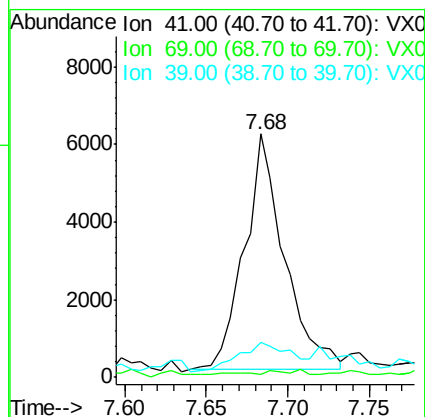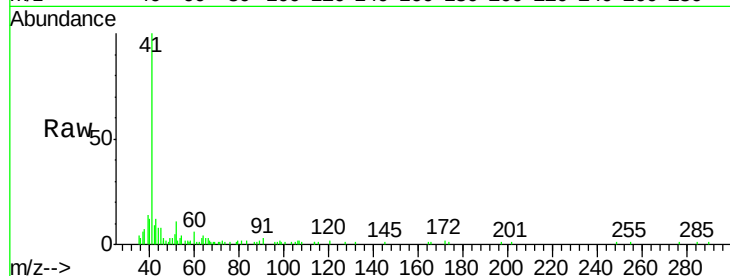

#49

1,4-Dioxane

Concen: Below Cal

RT: 7.77 min Scan# 1085

Delta R.T. 0.02 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58




Tgt Ion: 88 Resp: 186


Ion Ratio Lower Upper

88 100

43 0.0 22.2 33.4#

58 154.3 51.0 76.4#



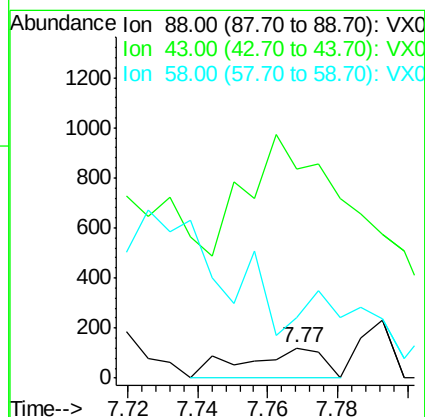



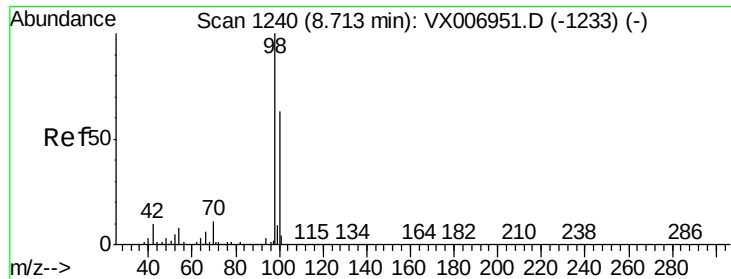

#50
Toluene-d8
Concen: 52.702 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX007269.D
Acq: 28 Jan 2019 18:58




Instrument :
MSVOA_X
ClientSampleId :
OR-01-012519-A


Tot Ion: 98 Resp: 1020985
Ion Ratio Lower Upper
98 100
100 63.1 52.0 78.0

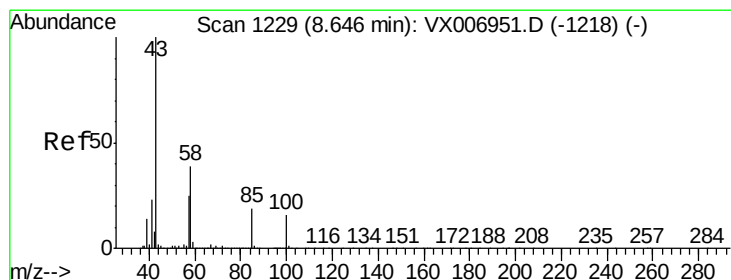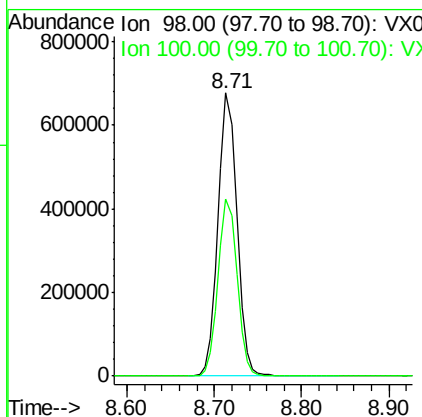

#51
4-Methyl-2-Pentanone
Concen: 14.618 ug/l
RT: 8.62 min Scan# 1224
Delta R.T. -0.03 min
Lab File: VX007269.D
Acq: 28 Jan 2019 18:58

Tgt Ion: 43 Resp: 114153
Ion Ratio Lower Upper
43 100
58 9.2 31.8 47.6#

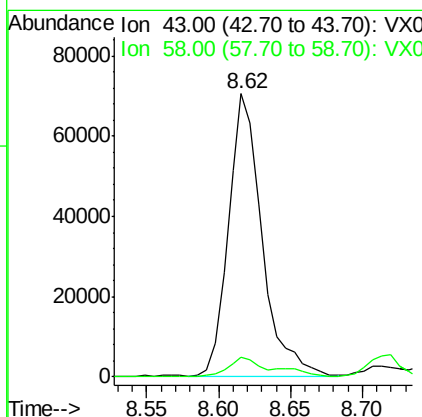



#52

Toluene

Concen: 0.276 ug/l

RT: 8.79 min Scan# 1252

Delta R.T. -0.00 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :


OR-01-012519-A

Tot Ion: 92 Resp: 3893

Ion Ratio Lower Upper




92 100

91 149.1 137.6 206.4

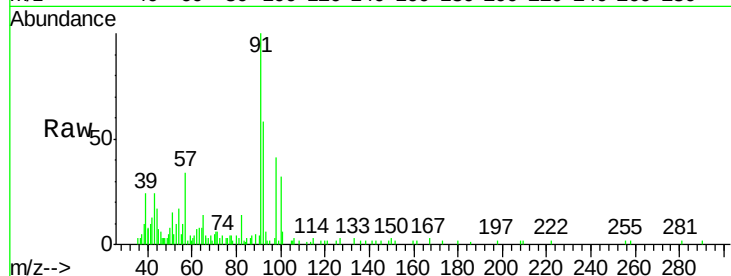

Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0

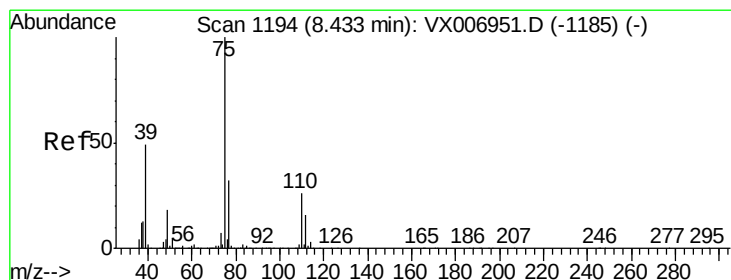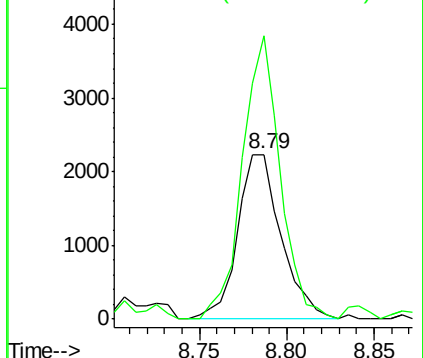

#54

cis-1,3-Dichloropropene

Concen: 6.689 ug/l

RT: 8.62 min Scan# 1224

Delta R.T. 0.18 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58


Tgt Ion: 75 Resp: 54010

Ion Ratio Lower Upper

75 100

77 1.0 26.2 39.2#



39 35.0 36.7 55.1#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

Ion 39.00 (38.70 to 39.70): VX0



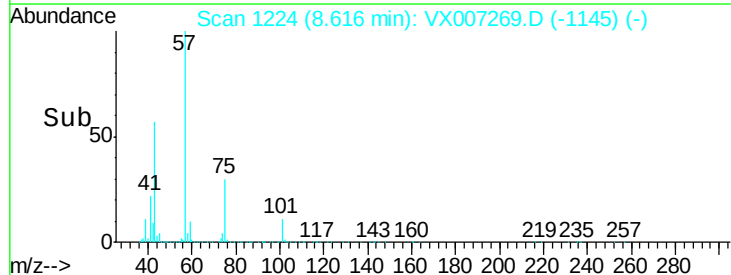
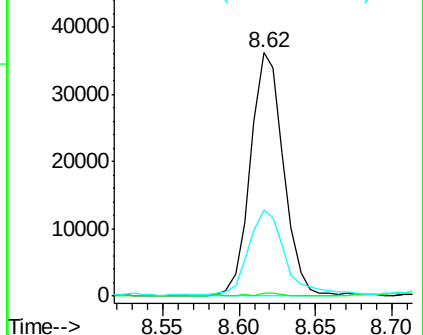




#59
2-Hexanone
Concen: 19.583 ug/l
RT: 9.54 min Scan# 1376
Delta R.T. 0.05 min
Lab File: VX007269.D
Acq: 28 Jan 2019 18:58




Instrument :
MSVOA_X
ClientSampleId :
OR-01-012519-A


Tot Ion: 43 Resp: 116539
Ion Ratio Lower Upper
43 100
58 21.2 27.7 83.1#

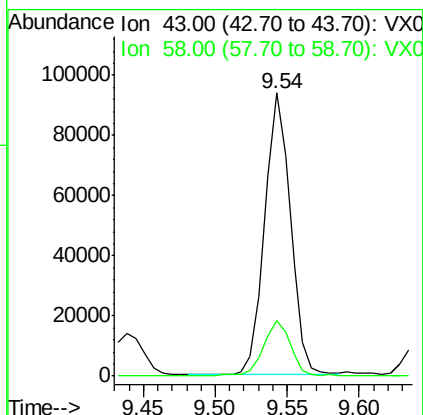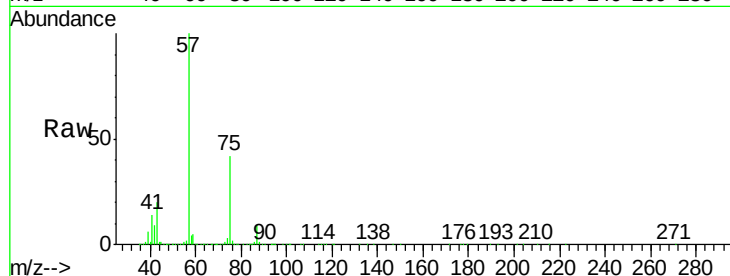

#62
4-Bromofluorobenzene
Concen: 53.233 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX007269.D
Acq: 28 Jan 2019 18:58

Tgt Ion: 95 Resp: 359521
Ion Ratio Lower Upper
95 100
174 92.9 0.0 182.2
176 91.1 0.0 178.8

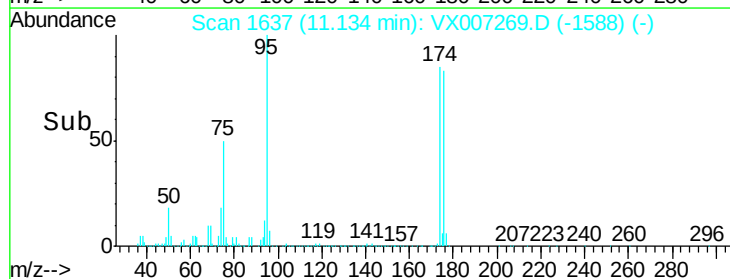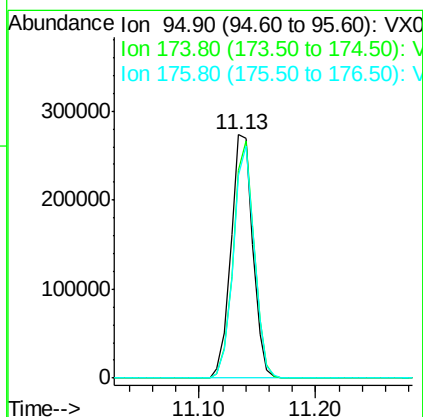



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. -0.00 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :

OR-01-012519-A


Tot Ion:117 Resp: 792037

Ion Ratio Lower Upper

117 100

82 49.8 41.0 61.6




119 32.7 25.4 38.0



Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

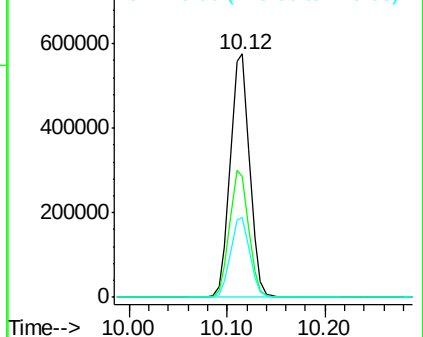

#71

Bromoform

Concen: 4.743 ug/l

RT: 10.86 min Scan# 1592

Delta R.T. 0.00 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58


Tgt Ion:173 Resp: 91

Ion Ratio Lower Upper

173 100

175 0.0 24.7 74.1#



254 0.0 0.2 0.2#




Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

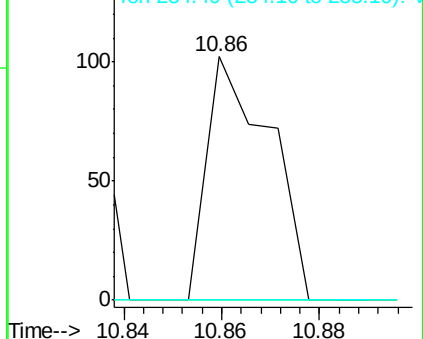



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :

OR-01-012519-A


Tot Ion:152 Resp: 387742

Ion Ratio Lower Upper

152 100

115 55.2 39.1 117.2




150 157.5 0.0 344.8

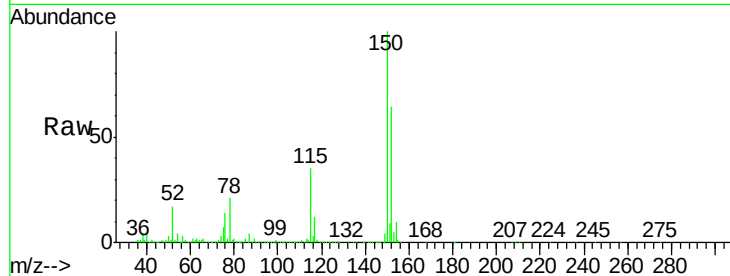

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

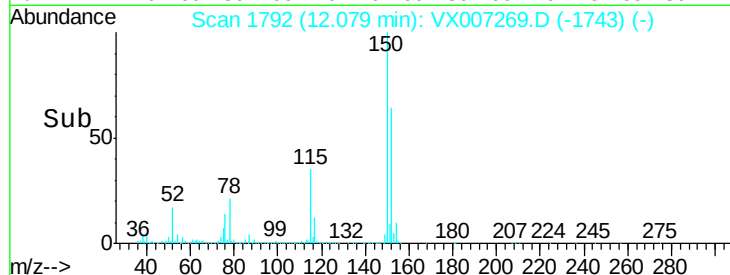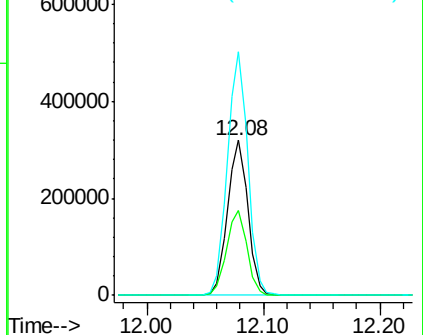

#76

1,2,3-Trichloropropane

Concen: 22.221 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX007269.D


Acq: 28 Jan 2019 18:58

Tgt Ion: 75 Resp: 174602

Ion Ratio Lower Upper



75 100


77 1.4 18.5 55.5#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

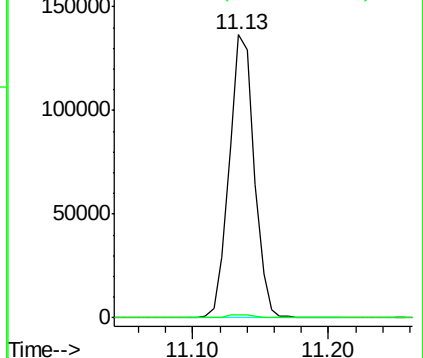

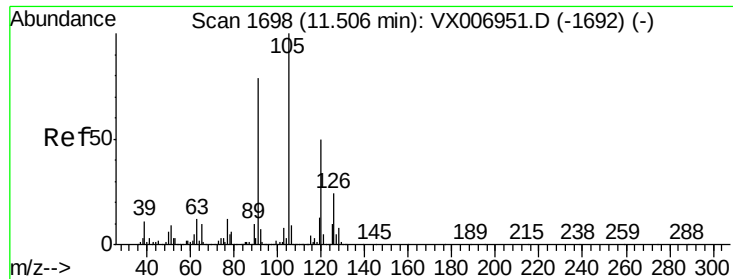

#80

1,3,5-Trimethylbenzene

Concen: 0.200 ug/l

RT: 11.51 min Scan# 1698

Delta R.T. -0.00 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58

Instrument :

MSVOA_X

ClientSampleId :


OR-01-012519-A

Tot Ion:105 Resp: 4572

Ion Ratio Lower Upper




105 100

120 50.2 25.1 75.3

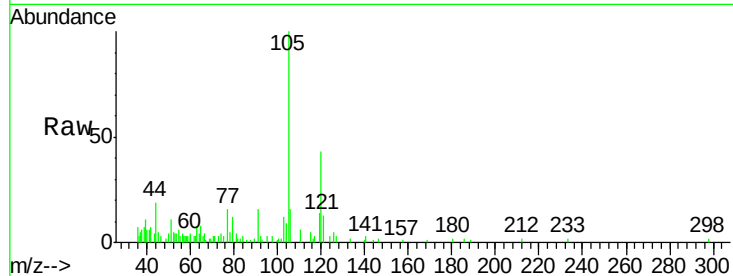

Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

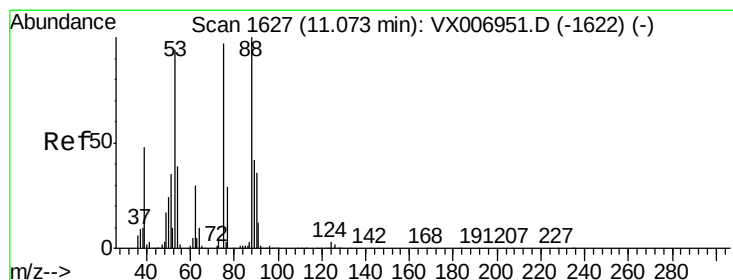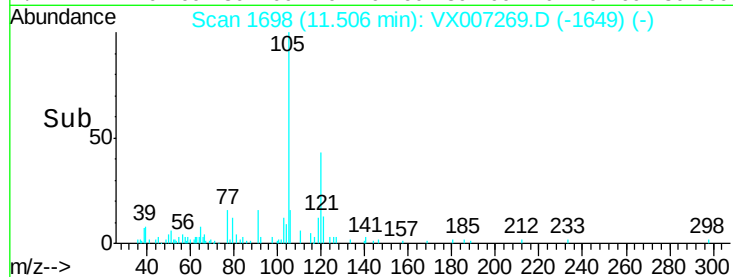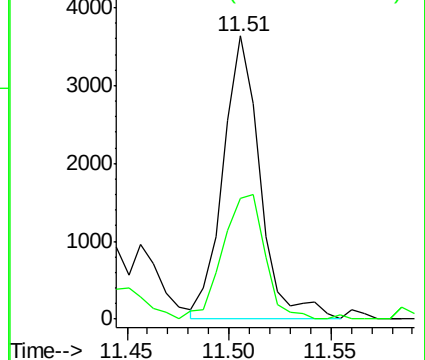

#81

trans-1,4-Dichloro-2-butene

Concen: 65.770 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX007269.D

Acq: 28 Jan 2019 18:58


Tgt Ion: 75 Resp: 174602

Ion Ratio Lower Upper

75 100

53 0.1 79.7 119.5#



89 0.0 38.0 57.0#

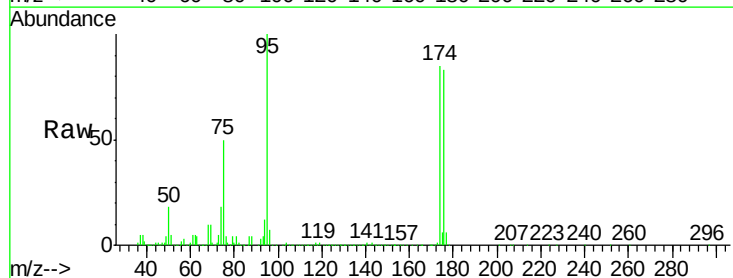


Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0



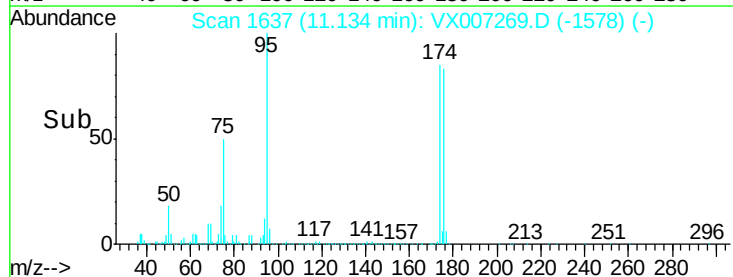
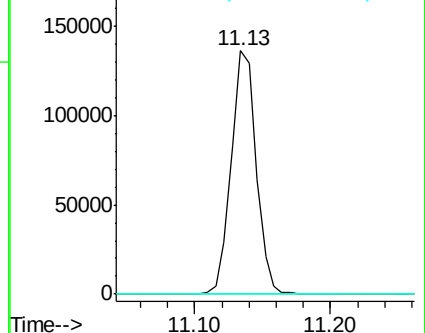




#84
 1,2,4-Trimethylbenzene
 Concen: 0.255 ug/l
 RT: 11.80 min Scan# 1747
 Delta R.T. -0.00 min
 Lab File: VX007269.D
 Acq: 28 Jan 2019 18:58




Instrument :
 MSVOA_X
 ClientSampleId :
 OR-01-012519-A


Tot Ion:105 Resp: 5852
 Ion Ratio Lower Upper
 105 100
 120 52.0 23.2 69.6

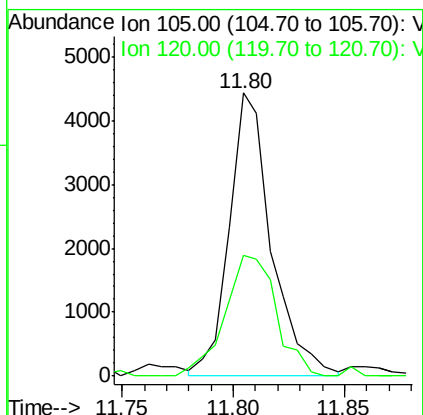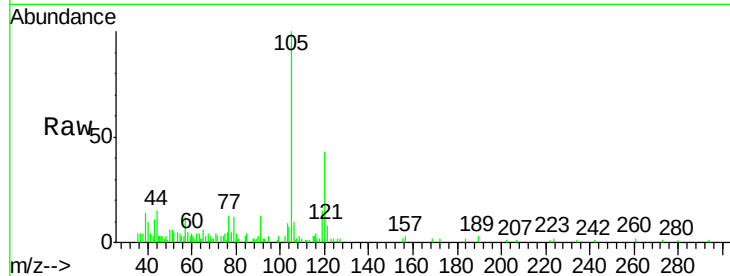

#90
 Hexachloroethane
 Concen: 2.993 ug/l
 RT: 12.61 min Scan# 1879
 Delta R.T. 0.01 min
 Lab File: VX007269.D
 Acq: 28 Jan 2019 18:58

Tgt Ion:117 Resp: 349
 Ion Ratio Lower Upper
 117 100
 201 0.0 42.9 128.7#

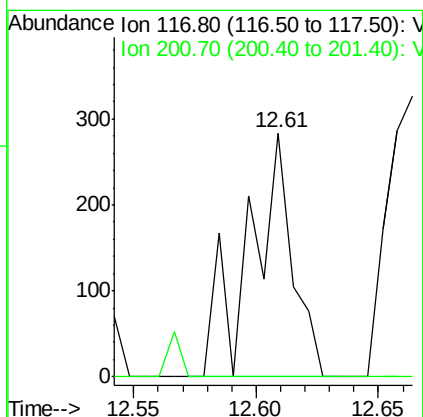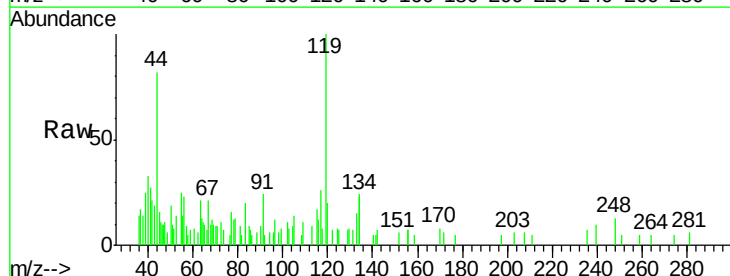

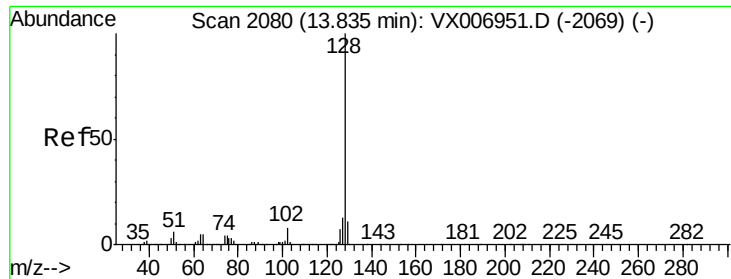

#95
Naphthalene
Concen: 1.287 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. -0.00 min
Lab File: VX007269.D
Acq: 28 Jan 2019 18:58

Instrument :
MSVOA_X
ClientSampleId :
OR-01-012519-A

Tot Ion	Ratio	Lower	Upper
128	100		
127	13.1	10.1	15.1
129	11.9	8.6	13.0

