


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX012820\
Data File : VX014739.D
Acq On : 28 Jan 2020 09:46
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Title : SW846 8260
Last Update : Wed Jan 22 12:35:15 2020

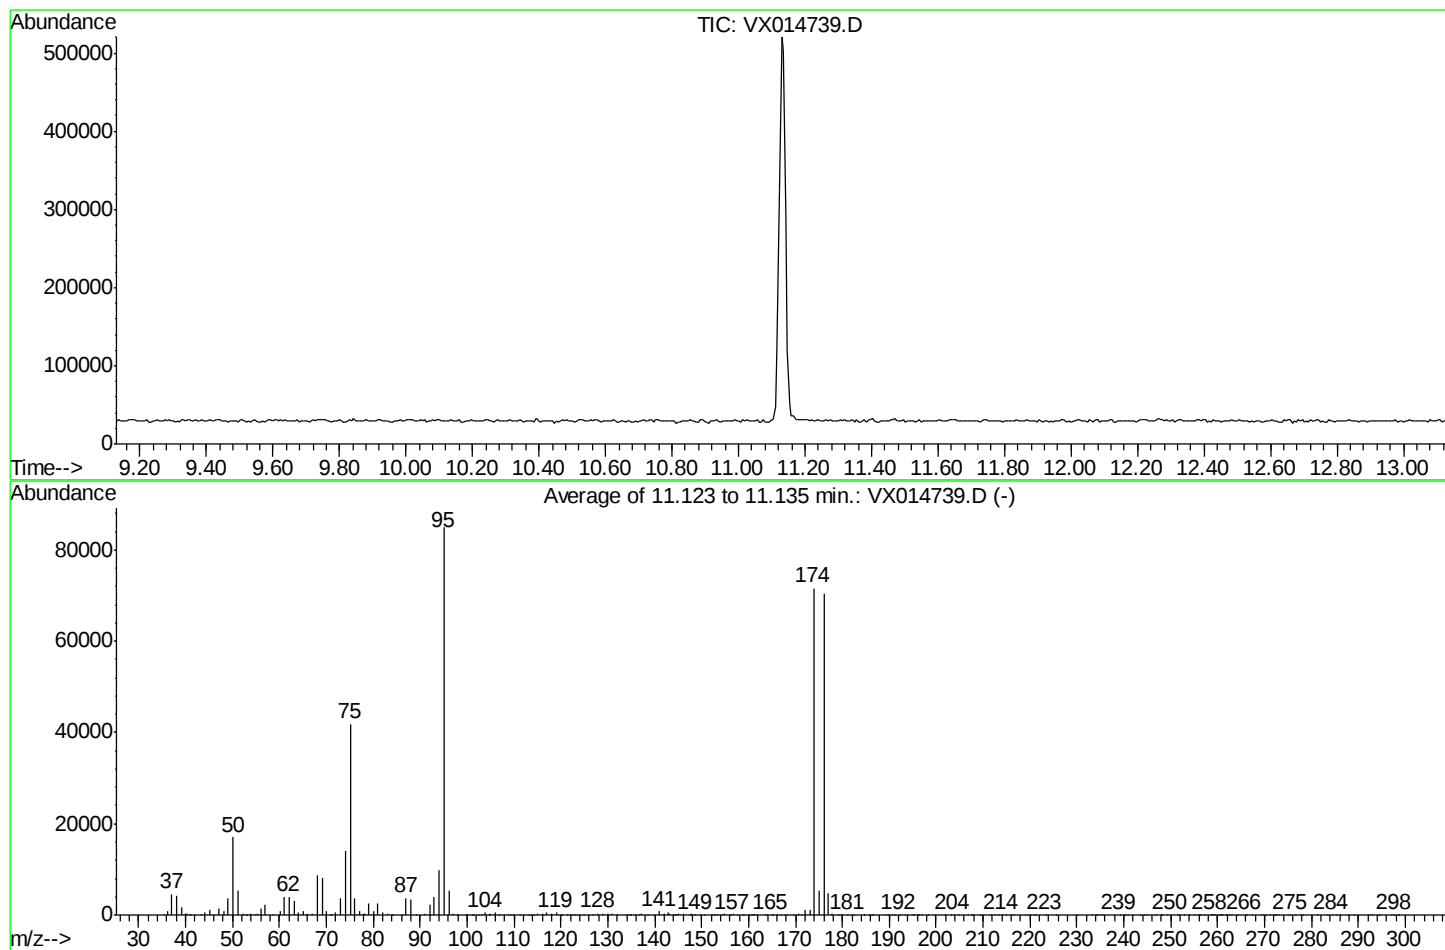

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	16991	PASS
75	95	30	60	49.3	41866	PASS
95	95	100	100	100.0	84977	PASS
96	95	5	9	6.4	5461	PASS
173	174	0.00	2	1.6	1133	PASS
174	95	50	100	84.2	71575	PASS
175	174	5	9	7.4	5276	PASS
176	174	95	101	98.4	70445	PASS
177	176	5	9	6.9	4876	PASS