


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012821\
Data File : VX020786.D
Acq On : 28 Jan 2021 09:07
Operator : JC/SP
Sample : VSTD0.0534
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTD0.05304

Manual Integrations
APPROVED

MMDadoda
2/3/2021 9:42:21 AM

Quant Time: Jan 29 01:43:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 29 01:43:09 2021
Response via : Initial Calibration

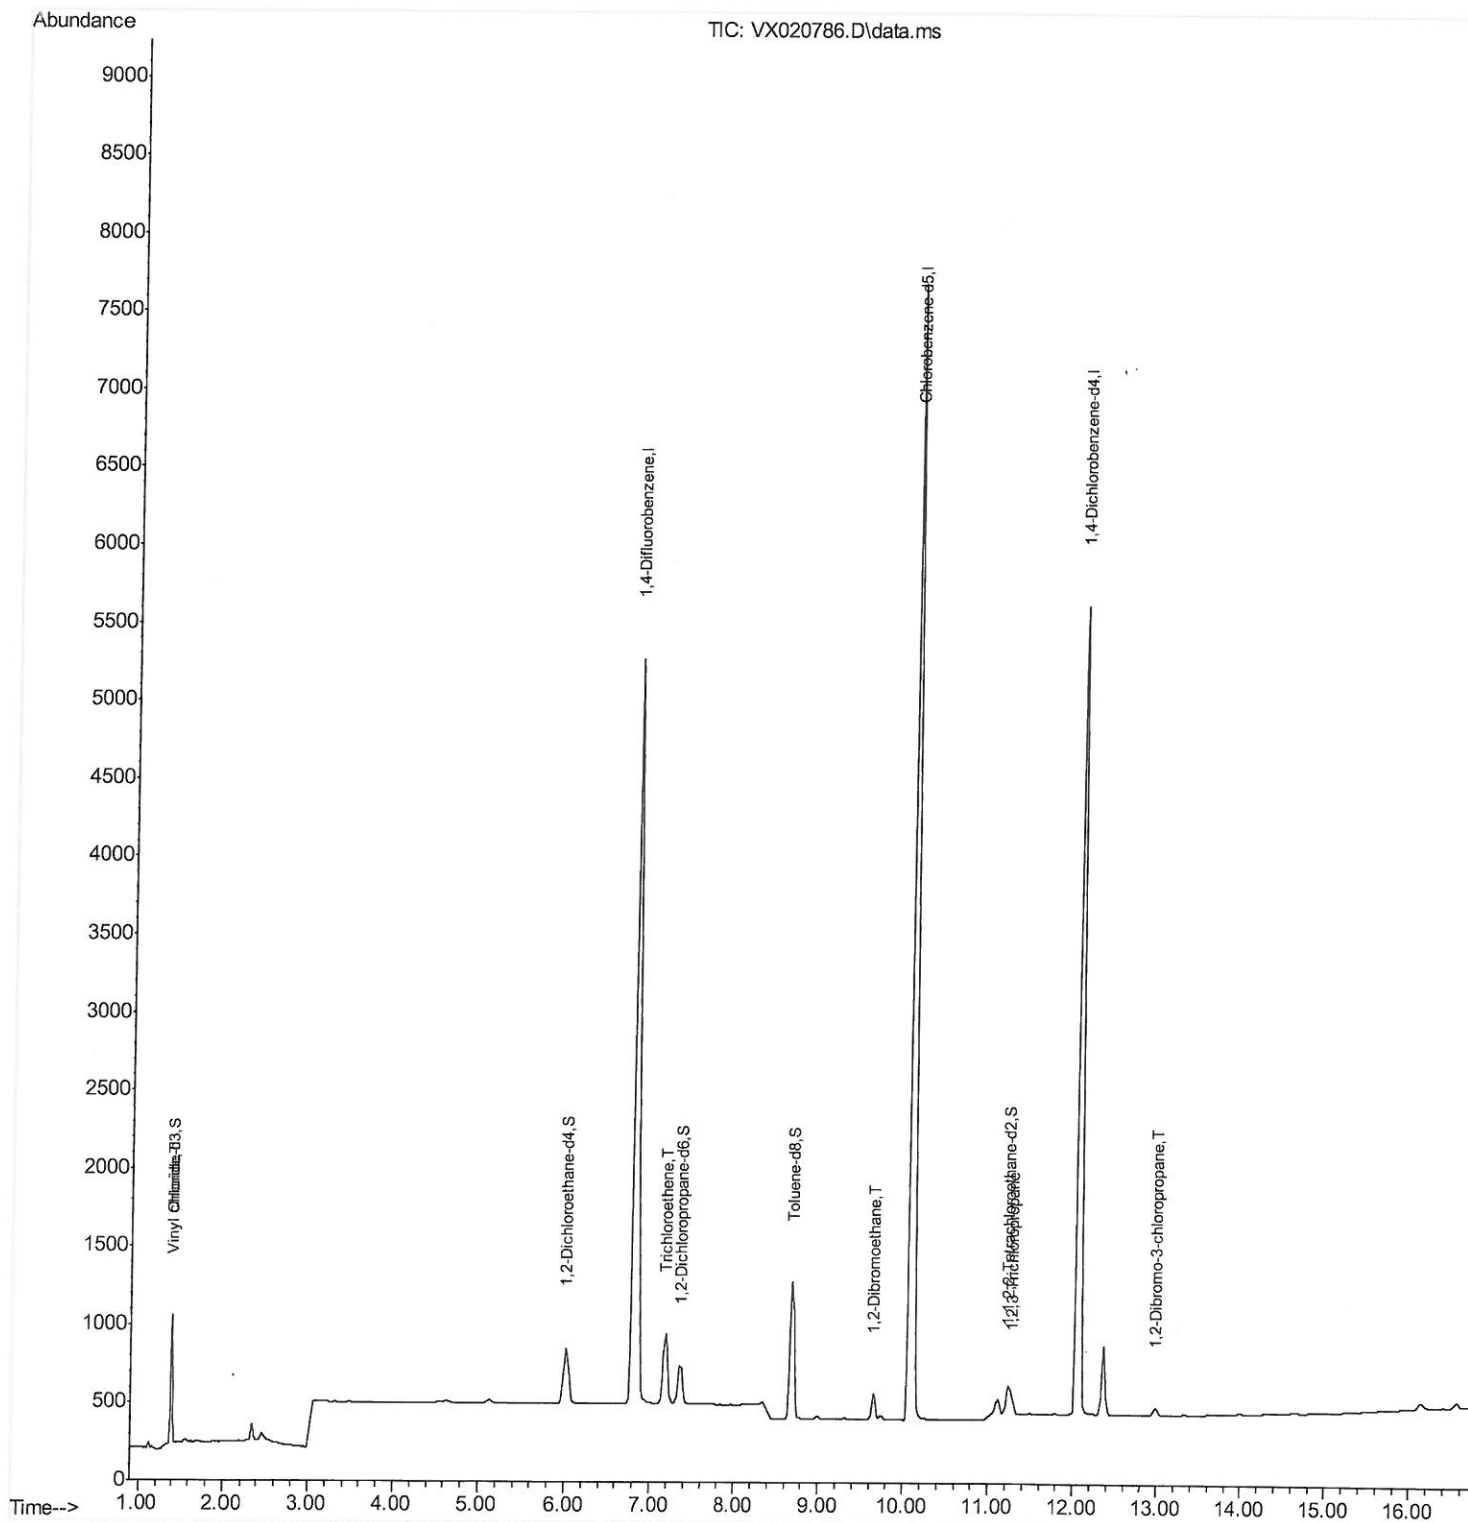

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012821\
Data File : VX020786.D
Acq On : 28 Jan 2021 09:07
Operator : JC/SP
Sample : VSTD0.0534
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTD0.05304

Manual Integrations
APPROVED

MMDadoda
2/3/2021 9:42:21 AM

Quant Time: Jan 29 01:43:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 29 01:43:09 2021
Response via : Initial Calibration

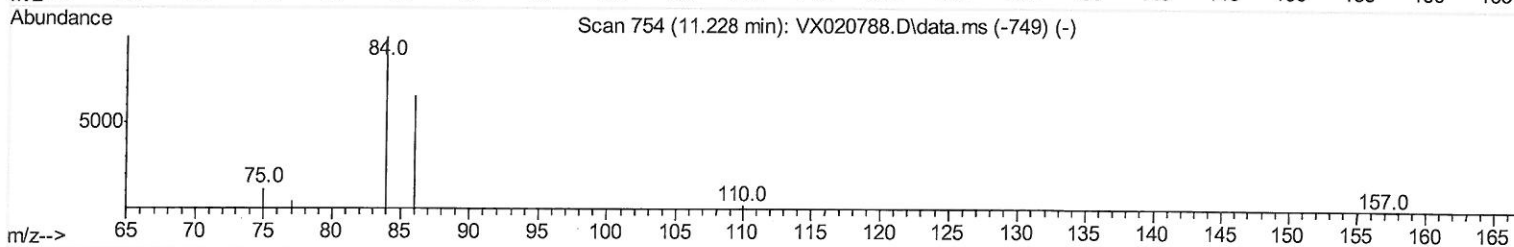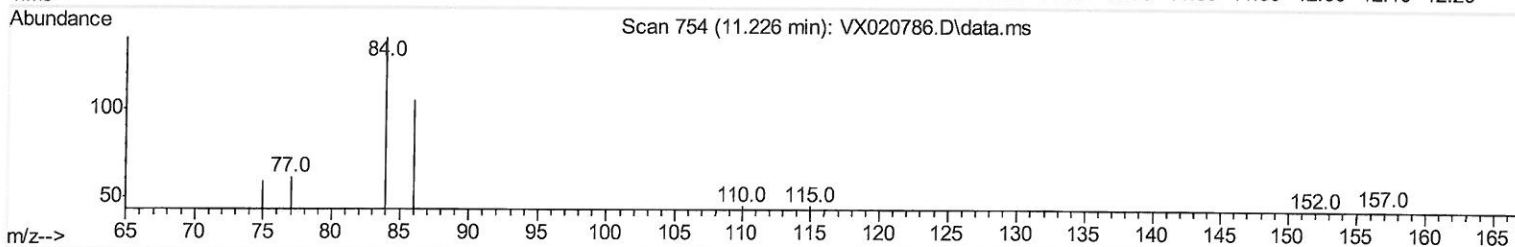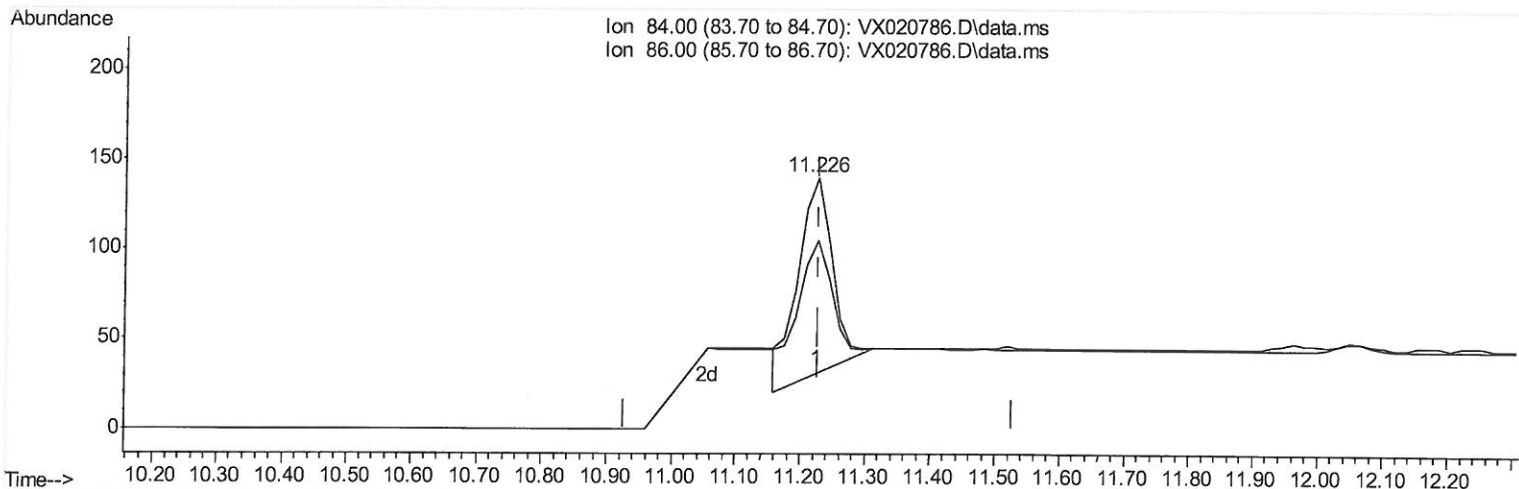

TIC: VX020786.D\data.ms

(10) 1,1,2,2-Tetrachloroethane-d2 (S)

11.226min (-0.002) 0.05 ug/L

response 410

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.10	68.54
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012821\
 Data File : VX020786.D
 Acq On : 28 Jan 2021 09:07
 Operator : JC/SP
 Sample : VSTD0.0534
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTD0.05304

Manual Integrations
 APPROVED

MMDadoda
 2/3/2021 9:42:21 AM

Quant Time: Jan 29 01:43:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
 Quant Title : TRACE VOA SOM01.0
 Qlast Update : Fri Jan 29 01:43:09 2021
 Response via : Initial Calibration

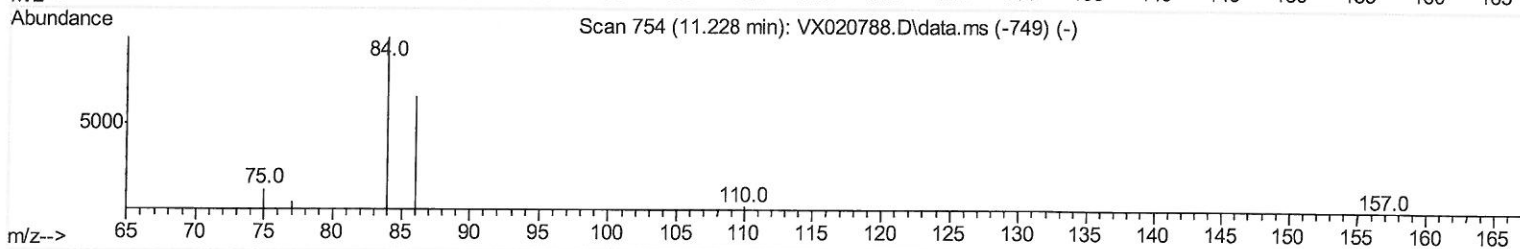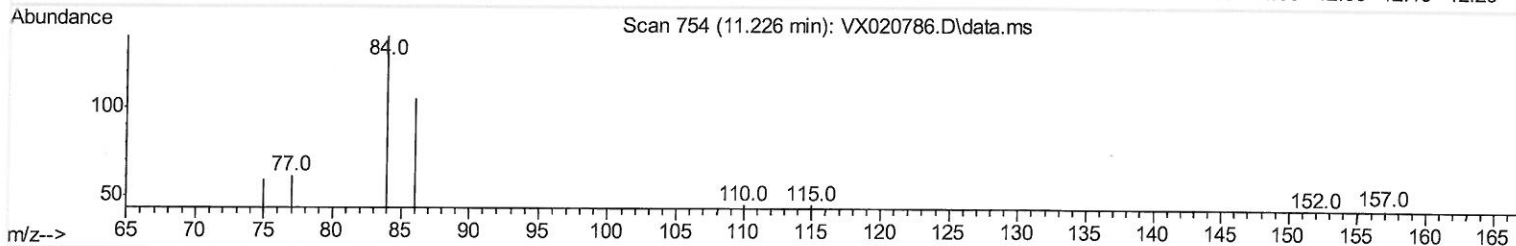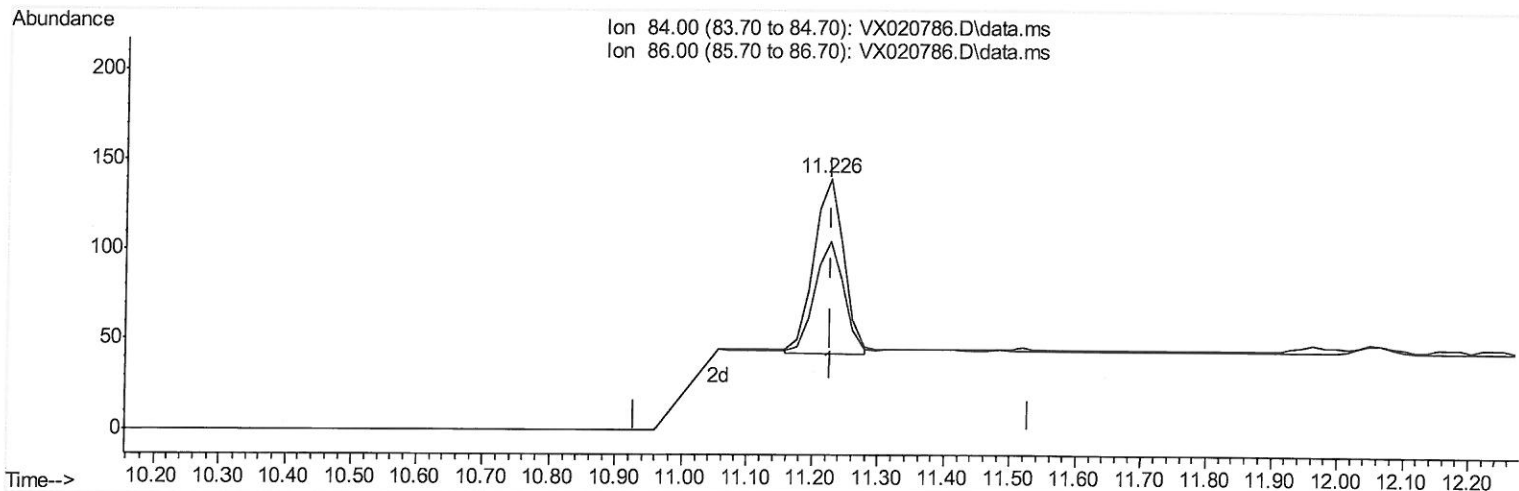

TIC: VX020786.D\data.ms

(10) 1,1,2,2-Tetrachloroethane-d2 (S)

11.226min (-0.002) 0.04 ug/L m

response 312

7 MB
 02/04/21

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.10	90.06#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VOX012821\
 Data File : VX020786.D
 Acq On : 28 Jan 2021 09:07
 Operator : JC/SP
 Sample : VSTD0.0534
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTD0.05304

Manual Integrations
 APPROVED

MMDadoda
 2/3/2021 9:42:21 AM

Quant Time: Jan 29 01:43:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 29 01:43:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.823	114	13255	0.50	ug/L	0.00
5) Chlorobenzene-d5	10.093	117	11433	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	12.066	152	5164	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.387	65	530	0.05	ug/L	0.00
4) 1,2-Dichloroethane-d4	6.013	65	772	0.06	ug/L	0.00
7) 1,2-Dichloropropane-d6	7.350	67	434	0.04	ug/L	-0.02
8) Toluene-d8	8.685	98	1513	0.05	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	11.226	84	312m	0.04	ug/L	0.00
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.387	62	558	0.05	ug/L #	82
6) Trichloroethene	7.180	95	461	0.04	ug/L	97
9) 1,2-Dibromoethane	9.644	107	263	0.04	ug/L #	93
12) 1,2,3-Trichloropropane	11.261	75	227	0.04	ug/L #	86
13) 1,2-Dibromo-3-chloropr...	12.974	75	51	0.05	ug/L	95

> MD
 02/06/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed