

Quantitation Report (QT Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012821\
 Data File : VX020787.D
 Acq On : 28 Jan 2021 09:37
 Operator : JC/SP
 Sample : VSTD0.135
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 VSTD0.1305

Quant Time: Jan 29 01:43:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 29 01:43:09 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 2/3/2021 9:42:26 AM

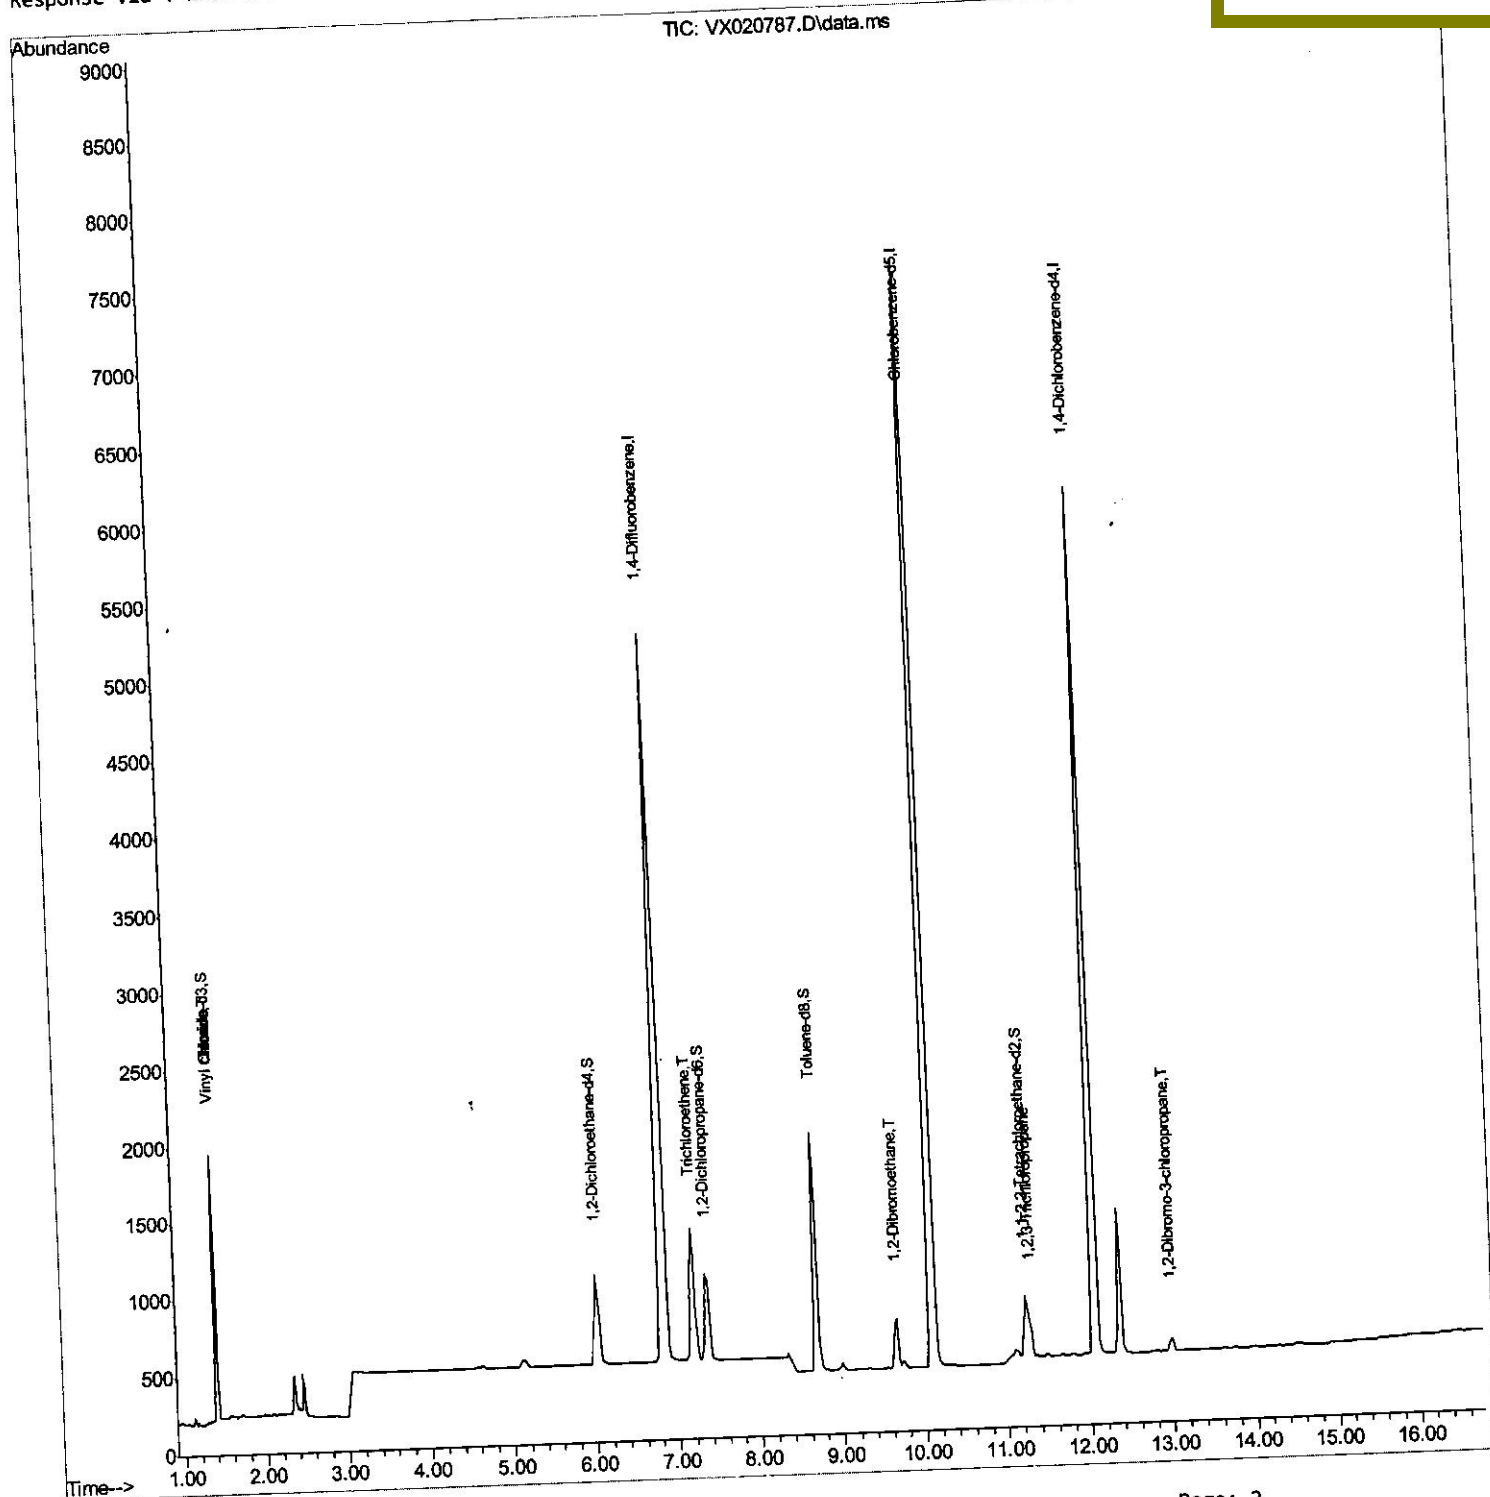

Page: 2

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012821\
 Data File : VX020787.D
 Acq On : 28 Jan 2021 09:37
 Operator : JC/SP
 Sample : VSTD0.135
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 VSTD0.1305

Quant Time: Feb 09 03:06:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Feb 04 07:04:06 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 2/3/2021 9:42:26 AM

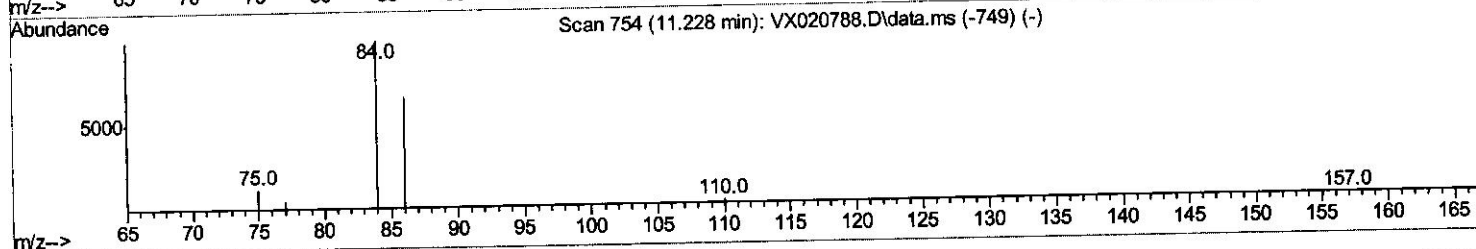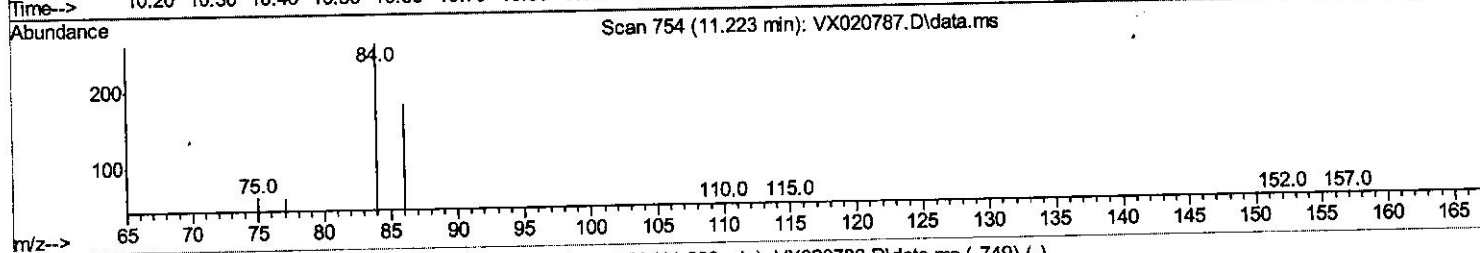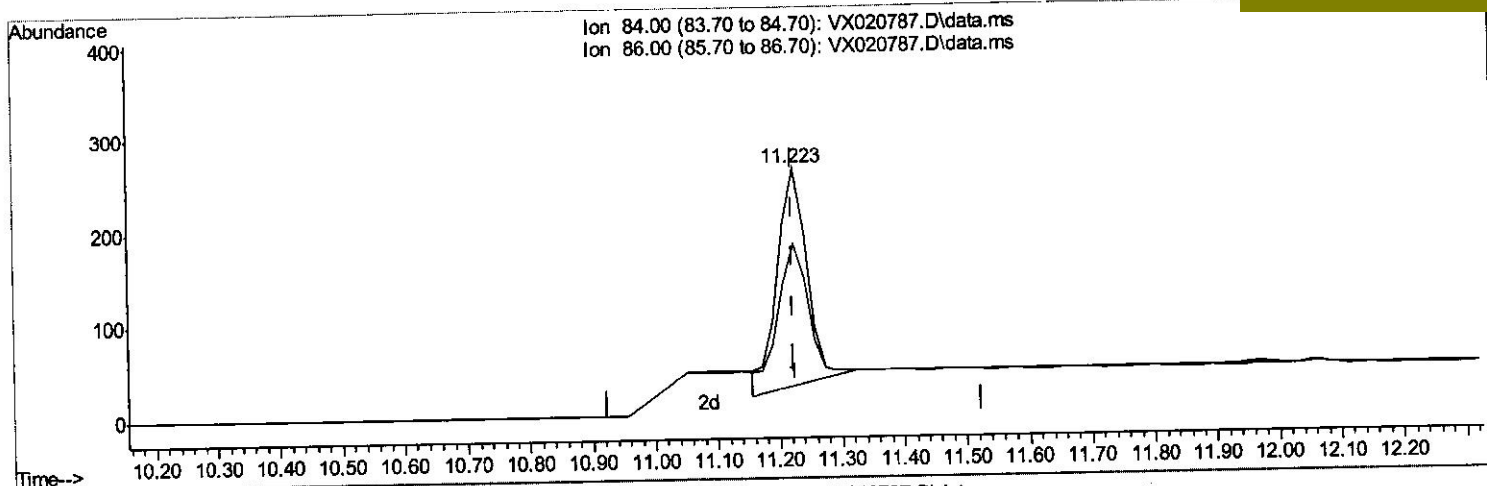

TIC: VX020787.D\data.ms

(10) 1,1,2,2-Tetrachloroethane-d2 (S)

11.223min (-0.000) 0.11 ug/L

response 784

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.10	66.96
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012821\
 Data File : VX020787.D
 Acq On : 28 Jan 2021 09:37
 Operator : JC/SP
 Sample : VSTD0.135
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 VSTD0.1305

Quant Time: Jan 29 01:43:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 29 01:43:09 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 2/3/2021 9:42:26 AM

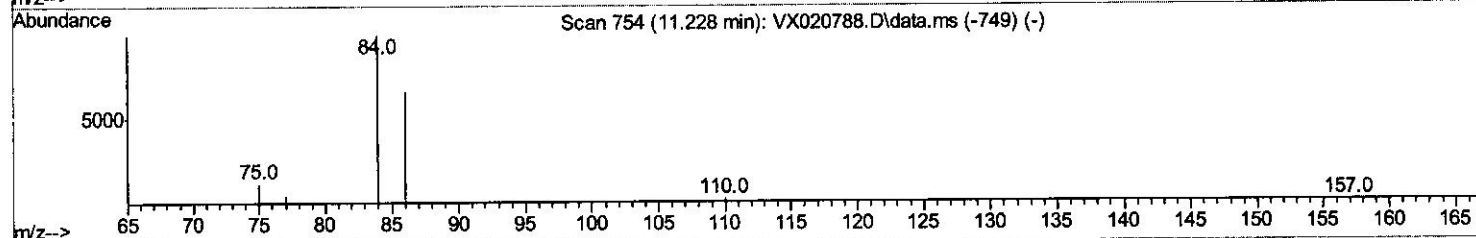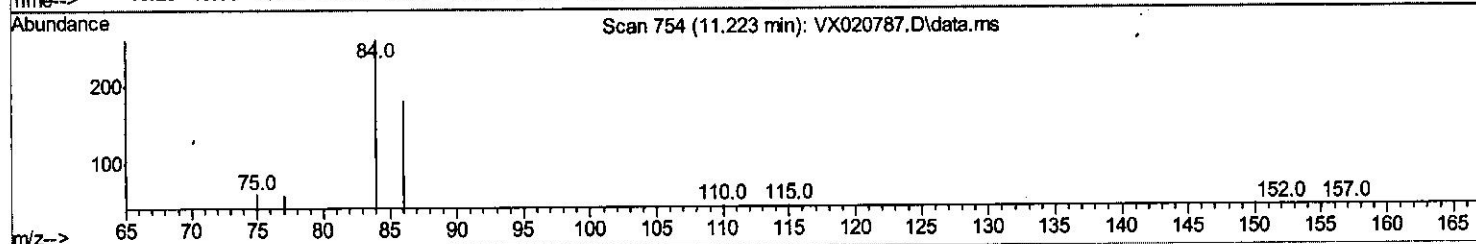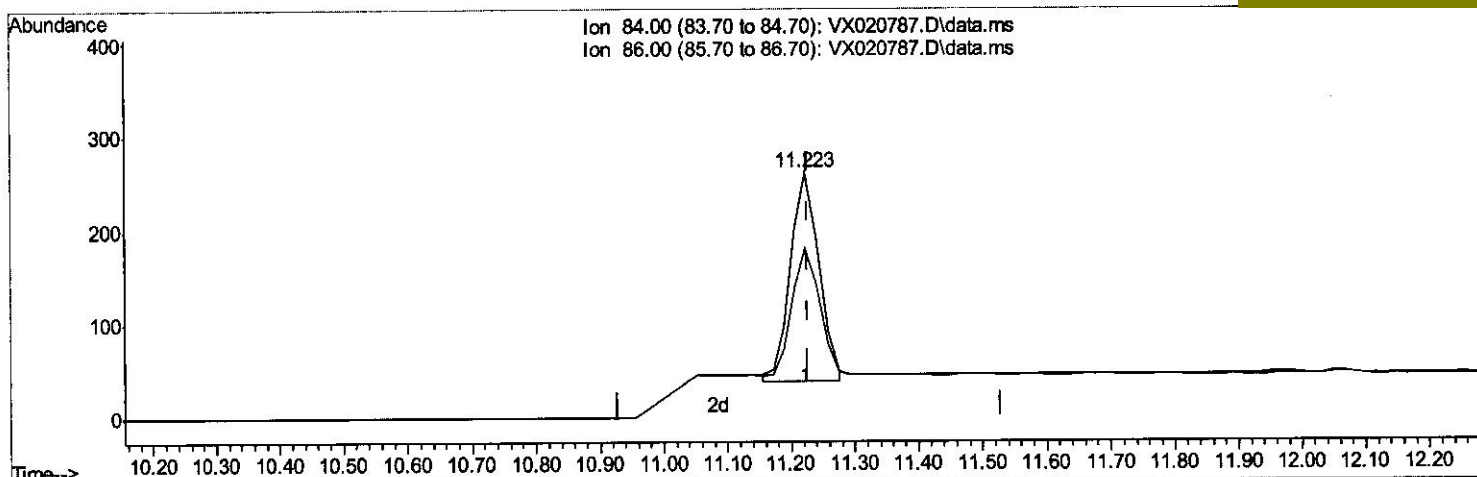

TIC: VX020787.D\data.ms

(10) 1,1,2,2-Tetrachloroethane-d2 (S)

11.223min (-0.005) 0.08 ug/L m

response 699

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.10	75.11
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012821\
 Data File : VX020787.D
 Acq On : 28 Jan 2021 09:37
 Operator : JC/SP
 Sample : VSTD0.135
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampled :
 VSTD0.1305

Quant Time: Jan 29 01:43:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jan 29 01:43:09 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 2/3/2021 9:42:26 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.823	114	12989	0.50	ug/L	0.00
5) Chlorobenzene-d5	10.089	117	11278	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	12.063	152	5279	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.387	65	1021	0.09	ug/L	0.00
4) 1,2-Dichloroethane-d4	6.013	65	1172	0.10	ug/L	0.00
7) 1,2-Dichloropropane-d6	7.349	67	927	0.09	ug/L	-0.02
8) Toluene-d8	8.682	98	2661	0.09	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	11.223	84	699m	0.08	ug/L	0.00
Target Compounds						
3) Vinyl chloride	1.387	62	998	0.09	ug/L	89
6) Trichloroethene	7.180	95	834	0.08	ug/L	96
9) 1,2-Dibromoethane	9.656	107	490	0.08	ug/L #	90
12) 1,2,3-Trichloropropane	11.274	75	443	0.08	ug/L #	93
13) 1,2-Dibromo-3-chloropr...	12.971	75	92	0.09	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

m n
 2/3/21