
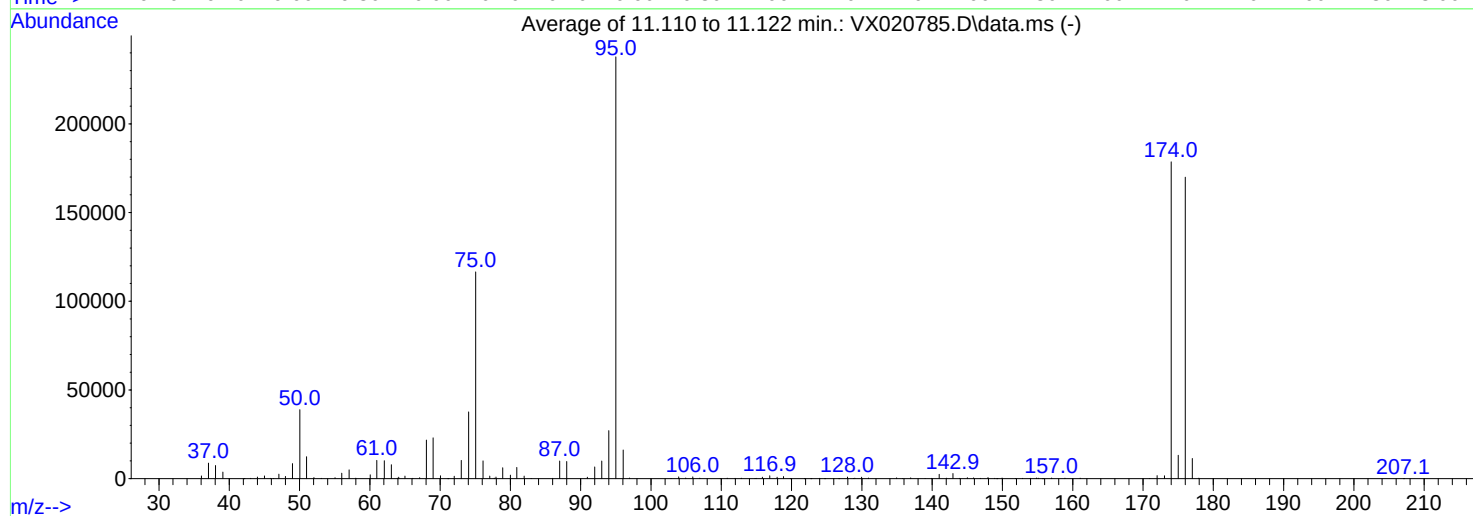


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012821\
 Data File : VX020785.D
 Acq On : 28 Jan 2021 08:38
 Operator : JC/SP
 Sample : BFB05
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB050

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jan 30 02:01:56 2021

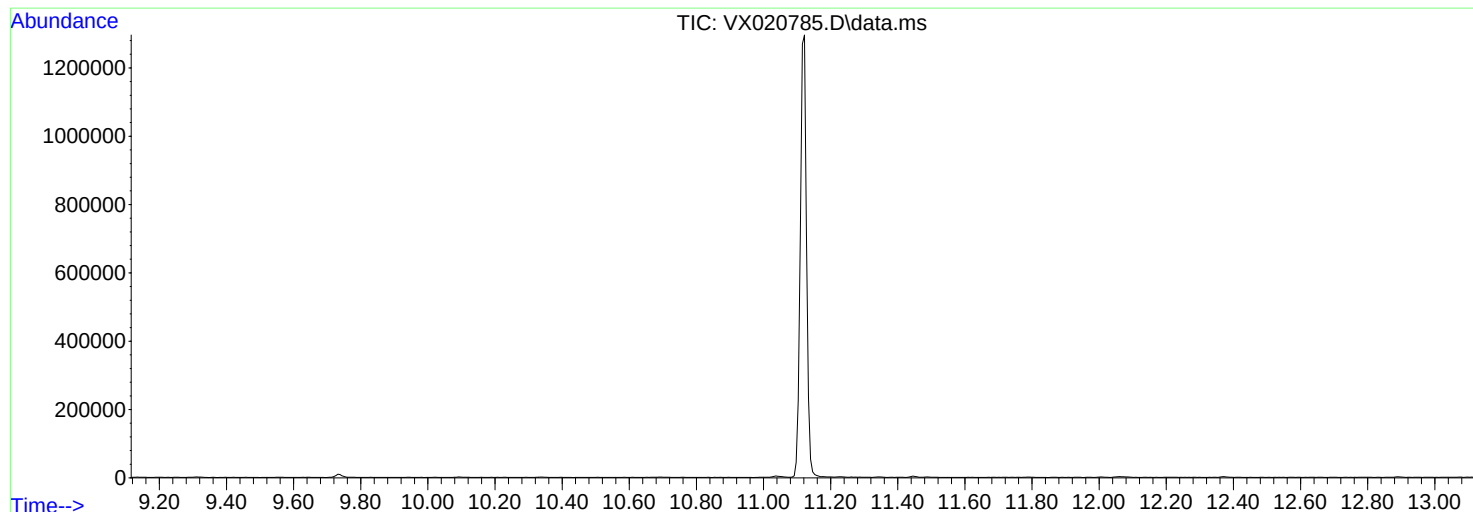

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	38893	PASS
75	95	30	80	49.0	116557	PASS
95	95	100	100	100.0	237781	PASS
96	95	5	9	6.8	16104	PASS
173	174	0.00	2	0.9	1592	PASS
174	95	50	120	75.1	178587	PASS
175	174	5	9	7.4	13216	PASS
176	174	95	101	95.1	169915	PASS
177	176	5	9	6.7	11407	PASS

m/z	Abundance
36.00	1232.0
37.00	7069.0
38.00	5708.0
39.10	2907.0
40.00	731.0
40.90	68.0
42.20	67.0
43.10	141.0
44.10	1694.0
45.00	1287.0
45.90	172.0
47.00	1745.0
48.00	946.0
49.00	6688.0
50.10	29096.0
51.00	9035.0
52.10	451.0
53.00	152.0
55.00	401.0
56.00	2164.0
57.00	3741.0
58.00	137.0
60.00	1764.0
61.00	7413.0
62.10	7418.0
63.00	5711.0
63.90	762.0
65.00	1267.0
66.20	127.0
67.10	387.0
68.10	15805.0
69.00	16043.0
70.00	1127.0
71.10	109.0
72.00	892.0
73.00	7459.0
74.10	26800.0
75.00	81296.0
76.10	7235.0
77.00	922.0
77.70	698.0
78.90	4122.0
80.00	1413.0
80.90	4394.0
81.90	947.0
83.00	69.0
86.00	210.0
87.00	6633.0
88.00	6653.0
90.90	472.0
92.00	4443.0
93.00	6676.0
94.00	17248.0
95.00	160576.0
96.00	10848.0
96.90	281.0
104.00	696.0
105.00	222.0
105.90	586.0
107.00	162.0
111.00	110.0
112.00	146.0
112.90	164.0
114.80	196.0
115.80	419.0
116.90	1204.0
118.00	490.0
118.80	608.0
124.00	133.0
127.90	667.0
128.80	172.0
130.00	513.0
131.00	157.0
134.90	278.0
135.80	69.0
137.10	245.0
139.00	93.0
139.90	122.0
141.00	1494.0
142.00	231.0
143.00	1919.0
143.90	161.0
145.10	328.0
145.90	244.0
146.90	105.0
148.00	411.0
149.20	60.0
150.00	202.0
152.80	94.0
153.90	80.0
154.80	279.0
155.10	221.0

Instrument :
MSVOA_X
ClientSampleId :
BFB050

157.00	264.0
159.00	160.0
161.00	155.0
171.10	130.0
172.00	1323.0
173.00	947.0
174.00	100240.0
175.00	6947.0
176.00	95728.0
177.00	6835.0
178.00	174.0

Instrument :
MSVOA_X
ClientSampleId :
BFB050

m/z	Abundance
36.00	1802.0
37.10	10570.0
38.00	9363.0
39.10	4457.0
40.00	686.0
40.90	75.0
42.00	52.0
43.00	155.0
44.00	1816.0
45.10	2119.0
45.90	271.0
46.30	316.0
47.10	3234.0
48.00	1466.0
49.00	9993.0
50.00	46584.0
51.00	14523.0
52.10	766.0
53.10	143.0
55.00	581.0
56.00	3959.0
57.10	6313.0
58.00	305.0
60.10	2152.0
61.00	12418.0
62.10	12122.0
63.00	9993.0
64.10	1419.0
65.00	1627.0
66.10	193.0
67.10	657.0
68.00	26200.0
69.00	28152.0
70.10	1880.0
71.10	136.0
72.00	1596.0
73.00	12001.0
74.10	45216.0
75.10	138176.0
76.10	11883.0
77.10	1831.0
77.90	1290.0
78.90	7550.0
80.00	2469.0
80.90	7206.0
82.00	1786.0
82.90	187.0
87.00	12176.0
88.00	11457.0
91.00	869.0
92.00	8062.0
93.00	11858.0
94.00	32304.0
95.00	279616.0
96.10	19592.0
97.00	567.0
102.80	147.0
103.90	946.0
105.00	499.0
105.90	1319.0
107.00	313.0
109.90	138.0
110.90	378.0
111.90	169.0
112.70	155.0
113.00	184.0
115.00	312.0
115.90	958.0
116.90	1926.0
117.90	969.0
118.90	1488.0
119.80	77.0
122.90	51.0
123.90	103.0
124.70	96.0
126.00	140.0
126.70	101.0
127.90	887.0
129.00	478.0
130.00	1010.0
131.00	363.0
135.00	532.0
135.80	78.0
136.90	499.0
138.90	121.0
139.90	237.0
141.00	2820.0
142.00	266.0
142.90	3759.0
143.90	304.0
145.00	834.0
145.90	544.0

Instrument :
MSVOA_X
ClientSampleId :
BFB050

146.80	251.0
148.00	734.0
148.90	210.0
149.90	356.0
151.80	90.0
152.90	200.0
153.90	166.0
154.90	686.0
155.70	129.0
157.10	488.0
158.80	230.0
161.00	392.0
170.90	140.0
172.00	2002.0
173.10	1696.0
174.00	193920.0
175.00	15748.0
176.00	191040.0
177.00	13523.0
177.90	320.0
207.00	141.0

Instrument :
MSVOA_X
ClientSampleId :
BFB050

m/z	Abundance
36.10	1703.0
37.00	8658.0
38.10	7110.0
39.10	3628.0
39.90	642.0
43.00	175.0
44.00	1929.0
45.00	1499.0
45.90	130.0
47.00	2621.0
48.00	1274.0
49.00	8685.0
50.00	41000.0
51.00	13561.0
52.00	607.0
53.20	164.0
55.10	727.0
56.00	3037.0
57.00	5902.0
58.00	320.0
60.00	2489.0
61.00	11098.0
62.00	10870.0
63.10	7928.0
64.10	993.0
65.00	1339.0
66.00	145.0
67.10	599.0
68.00	23104.0
69.00	24832.0
70.00	1959.0
71.10	52.0
72.00	1449.0
73.00	11469.0
74.00	40912.0
75.00	130200.0
76.10	10867.0
77.10	1690.0
78.00	1448.0
78.90	6806.0
80.00	2035.0
80.90	7356.0
82.00	1591.0
83.00	151.0
86.00	319.0
87.00	11043.0
88.00	10829.0
90.90	1014.0
92.00	7398.0
93.00	11294.0
94.00	31656.0
95.00	273152.0
96.10	17872.0
97.00	363.0
102.90	148.0
104.00	1301.0
104.90	273.0
106.00	1234.0
106.90	246.0
109.80	137.0
110.80	235.0
111.90	220.0
112.80	258.0
114.90	286.0
115.90	1077.0
116.90	1849.0
117.90	1123.0
118.90	1514.0
121.80	51.0
122.70	90.0
124.00	268.0
126.00	95.0
128.00	1089.0
129.00	417.0
129.90	905.0
130.90	485.0
134.90	665.0
135.80	67.0
137.00	537.0
139.10	96.0
139.90	246.0
141.00	2894.0
142.10	383.0
142.90	3062.0
144.00	127.0
144.90	474.0
145.90	522.0
146.90	261.0
147.90	695.0
148.90	283.0
149.90	414.0
151.90	99.0

Instrument :
MSVOA_X
ClientSampleId :
BFB050

152.80	195.0
154.00	226.0
155.10	652.0
156.90	382.0
158.90	557.0
161.10	358.0
170.90	160.0
172.00	1807.0
173.00	2134.0
174.00	241600.0
175.00	16952.0
176.00	222976.0
177.00	13864.0
178.00	412.0
207.00	171.0

Instrument :
MSVOA_X
ClientSampleId :
BFB050

m/z	Abundance
40.00	747.0
41.10	160.0
44.00	916.0
44.90	115.0
57.10	312.0
71.20	91.0
73.00	57.0
87.10	67.0
207.20	73.0

Instrument :
MSVOA_X
ClientSampleId :
BFB050