

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012822\
 Data File : VX026651.D
 Acq On : 28 Jan 2022 15:12
 Operator : JC/MD
 Sample : N1323-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Jan 29 02:19:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	129683	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	221231	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	189117	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	78558	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	86083	47.518	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.040%
35) Dibromofluoromethane	5.391	113	70073	49.049	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.100%
50) Toluene-d8	8.653	98	254243	49.385	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.760%
62) 4-Bromofluorobenzene	11.079	95	87916	48.072	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012822\
Data File : VX026651.D
Acq On : 28 Jan 2022 15:12
Operator : JC/MD
Sample : N1323-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Jan 29 02:19:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration




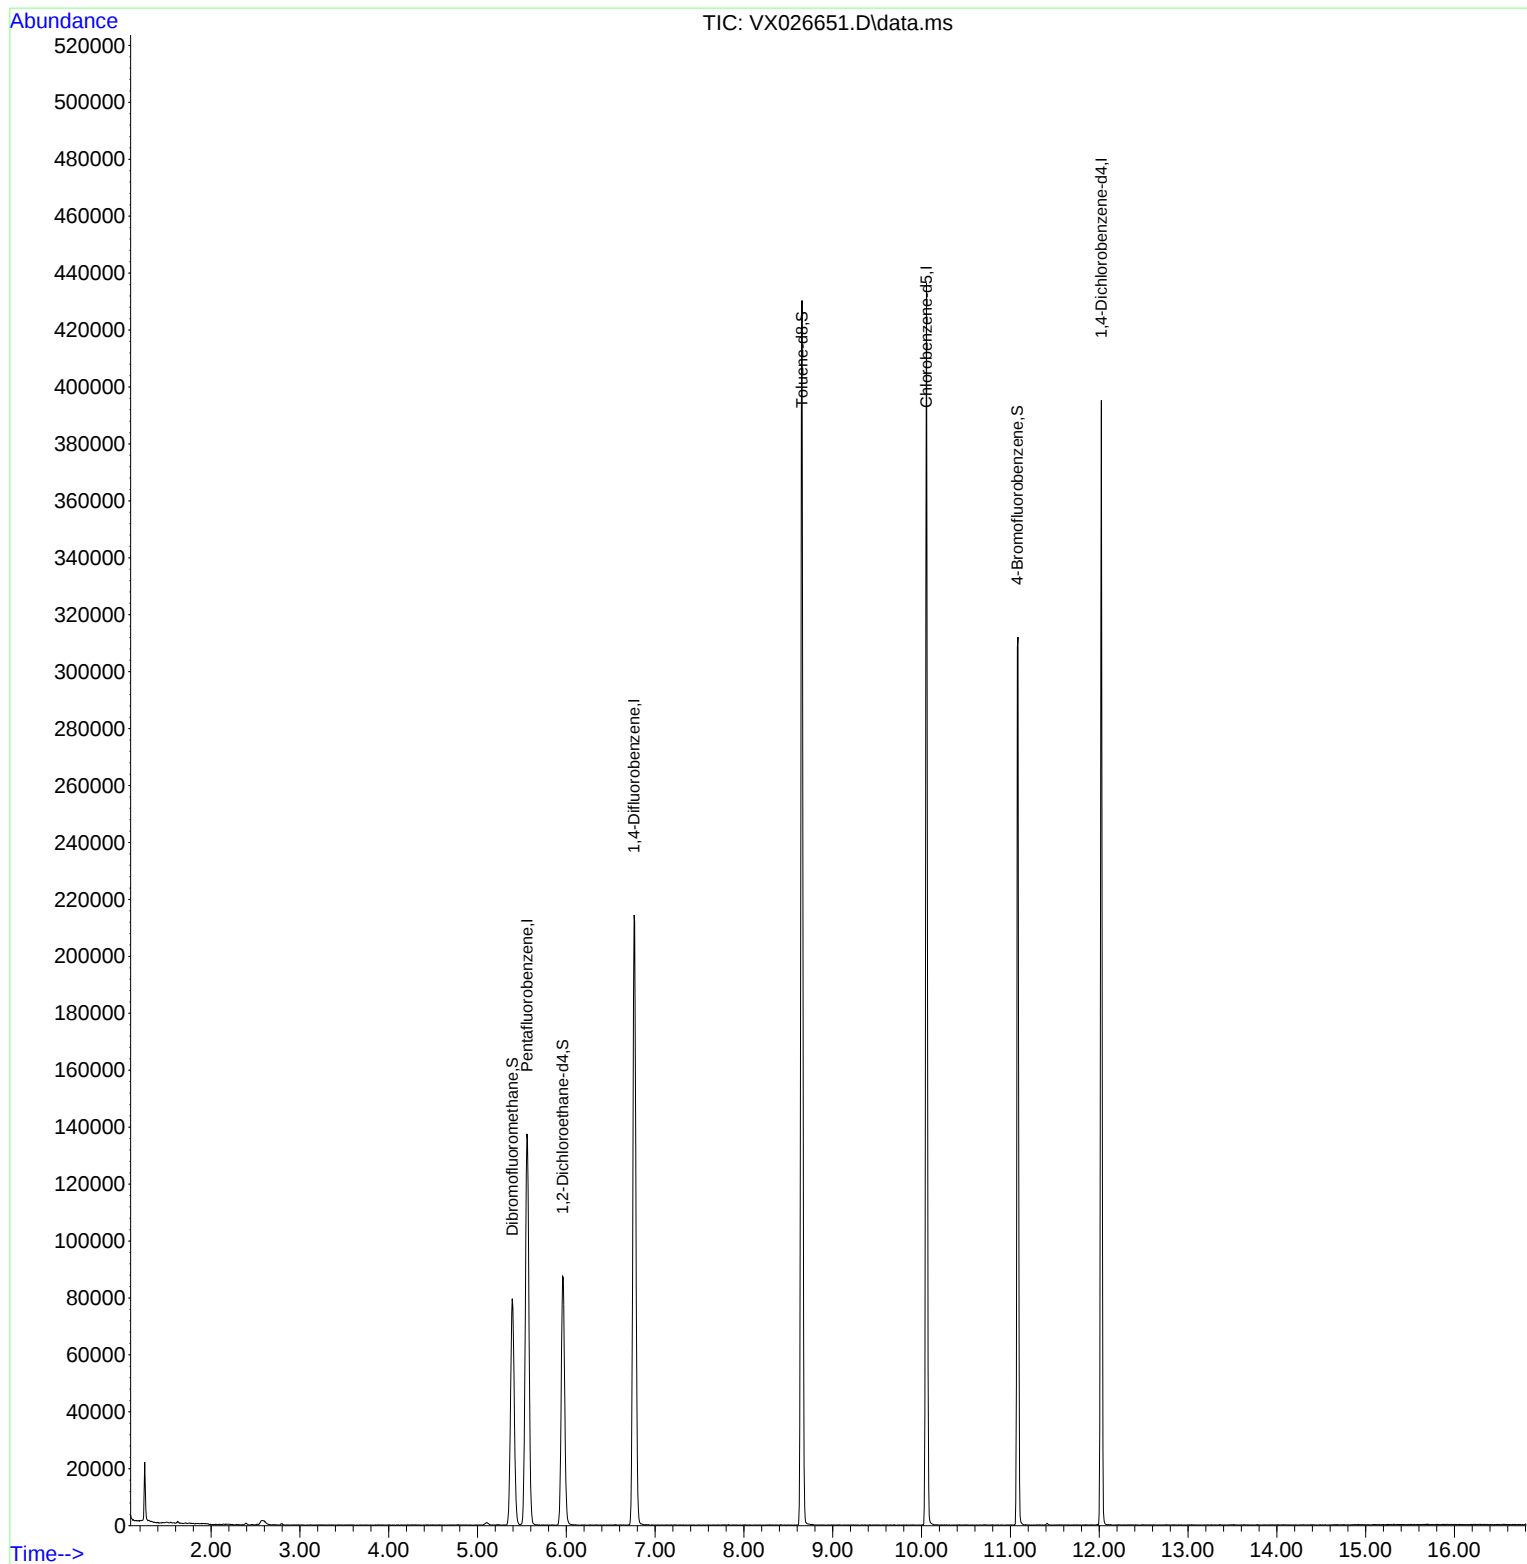


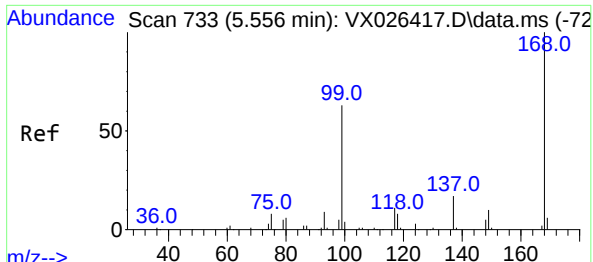

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX026651.D
Acq: 28 Jan 2022 15:12




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 129683
Ion Ratio Lower Upper
168 100
99 61.1 50.3 75.5

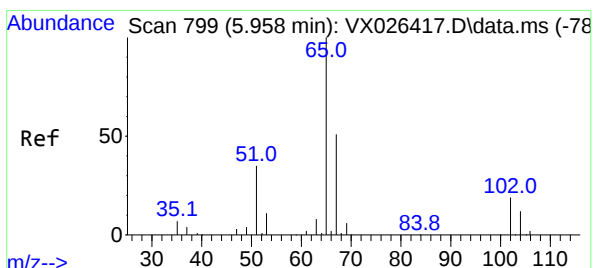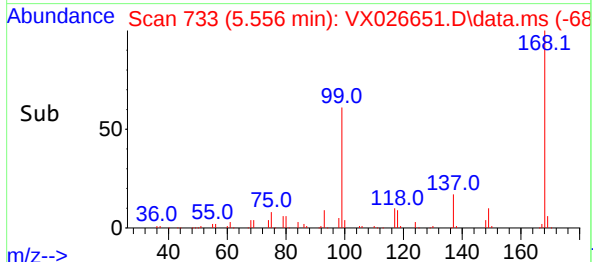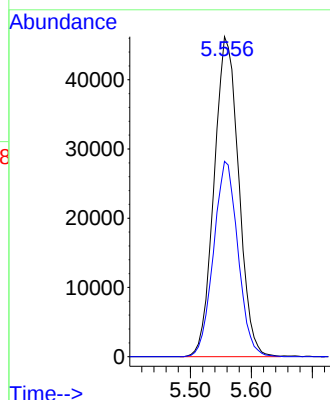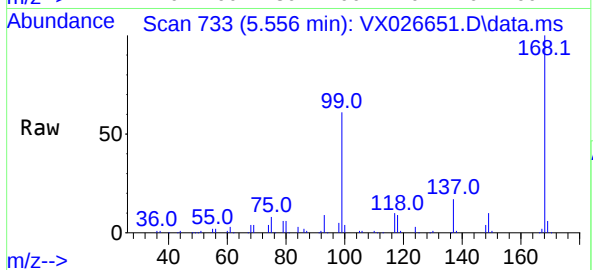

#33
1,2-Dichloroethane-d4
Concen: 47.518 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX026651.D
Acq: 28 Jan 2022 15:12

Tgt Ion: 65 Resp: 86083
Ion Ratio Lower Upper
65 100
67 52.1 0.0 100.8


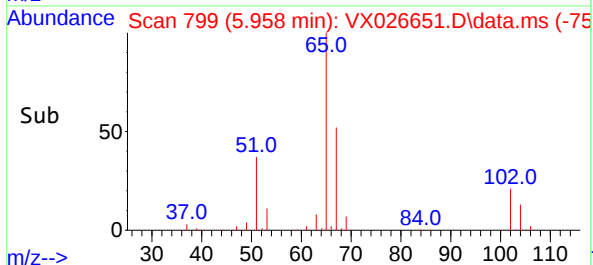
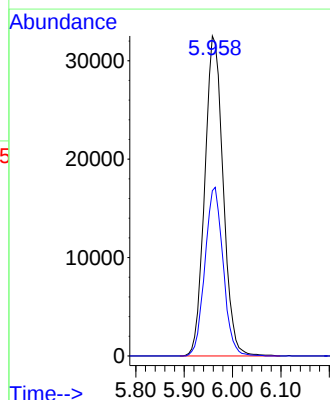
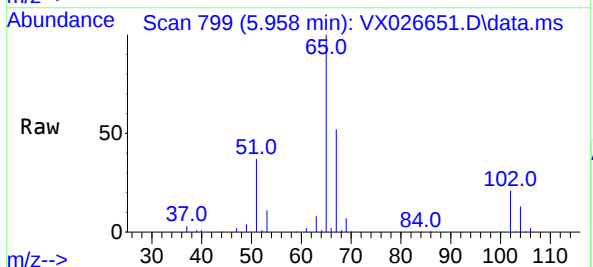


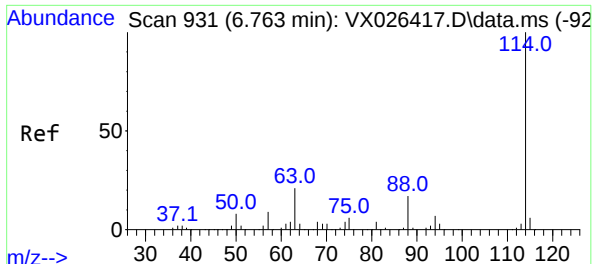

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX026651.D
Acq: 28 Jan 2022 15:12




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:114 Resp: 221231
Ion Ratio Lower Upper
114 100
63 20.9 0.0 42.8
88 15.8 0.0 33.0

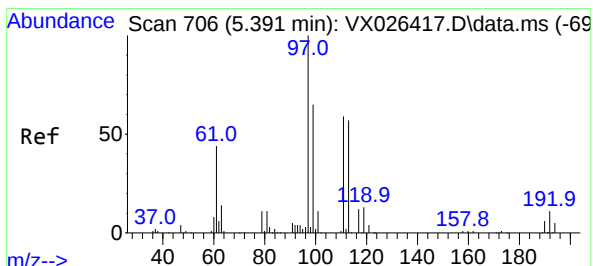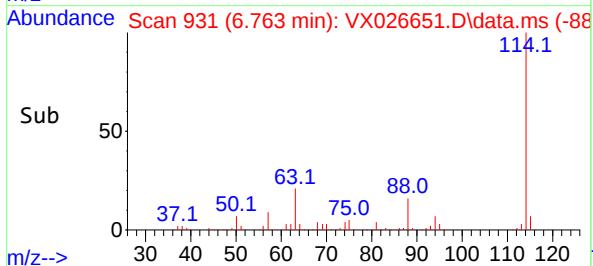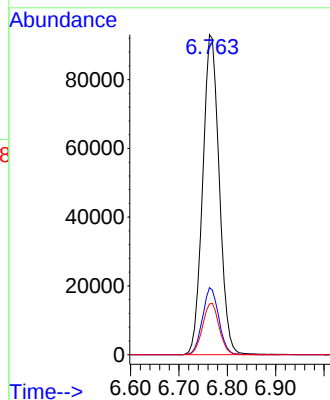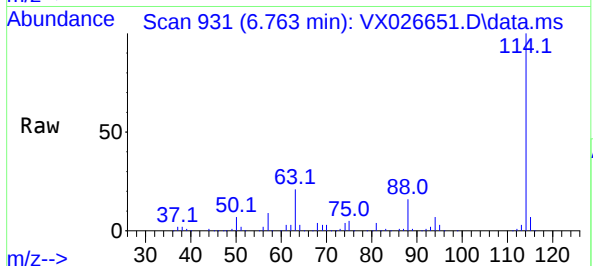

#35
Dibromofluoromethane
Concen: 49.049 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX026651.D
Acq: 28 Jan 2022 15:12

Tgt Ion:113 Resp: 70073
Ion Ratio Lower Upper
113 100
111 102.9 81.2 121.8
192 19.3 15.0 22.4

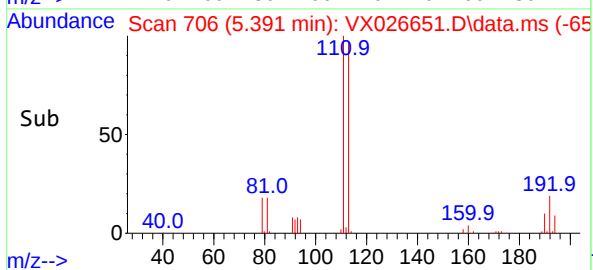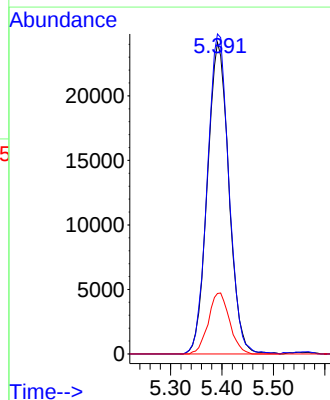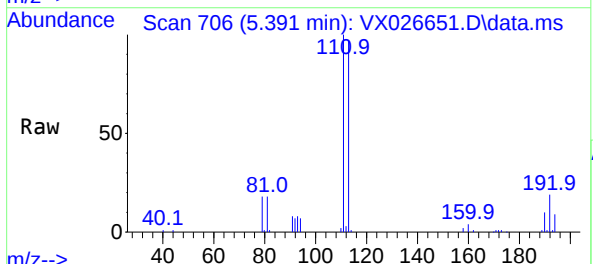

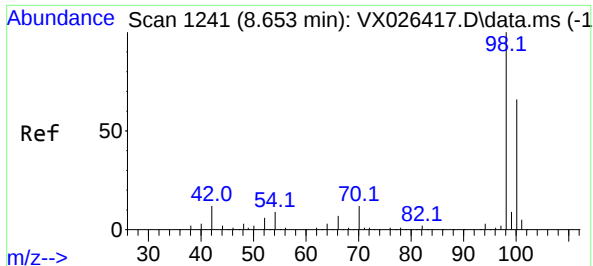

#50

Toluene-d8

Concen: 49.385 ug/l

RT: 8.653 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX026651.D

Acq: 28 Jan 2022 15:12

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-SOIL-REF-6

Tgt Ion: 98 Resp: 254243

Ion Ratio Lower Upper

98 100

100 66.1 53.2 79.8

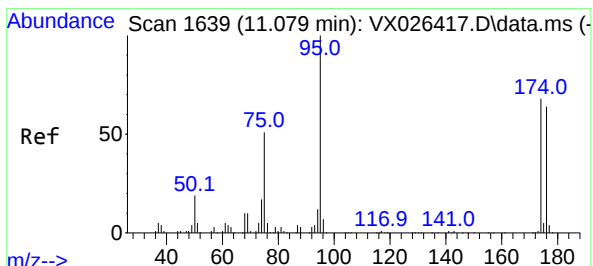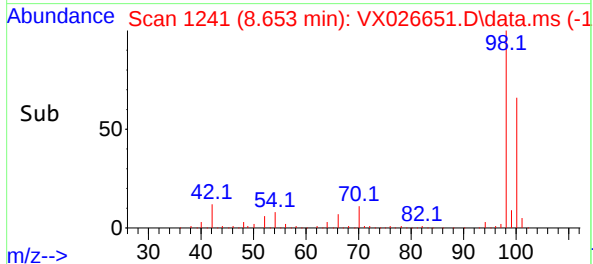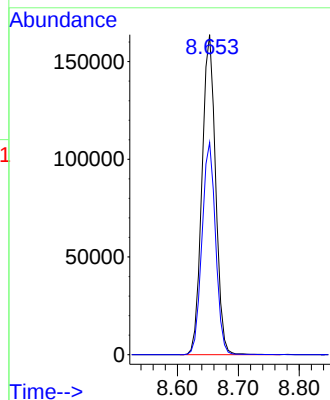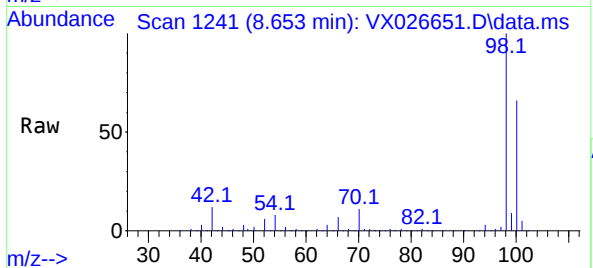

#62

4-Bromofluorobenzene

Concen: 48.072 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX026651.D

Acq: 28 Jan 2022 15:12




Tgt Ion: 95 Resp: 87916


Ion Ratio Lower Upper

95 100

174 74.2 0.0 148.6

176 71.9 0.0 141.4


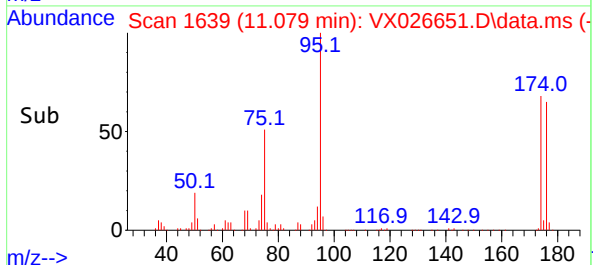
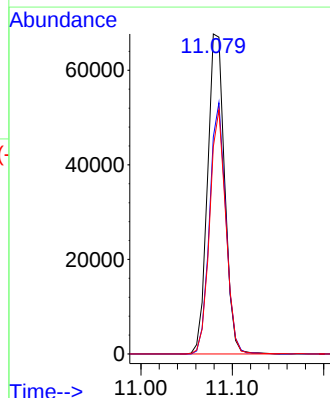
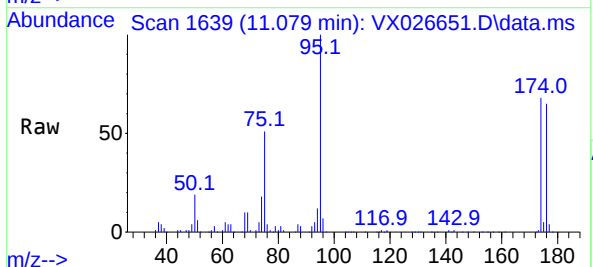


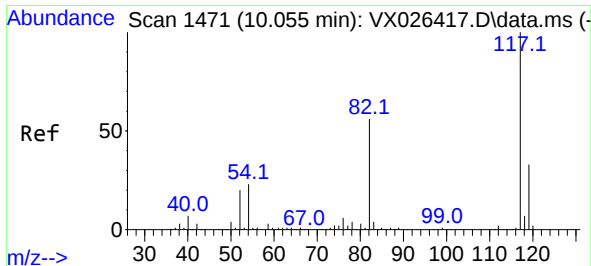

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX026651.D
Acq: 28 Jan 2022 15:12

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 189117
Ion Ratio Lower Upper
117 100
82 55.9 45.2 67.8
119 32.0 26.2 39.2

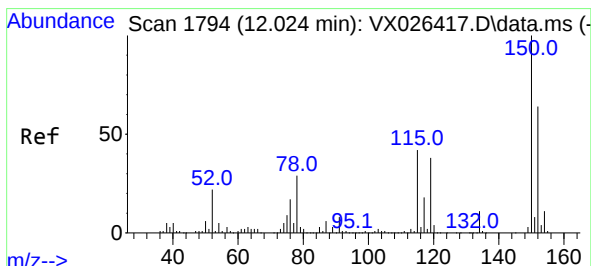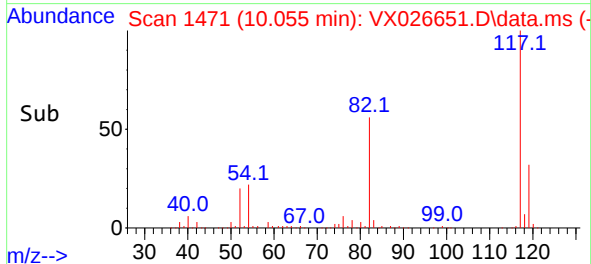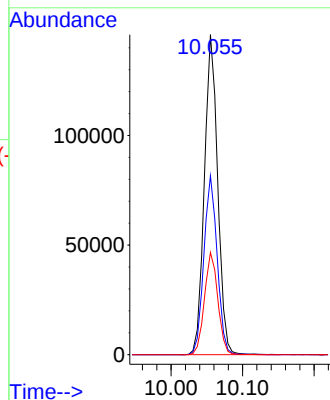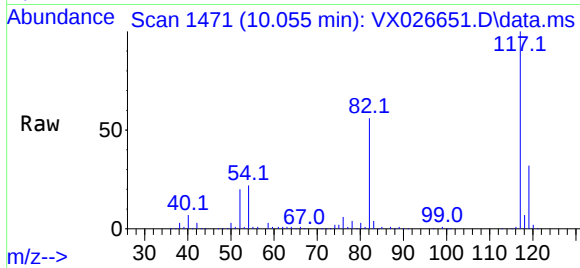

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX026651.D
Acq: 28 Jan 2022 15:12

Tgt Ion:152 Resp: 78558
Ion Ratio Lower Upper
152 100
115 60.2 44.2 132.6
150 156.1 0.0 348.2

