

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012822\
 Data File : VX026656.D
 Acq On : 28 Jan 2022 17:08
 Operator : JC/MD
 Sample : N1297-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-7M

Quant Time: Jan 29 02:19:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 11 14:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	120559	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	205306	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	177730	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	73044	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	80428	47.757	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	95.520%		
35) Dibromofluoromethane	5.391	113	65203	49.180	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.360%		
50) Toluene-d8	8.653	98	239855	50.204	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	100.400%		
62) 4-Bromofluorobenzene	11.085	95	81769	48.179	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	96.360%		
Target Compounds						
16) Acetone	2.386	43	1811	2.109	ug/l	99
30) Chloroform	5.099	83	1454	0.551	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012822\
Data File : VX026656.D
Acq On : 28 Jan 2022 17:08
Operator : JC/MD
Sample : N1297-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-7M


Quant Time: Jan 29 02:19:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Quant Title : SW846 8260
QLast Update : Tue Jan 11 14:45:13 2022
Response via : Initial Calibration

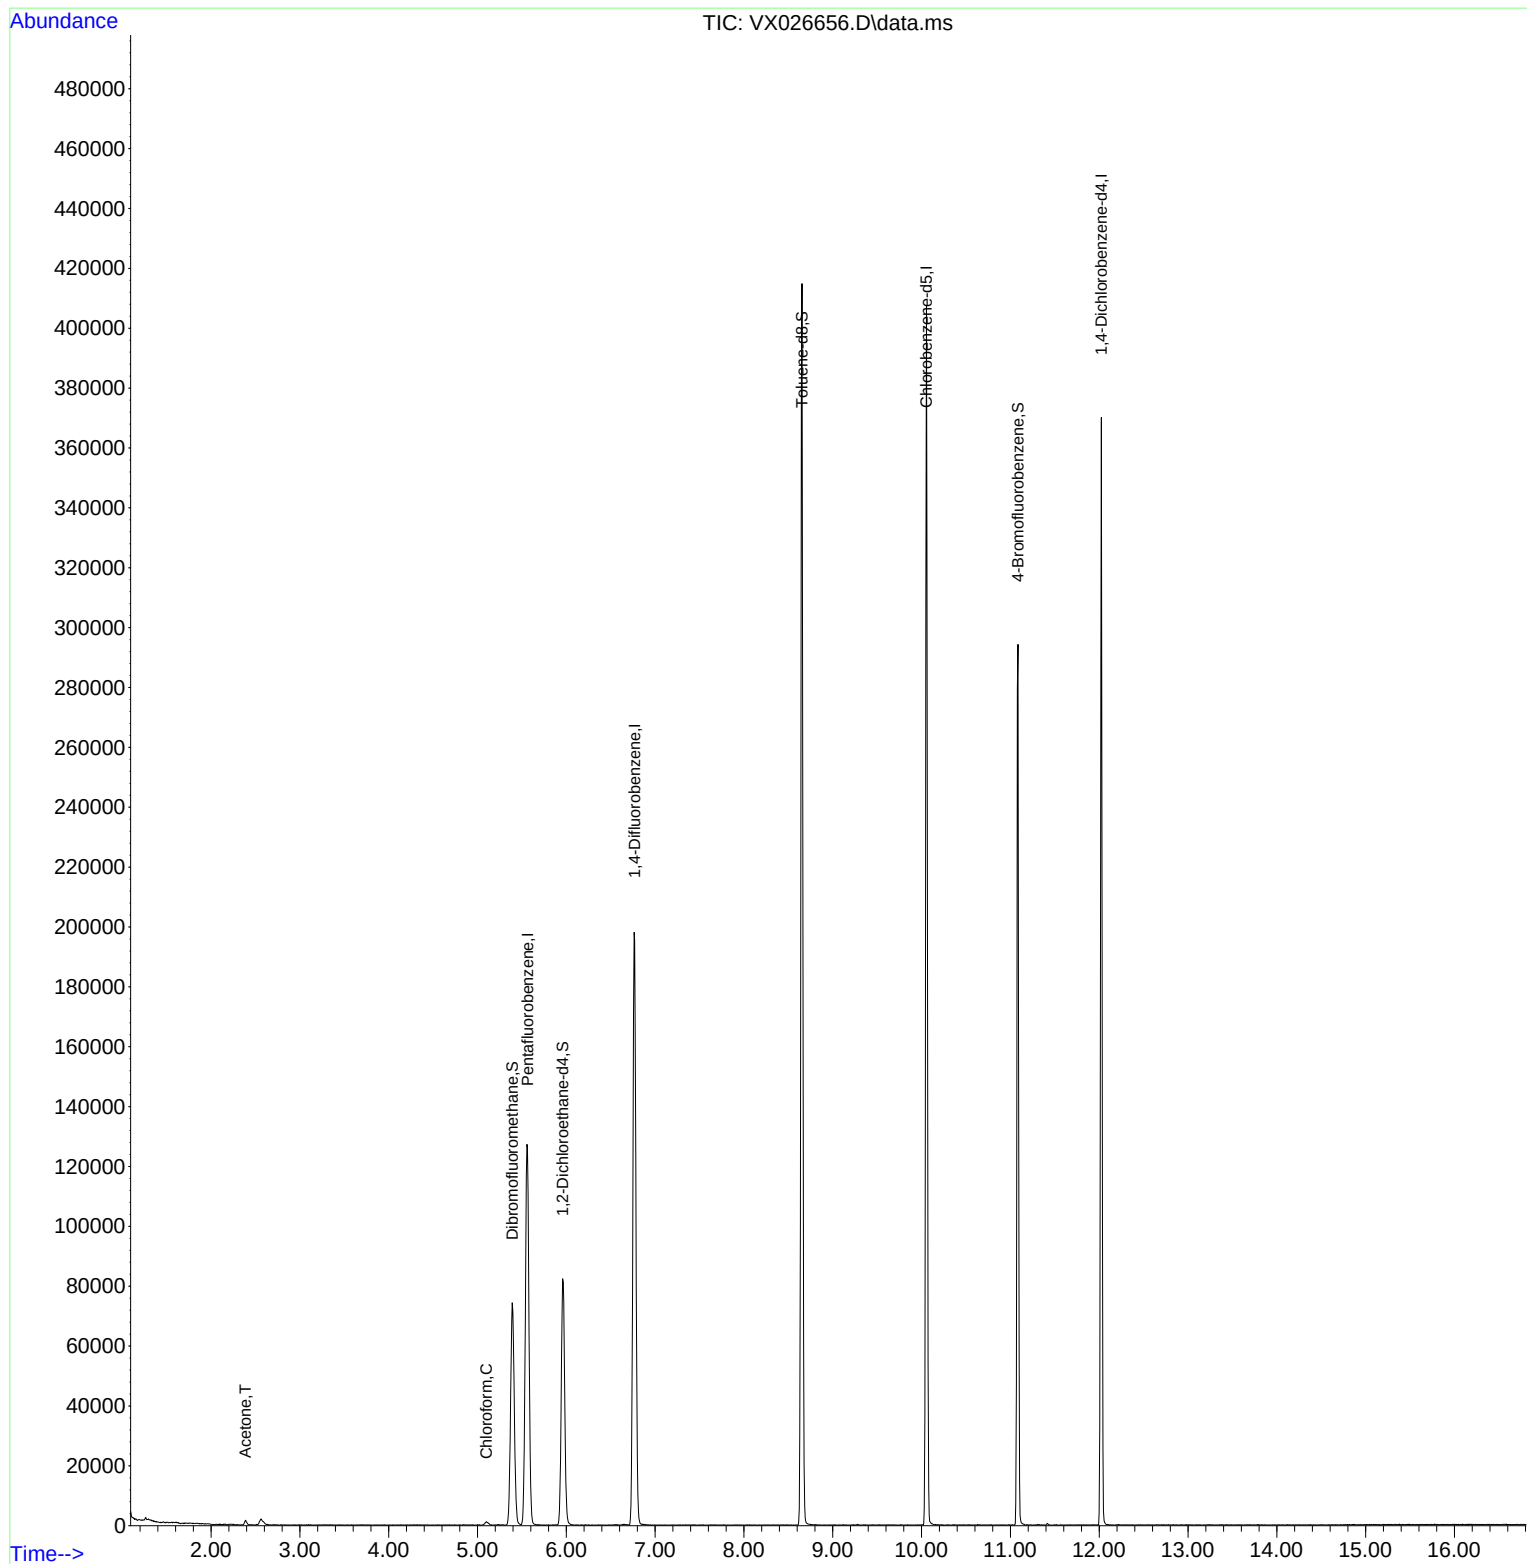



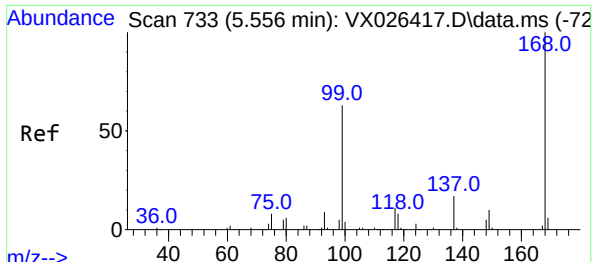


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX026656.D
Acq: 28 Jan 2022 17:08

Instrument :
MSVOA_X
ClientSampleId :
MW-7M



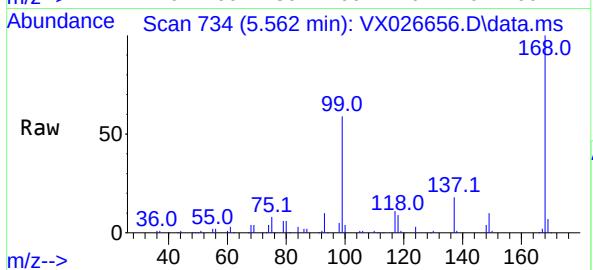



Tgt Ion:168 Resp: 120559
Ion Ratio Lower Upper
168 100
99 58.6 50.3 75.5

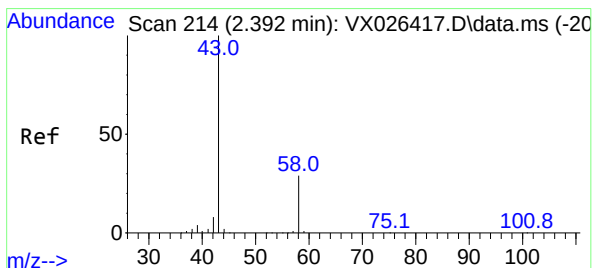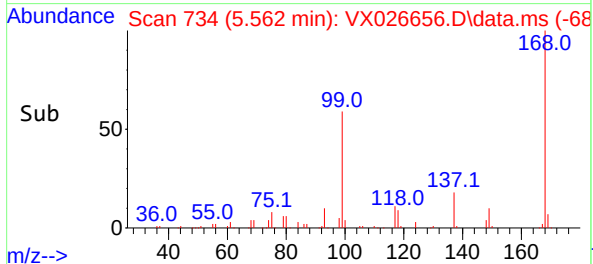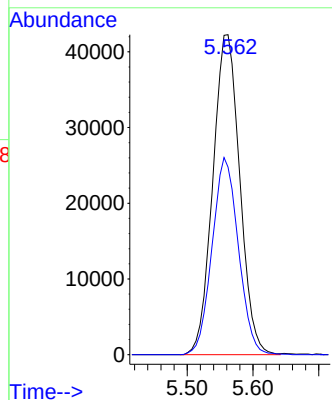

#16
Acetone
Concen: 2.109 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX026656.D
Acq: 28 Jan 2022 17:08

Tgt Ion: 43 Resp: 1811
Ion Ratio Lower Upper
43 100
58 29.2 23.0 34.6


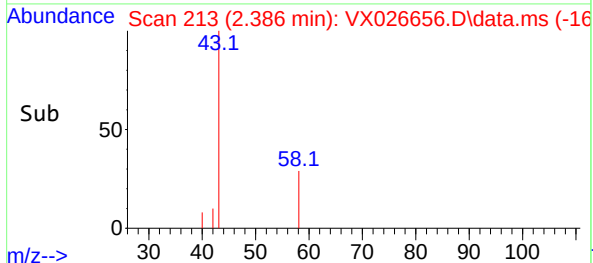
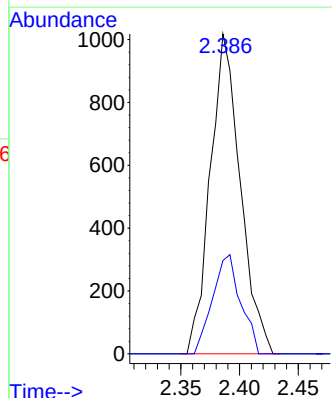
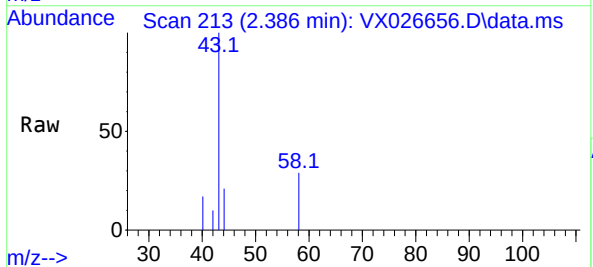


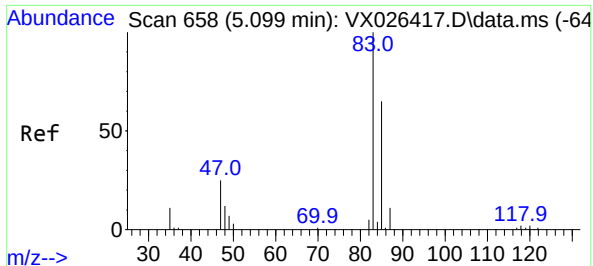

#30
Chloroform
Concen: 0.551 ug/l
RT: 5.099 min Scan# 610
Delta R.T. 0.000 min
Lab File: VX026656.D
Acq: 28 Jan 2022 17:08




Instrument :
MSVOA_X
ClientSampleId :
MW-7M


Tgt Ion: 83 Resp: 1454
Ion Ratio Lower Upper
83 100
85 57.0 51.6 77.4

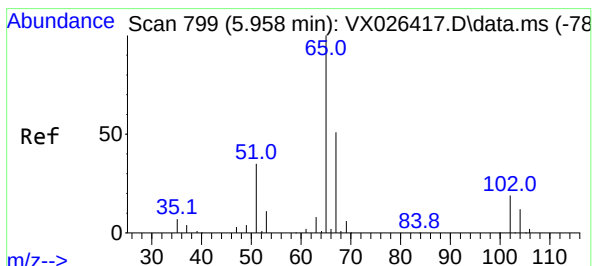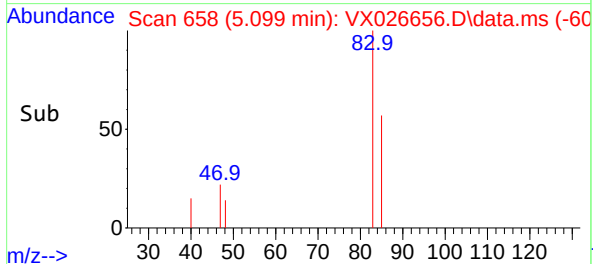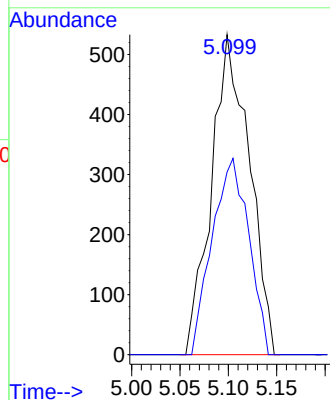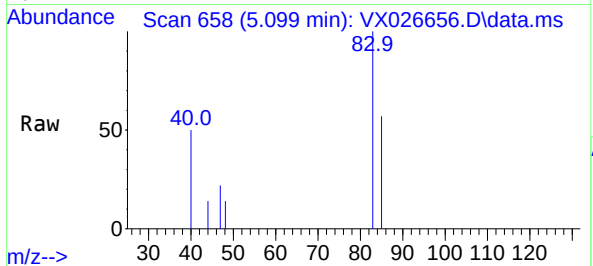

#33
1,2-Dichloroethane-d4
Concen: 47.757 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX026656.D
Acq: 28 Jan 2022 17:08

Tgt Ion: 65 Resp: 80428
Ion Ratio Lower Upper
65 100
67 51.9 0.0 100.8


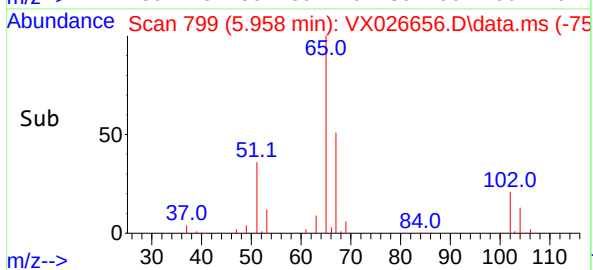
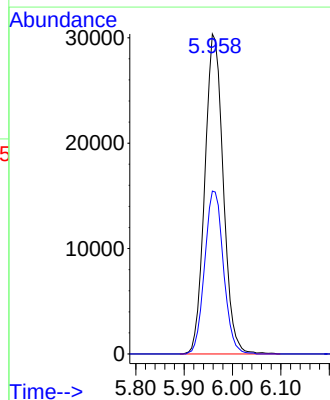
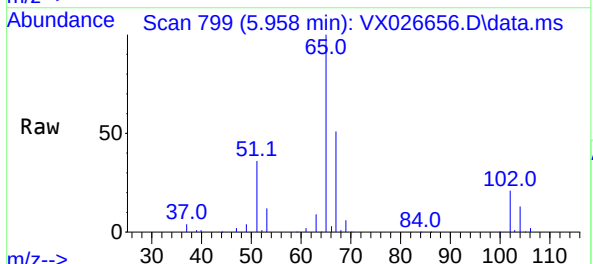


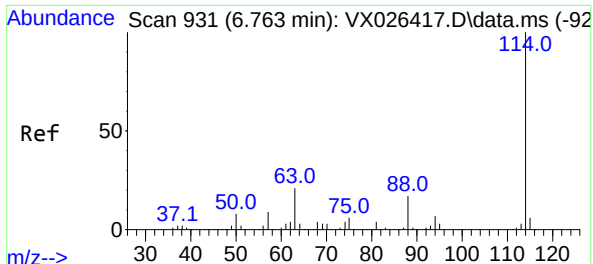

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.006 min
Lab File: VX026656.D
Acq: 28 Jan 2022 17:08




Instrument :
MSVOA_X
ClientSampleId :
MW-7M


Tgt Ion:114 Resp: 205306
Ion Ratio Lower Upper
114 100
63 20.6 0.0 42.8
88 16.0 0.0 33.0

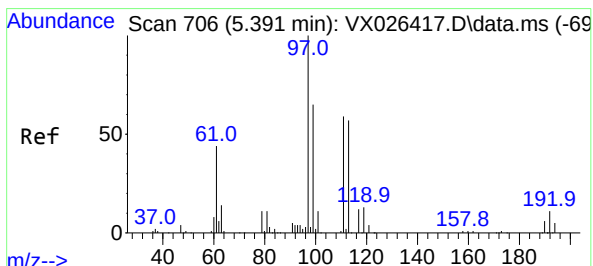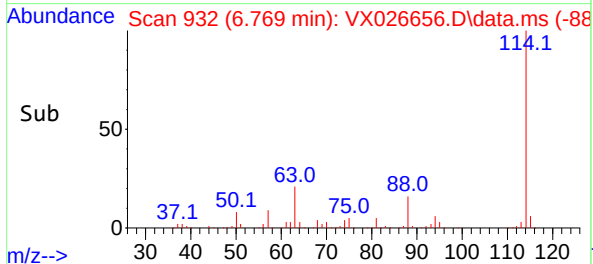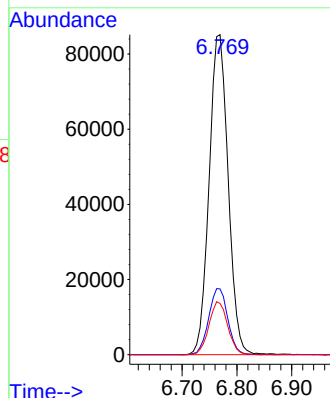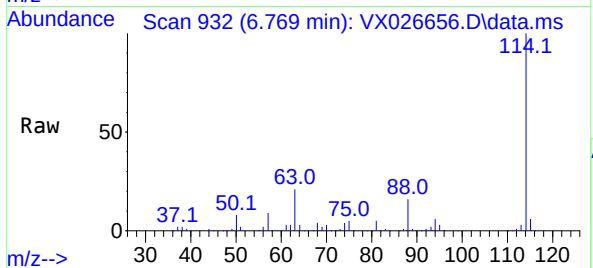

#35
Dibromofluoromethane
Concen: 49.180 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX026656.D
Acq: 28 Jan 2022 17:08

Tgt Ion:113 Resp: 65203
Ion Ratio Lower Upper
113 100
111 102.1 81.2 121.8
192 19.0 15.0 22.4

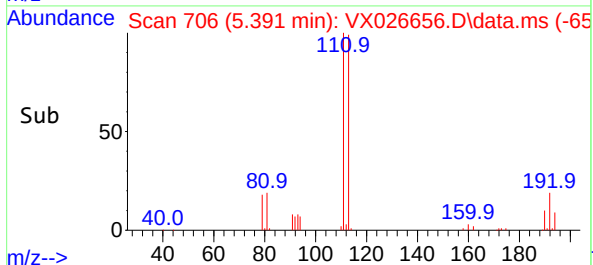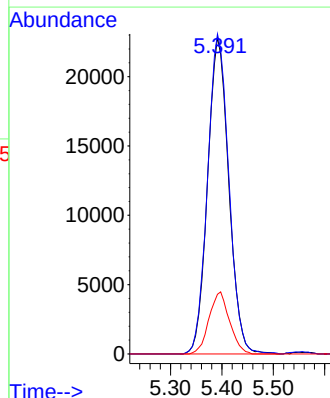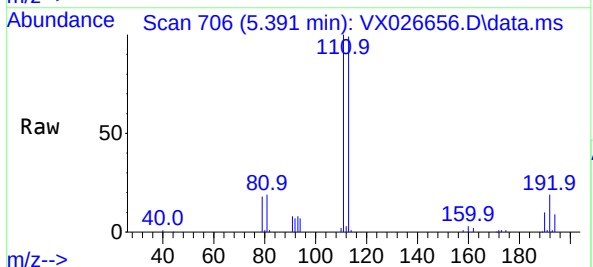

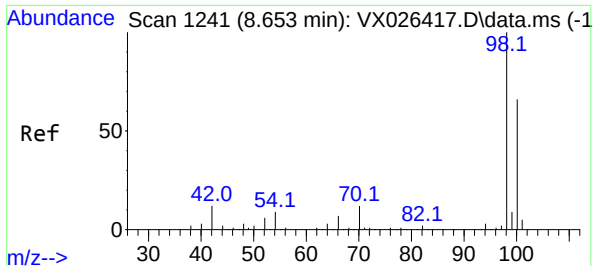

#50

Toluene-d8

Concen: 50.204 ug/l

RT: 8.653 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX026656.D

Acq: 28 Jan 2022 17:08

Instrument :

MSVOA_X

ClientSampleId :





MW-7M

Tgt Ion: 98 Resp: 239855

Ion Ratio Lower Upper

98 100

100 65.8 53.2 79.8

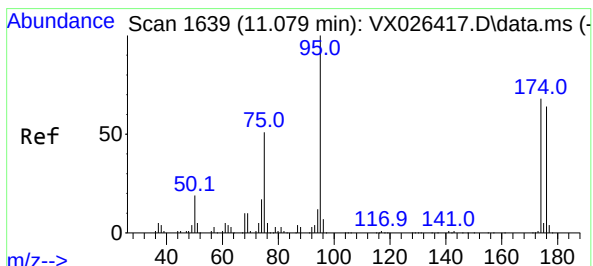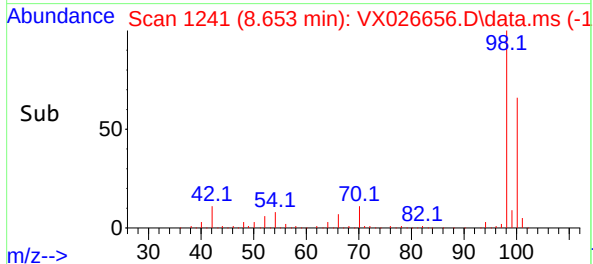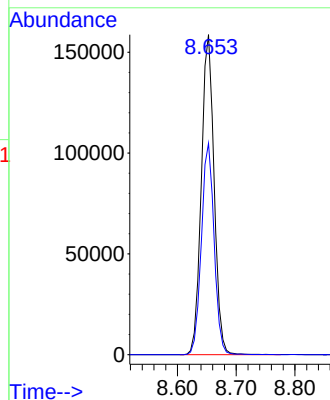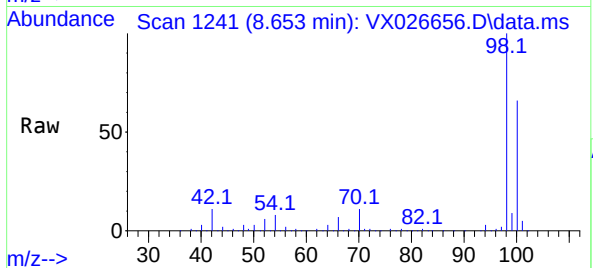

#62

4-Bromofluorobenzene

Concen: 48.179 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.006 min

Lab File: VX026656.D

Acq: 28 Jan 2022 17:08




Tgt Ion: 95 Resp: 81769


Ion Ratio Lower Upper

95 100

174 74.9 0.0 148.6

176 72.3 0.0 141.4


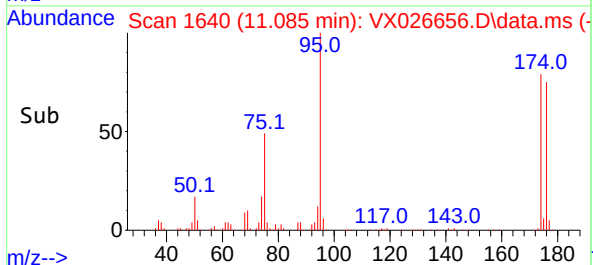
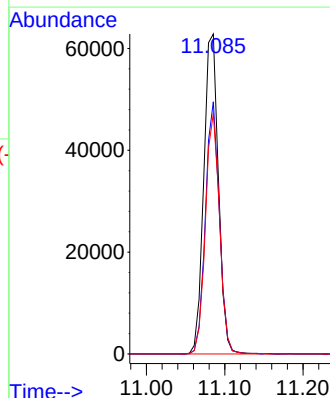
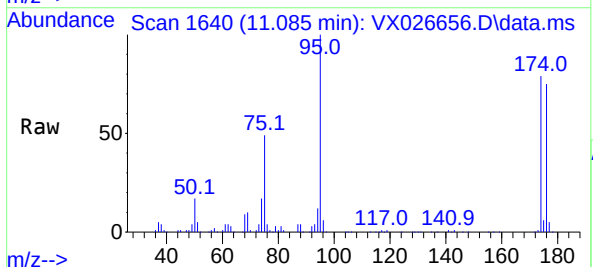


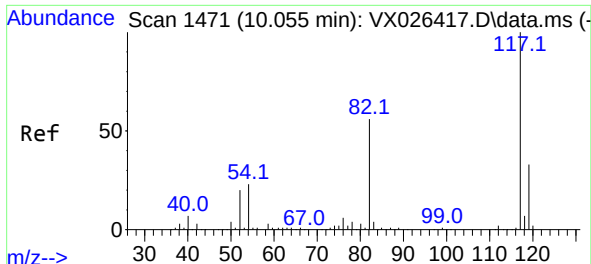

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX026656.D
Acq: 28 Jan 2022 17:08

Instrument :
MSVOA_X
ClientSampleId :
MW-7M

Tgt Ion:117 Resp: 177730
Ion Ratio Lower Upper
117 100
82 57.2 45.2 67.8
119 32.4 26.2 39.2

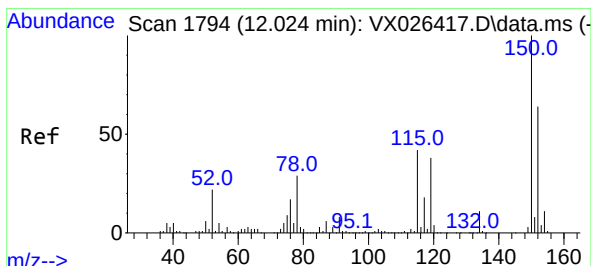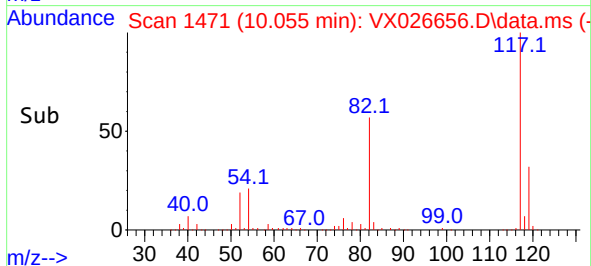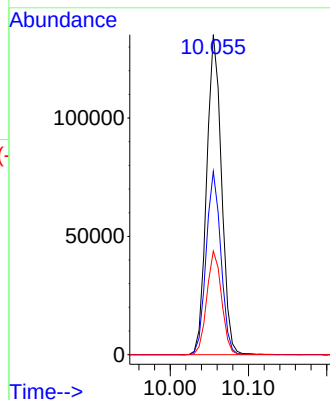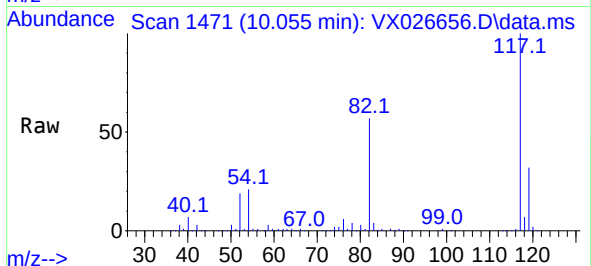

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX026656.D
Acq: 28 Jan 2022 17:08

Tgt Ion:152 Resp: 73044
Ion Ratio Lower Upper
152 100
115 60.9 44.2 132.6
150 156.4 0.0 348.2

