


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012822\
Data File : VX026640.D
Acq On : 28 Jan 2022 09:59
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011122W.M
Title : SW846 8260
Last Update : Tue Jan 11 14:45:13 2022

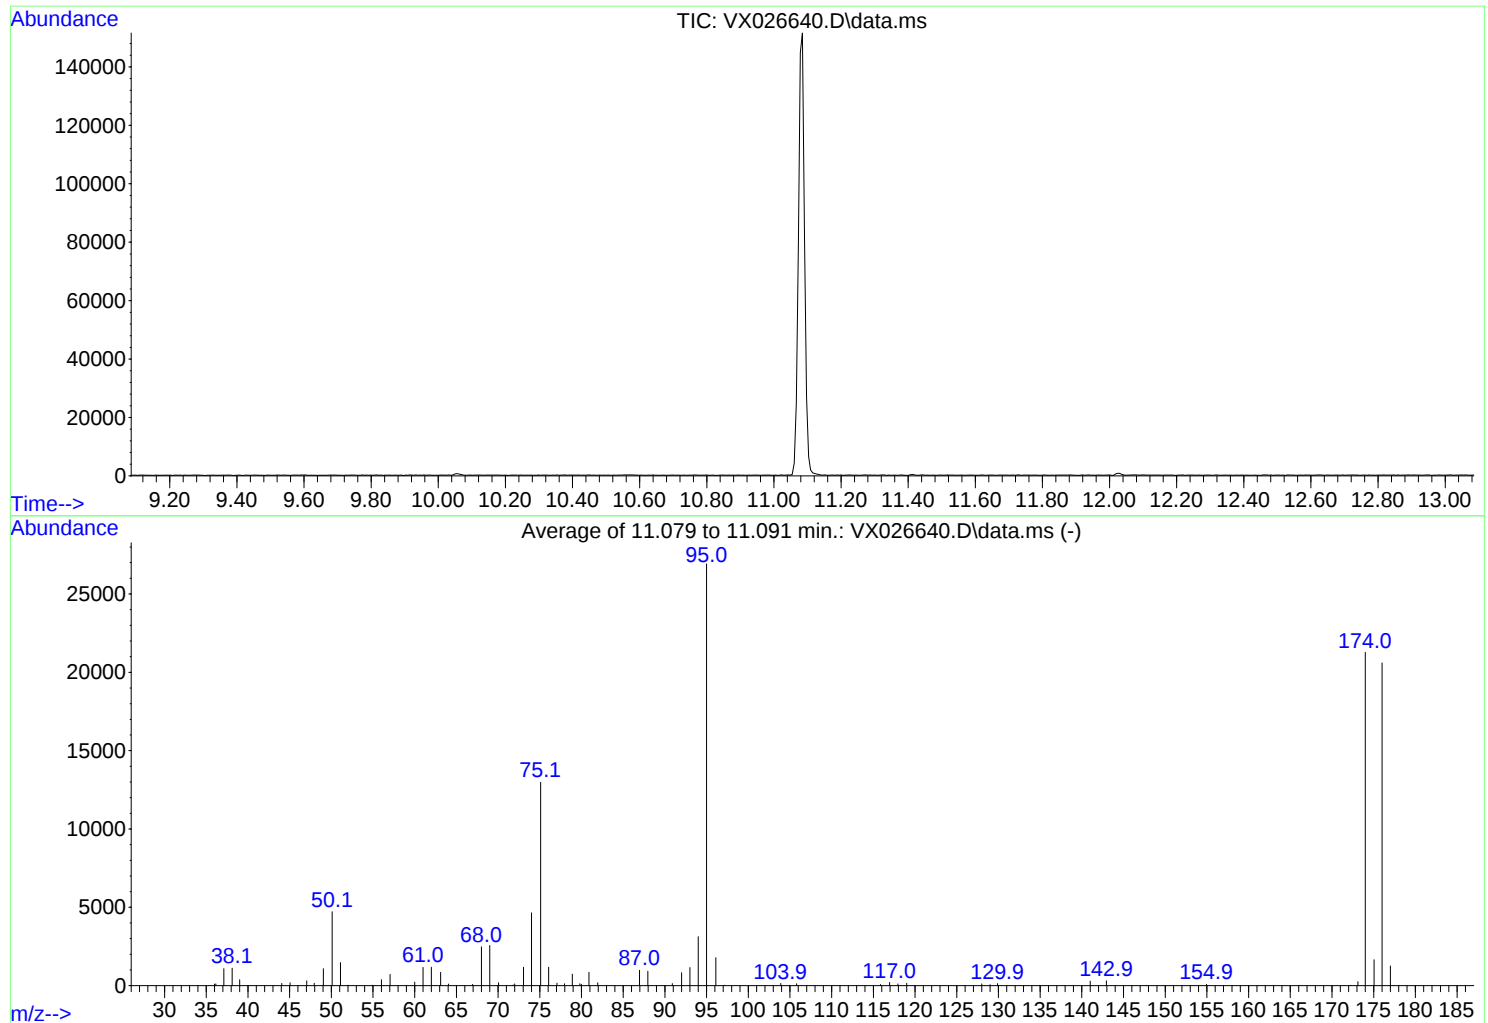

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	4716	PASS
75	95	30	60	48.2	12979	PASS
95	95	100	100	100.0	26925	PASS
96	95	5	9	6.7	1792	PASS
173	174	0.00	2	1.2	257	PASS
174	95	50	100	79.0	21274	PASS
175	174	5	9	7.8	1653	PASS
176	174	95	101	96.8	20600	PASS
177	176	5	9	6.1	1254	PASS