

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044744.D
 Acq On : 28 Jan 2025 15:02
 Operator : JC/MD
 Sample : VX0128MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 29 07:40:13 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 28 12:04:44 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	306132	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	271147	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	115927	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	99947	43.373	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.740%		
7) Chloroethane-d5	1.642	69	34907	39.874	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.740%		
11) 1,1-Dichloroethene-d2	2.294	65	39606	40.209	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.420%		
21) 2-Butanone-d5	4.452	46	115617	117.362	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	117.360%		
24) Chloroform-d	5.044	84	172589	42.622	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.240%		
26) 1,2-Dichloroethane-d4	5.946	65	107410	44.192	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.380%		
32) Benzene-d6	5.964	84	377431	44.518	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.040%		
36) 1,2-Dichloropropane-d6	7.299	67	118985	44.339	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.680%		
41) Toluene-d8	8.641	98	330540	44.050	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.100%		
43) trans-1,3-Dichloroprop...	8.945	79	55232	43.390	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.780%		
47) 2-Hexanone-d5	9.384	63	74248	93.488	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.490%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	155135	46.521	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.040%		
66) 1,2-Dichlorobenzene-d4	12.317	152	104409	46.030	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.060%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	12.018	75	15991	6.248	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044744.D
Acq On : 28 Jan 2025 15:02
Operator : JC/MD
Sample : VX0128MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 29 07:40:13 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 12:04:44 2025
Response via : Initial Calibration

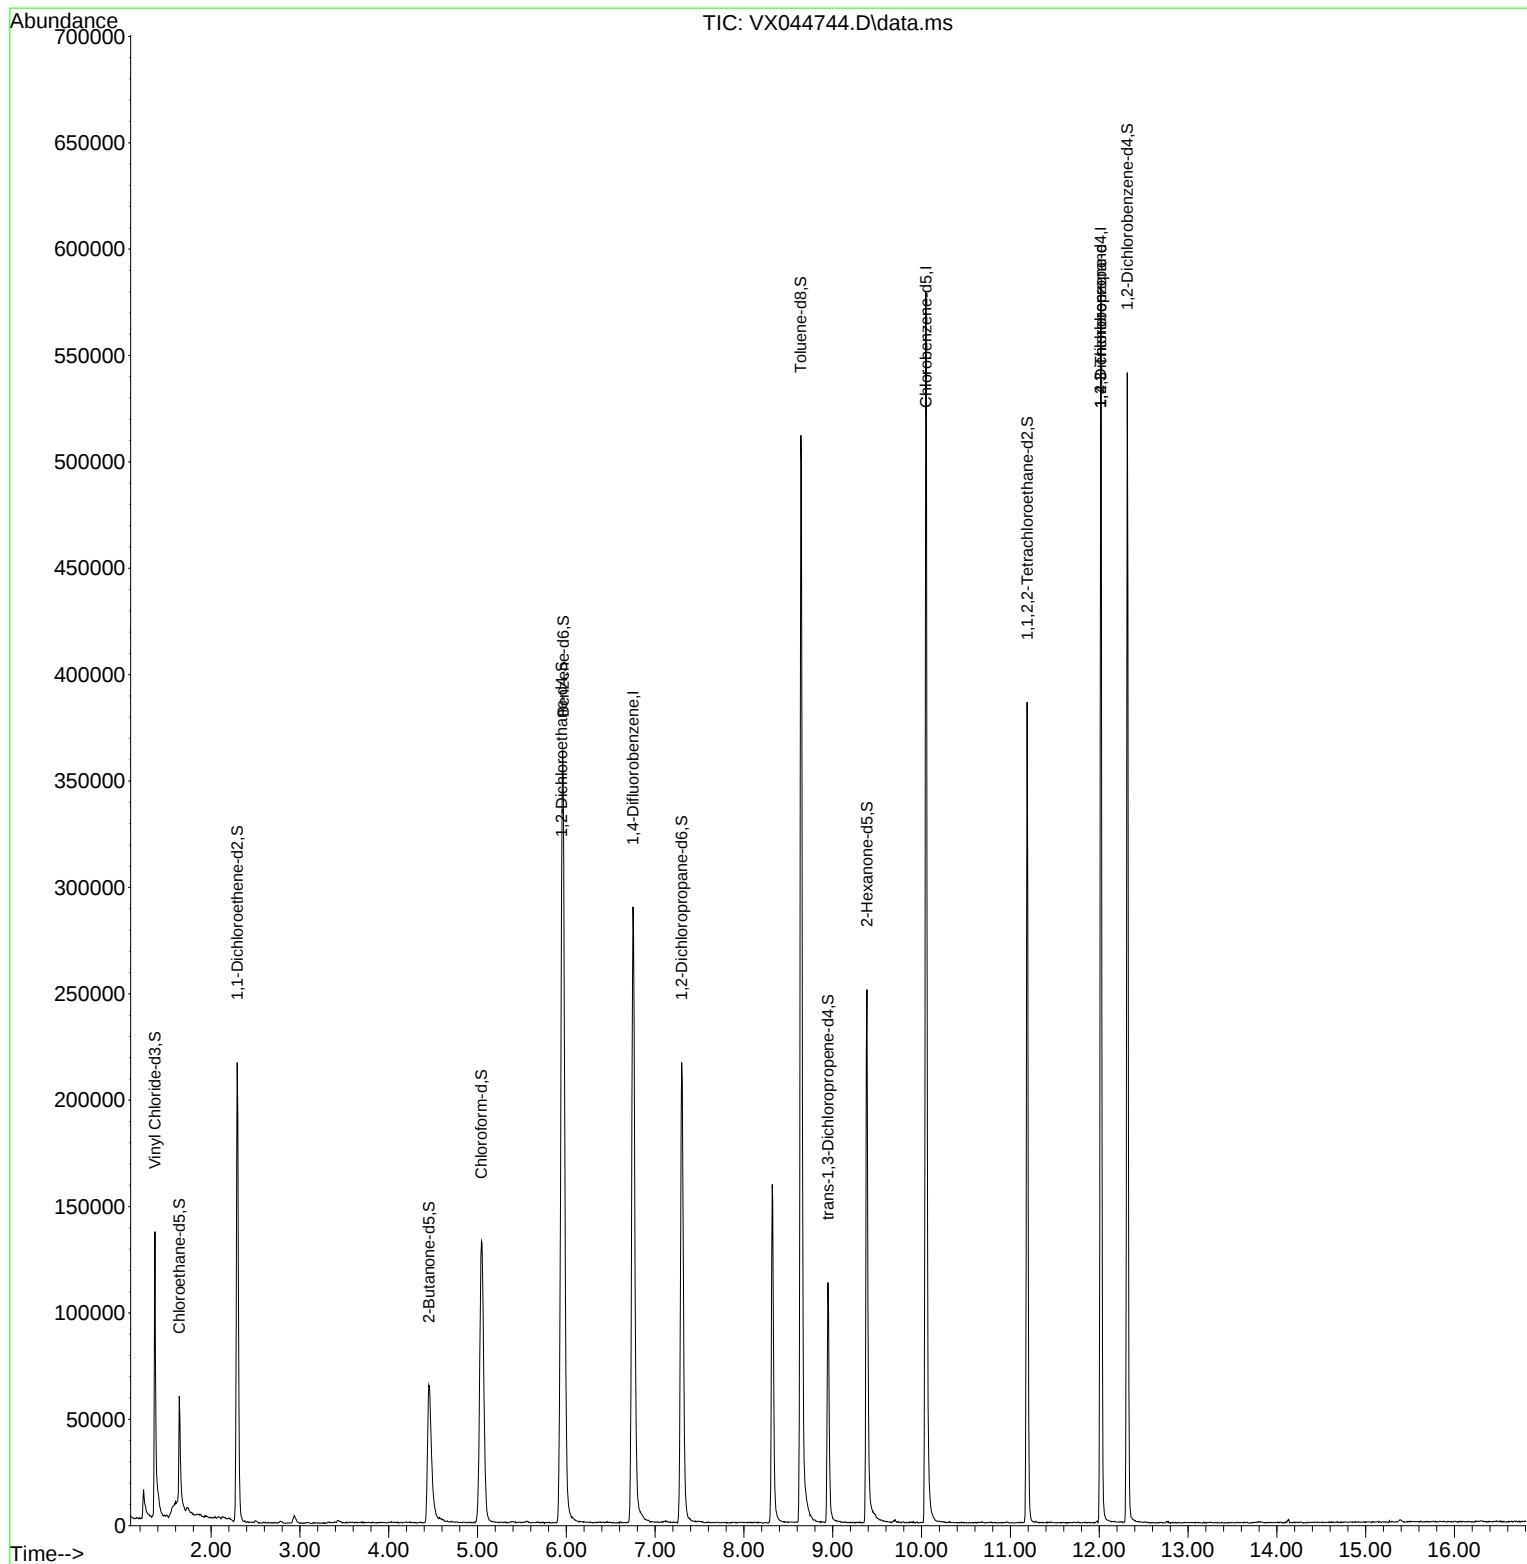

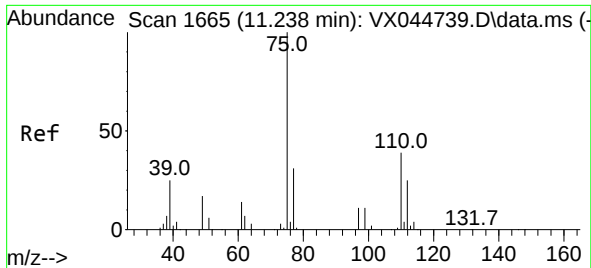

#61
 1,2,3-Trichloropropane
 Concen: 6.248 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX044744.D
 Acq: 28 Jan 2025 15:02

Instrument :
 MSVOA_X
 ClientSampleId :

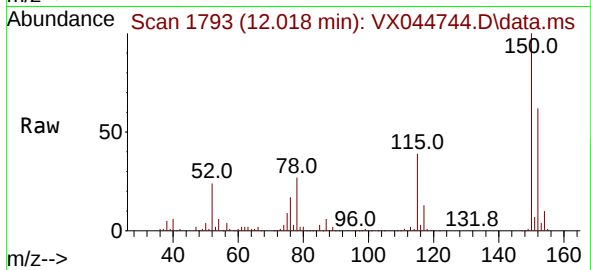

Tgt Ion: 75 Resp: 15991
 Ion Ratio Lower Upper
 75 100
 77 30.5 25.8 38.6
 110 2.4 30.8 46.2#

