

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044748.D
 Acq On : 28 Jan 2025 16:44
 Operator : JC/MD
 Sample : PB166233TB 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 29 07:41:17 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 28 12:04:44 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	311405	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	271246	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	111335	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	98763	42.133	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.260%	
7) Chloroethane-d5	1.648	69	48235	54.166	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	108.340%	
11) 1,1-Dichloroethene-d2	2.294	65	40934	40.854	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	81.700%	
21) 2-Butanone-d5	4.458	46	120376	120.123	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	120.120%	
24) Chloroform-d	5.050	84	176337	42.810	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	85.620%	
26) 1,2-Dichloroethane-d4	5.952	65	111597	45.137	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.280%	
32) Benzene-d6	5.970	84	382329	45.079	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.160%	
36) 1,2-Dichloropropane-d6	7.305	67	122755	45.727	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	91.460%	
41) Toluene-d8	8.647	98	334007	44.496	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	89.000%	
43) trans-1,3-Dichloroprop...	8.945	79	55990	43.970	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	87.940%	
47) 2-Hexanone-d5	9.384	63	76098	95.782	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	95.780%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	155469	46.605	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	93.200%	
66) 1,2-Dichlorobenzene-d4	12.317	152	100911	46.322	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.640%	
Target Compounds						
13) Acetone	2.386	43	6552	6.557	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044748.D
Acq On : 28 Jan 2025 16:44
Operator : JC/MD
Sample : PB166233TB 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jan 29 07:41:17 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 12:04:44 2025
Response via : Initial Calibration

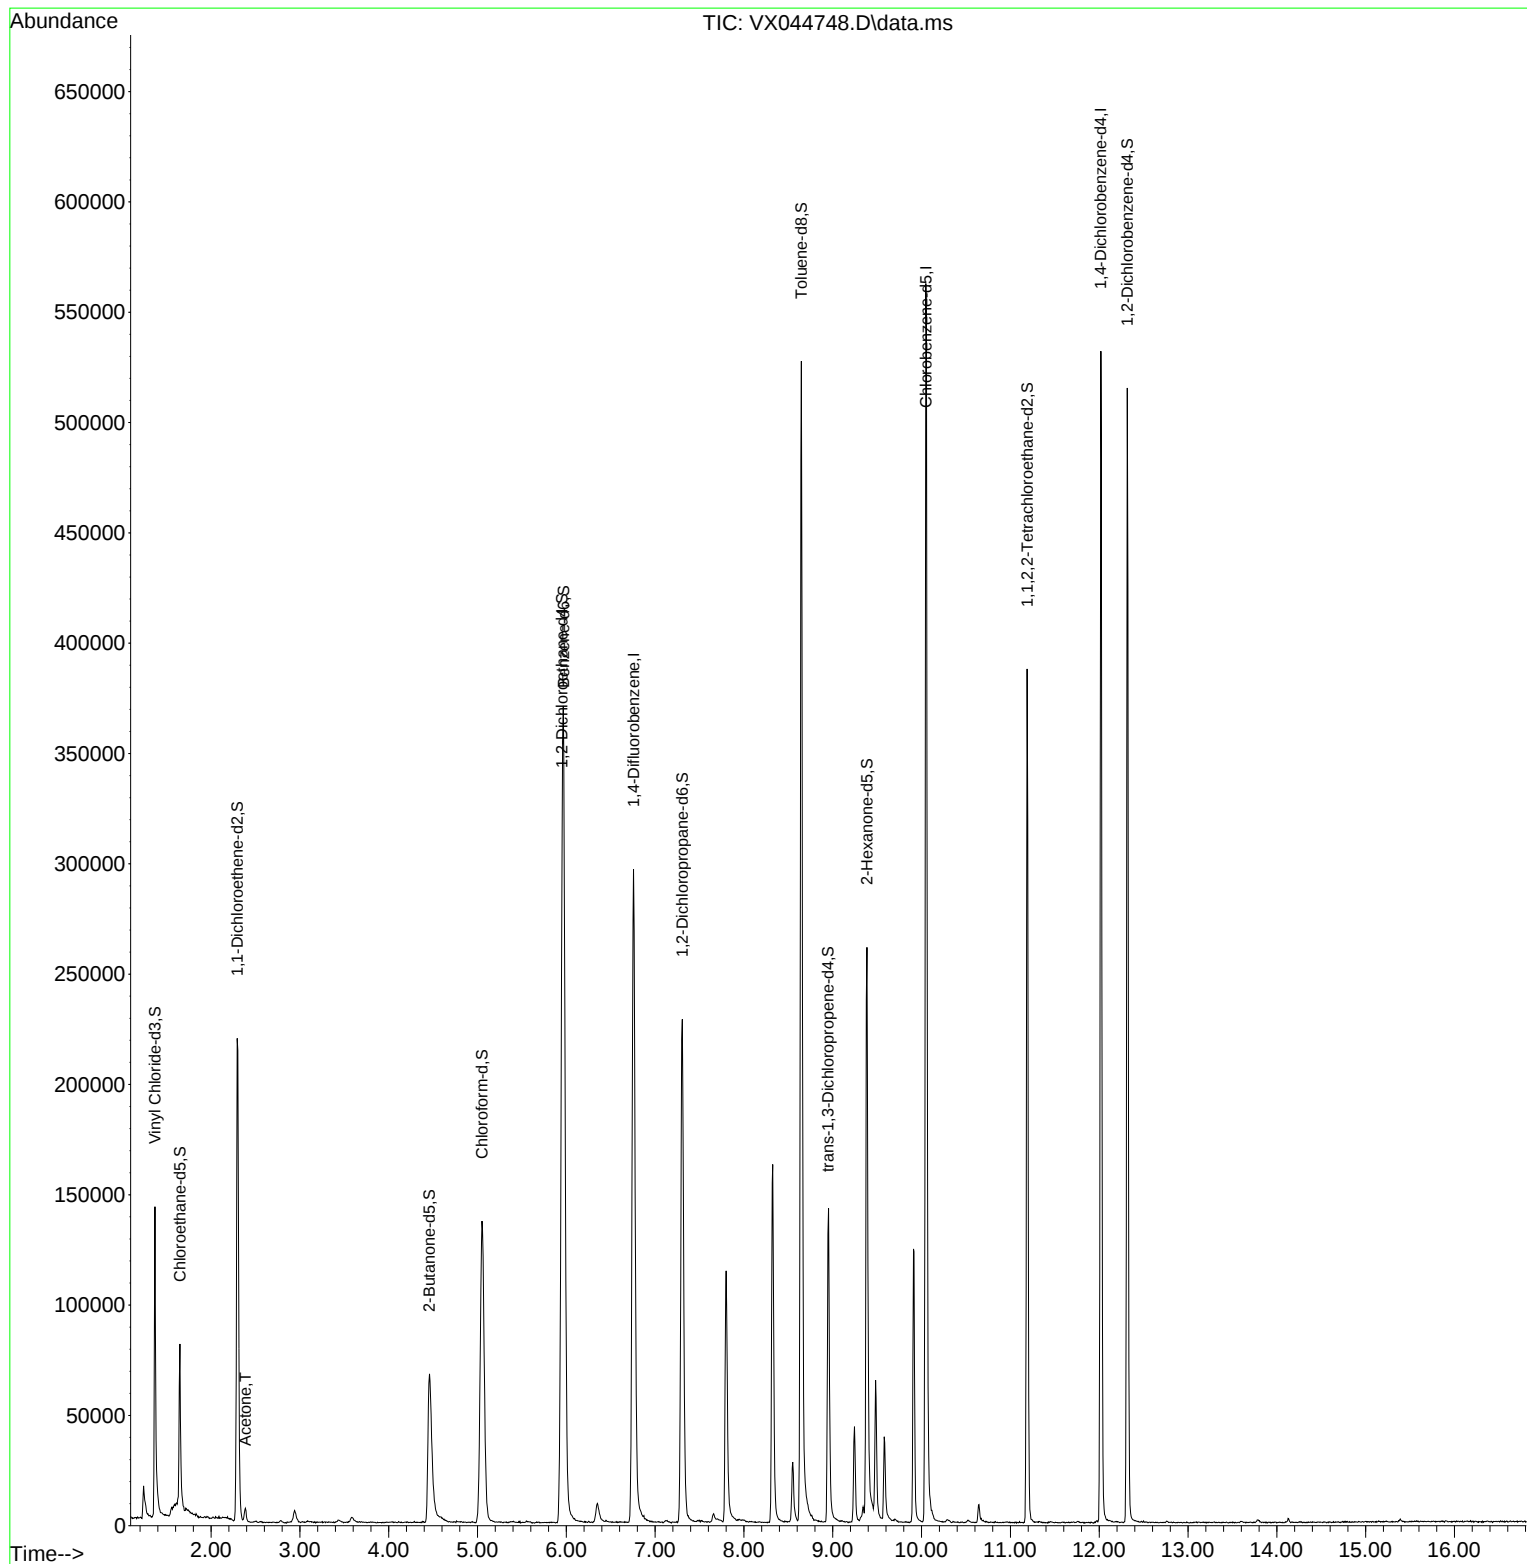

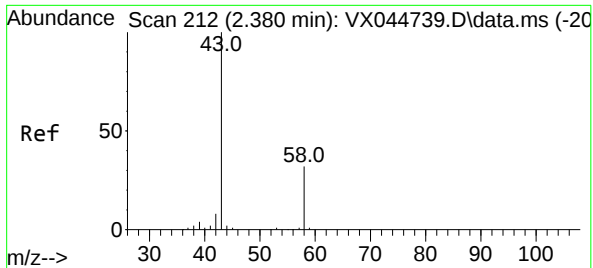

#13
 Acetone
 Concen: 6.557 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX044748.D
 Acq: 28 Jan 2025 16:44

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 43 Resp: 6552
 Ion Ratio Lower Upper
 43 100
 58 26.9 0.0 64.6

