

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044744.D
 Acq On : 28 Jan 2025 15:02
 Operator : JC/MD
 Sample : VX0128MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK753

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

Signal : TIC: VX044744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	37	rBV	13527	25733	2.37%	0.320%
2	1.368	42	46	61	rVB	133925	163654	15.08%	2.034%
3	1.642	88	91	102	rVB	53820	72761	6.71%	0.904%
4	2.294	192	198	211	rVV	215779	342068	31.52%	4.251%
5	2.410	215	217	219	rBV	424	300	0.03%	0.004%
6	2.495	229	231	238	rVB4	1188	2224	0.20%	0.028%
7	2.544	238	239	244	rBV2	383	408	0.04%	0.005%
8	2.593	244	247	249	rVV3	558	575	0.05%	0.007%
9	2.611	249	250	252	rVB	450	252	0.02%	0.003%
10	2.642	252	255	256	rBV3	390	290	0.03%	0.004%
11	2.751	272	273	274	rBV	291	173	0.02%	0.002%
12	2.776	275	277	280	rVV2	670	860	0.08%	0.011%
13	2.855	288	290	292	rBV	200	173	0.02%	0.002%
14	2.934	298	303	313	rVB3	3752	8810	0.81%	0.109%
15	3.007	313	315	320	rBV2	404	516	0.05%	0.006%
16	3.099	322	330	333	rVB4	482	1153	0.11%	0.014%
17	3.148	336	338	339	rBV2	321	199	0.02%	0.002%
18	3.166	339	341	342	rBV	369	238	0.02%	0.003%
19	3.209	347	348	351	rVV2	364	315	0.03%	0.004%
20	3.233	351	352	354	rVV	223	207	0.02%	0.003%
21	3.257	354	356	357	rVB2	337	206	0.02%	0.003%
22	3.318	363	366	367	rBV	555	625	0.06%	0.008%
23	3.373	373	375	376	rBV	313	207	0.02%	0.003%
24	3.428	381	384	388	rBV4	906	1616	0.15%	0.020%
25	3.526	399	400	402	rVB	585	312	0.03%	0.004%
26	3.556	402	405	408	rBV2	471	638	0.06%	0.008%
27	3.629	416	417	420	rVB2	478	334	0.03%	0.004%
28	3.696	426	428	431	rVB	579	467	0.04%	0.006%
29	3.745	434	436	439	rBV	339	425	0.04%	0.005%
30	3.818	446	448	450	rBV	505	444	0.04%	0.006%
31	3.891	458	460	461	rBV	294	161	0.01%	0.002%
32	4.001	474	478	480	rBV3	482	697	0.06%	0.009%
33	4.288	524	525	529	rVB2	402	402	0.04%	0.005%
34	4.452	544	552	570	rBV2	64613	208313	19.20%	2.589%
35	4.958	633	635	637	rVB2	413	357	0.03%	0.004%
36	5.044	637	649	664	rBV	132628	418799	38.59%	5.205%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044744.D
 Acq On : 28 Jan 2025 15:02
 Operator : JC/MD
 Sample : VX0128MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK753

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

37	5.300	689	691	693	rBV2	305	240	0.02%	0.003%
38	5.367	700	702	703	rBV	393	292	0.03%	0.004%
39	5.672	751	752	755	rBV	380	279	0.03%	0.003%
40	5.763	765	767	768	rBV	546	516	0.05%	0.006%
41	5.842	778	780	783	rBV	348	297	0.03%	0.004%
42	5.958	788	799	816	rBV2	363114	1085148	100.00%	13.487%
43	6.318	856	858	861	rBV2	347	443	0.04%	0.006%
44	6.592	902	903	904	rVB	404	148	0.01%	0.002%
45	6.604	904	905	908	rBV	683	666	0.06%	0.008%
46	6.751	920	929	956	rBV	289414	722330	66.57%	8.977%
47	7.208	1002	1004	1007	rBV3	429	409	0.04%	0.005%
48	7.299	1011	1019	1038	rBV	216455	495840	45.69%	6.163%
49	7.586	1065	1066	1068	rBV2	316	217	0.02%	0.003%
50	7.811	1102	1103	1105	rBV	380	261	0.02%	0.003%
51	8.159	1159	1160	1161	rBV	413	162	0.01%	0.002%
52	8.226	1169	1171	1174	rBV2	342	457	0.04%	0.006%
53	8.317	1180	1186	1200	rBV	158798	272247	25.09%	3.384%
54	8.641	1233	1239	1262	rBV	510860	878378	80.95%	10.917%
55	8.945	1284	1289	1304	rBV	112822	174821	16.11%	2.173%
56	9.384	1356	1361	1386	rBV	250315	400006	36.86%	4.971%
57	9.683	1408	1410	1411	rBV2	663	479	0.04%	0.006%
58	9.848	1435	1437	1438	rBV2	305	231	0.02%	0.003%
59	9.909	1446	1447	1449	rBV	657	341	0.03%	0.004%
60	9.951	1451	1454	1455	rVB	508	445	0.04%	0.006%
61	10.049	1465	1470	1493	rBV	578386	843838	77.76%	10.488%
62	10.530	1548	1549	1552	rBV	296	314	0.03%	0.004%
63	10.634	1564	1566	1567	rBV	343	329	0.03%	0.004%
64	10.726	1579	1581	1582	rBV	388	275	0.03%	0.003%
65	10.768	1586	1588	1590	rVV2	347	280	0.03%	0.003%
66	10.848	1599	1601	1603	rBV	308	286	0.03%	0.004%
67	10.878	1604	1606	1608	rBV	267	239	0.02%	0.003%
68	11.122	1645	1646	1649	rBV	309	304	0.03%	0.004%
69	11.189	1652	1657	1670	rVB	385540	494641	45.58%	6.148%
70	11.408	1692	1693	1694	rVB	413	151	0.01%	0.002%
71	11.451	1699	1700	1705	rVB3	452	595	0.05%	0.007%
72	11.658	1732	1734	1735	rBV	322	267	0.02%	0.003%
73	11.713	1740	1743	1745	rBV2	457	552	0.05%	0.007%
74	11.817	1759	1760	1761	rBV	316	204	0.02%	0.003%
75	11.981	1782	1787	1788	rBV2	798	1094	0.10%	0.014%
76	12.018	1788	1793	1811	rVV	582376	728686	67.15%	9.056%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044744.D
 Acq On : 28 Jan 2025 15:02
 Operator : JC/MD
 Sample : VX0128MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK753

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

77	12.274	1834	1835	1837	rBV	380	390	0.04%	0.005%
78	12.317	1837	1842	1859	rVV	540460	674709	62.18%	8.386%
79	12.585	1882	1886	1887	rVB	255	248	0.02%	0.003%
80	12.609	1887	1890	1894	rBV	371	362	0.03%	0.004%
81	12.683	1900	1902	1903	rBV	421	350	0.03%	0.004%
82	12.762	1911	1915	1917	rBV2	665	733	0.07%	0.009%
83	12.823	1922	1925	1926	rBV2	439	479	0.04%	0.006%
84	12.841	1926	1928	1930	rBV	245	294	0.03%	0.004%
85	12.896	1935	1937	1940	rVB3	365	352	0.03%	0.004%
86	13.176	1981	1983	1984	rBV	509	307	0.03%	0.004%
87	13.304	2002	2004	2006	rBV	346	268	0.02%	0.003%
88	13.329	2006	2008	2009	rVB2	287	167	0.02%	0.002%
89	13.378	2014	2016	2021	rVB2	445	545	0.05%	0.007%
90	13.640	2057	2059	2062	rBV2	367	433	0.04%	0.005%
91	13.707	2068	2070	2072	rBV	351	265	0.02%	0.003%
92	13.780	2080	2082	2084	rBV	468	426	0.04%	0.005%
93	14.097	2133	2134	2135	rBV	451	204	0.02%	0.003%
94	14.134	2136	2140	2142	rVB2	1593	1834	0.17%	0.023%
95	14.255	2159	2160	2162	rBV	335	305	0.03%	0.004%
96	14.347	2174	2175	2176	rBV2	400	246	0.02%	0.003%
97	14.597	2214	2216	2218	rBV2	447	319	0.03%	0.004%
98	15.078	2293	2295	2296	rBV	545	475	0.04%	0.006%
99	15.158	2306	2308	2311	rVB2	411	260	0.02%	0.003%
100	15.267	2325	2326	2328	rBV	824	464	0.04%	0.006%

Sum of corrected areas: 8046055




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044744.D
Acq On : 28 Jan 2025 15:02
Operator : JC/MD
Sample : VX0128MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK753

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

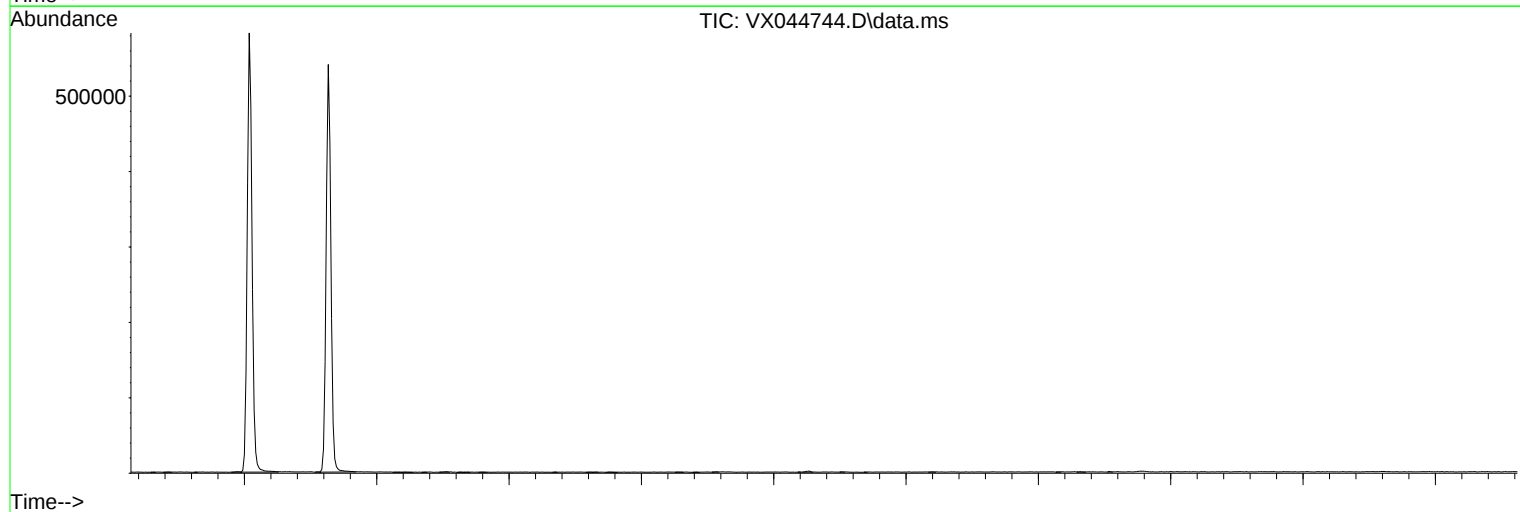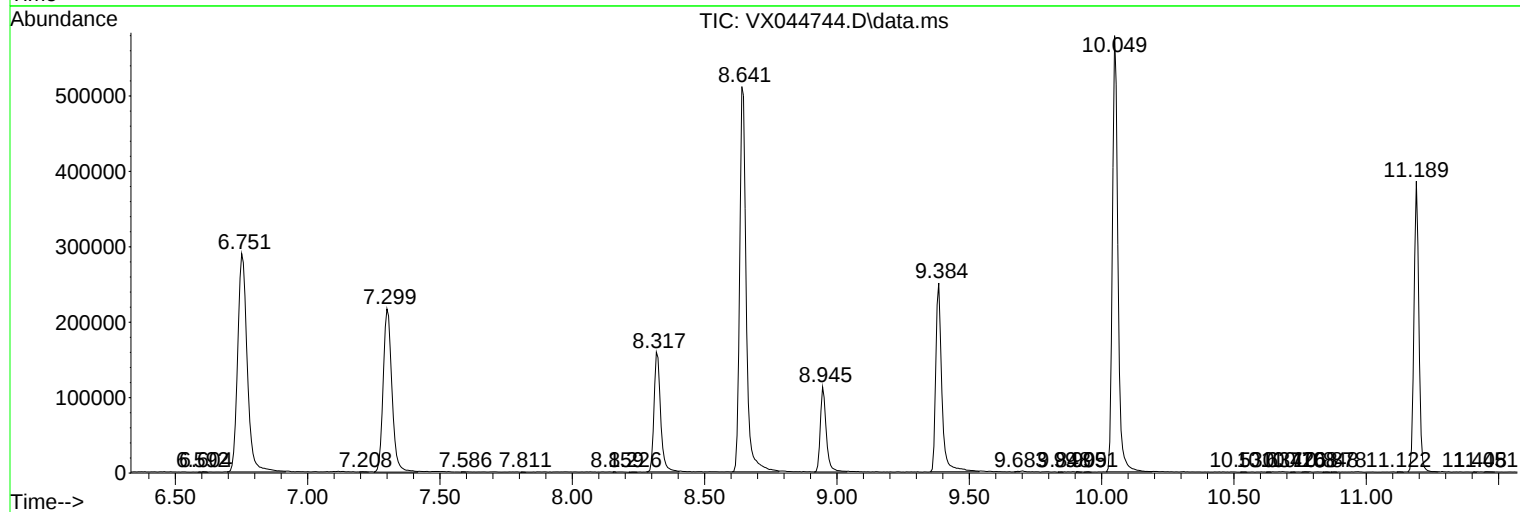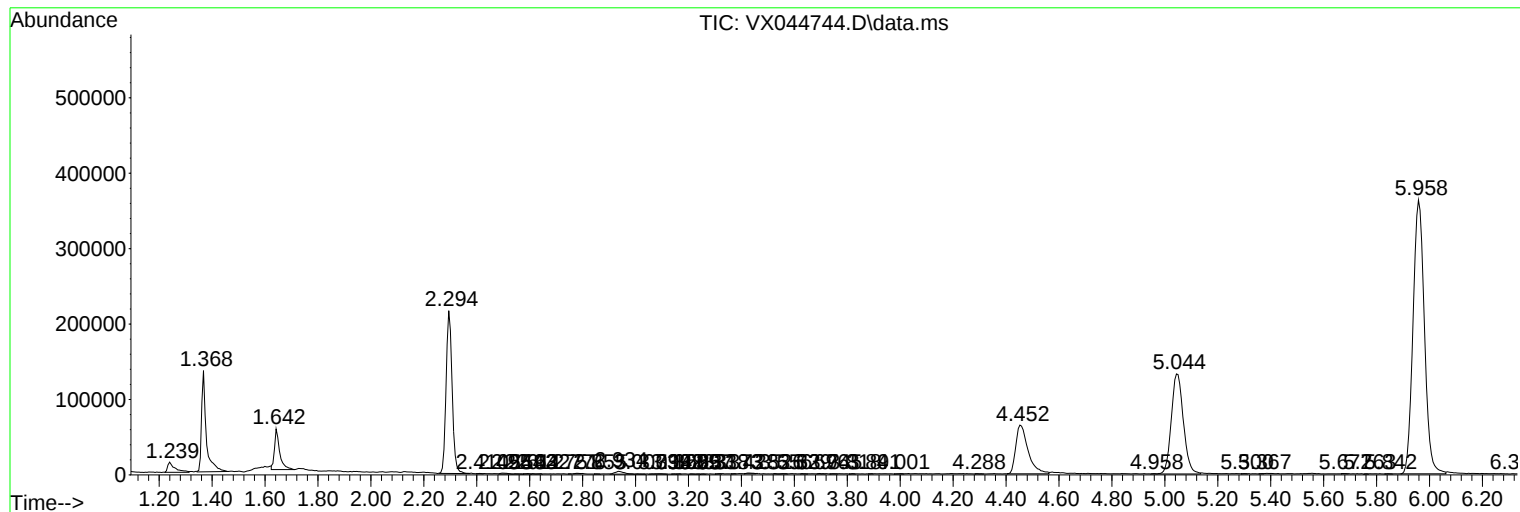

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044744.D
Acq On : 28 Jan 2025 15:02
Operator : JC/MD
Sample : VX0128MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK753

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044744.D
Acq On : 28 Jan 2025 15:02
Operator : JC/MD
Sample : VX0128MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK753

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc