

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044745.D
 Acq On : 28 Jan 2025 15:29
 Operator : JC/MD
 Sample : VX0128WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK754

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

Signal : TIC: VX044745.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	36	rBV	14929	24853	2.25%	0.309%
2	1.368	42	46	59	rBV	129683	155992	14.12%	1.942%
3	1.642	88	91	103	rVB	52870	68771	6.23%	0.856%
4	2.294	192	198	212	rVB	250582	388585	35.18%	4.838%
5	2.782	274	278	283	rVB5	925	1598	0.14%	0.020%
6	2.941	296	304	311	rBV2	5242	13078	1.18%	0.163%
7	3.056	320	323	324	rBV2	487	503	0.05%	0.006%
8	3.130	333	335	336	rBV2	367	328	0.03%	0.004%
9	3.410	377	381	382	rBV2	506	720	0.07%	0.009%
10	3.532	399	401	403	rVV2	448	326	0.03%	0.004%
11	3.587	406	410	412	rBV3	594	710	0.06%	0.009%
12	3.855	452	454	456	rBV2	332	379	0.03%	0.005%
13	3.898	459	461	462	rVV	410	340	0.03%	0.004%
14	3.916	462	464	466	rVB	534	356	0.03%	0.004%
15	4.129	497	499	502	rVB2	451	391	0.04%	0.005%
16	4.178	504	507	510	rVB2	520	497	0.04%	0.006%
17	4.215	510	513	514	rBV	644	604	0.05%	0.008%
18	4.294	524	526	529	rVB2	361	337	0.03%	0.004%
19	4.331	529	532	533	rBV2	537	458	0.04%	0.006%
20	4.459	545	553	569	rBV	65982	211887	19.18%	2.638%
21	4.800	607	609	611	rBV2	495	393	0.04%	0.005%
22	4.837	614	615	618	rBV3	428	497	0.04%	0.006%
23	5.050	638	650	669	rVV	137873	425665	38.53%	5.300%
24	5.263	684	685	692	rVB3	453	451	0.04%	0.006%
25	5.318	692	694	697	rBV3	511	461	0.04%	0.006%
26	5.373	700	703	704	rBV	648	800	0.07%	0.010%
27	5.544	730	731	734	rVV2	695	631	0.06%	0.008%
28	5.794	769	772	776	rBV2	572	894	0.08%	0.011%
29	5.958	786	799	818	rBV2	368332	1104628	100.00%	13.753%
30	6.355	862	864	866	rVV2	455	414	0.04%	0.005%
31	6.391	869	870	872	rBV	489	411	0.04%	0.005%
32	6.464	879	882	884	rBV3	492	485	0.04%	0.006%
33	6.629	906	909	910	rBV	305	325	0.03%	0.004%
34	6.757	920	930	950	rBV	282231	718090	65.01%	8.941%
35	6.952	961	962	964	rBV2	682	528	0.05%	0.007%
36	7.202	999	1003	1006	rBV3	305	462	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044745.D
 Acq On : 28 Jan 2025 15:29
 Operator : JC/MD
 Sample : VX0128WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK754

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

37	7.300	1011	1019	1041	rVV	222137	503627	45.59%	6.270%
38	7.684	1079	1082	1085	rBV3	254	362	0.03%	0.005%
39	7.751	1092	1093	1095	rBV	397	323	0.03%	0.004%
40	7.921	1119	1121	1123	rVV2	366	305	0.03%	0.004%
41	7.964	1126	1128	1129	rVV2	423	302	0.03%	0.004%
42	8.007	1131	1135	1137	rVV3	581	750	0.07%	0.009%
43	8.031	1137	1139	1140	rVV	504	318	0.03%	0.004%
44	8.220	1167	1170	1171	rBV2	301	299	0.03%	0.004%
45	8.318	1180	1186	1204	rVV	160271	278021	25.17%	3.461%
46	8.537	1219	1222	1225	rBV5	374	566	0.05%	0.007%
47	8.580	1227	1229	1230	rBV	572	359	0.03%	0.004%
48	8.641	1233	1239	1263	rVV	501456	877152	79.41%	10.921%
49	8.946	1284	1289	1305	rBV	111499	172415	15.61%	2.147%
50	9.250	1336	1339	1340	rBV	377	291	0.03%	0.004%
51	9.281	1340	1344	1346	rBV2	675	622	0.06%	0.008%
52	9.385	1356	1361	1382	rBV	252153	402575	36.44%	5.012%
53	9.616	1398	1399	1401	rBV2	465	353	0.03%	0.004%
54	9.677	1407	1409	1410	rBV	491	449	0.04%	0.006%
55	9.695	1410	1412	1417	rVB3	1739	2079	0.19%	0.026%
56	9.775	1423	1425	1426	rVB2	576	365	0.03%	0.005%
57	9.842	1433	1436	1438	rVB2	514	482	0.04%	0.006%
58	10.049	1465	1470	1492	rVV	557001	816761	73.94%	10.169%
59	10.311	1508	1513	1514	rBV3	502	720	0.07%	0.009%
60	10.360	1517	1521	1523	rBV	292	434	0.04%	0.005%
61	10.451	1532	1536	1540	rBV2	468	938	0.08%	0.012%
62	10.878	1603	1606	1609	rBV2	381	475	0.04%	0.006%
63	11.104	1641	1643	1644	rVB2	417	287	0.03%	0.004%
64	11.189	1652	1657	1668	rVV	382749	490389	44.39%	6.106%
65	11.378	1687	1688	1691	rBV2	347	309	0.03%	0.004%
66	11.439	1694	1698	1699	rBV2	421	513	0.05%	0.006%
67	11.518	1708	1711	1713	rBV2	341	410	0.04%	0.005%
68	11.616	1724	1727	1729	rVV2	335	354	0.03%	0.004%
69	11.848	1762	1765	1766	rBV2	486	365	0.03%	0.005%
70	12.018	1788	1793	1807	rVV	538427	683684	61.89%	8.512%
71	12.238	1827	1829	1832	rVB	531	384	0.03%	0.005%
72	12.317	1836	1842	1854	rBV	517438	651570	58.99%	8.112%
73	12.591	1885	1887	1889	rBV2	414	463	0.04%	0.006%
74	12.610	1889	1890	1894	rVB2	628	620	0.06%	0.008%
75	12.652	1894	1897	1899	rBV2	329	435	0.04%	0.005%
76	12.671	1899	1900	1903	rVB2	606	432	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044745.D
 Acq On : 28 Jan 2025 15:29
 Operator : JC/MD
 Sample : VX0128WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK754

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

77	12.762	1908	1915	1922	rBV4	806	1856	0.17%	0.023%
78	12.908	1933	1939	1943	rBV3	432	788	0.07%	0.010%
79	13.189	1981	1985	1988	rBV2	281	395	0.04%	0.005%
80	13.311	2003	2005	2008	rVB2	363	378	0.03%	0.005%
81	13.341	2008	2010	2014	rBV2	305	494	0.04%	0.006%
82	13.518	2038	2039	2043	rVB2	442	505	0.05%	0.006%
83	13.603	2049	2053	2054	rBV2	342	403	0.04%	0.005%
84	13.841	2090	2092	2094	rBV2	409	391	0.04%	0.005%
85	13.896	2100	2101	2105	rVB	350	336	0.03%	0.004%
86	13.933	2105	2107	2109	rBV2	447	418	0.04%	0.005%
87	14.128	2136	2139	2145	rVB3	1485	2255	0.20%	0.028%
88	14.274	2161	2163	2166	rBV	291	313	0.03%	0.004%
89	14.323	2169	2171	2173	rVB2	665	468	0.04%	0.006%
90	14.396	2181	2183	2186	rVB2	443	371	0.03%	0.005%
91	14.420	2186	2187	2191	rBV3	284	347	0.03%	0.004%
92	14.457	2191	2193	2196	rBV4	432	478	0.04%	0.006%
93	14.560	2208	2210	2213	rVB3	502	593	0.05%	0.007%
94	14.884	2261	2263	2268	rBV3	457	835	0.08%	0.010%
95	15.012	2281	2284	2285	rBV2	364	376	0.03%	0.005%
96	15.243	2320	2322	2323	rBV	426	318	0.03%	0.004%
97	16.042	2451	2453	2456	rBV2	603	586	0.05%	0.007%
98	16.213	2478	2481	2483	rBV3	553	541	0.05%	0.007%
99	16.420	2513	2515	2518	rBV3	397	365	0.03%	0.005%
100	16.719	2560	2564	2565	rBV2	531	605	0.05%	0.008%

Sum of corrected areas: 8031821




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044745.D
Acq On : 28 Jan 2025 15:29
Operator : JC/MD
Sample : VX0128WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK754

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

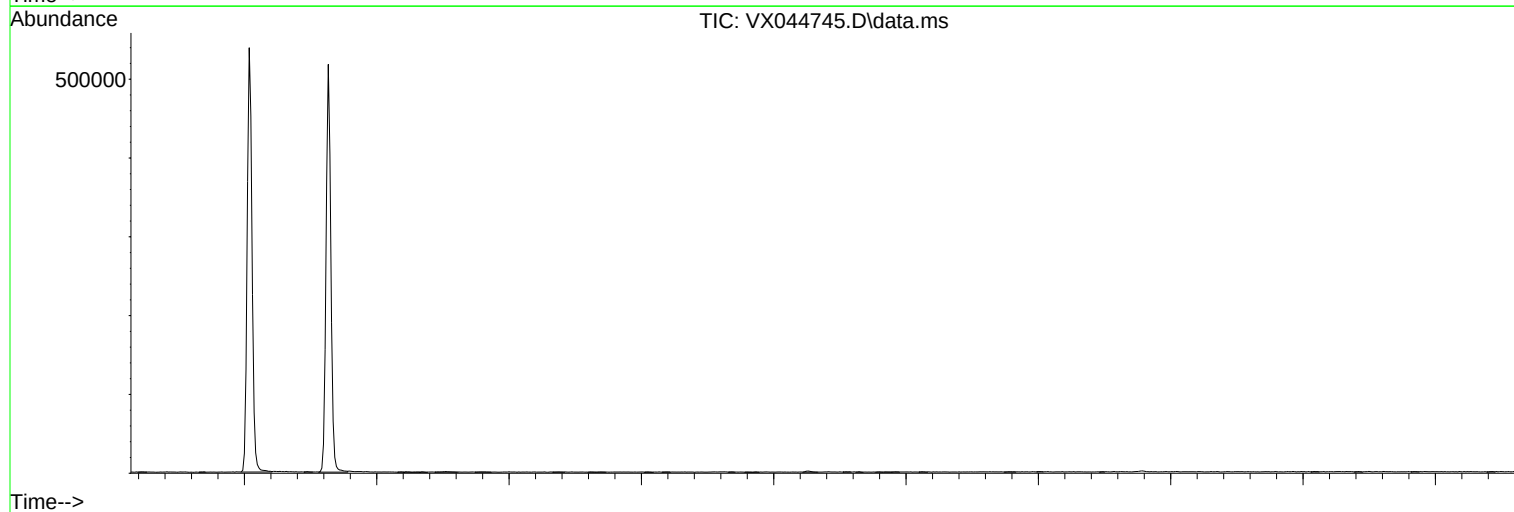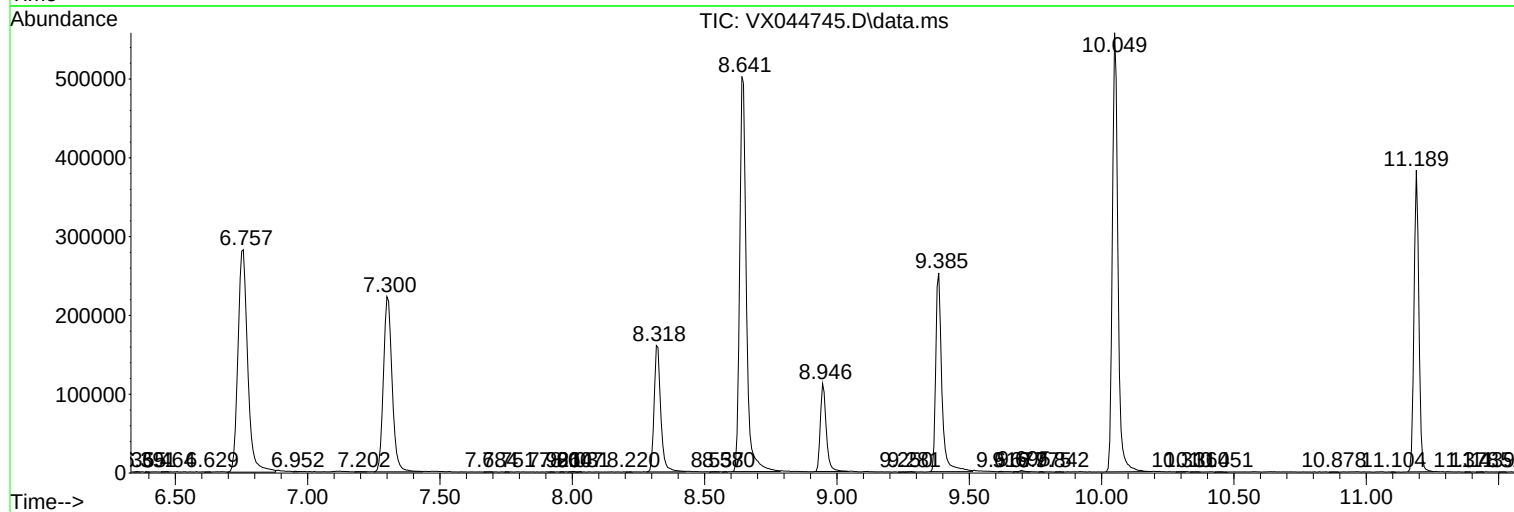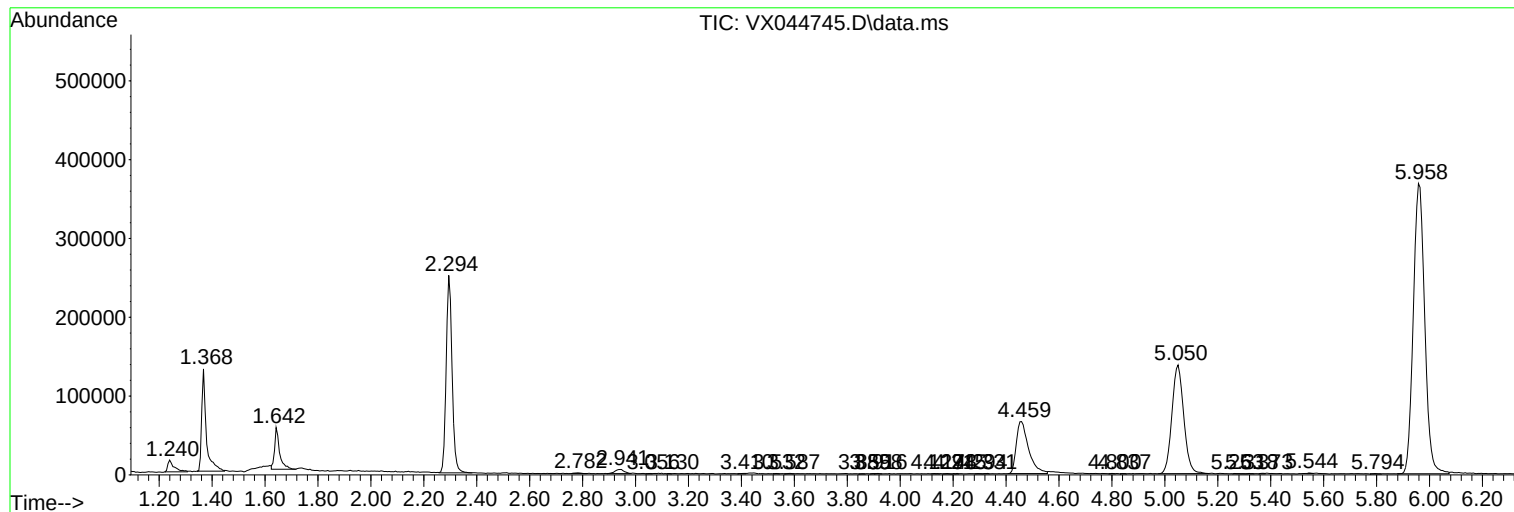

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044745.D
Acq On : 28 Jan 2025 15:29
Operator : JC/MD
Sample : VX0128WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK754

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044745.D
Acq On : 28 Jan 2025 15:29
Operator : JC/MD
Sample : VX0128WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK754

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc