

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044747.D
 Acq On : 28 Jan 2025 16:21
 Operator : JC/MD
 Sample : VIBLK691
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK691

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

Signal : TIC: VX044747.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	40	rBV	15114	28858	2.47%	0.349%
2	1.368	42	46	58	rVV	155657	178646	15.28%	2.160%
3	1.642	88	91	104	rVB	58089	78599	6.72%	0.950%
4	2.294	192	198	209	rVB	265320	413635	35.38%	5.001%
5	2.782	272	278	284	rVB3	1246	2233	0.19%	0.027%
6	2.849	286	289	291	rBV	462	466	0.04%	0.006%
7	2.940	298	304	315	rVB2	4927	11931	1.02%	0.144%
8	3.081	323	327	330	rBV3	1244	1833	0.16%	0.022%
9	3.148	336	338	340	rBB	324	324	0.03%	0.004%
10	3.227	349	351	354	rBV2	454	556	0.05%	0.007%
11	3.349	369	371	373	rVV2	401	279	0.02%	0.003%
12	3.379	375	376	378	rBV	564	397	0.03%	0.005%
13	3.544	402	403	406	rVB	612	437	0.04%	0.005%
14	3.593	406	411	413	rBV2	390	444	0.04%	0.005%
15	3.721	431	432	435	rBV2	377	340	0.03%	0.004%
16	3.818	447	448	450	rBV	420	286	0.02%	0.003%
17	3.946	466	469	472	rBV2	262	278	0.02%	0.003%
18	3.971	472	473	476	rBV2	370	381	0.03%	0.005%
19	4.038	482	484	486	rBV	342	341	0.03%	0.004%
20	4.074	488	490	492	rBV	404	358	0.03%	0.004%
21	4.172	504	506	510	rBV	553	595	0.05%	0.007%
22	4.330	530	532	535	rVB2	348	278	0.02%	0.003%
23	4.458	545	553	569	rVV	66907	215284	18.42%	2.603%
24	5.050	639	650	670	rBV	141396	446771	38.22%	5.402%
25	5.312	692	693	696	rBV2	481	466	0.04%	0.006%
26	5.361	699	701	702	rBV	444	322	0.03%	0.004%
27	5.397	702	707	711	rBV3	881	1694	0.14%	0.020%
28	5.562	728	734	736	rBV4	916	1373	0.12%	0.017%
29	5.678	751	753	756	rBV	404	492	0.04%	0.006%
30	5.757	763	766	769	rBV2	347	412	0.04%	0.005%
31	5.964	788	800	819	rBV2	393843	1168977	100.00%	14.135%
32	6.300	854	855	858	rBV2	289	327	0.03%	0.004%
33	6.391	868	870	874	rVB3	427	368	0.03%	0.004%
34	6.617	904	907	909	rBV2	325	400	0.03%	0.005%
35	6.757	919	930	955	rBV	289162	710847	60.81%	8.595%
36	7.129	985	991	995	rBV5	1430	2724	0.23%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044747.D
 Acq On : 28 Jan 2025 16:21
 Operator : JC/MD
 Sample : VIBLK691
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK691

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

37	7.196	999	1002	1005	rBV3	419	788	0.07%	0.010%
38	7.220	1005	1006	1010	rVB3	499	280	0.02%	0.003%
39	7.306	1011	1020	1041	rBV	237419	530862	45.41%	6.419%
40	7.690	1081	1083	1087	rBV2	354	499	0.04%	0.006%
41	7.787	1098	1099	1102	rVB2	401	316	0.03%	0.004%
42	7.915	1119	1120	1124	rVB2	273	334	0.03%	0.004%
43	8.025	1136	1138	1141	rVB2	409	289	0.02%	0.003%
44	8.135	1154	1156	1158	rBV	456	330	0.03%	0.004%
45	8.196	1164	1166	1169	rBV2	408	492	0.04%	0.006%
46	8.324	1181	1187	1203	rBV	166408	287977	24.63%	3.482%
47	8.647	1232	1240	1262	rBV	567249	934192	79.92%	11.296%
48	8.945	1284	1289	1302	rBV	114822	182002	15.57%	2.201%
49	9.275	1341	1343	1347	rVB2	787	927	0.08%	0.011%
50	9.311	1347	1349	1352	rVB2	386	401	0.03%	0.005%
51	9.384	1356	1361	1382	rBV	263122	406593	34.78%	4.916%
52	9.744	1418	1420	1423	rBV	361	498	0.04%	0.006%
53	10.049	1465	1470	1490	rBV	547342	800053	68.44%	9.674%
54	10.311	1510	1513	1517	rBV3	851	1396	0.12%	0.017%
55	10.372	1522	1523	1525	rBV	294	313	0.03%	0.004%
56	10.421	1529	1531	1532	rBV	608	413	0.04%	0.005%
57	10.488	1540	1542	1545	rBV2	391	302	0.03%	0.004%
58	10.518	1545	1547	1552	rVB	387	524	0.04%	0.006%
59	10.640	1566	1567	1569	rBV2	650	508	0.04%	0.006%
60	10.665	1569	1571	1576	rVB3	697	819	0.07%	0.010%
61	10.787	1589	1591	1595	rVV2	344	344	0.03%	0.004%
62	10.848	1598	1601	1603	rVB	395	390	0.03%	0.005%
63	10.872	1603	1605	1606	rBV2	330	299	0.03%	0.004%
64	10.909	1610	1611	1614	rVB2	303	281	0.02%	0.003%
65	10.951	1617	1618	1619	rBV	609	364	0.03%	0.004%
66	11.189	1652	1657	1669	rBV	388822	501726	42.92%	6.067%
67	11.384	1687	1689	1693	rBV2	420	486	0.04%	0.006%
68	11.457	1698	1701	1707	rVB3	908	1405	0.12%	0.017%
69	11.506	1707	1709	1711	rBV2	340	320	0.03%	0.004%
70	11.543	1713	1715	1717	rBV	340	290	0.02%	0.004%
71	11.604	1721	1725	1726	rBV	371	499	0.04%	0.006%
72	11.762	1746	1751	1754	rBV2	1191	2045	0.17%	0.025%
73	11.945	1779	1781	1783	rBV	349	357	0.03%	0.004%
74	11.975	1783	1786	1788	rBV2	1306	1714	0.15%	0.021%
75	12.018	1788	1793	1803	rBV	499042	653255	55.88%	7.899%
76	12.317	1837	1842	1853	rBV	509441	656783	56.18%	7.941%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
 Data File : VX044747.D
 Acq On : 28 Jan 2025 16:21
 Operator : JC/MD
 Sample : VIBLK691
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK691

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

77	12.475	1866	1868	1870	rVB2	647	387	0.03%	0.005%
78	12.573	1882	1884	1886	rBV2	390	313	0.03%	0.004%
79	12.616	1889	1891	1893	rBV	372	366	0.03%	0.004%
80	12.762	1910	1915	1918	rBV2	885	1270	0.11%	0.015%
81	12.896	1935	1937	1940	rBV	428	372	0.03%	0.004%
82	13.054	1957	1963	1965	rBV2	297	553	0.05%	0.007%
83	13.073	1965	1966	1968	rBV	469	315	0.03%	0.004%
84	13.122	1972	1974	1977	rBV2	330	355	0.03%	0.004%
85	13.378	2014	2016	2018	rVB	514	361	0.03%	0.004%
86	13.396	2018	2019	2021	rBV	387	310	0.03%	0.004%
87	13.487	2032	2034	2037	rVB	423	325	0.03%	0.004%
88	13.542	2040	2043	2044	rBV	676	579	0.05%	0.007%
89	13.560	2044	2046	2049	rBV2	292	361	0.03%	0.004%
90	13.597	2049	2052	2058	rVB3	1743	2601	0.22%	0.031%
91	13.725	2070	2073	2076	rVB3	594	739	0.06%	0.009%
92	13.780	2078	2082	2091	rVV	6534	11740	1.00%	0.142%
93	14.134	2135	2140	2143	rVB2	1458	2070	0.18%	0.025%
94	14.304	2166	2168	2169	rBV	463	376	0.03%	0.005%
95	14.841	2254	2256	2258	rBV2	475	456	0.04%	0.006%
96	15.560	2371	2374	2375	rBV2	426	494	0.04%	0.006%
97	15.682	2391	2394	2396	rBV2	589	602	0.05%	0.007%
98	15.822	2416	2417	2420	rBV2	753	384	0.03%	0.005%
99	15.962	2438	2440	2443	rVB2	762	702	0.06%	0.008%
100	16.444	2517	2519	2521	rBV2	533	644	0.06%	0.008%

Sum of corrected areas: 8270293




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044747.D
Acq On : 28 Jan 2025 16:21
Operator : JC/MD
Sample : VIBLK691
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

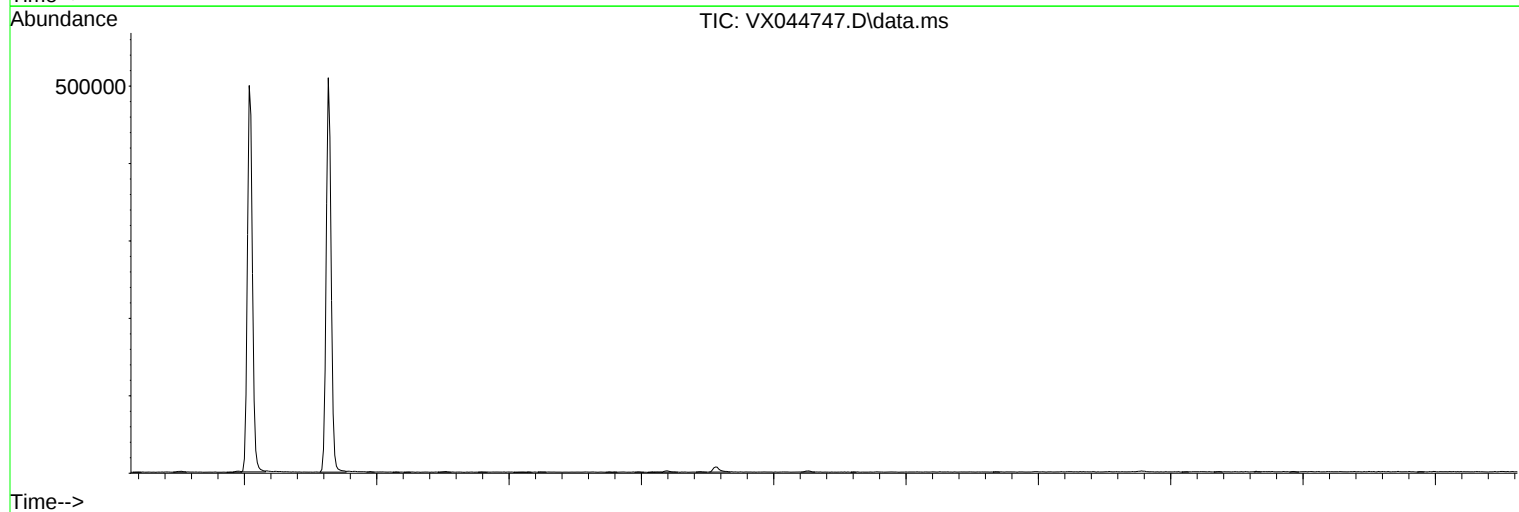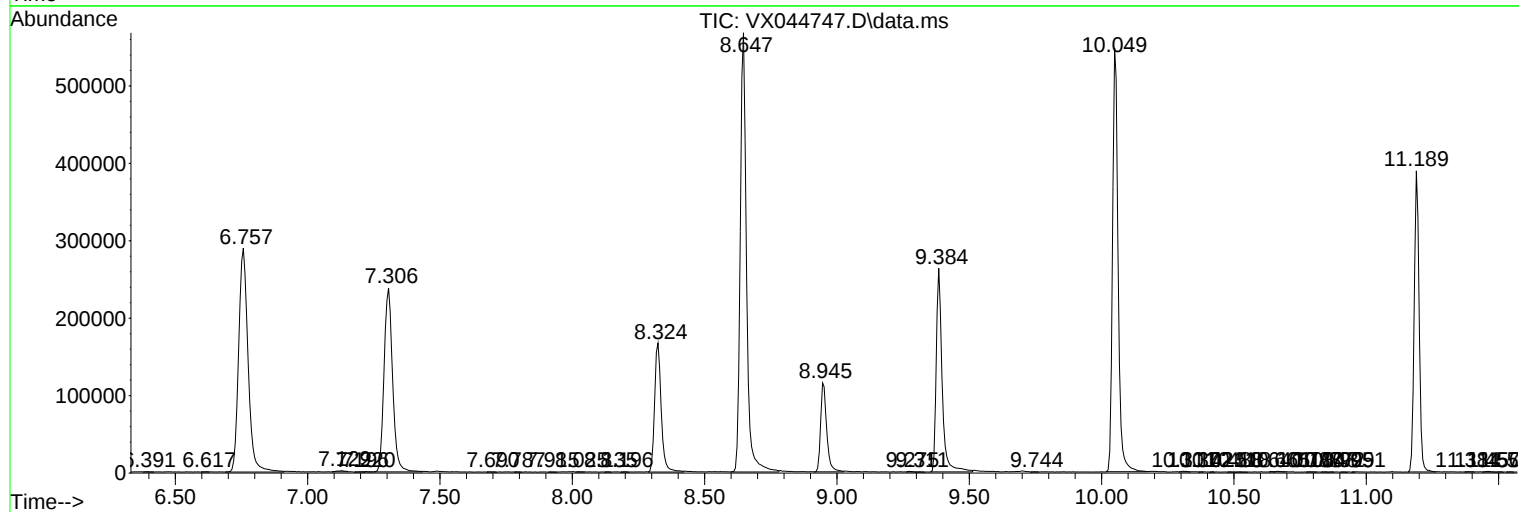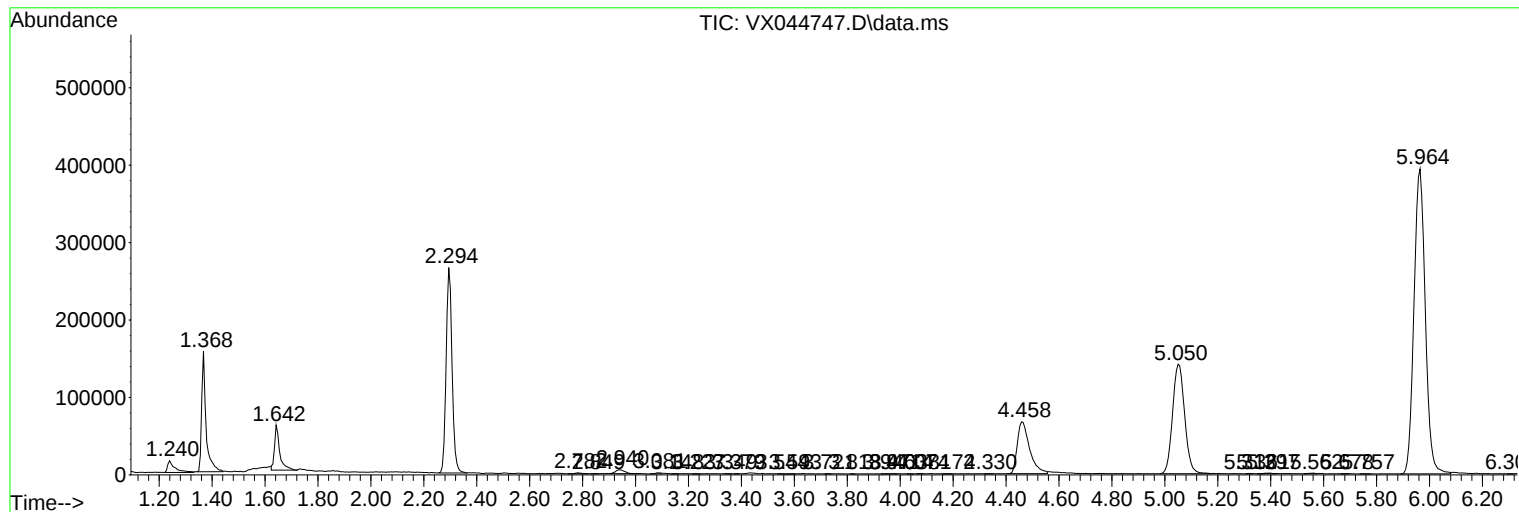

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044747.D
Acq On : 28 Jan 2025 16:21
Operator : JC/MD
Sample : VIBLK691
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044747.D
Acq On : 28 Jan 2025 16:21
Operator : JC/MD
Sample : VIBLK691
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK691

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
