
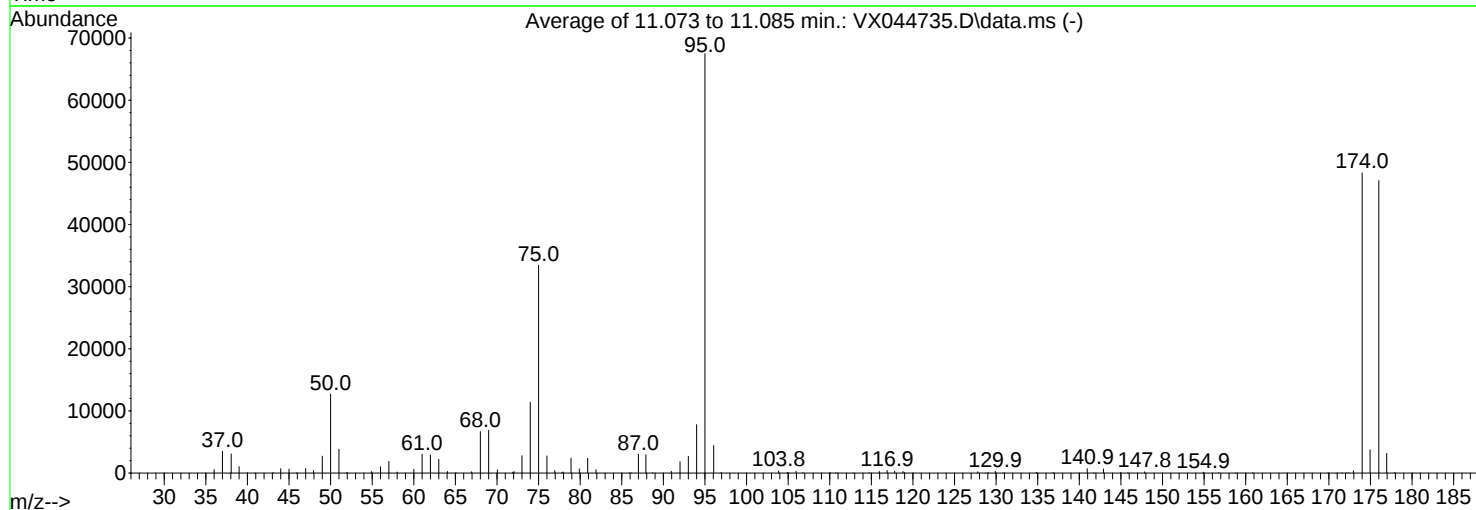


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012825\
Data File : VX044735.D
Acq On : 28 Jan 2025 08:16
Operator : JC/MD
Sample : BFB714
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB714

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM012825WMA.M
Title : VOC Analysis
Last Update : Tue Jan 28 12:04:44 2025

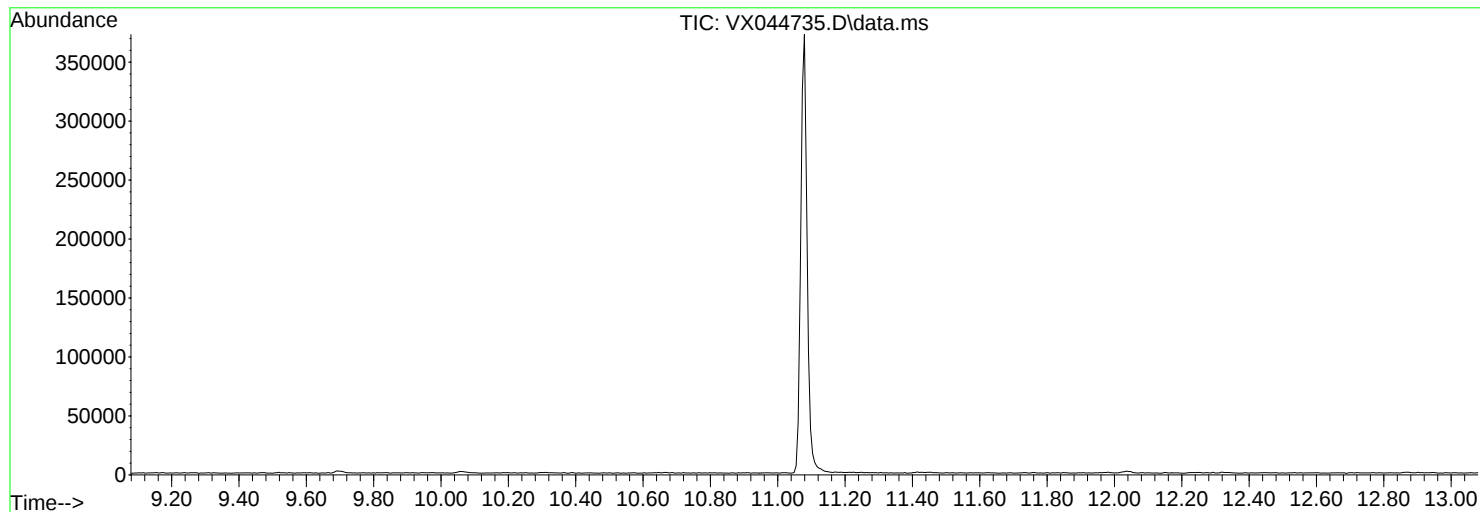

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	12691	PASS
75	95	30	80	49.6	33472	PASS
95	95	100	100	100.0	67480	PASS
96	95	5	9	6.6	4435	PASS
173	174	0.00	2	0.8	379	PASS
174	95	50	120	71.6	48304	PASS
175	174	5	9	7.7	3742	PASS
176	174	95	101	97.5	47077	PASS
177	176	5	9	6.7	3161	PASS

m/z	Abundance
39.00	63.0
40.00	1038.0
41.30	64.0
44.00	334.0

Instrument :
MSVOA_X
ClientSampleId :
BFB714

m/z	Abundance
36.00	605.0
37.00	4012.0
38.00	3510.0
39.10	1228.0
40.00	1103.0
40.90	54.0
41.20	53.0
44.00	1198.0
45.00	607.0
45.90	94.0
47.00	898.0
48.00	581.0
49.00	3156.0
50.00	14728.0
51.00	4379.0
52.00	145.0
55.00	310.0
56.00	1094.0
57.00	2080.0
58.00	149.0
60.00	722.0
61.00	3438.0
62.00	3340.0
63.00	2598.0
64.00	330.0
66.90	254.0
68.00	7440.0
69.00	7278.0
70.00	653.0
71.90	445.0
73.00	3067.0
74.00	12878.0
75.00	37400.0
76.00	3099.0
77.00	500.0
77.80	314.0
78.90	2679.0
79.90	722.0
80.90	2543.0
81.90	507.0
85.90	106.0
87.00	3149.0
87.90	3292.0
91.00	252.0
92.00	1973.0
93.00	2749.0
94.00	7948.0
95.00	71528.0
96.10	4688.0
97.00	130.0
103.90	344.0
104.90	162.0
105.90	369.0
106.80	53.0
110.10	67.0
110.70	84.0
115.90	262.0
116.90	488.0
117.80	301.0
118.80	329.0
127.80	224.0
129.10	76.0
129.90	328.0
130.80	80.0
134.80	91.0
137.00	64.0
141.00	653.0
142.90	621.0
145.00	93.0
145.90	68.0
147.90	221.0
154.90	144.0
156.80	97.0
158.80	114.0
171.60	52.0
172.40	136.0
173.00	361.0
174.00	44112.0
175.00	3570.0
176.00	43248.0
177.00	2968.0

Instrument :
MSVOA_X
ClientSampleId :
BFB714

m/z	Abundance
36.00	699.0
37.00	4093.0
38.10	3788.0
39.00	1374.0
40.00	1124.0
41.10	105.0
43.10	94.0
44.00	999.0
45.00	811.0
47.00	846.0
47.90	427.0
49.00	3201.0
50.00	15019.0
51.00	4656.0
51.90	190.0
54.80	282.0
56.00	1280.0
57.00	2067.0
58.00	193.0
60.00	660.0
61.00	3822.0
62.00	3464.0
63.00	2474.0
64.10	278.0
65.10	50.0
67.00	257.0
68.00	7743.0
69.00	8634.0
70.10	580.0
72.10	421.0
73.00	3431.0
74.00	13498.0
75.00	39200.0
76.00	3410.0
76.90	416.0
78.00	273.0
78.90	2769.0
79.90	835.0
80.90	2718.0
81.90	646.0
87.00	3668.0
87.90	3463.0
88.70	173.0
90.90	342.0
92.00	2178.0
93.00	3391.0
94.00	9351.0
95.00	79832.0
96.00	5717.0
96.90	140.0
103.80	346.0
104.90	184.0
105.90	246.0
106.80	73.0
110.10	70.0
110.90	102.0
112.80	59.0
114.70	77.0
115.90	308.0
116.90	524.0
117.80	332.0
118.80	439.0
127.80	265.0
129.00	149.0
129.90	326.0
131.00	86.0
134.90	164.0
136.80	135.0
140.90	852.0
141.70	75.0
142.90	764.0
144.90	128.0
145.80	71.0
147.80	163.0
154.90	199.0
156.70	79.0
160.90	83.0
169.90	65.0
171.00	62.0
171.60	56.0
172.10	70.0
172.90	397.0
174.00	57800.0
174.90	4278.0
176.00	55280.0
177.00	3825.0
177.90	137.0

Instrument :
MSVOA_X
ClientSampleId :
BFB714

m/z	Abundance
36.00	397.0
37.00	2418.0
38.00	1968.0
39.10	722.0
40.00	1018.0
43.10	107.0
44.00	910.0
45.00	433.0
47.10	483.0
47.90	258.0
49.10	1801.0
50.00	8327.0
51.00	2473.0
51.90	70.0
55.00	166.0
55.90	684.0
57.00	1491.0
58.00	141.0
59.90	450.0
60.90	1871.0
62.00	1940.0
63.10	1622.0
64.10	139.0
67.00	156.0
68.00	4867.0
69.00	4724.0
70.00	336.0
72.00	334.0
73.00	1868.0
74.00	7860.0
75.00	23816.0
76.00	1771.0
76.90	268.0
77.90	281.0
78.90	1777.0
79.90	445.0
80.90	1831.0
81.90	480.0
86.20	77.0
87.00	2340.0
88.00	2126.0
90.90	271.0
92.00	1330.0
92.90	1940.0
94.00	6096.0
95.00	51080.0
96.00	2900.0
97.00	128.0
103.90	329.0
105.10	77.0
106.00	300.0
106.70	80.0
110.90	60.0
114.80	79.0
116.00	259.0
116.90	279.0
117.80	244.0
119.00	210.0
127.90	140.0
128.70	52.0
129.90	189.0
134.90	121.0
136.90	78.0
140.90	617.0
141.80	74.0
142.90	607.0
145.80	112.0
147.80	218.0
154.90	126.0
160.80	79.0
169.90	61.0
172.10	106.0
173.00	380.0
174.00	43000.0
175.00	3379.0
176.00	42704.0
176.90	2691.0
177.90	58.0

Instrument :
MSVOA_X
ClientSampleId :
BFB714