


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012921\
 Data File : VX020796.D
 Acq On : 29 Jan 2021 08:48
 Operator : JC/SP
 Sample : BFB06
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB06

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXSIM012821.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jan 30 02:01:56 2021

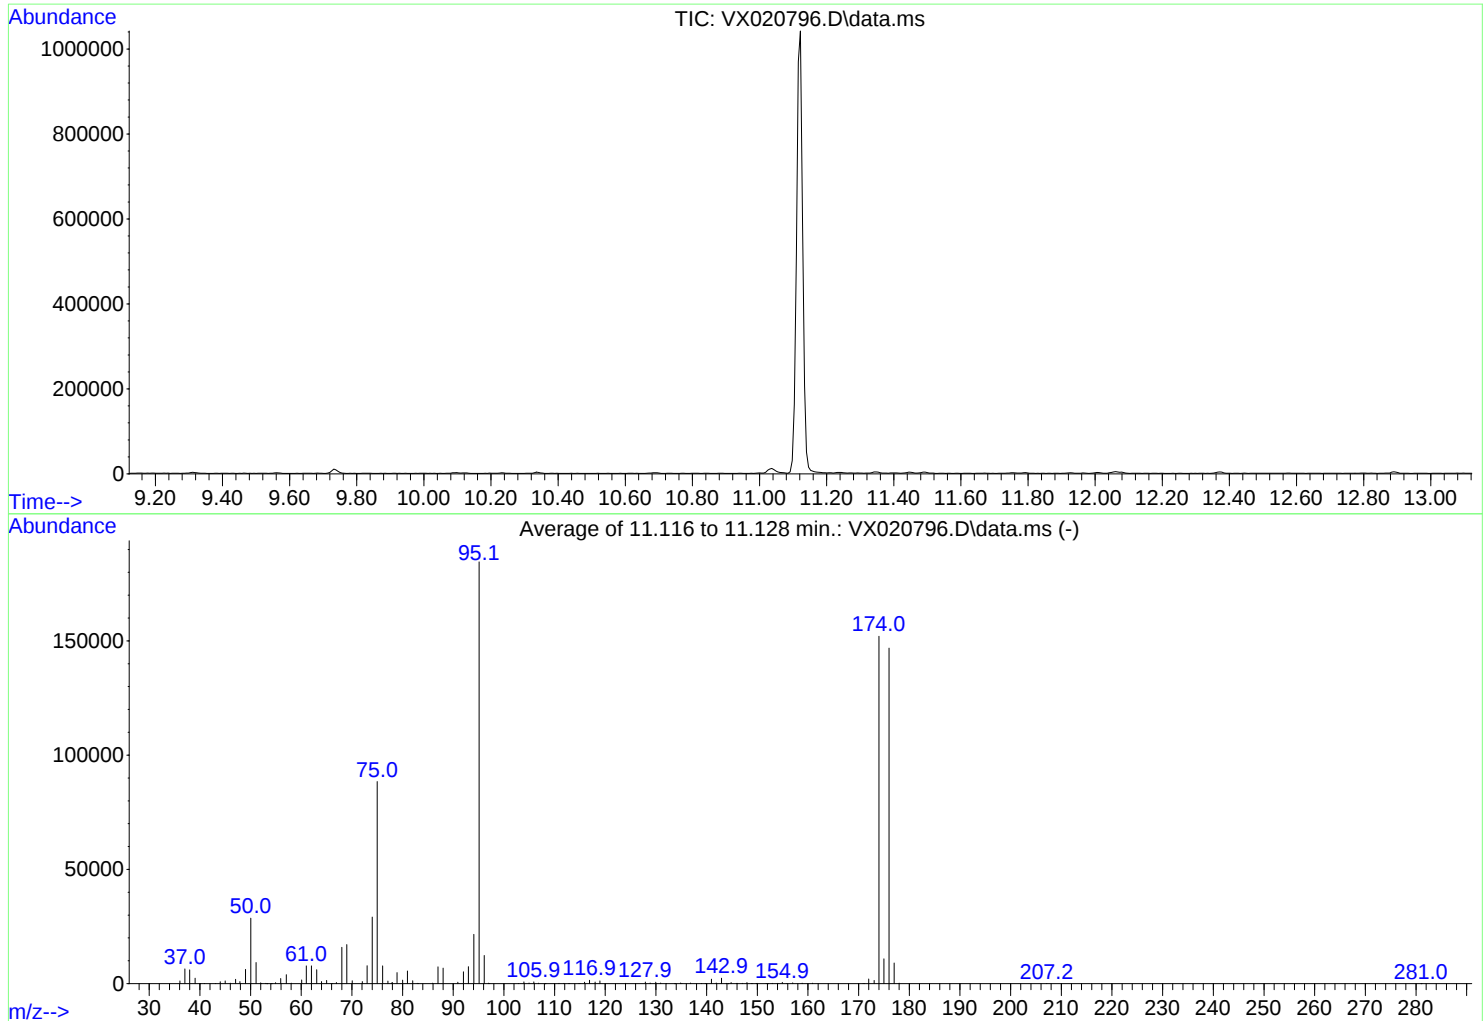

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	28629	PASS
75	95	30	80	47.9	88429	PASS
95	95	100	100	100.0	184592	PASS
96	95	5	9	6.7	12349	PASS
173	174	0.00	2	0.9	1425	PASS
174	95	50	120	82.4	152045	PASS
175	174	5	9	7.2	10885	PASS
176	174	95	101	96.6	146803	PASS
177	176	5	9	6.2	9059	PASS

m/z	Abundance
36.00	1220.0
37.00	8535.0
38.00	7681.0
39.10	3435.0
39.90	611.0
40.90	64.0
43.10	80.0
44.00	1689.0
45.10	1454.0
46.00	293.0
47.00	2325.0
47.90	1330.0
49.00	8243.0
50.10	36336.0
51.10	11751.0
52.00	550.0
53.00	191.0
54.10	66.0
55.00	565.0
56.00	2861.0
57.00	4966.0
58.10	193.0
60.10	2182.0
61.00	9410.0
62.00	9826.0
63.00	7553.0
64.00	1125.0
65.00	1711.0
65.90	204.0
66.30	143.0
66.90	585.0
68.00	18128.0
69.00	19880.0
70.10	1486.0
72.00	1011.0
73.00	9213.0
74.00	35048.0
75.00	107448.0
76.10	9581.0
77.10	1330.0
77.80	815.0
78.90	5559.0
80.00	1841.0
80.90	6552.0
82.00	1492.0
82.90	212.0
86.00	305.0
87.00	8549.0
88.00	8008.0
90.90	771.0
92.00	6273.0
93.00	8865.0
94.00	25256.0
95.10	211968.0
96.10	14647.0
96.90	320.0
103.00	127.0
103.90	772.0
105.00	370.0
105.90	977.0
106.90	179.0
108.10	50.0
110.00	114.0
110.90	123.0
111.80	176.0
112.80	171.0
114.80	200.0
115.90	753.0
116.90	1692.0
118.00	804.0
118.90	1218.0
124.00	146.0
126.00	58.0
127.90	596.0
129.00	216.0
129.90	654.0
131.00	275.0
133.70	57.0
134.80	351.0
136.90	405.0
139.00	119.0
139.70	107.0
140.90	2006.0
141.90	217.0
143.00	2506.0
144.00	192.0
144.80	584.0
145.90	257.0
147.00	146.0
148.10	510.0
148.80	85.0
149.20	139.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

149.80	174.0
151.70	136.0
153.00	168.0
154.10	130.0
154.90	548.0
155.90	73.0
157.10	415.0
158.90	246.0
160.90	240.0
170.00	64.0
170.90	236.0
172.00	2216.0
173.10	1496.0
174.00	151936.0
175.00	11109.0
176.00	142080.0
177.00	9512.0
178.00	235.0
207.20	95.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

m/z	Abundance
36.10	1614.0
37.10	7196.0
38.00	7104.0
39.10	2554.0
40.00	520.0
40.90	121.0
43.10	86.0
44.00	1749.0
45.00	1687.0
46.00	200.0
47.10	2249.0
47.90	870.0
49.00	7203.0
50.00	33104.0
51.10	10446.0
52.00	494.0
53.00	238.0
54.90	418.0
56.00	2617.0
57.10	5309.0
58.00	246.0
60.10	1690.0
61.00	9298.0
62.00	9032.0
63.10	6996.0
64.00	1084.0
65.00	1611.0
66.10	144.0
67.00	479.0
68.00	19232.0
69.00	21048.0
70.00	1654.0
72.10	1216.0
73.00	9365.0
74.00	33952.0
75.00	103136.0
76.00	9099.0
77.10	1191.0
78.00	989.0
78.90	5962.0
80.00	1893.0
81.00	6646.0
82.00	1572.0
82.90	161.0
86.00	272.0
87.00	9049.0
88.00	8515.0
90.90	721.0
92.00	5870.0
93.00	8644.0
94.10	25576.0
95.10	219264.0
96.10	14611.0
97.00	388.0
102.80	112.0
103.90	907.0
104.90	303.0
105.90	826.0
106.90	179.0
109.90	133.0
110.80	274.0
111.90	181.0
113.00	175.0
115.00	206.0
115.90	802.0
116.90	1884.0
118.00	770.0
118.90	1414.0
123.90	104.0
125.90	89.0
127.90	994.0
128.80	444.0
130.00	741.0
130.90	189.0
132.10	54.0
134.90	435.0
136.80	308.0
139.00	76.0
140.00	152.0
140.90	2417.0
141.90	413.0
142.90	3153.0
143.90	130.0
144.90	667.0
146.10	456.0
147.00	148.0
147.90	614.0
149.00	180.0
150.00	261.0
151.80	109.0
152.90	230.0
153.90	156.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

155.00	669.0
155.80	102.0
156.90	388.0
158.80	198.0
160.80	245.0
170.00	100.0
171.10	142.0
172.00	2153.0
173.00	1782.0
174.00	186560.0
175.00	13953.0
176.00	177984.0
177.00	10521.0
178.00	389.0
207.10	80.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

m/z	Abundance
36.10	668.0
37.10	3600.0
38.00	3257.0
39.00	1394.0
40.00	583.0
41.10	71.0
43.10	138.0
44.00	1310.0
45.00	924.0
46.10	135.0
47.00	1069.0
47.90	529.0
49.00	3308.0
50.00	16448.0
51.10	5530.0
52.20	300.0
53.20	96.0
55.10	196.0
56.00	1382.0
57.00	2700.0
58.10	122.0
60.00	961.0
61.00	4666.0
62.10	4481.0
63.10	3666.0
64.00	572.0
65.00	990.0
66.90	346.0
68.10	10360.0
69.00	10300.0
70.10	763.0
72.10	527.0
73.00	4963.0
74.10	18400.0
75.00	54704.0
76.00	4658.0
77.10	780.0
78.00	553.0
78.90	2919.0
79.90	959.0
80.90	3322.0
81.90	779.0
83.10	193.0
85.80	142.0
87.00	4782.0
87.90	3964.0
90.90	424.0
92.00	3383.0
93.00	4815.0
94.00	13795.0
95.00	122544.0
96.00	7788.0
97.20	234.0
104.00	611.0
105.00	153.0
106.00	522.0
106.80	195.0
110.80	90.0
111.90	154.0
112.90	135.0
115.00	121.0
116.00	395.0
116.90	928.0
117.90	447.0
119.00	901.0
124.00	97.0
127.90	542.0
128.80	250.0
129.90	481.0
131.00	323.0
132.00	65.0
135.10	340.0
136.90	241.0
139.10	61.0
139.80	91.0
141.00	1569.0
141.90	195.0
143.00	1482.0
143.80	84.0
144.20	110.0
144.90	262.0
145.90	271.0
147.10	158.0
147.80	362.0
148.90	73.0
149.90	208.0
152.00	63.0
153.00	119.0
154.10	110.0
155.00	432.0
157.00	266.0
158.90	194.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

161.00	194.0
171.10	145.0
172.00	1745.0
173.00	998.0
174.00	117640.0
175.00	7594.0
176.00	120344.0
177.00	7144.0
281.00	66.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

m/z	Abundance
39.00	70.0
40.00	535.0
41.20	270.0
42.00	127.0
44.00	723.0
45.00	192.0
55.90	74.0
57.10	410.0
87.10	71.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06