

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
 Data File : VX044758.D
 Acq On : 29 Jan 2025 10:34
 Operator : JC/MD
 Sample : VX0129WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 30 07:48:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 28 12:04:44 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	315595	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	274779	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	116059	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	105050	44.220	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	88.440%	
7) Chloroethane-d5	1.642	69	35756	39.619	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.240%	
11) 1,1-Dichloroethene-d2	2.294	65	46274	45.570	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.140%	
21) 2-Butanone-d5	4.452	46	122798	120.913	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	120.910%	
24) Chloroform-d	5.050	84	185387	44.410	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.820%	
26) 1,2-Dichloroethane-d4	5.946	65	116041	46.311	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.620%	
32) Benzene-d6	5.964	84	397120	46.221	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.440%	
36) 1,2-Dichloropropane-d6	7.299	67	128108	47.108	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.220%	
41) Toluene-d8	8.640	98	358462	47.140	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	94.280%	
43) trans-1,3-Dichloroprop...	8.945	79	59595	46.199	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	92.400%	
47) 2-Hexanone-d5	9.384	63	77617	96.438	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	96.440%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	163983	48.525	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	97.040%	
66) 1,2-Dichlorobenzene-d4	12.317	152	110315	48.578	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.160%	
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	15685	6.121	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
Data File : VX044758.D
Acq On : 29 Jan 2025 10:34
Operator : JC/MD
Sample : VX0129WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 30 07:48:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 12:04:44 2025
Response via : Initial Calibration

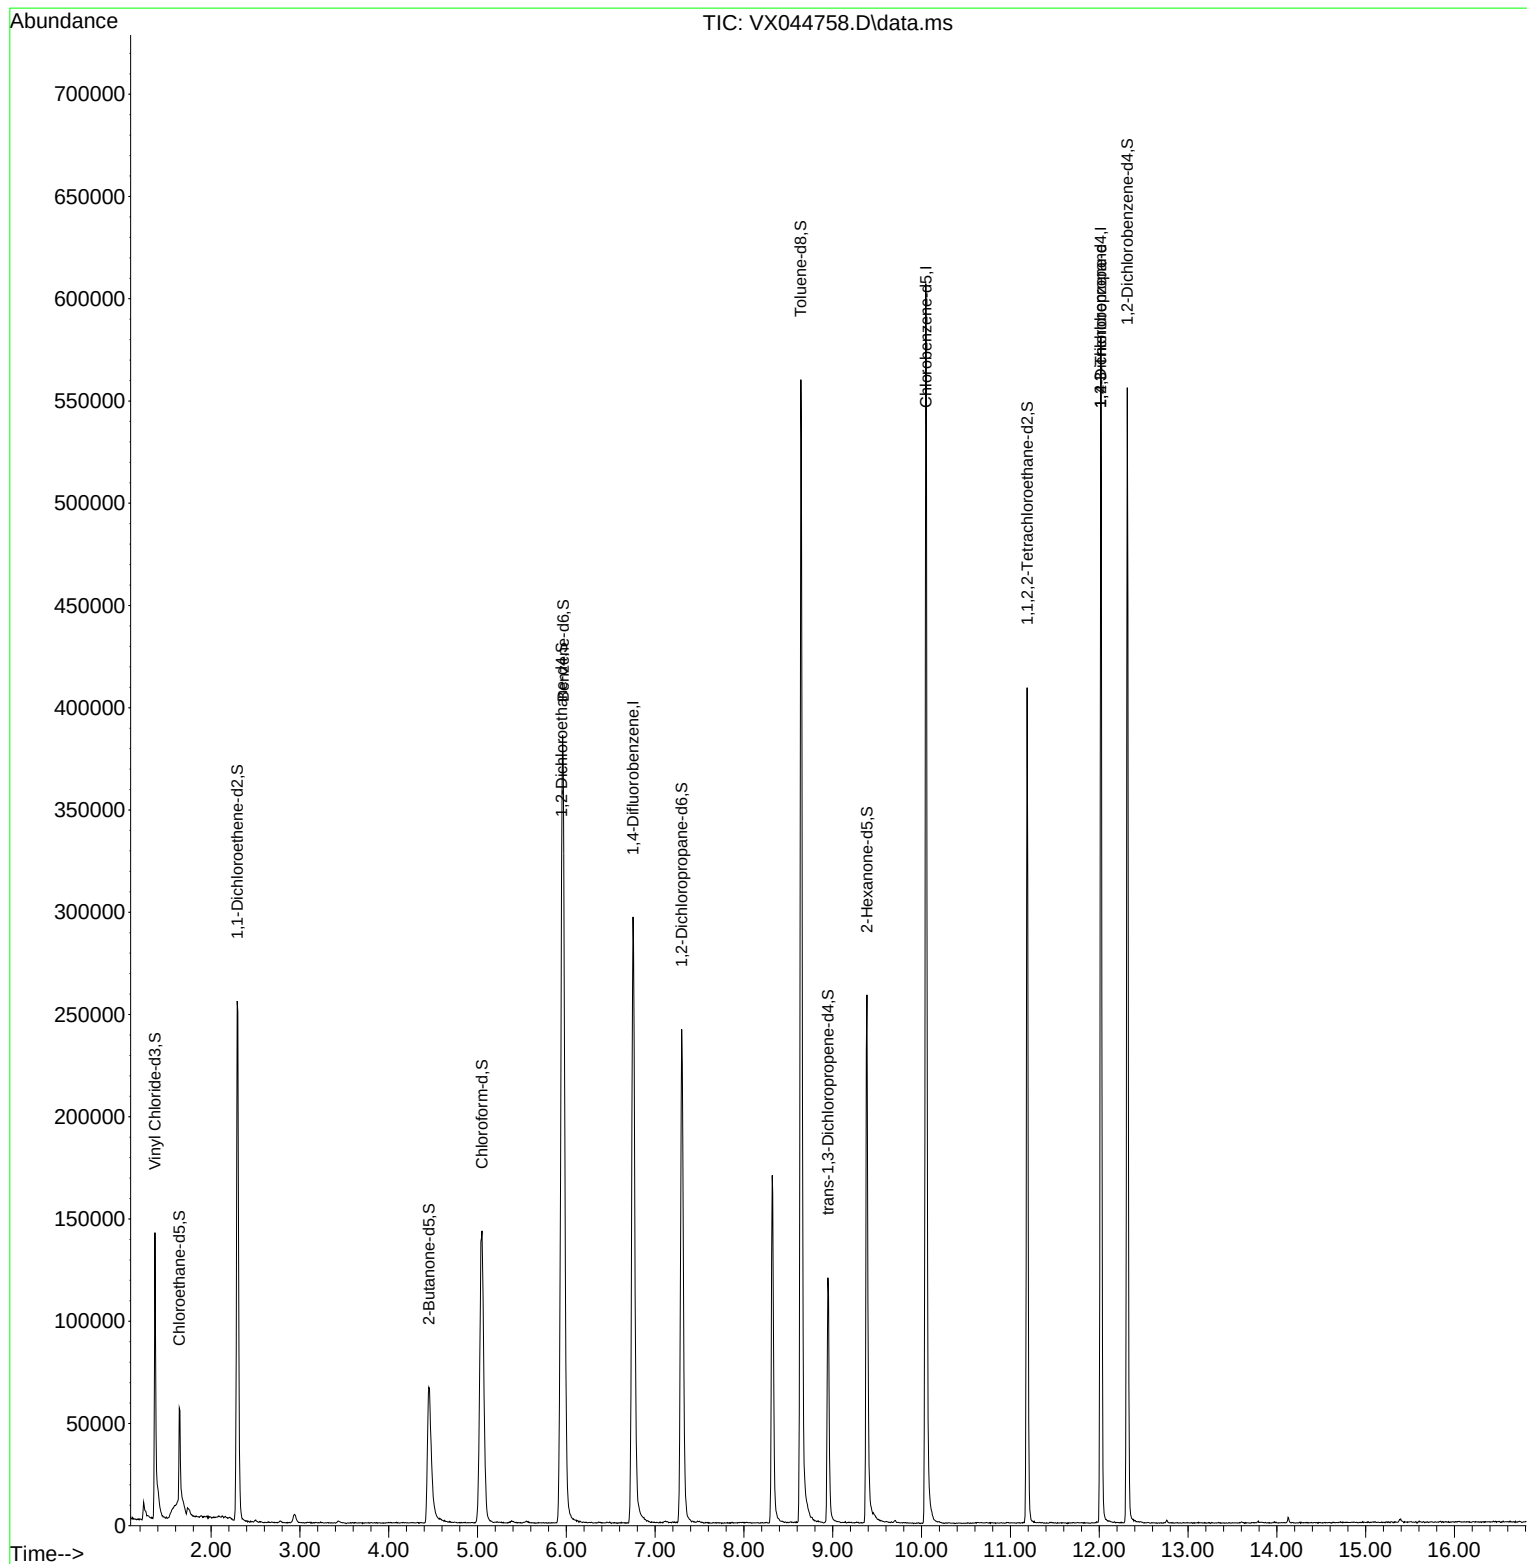

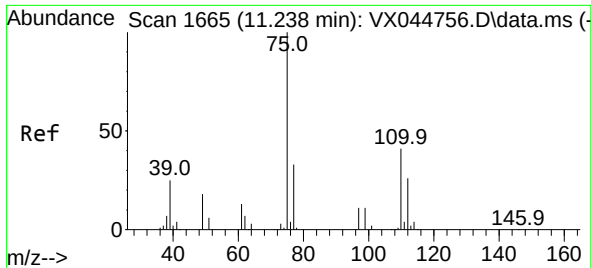

#61
1,2,3-Trichloropropane
Concen: 6.121 ug/L
RT: 12.018 min Scan# 11
Delta R.T. 0.780 min
Lab File: VX044758.D
Acq: 29 Jan 2025 10:34

Instrument :
MSVOA_X
ClientSampleId :

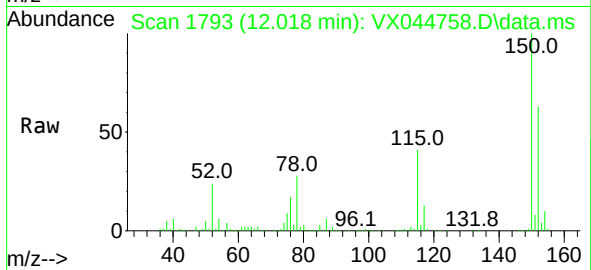

Tgt Ion: 75 Resp: 15685
Ion Ratio Lower Upper
75 100
77 30.5 25.8 38.6
110 2.6 30.8 46.2#

