

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
 Data File : VX044759.D
 Acq On : 29 Jan 2025 11:02
 Operator : JC/MD
 Sample : Q1190-20
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 30 07:48:41 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 28 12:04:44 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	305666	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	272026	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	121404	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	54741	23.791	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	47.580%#
7) Chloroethane-d5	1.648	69	8341	9.542	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	19.080%#
11) 1,1-Dichloroethene-d2	2.276	65	35936	36.539	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.080%
21) 2-Butanone-d5	4.483	46	92352	93.889	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.890%
24) Chloroform-d	5.050	84	164362	40.652	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.300%
26) 1,2-Dichloroethane-d4	5.946	65	104588	43.096	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.200%
32) Benzene-d6	5.958	84	362850	42.660	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.320%
36) 1,2-Dichloropropane-d6	7.300	67	112790	41.895	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.780%
41) Toluene-d8	8.641	98	325660	43.260	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.520%
43) trans-1,3-Dichloroprop...	8.946	79	52510	41.119	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.240%
47) 2-Hexanone-d5	9.391	63	65040	81.629	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.630%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	143653	42.939	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.880%
66) 1,2-Dichlorobenzene-d4	12.317	152	107419	45.220	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.440%
Target Compounds						
37) 1,2-Dichloropropane	7.300	63	11813	4.872	ug/L	Qvalue # 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
Data File : VX044759.D
Acq On : 29 Jan 2025 11:02
Operator : JC/MD
Sample : Q1190-20
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 30 07:48:41 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 12:04:44 2025
Response via : Initial Calibration

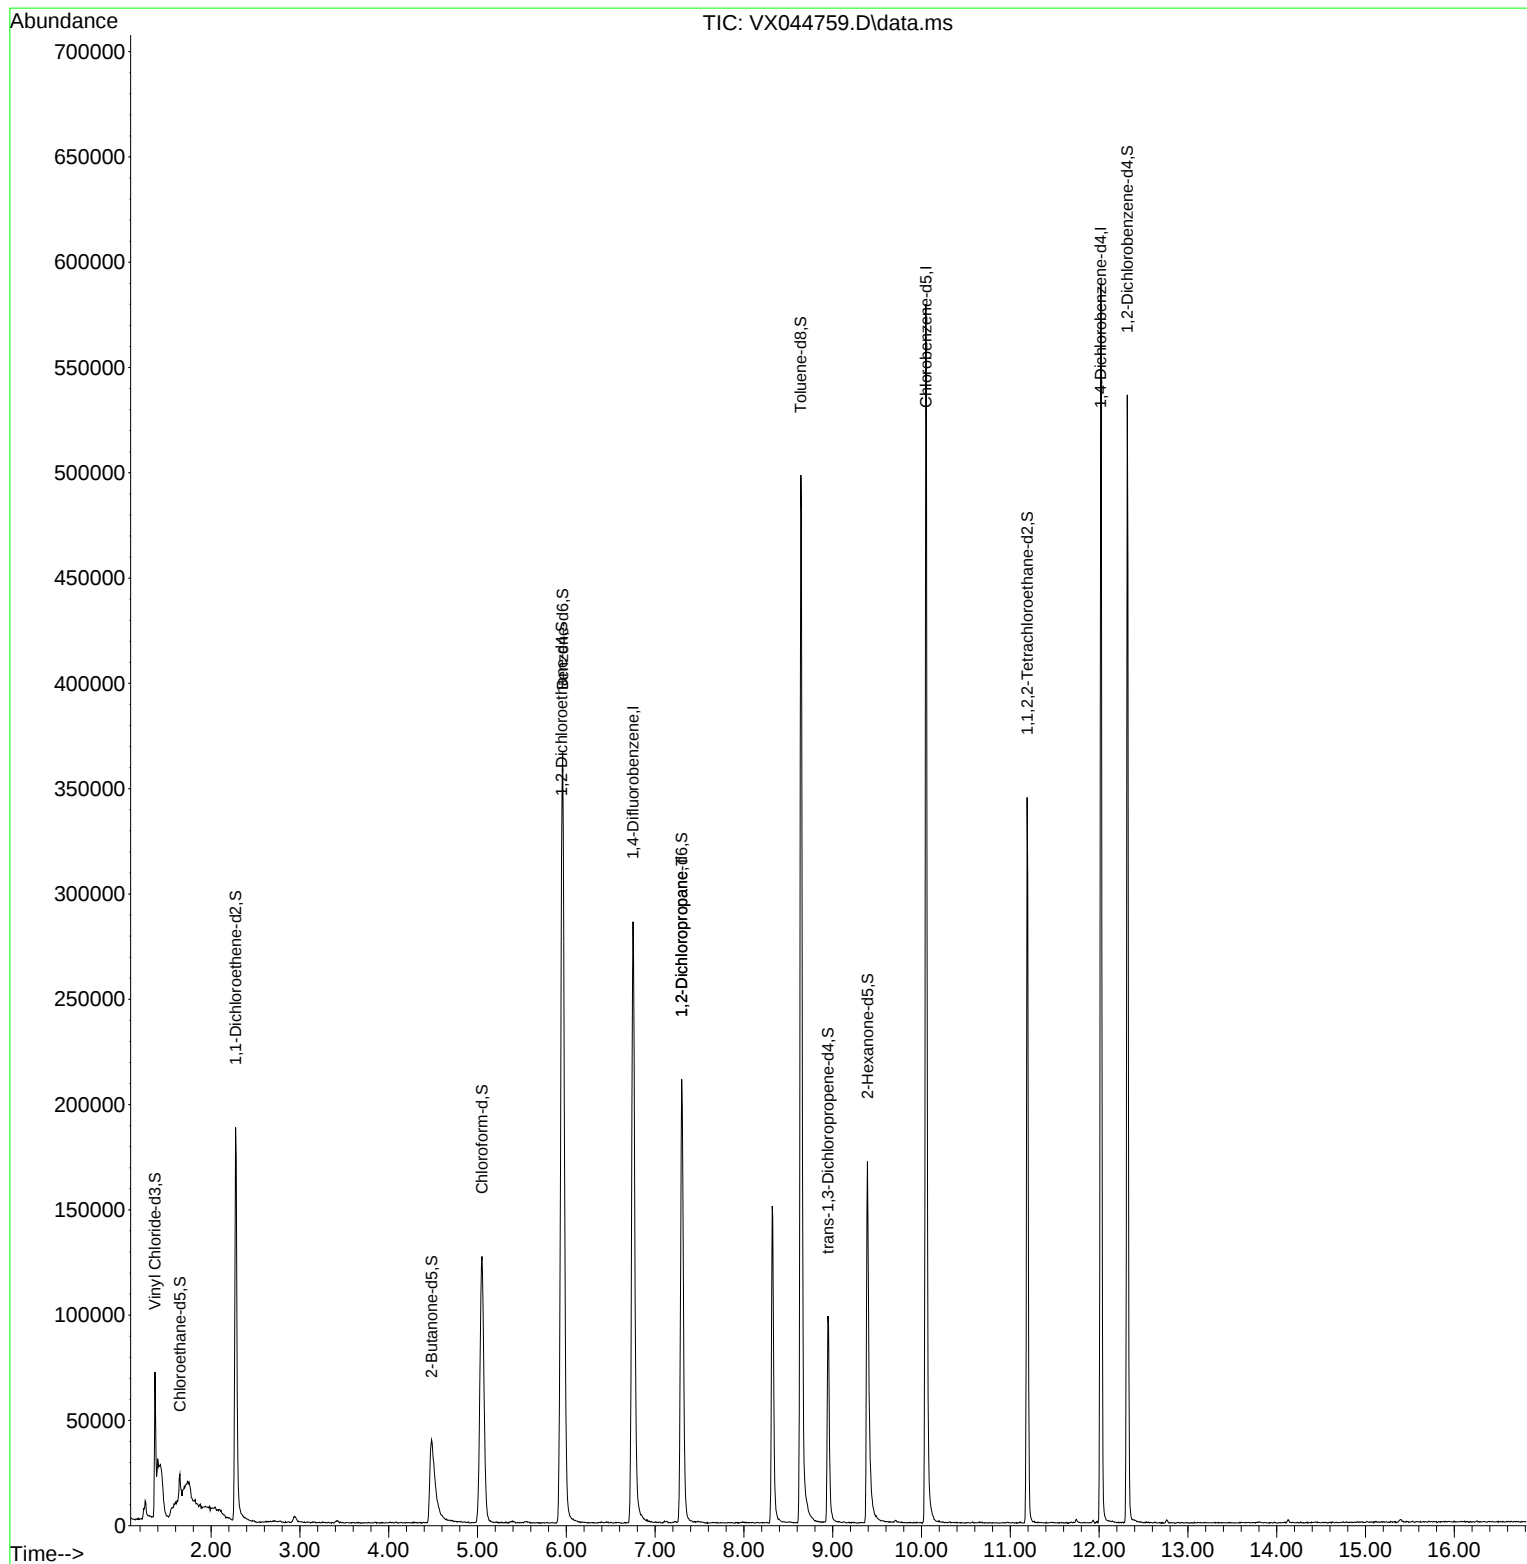

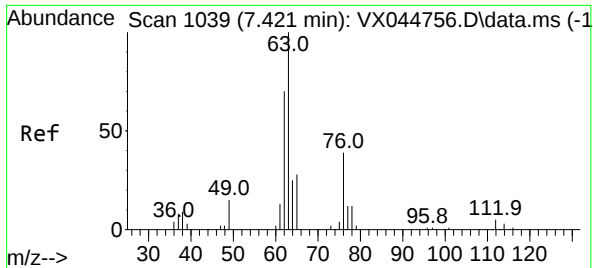

#37
1,2-Dichloropropane
Concen: 4.872 ug/L
RT: 7.300 min Scan# 10
Delta R.T. -0.122 min
Lab File: VX044759.D
Acq: 29 Jan 2025 11:02

Instrument :
MSVOA_X
ClientSampleId :

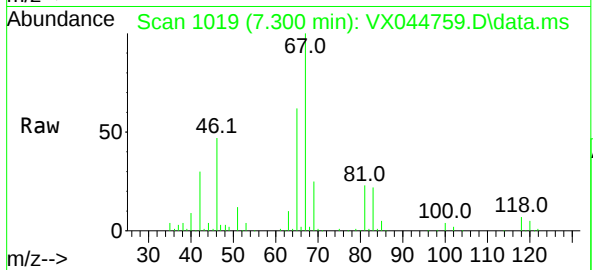

Tgt Ion: 63 Resp: 11813
Ion Ratio Lower Upper
63 100
112 0.0 3.5 5.3#

