

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
 Data File : VX044766.D
 Acq On : 29 Jan 2025 13:43
 Operator : JC/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jan 30 07:49:30 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 28 12:04:44 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	287713	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	242513	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	98175	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	80086	36.979	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	73.960%	
7) Chloroethane-d5	1.648	69	34390	41.799	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	83.600%	
11) 1,1-Dichloroethene-d2	2.300	65	38005	41.054	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.100%	
21) 2-Butanone-d5	4.458	46	118940	128.464	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	128.460%	
24) Chloroform-d	5.056	84	166685	43.799	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.600%	
26) 1,2-Dichloroethane-d4	5.952	65	109159	47.786	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.580%	
32) Benzene-d6	5.970	84	351761	46.389	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.780%	
36) 1,2-Dichloropropane-d6	7.306	67	115022	47.923	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	95.840%	
41) Toluene-d8	8.647	98	294826	43.930	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	87.860%	
43) trans-1,3-Dichloroprop...	8.945	79	52212	45.861	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.720%	
47) 2-Hexanone-d5	9.384	63	77498	109.101	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	109.100%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	150694	50.525	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	101.060%	
66) 1,2-Dichlorobenzene-d4	12.317	152	92248	48.022	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.040%	
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	13376	6.171	ug/L	Qvalue # 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
Data File : VX044766.D
Acq On : 29 Jan 2025 13:43
Operator : JC/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jan 30 07:49:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 12:04:44 2025
Response via : Initial Calibration

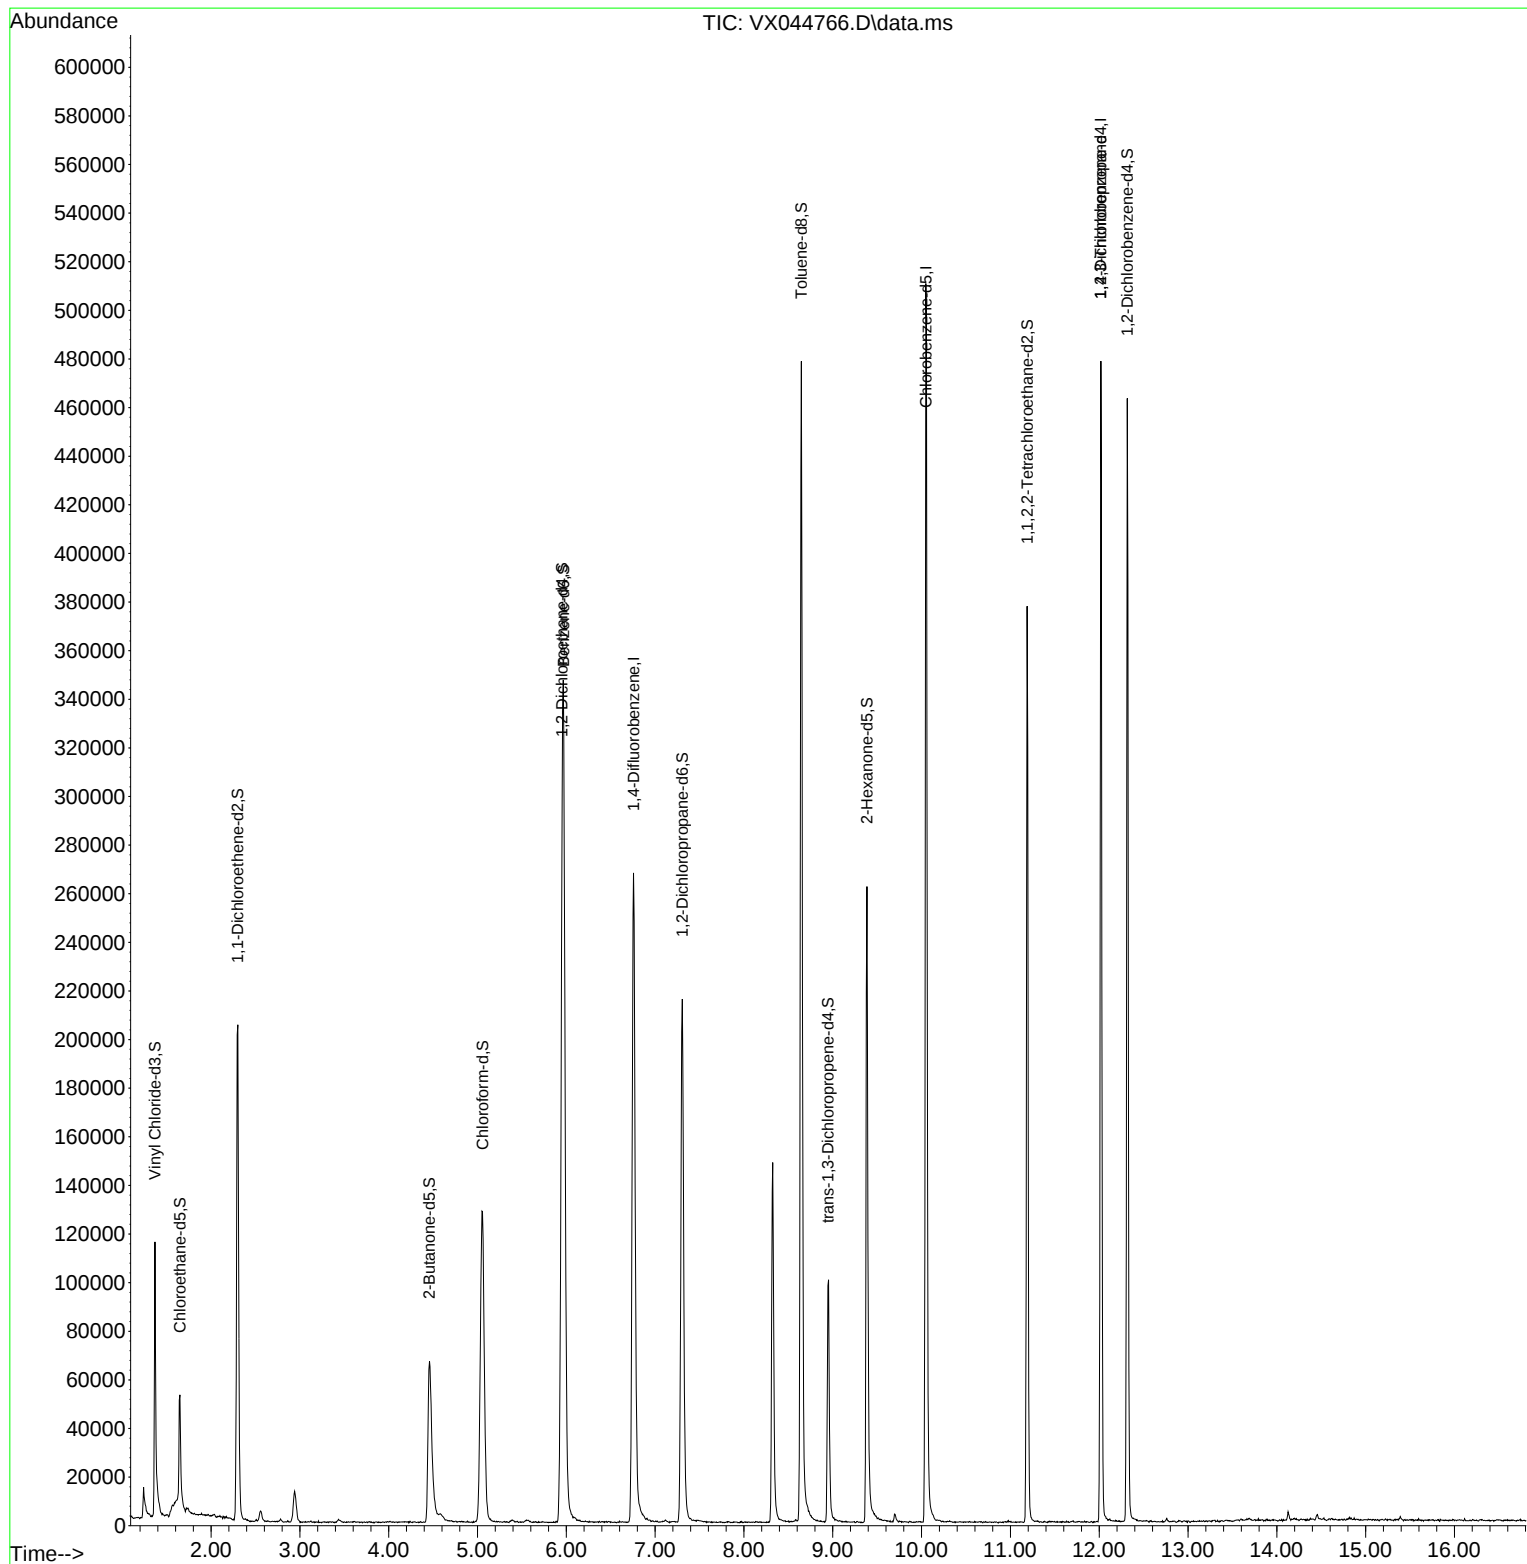

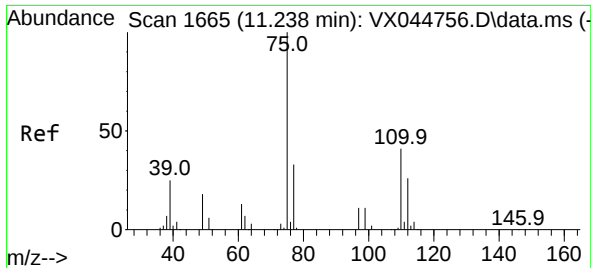

#61
1,2,3-Trichloropropane
Concen: 6.171 ug/L
RT: 12.018 min Scan# 11
Delta R.T. 0.780 min
Lab File: VX044766.D
Acq: 29 Jan 2025 13:43

Instrument :
MSVOA_X
ClientSampleId :

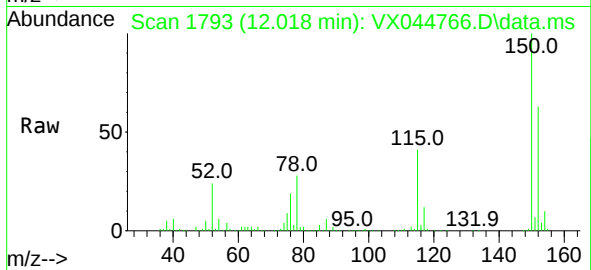

Tgt Ion: 75	Resp:	13376
Ion	Ratio	Lower Upper
75	100	
77	32.0	25.8 38.6
110	2.6	30.8 46.2#

