

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
 Data File : VX044758.D
 Acq On : 29 Jan 2025 10:34
 Operator : JC/MD
 Sample : VX0129WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK756

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

Signal : TIC: VX044758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	31	rBV2	8713	14746	1.27%	0.174%
2	1.367	42	46	61	rBV	139843	172847	14.92%	2.041%
3	1.642	88	91	104	rVB	51928	79834	6.89%	0.942%
4	2.294	192	198	213	rVB	254338	409608	35.36%	4.836%
5	2.440	221	222	223	rBV	552	247	0.02%	0.003%
6	2.940	296	304	315	rBV2	4142	10402	0.90%	0.123%
7	3.172	340	342	343	rBV	351	238	0.02%	0.003%
8	3.233	350	352	353	rBV2	469	243	0.02%	0.003%
9	3.428	380	384	392	rBV3	1052	2433	0.21%	0.029%
10	3.544	399	403	404	rBV2	390	469	0.04%	0.006%
11	3.568	405	407	409	rVV2	424	306	0.03%	0.004%
12	3.593	409	411	412	rVV2	408	304	0.03%	0.004%
13	3.611	412	414	415	rVB	365	201	0.02%	0.002%
14	3.708	429	430	431	rBV	394	192	0.02%	0.002%
15	3.806	443	446	448	rBV2	338	368	0.03%	0.004%
16	3.861	454	455	457	rVB	397	227	0.02%	0.003%
17	3.958	469	471	472	rBV2	221	195	0.02%	0.002%
18	4.452	544	552	571	rBV	66260	213304	18.41%	2.518%
19	5.050	637	650	665	rBV	142806	451221	38.95%	5.327%
20	5.550	724	732	734	rBV3	1012	2050	0.18%	0.024%
21	5.958	788	799	818	rBV2	385097	1158397	100.00%	13.676%
22	6.360	864	865	870	rVB4	457	637	0.05%	0.008%
23	6.488	884	886	889	rVB3	759	688	0.06%	0.008%
24	6.519	889	891	892	rBV	352	356	0.03%	0.004%
25	6.598	901	904	905	rBV2	347	420	0.04%	0.005%
26	6.616	905	907	908	rVB	459	196	0.02%	0.002%
27	6.635	908	910	911	rBV2	234	203	0.02%	0.002%
28	6.683	916	918	920	rBV2	345	254	0.02%	0.003%
29	6.751	920	929	951	rBV	296490	734250	63.39%	8.668%
30	6.958	961	963	964	rBV2	419	243	0.02%	0.003%
31	7.055	977	979	980	rBV2	593	401	0.03%	0.005%
32	7.116	984	989	991	rBV4	986	1772	0.15%	0.021%
33	7.196	1000	1002	1004	rBV3	405	361	0.03%	0.004%
34	7.244	1008	1010	1011	rBV	431	218	0.02%	0.003%
35	7.299	1011	1019	1037	rBV	241327	535090	46.19%	6.317%
36	7.476	1046	1048	1050	rBV2	600	541	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
 Data File : VX044758.D
 Acq On : 29 Jan 2025 10:34
 Operator : JC/MD
 Sample : VX0129WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK756

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

37	7.567	1062	1063	1065	rBV	372	301	0.03%	0.004%
38	7.659	1074	1078	1081	rBV2	340	460	0.04%	0.005%
39	7.763	1093	1095	1097	rBV	378	380	0.03%	0.004%
40	7.781	1097	1098	1099	rVV	370	193	0.02%	0.002%
41	7.866	1110	1112	1114	rBV2	456	332	0.03%	0.004%
42	8.189	1163	1165	1166	rBV	324	220	0.02%	0.003%
43	8.317	1180	1186	1203	rBV	170039	297503	25.68%	3.512%
44	8.640	1233	1239	1258	rBV	558696	946790	81.73%	11.178%
45	8.945	1284	1289	1308	rBV	119599	186834	16.13%	2.206%
46	9.140	1319	1321	1323	rVB	729	482	0.04%	0.006%
47	9.177	1323	1327	1328	rBV2	369	430	0.04%	0.005%
48	9.384	1356	1361	1372	rBV	257932	397176	34.29%	4.689%
49	9.659	1404	1406	1409	rBV3	462	375	0.03%	0.004%
50	9.896	1444	1445	1447	rVB	377	225	0.02%	0.003%
51	9.963	1455	1456	1460	rVB2	519	451	0.04%	0.005%
52	9.994	1460	1461	1464	rBV2	329	391	0.03%	0.005%
53	10.049	1465	1470	1489	rBV	605912	875026	75.54%	10.330%
54	10.268	1504	1506	1507	rBV2	319	241	0.02%	0.003%
55	10.299	1509	1511	1516	rVB4	324	437	0.04%	0.005%
56	10.390	1524	1526	1529	rBV2	280	336	0.03%	0.004%
57	10.518	1546	1547	1550	rVB2	358	313	0.03%	0.004%
58	10.610	1560	1562	1563	rVB	454	255	0.02%	0.003%
59	10.628	1563	1565	1569	rBV3	484	851	0.07%	0.010%
60	10.768	1586	1588	1589	rVB	402	229	0.02%	0.003%
61	10.853	1600	1602	1606	rVB	210	207	0.02%	0.002%
62	10.957	1618	1619	1622	rBV2	340	374	0.03%	0.004%
63	11.006	1625	1627	1630	rBV2	229	222	0.02%	0.003%
64	11.134	1644	1648	1649	rBV	394	442	0.04%	0.005%
65	11.189	1652	1657	1669	rVV	408408	517463	44.67%	6.109%
66	11.445	1697	1699	1700	rBV2	413	299	0.03%	0.004%
67	11.506	1707	1709	1711	rVB	345	269	0.02%	0.003%
68	11.530	1711	1713	1716	rBV2	362	281	0.02%	0.003%
69	11.585	1721	1722	1726	rBV	330	471	0.04%	0.006%
70	11.652	1732	1733	1734	rBV	483	254	0.02%	0.003%
71	11.670	1734	1736	1738	rBV2	248	186	0.02%	0.002%
72	11.914	1774	1776	1779	rBV	320	452	0.04%	0.005%
73	11.969	1784	1785	1788	rBV2	535	540	0.05%	0.006%
74	12.018	1788	1793	1805	rVV	579817	723566	62.46%	8.542%
75	12.317	1837	1842	1854	rBV	554492	705663	60.92%	8.331%
76	12.512	1873	1874	1876	rBV2	348	258	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
 Data File : VX044758.D
 Acq On : 29 Jan 2025 10:34
 Operator : JC/MD
 Sample : VX0129WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK756

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
 Title : VOC Analysis

77	12.591	1885	1887	1889	rBV2	273	185	0.02%	0.002%
78	12.762	1912	1915	1919	rVB	1480	1734	0.15%	0.020%
79	13.060	1963	1964	1966	rBV	400	334	0.03%	0.004%
80	13.121	1973	1974	1975	rBV	525	262	0.02%	0.003%
81	13.231	1991	1992	1995	rVB2	521	460	0.04%	0.005%
82	13.268	1995	1998	1999	rBV	456	409	0.04%	0.005%
83	13.383	2015	2017	2019	rBV2	228	247	0.02%	0.003%
84	13.469	2028	2031	2032	rBV2	278	268	0.02%	0.003%
85	13.603	2050	2053	2055	rBV2	536	668	0.06%	0.008%
86	13.646	2058	2060	2061	rBV	453	279	0.02%	0.003%
87	13.713	2069	2071	2072	rBV	316	202	0.02%	0.002%
88	13.792	2080	2084	2085	rBV	847	710	0.06%	0.008%
89	14.127	2135	2139	2145	rVB	2728	3371	0.29%	0.040%
90	14.170	2145	2146	2149	rVB2	336	294	0.03%	0.003%
91	14.255	2158	2160	2162	rVB2	591	428	0.04%	0.005%
92	14.274	2162	2163	2165	rBV2	660	436	0.04%	0.005%
93	14.517	2202	2203	2204	rBV	327	188	0.02%	0.002%
94	14.633	2220	2222	2224	rBV	471	366	0.03%	0.004%
95	14.969	2275	2277	2278	rBV	565	272	0.02%	0.003%
96	15.322	2333	2335	2336	rBV	490	278	0.02%	0.003%
97	15.395	2342	2347	2353	rVB5	1782	3466	0.30%	0.041%
98	15.603	2379	2381	2382	rBV	588	340	0.03%	0.004%
99	16.529	2532	2533	2534	rBV	451	218	0.02%	0.003%
100	16.548	2534	2536	2538	rVV	572	419	0.04%	0.005%

Sum of corrected areas: 8470474




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
Data File : VX044758.D
Acq On : 29 Jan 2025 10:34
Operator : JC/MD
Sample : VX0129WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK756

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

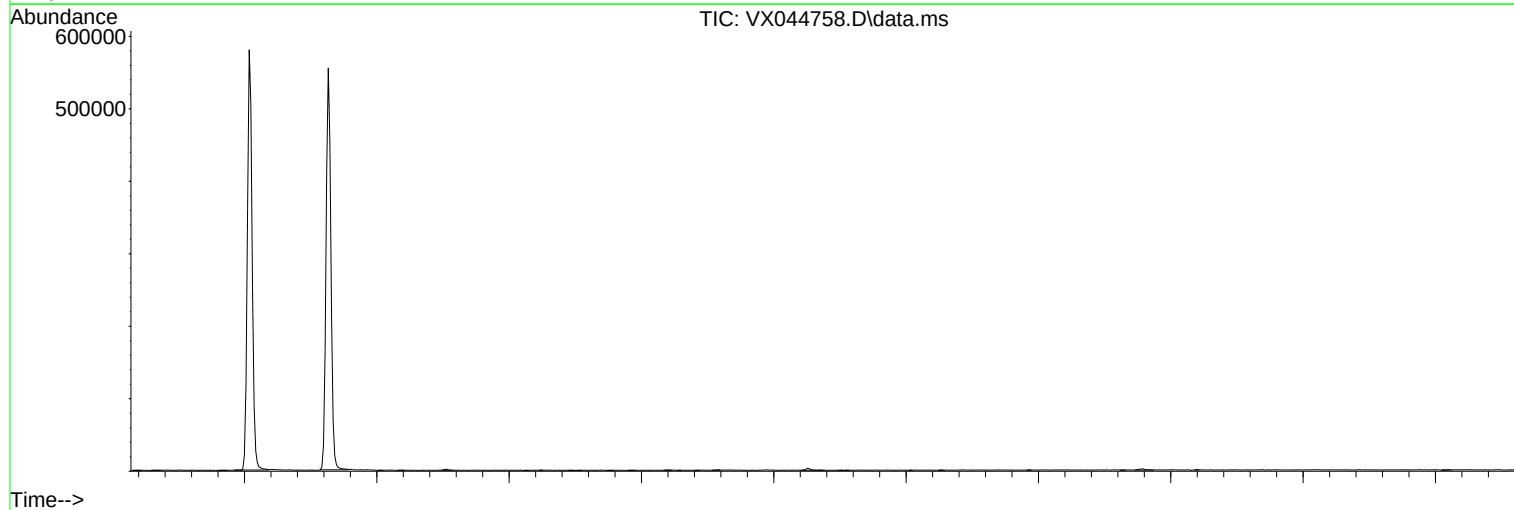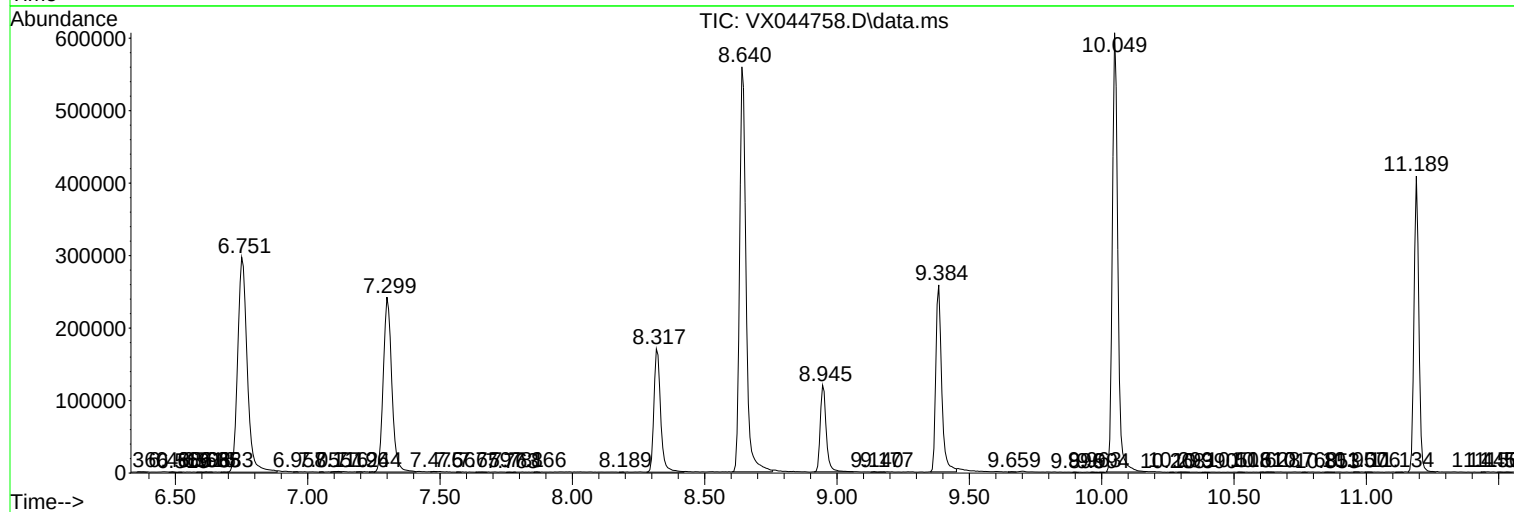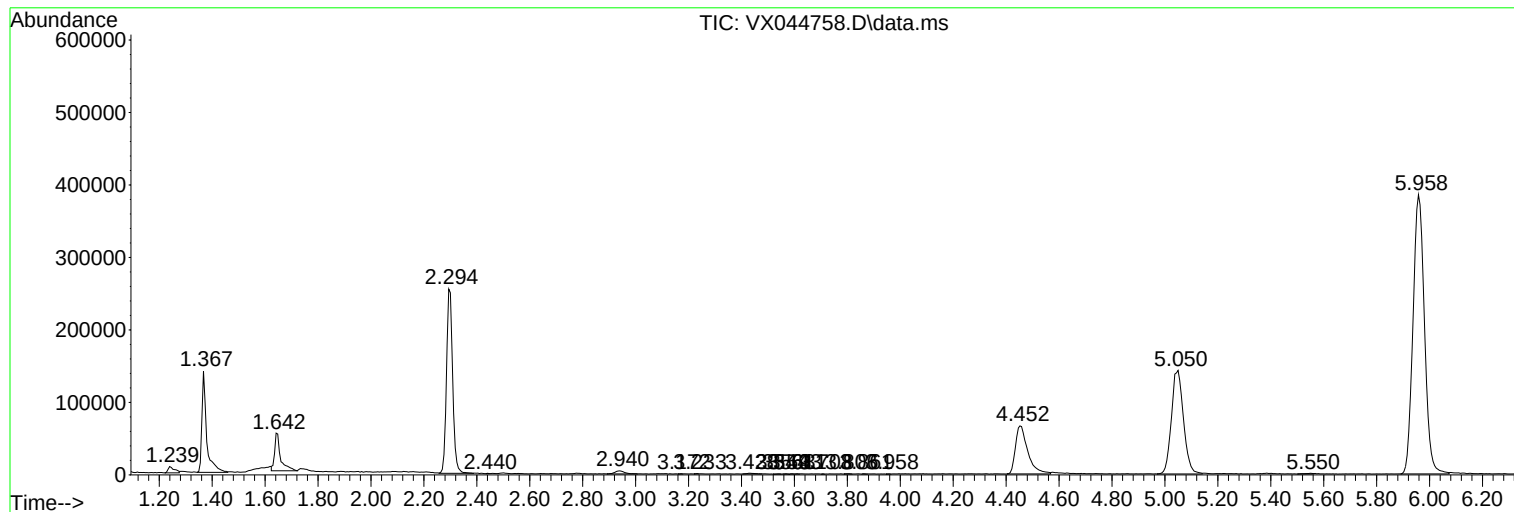

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
Data File : VX044758.D
Acq On : 29 Jan 2025 10:34
Operator : JC/MD
Sample : VX0129WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK756

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
Data File : VX044758.D
Acq On : 29 Jan 2025 10:34
Operator : JC/MD
Sample : VX0129WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK756

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML012825WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
