
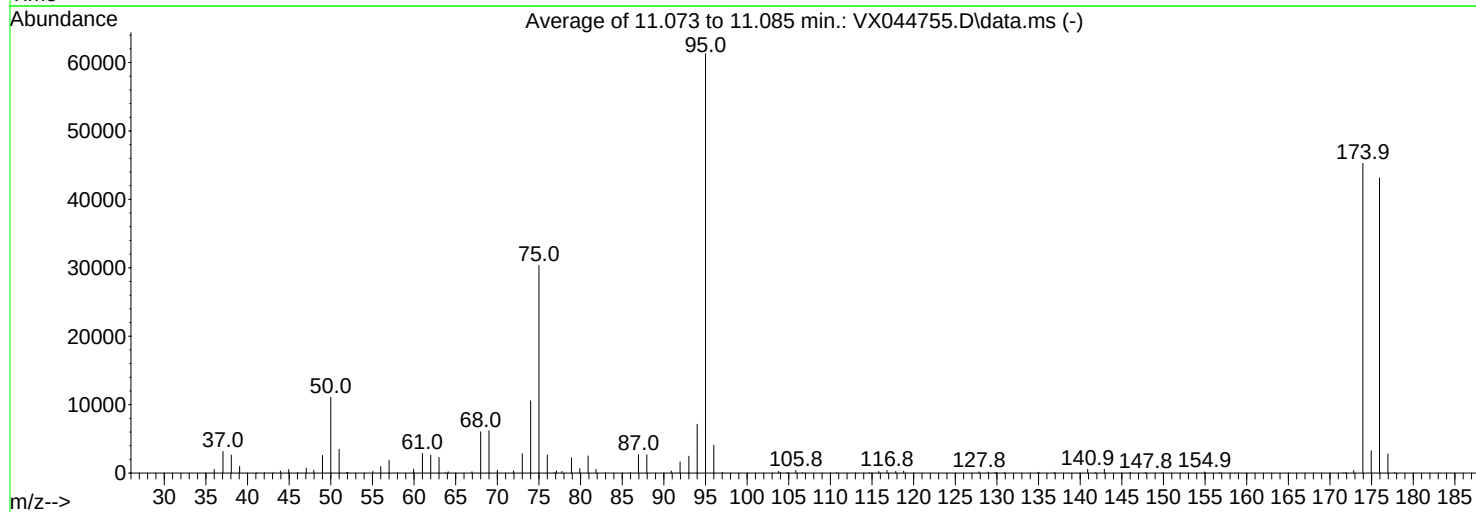


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012925\
Data File : VX044755.D
Acq On : 29 Jan 2025 08:48
Operator : JC/MD
Sample : BFB715
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB715

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM012825WMA.M
Title : VOC Analysis
Last Update : Tue Jan 28 12:04:44 2025

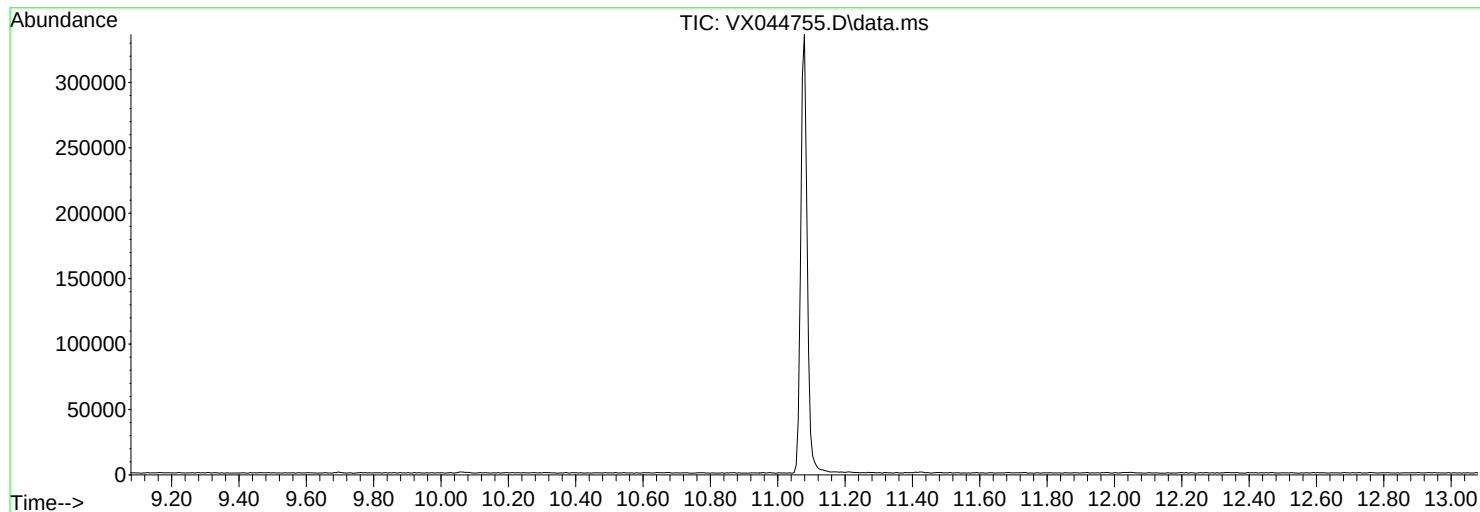

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	11056	PASS
75	95	30	80	49.5	30347	PASS
95	95	100	100	100.0	61288	PASS
96	95	5	9	6.6	4072	PASS
173	174	0.00	2	0.9	386	PASS
174	95	50	120	73.9	45272	PASS
175	174	5	9	7.2	3265	PASS
176	174	95	101	95.2	43109	PASS
177	176	5	9	6.5	2801	PASS

Scan 1632 (11.037 min): VX044755.D\data.ms
BFB715

m/z	Abundance
40.00	1102.0
43.90	486.0

Instrument :
MSVOA_X
ClientSampleId :
BFB715

m/z	Abundance
36.00	695.0
37.10	3960.0
38.10	2893.0
39.00	1188.0
40.00	814.0
41.20	63.0
43.10	85.0
44.00	902.0
45.00	567.0
46.10	95.0
47.00	885.0
48.00	460.0
49.00	2942.0
50.00	12567.0
51.00	4358.0
51.90	183.0
55.10	268.0
56.00	1219.0
57.00	2075.0
58.10	96.0
59.90	642.0
61.00	3085.0
62.00	3179.0
63.00	2634.0
64.10	209.0
66.90	180.0
68.00	7094.0
69.00	6774.0
70.00	520.0
72.00	379.0
73.00	3380.0
74.00	11743.0
75.00	33928.0
76.00	3061.0
77.10	428.0
77.80	301.0
78.90	2546.0
79.90	804.0
80.90	2697.0
81.80	588.0
83.00	105.0
86.10	103.0
87.00	2649.0
87.90	3089.0
90.90	374.0
92.00	1594.0
93.00	2579.0
94.00	7650.0
95.00	66696.0
96.00	4683.0
97.00	119.0
103.80	384.0
104.90	88.0
105.80	460.0
106.60	59.0
110.70	65.0
113.00	55.0
115.80	272.0
116.80	424.0
117.80	253.0
118.80	294.0
127.80	224.0
129.00	85.0
129.80	270.0
130.90	145.0
134.90	143.0
136.90	107.0
140.90	583.0
141.80	54.0
142.90	484.0
146.00	122.0
147.90	110.0
149.80	80.0
155.00	203.0
156.70	140.0
172.00	133.0
172.90	421.0
174.00	41952.0
175.00	3134.0
176.00	40856.0
177.00	2888.0
177.80	84.0

Instrument :
MSVOA_X
ClientSampleId :
BFB715

m/z	Abundance
36.00	573.0
37.00	3507.0
38.00	3300.0
39.10	1167.0
39.90	970.0
42.10	81.0
44.10	840.0
44.90	615.0
46.00	90.0
47.10	760.0
47.90	478.0
49.00	2998.0
50.00	12791.0
51.00	3958.0
52.10	192.0
55.00	213.0
56.00	1142.0
57.00	2302.0
57.90	102.0
60.00	784.0
61.00	3405.0
62.00	3002.0
63.00	2679.0
64.10	285.0
67.00	234.0
68.00	6756.0
69.00	7371.0
70.00	443.0
71.90	428.0
73.00	3008.0
74.00	12163.0
75.00	34784.0
76.00	2996.0
77.00	417.0
77.70	242.0
78.90	2677.0
79.90	629.0
80.90	2944.0
81.90	686.0
83.00	86.0
85.90	80.0
86.90	3150.0
88.00	2931.0
90.90	371.0
92.00	1992.0
93.00	2922.0
94.00	8287.0
95.00	71728.0
96.00	4687.0
97.10	81.0
103.80	326.0
104.70	174.0
105.90	397.0
106.70	80.0
110.80	161.0
113.10	89.0
115.80	270.0
116.90	461.0
117.90	265.0
118.80	363.0
127.90	185.0
128.90	184.0
130.00	167.0
130.90	128.0
134.90	212.0
136.90	177.0
140.90	797.0
141.70	116.0
142.90	743.0
146.00	120.0
147.80	118.0
149.90	66.0
154.90	184.0
156.90	101.0
158.60	69.0
171.80	109.0
172.90	374.0
173.90	53736.0
175.00	3813.0
175.90	50720.0
176.90	3395.0
177.70	94.0

Instrument :
MSVOA_X
ClientSampleId :
BFB715

m/z	Abundance
35.90	334.0
37.00	2008.0
38.00	1737.0
39.10	629.0
40.00	945.0
41.00	56.0
42.00	65.0
44.00	621.0
45.00	392.0
47.00	568.0
47.90	299.0
49.00	1764.0
50.00	7810.0
51.00	2133.0
52.00	101.0
55.00	277.0
56.10	534.0
57.00	1307.0
59.90	302.0
61.00	2140.0
62.00	1700.0
63.10	1565.0
63.80	93.0
64.20	108.0
66.90	160.0
68.00	4254.0
69.00	4398.0
70.00	347.0
71.90	199.0
73.00	2091.0
74.00	7781.0
75.00	22328.0
76.00	1828.0
76.80	135.0
77.20	218.0
77.80	183.0
78.90	1482.0
79.90	539.0
80.90	1926.0
81.90	362.0
87.00	2290.0
88.00	2005.0
90.90	182.0
91.90	1307.0
93.00	1906.0
94.00	5463.0
95.00	45440.0
96.00	2847.0
97.00	109.0
104.00	227.0
104.90	64.0
105.90	294.0
110.80	61.0
114.70	101.0
115.90	152.0
116.70	243.0
117.80	237.0
118.80	236.0
127.90	134.0
128.90	147.0
129.90	120.0
130.90	54.0
135.10	83.0
136.90	86.0
140.80	340.0
141.90	90.0
142.90	460.0
145.90	64.0
154.90	115.0
171.60	67.0
172.70	364.0
173.90	40128.0
174.90	2849.0
175.90	37752.0
177.00	2121.0

Instrument :
MSVOA_X
ClientSampleId :
BFB715