

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX013020\
 Data File : VX014772.D
 Acq On : 30 Jan 2020 17:21
 Operator : JC/SP
 Sample : L1332-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 KIT-SINK-1ST-DRAW

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	44	rBV	934629	1154811	54.49%	9.426%
2	1.594	107	116	118	rBV5	23917	46696	2.20%	0.381%
3	5.484	742	754	766	rBV	249929	717641	33.86%	5.858%
4	5.643	768	780	794	rBV	424646	1191594	56.22%	9.726%
5	6.045	837	846	859	rBV	281399	718973	33.92%	5.868%
6	6.844	966	977	989	rBV	670190	1551949	73.22%	12.668%
7	8.703	1275	1282	1290	rBV	1321593	2119460	100.00%	17.300%
8	10.105	1506	1512	1522	rBV	1383290	1821989	85.96%	14.872%
9	11.129	1675	1680	1686	rBV	1076207	1341573	63.30%	10.950%
10	12.074	1829	1835	1844	rBV	1235773	1586736	74.87%	12.951%


Sum of corrected areas: 12251422

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX013020\
Data File : VX014772.D
Acq On : 30 Jan 2020 17:21
Operator : JC/SP
Sample : L1332-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KIT-SINK-1ST-DRAW

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

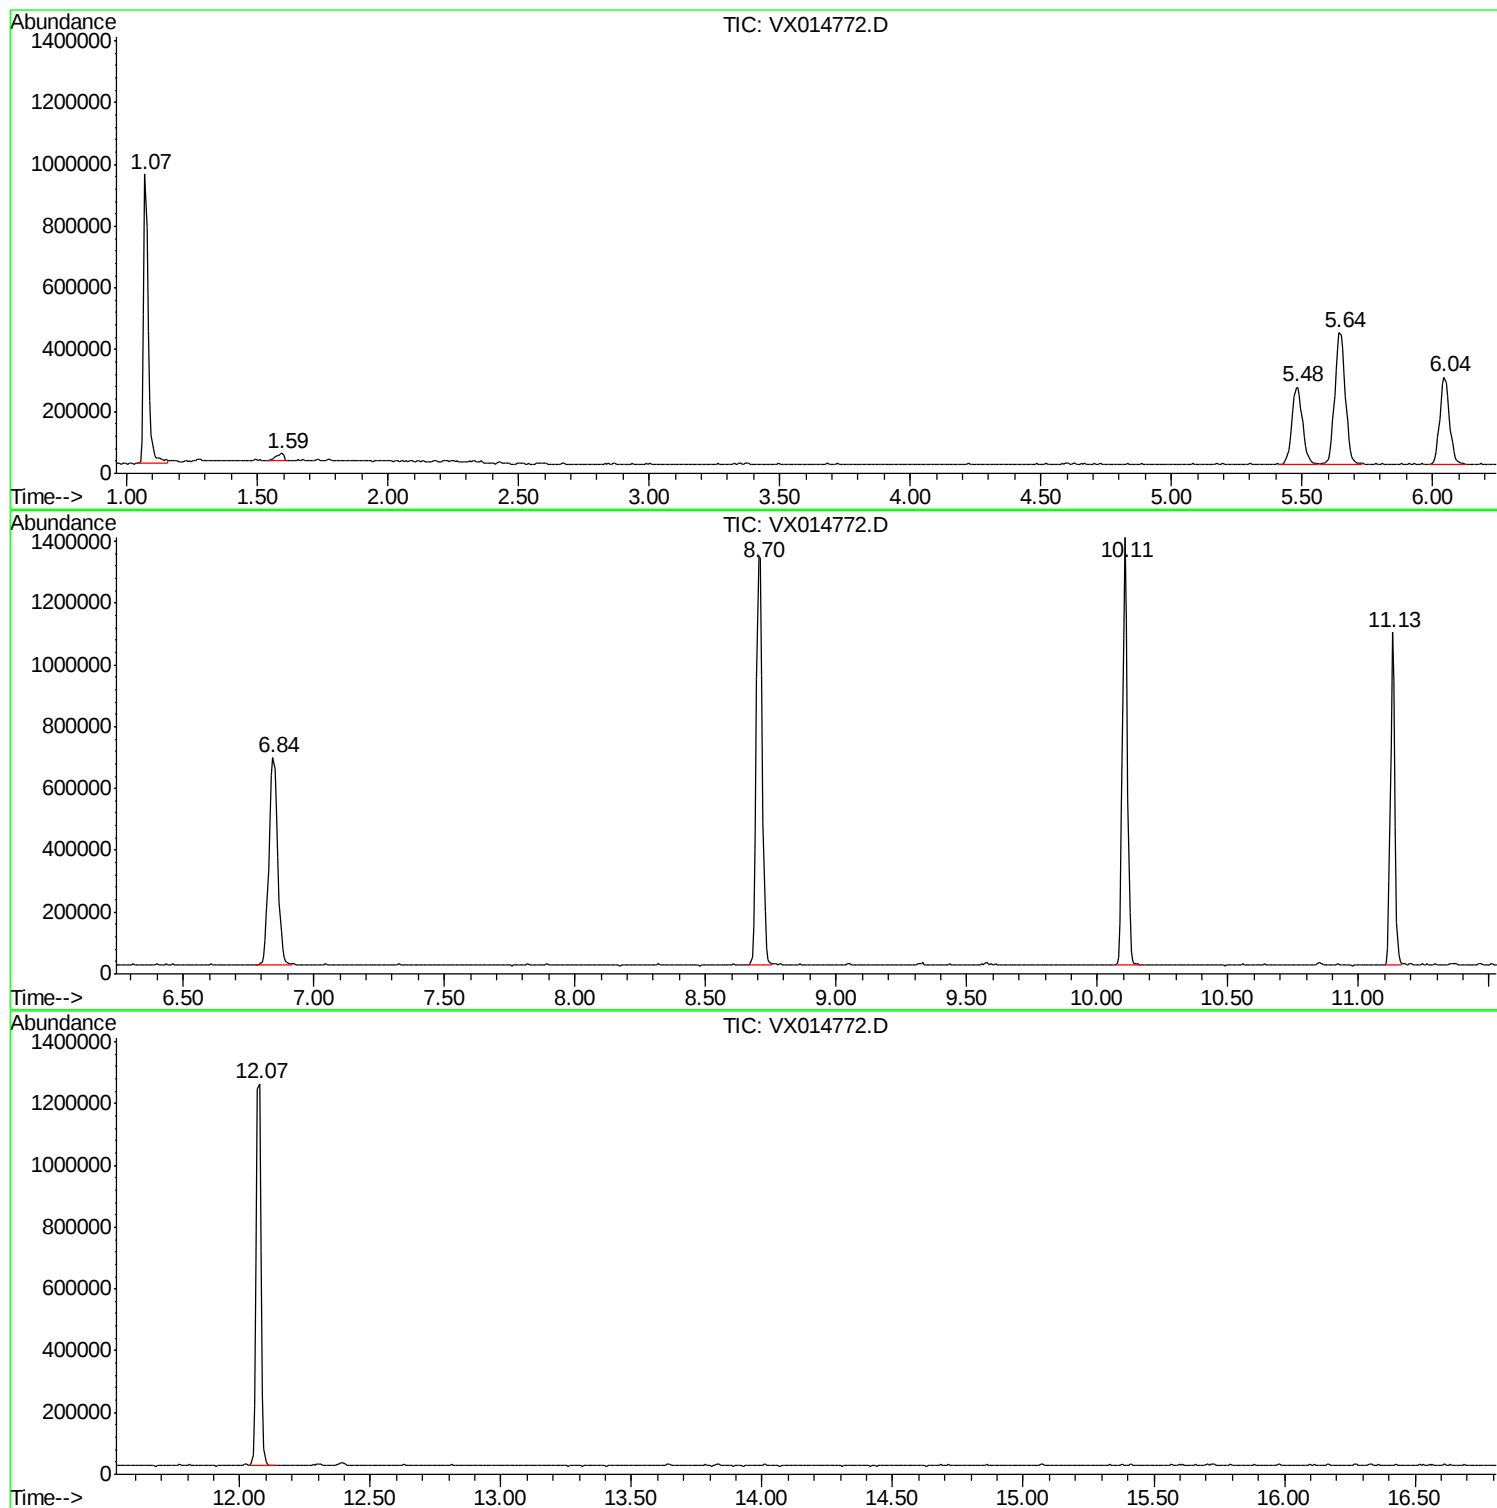

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX013020\
Data File : VX014772.D
Acq On : 30 Jan 2020 17:21
Operator : JC/SP
Sample : L1332-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KIT-SINK-1ST-DRAW

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX013020\
Data File : VX014772.D
Acq On : 30 Jan 2020 17:21
Operator : JC/SP
Sample : L1332-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KIT-SINK-1ST-DRAW

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012220W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc