

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013021\
 Data File : VX020806.D
 Acq On : 29 Jan 2021 16:47
 Operator : JC/SP
 Sample : M1285-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Jan 30 02:36:37 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	280807	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	466502	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.092	117	427811	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	171049	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.025	65	183569	47.93	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.86%
35) Dibromofluoromethane	5.458	113	158816	49.70	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	99.40%
50) Toluene-d8	8.696	98	571007	48.74	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.48%
62) 4-Bromofluorobenzene	11.122	95	189781	41.71	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	83.42%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013021\
Data File : VX020806.D
Acq On : 29 Jan 2021 16:47
Operator : JC/SP
Sample : M1285-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Jan 30 02:36:37 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration




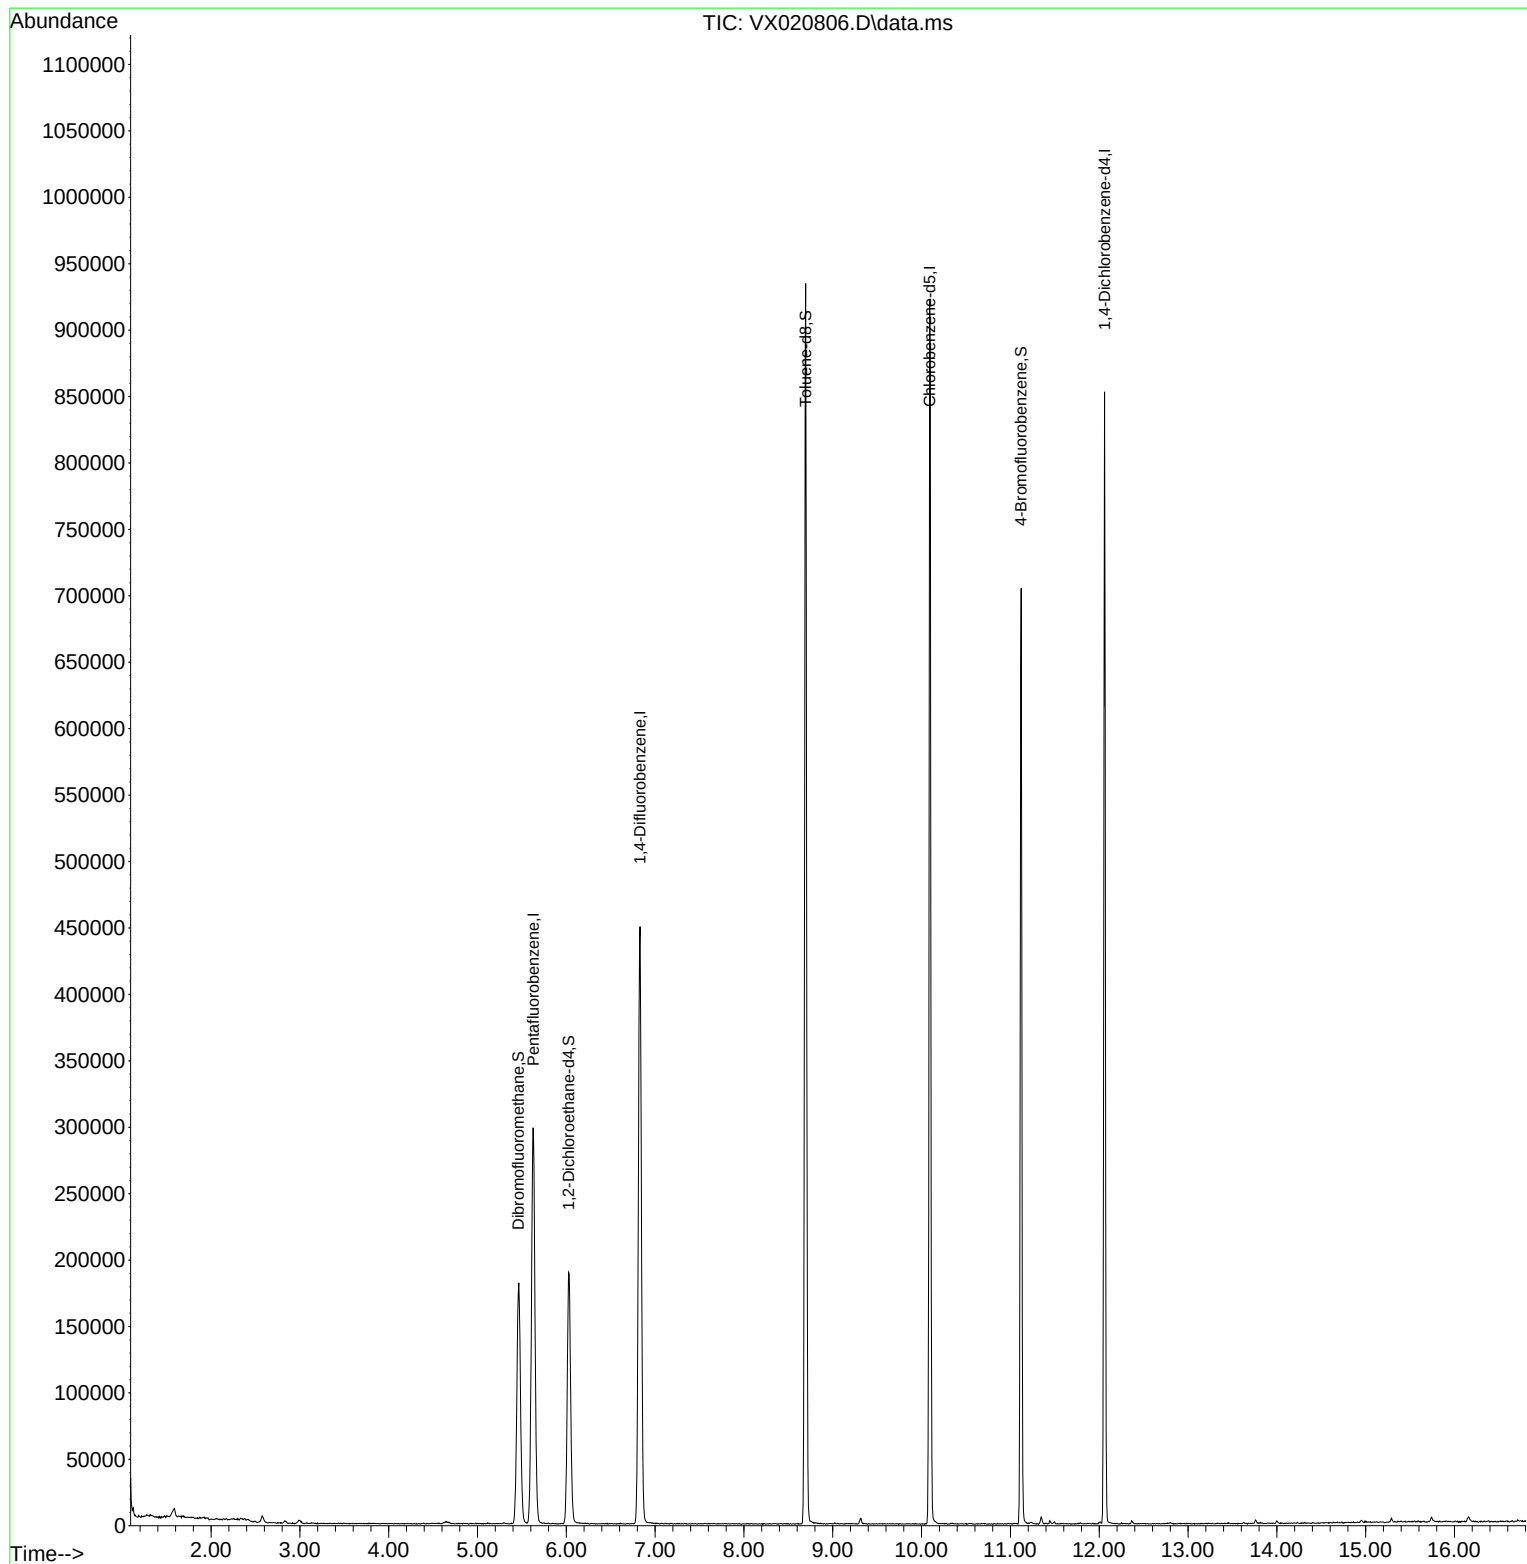


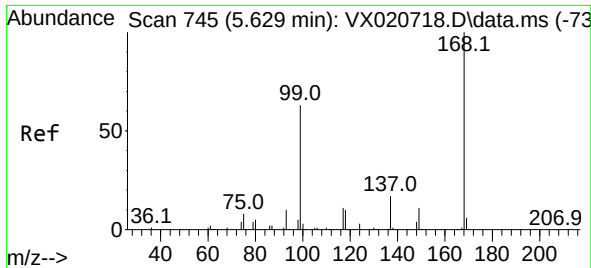

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.000 min
Lab File: VX020806.D
Acq: 29 Jan 2021 16:47




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 280807
Ion Ratio Lower Upper
168 100
99 57.4 45.8 68.6

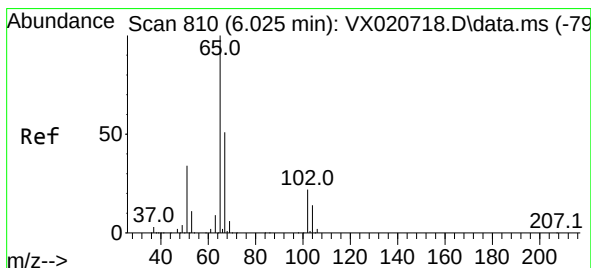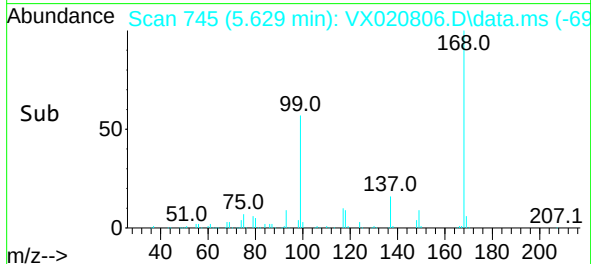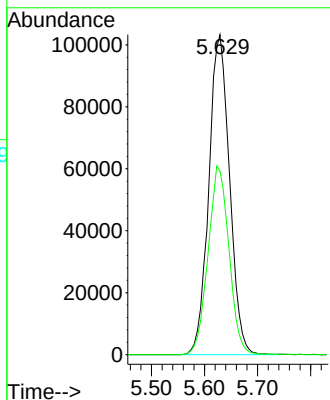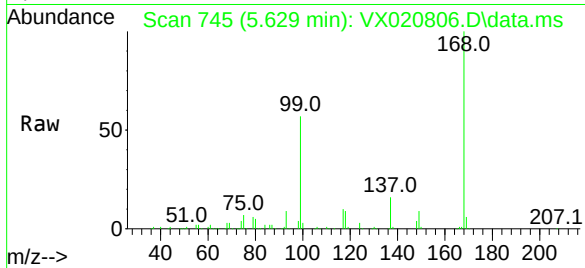

#33
1,2-Dichloroethane-d4
Concen: 47.93 ug/l
RT: 6.025 min Scan# 810
Delta R.T. 0.000 min
Lab File: VX020806.D
Acq: 29 Jan 2021 16:47

Tgt Ion: 65 Resp: 183569
Ion Ratio Lower Upper
65 100
67 52.5 0.0 105.4


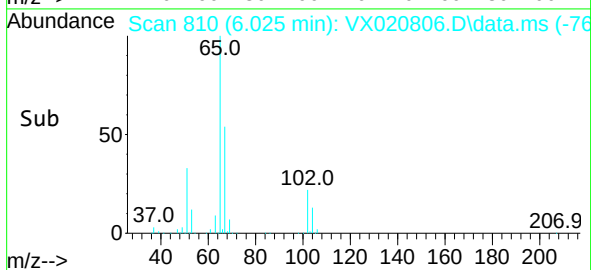
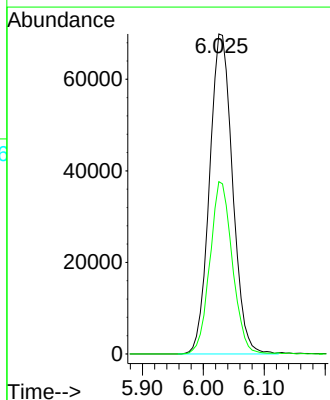
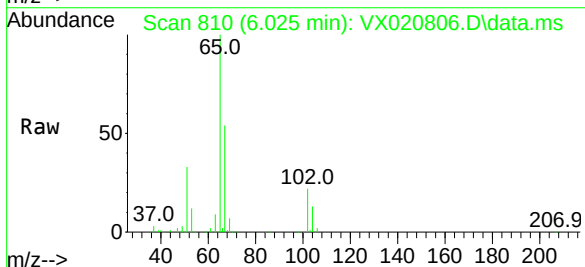


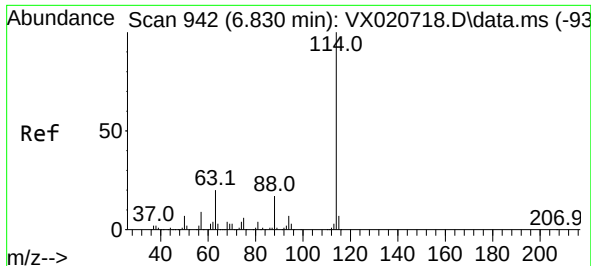

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. 0.000 min
Lab File: VX020806.D
Acq: 29 Jan 2021 16:47




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:114 Resp: 466502
Ion Ratio Lower Upper
114 100
63 19.9 0.0 40.8
88 15.9 0.0 32.8

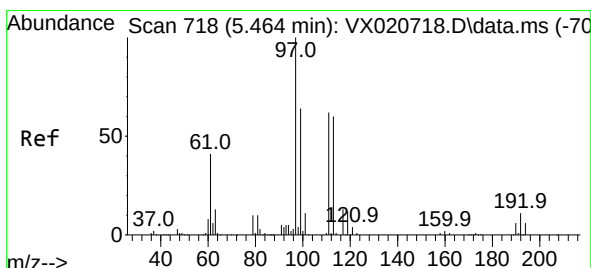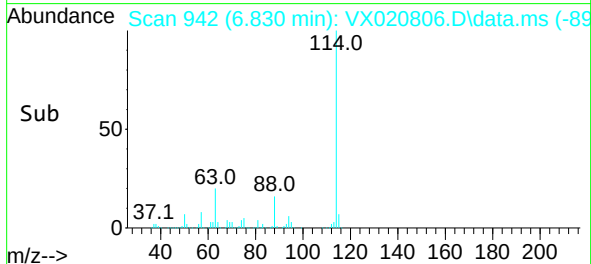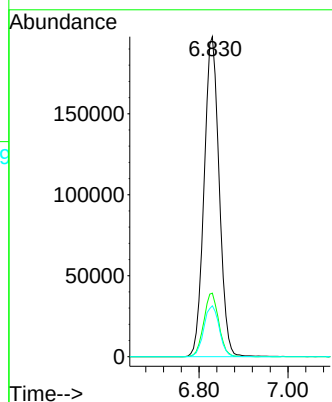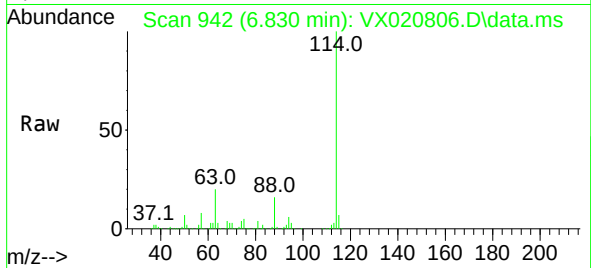

#35
Dibromofluoromethane
Concen: 49.70 ug/l
RT: 5.458 min Scan# 717
Delta R.T. -0.006 min
Lab File: VX020806.D
Acq: 29 Jan 2021 16:47

Tgt Ion:113 Resp: 158816
Ion Ratio Lower Upper
113 100
111 102.3 81.9 122.9
192 19.8 16.7 25.1


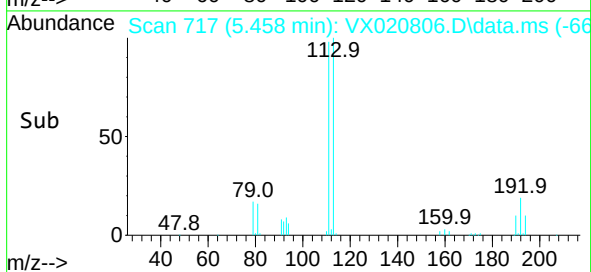
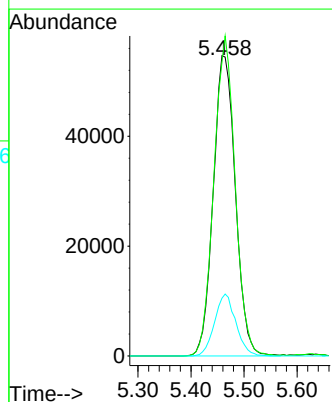
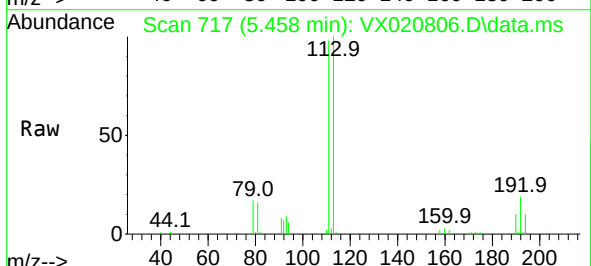


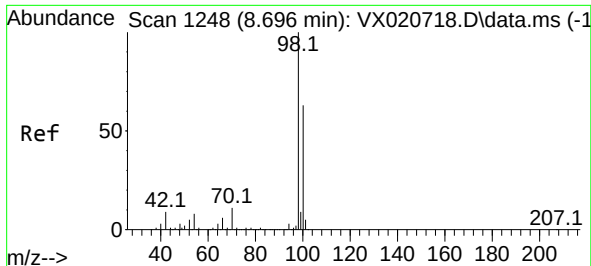

#50
Toluene-d8
Concen: 48.74 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. -0.000 min
Lab File: VX020806.D
Acq: 29 Jan 2021 16:47




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 571007
Ion Ratio Lower Upper
98 100
100 65.1 51.9 77.9

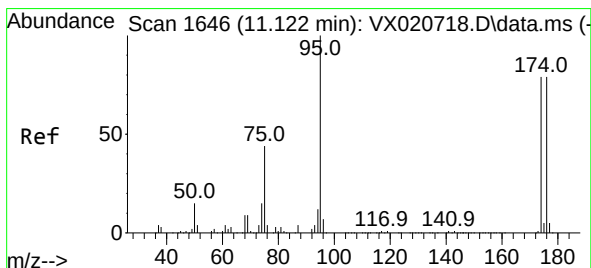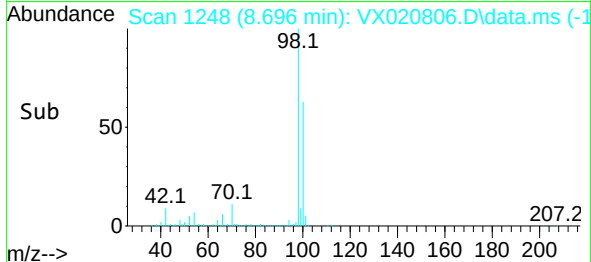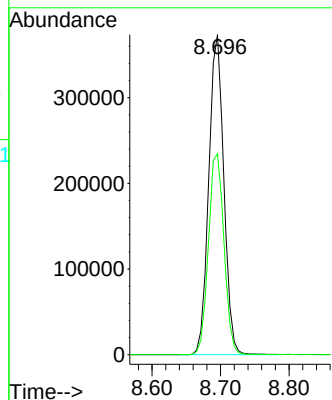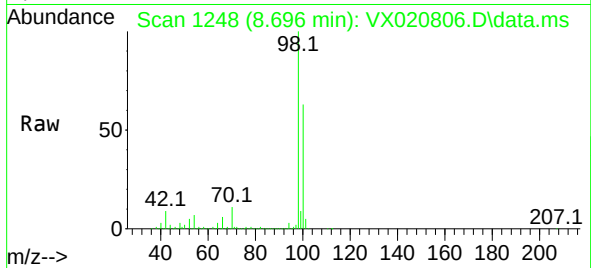

#62
4-Bromofluorobenzene
Concen: 41.71 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020806.D
Acq: 29 Jan 2021 16:47

Tgt Ion: 95 Resp: 189781
Ion Ratio Lower Upper
95 100
174 79.7 0.0 154.6
176 73.5 0.0 155.8


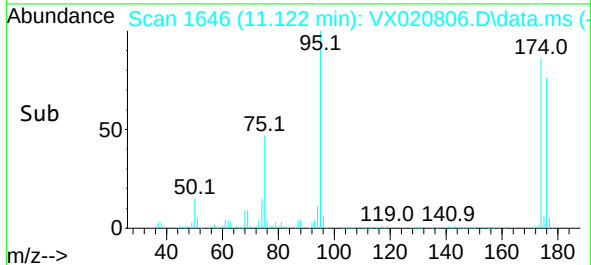
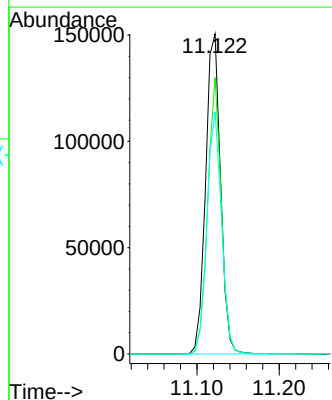
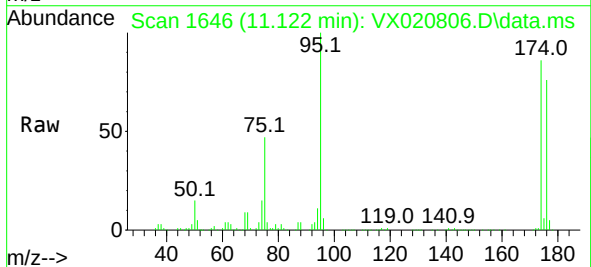


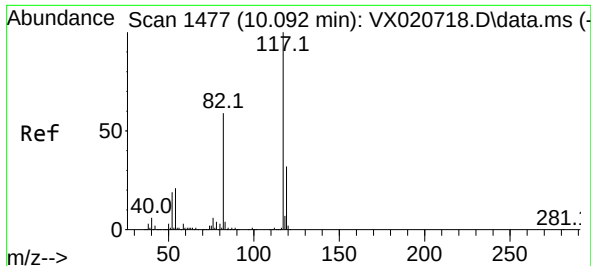

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.092 min Scan# 1477
Delta R.T. -0.000 min
Lab File: VX020806.D
Acq: 29 Jan 2021 16:47

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 427811
Ion Ratio Lower Upper
117 100
82 59.8 47.4 71.2
119 32.4 26.6 39.8

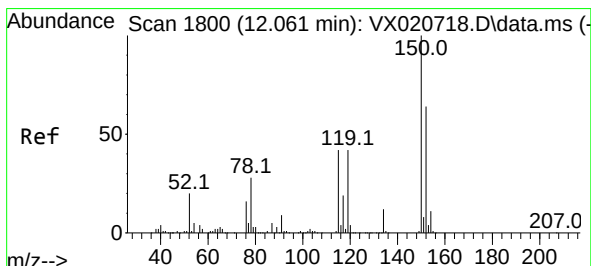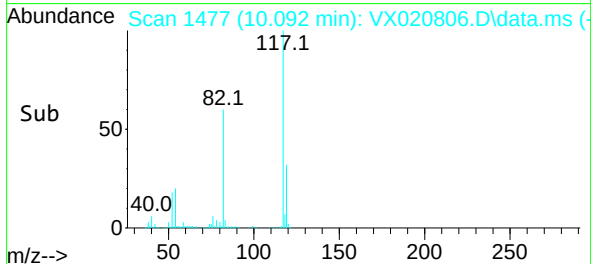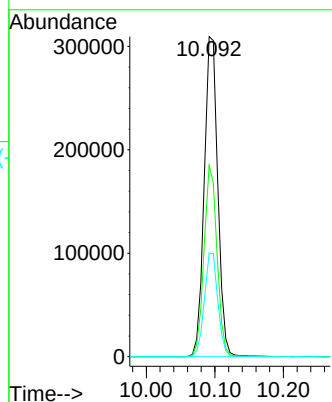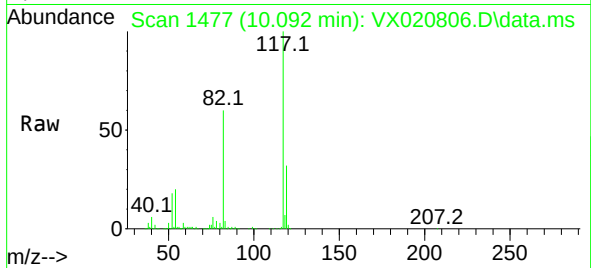

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020806.D
Acq: 29 Jan 2021 16:47

Tgt Ion:152 Resp: 171049
Ion Ratio Lower Upper
152 100
115 60.9 41.1 123.3
150 159.4 0.0 349.0

