

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013021\
 Data File : VX020808.D
 Acq On : 29 Jan 2021 17:34
 Operator : JC/SP
 Sample : M1285-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Jan 30 02:37:15 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	293338	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	495187	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	469591	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	198789	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	197380	49.33	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.66%
35) Dibromofluoromethane	5.464	113	167894	49.50	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	99.00%
50) Toluene-d8	8.696	98	606810	48.80	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.60%
62) 4-Bromofluorobenzene	11.122	95	212659	44.04	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	88.08%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013021\
Data File : VX020808.D
Acq On : 29 Jan 2021 17:34
Operator : JC/SP
Sample : M1285-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Jan 30 02:37:15 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration




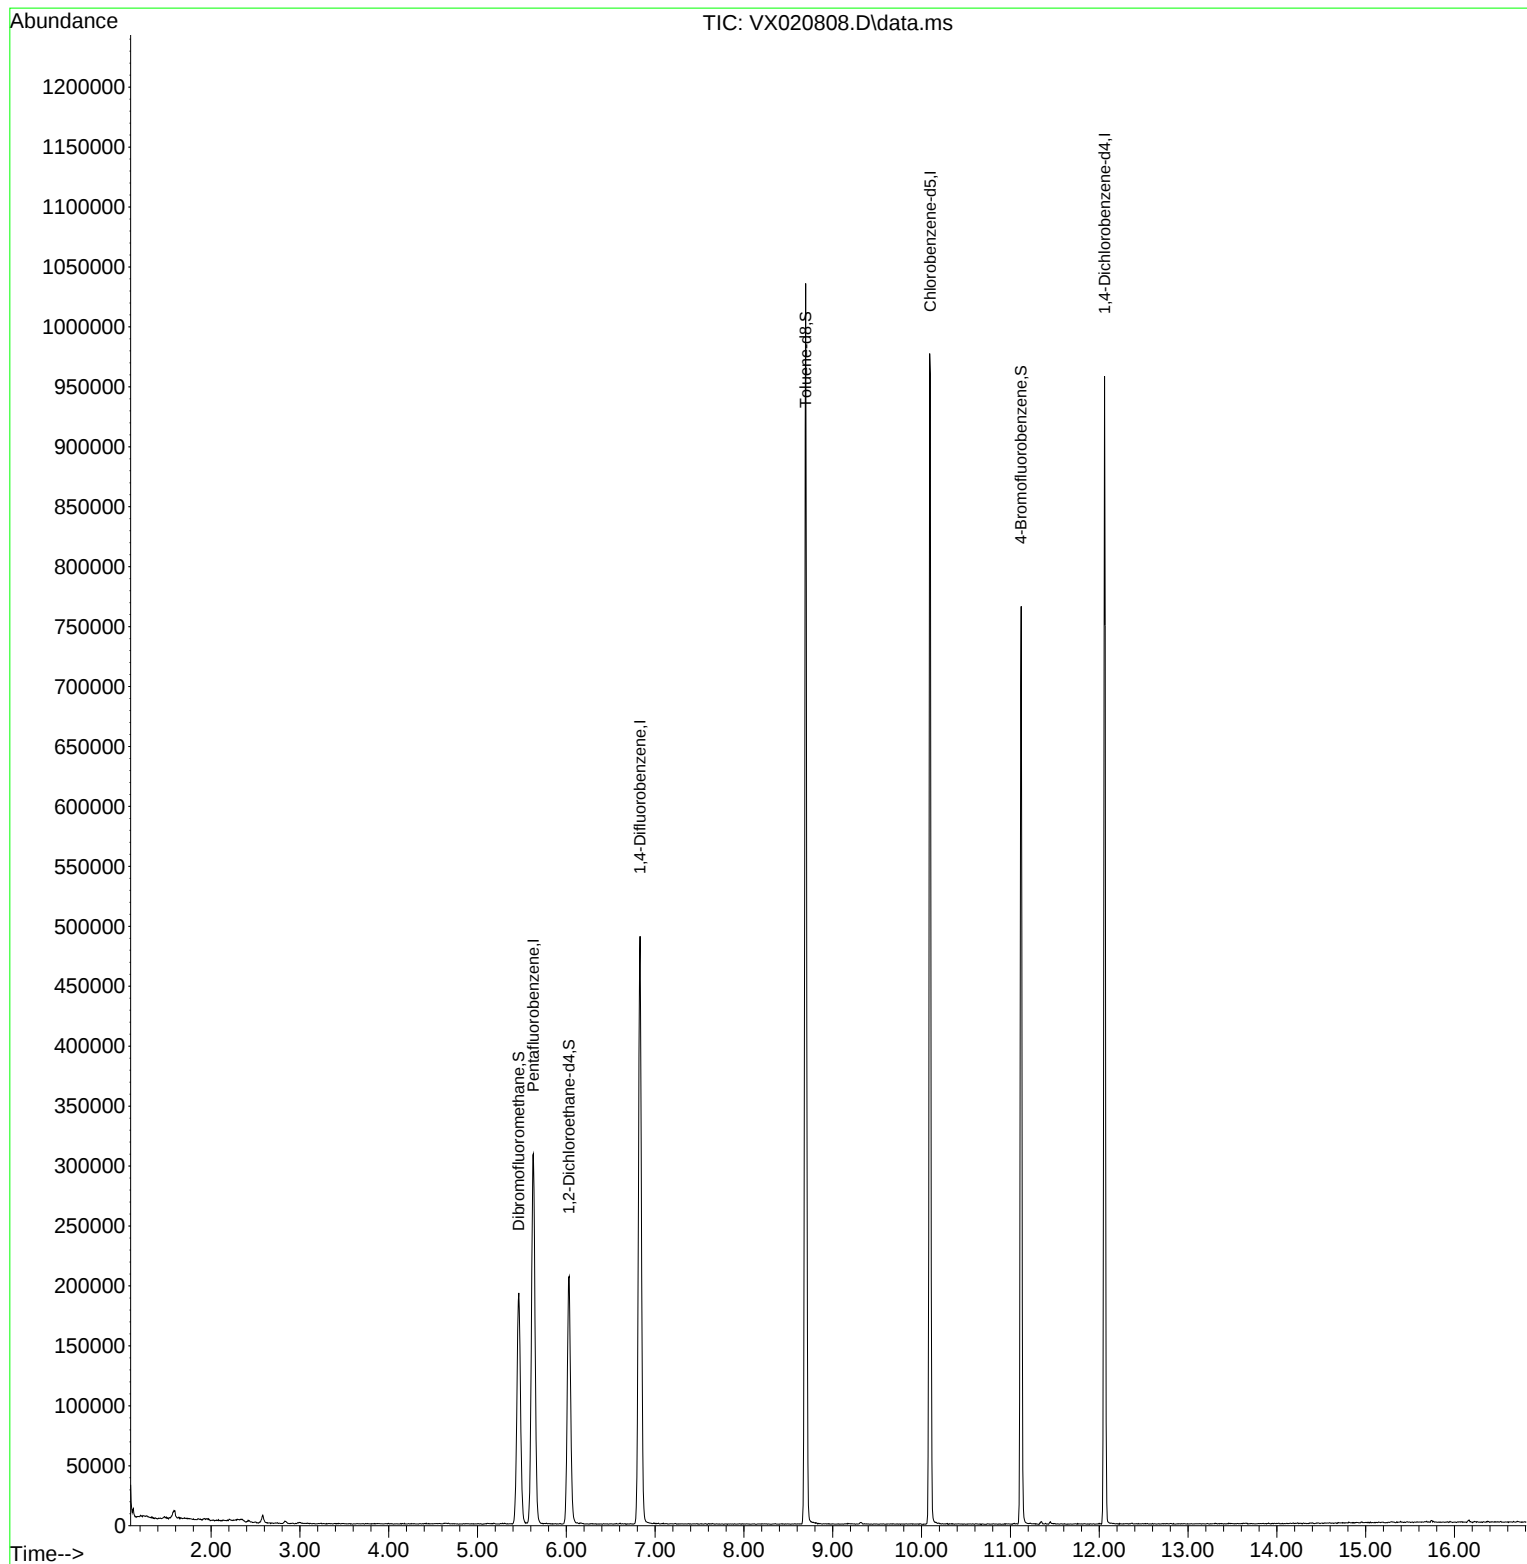


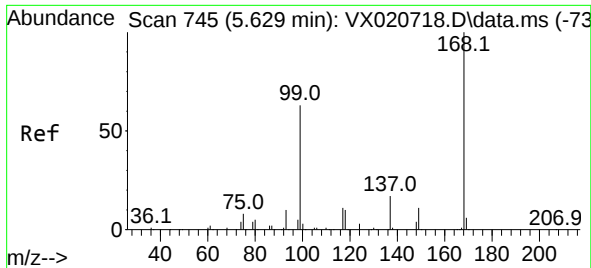

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.000 min
Lab File: VX020808.D
Acq: 29 Jan 2021 17:34




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 293338
Ion Ratio Lower Upper
168 100
99 62.0 45.8 68.6

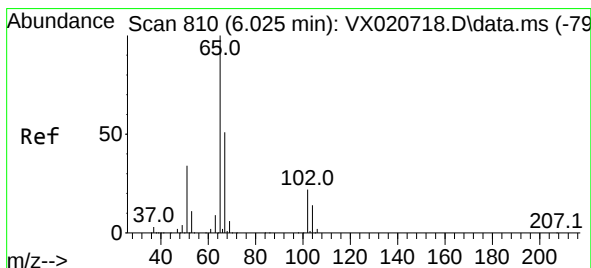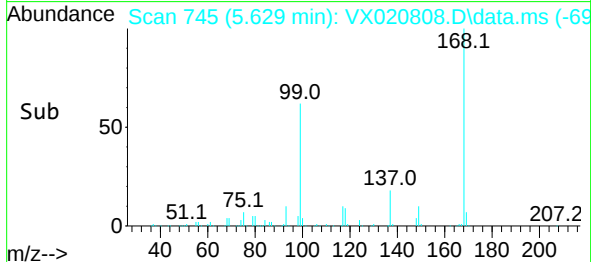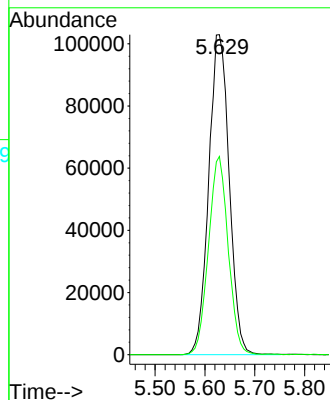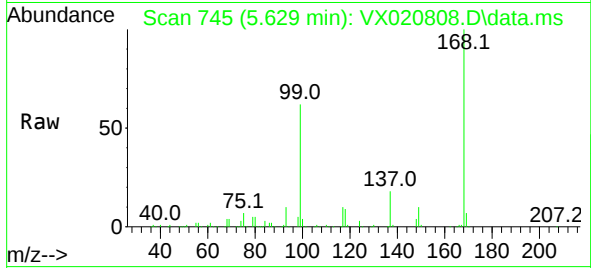

#33
1,2-Dichloroethane-d4
Concen: 49.33 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX020808.D
Acq: 29 Jan 2021 17:34


Tgt Ion: 65 Resp: 197380
Ion Ratio Lower Upper
65 100
67 51.8 0.0 105.4

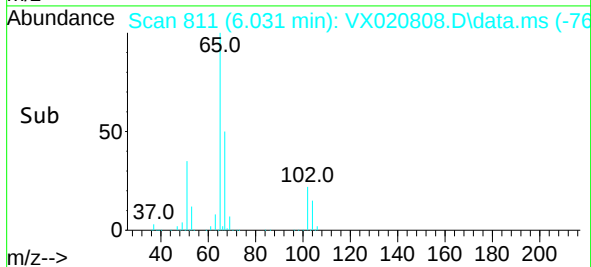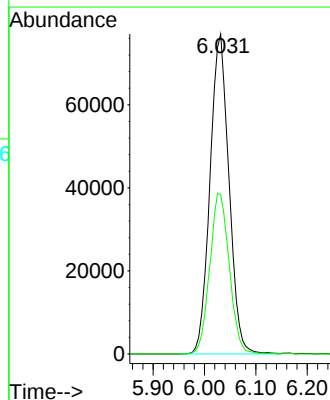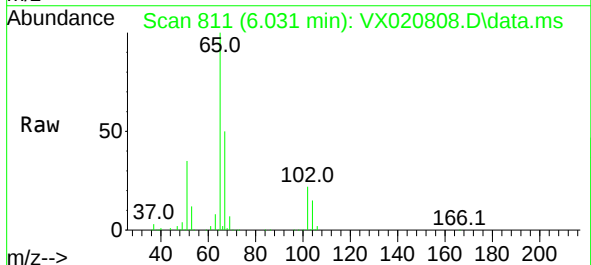



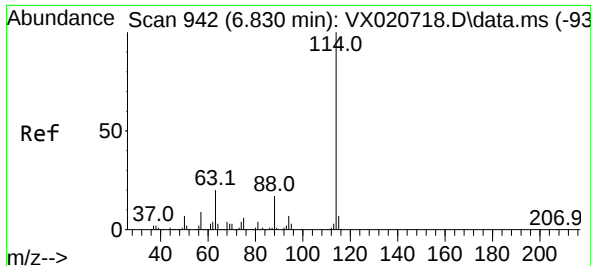


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. 0.000 min
Lab File: VX020808.D
Acq: 29 Jan 2021 17:34


Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

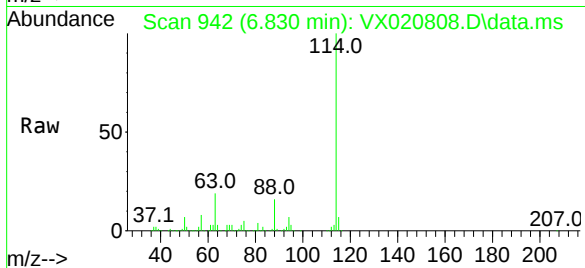



Tgt Ion:114 Resp: 495187
Ion Ratio Lower Upper
114 100
63 19.4 0.0 40.8
88 15.8 0.0 32.8

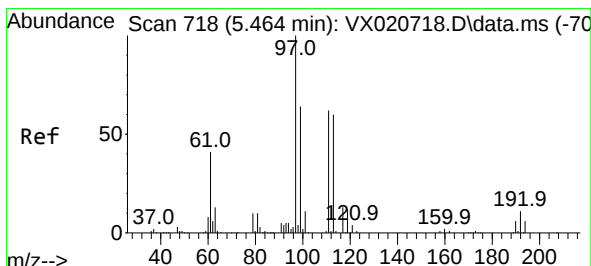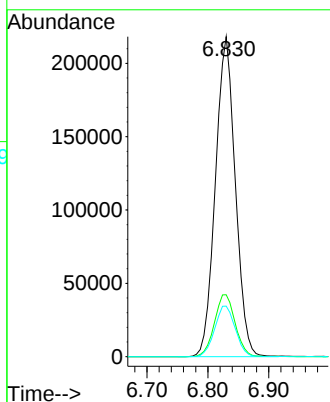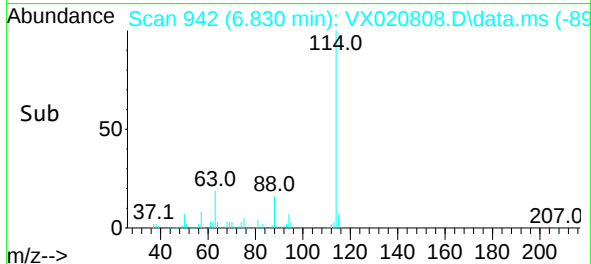


#35
Dibromofluoromethane
Concen: 49.50 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX020808.D
Acq: 29 Jan 2021 17:34

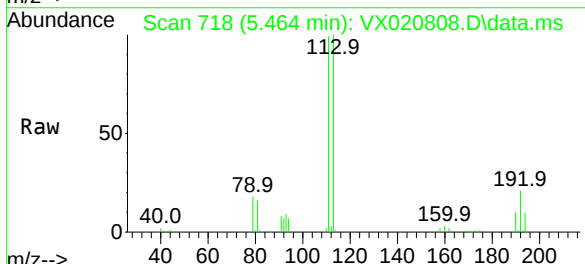

Tgt Ion:113 Resp: 167894
Ion Ratio Lower Upper
113 100
111 102.0 81.9 122.9
192 20.3 16.7 25.1



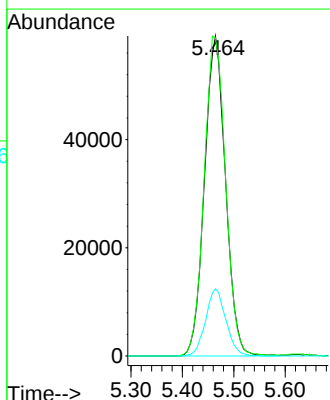
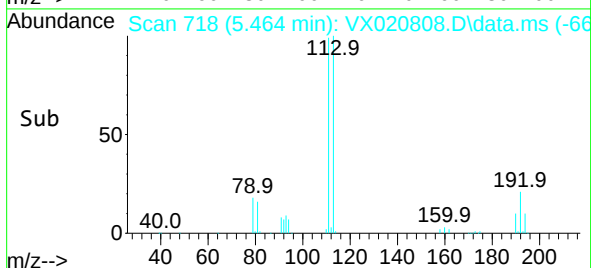


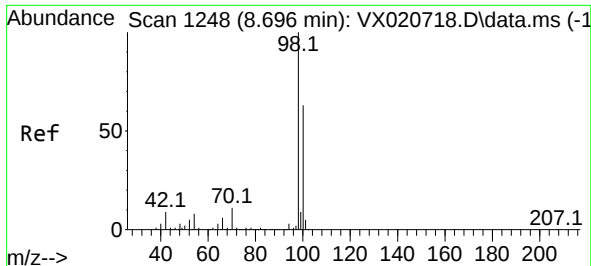

#50
Toluene-d8
Concen: 48.80 ug/l
RT: 8.696 min Scan# 1248
Delta R.T. -0.000 min
Lab File: VX020808.D
Acq: 29 Jan 2021 17:34




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 606810
Ion Ratio Lower Upper
98 100
100 65.3 51.9 77.9

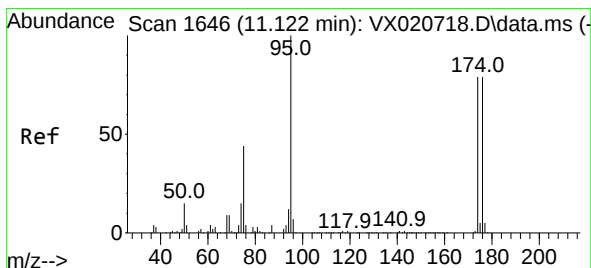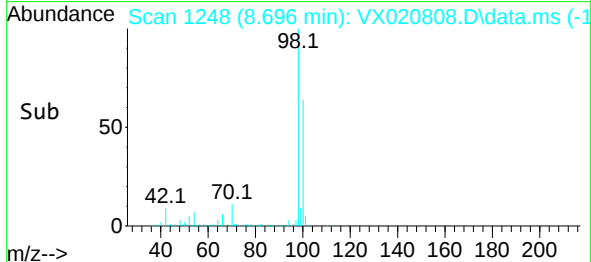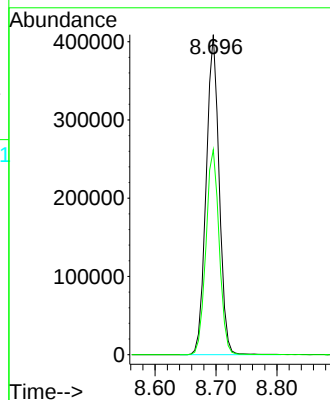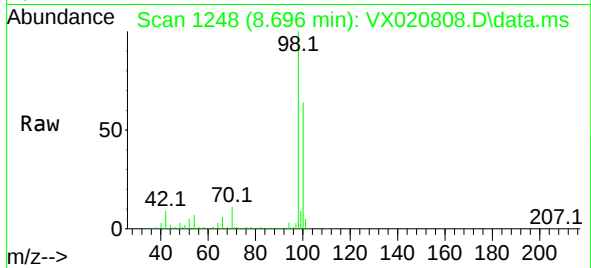

#62
4-Bromofluorobenzene
Concen: 44.04 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020808.D
Acq: 29 Jan 2021 17:34

Tgt Ion: 95 Resp: 212659
Ion Ratio Lower Upper
95 100
174 77.6 0.0 154.6
176 74.9 0.0 155.8


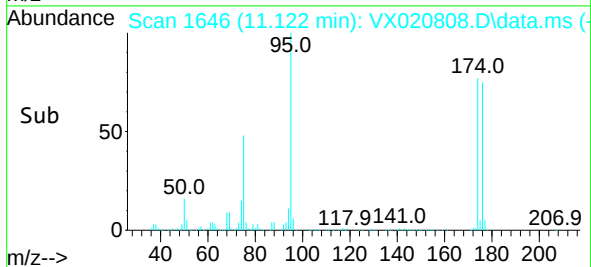
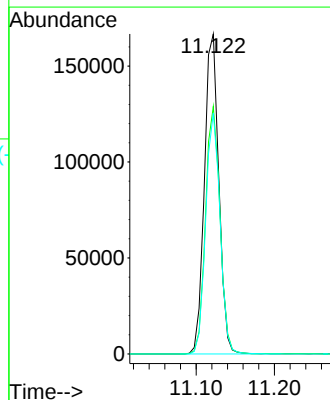
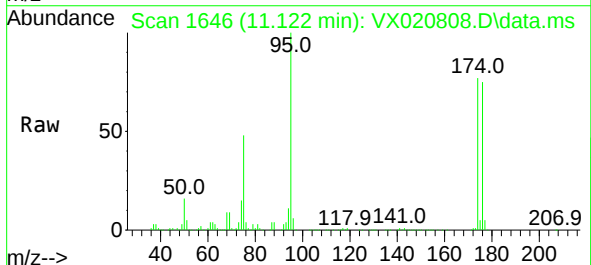


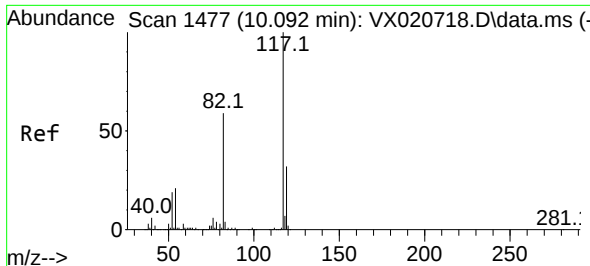

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.006 min
Lab File: VX020808.D
Acq: 29 Jan 2021 17:34

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 469591
Ion Ratio Lower Upper
117 100
82 55.1 47.4 71.2
119 32.4 26.6 39.8

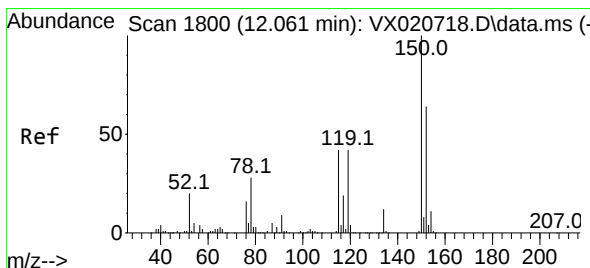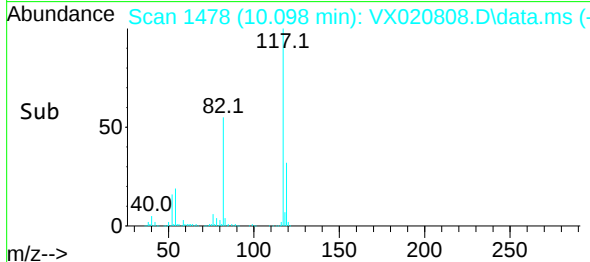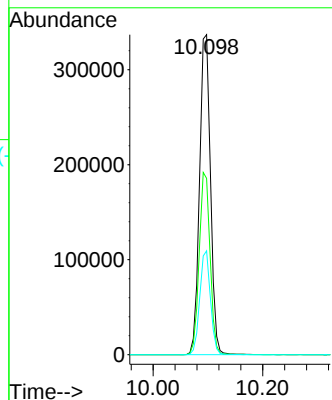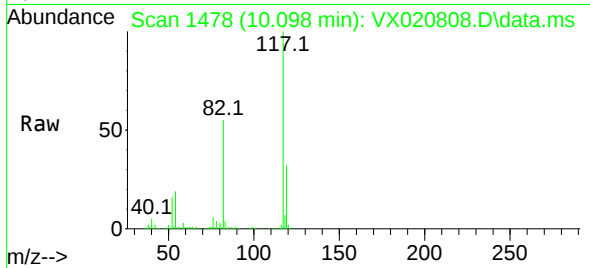

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX020808.D
Acq: 29 Jan 2021 17:34

Tgt Ion:152 Resp: 198789
Ion Ratio Lower Upper
152 100
115 60.6 41.1 123.3
150 157.3 0.0 349.0

