

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013021\
 Data File : VX020814.D
 Acq On : 29 Jan 2021 19:55
 Operator : JC/SP
 Sample : M1296-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-VPB-RW6-GW-98-100

Quant Time: Jan 30 02:39:02 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jan 25 13:38:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.629	168	288783	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	498025	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.097	117	485373	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.060	152	211007	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	198619	50.42	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 100.84%	
35) Dibromofluoromethane	5.464	113	171611	50.31	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 100.62%	
50) Toluene-d8	8.695	98	606302	48.48	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 96.96%	
62) 4-Bromofluorobenzene	11.122	95	216155	44.50	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 89.00%	
Target Compounds						
16) Acetone	2.416	43	4960	3.32	ug/l	98
64) Tetrachloroethene	9.311	164	916	0.25	ug/l #	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013021\
Data File : VX020814.D
Acq On : 29 Jan 2021 19:55
Operator : JC/SP
Sample : M1296-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-98-100


Quant Time: Jan 30 02:39:02 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X012521W.M
Quant Title : SW846 8260
QLast Update : Mon Jan 25 13:38:15 2021
Response via : Initial Calibration

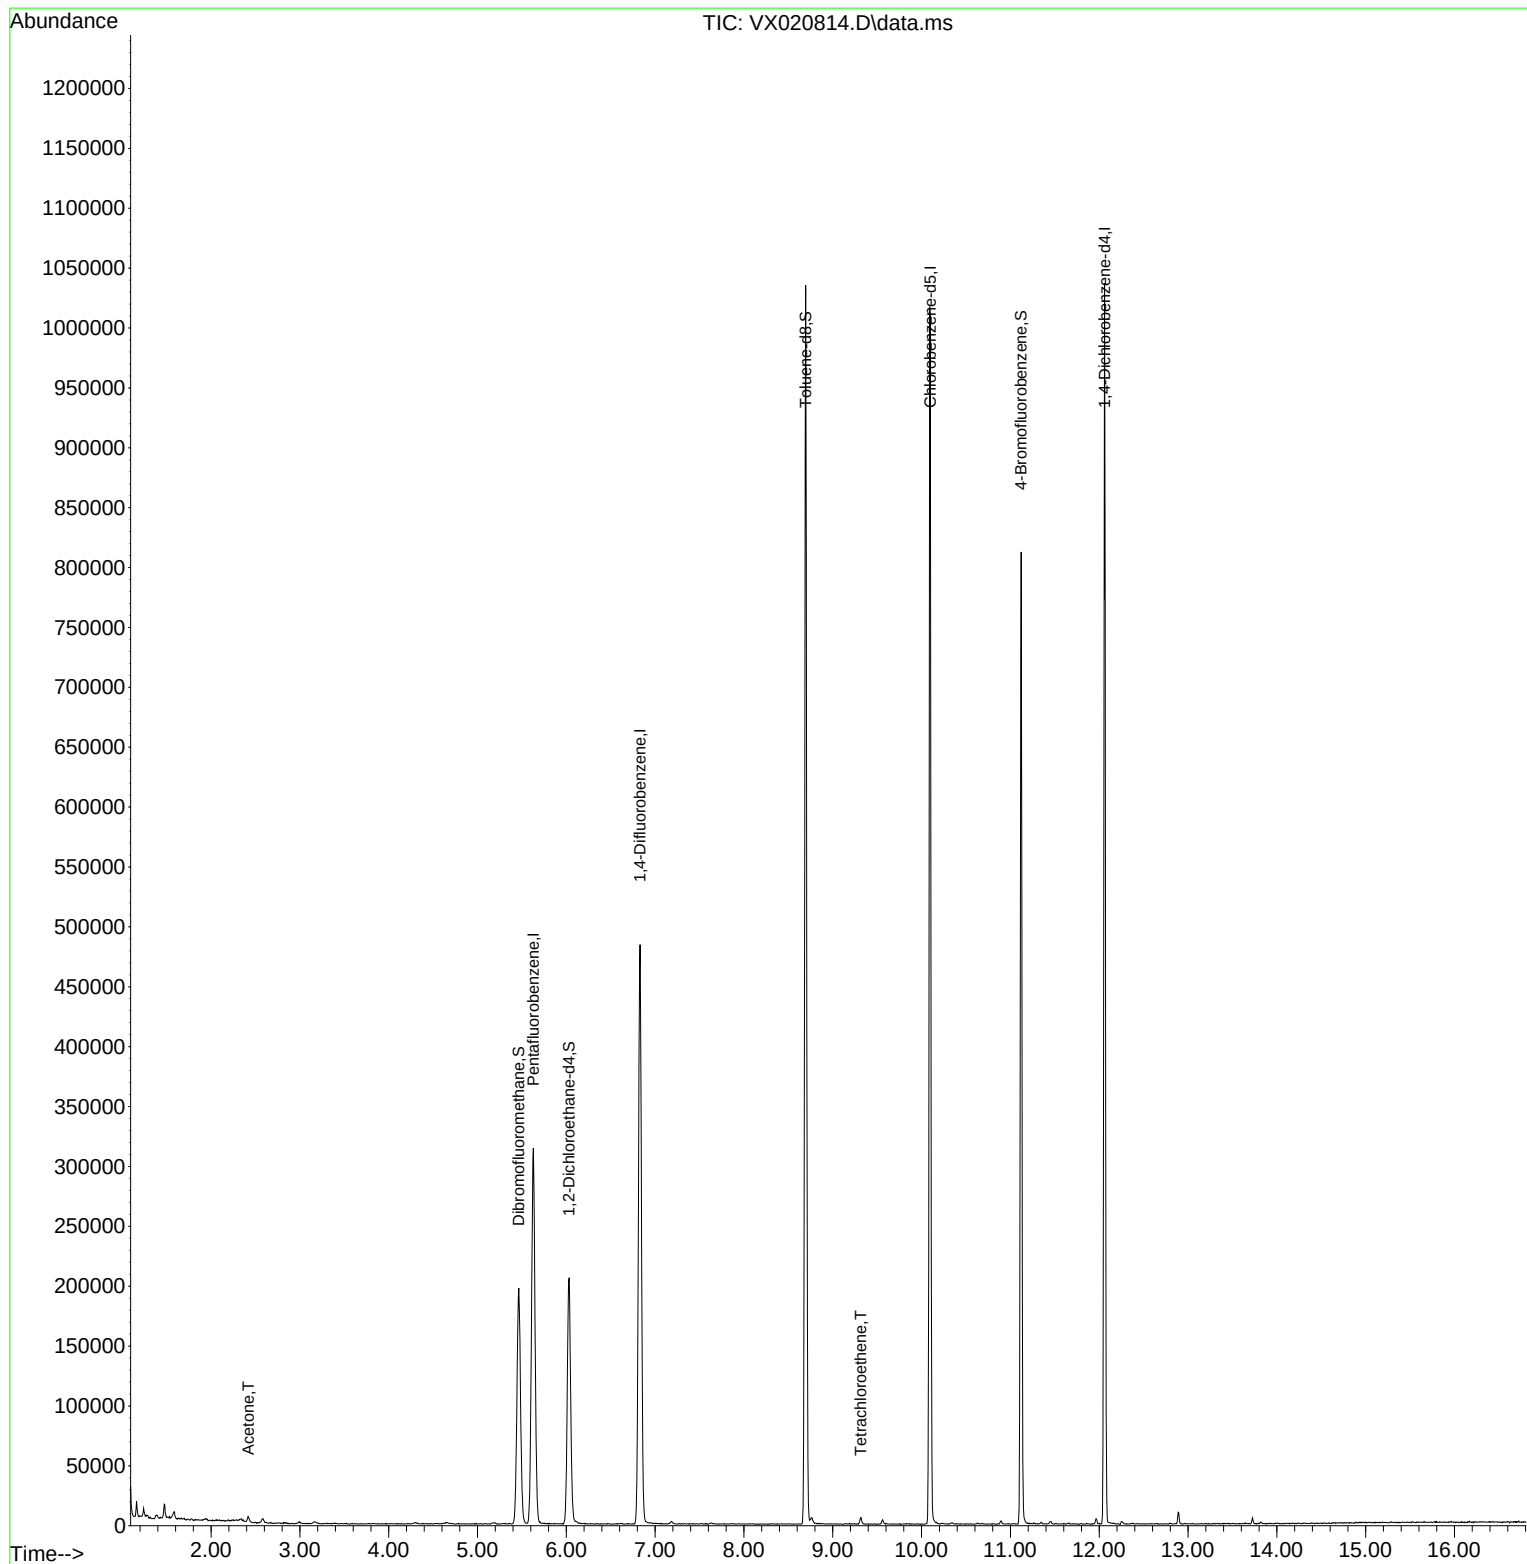



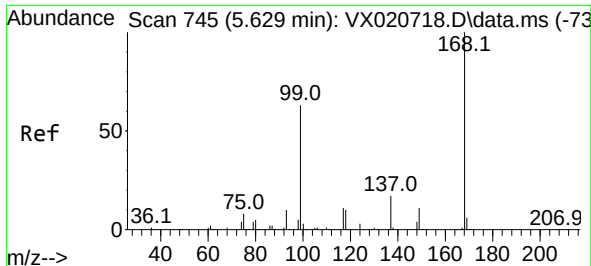


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.000 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-98-100



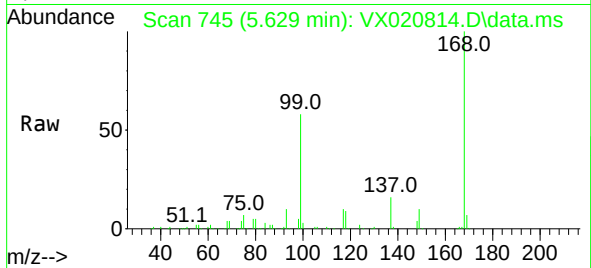



Tgt Ion:168 Resp: 288783
Ion Ratio Lower Upper
168 100
99 58.4 45.8 68.6

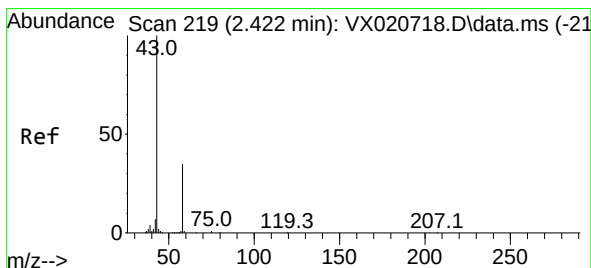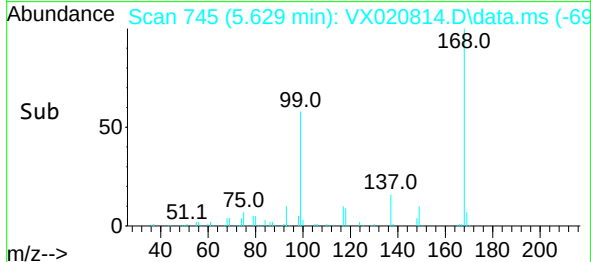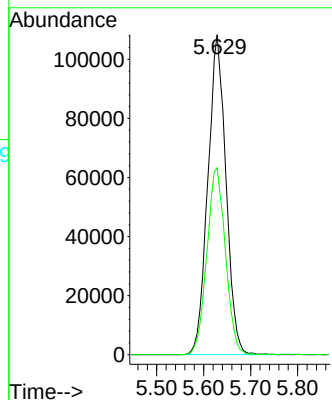

#16
Acetone
Concen: 3.32 ug/l
RT: 2.416 min Scan# 218
Delta R.T. -0.006 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55

Tgt Ion: 43 Resp: 4960
Ion Ratio Lower Upper
43 100
58 36.2 27.8 41.8


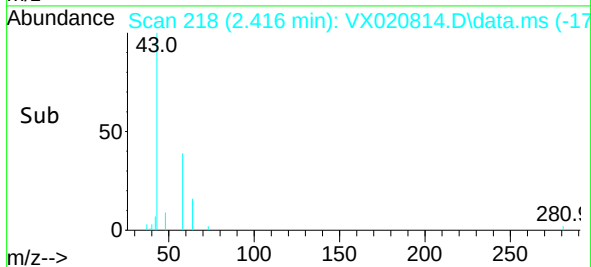
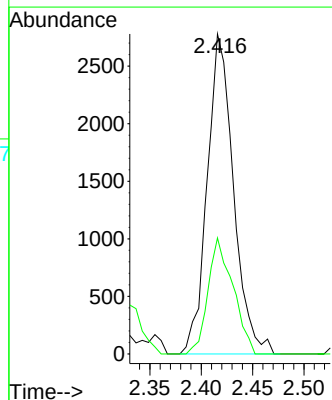
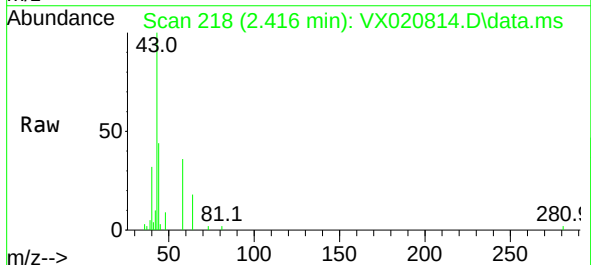


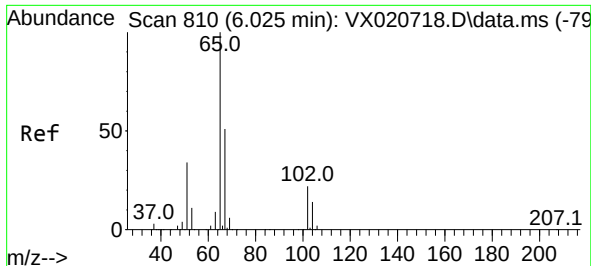

#33
1,2-Dichloroethane-d4
Concen: 50.42 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-98-100


Tgt Ion: 65 Resp: 198619
Ion Ratio Lower Upper
65 100
67 52.0 0.0 105.4

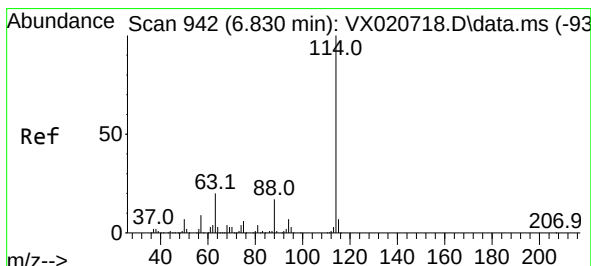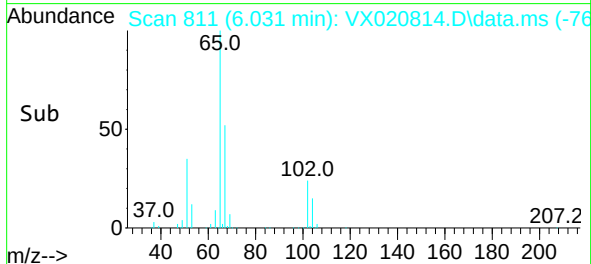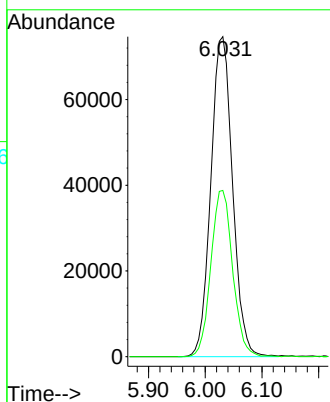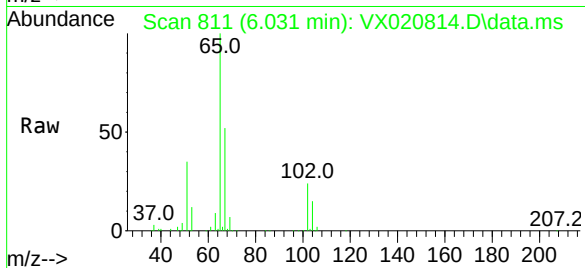

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. -0.000 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55

Tgt Ion: 114 Resp: 498025
Ion Ratio Lower Upper
114 100
63 19.4 0.0 40.8
88 16.0 0.0 32.8


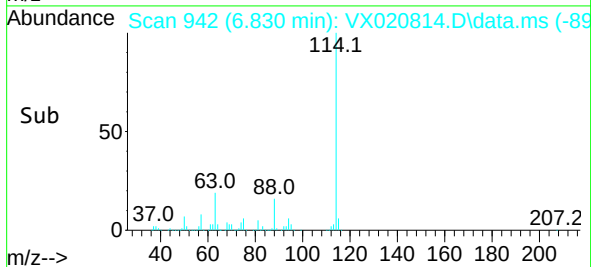
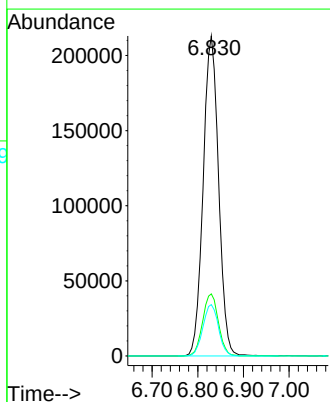
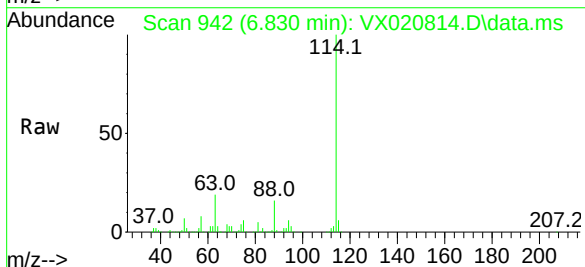


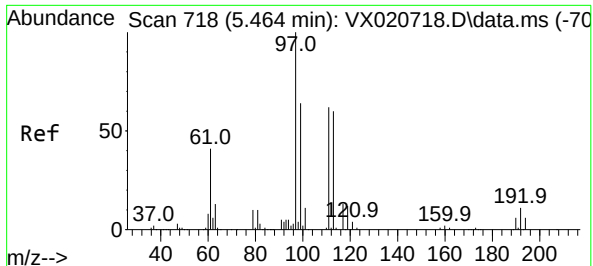

#35
Dibromofluoromethane
Concen: 50.31 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-98-100


Tgt Ion:113 Resp: 171611
Ion Ratio Lower Upper
113 100
111 101.9 81.9 122.9
192 19.9 16.7 25.1

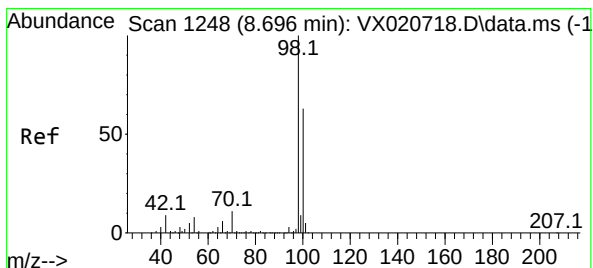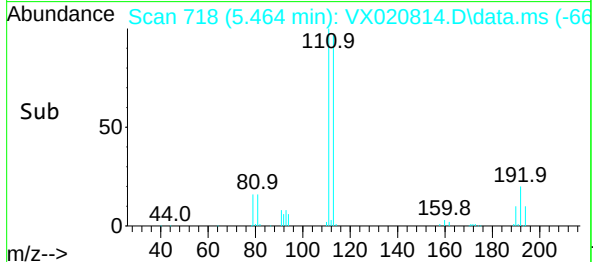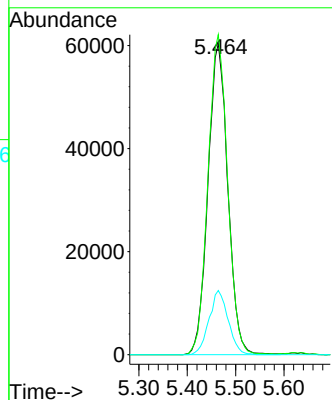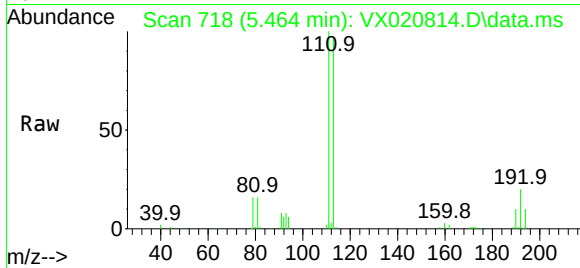

#50
Toluene-d8
Concen: 48.48 ug/l
RT: 8.695 min Scan# 1248
Delta R.T. -0.001 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55

Tgt Ion: 98 Resp: 606302
Ion Ratio Lower Upper
98 100
100 66.4 51.9 77.9


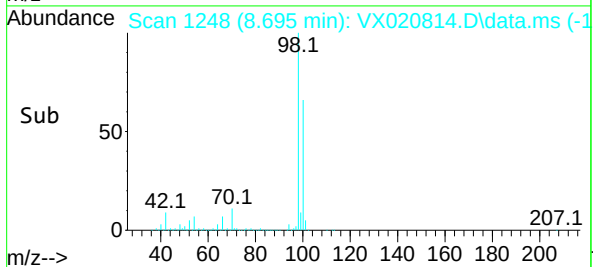
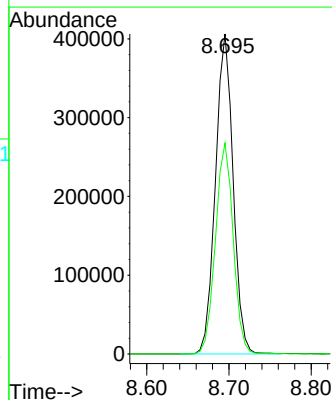
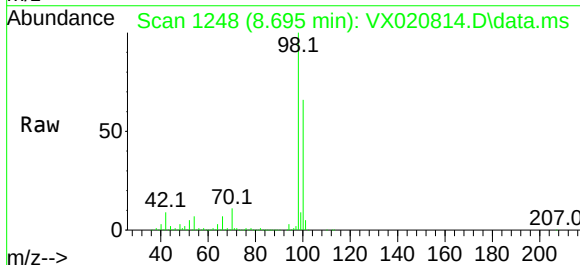


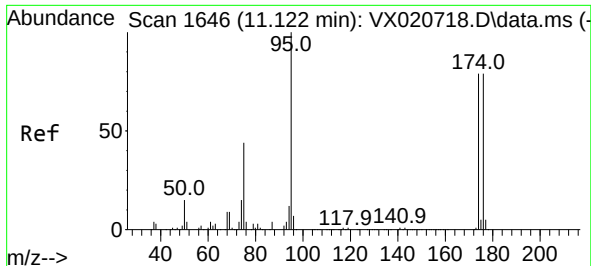

#62
4-Bromofluorobenzene
Concen: 44.50 ug/l
RT: 11.122 min Scan# 1646
Delta R.T. -0.000 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-98-100


Tgt Ion: 95 Resp: 216155
Ion Ratio Lower Upper
95 100
174 79.2 0.0 154.6
176 75.5 0.0 155.8

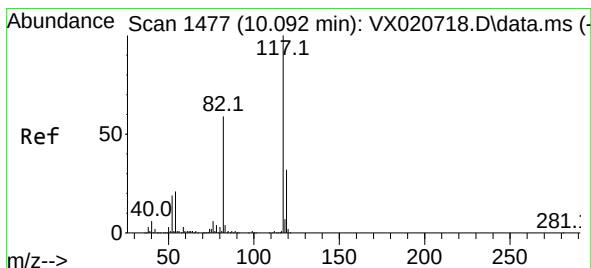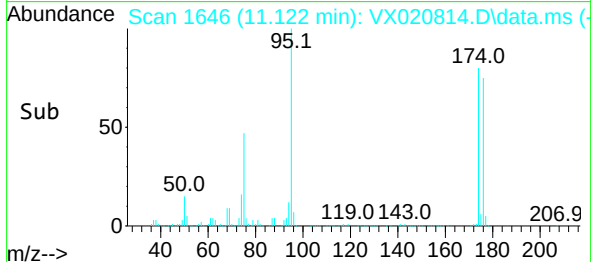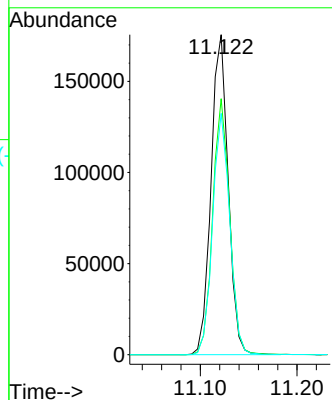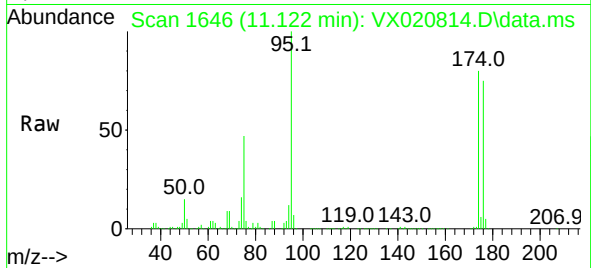

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.097 min Scan# 1478
Delta R.T. 0.005 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55


Tgt Ion: 117 Resp: 485373
Ion Ratio Lower Upper
117 100
82 54.6 47.4 71.2
119 31.7 26.6 39.8

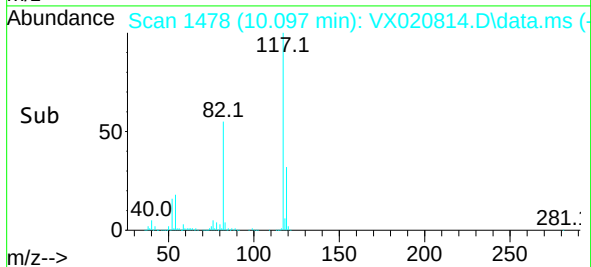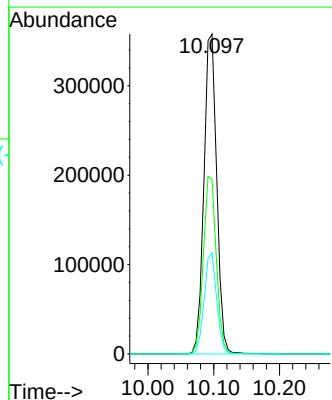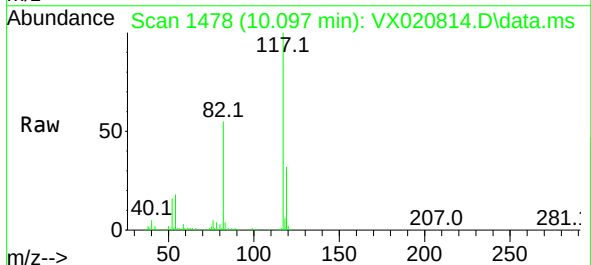

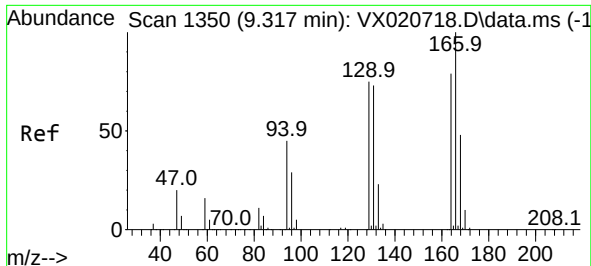




#64
Tetrachloroethene
Concen: 0.25 ug/l
RT: 9.311 min Scan# 1349
Delta R.T. -0.006 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW6-GW-98-100

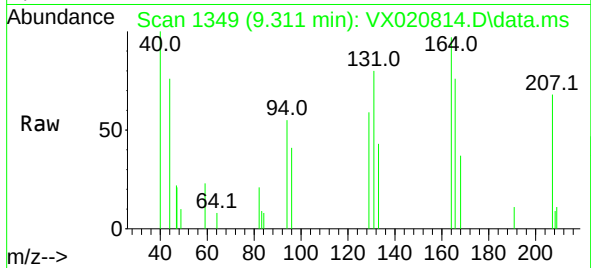


Tgt Ion:164 Resp: 916

Ion	Ratio	Lower	Upper
164	100		
166	78.3	103.4	155.2#
129	60.6	70.8	106.2#
131	82.9	72.5	108.7

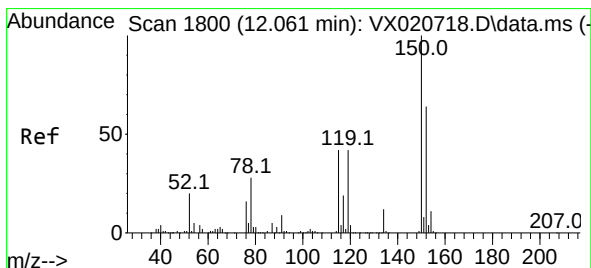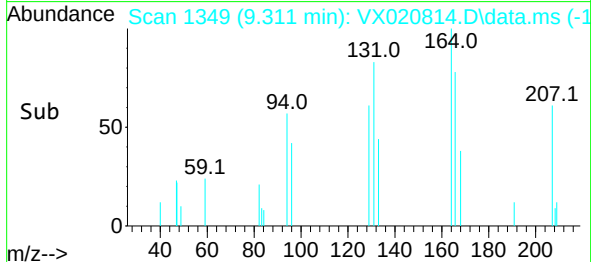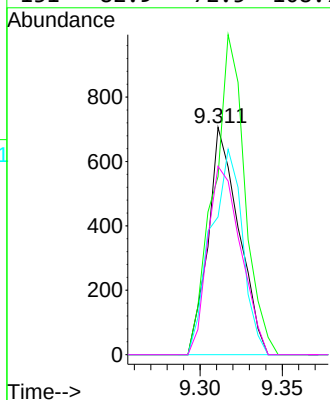

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.060 min Scan# 1800
Delta R.T. -0.001 min
Lab File: VX020814.D
Acq: 29 Jan 2021 19:55

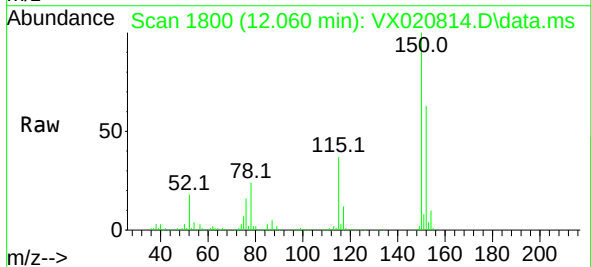

Tgt Ion:152 Resp: 211007

Ion	Ratio	Lower	Upper
152	100		
115	59.2	41.1	123.3
150	156.3	0.0	349.0

