

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013023\
 Data File : VX033950.D
 Acq On : 30 Jan 2023 16:51
 Operator : JC/MD
 Sample : 01345-01 20X
 Misc : 5.01g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RBR200007

Quant Time: Jan 31 04:49:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 11 14:48:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	156083	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	222343	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	195840	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	92424	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	73243	44.568	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	89.140%
35) Dibromofluoromethane	5.385	113	68119	49.339	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.680%
50) Toluene-d8	8.647	98	251065	49.910	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.820%
62) 4-Bromofluorobenzene	11.079	95	85969	46.030	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.060%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013023\
Data File : VX033950.D
Acq On : 30 Jan 2023 16:51
Operator : JC/MD
Sample : 01345-01 20X
Misc : 5.01g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RBR200007

Quant Time: Jan 31 04:49:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 11 14:48:42 2023
Response via : Initial Calibration




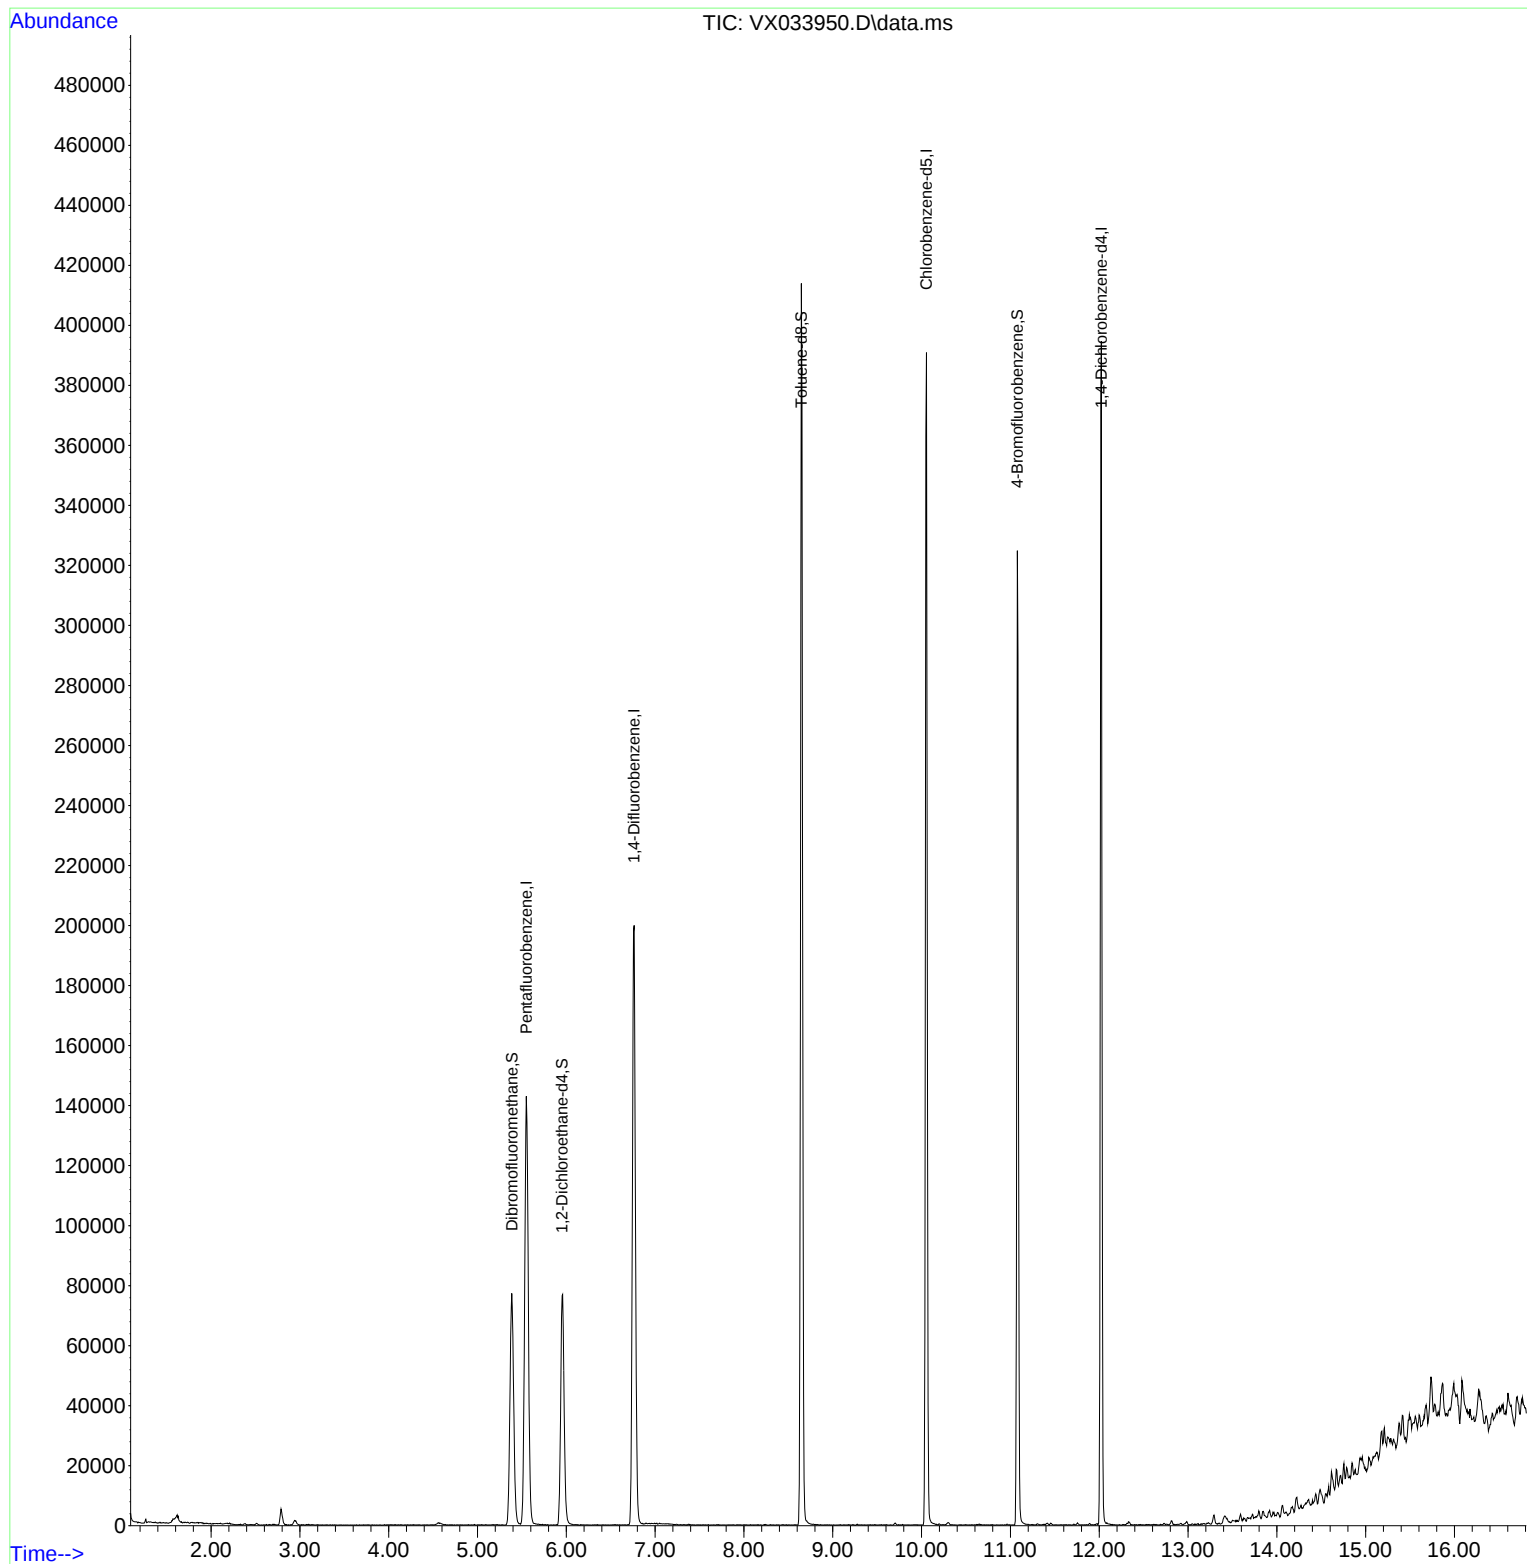




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX033950.D
Acq: 30 Jan 2023 16:51




Instrument :
MSVOA_X
ClientSampleId :
RBR200007


Tgt Ion:168 Resp: 156083
Ion Ratio Lower Upper
168 100
99 46.6 39.6 59.4

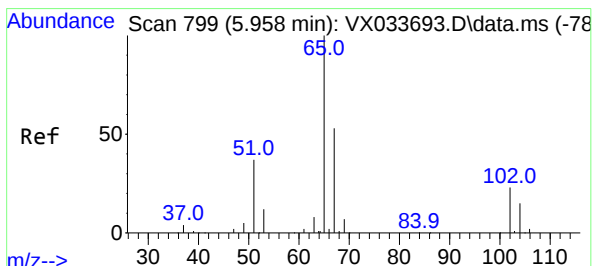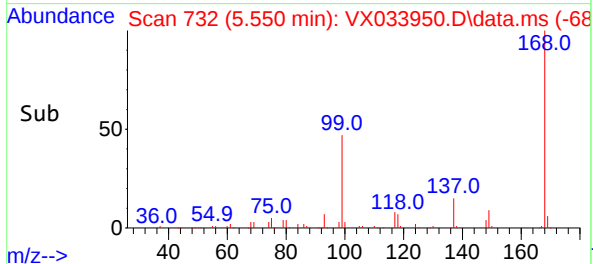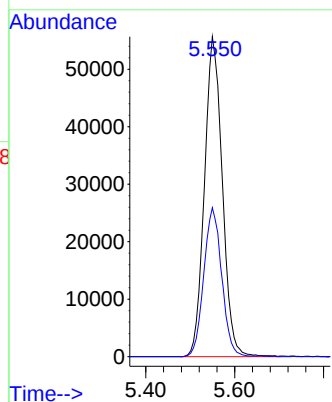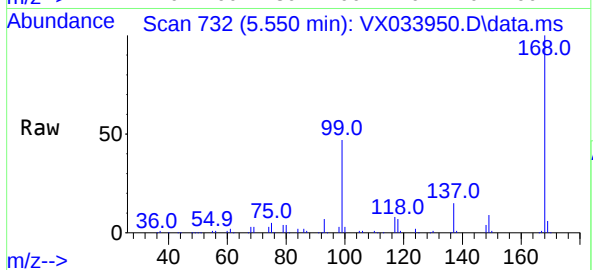

#33
1,2-Dichloroethane-d4
Concen: 44.568 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX033950.D
Acq: 30 Jan 2023 16:51

Tgt Ion: 65 Resp: 73243
Ion Ratio Lower Upper
65 100
67 53.0 0.0 104.8


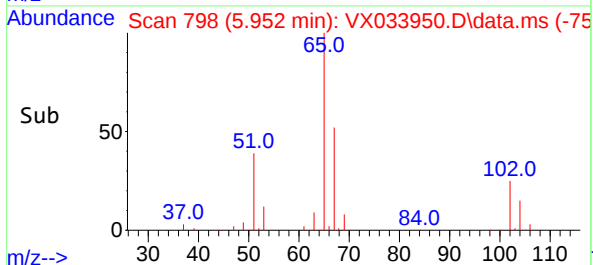
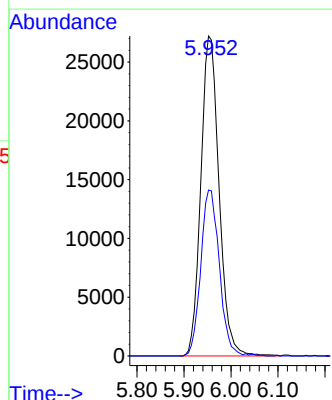
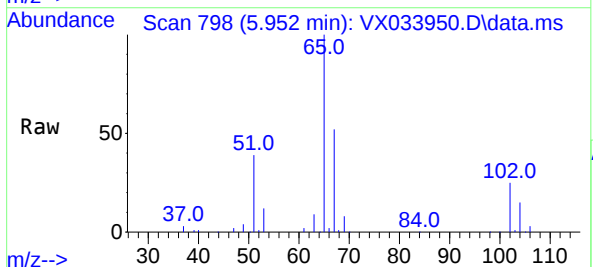


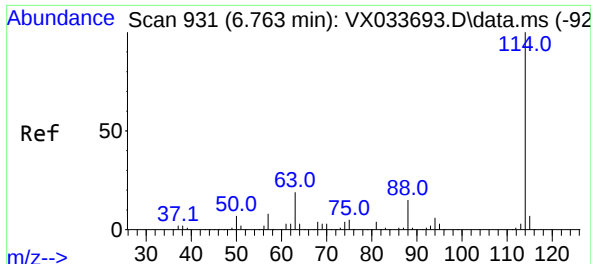

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX033950.D
Acq: 30 Jan 2023 16:51




Instrument :
MSVOA_X
ClientSampleId :
RBR200007


Tgt Ion:114 Resp: 222343
Ion Ratio Lower Upper
114 100
63 17.7 0.0 37.4
88 14.7 0.0 30.6

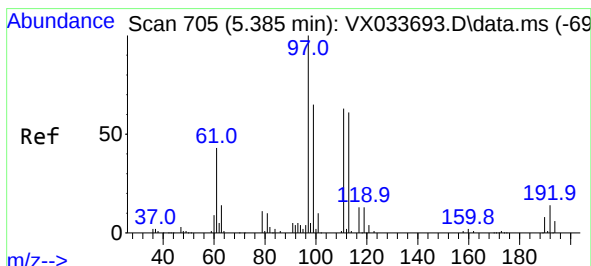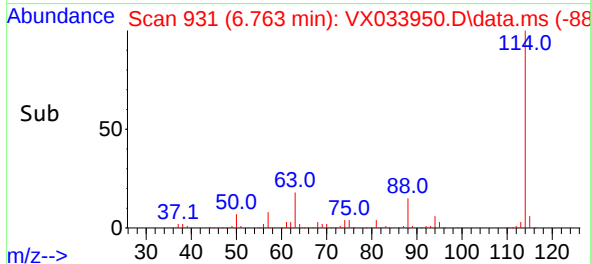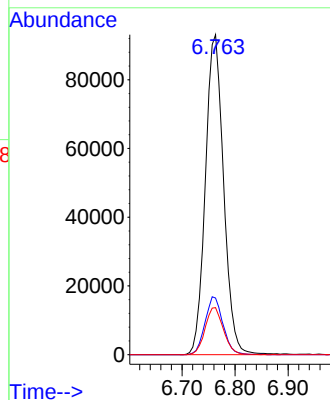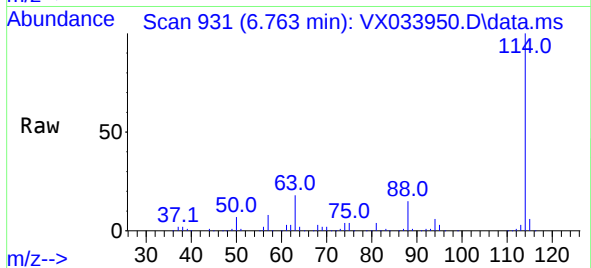

#35
Dibromofluoromethane
Concen: 49.339 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX033950.D
Acq: 30 Jan 2023 16:51

Tgt Ion:113 Resp: 68119
Ion Ratio Lower Upper
113 100
111 101.7 83.0 124.6
192 24.3 19.0 28.4

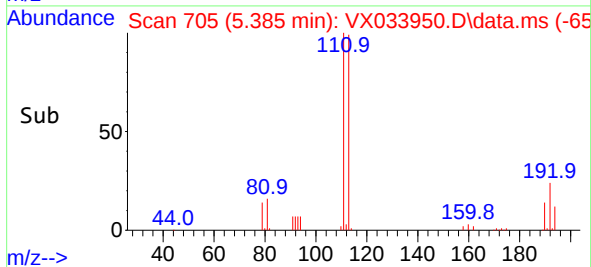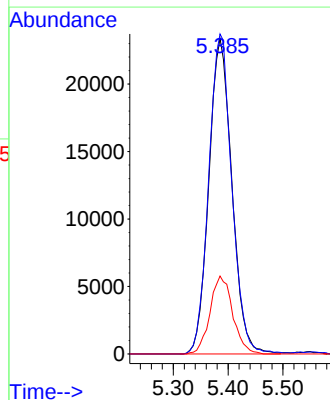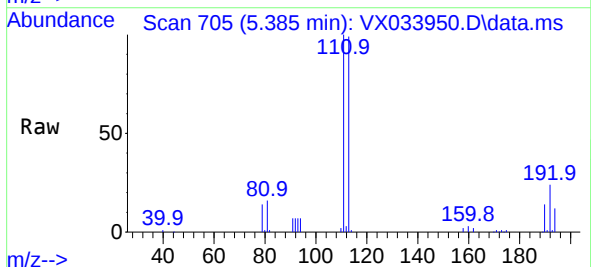

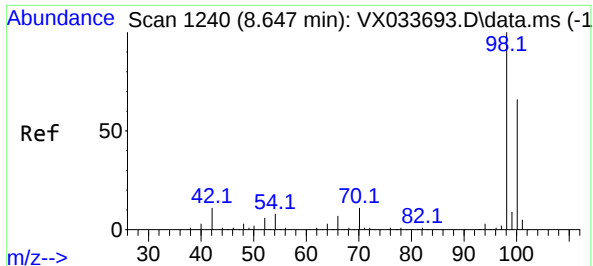

#50

Toluene-d8

Concen: 49.910 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX033950.D

Acq: 30 Jan 2023 16:51

Instrument :

MSVOA_X

ClientSampleId :





RBR200007

Tgt Ion: 98 Resp: 251065

Ion Ratio Lower Upper

98 100

100 67.4 53.6 80.4

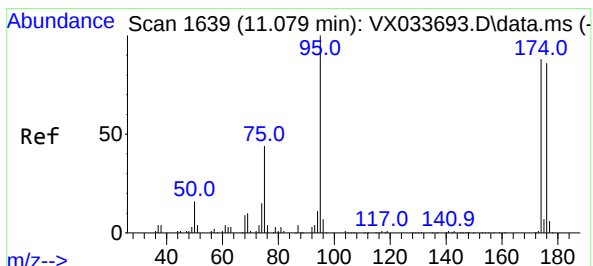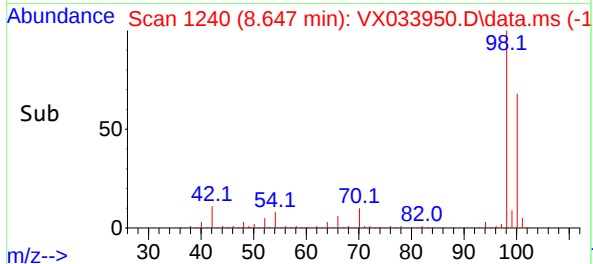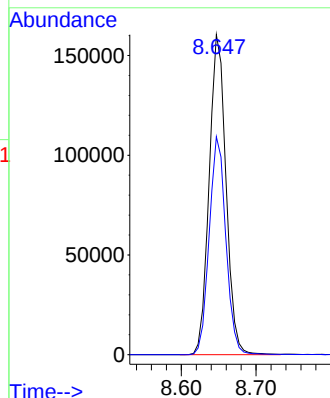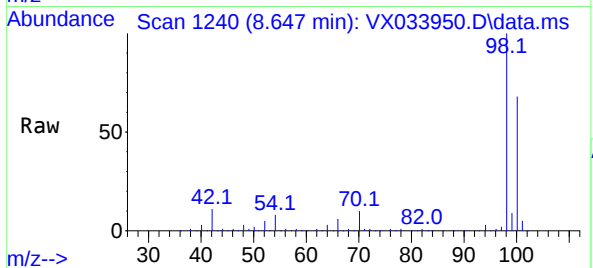

#62

4-Bromofluorobenzene

Concen: 46.030 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX033950.D

Acq: 30 Jan 2023 16:51




Tgt Ion: 95 Resp: 85969


Ion Ratio Lower Upper

95 100

174 93.8 0.0 184.4

176 93.2 0.0 178.8


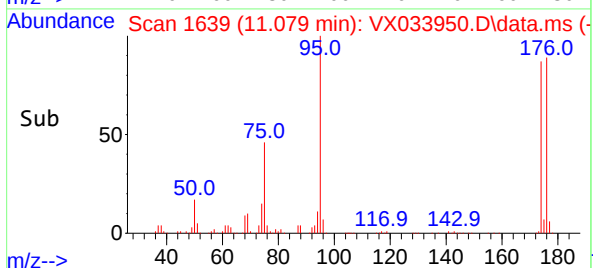
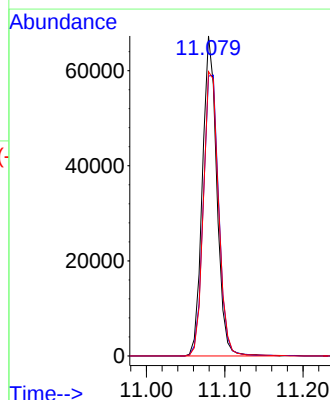
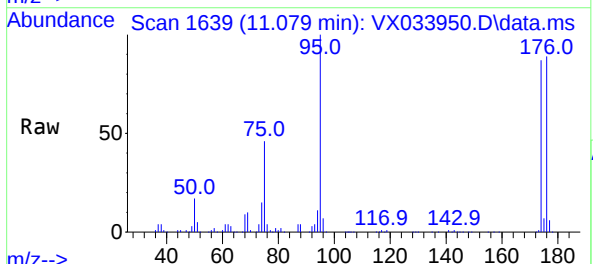


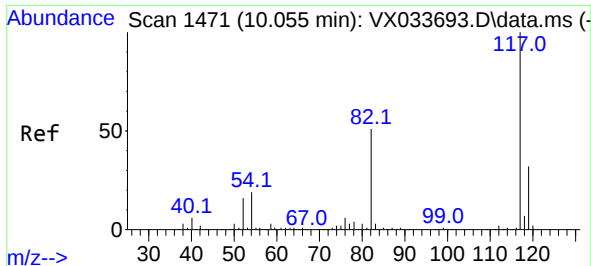

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033950.D
Acq: 30 Jan 2023 16:51

Instrument :
MSVOA_X
ClientSampleId :
RBR200007

Tgt Ion:117 Resp: 195840
Ion Ratio Lower Upper
117 100
82 49.0 40.6 60.8
119 31.7 25.6 38.4

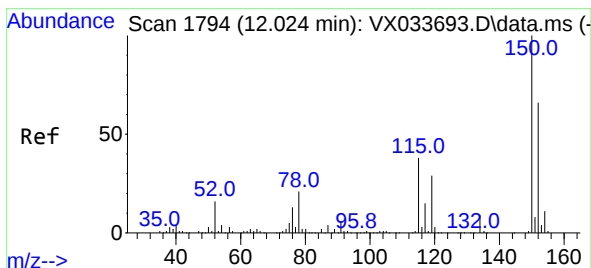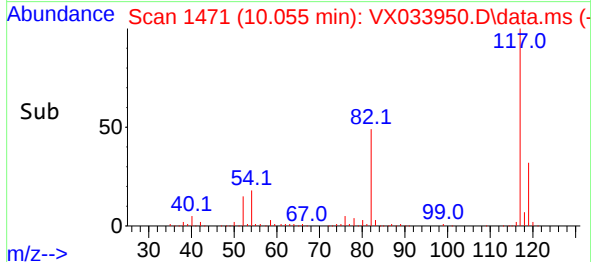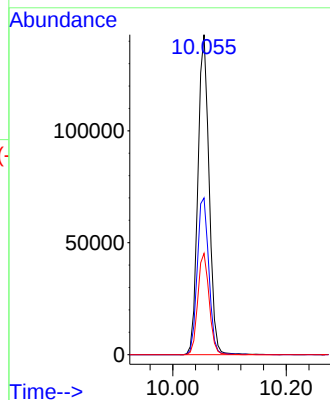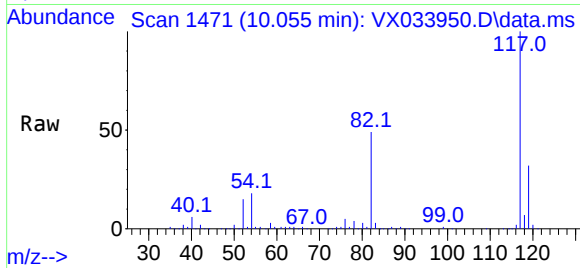

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX033950.D
Acq: 30 Jan 2023 16:51

Tgt Ion:152 Resp: 92424
Ion Ratio Lower Upper
152 100
115 53.1 38.7 116.1
150 157.0 0.0 348.2

