

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013023\
 Data File : VX033955.D
 Acq On : 30 Jan 2023 18:47
 Operator : JC/MD
 Sample : 01328-05
 Misc : 5.21g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOTAL-VOC-1-BORING-1-0-7-GRAB-2

Quant Time: Jan 31 04:52:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 11 14:48:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	159446	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	221402	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	190272	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93237	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	72138	42.969	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	85.940%
35) Dibromofluoromethane	5.385	113	63830	46.429	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.860%
50) Toluene-d8	8.647	98	248356	49.581	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.160%
62) 4-Bromofluorobenzene	11.085	95	83456	44.874	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.740%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013023\
Data File : VX033955.D
Acq On : 30 Jan 2023 18:47
Operator : JC/MD
Sample : 01328-05
Misc : 5.21g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTAL-VOC-1-BORING-1-0-7-GRAB-2

Quant Time: Jan 31 04:52:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X011123W.M
Quant Title : SW846 8260
QLast Update : Wed Jan 11 14:48:42 2023
Response via : Initial Calibration




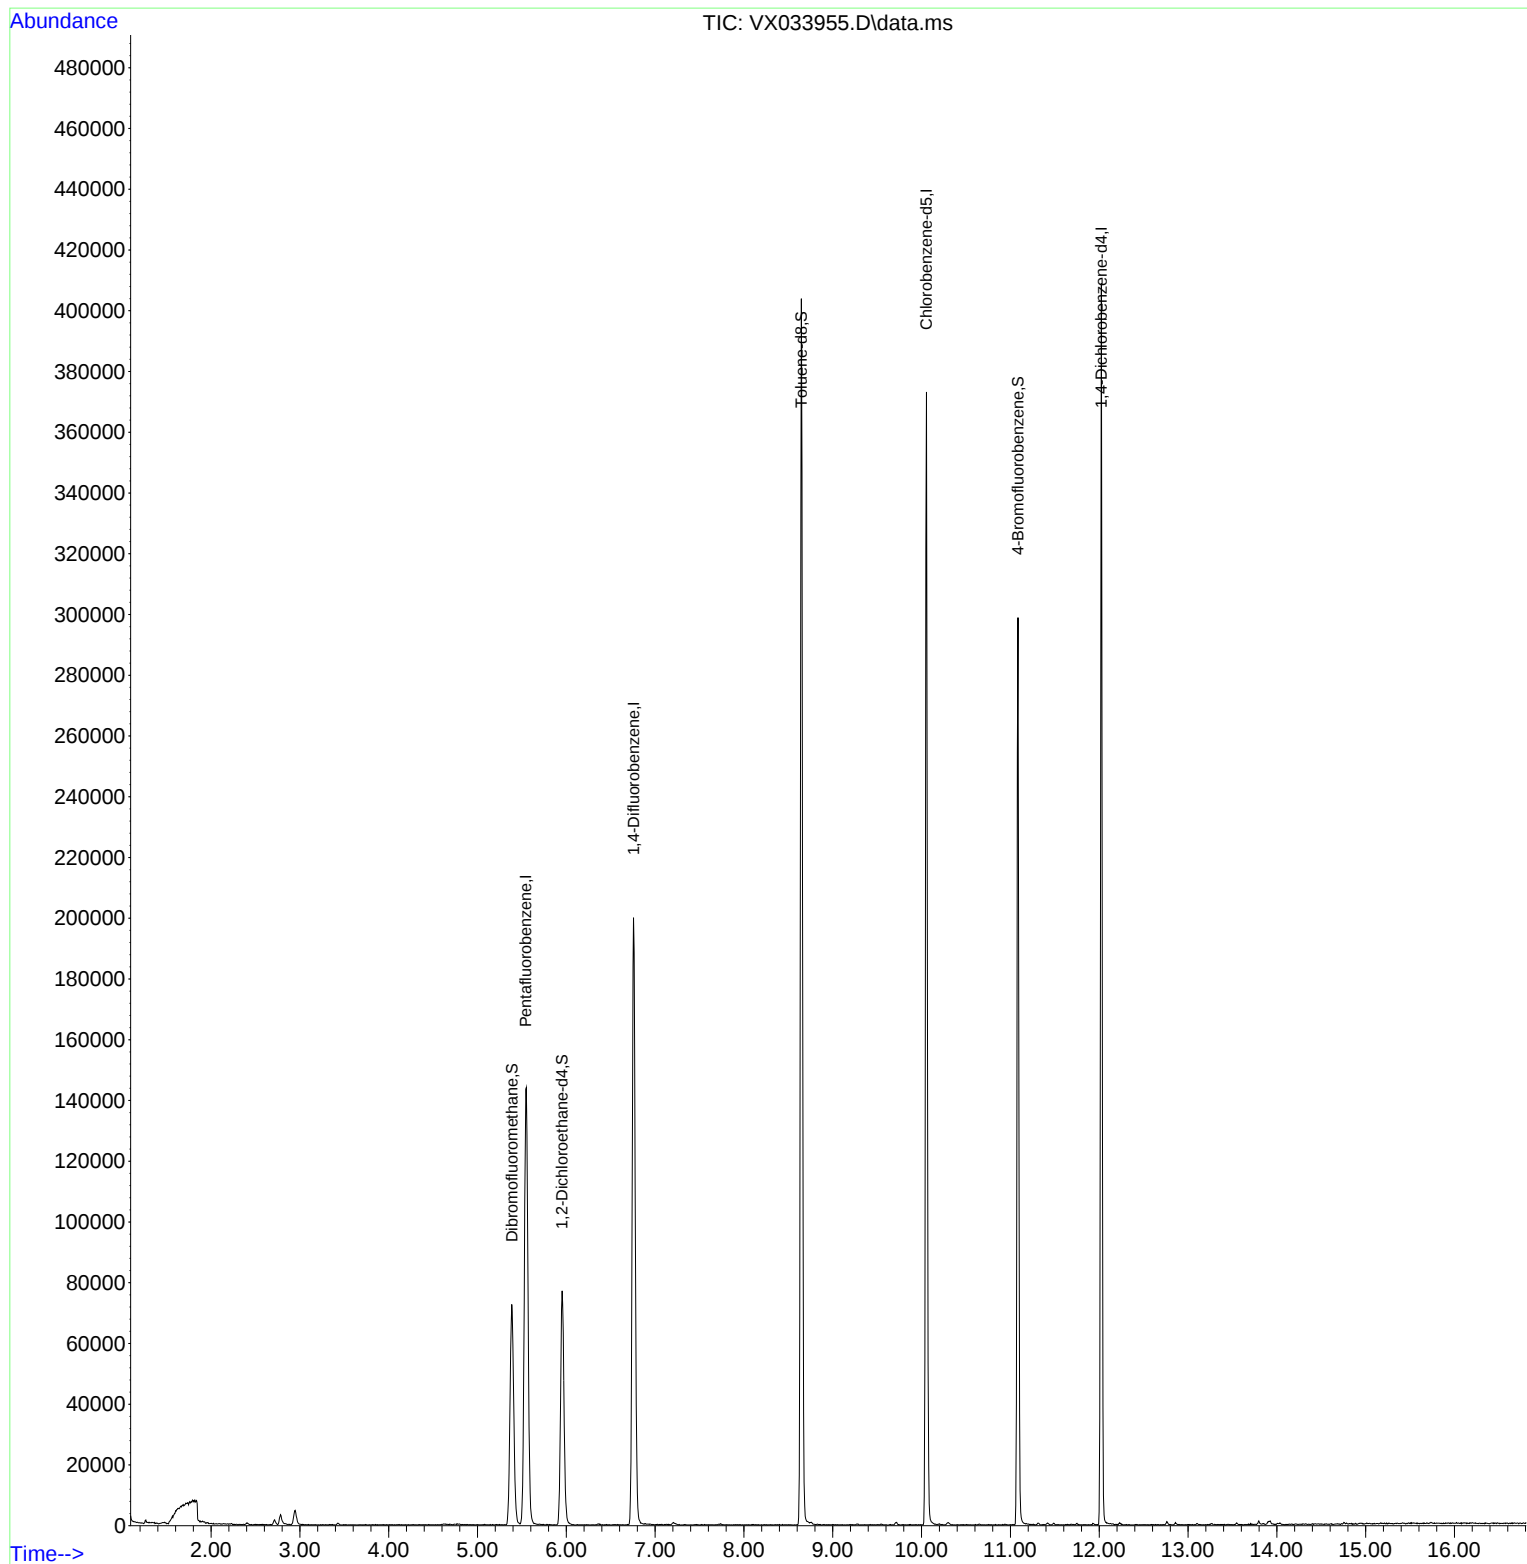




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX033955.D
Acq: 30 Jan 2023 18:47




Instrument :
MSVOA_X
ClientSampleId :
TOTAL-VOC-1-BORING-1-0-7-GRAB-2


Tgt Ion:168 Resp: 159446
Ion Ratio Lower Upper
168 100
99 46.0 39.6 59.4

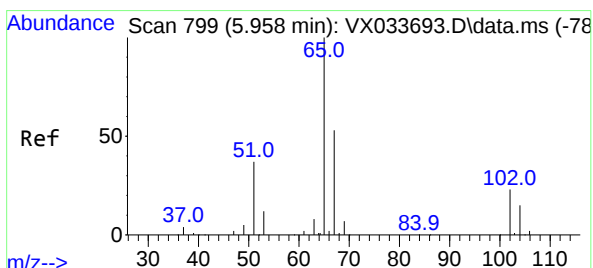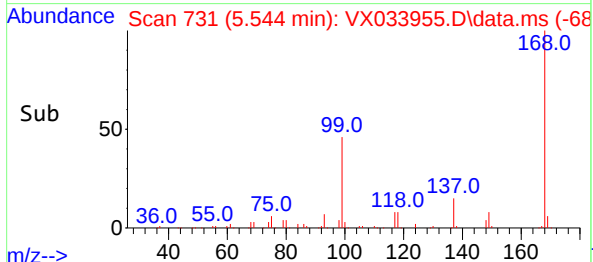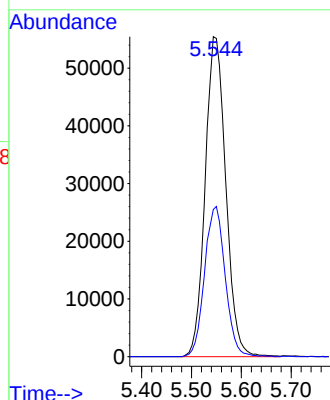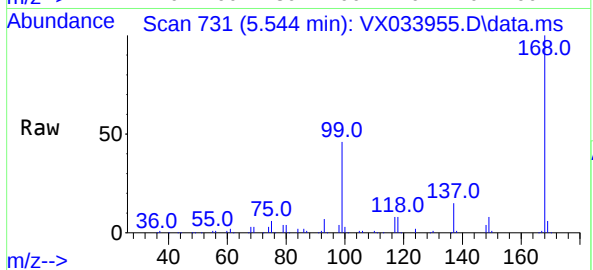

#33
1,2-Dichloroethane-d4
Concen: 42.969 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX033955.D
Acq: 30 Jan 2023 18:47

Tgt Ion: 65 Resp: 72138
Ion Ratio Lower Upper
65 100
67 53.7 0.0 104.8

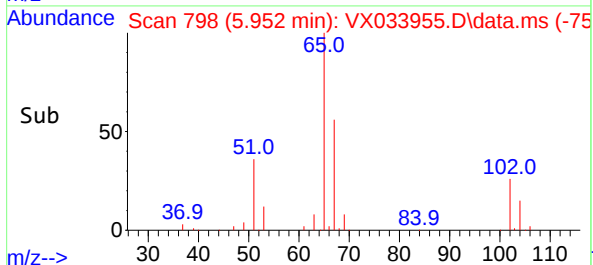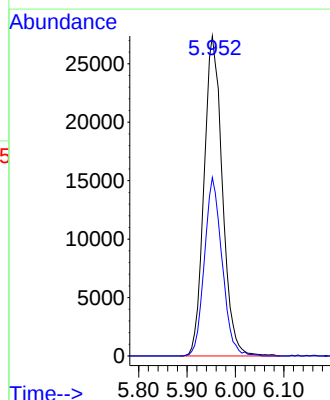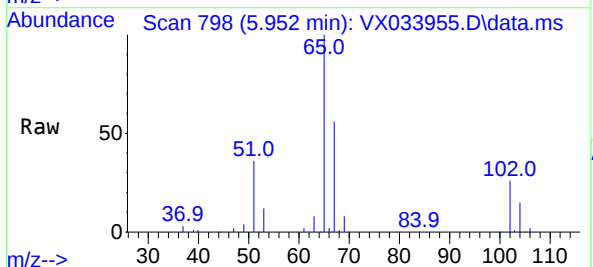

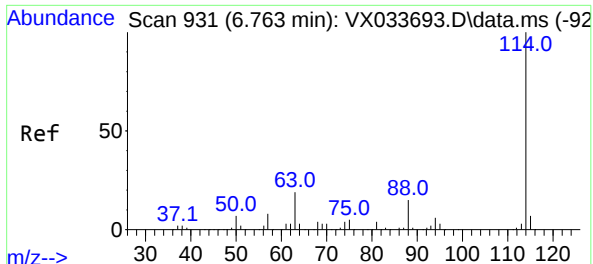

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 91

Delta R.T. -0.006 min

Lab File: VX033955.D

Acq: 30 Jan 2023 18:47

Instrument :

MSVOA_X

ClientSampleId :

TOTAL-VOC-1-BORING-1-0-7-GRAB-2





Tgt Ion:114 Resp: 221402

Ion Ratio Lower Upper

114 100

63 19.0 0.0 37.4

88 16.1 0.0 30.6

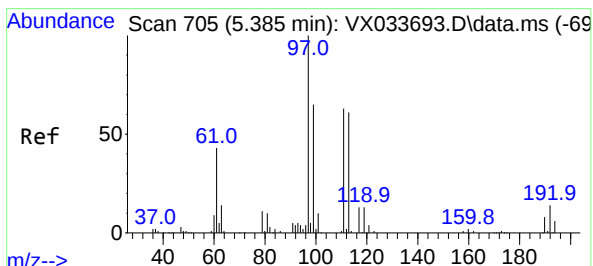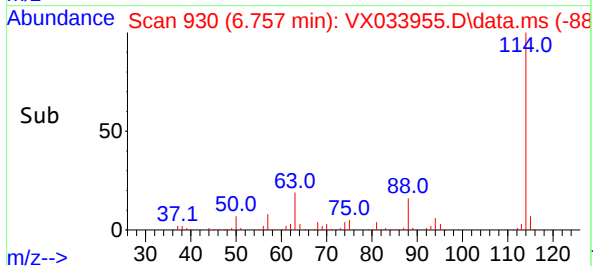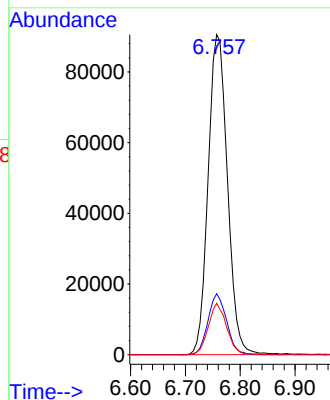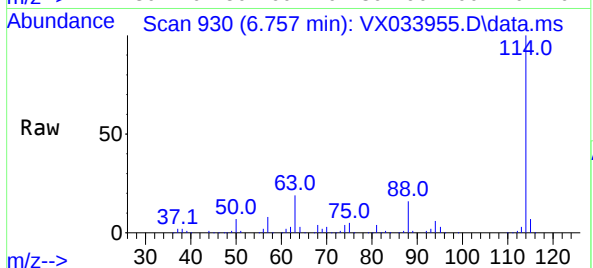

#35

Dibromofluoromethane

Concen: 46.429 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.000 min

Lab File: VX033955.D

Acq: 30 Jan 2023 18:47




Tgt Ion:113 Resp: 63830


Ion Ratio Lower Upper

113 100

111 101.6 83.0 124.6

192 25.0 19.0 28.4


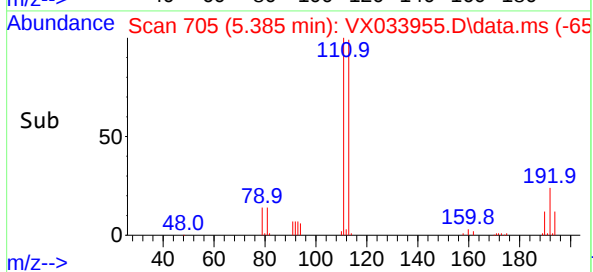
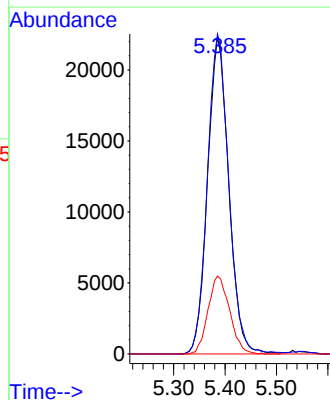
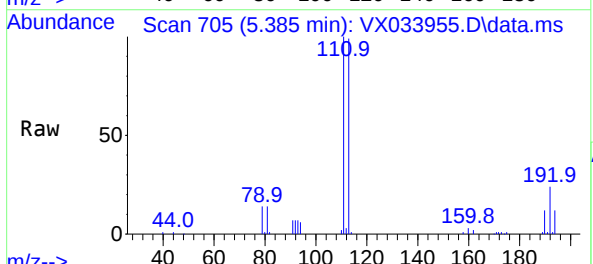


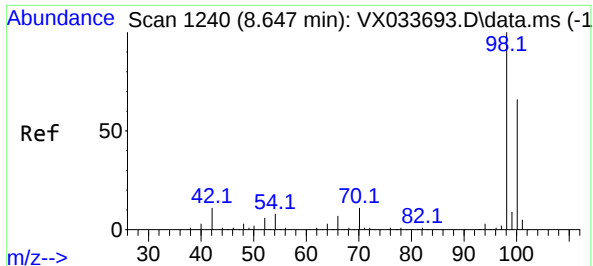

#50
Toluene-d8
Concen: 49.581 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX033955.D
Acq: 30 Jan 2023 18:47




Instrument : MSVOA_X
ClientSampleId : TOTAL-VOC-1-BORING-1-0-7-GRAB-2


Tgt Ion: 98 Resp: 248356
Ion Ratio Lower Upper
98 100
100 67.6 53.6 80.4

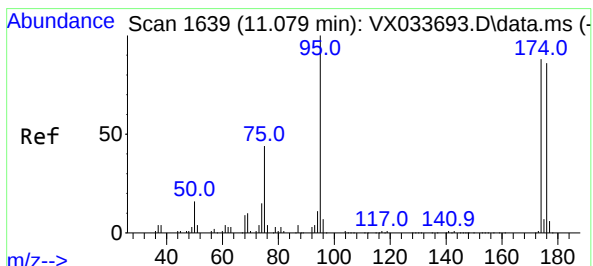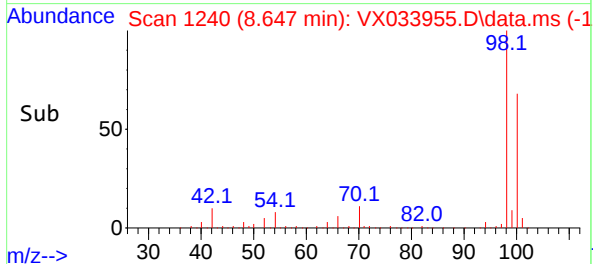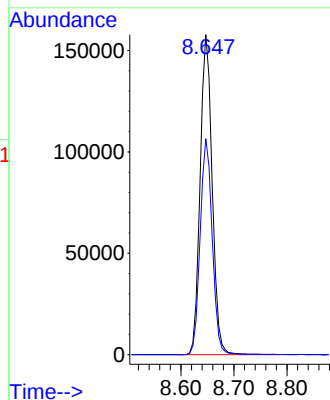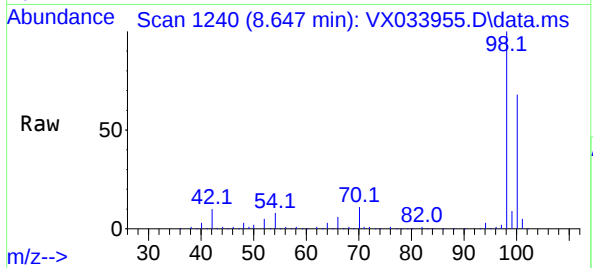

#62
4-Bromofluorobenzene
Concen: 44.874 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX033955.D
Acq: 30 Jan 2023 18:47

Tgt Ion: 95 Resp: 83456
Ion Ratio Lower Upper
95 100
174 94.2 0.0 184.4
176 92.1 0.0 178.8


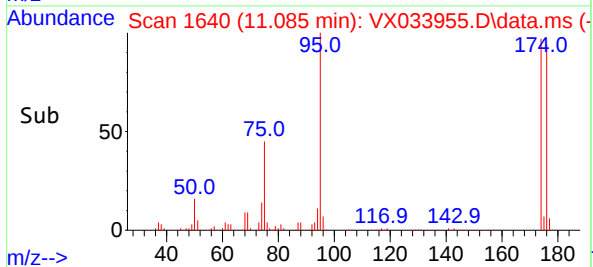
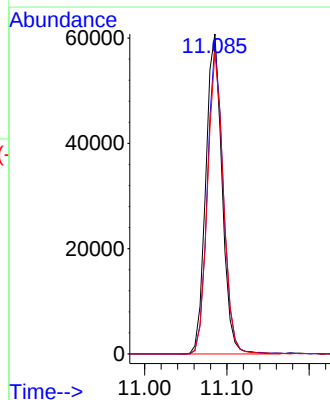
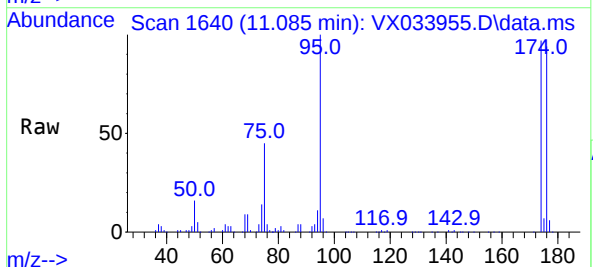


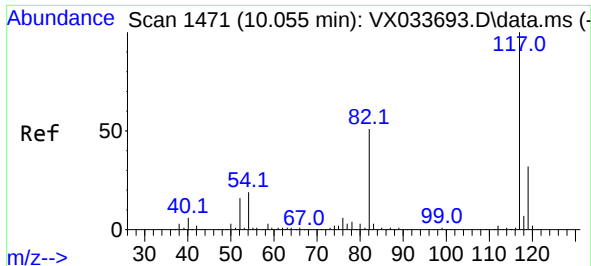

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033955.D
Acq: 30 Jan 2023 18:47

Instrument :
MSVOA_X
ClientSampleId :
TOTAL-VOC-1-BORING-1-0-7-GRAB-2

Tgt Ion:117 Resp: 190272
Ion Ratio Lower Upper
117 100
82 51.1 40.6 60.8
119 33.0 25.6 38.4

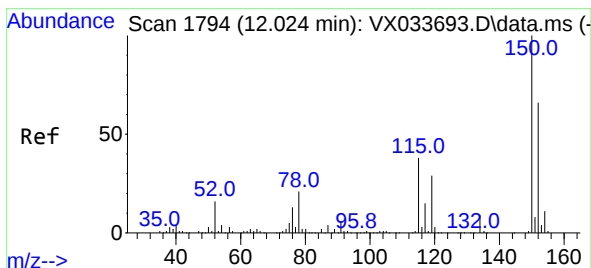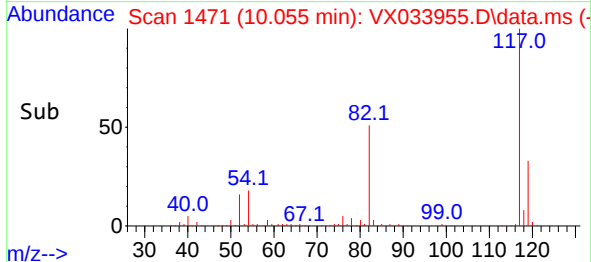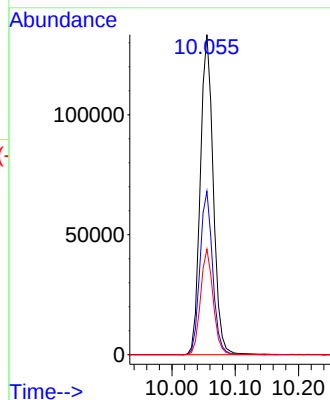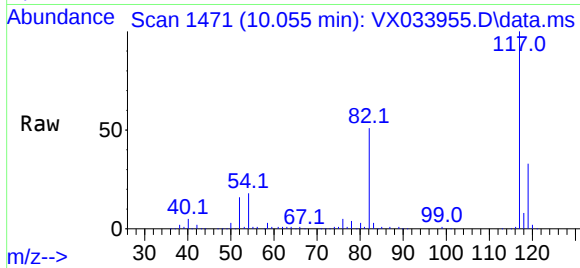

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX033955.D
Acq: 30 Jan 2023 18:47

Tgt Ion:152 Resp: 93237
Ion Ratio Lower Upper
152 100
115 52.9 38.7 116.1
150 157.6 0.0 348.2

