

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013025\
 Data File : VX044780.D
 Acq On : 30 Jan 2025 13:55
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Jan 31 00:42:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011625W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Jan 17 01:21:41 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.898	128	24187	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.757	114	130445	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	112829	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.952	65	63658	27.263	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	90.867%#
60) 4-Bromofluorobenzene	11.079	95	61462	28.045	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	93.500%
63) Toluene-d8	8.647	98	186168	30.337	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	101.133%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013025\
Data File : VX044780.D
Acq On : 30 Jan 2025 13:55
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Jan 31 00:42:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011625W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Jan 17 01:21:41 2025
Response via : Initial Calibration




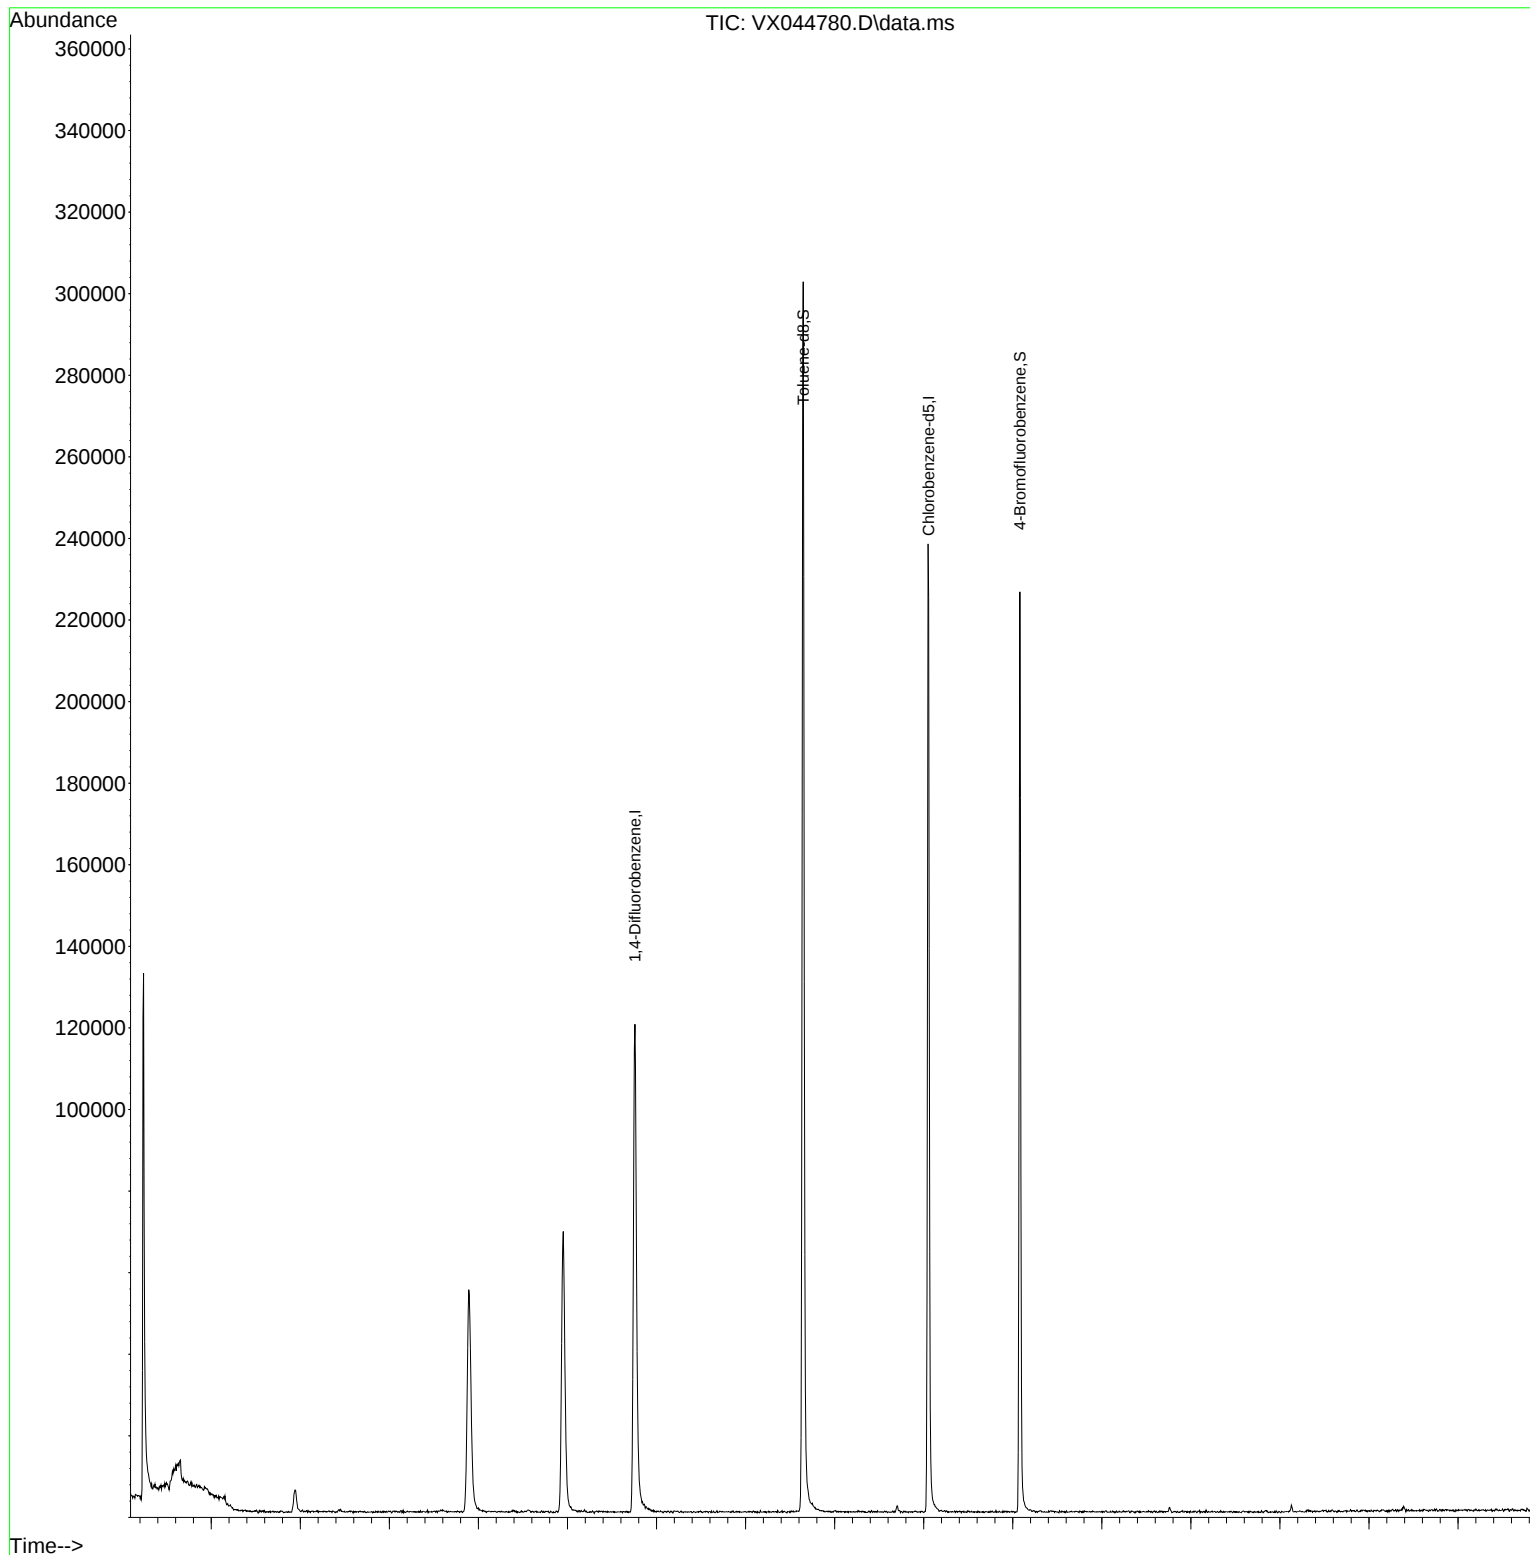


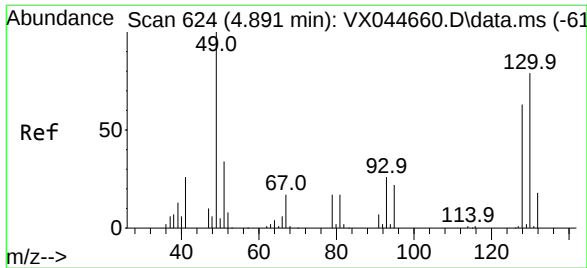

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.898 min Scan# 62
Delta R.T. 0.007 min
Lab File: VX044780.D
Acq: 30 Jan 2025 13:55




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion	Ratio	Lower	Upper
128	100		
49	168.1	0.0	411.5
130	125.4	0.0	324.3

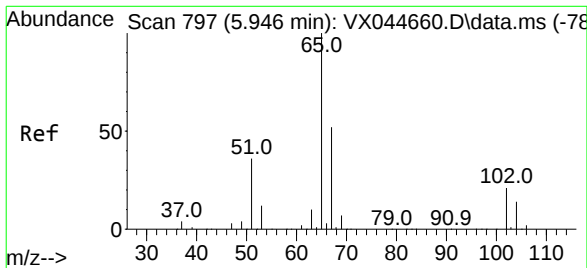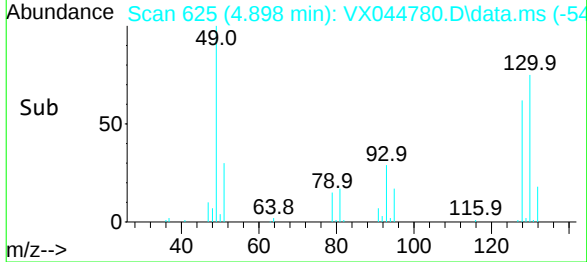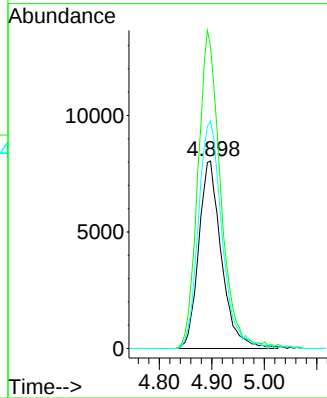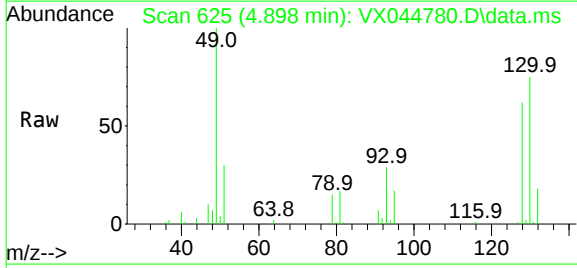

#27
1,2-Dichloroethane-d4
Concen: 27.263 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX044780.D
Acq: 30 Jan 2025 13:55

Tgt Ion	Ratio	Lower	Upper
65	100		
67	53.7	41.4	62.2


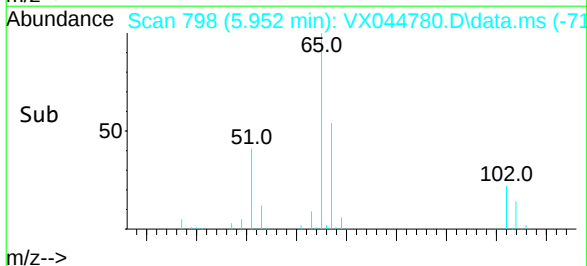
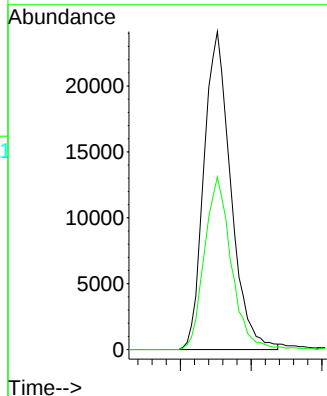
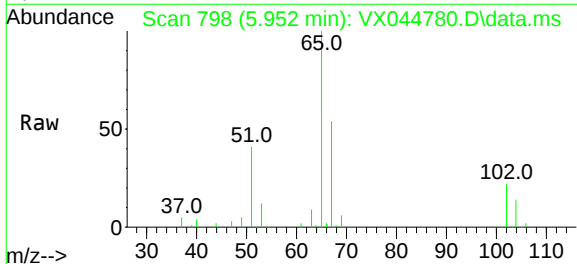


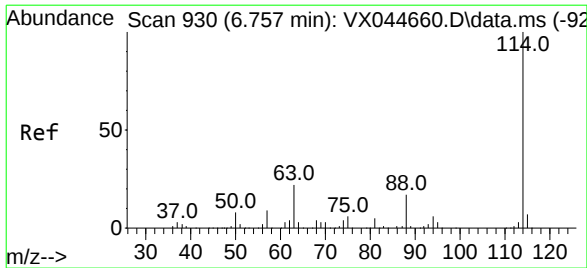

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. 0.000 min
Lab File: VX044780.D
Acq: 30 Jan 2025 13:55




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:	114	Resp:	130445
Ion	Ratio	Lower	Upper
114	100		
63	20.2	16.6	24.8
88	15.8	13.4	20.2

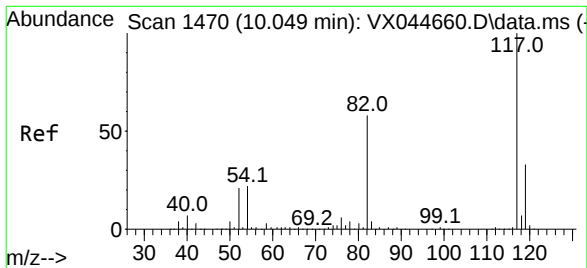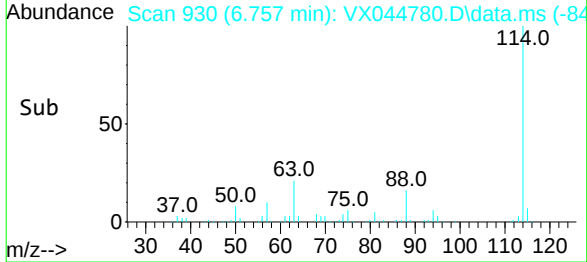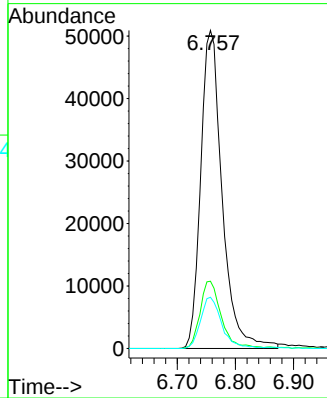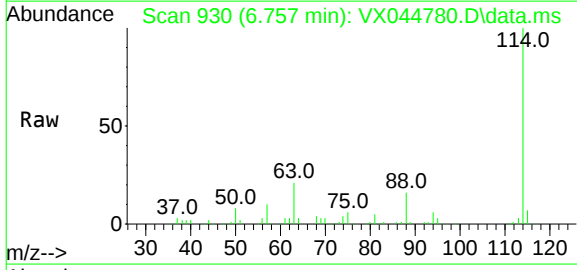

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX044780.D
Acq: 30 Jan 2025 13:55


Tgt Ion:	117	Resp:	112829
Ion	Ratio	Lower	Upper
117	100		
82	56.6	45.8	68.6
119	32.3	25.8	38.6

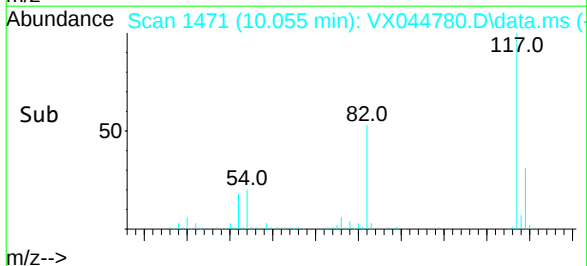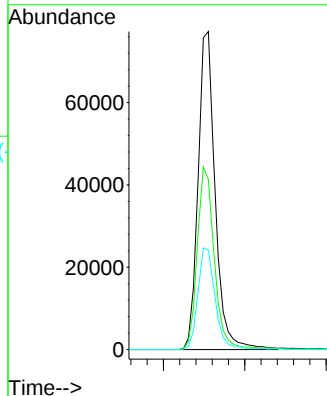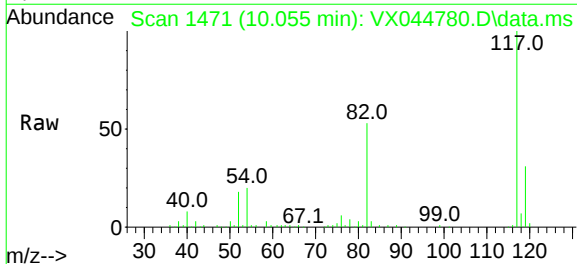



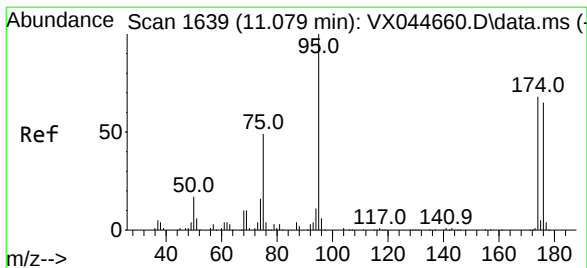


#60
4-Bromofluorobenzene
Concen: 28.045 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX044780.D
Acq: 30 Jan 2025 13:55

Instrument :
MSVOA_X
ClientSampleId :
IBLK

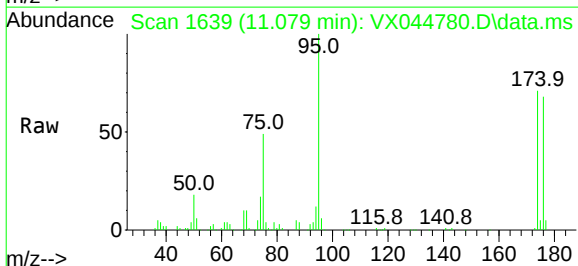

Tgt Ion: 95 Resp: 61462
Ion Ratio Lower Upper
95 100
174 73.2 54.6 81.8
176 71.7 52.8 79.2

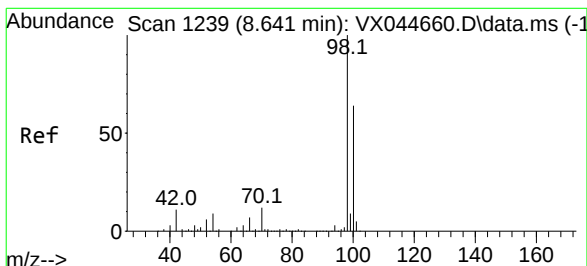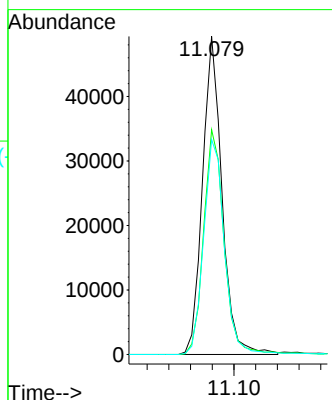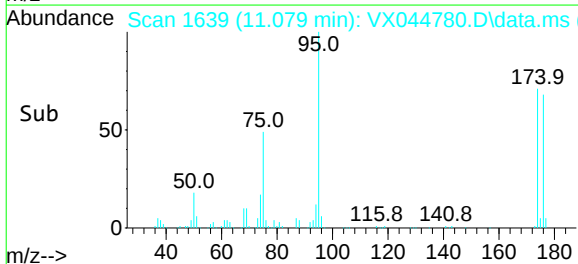

#63
Toluene-d8
Concen: 30.337 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.006 min
Lab File: VX044780.D
Acq: 30 Jan 2025 13:55

Tgt Ion: 98 Resp: 186168
Ion Ratio Lower Upper
98 100
100 66.0 53.6 80.4

