
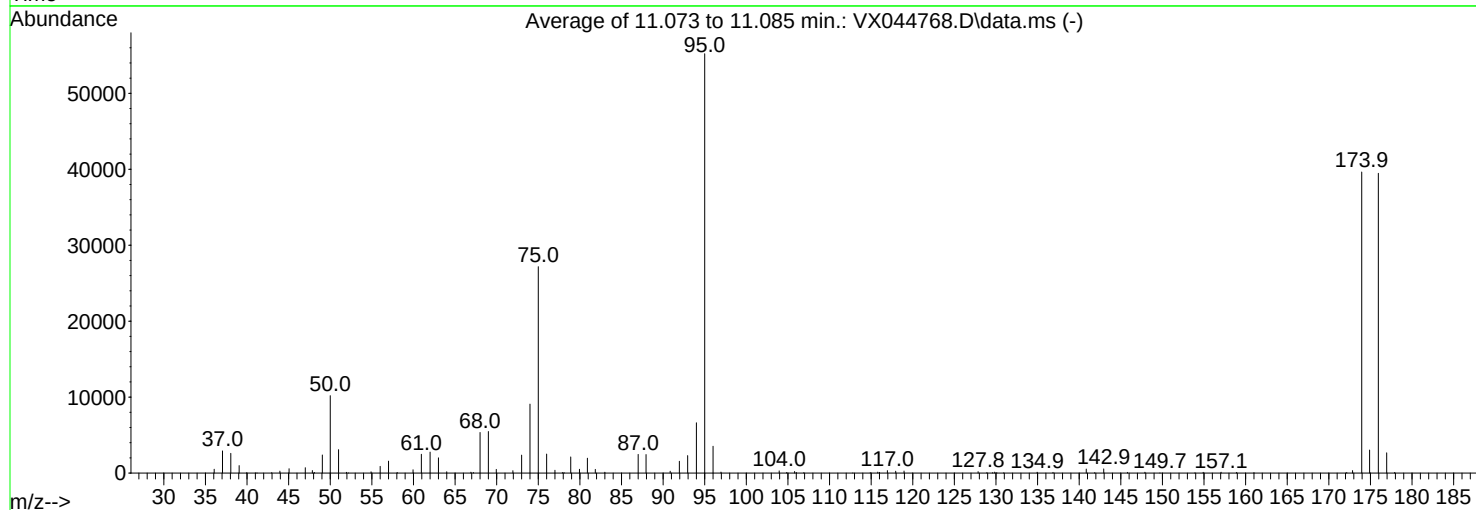


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX013025\
Data File : VX044768.D
Acq On : 30 Jan 2025 08:49
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X011625W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Jan 17 01:21:41 2025

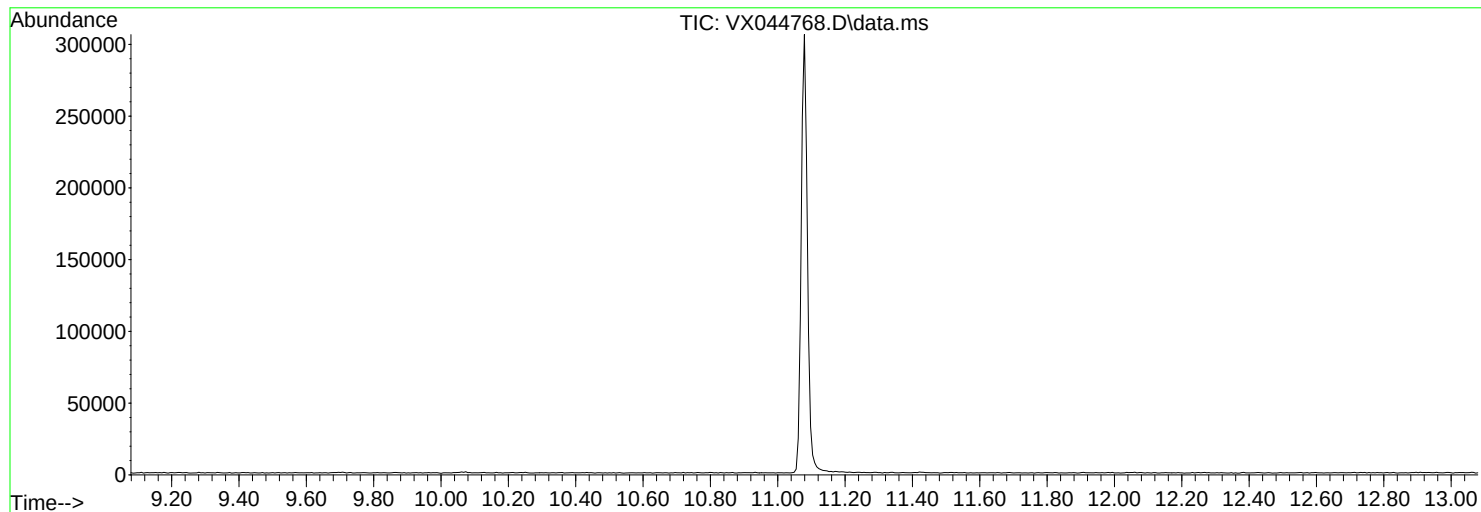

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	10194	PASS
75	95	30	60	49.2	27179	PASS
95	95	100	100	100.0	55216	PASS
96	95	5	9	6.4	3536	PASS
173	174	0.00	2	0.8	330	PASS
174	95	50	100	71.8	39645	PASS
175	174	5	9	7.7	3034	PASS
176	174	95	101	99.6	39472	PASS
177	176	5	9	6.8	2669	PASS